
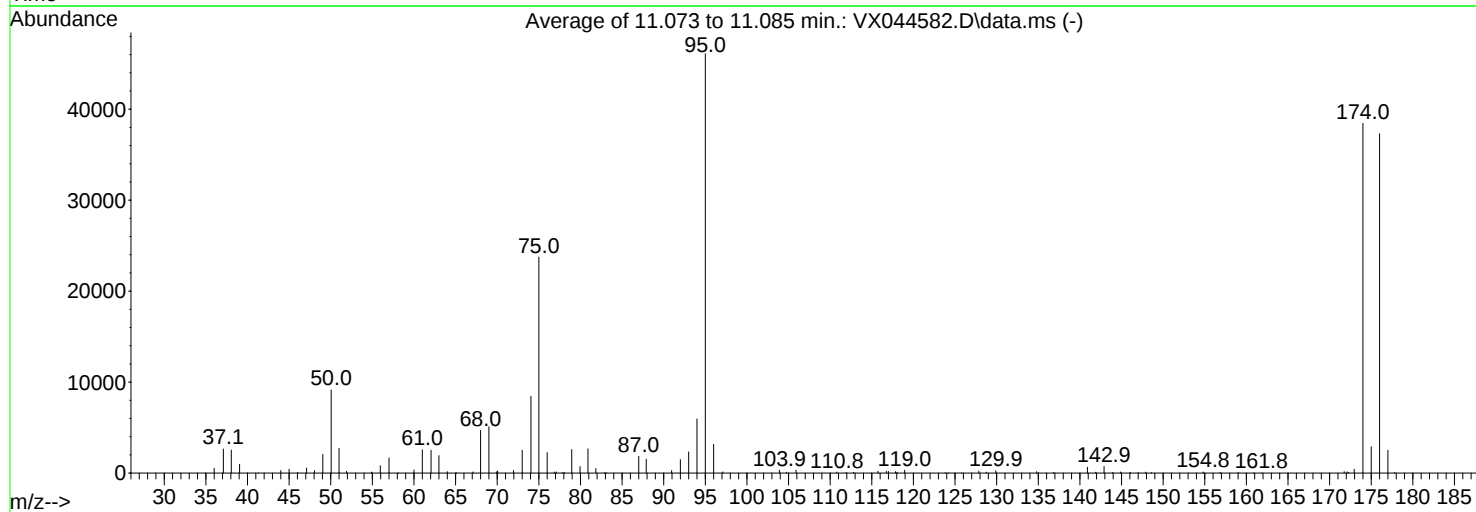


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010625\
Data File : VX044582.D
Acq On : 06 Jan 2025 07:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Title : SW846 8260
Last Update : Thu Dec 12 04:28:14 2024

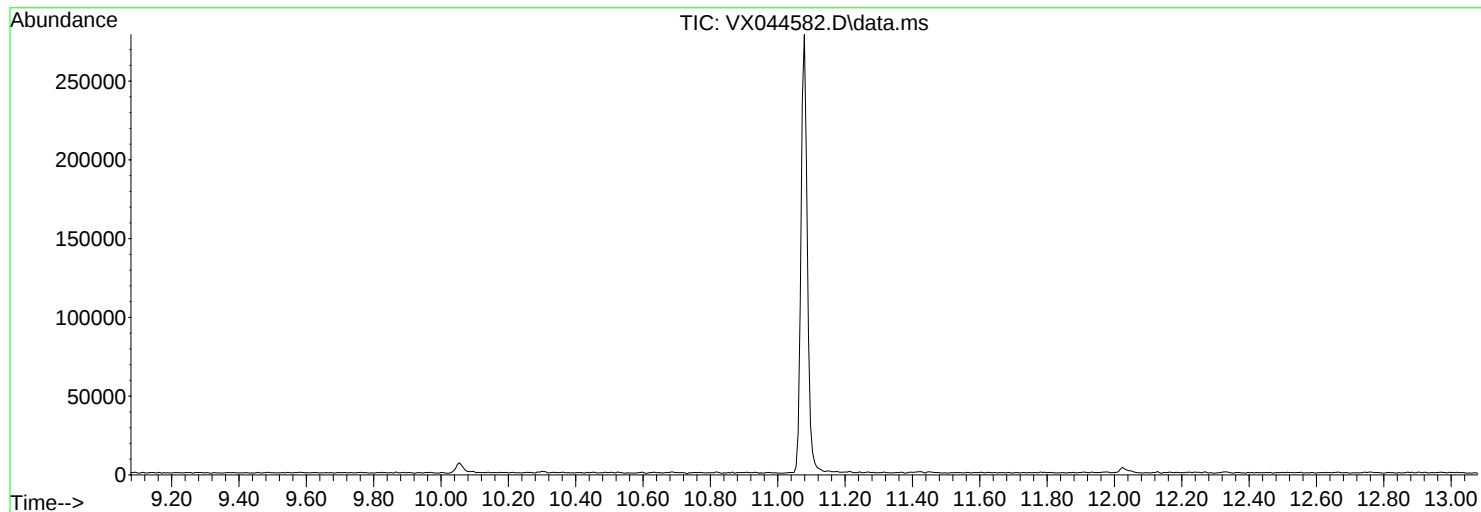

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9133	PASS
75	95	30	60	51.5	23736	PASS
95	95	100	100	100.0	46096	PASS
96	95	5	9	6.8	3148	PASS
173	174	0.00	2	1.1	414	PASS
174	95	50	100	83.4	38456	PASS
175	174	5	9	7.5	2895	PASS
176	174	95	101	97.0	37296	PASS
177	176	5	9	6.7	2507	PASS