
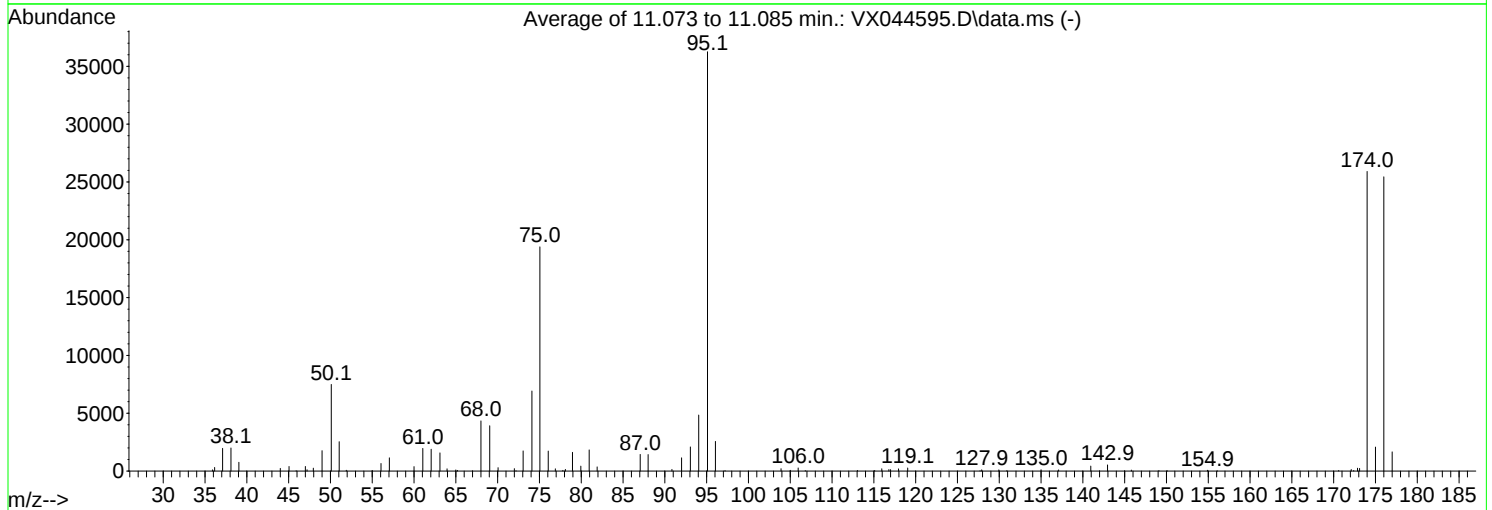


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
Data File : VX044595.D
Acq On : 07 Jan 2025 09:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Title : SW846 8260
Last Update : Wed Jan 08 03:57:12 2025

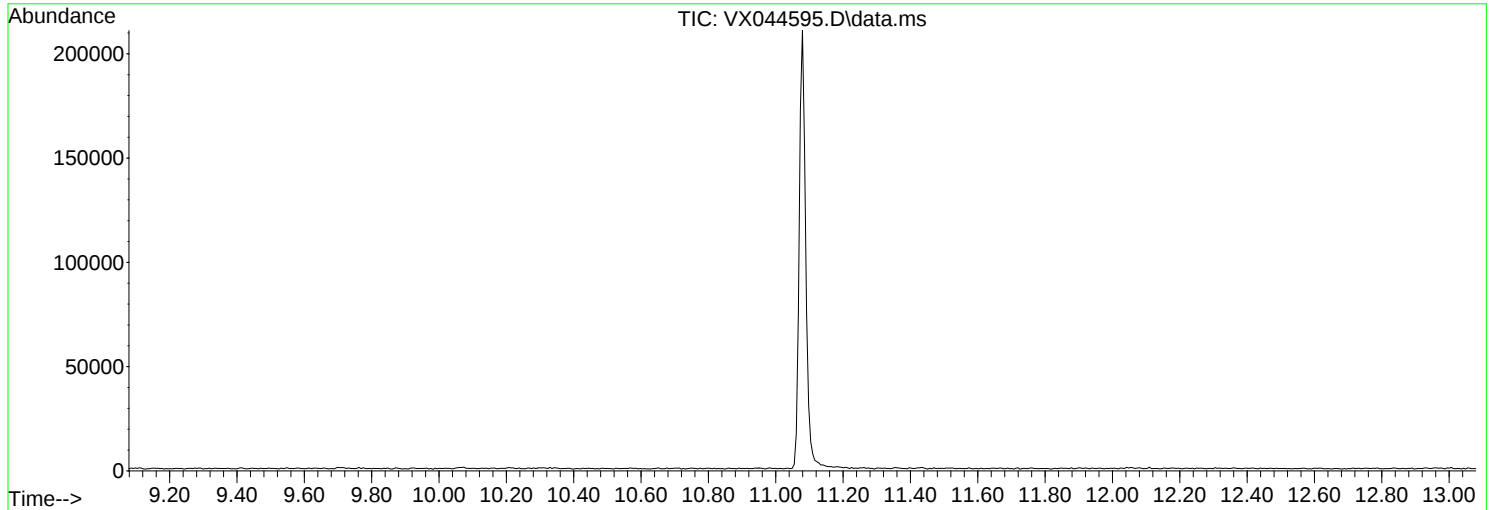

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	7495	PASS
75	95	30	60	53.5	19386	PASS
95	95	100	100	100.0	36261	PASS
96	95	5	9	7.1	2567	PASS
173	174	0.00	2	1.0	251	PASS
174	95	50	100	71.5	25909	PASS
175	174	5	9	8.0	2077	PASS
176	174	95	101	98.2	25445	PASS
177	176	5	9	6.5	1661	PASS