

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010825\
 Data File : VX044623.D
 Acq On : 08 Jan 2025 13:19
 Operator : JC/MD
 Sample : Q1006-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-WATER-REF-5

Quant Time: Jan 09 00:28:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 08 03:57:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	198813	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	364529	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	328697	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	140600	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	140435	43.809	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.620%
35) Dibromofluoromethane	5.379	113	115221	46.095	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.200%
50) Toluene-d8	8.647	98	428665	50.206	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.420%
62) 4-Bromofluorobenzene	11.079	95	149298	49.540	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.080%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010825\
Data File : VX044623.D
Acq On : 08 Jan 2025 13:19
Operator : JC/MD
Sample : Q1006-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Quant Time: Jan 09 00:28:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 08 03:57:12 2025
Response via : Initial Calibration

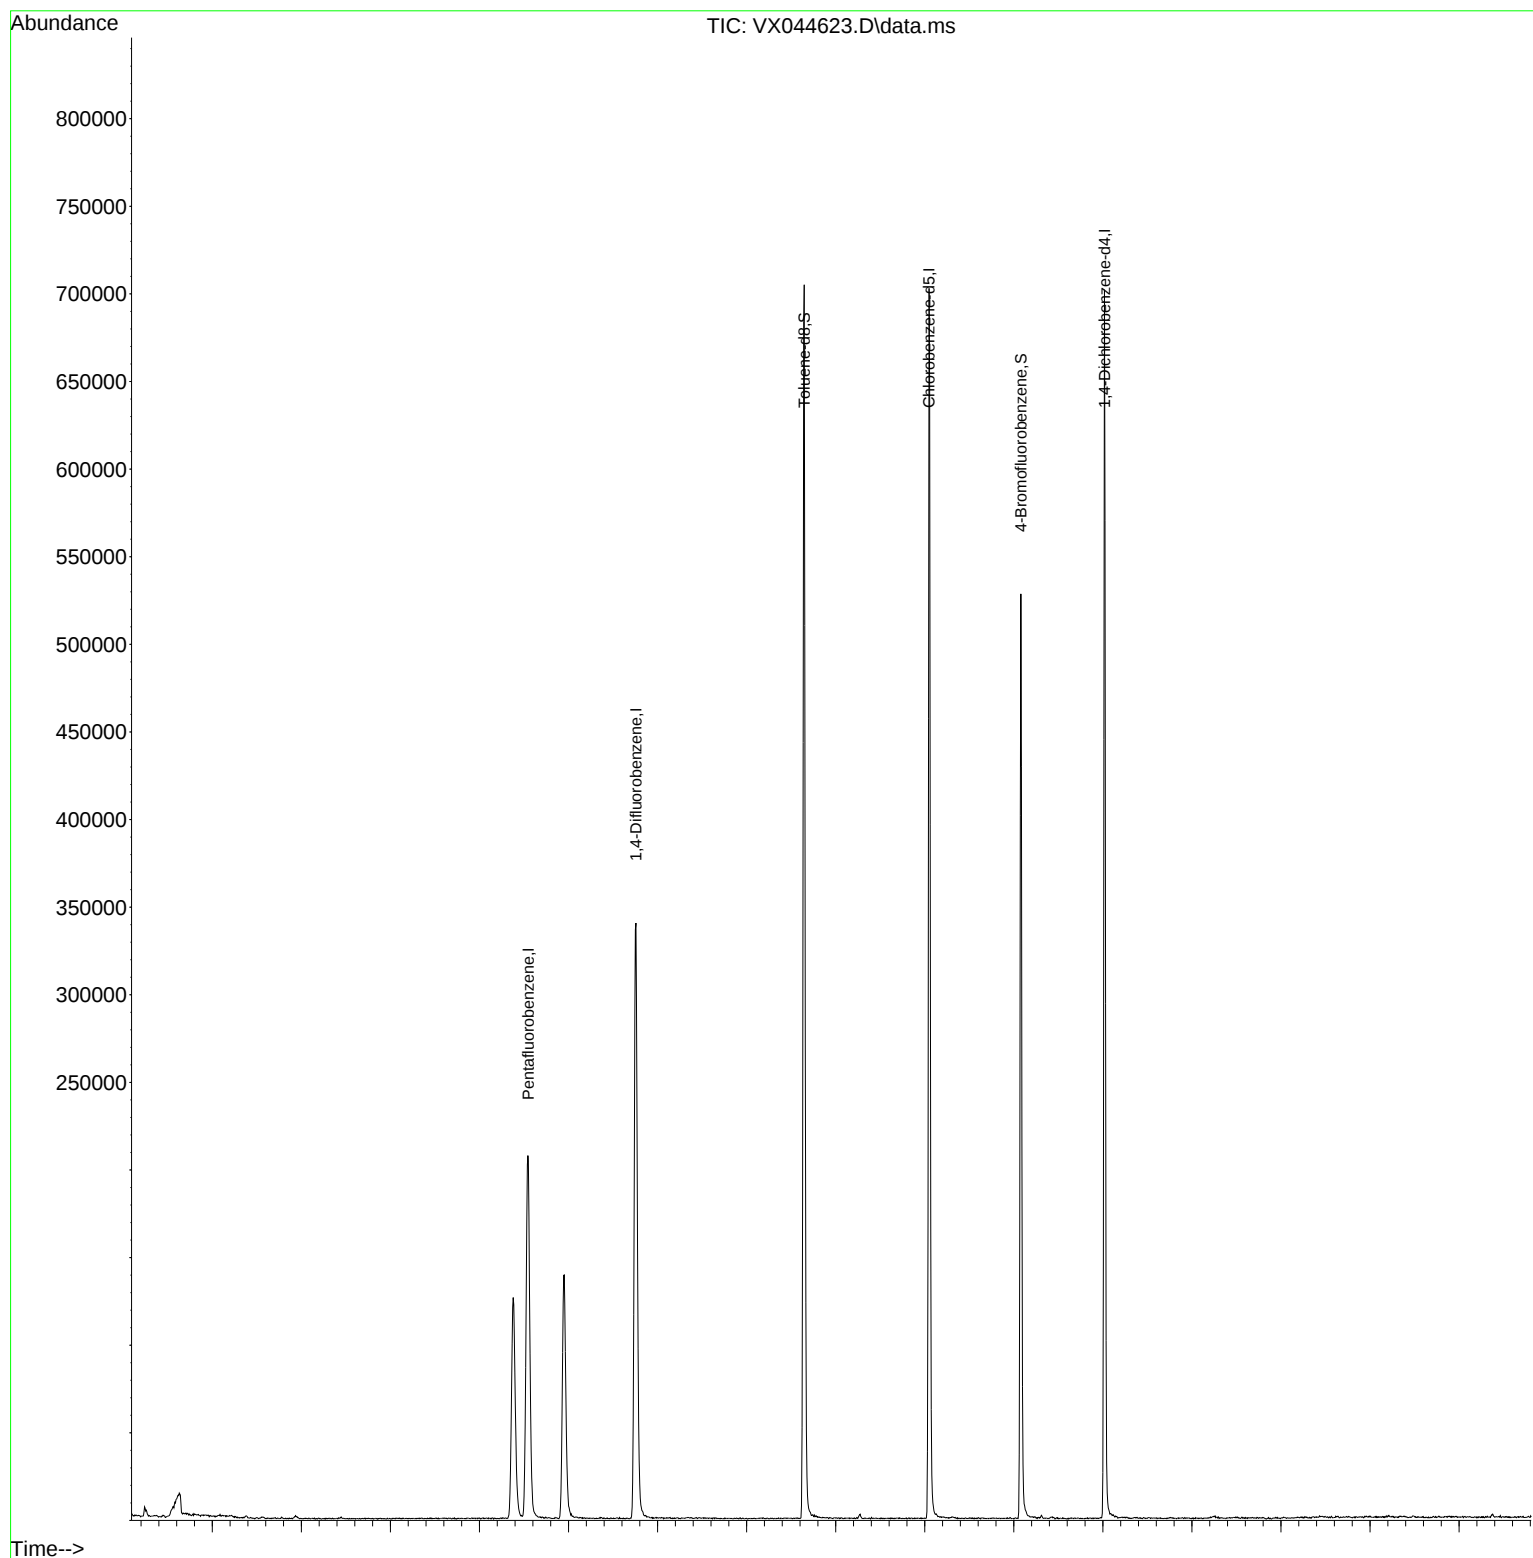






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 731
Delta R.T. 0.006 min
Lab File: VX044623.D
Acq: 08 Jan 2025 13:19

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5



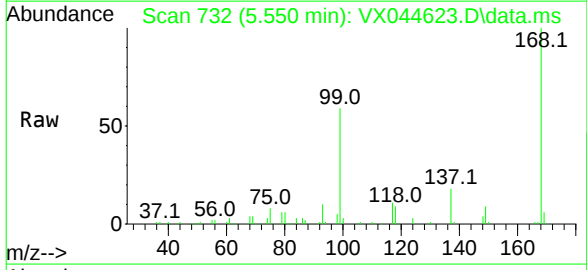



Tgt Ion:168 Resp: 198813
Ion Ratio Lower Upper
168 100
99 58.5 53.5 80.3

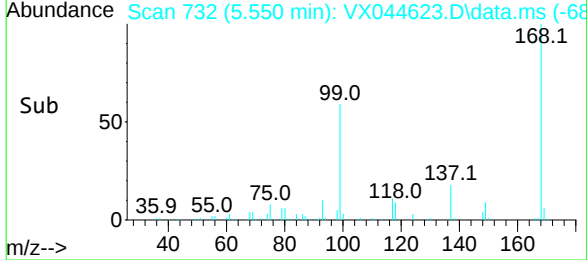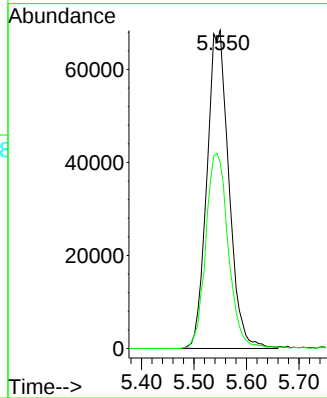

#33
1,2-Dichloroethane-d4
Concen: 43.809 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX044623.D
Acq: 08 Jan 2025 13:19

Tgt Ion: 65 Resp: 140435
Ion Ratio Lower Upper
65 100
67 52.0 0.0 99.0



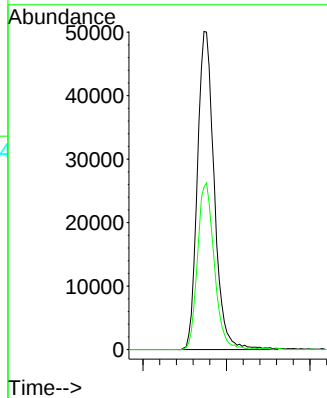
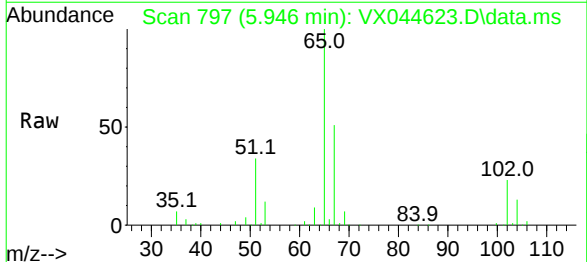


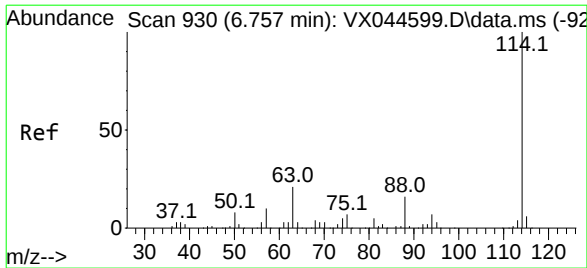

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX044623.D
Acq: 08 Jan 2025 13:19




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:	114	Resp:	364529
Ion	Ratio	Lower	Upper
114	100		
63	19.1	0.0	42.6
88	15.5	0.0	32.6

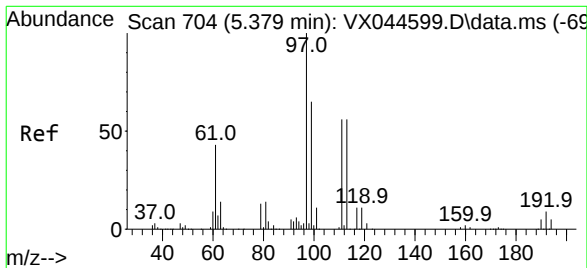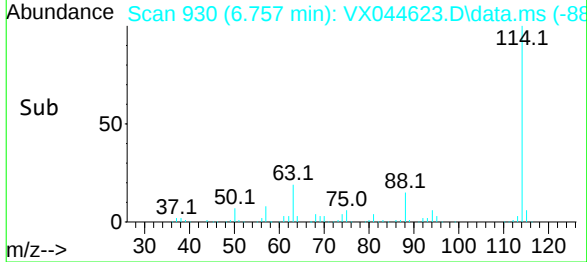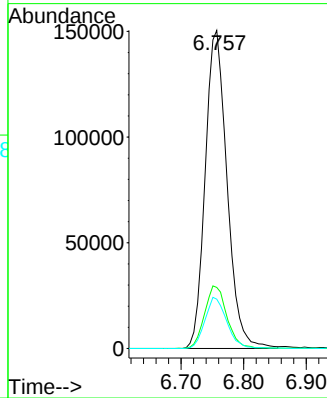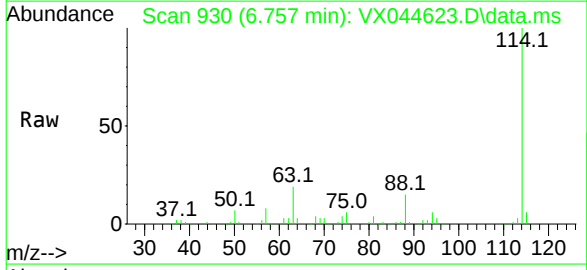

#35
Dibromofluoromethane
Concen: 46.095 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX044623.D
Acq: 08 Jan 2025 13:19

Tgt Ion:	113	Resp:	115221
Ion	Ratio	Lower	Upper
113	100		
111	101.2	83.3	124.9
192	17.4	14.3	21.5

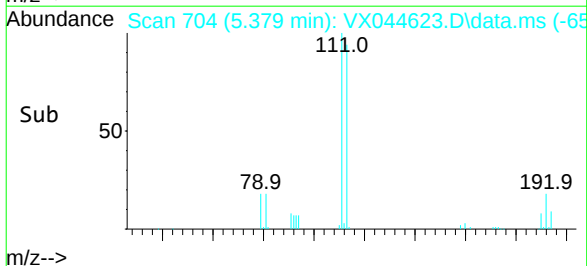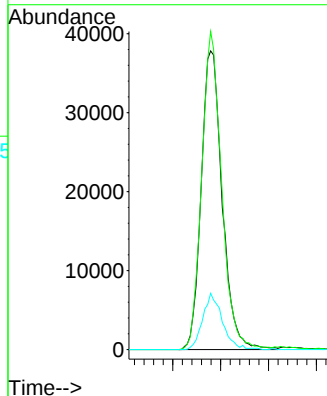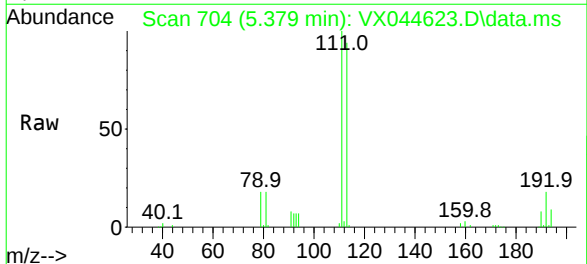

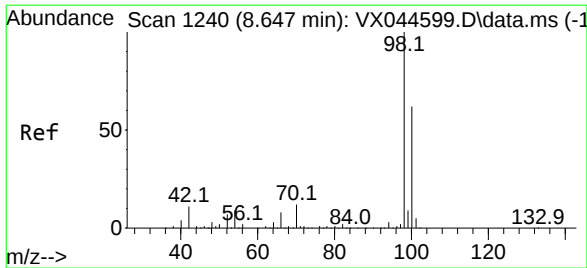

#50

Toluene-d8

Concen: 50.206 ug/l

RT: 8.647 min Scan# 12

Delta R.T. 0.000 min

Lab File: VX044623.D

Acq: 08 Jan 2025 13:19

Instrument :

MSVOA_X

ClientSampleId :





Storage-Blank-WATER-REF-5

Tgt Ion: 98 Resp: 428665

Ion Ratio Lower Upper

98 100

100 66.3 52.5 78.7

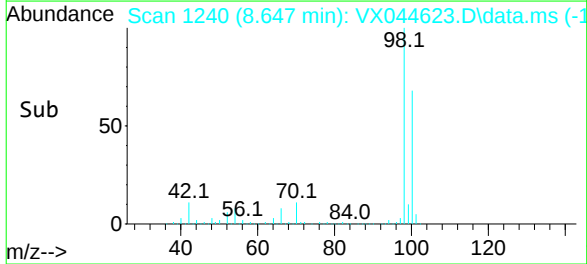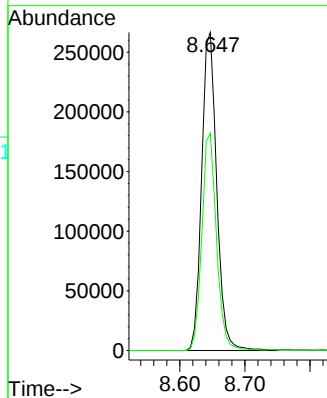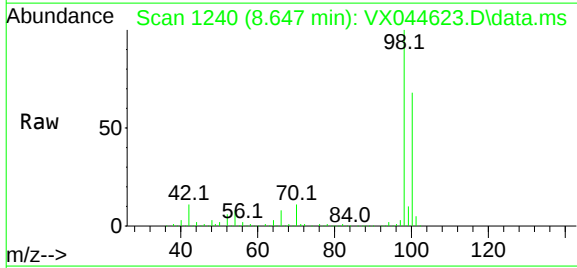

#62

4-Bromofluorobenzene

Concen: 49.540 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX044623.D

Acq: 08 Jan 2025 13:19




Tgt Ion: 95 Resp: 149298


Ion Ratio Lower Upper

95 100

174 75.4 0.0 148.8

176 72.1 0.0 139.8

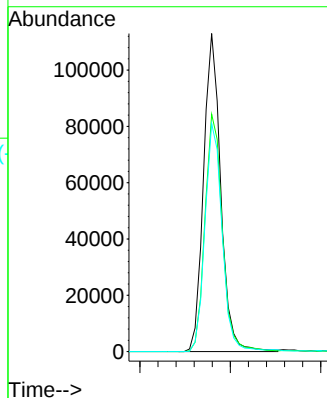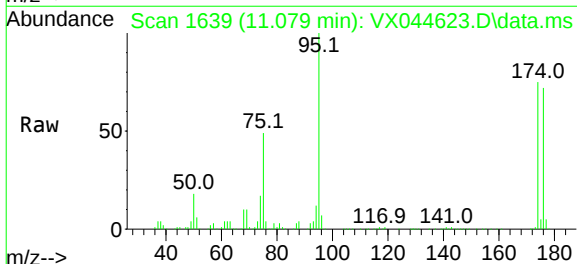

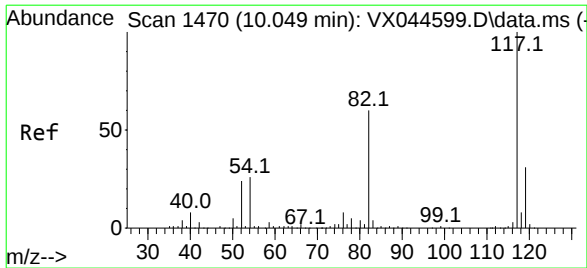

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX044623.D

Acq: 08 Jan 2025 13:19

Instrument :

MSVOA_X

ClientSampleId :

Storage-Blank-WATER-REF-5





Tgt Ion:117 Resp: 328697

Ion Ratio Lower Upper

117 100

82 55.5 47.8 71.6

119 31.4 25.0 37.6

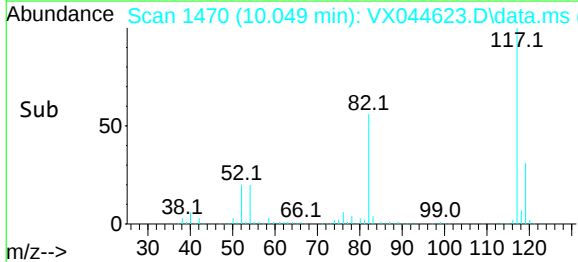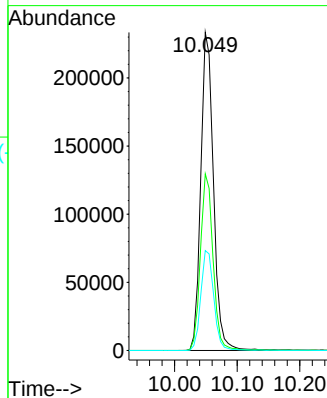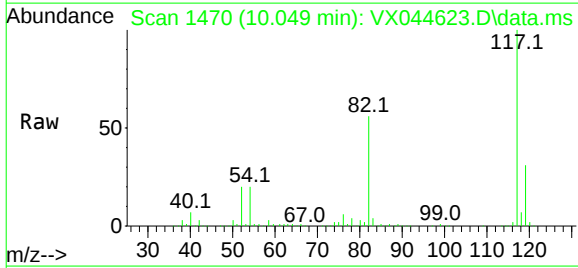

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX044623.D

Acq: 08 Jan 2025 13:19

Tgt Ion:152 Resp: 140600

Ion Ratio Lower Upper

152 100

115 61.3 44.4 133.1

150 157.5 0.0 355.0

