

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010825\
 Data File : VX044624.D
 Acq On : 08 Jan 2025 13:42
 Operator : JC/MD
 Sample : Q1006-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-WATER-REF-4

Quant Time: Jan 09 00:28:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 08 03:57:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	181030	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	329662	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	320820	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	129243	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	147321	50.472	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	100.940%
35) Dibromofluoromethane	5.379	113	104004	46.009	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.020%
50) Toluene-d8	8.647	98	422950	54.775	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	109.560%
62) 4-Bromofluorobenzene	11.079	95	150892	55.365	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	110.720%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010825\
Data File : VX044624.D
Acq On : 08 Jan 2025 13:42
Operator : JC/MD
Sample : Q1006-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-4


Quant Time: Jan 09 00:28:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 08 03:57:12 2025
Response via : Initial Calibration

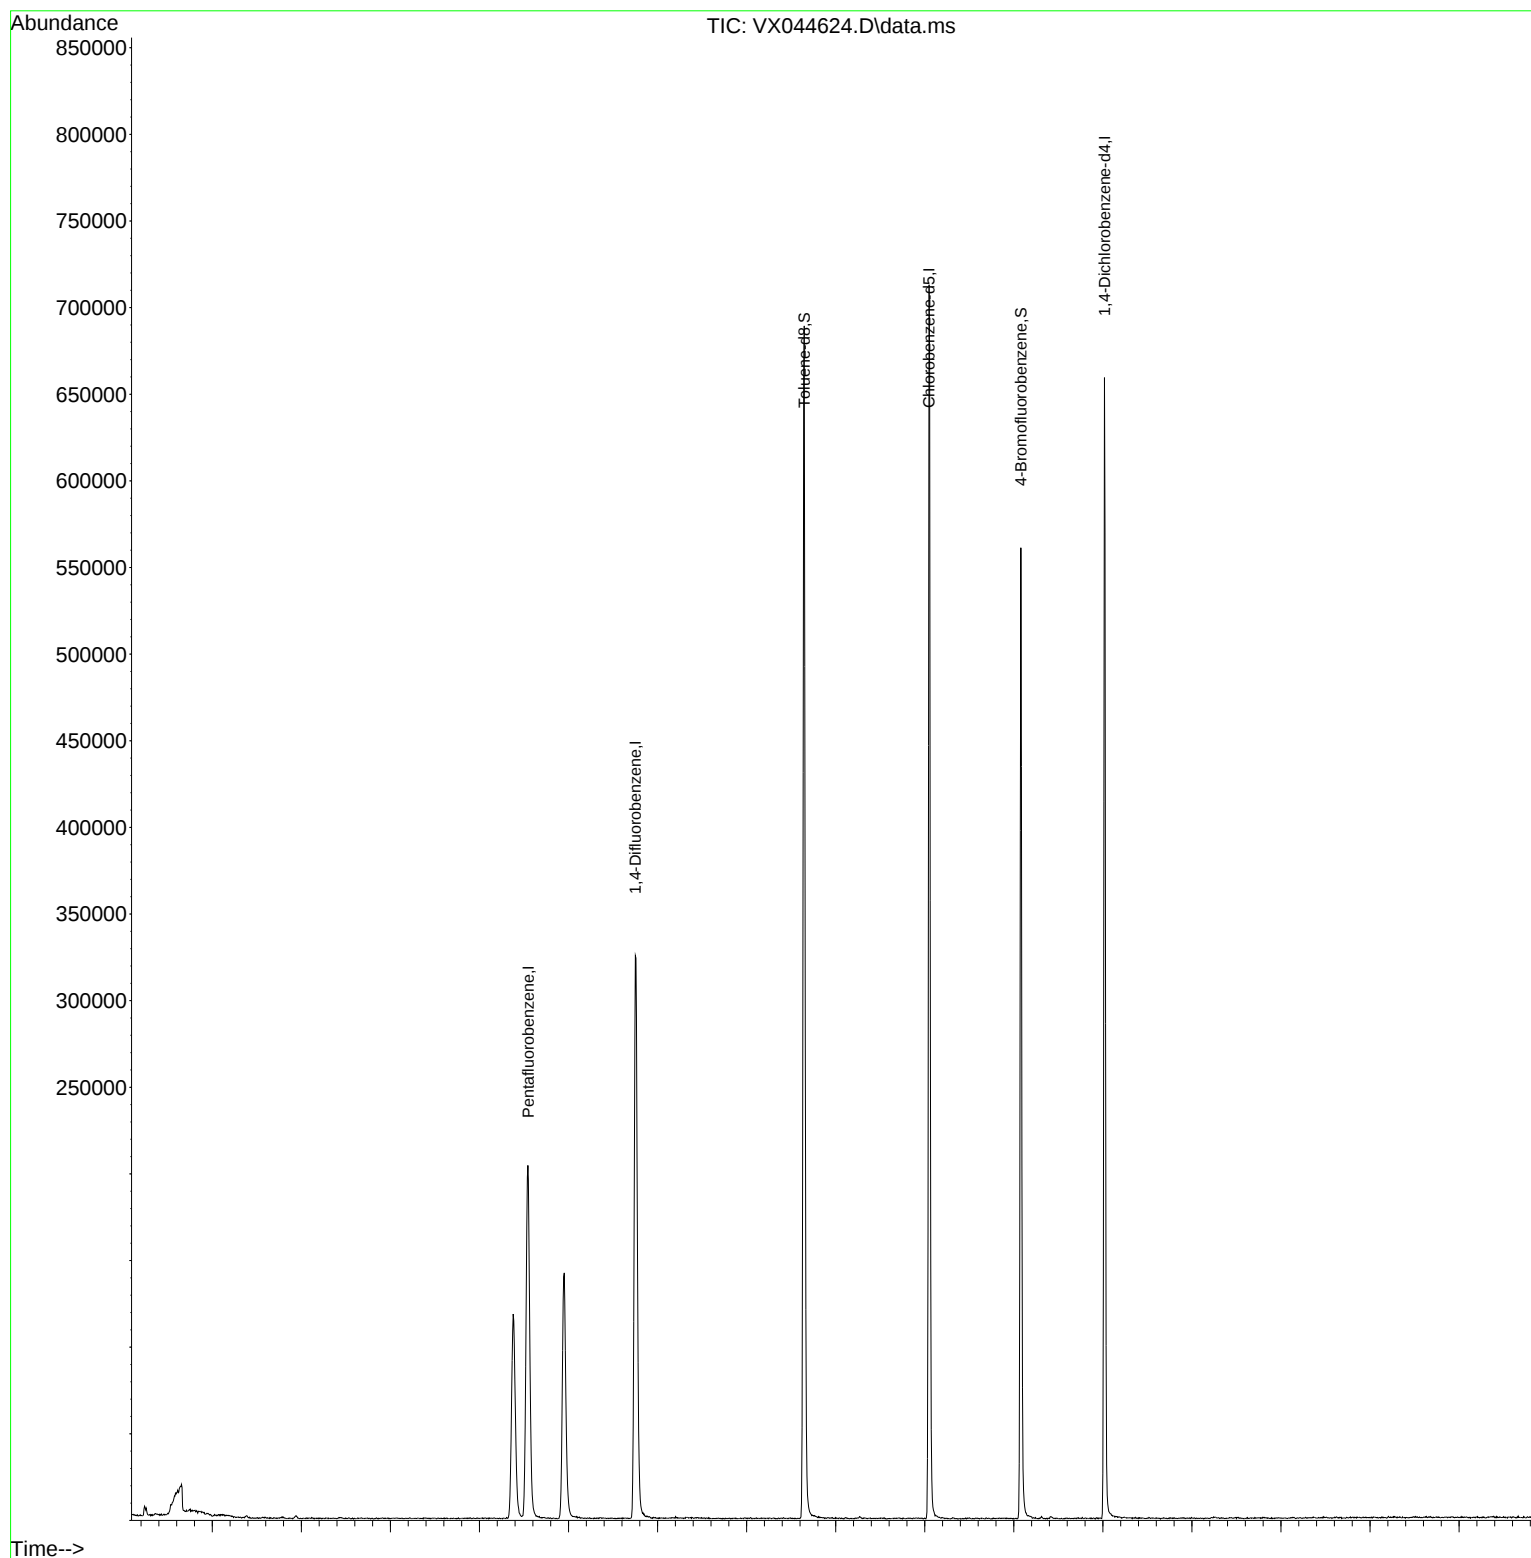



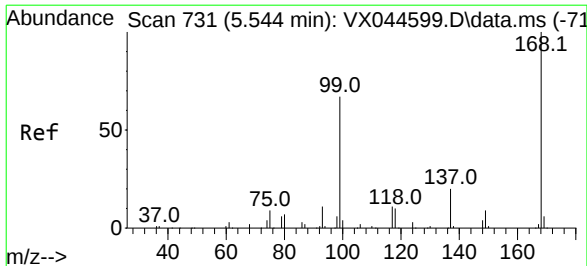


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 731
Delta R.T. 0.006 min
Lab File: VX044624.D
Acq: 08 Jan 2025 13:42

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-4



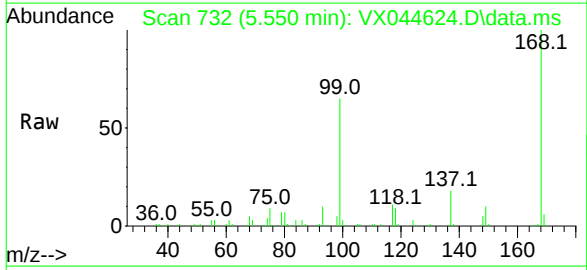



Tgt Ion:168 Resp: 181030
Ion Ratio Lower Upper
168 100
99 65.2 53.5 80.3

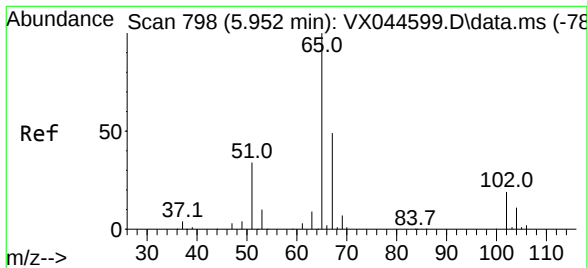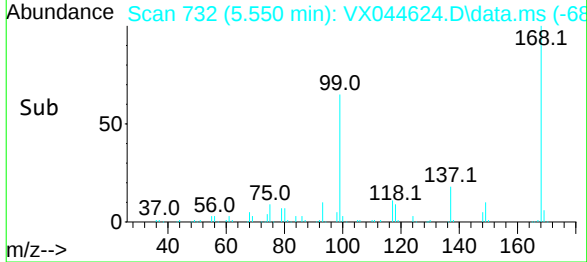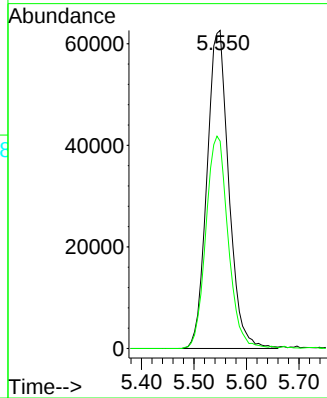

#33
1,2-Dichloroethane-d4
Concen: 50.472 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX044624.D
Acq: 08 Jan 2025 13:42

Tgt Ion: 65 Resp: 147321
Ion Ratio Lower Upper
65 100
67 49.1 0.0 99.0


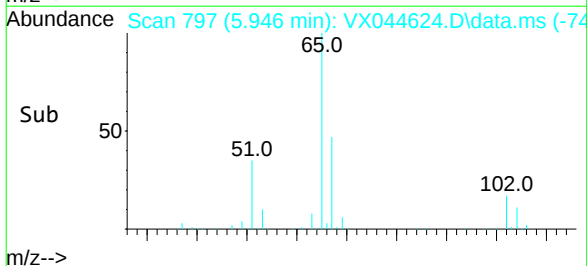
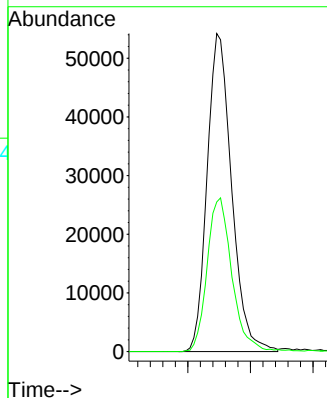
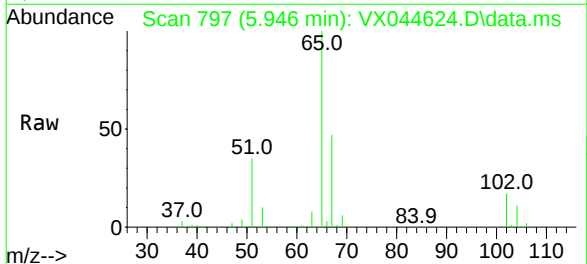


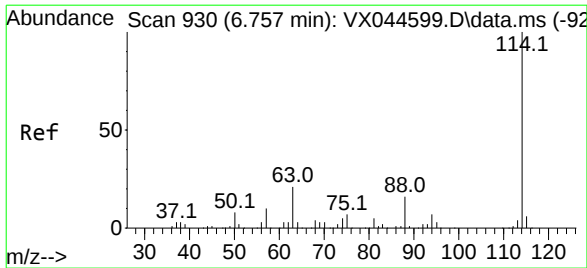

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 92
Delta R.T. -0.006 min
Lab File: VX044624.D
Acq: 08 Jan 2025 13:42




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-4


Tgt Ion:	114	Resp:	329662
Ion	Ratio	Lower	Upper
114	100		
63	21.5	0.0	42.6
88	16.2	0.0	32.6

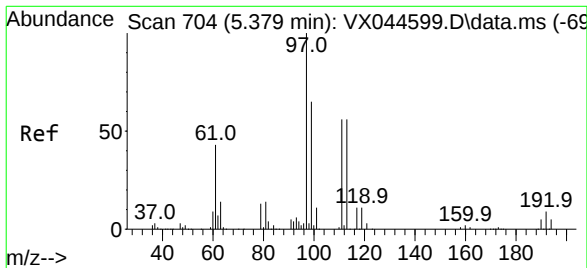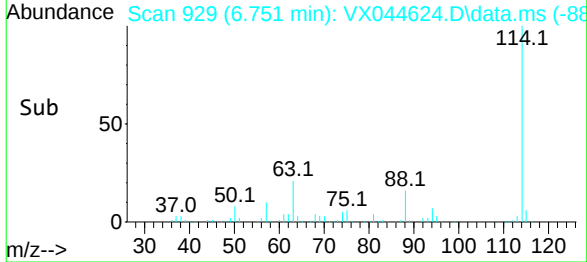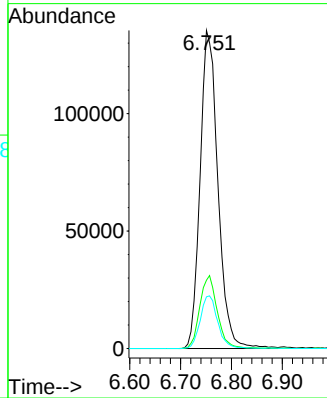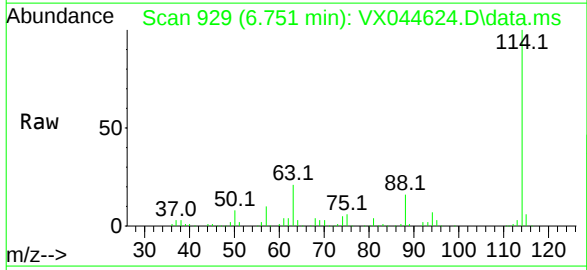

#35
Dibromofluoromethane
Concen: 46.009 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX044624.D
Acq: 08 Jan 2025 13:42

Tgt Ion:	113	Resp:	104004
Ion	Ratio	Lower	Upper
113	100		
111	103.4	83.3	124.9
192	18.4	14.3	21.5

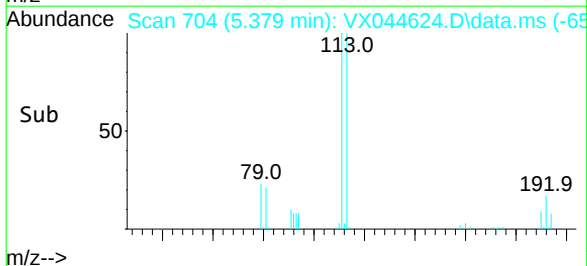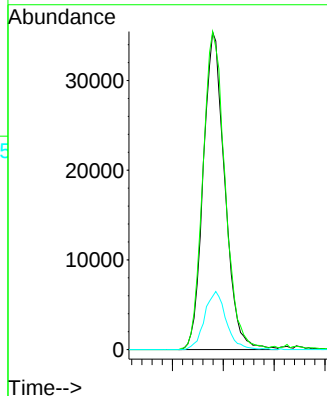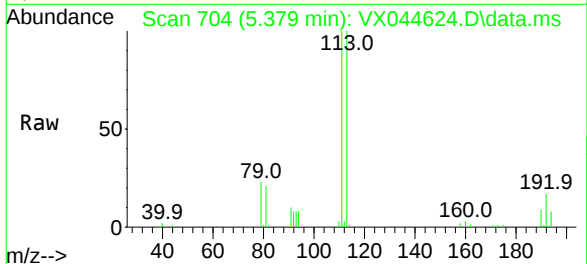

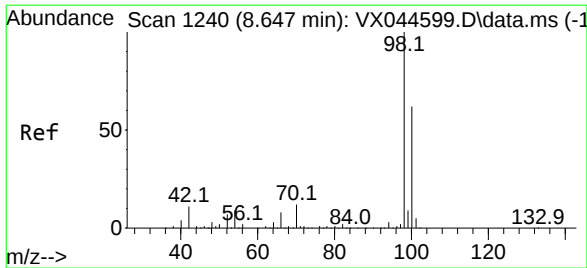

#50

Toluene-d8

Concen: 54.775 ug/l

RT: 8.647 min Scan# 12

Delta R.T. 0.000 min

Lab File: VX044624.D

Acq: 08 Jan 2025 13:42

Instrument :

MSVOA_X

ClientSampleId :





Storage-Blank-WATER-REF-4

Tgt Ion: 98 Resp: 422950

Ion Ratio Lower Upper

98 100

100 65.2 52.5 78.7

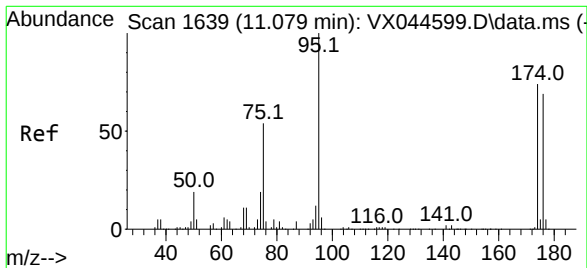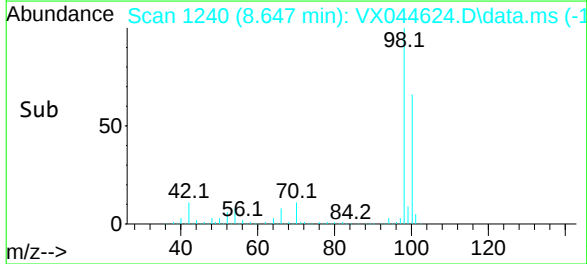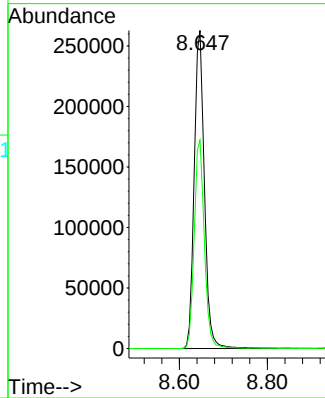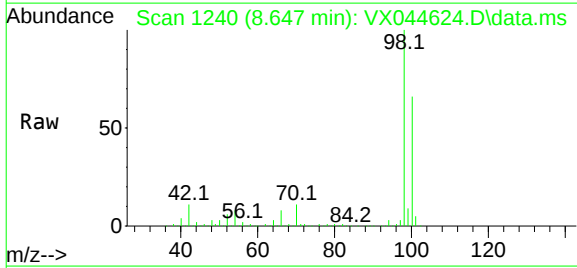

#62

4-Bromofluorobenzene

Concen: 55.365 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX044624.D

Acq: 08 Jan 2025 13:42




Tgt Ion: 95 Resp: 150892


Ion Ratio Lower Upper

95 100

174 75.3 0.0 148.8

176 71.9 0.0 139.8

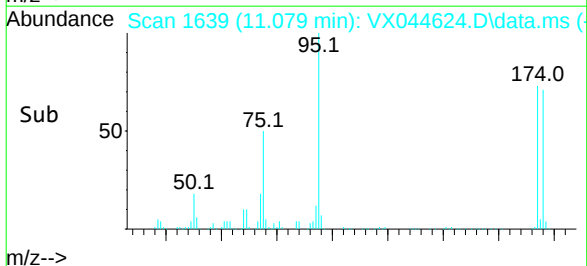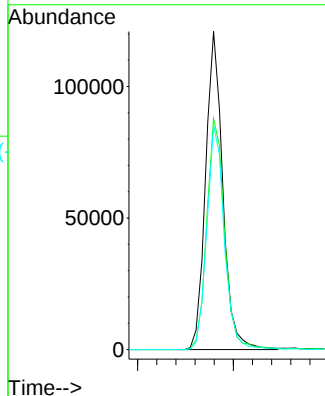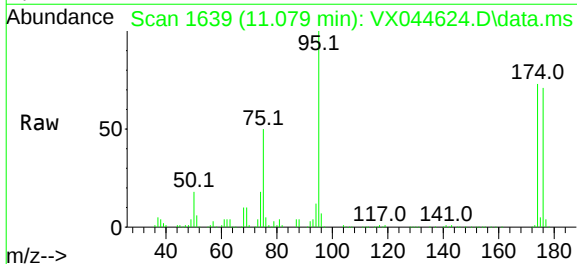

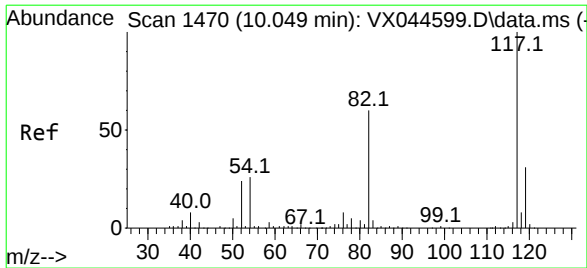

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX044624.D

Acq: 08 Jan 2025 13:42





Instrument :

MSVOA_X

ClientSampleId :

Storage-Blank-WATER-REF-4

Tgt Ion:	117	Resp:	320820
Ion	Ratio	Lower	Upper
117	100		
82	56.3	47.8	71.6
119	32.1	25.0	37.6

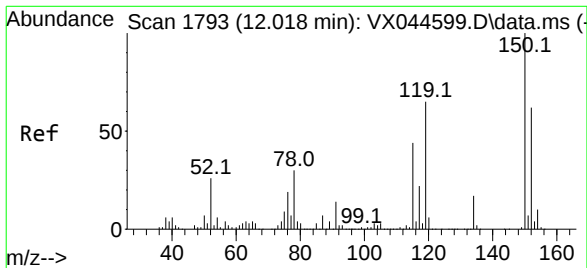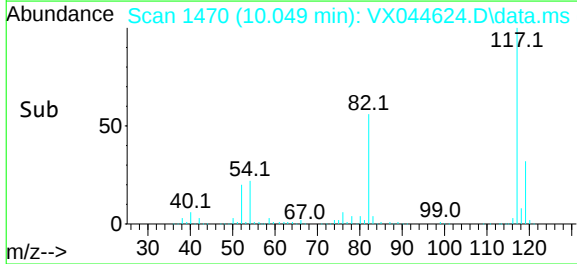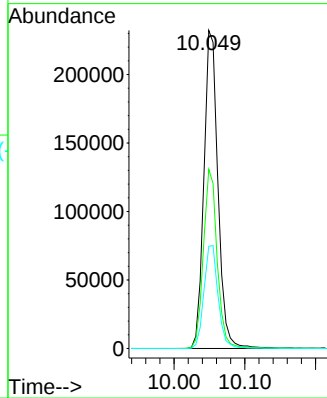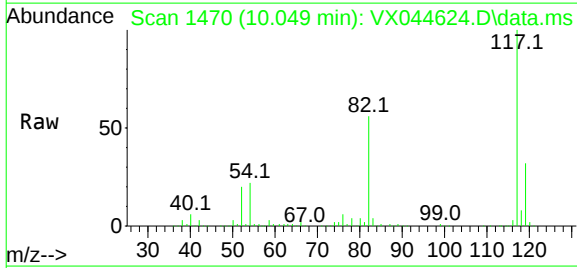

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX044624.D

Acq: 08 Jan 2025 13:42

Tgt Ion:	152	Resp:	129243
Ion	Ratio	Lower	Upper
152	100		
115	63.1	44.4	133.1
150	157.9	0.0	355.0

