
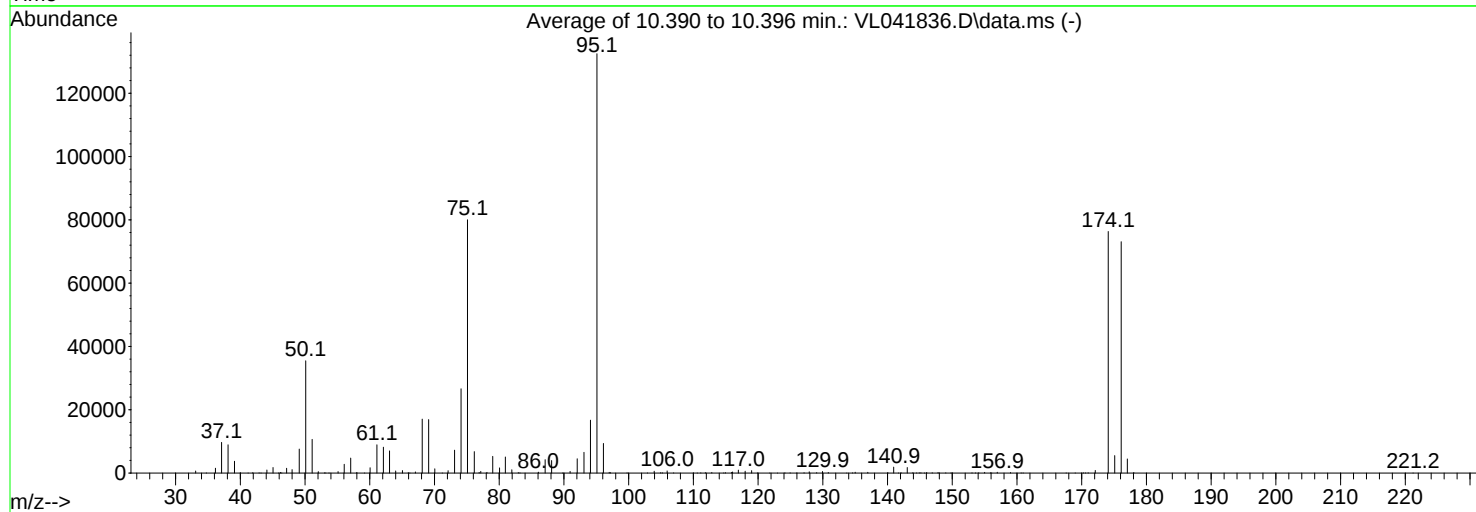


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL010725\
Data File : VL041836.D
Acq On : 07 Jan 2025 08:06
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL010725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Jan 08 03:26:12 2025

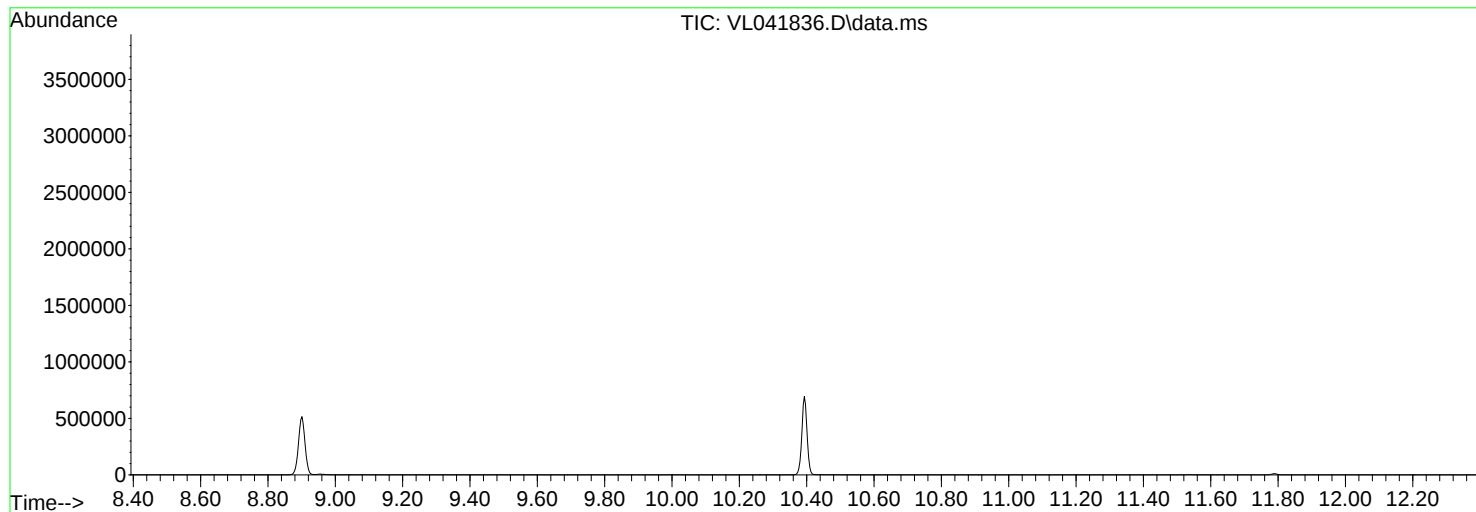

AutoFind: Scans 3183, 3184, 3185; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.8	35475	PASS
75	95	30	66	60.4	80027	PASS
95	95	100	100	100.0	132480	PASS
96	95	5	9	7.1	9366	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	57.6	76320	PASS
175	174	4	9	7.2	5523	PASS
176	174	93	101	95.8	73091	PASS
177	176	5	9	6.1	4466	PASS

Average of 10.390 to 10.396 min.: VL041836.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	650	44.10	978	53.00	75	63.05	7000
34.75	41	45.05	1757	53.20	63	64.00	665
36.15	1528	45.90	22	53.70	54	65.05	797
37.10	9699	46.20	204	55.10	476	65.95	128
38.10	8943	46.40	63	56.05	2780	66.20	47
39.10	3730	47.15	1514	57.05	4728	67.05	373
40.00	97	48.00	1099	58.00	215	68.10	17043
41.20	25	49.10	7584	59.20	38	69.10	16889
41.90	88	50.10	35475	60.05	1686	70.05	1350
42.90	86	51.10	10644	61.10	8934	71.20	28
43.20	24	52.05	463	62.10	8179	72.10	752

Average of 10.390 to 10.396 min.: VL041836.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	7232	82.95	157	96.10	9366	110.60	37
74.10	26627	83.20	86	97.00	230	111.15	73
75.10	80027	86.05	297	97.20	136	111.85	144
76.15	6787	87.10	4239	99.75	57	112.85	187
76.90	201	88.10	3966	102.90	43	114.70	42
77.15	541	89.80	23	103.95	599	114.95	130
78.10	233	90.95	542	104.95	132	115.90	216
79.00	5275	92.05	4523	105.20	90	116.05	350
80.05	1633	93.10	6550	105.95	691	116.95	943
80.95	5086	94.10	16713	106.95	57	118.00	594
81.95	1044	95.10	132480	110.00	19	119.00	783

Average of 10.390 to 10.396 min.: VL041836.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.90	26	133.70	21	144.90	98	153.60	41
121.80	18	134.60	84	145.15	117	154.10	73
123.00	19	135.00	283	145.70	34	155.00	235
124.15	63	136.95	243	146.05	179	155.90	101
124.95	74	140.05	139	146.90	112	156.10	50
126.00	66	140.95	1883	147.80	168	156.95	262
127.10	108	141.70	30	148.00	44	159.00	164
127.90	421	142.10	93	149.00	83	160.65	71
129.05	149	143.05	1759	149.80	63	160.95	46
129.95	505	143.90	98	150.00	63	167.60	43
130.85	190	144.50	42	153.05	81	169.00	46

Average of 10.390 to 10.396 min.: VL041836.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.25	76						
170.60	47						
171.00	92						
172.10	833						
174.10	76320						
175.10	5523						
176.10	73091						
177.05	4466						
178.05	171						
221.20	24						

Instrument :

MSVOA_L

ClientSampleId :

BFB