


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011025\
Data File : BN035903.D
Acq On : 10 Jan 2025 12:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

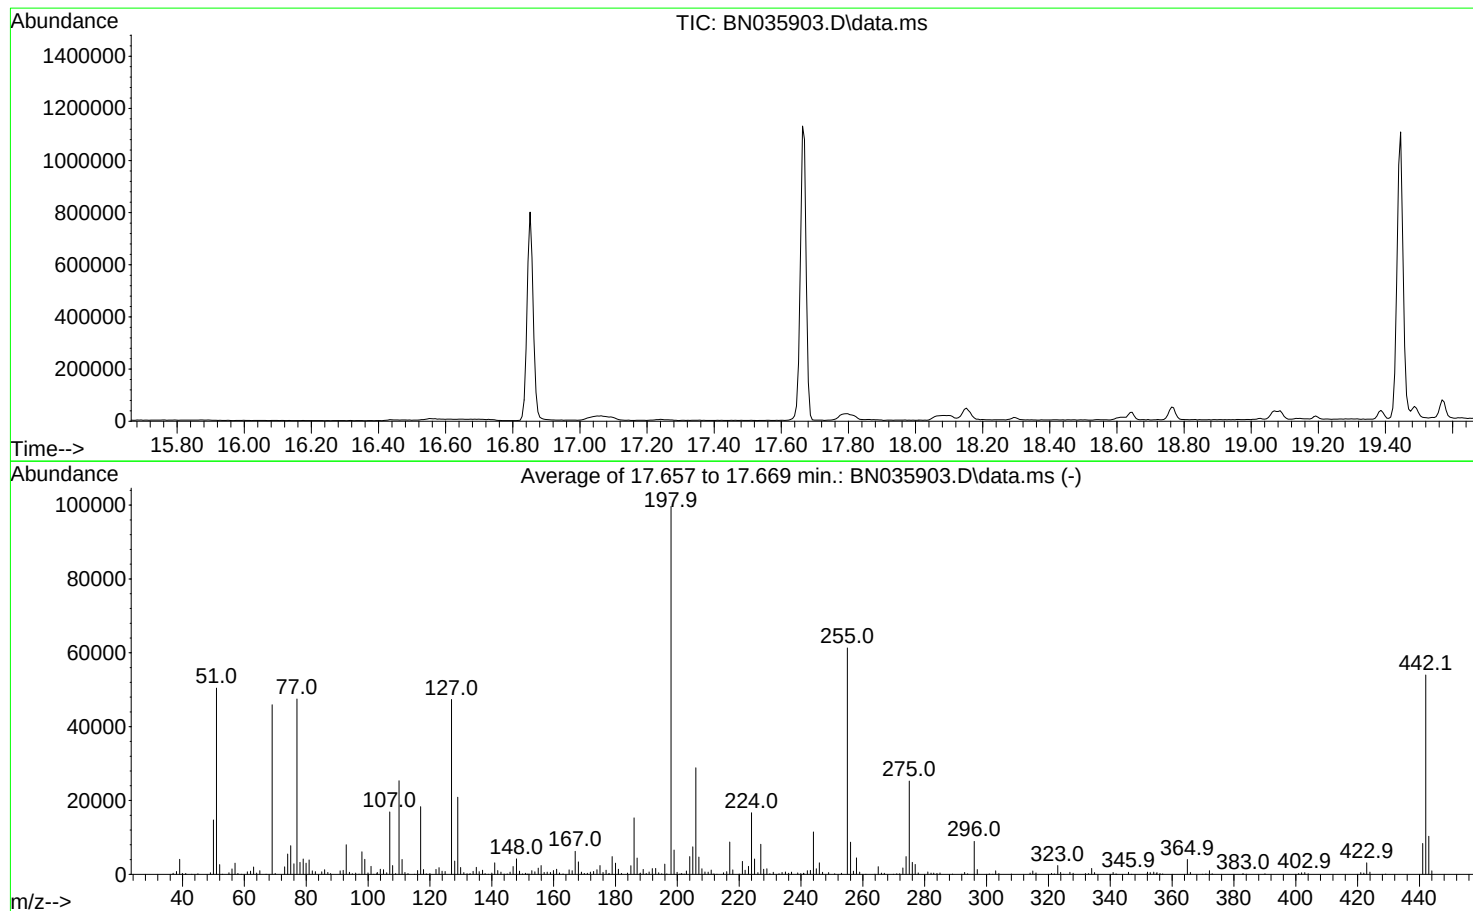

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	50453	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.1	45952	PASS
70	69	0.00	2	0.6	270	PASS
127	198	10	80	47.5	47347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99619	PASS
199	198	5	9	6.6	6598	PASS
275	198	10	60	25.4	25286	PASS
365	198	1	100	4.0	4026	PASS
441	198	0.01	100	8.4	8350	PASS
442	442	50	100	100.0	53997	PASS
443	442	15	24	19.1	10302	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/10/2025	BNA_N	<u>BN035903.D</u>
Compound Name	Response	Retention Time
DDT	276232	20.692
DDD	3896	20.245
DDE	164	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4060	280292	1.45

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011025\
Data File : BN035903.D
Acq On : 10 Jan 2025 12:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 17:41:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

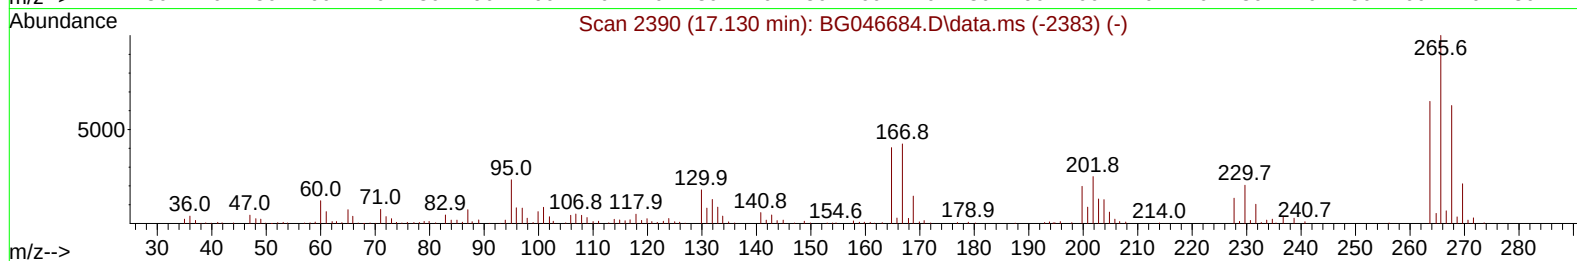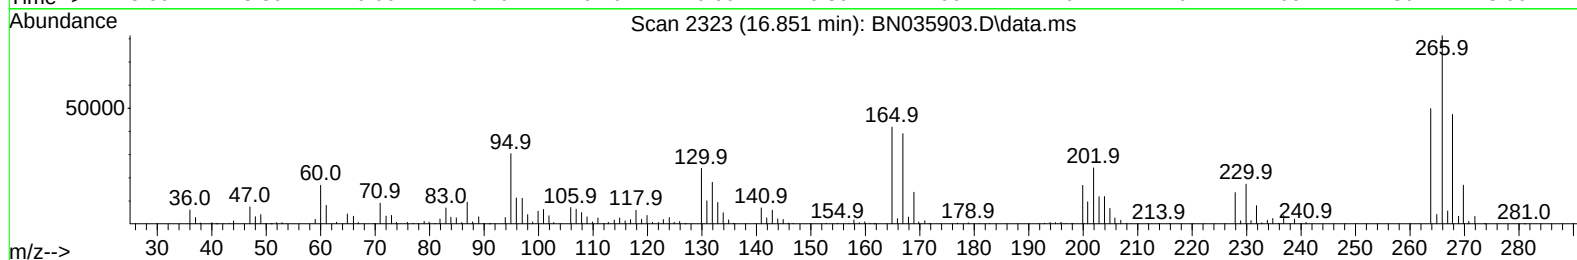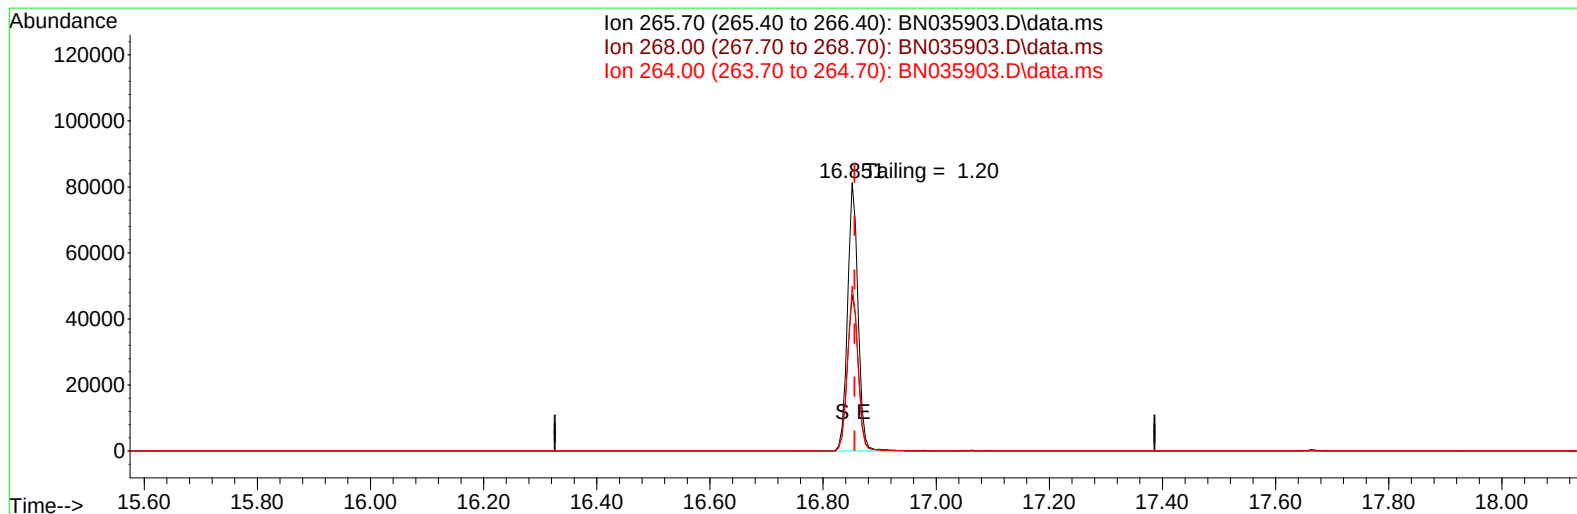

TIC: BN035903.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.005) 23526.14 ng




response 104499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.18
264.00	61.60	61.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011025\
Data File : BN035903.D
Acq On : 10 Jan 2025 12:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 17:41:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

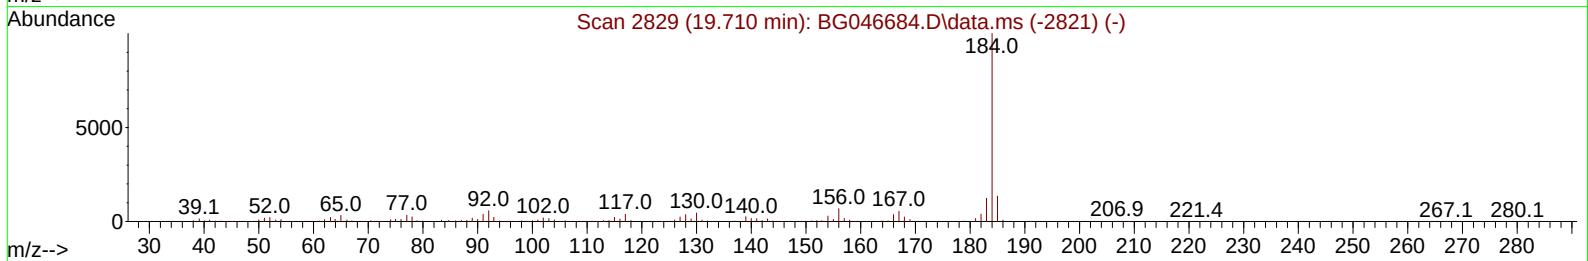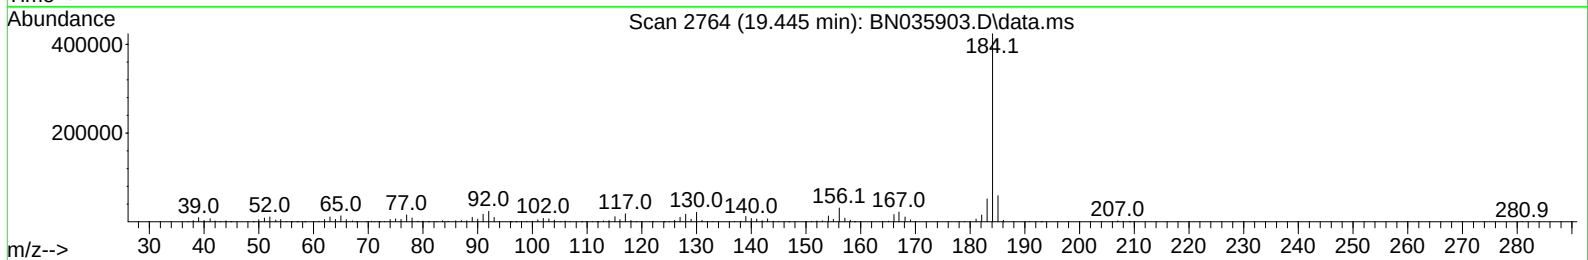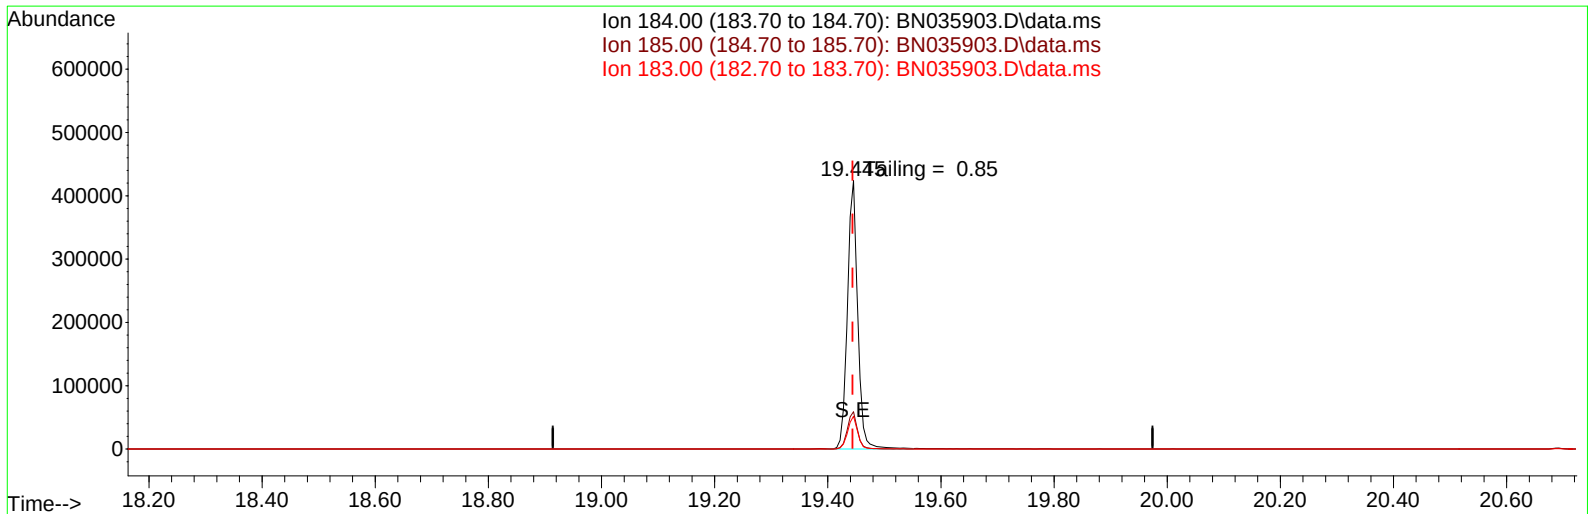

TIC: BN035903.D\data.ms

(77) Benzidine

19.445min (+ 0.001) 0.00 ng

response 537267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	12.22
0.00	0.00	0.00