
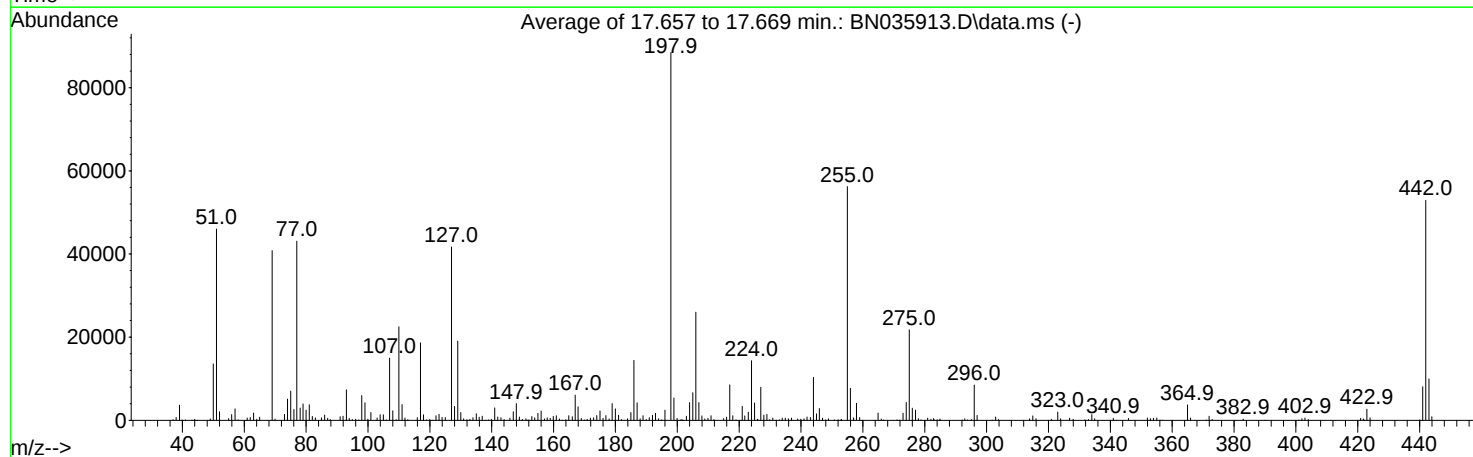


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011325\
Data File : BN035913.D
Acq On : 13 Jan 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

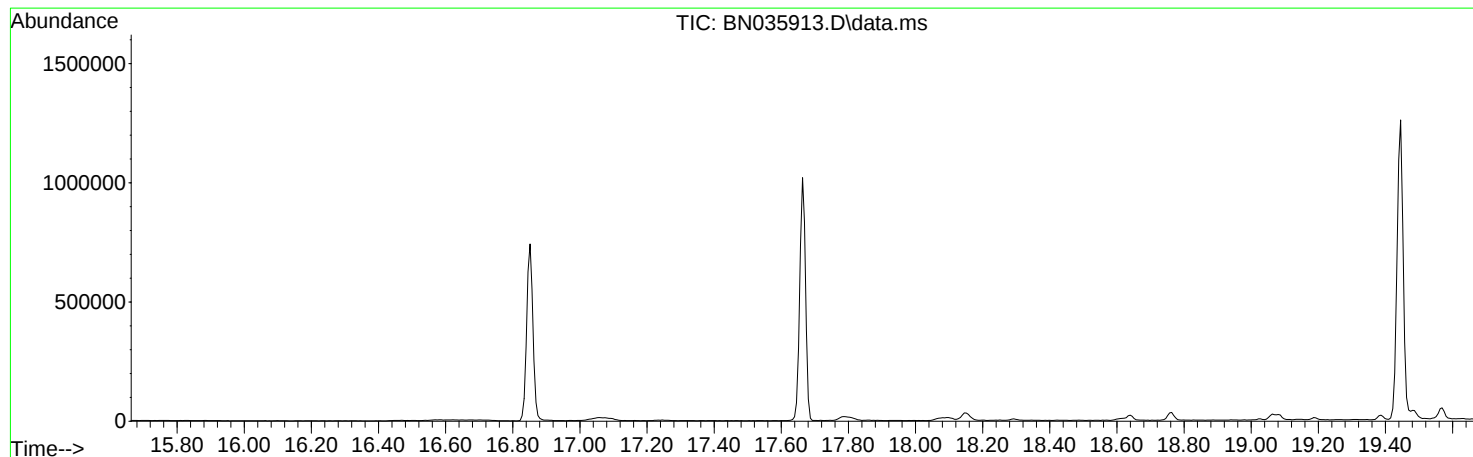




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	46029	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.2	40824	PASS
70	69	0.00	2	0.7	306	PASS
127	198	10	80	47.1	41691	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88453	PASS
199	198	5	9	6.1	5379	PASS
275	198	10	60	24.6	21773	PASS
365	198	1	100	4.2	3737	PASS
441	198	0.01	100	9.2	8095	PASS
442	442	50	100	100.0	52923	PASS
443	442	15	24	18.8	9949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011325\
Data File : BN035913.D
Acq On : 13 Jan 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 13 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

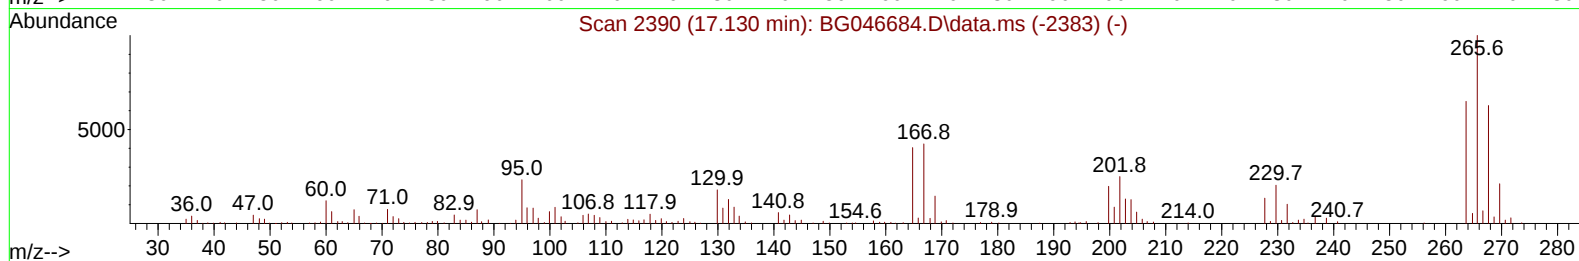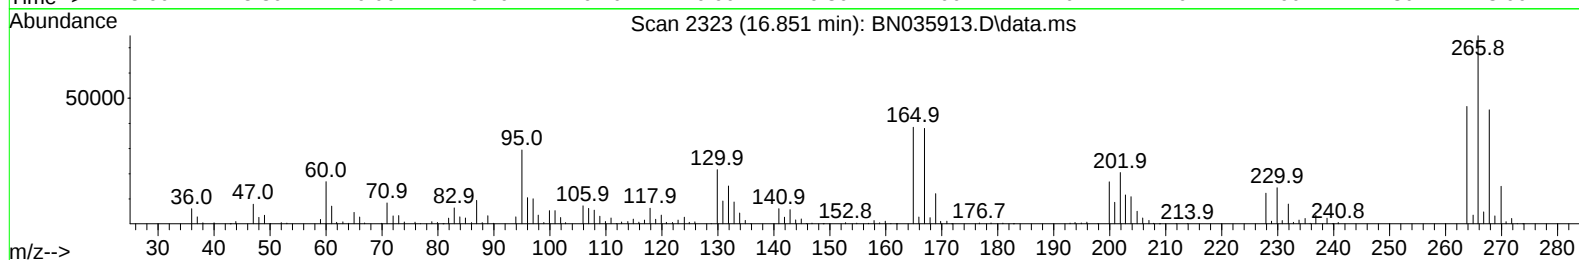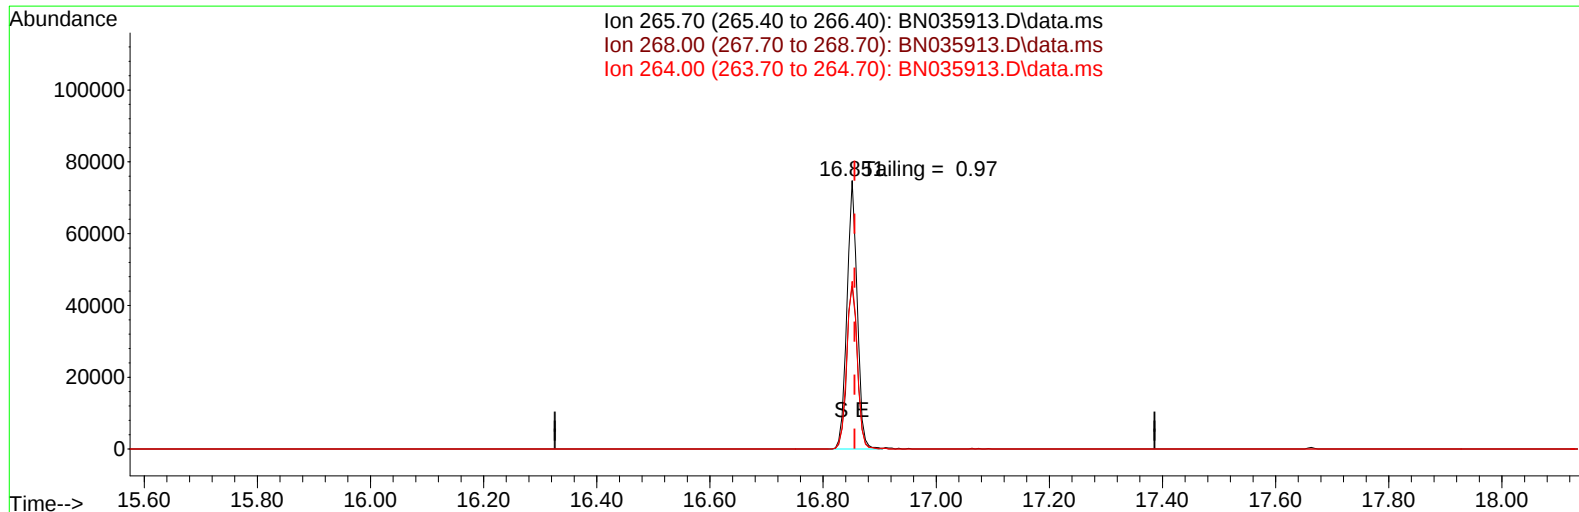

TIC: BN035913.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.005) 22555.44 ng




response 94169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.71
264.00	61.60	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011325\
Data File : BN035913.D
Acq On : 13 Jan 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 13 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

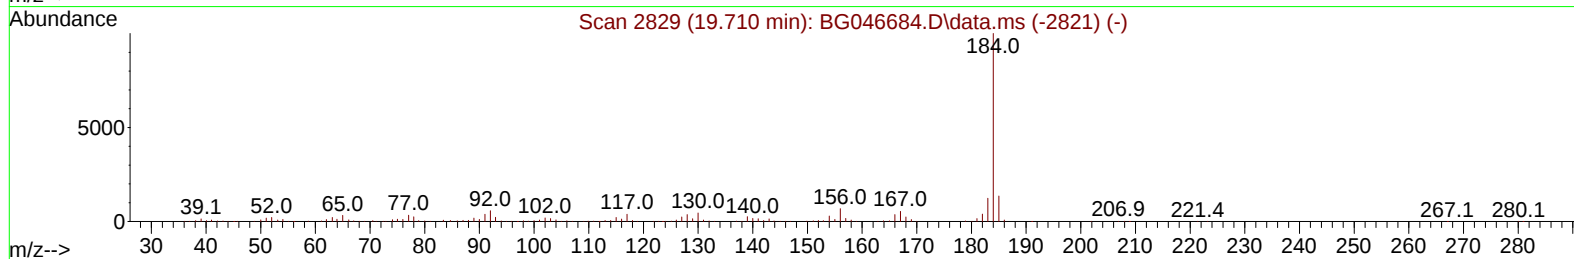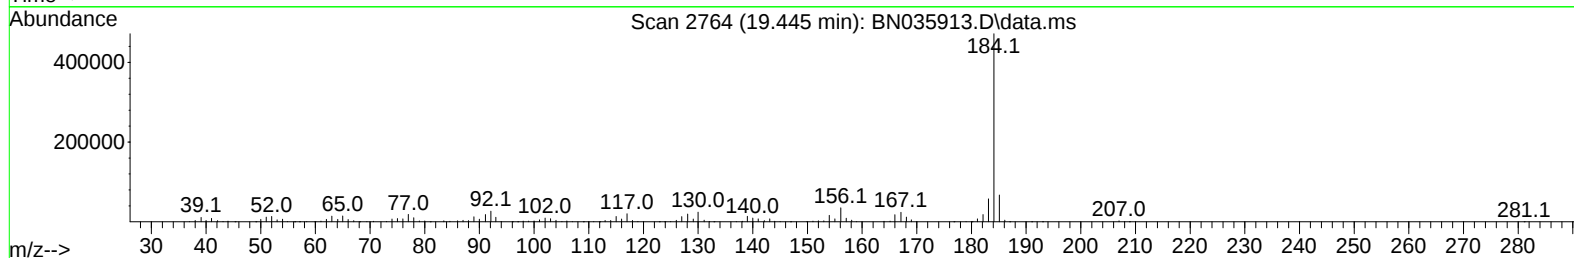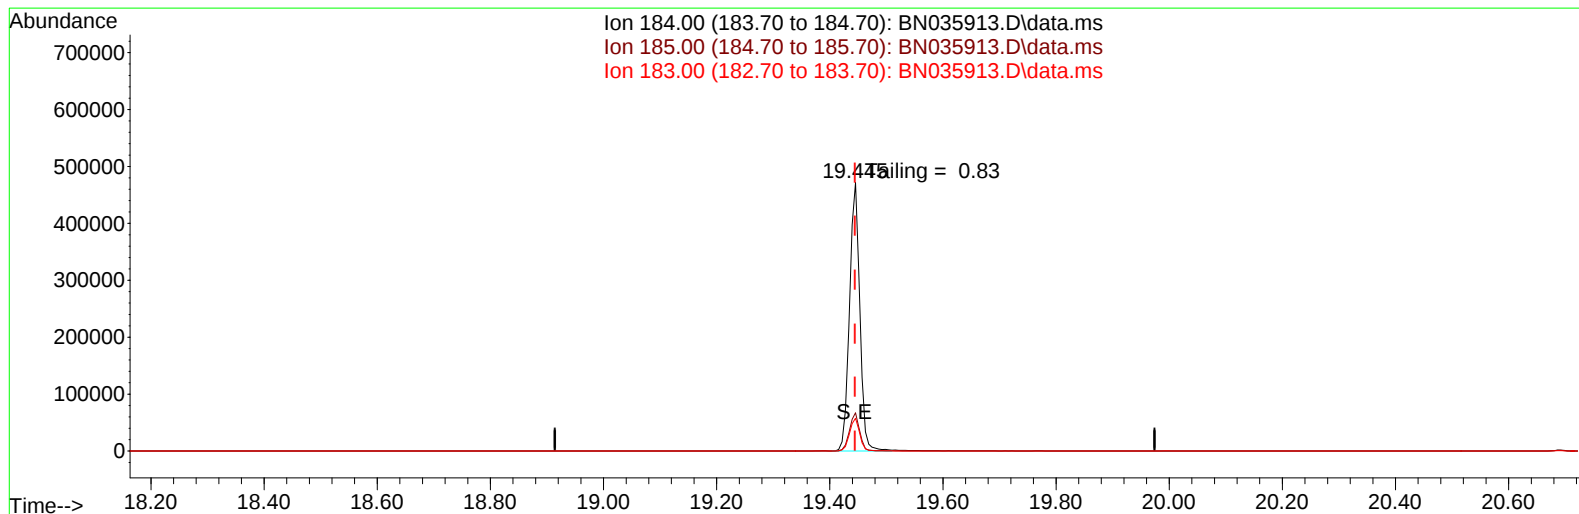

TIC: BN035913.D\data.ms

(77) Benzidine

19.445min (+ 0.001) 0.00 ng

response 602465

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2025	BNA_N	<u>BN035913.D</u>
Compound Name	Response	Retention Time
DDT	304929	20.692
DDD	4176	20.304
DDE	278	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4454	309383	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP