Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011425\
Data File : VN085443.D
Acq On : 14 Jan 2025 17:19
Operator : JC\MD
Sample : VSTDICC001
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 15 01:46:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 01:28:51 2025
Response via : Initial Calibration

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Compound	R.T.	QIon	Response	Conc	Units		Dev(Min)
Internal Standards							
1) Pentafluorobenzene	8.224	168	166880	50.000	ug/l		0.00
34) 1,4-Difluorobenzene	9.100	114	302938	50.000	ug/l		0.00
63) Chlorobenzene-d5	11.865	117	256851	50.000	ug/l		0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	99539	50.000	ug/l		0.00
System Monitoring Compounds							
33) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/l		
Spiked Amount 50.000	Range 74 - 125		Recovery =	0.000%#			
35) Dibromofluoromethane	0.000	113	0d	0.000	ug/l		
Spiked Amount 50.000	Range 75 - 124		Recovery =	0.000%#			
50) Toluene-d8	0.000	98	0d	0.000	ug/l		
Spiked Amount 50.000	Range 86 - 113		Recovery =	0.000%#			
62) 4-Bromofluorobenzene	0.000	95	0d	0.000	ug/l		
Spiked Amount 50.000	Range 77 - 121		Recovery =	0.000%#			
Target Compounds							Qvalue
2) Dichlorodifluoromethane	2.124	85	2382	1.054	ug/l		91
3) Chloromethane	2.359	50	2801	1.145	ug/l		93
4) Vinyl Chloride	2.512	62	2732	1.111	ug/l	#	81
6) Chloroethane	3.124	64	1809	1.160	ug/l		94
7) Trichlorofluoromethane	3.512	101	3860	1.082	ug/l		88
8) Diethyl Ether	3.953	74	1526	1.238	ug/l		81
9) 1,1,2-Trichlorotrifluo...	4.359	101	2156m	1.073	ug/l		
12) 1,1-Dichloroethene	4.330	96	1660	0.927	ug/l	#	67
14) Allyl chloride	5.024	41	3179	1.094	ug/l	#	85
15) Acrylonitrile	5.718	53	4967	5.070	ug/l	#	70
16) Acetone	4.436	43	5102	5.862	ug/l		92
17) Carbon Disulfide	4.706	76	6601	1.197	ug/l	#	87
18) Methyl Acetate	5.030	43	2908	1.099	ug/l	#	80
19) Methyl tert-butyl Ether	5.789	73	5156	0.887	ug/l	#	87
20) Methylene Chloride	5.265	84	2190	1.016	ug/l	#	87
21) trans-1,2-Dichloroethene	5.794	96	2110	1.102	ug/l	#	66
22) Diisopropyl ether	6.677	45	5691	0.882	ug/l	#	88
23) Vinyl Acetate	6.606	43	18526m	4.090	ug/l		
24) 1,1-Dichloroethane	6.583	63	4020m	1.022	ug/l		
25) 2-Butanone	7.483	43	6448m	5.034	ug/l		
26) 2,2-Dichloropropane	7.488	77	3104	0.976	ug/l		92
27) cis-1,2-Dichloroethene	7.477	96	2185	0.969	ug/l		92
28) Bromochloromethane	7.812	49	2082	1.138	ug/l	#	89
29) Tetrahydrofuran	7.835	42	3693	4.548	ug/l		98
30) Chloroform	7.965	83	4250	1.045	ug/l	#	80
32) 1,1,1-Trichloroethane	8.165	97	3678	1.031	ug/l	#	56
36) 1,1-Dichloropropene	8.371	75	3084	1.046	ug/l	#	84
37) Ethyl Acetate	7.577	43	3056m	1.026	ug/l		
38) Carbon Tetrachloride	8.359	117	3436	1.018	ug/l		90
39) Methylcyclohexane	9.600	83	2403	0.867	ug/l	#	87
40) Benzene	8.606	78	8480	0.957	ug/l		91
41) Methacrylonitrile	7.771	41	1458	0.941	ug/l	#	76
42) 1,2-Dichloroethane	8.665	62	3131	0.938	ug/l		91
43) Isopropyl Acetate	8.682	43	4803	1.007	ug/l	#	87
44) Trichloroethene	9.347	130	2133	1.034	ug/l		71
45) 1,2-Dichloropropane	9.618	63	2246	0.992	ug/l		99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011425\
Data File : VN085443.D
Acq On : 14 Jan 2025 17:19
Operator : JC\MD
Sample : VSTDICC001
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 15 01:46:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 01:28:51 2025
Response via : Initial Calibration

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
46) Dibromomethane	9.706	93	1769	1.083 ug/l	92
47) Bromodichloromethane	9.882	83	2935	0.882 ug/l	90
48) Methyl methacrylate	9.677	41	1886	0.878 ug/l	96
49) 1,4-Dioxane	9.688	88	673	18.616 ug/l #	47
51) 4-Methyl-2-Pentanone	10.441	43	11523	4.163 ug/l	93
52) Toluene	10.618	92	4180	0.814 ug/l	93
53) t-1,3-Dichloropropene	10.835	75	2522	0.802 ug/l	92
54) cis-1,3-Dichloropropene	10.312	75	2725	0.811 ug/l #	83
55) 1,1,2-Trichloroethane	11.018	97	1901	0.935 ug/l	91
56) Ethyl methacrylate	10.871	69	1923	2.471 ug/l #	88
57) 1,3-Dichloropropane	11.165	76	3113	0.881 ug/l	95
58) 2-Chloroethyl Vinyl ether	10.153	63	4929	3.822 ug/l	91
59) 2-Hexanone	11.194	43	7905	4.058 ug/l	87
60) Dibromochloromethane	11.359	129	2339	0.953 ug/l	98
61) 1,2-Dibromoethane	11.465	107	2022	1.000 ug/l	90
64) Tetrachloroethene	11.106	164	1658	0.947 ug/l #	83
65) Chlorobenzene	11.888	112	5401	0.960 ug/l	93
66) 1,1,1,2-Tetrachloroethane	11.959	131	2185	1.058 ug/l #	64
67) Ethyl Benzene	11.959	91	7347	0.802 ug/l	94
68) m/p-Xylenes	12.070	106	5059	1.494 ug/l	100
69) o-Xylene	12.394	106	2478	0.766 ug/l	97
70) Styrene	12.406	104	3812	0.712 ug/l	99
71) Bromoform	12.582	173	1208	0.818 ug/l #	88
73) Isopropylbenzene	12.688	105	5506	0.820 ug/l	98
74) N-amyl acetate	12.494	43	2716	0.899 ug/l #	87
75) 1,1,2,2-Tetrachloroethane	12.935	83	2616	1.102 ug/l #	96
76) 1,2,3-Trichloropropane	12.982	75	2198m	1.088 ug/l	
77) Bromobenzene	12.976	156	1733	0.987 ug/l	97
78) n-propylbenzene	13.029	91	6424	0.808 ug/l	93
79) 2-Chlorotoluene	13.117	91	4483	0.871 ug/l	97
80) 1,3,5-Trimethylbenzene	13.165	105	4301	0.775 ug/l	90
82) 4-Chlorotoluene	13.223	91	4268	0.833 ug/l	99
83) tert-Butylbenzene	13.435	119	3753	0.805 ug/l	96
84) 1,2,4-Trimethylbenzene	13.482	105	3758	0.679 ug/l	93
85) sec-Butylbenzene	13.612	105	4614	0.714 ug/l	99
86) p-Isopropyltoluene	13.723	119	3538	0.716 ug/l	98
87) 1,3-Dichlorobenzene	13.723	146	3038	0.940 ug/l	95
88) 1,4-Dichlorobenzene	13.806	146	3517m	1.050 ug/l	
89) n-Butylbenzene	14.053	91	3527	0.761 ug/l	93
90) Hexachloroethane	14.341	117	1355	1.102 ug/l	99
91) 1,2-Dichlorobenzene	14.106	146	3515	1.090 ug/l	96
92) 1,2-Dibromo-3-Chloropr...	14.711	75	402	0.928 ug/l	74
93) 1,2,4-Trichlorobenzene	15.394	180	1310	0.874 ug/l #	80
94) Hexachlorobutadiene	15.500	225	822	1.033 ug/l	89
95) Naphthalene	15.641	128	4210	0.941 ug/l #	90
96) 1,2,3-Trichlorobenzene	15.835	180	1494	0.985 ug/l #	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011425\
Data File : VN085443.D
Acq On : 14 Jan 2025 17:19
Operator : JC\MD
Sample : VSTDICC001
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 15 01:46:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 15 01:28:51 2025
Response via : Initial Calibration

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

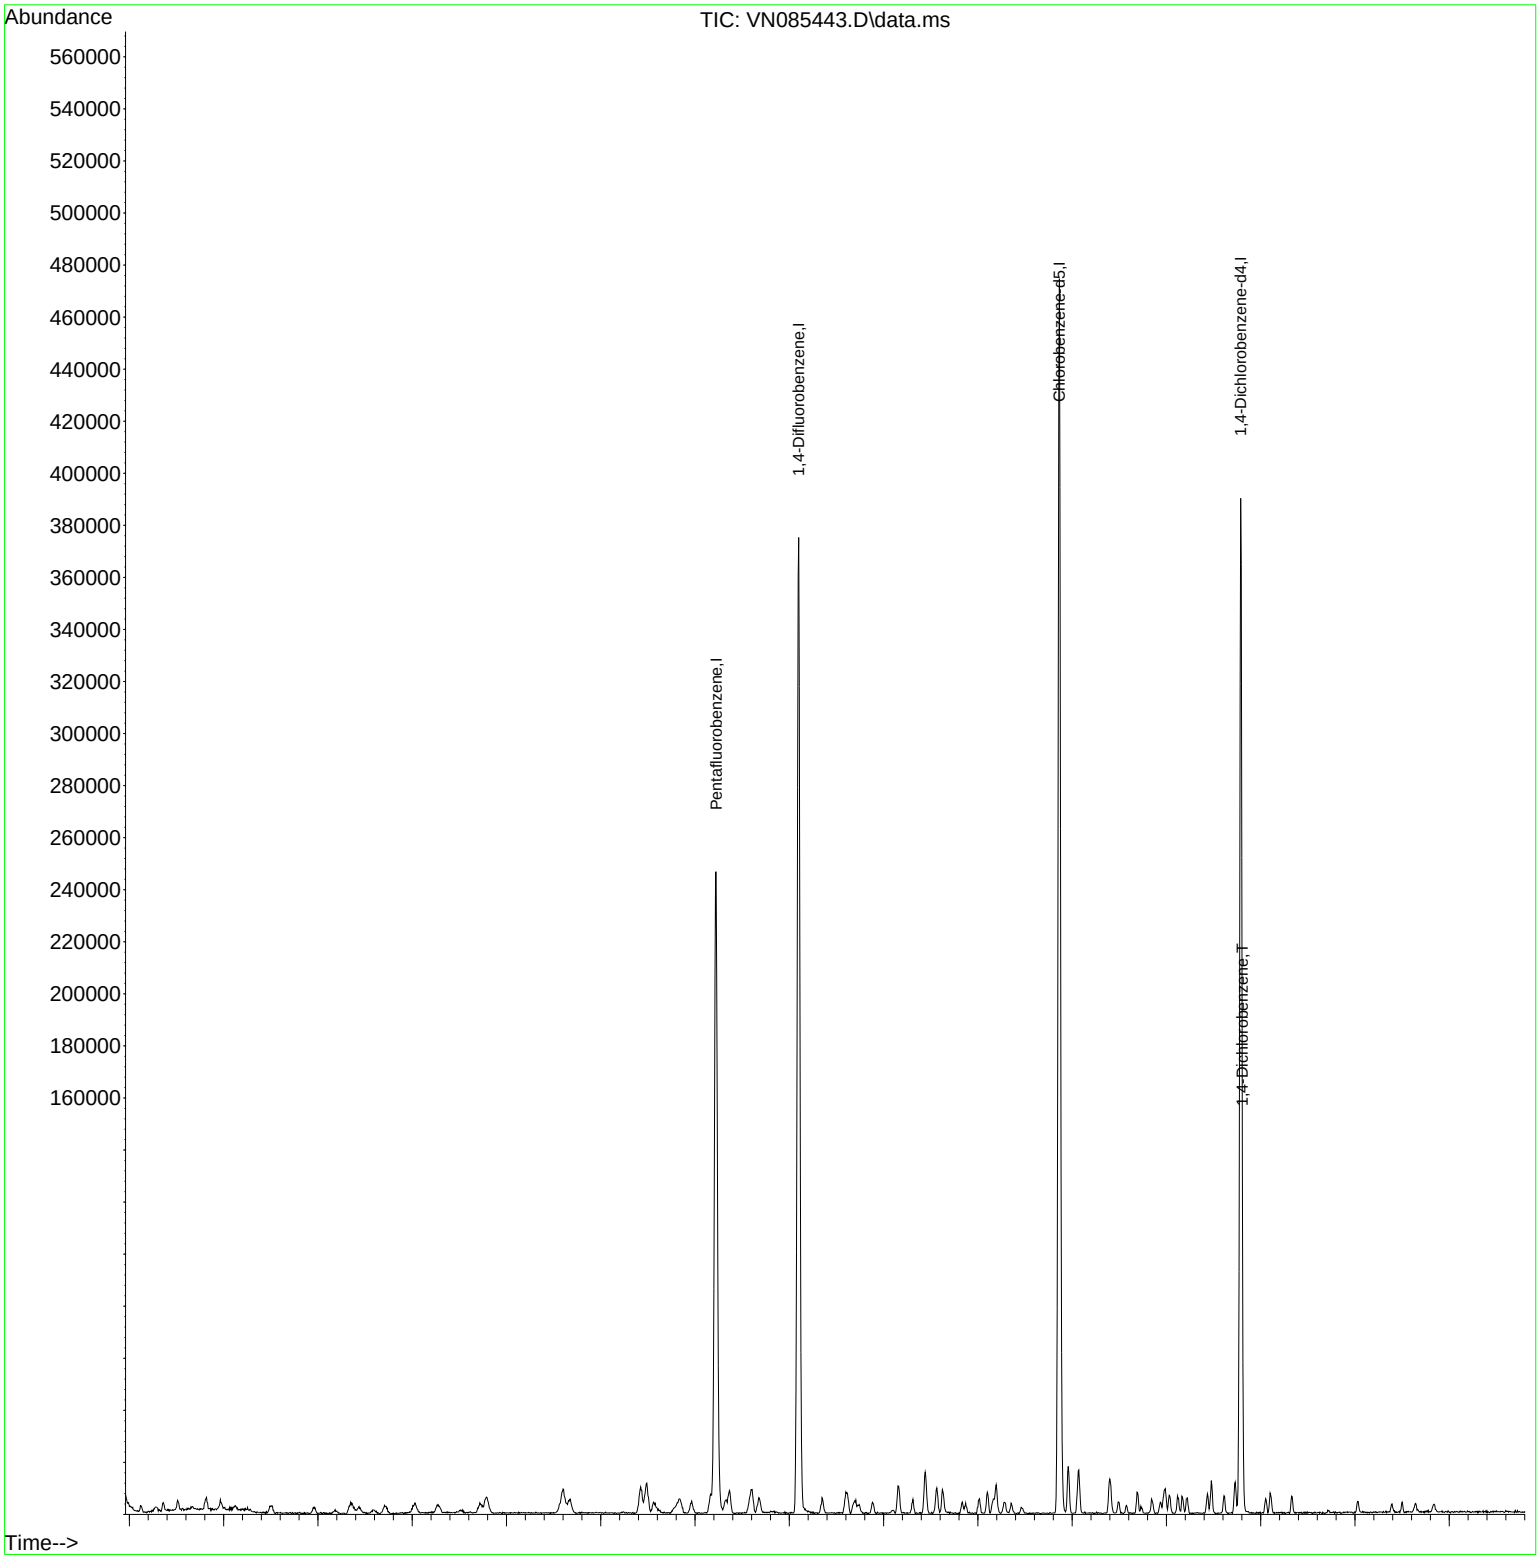

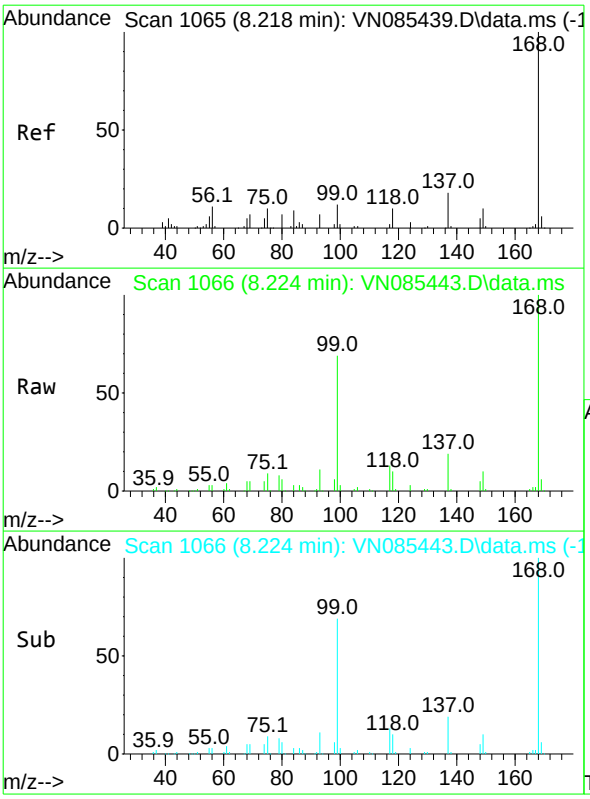

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:168 Resp: 166880

Ion	Ratio	Lower	Upper
168	100		
99	68.6	53.6	80.4



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

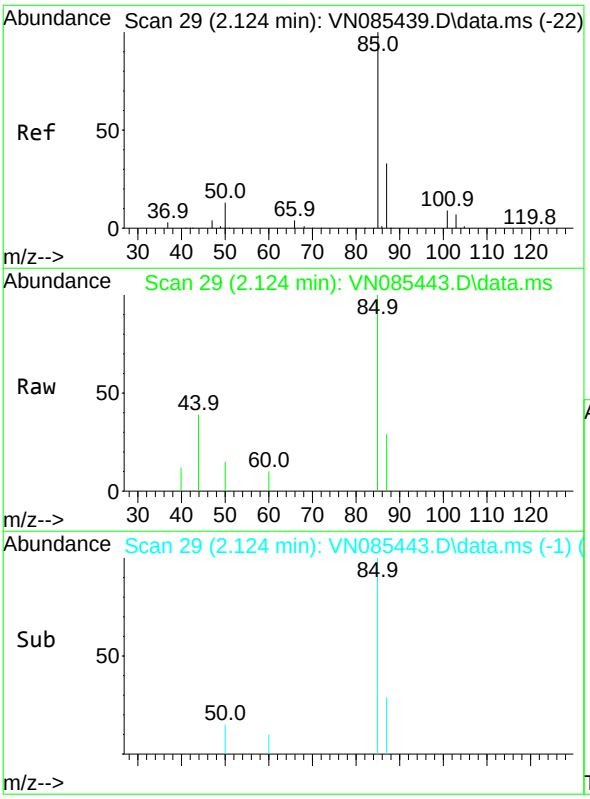

#2
Dichlorodifluoromethane
Concen: 1.054 ug/l
RT: 2.124 min Scan# 29
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 85 Resp: 2382

Ion	Ratio	Lower	Upper
85	100		
87	28.5	16.7	50.1



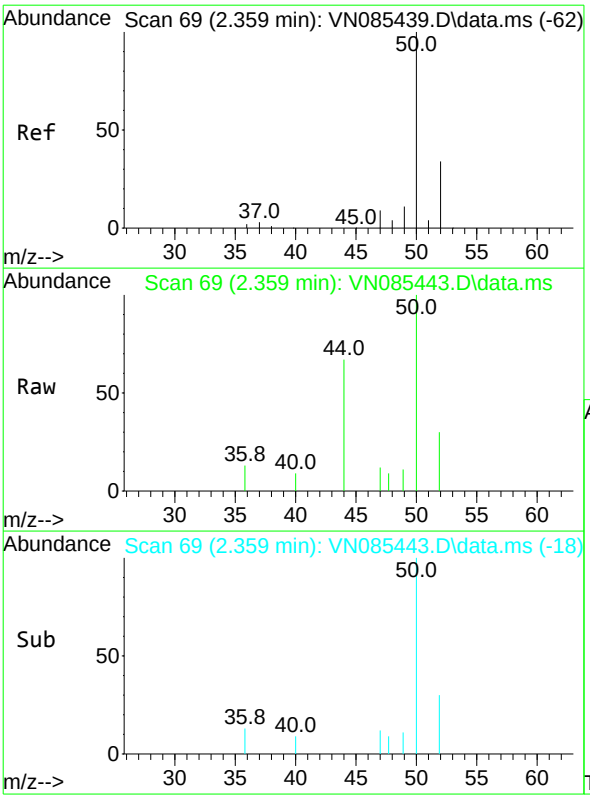

#3
Chloromethane
Concen: 1.145 ug/l
RT: 2.359 min Scan# 69
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 50 Resp: 2801

Ion	Ratio	Lower	Upper
50	100		
52	29.7	27.0	40.6



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

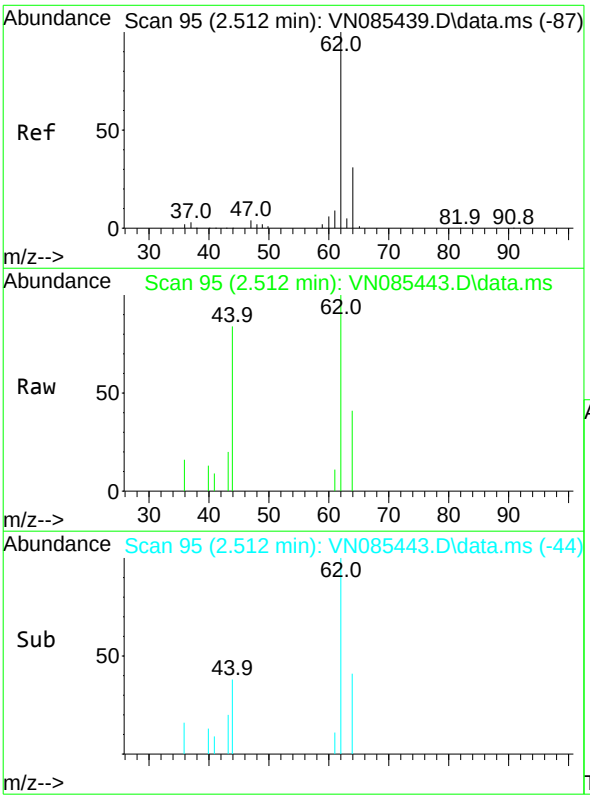

#4
Vinyl Chloride
Concen: 1.111 ug/l
RT: 2.512 min Scan# 95
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 62 Resp: 2732

Ion	Ratio	Lower	Upper
62	100		
64	41.4	24.8	37.2#



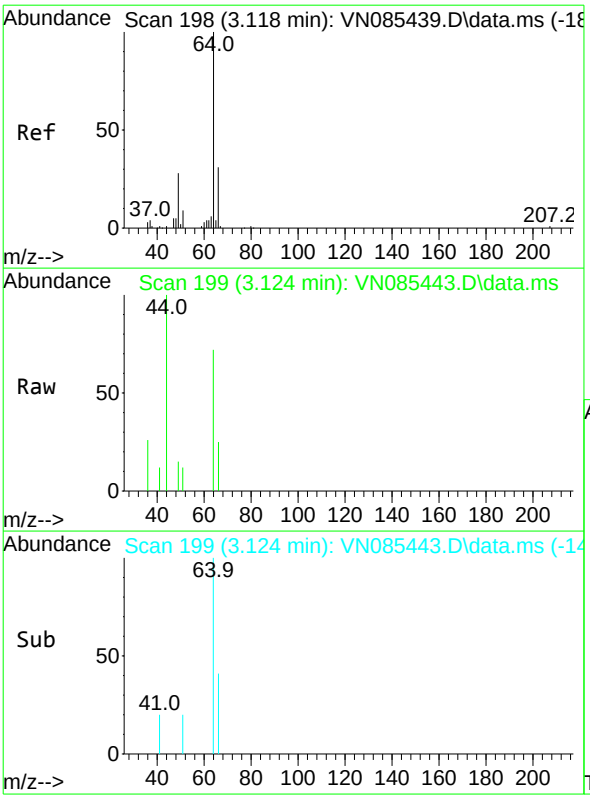

#6
Chloroethane
Concen: 1.160 ug/l
RT: 3.124 min Scan# 19
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 64 Resp: 1809

Ion	Ratio	Lower	Upper
64	100		
66	34.1	24.6	36.8



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

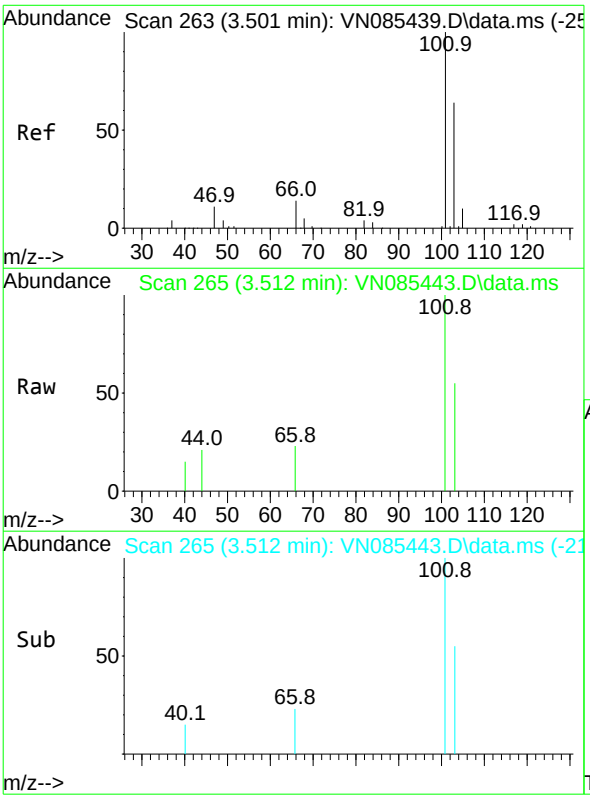

#7
Trichlorofluoromethane
Concen: 1.082 ug/l
RT: 3.512 min Scan# 265
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:101 Resp: 3860

Ion	Ratio	Lower	Upper
101	100		
103	55.0	51.4	77.2



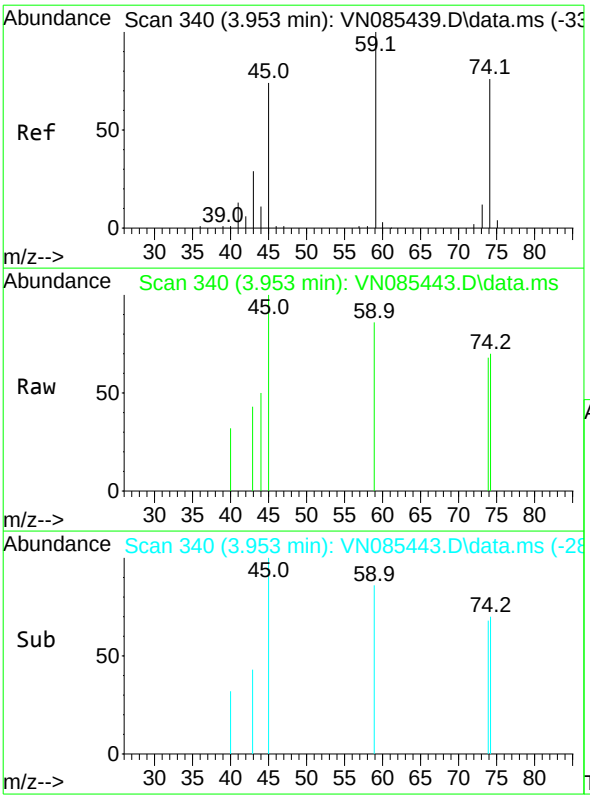

#8
Diethyl Ether
Concen: 1.238 ug/l
RT: 3.953 min Scan# 34
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 74 Resp: 1526

Ion	Ratio	Lower	Upper
74	100		
45	80.9	49.7	149.1

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



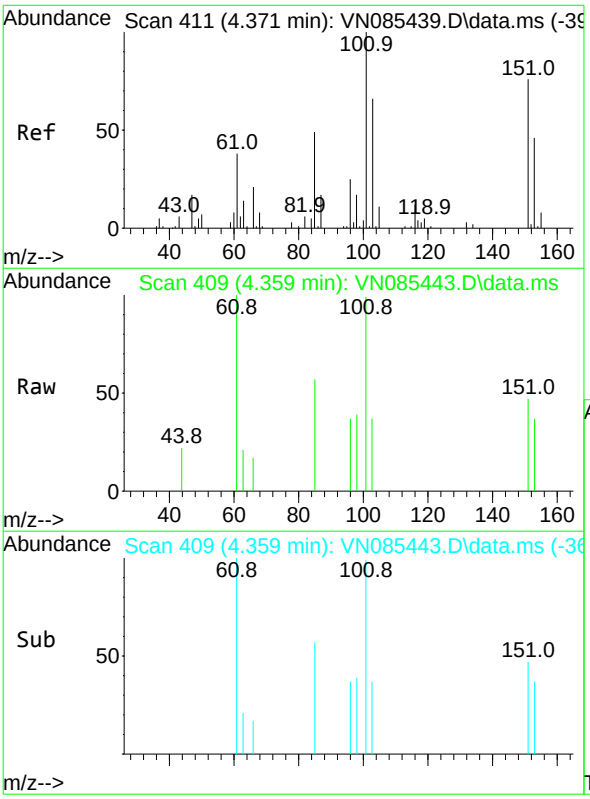

#9
1,1,2-Trichlorotrifluoroethane
Concen: 1.073 ug/l m
RT: 4.359 min Scan# 409
Delta R.T. -0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:101 Resp: 2156

Ion	Ratio	Lower	Upper
101	100		
85	35.3	37.8	56.8#
151	66.4	58.8	88.2



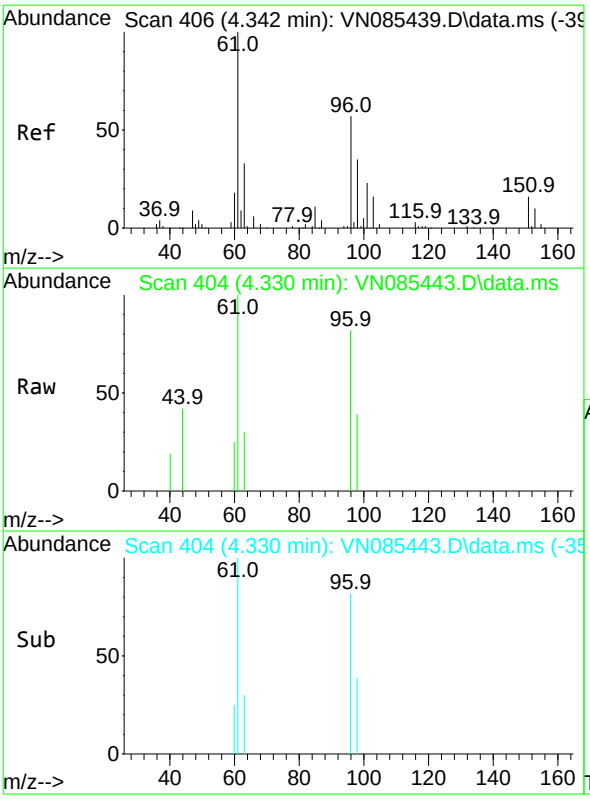

#12
1,1-Dichloroethene
Concen: 0.927 ug/l
RT: 4.330 min Scan# 40
Delta R.T. -0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 96 Resp: 1660

Ion	Ratio	Lower	Upper
96	100		
61	122.1	141.0	211.4#
98	48.1	49.0	73.6#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

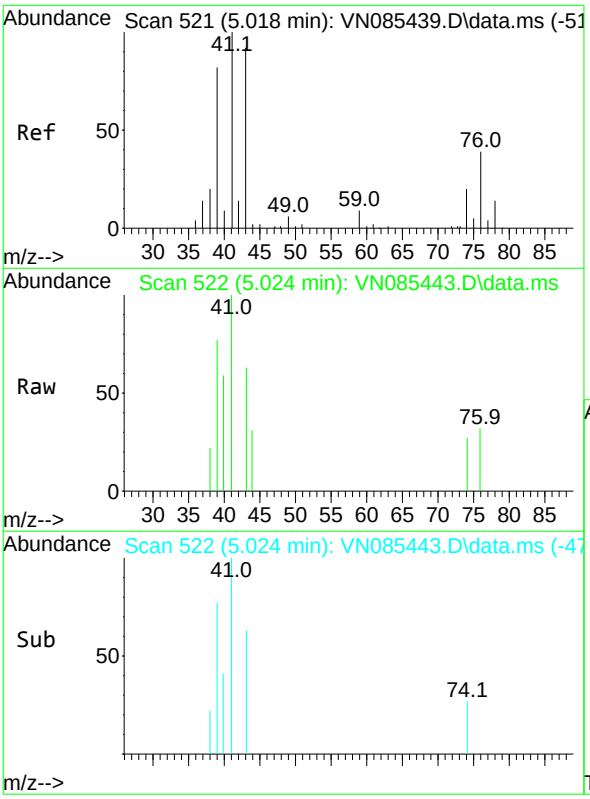

#14
Allyl chloride
Concen: 1.094 ug/l
RT: 5.024 min Scan# 522
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 41 Resp: 3179

Ion	Ratio	Lower	Upper
41	100		
39	73.1	64.4	96.6
76	21.4	30.5	45.7#



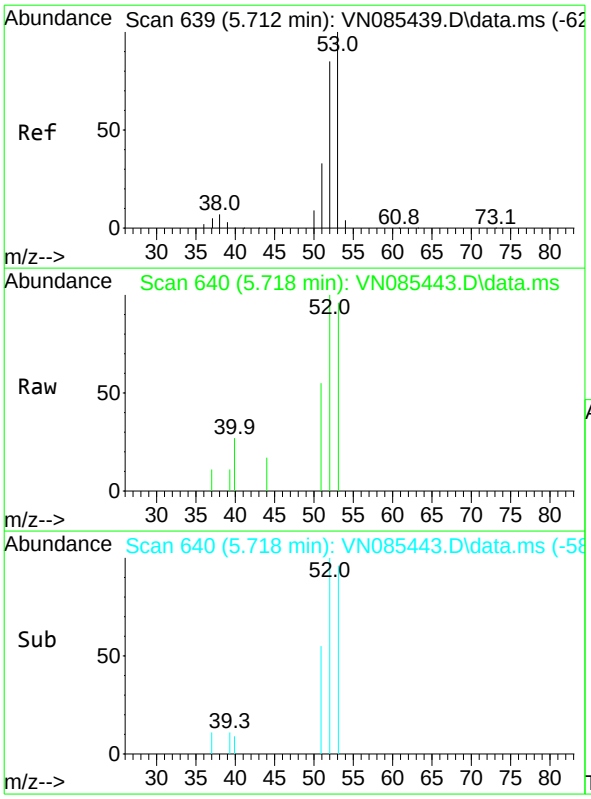

#15
Acrylonitrile
Concen: 5.070 ug/l
RT: 5.718 min Scan# 64
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 53 Resp: 4967

Ion	Ratio	Lower	Upper
53	100		
52	45.1	65.5	98.3#
51	33.3	29.8	44.8



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

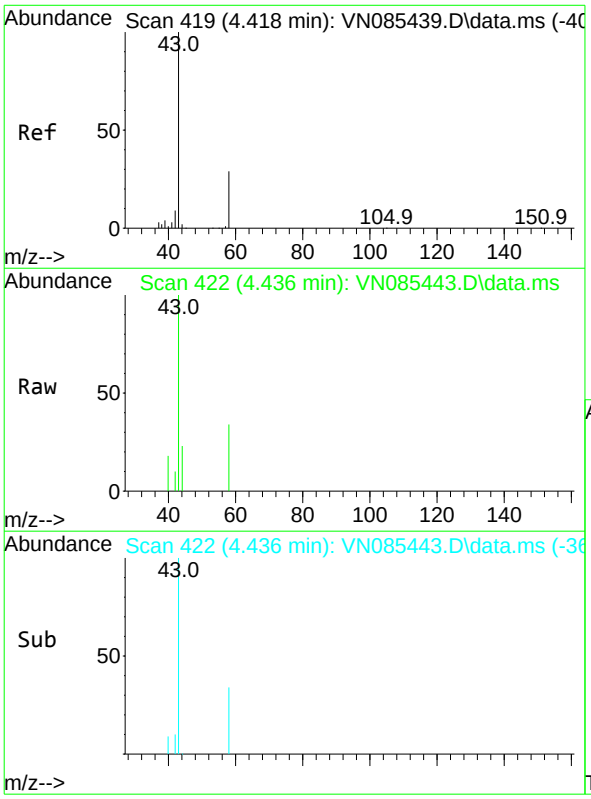

#16
Acetone
Concen: 5.862 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.018 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 5102

Ion	Ratio	Lower	Upper
43	100		
58	33.8	23.8	35.6



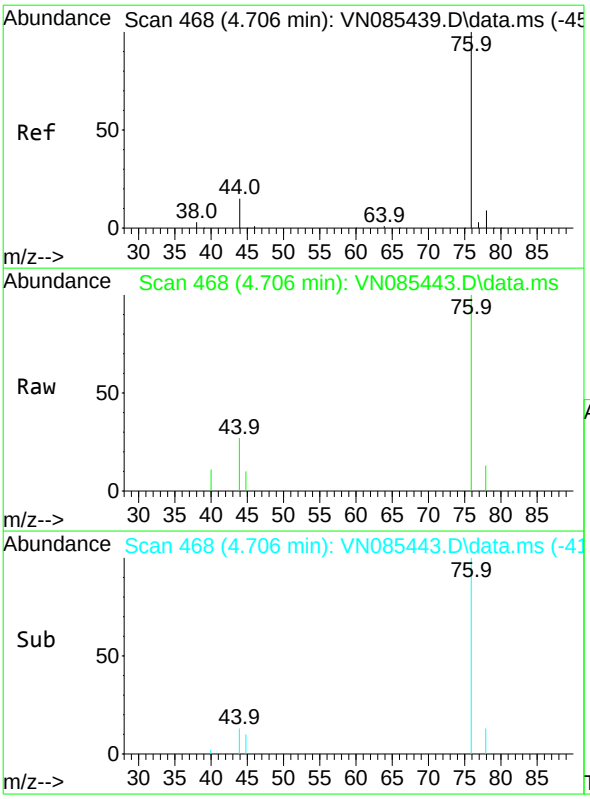

#17
Carbon Disulfide
Concen: 1.197 ug/l
RT: 4.706 min Scan# 46
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 76 Resp: 6601

Ion	Ratio	Lower	Upper
76	100		
78	13.2	6.9	10.3#

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



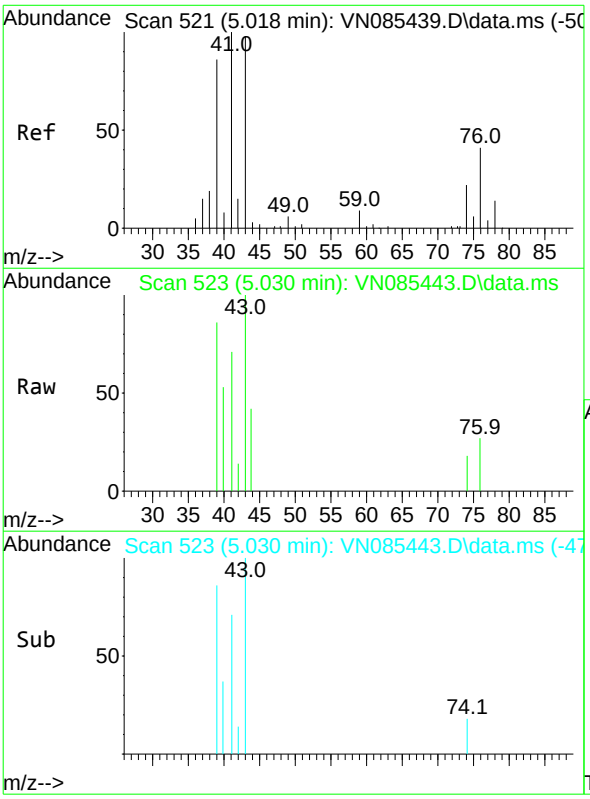

#18
Methyl Acetate
Concen: 1.099 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 2908

Ion	Ratio	Lower	Upper
43	100		
74	13.8	18.6	28.0#



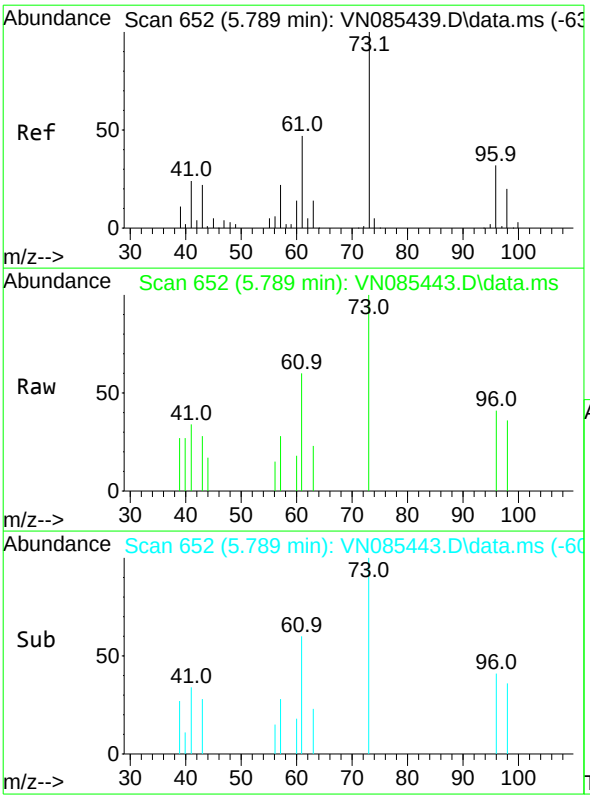

#19
Methyl tert-butyl Ether
Concen: 0.887 ug/l
RT: 5.789 min Scan# 65
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 73 Resp: 5156

Ion	Ratio	Lower	Upper
73	100		
57	28.4	17.8	26.8#

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



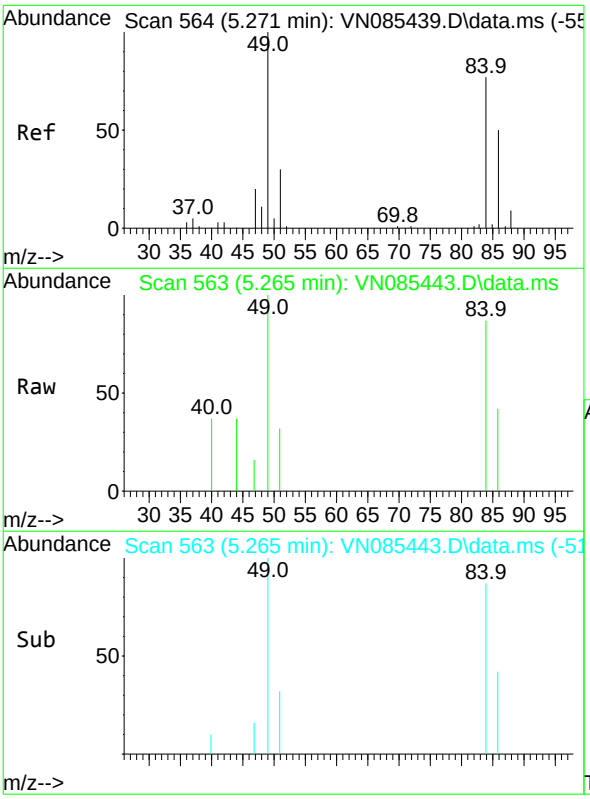

#20
Methylene Chloride
Concen: 1.016 ug/l
RT: 5.265 min Scan# 563
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 84 Resp: 2190

Ion	Ratio	Lower	Upper
84	100		
49	115.6	104.1	156.1
51	36.9	31.0	46.4
86	48.9	51.9	77.9#



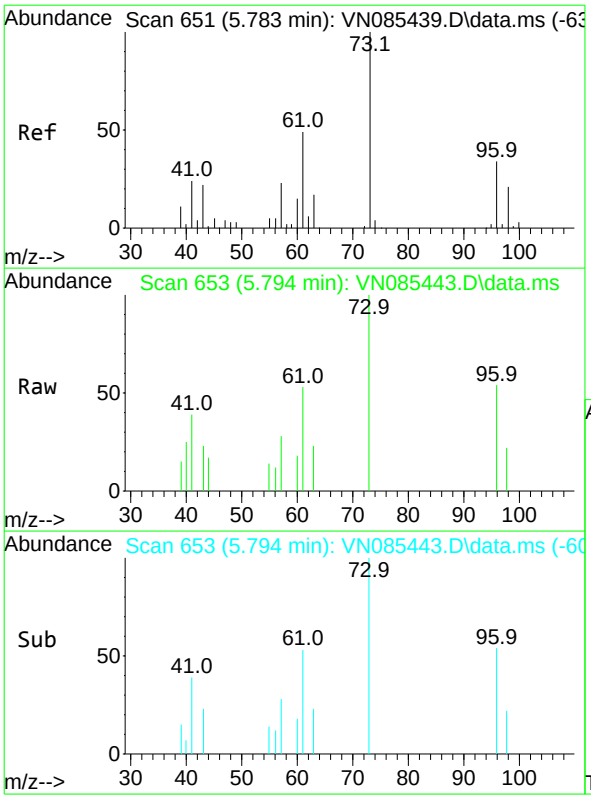

#21
trans-1,2-Dichloroethene
Concen: 1.102 ug/l
RT: 5.794 min Scan# 65
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 96 Resp: 2110

Ion	Ratio	Lower	Upper
96	100		
61	98.7	115.7	173.5#
98	41.8	49.8	74.8#

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



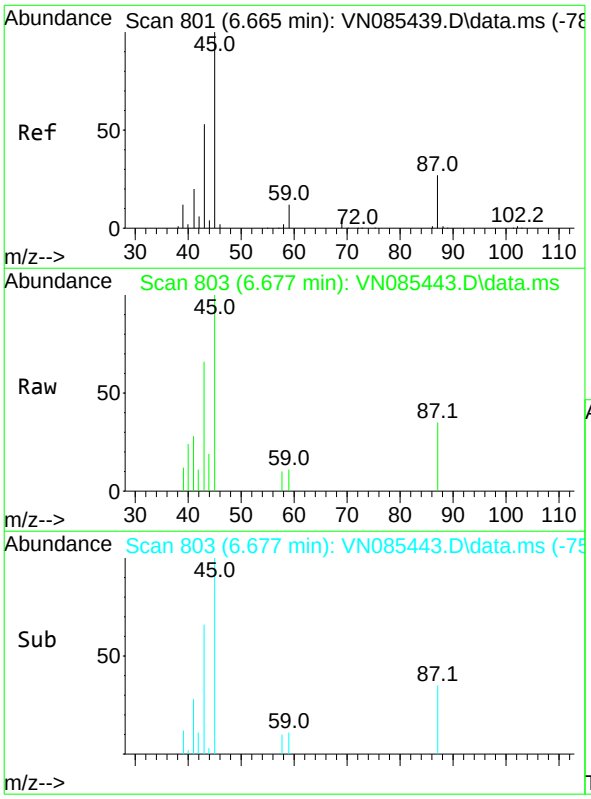

#22
Diisopropyl ether
Concen: 0.882 ug/l
RT: 6.677 min Scan# 803
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 45 Resp: 5691

Ion	Ratio	Lower	Upper
45	100		
43	65.9	45.0	67.6
87	35.0	21.8	32.8#
59	11.3	10.2	15.2



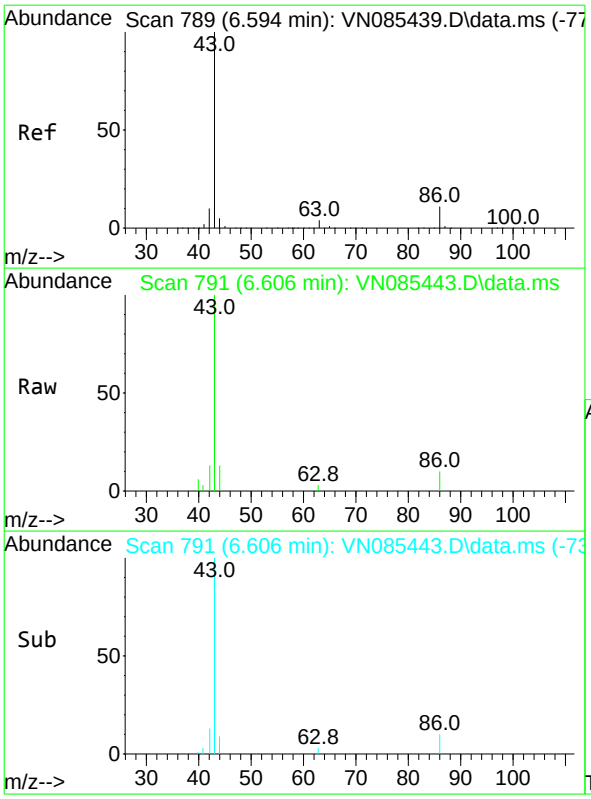

#23
Vinyl Acetate
Concen: 4.090 ug/l m
RT: 6.606 min Scan# 79
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 18526

Ion	Ratio	Lower	Upper
43	100		
86	9.8	8.4	12.6



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

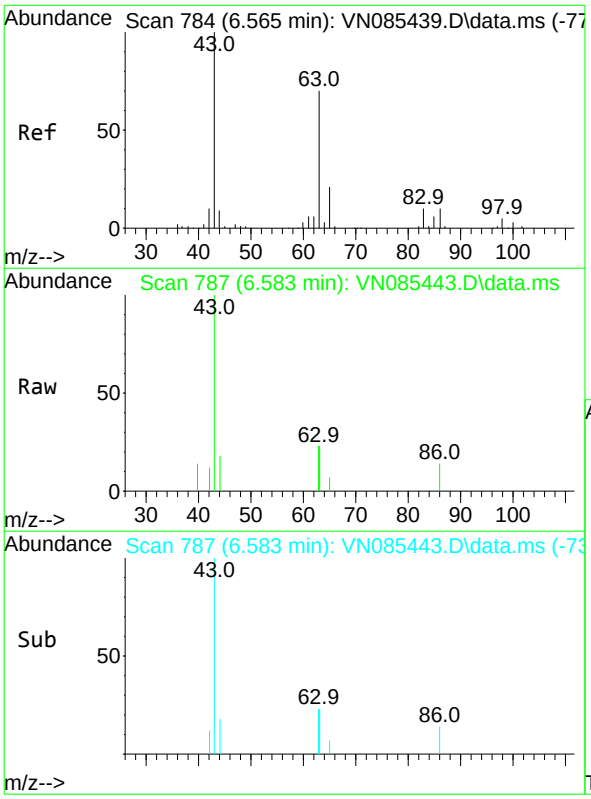

#24
1,1-Dichloroethane
Concen: 1.022 ug/l m
RT: 6.583 min Scan# 787
Delta R.T. 0.018 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 63 Resp: 4020

Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.3	9.8#
100	0.0	2.0	6.0#



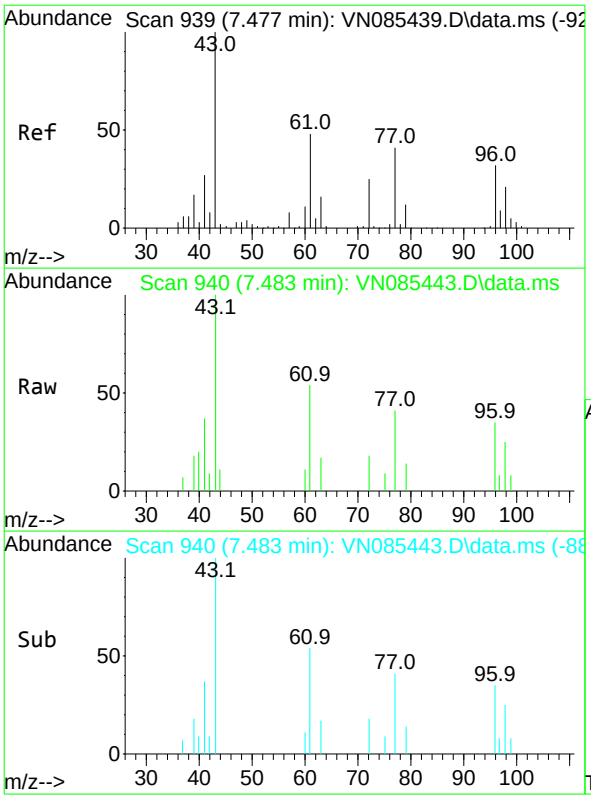

#25
2-Butanone
Concen: 5.034 ug/l m
RT: 7.483 min Scan# 94
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 6448

Ion	Ratio	Lower	Upper
43	100		
72	18.0	20.2	30.4#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

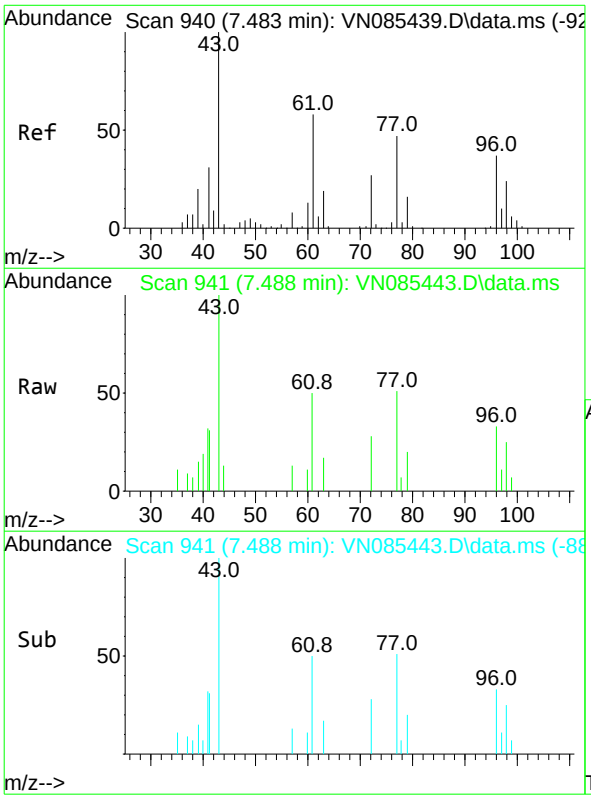

#26
2,2-Dichloropropane
Concen: 0.976 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 77 Resp: 3104

Ion	Ratio	Lower	Upper
77	100		
97	17.7	10.7	32.1



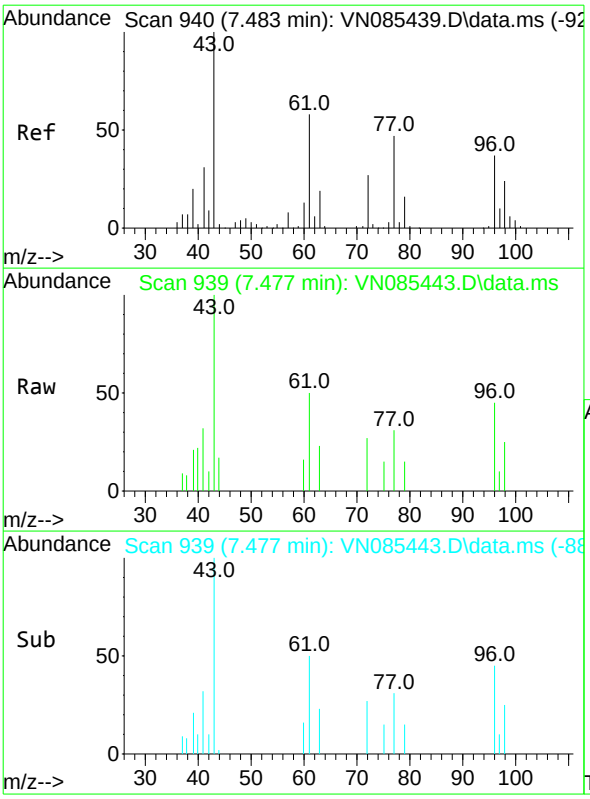

#27
cis-1,2-Dichloroethene
Concen: 0.969 ug/l
RT: 7.477 min Scan# 93
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 96 Resp: 2185

Ion	Ratio	Lower	Upper
96	100		
61	166.1	0.0	311.8
98	68.7	0.0	126.0



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

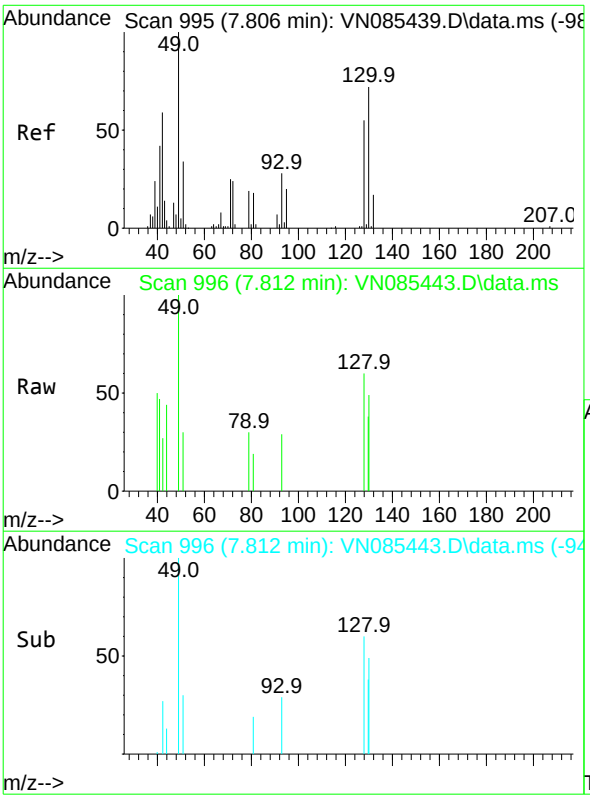

#28
Bromochloromethane
Concen: 1.138 ug/l
RT: 7.812 min Scan# 996
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 49 Resp: 2082

Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	4.4
130	78.0	55.0	82.4



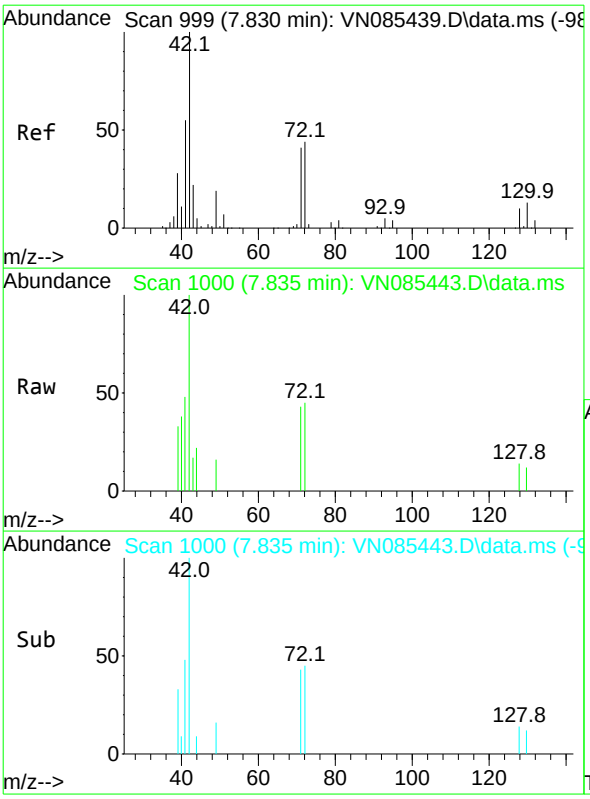

#29
Tetrahydrofuran
Concen: 4.548 ug/l
RT: 7.835 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 42 Resp: 3693

Ion	Ratio	Lower	Upper
42	100		
72	43.1	34.2	51.2
71	37.9	32.5	48.7

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



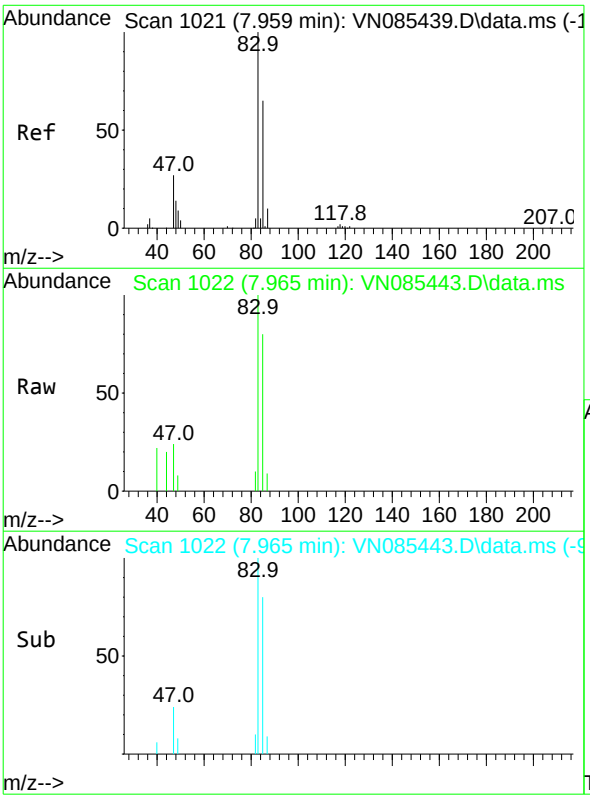

#30
Chloroform
Concen: 1.045 ug/l
RT: 7.965 min Scan# 1022
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 83 Resp: 4250

Ion	Ratio	Lower	Upper
83	100		
85	80.2	51.8	77.6#



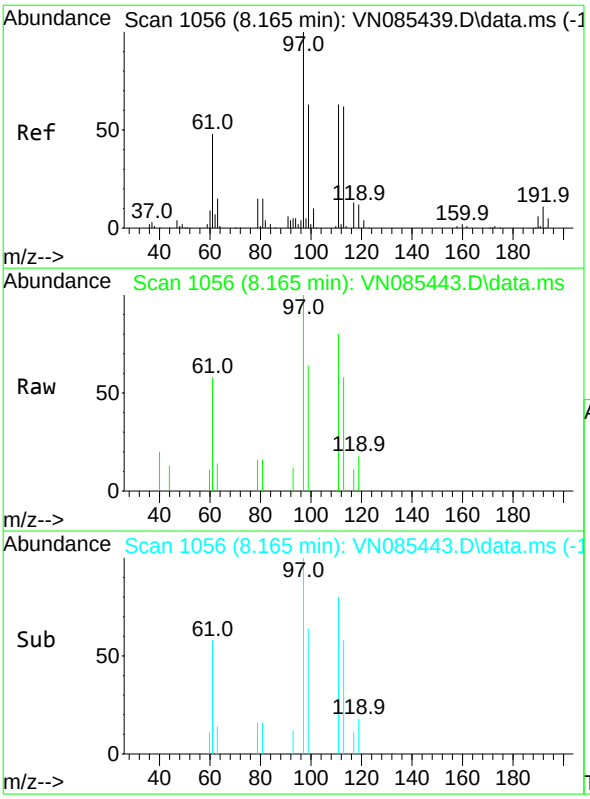

#32
1,1,1-Trichloroethane
Concen: 1.031 ug/l
RT: 8.165 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 97 Resp: 3678

Ion	Ratio	Lower	Upper
97	100		
99	0.0	49.8	74.6#
61	52.2	41.4	62.2

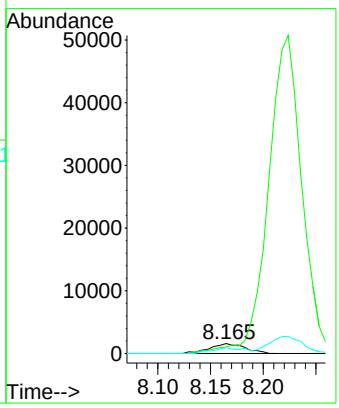

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

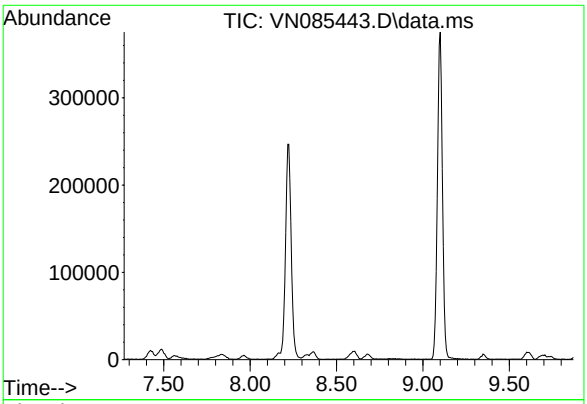

#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.57 min

Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 65

Sig	Exp Ratio
65	100
67	50.8

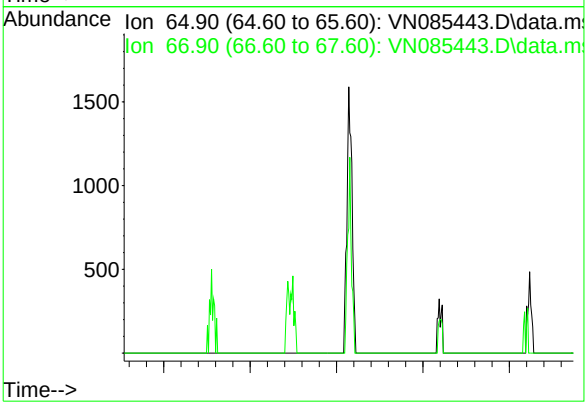

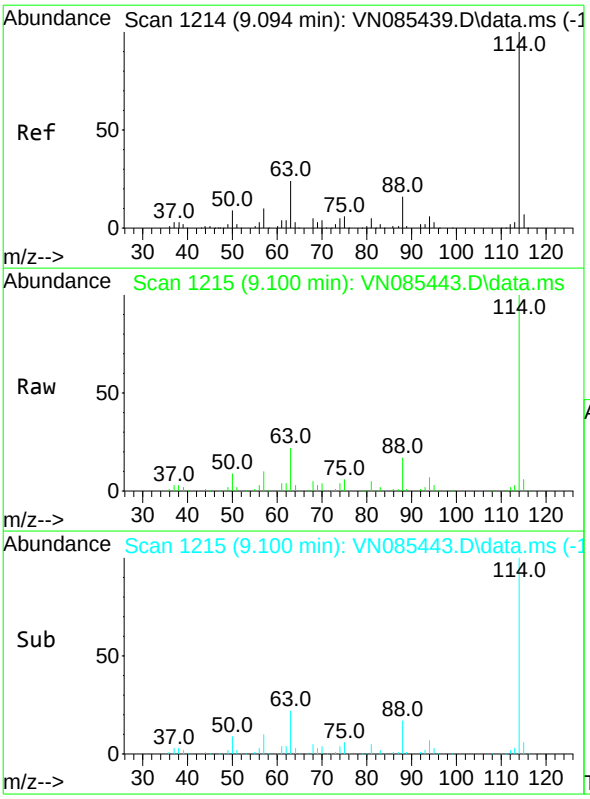

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 12
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:114 Resp: 302938

Ion	Ratio	Lower	Upper
114	100		
63	22.3	0.0	47.6
88	16.8	0.0	32.6

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



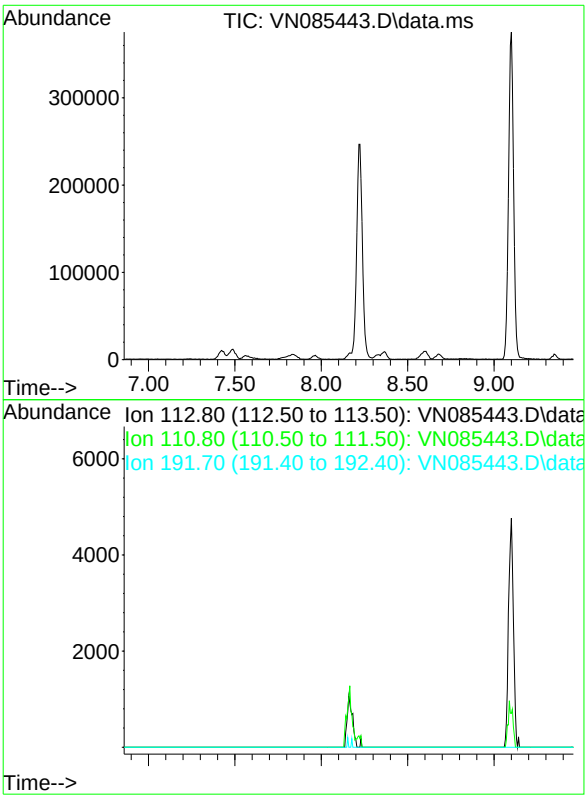

#35
Dibromofluoromethane
Concen: 0.000 ug/l
Expected RT: 8.16 min

Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 113

Sig	Exp Ratio
113	100
111	103.4
192	17.9

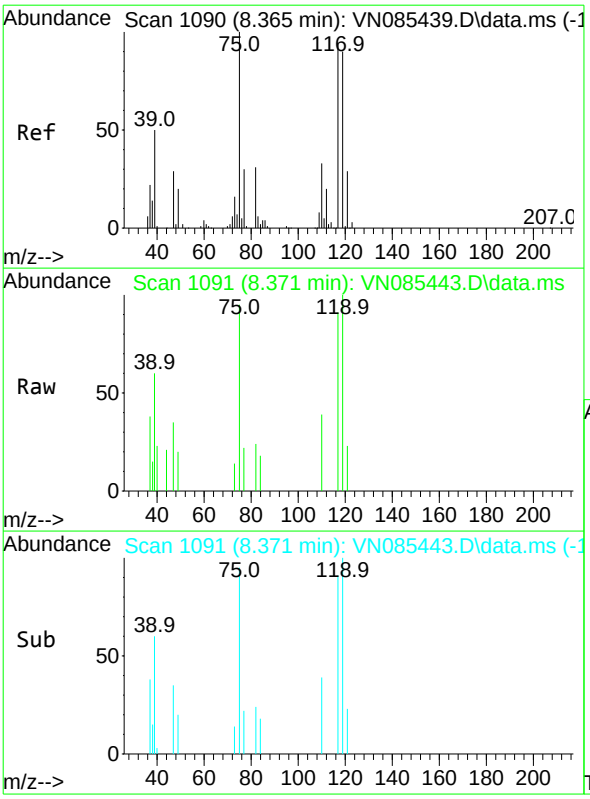

#36
1,1-Dichloropropene
Concen: 1.046 ug/l
RT: 8.371 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 75 Resp: 3084

Ion	Ratio	Lower	Upper
75	100		
110	30.1	16.5	49.5
77	15.9	24.4	36.6#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

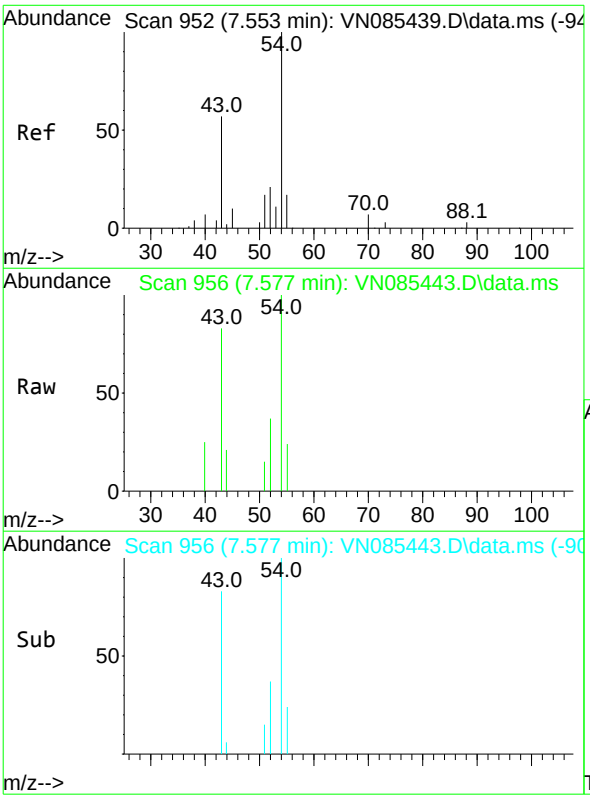

#37
Ethyl Acetate
Concen: 1.026 ug/l m
RT: 7.577 min Scan# 956
Delta R.T. 0.023 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 3056

Ion	Ratio	Lower	Upper
43	100		
61	4.3	10.9	16.3#
70	0.0	7.5	11.3#



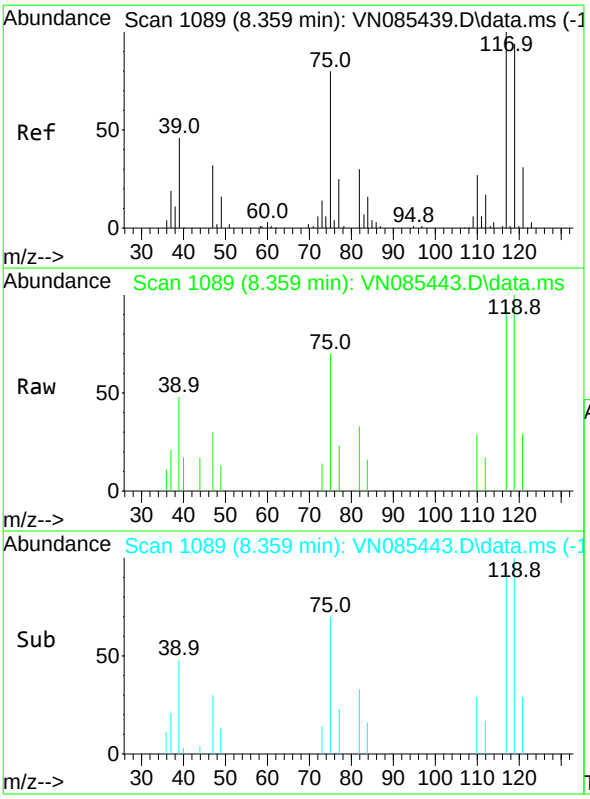

#38
Carbon Tetrachloride
Concen: 1.018 ug/l
RT: 8.359 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:117 Resp: 3436

Ion	Ratio	Lower	Upper
117	100		
119	106.6	75.4	113.2
121	31.0	24.6	37.0

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



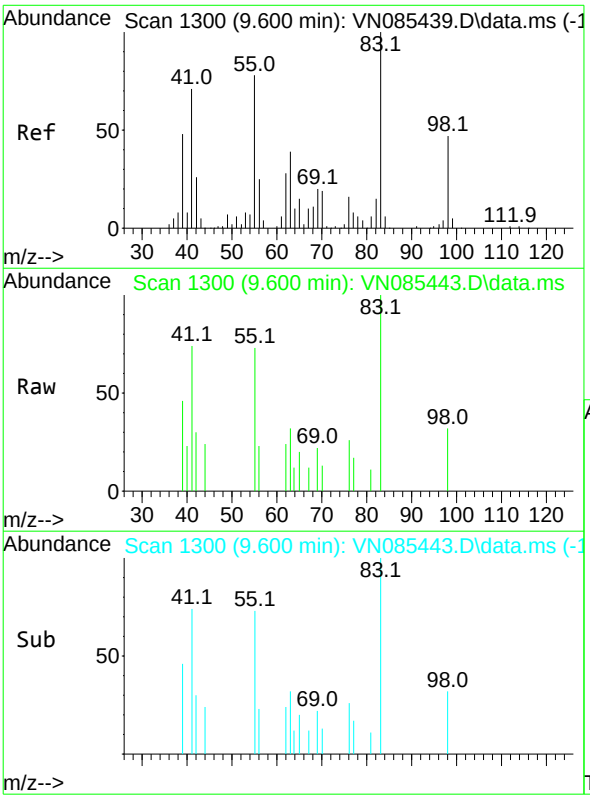

#39
Methylcyclohexane
Concen: 0.867 ug/l
RT: 9.600 min Scan# 1300
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 83 Resp: 2403

Ion	Ratio	Lower	Upper
83	100		
55	72.7	62.6	94.0
98	31.8	37.7	56.5#



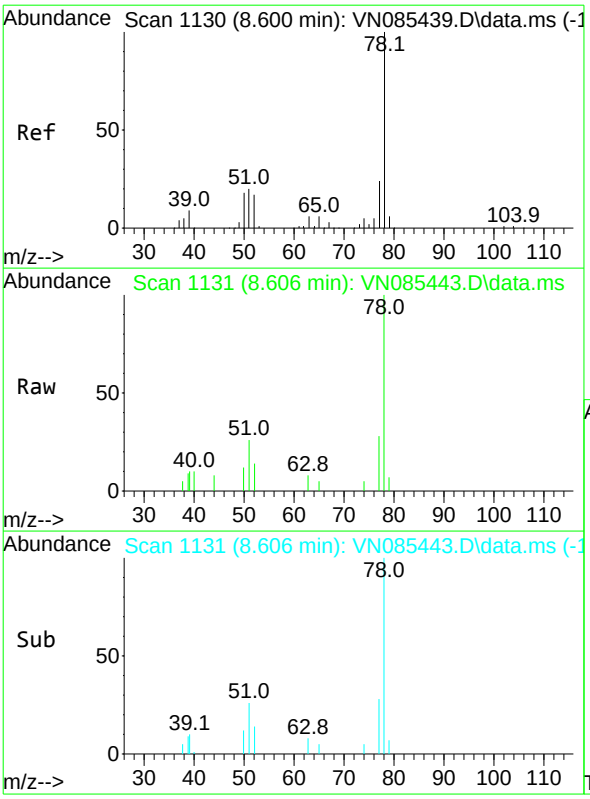

#40
Benzene
Concen: 0.957 ug/l
RT: 8.606 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 78 Resp: 8480

Ion	Ratio	Lower	Upper
78	100		
77	28.3	19.0	28.6



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

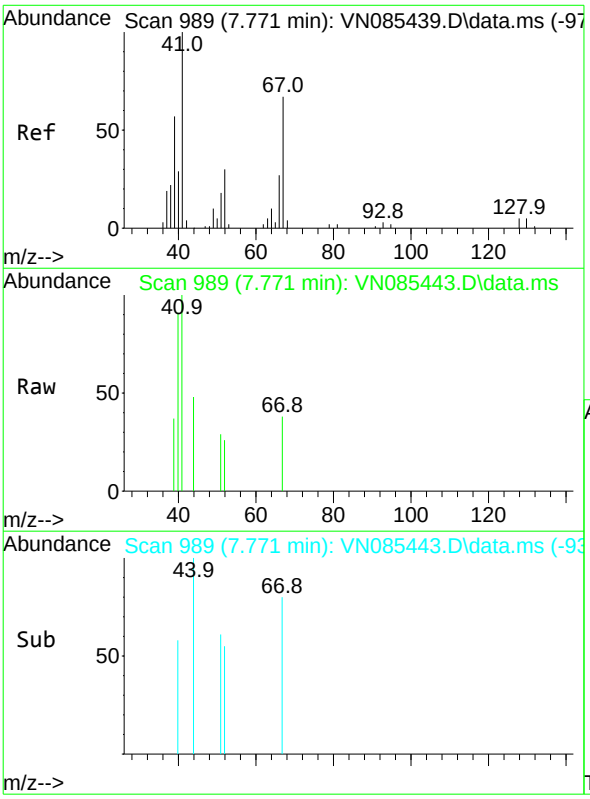

#41
Methacrylonitrile
Concen: 0.941 ug/l
RT: 7.771 min Scan# 989
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 41 Resp: 1458

Ion	Ratio	Lower	Upper
41	100		
39	37.6	46.0	69.0#
67	53.8	57.4	86.2#
52	18.5	25.5	38.3#



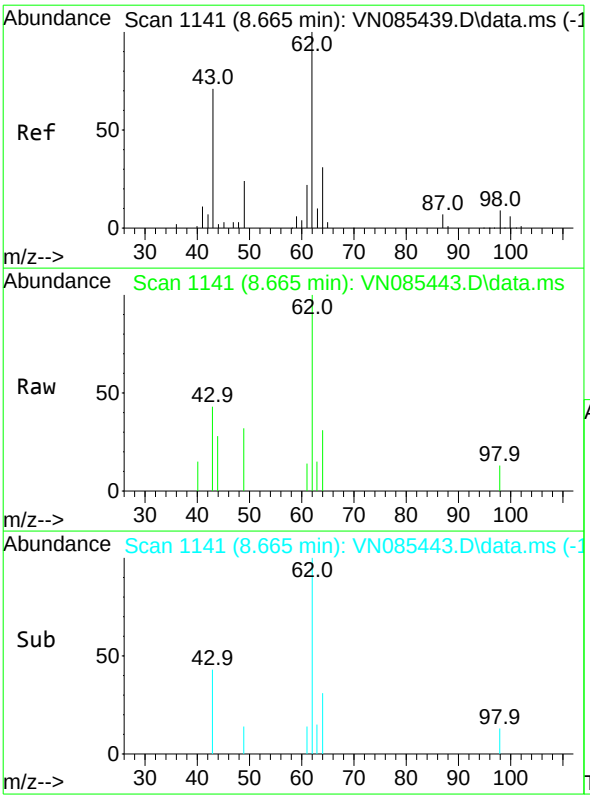

#42
1,2-Dichloroethane
Concen: 0.938 ug/l
RT: 8.665 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 62 Resp: 3131

Ion	Ratio	Lower	Upper
62	100		
98	5.4	0.0	17.0

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



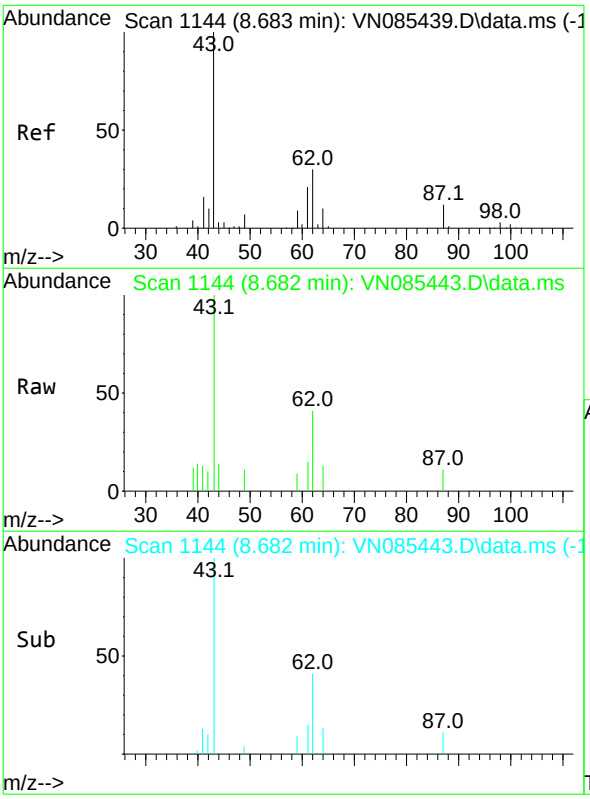

#43
Isopropyl Acetate
Concen: 1.007 ug/l
RT: 8.682 min Scan# 1144
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 4803

Ion	Ratio	Lower	Upper
43	100		
61	18.9	20.7	31.1#
87	7.3	9.8	14.8#



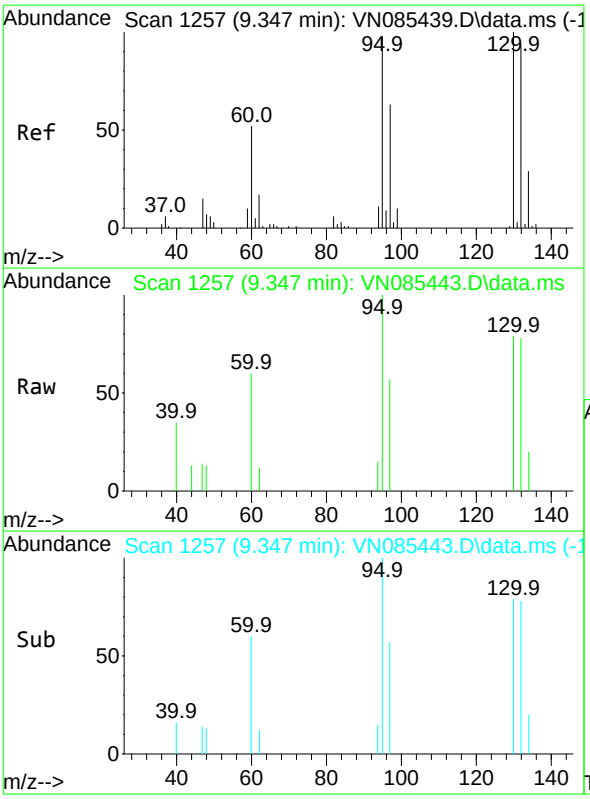

#44
Trichloroethene
Concen: 1.034 ug/l
RT: 9.347 min Scan# 12
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:130 Resp: 2133

Ion	Ratio	Lower	Upper
130	100		
95	126.1	0.0	195.8



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

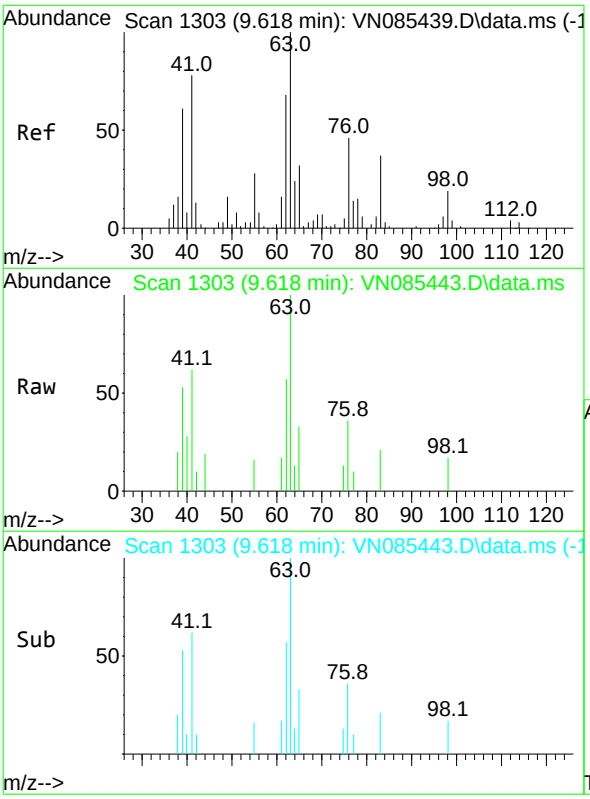

#45
1,2-Dichloropropane
Concen: 0.992 ug/l
RT: 9.618 min Scan# 1303
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 63 Resp: 2246

Ion	Ratio	Lower	Upper
63	100		
65	32.6	25.6	38.4



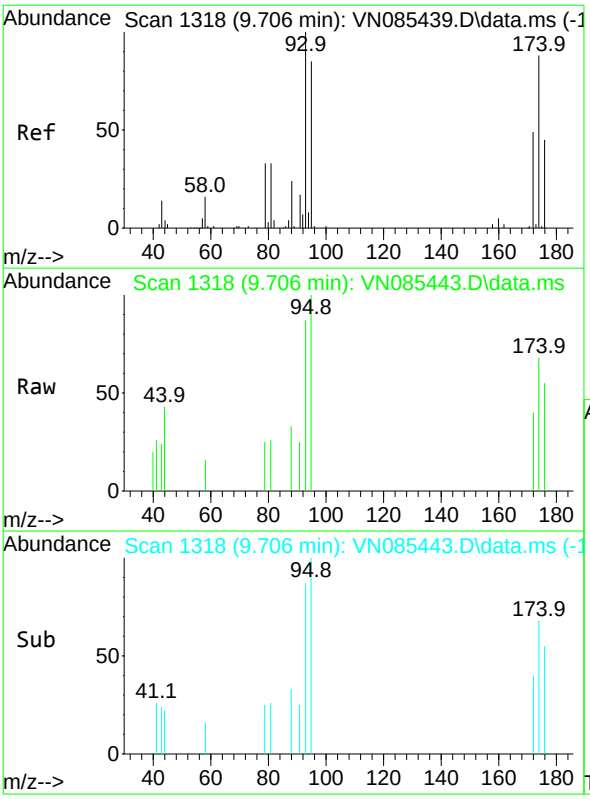

#46
Dibromomethane
Concen: 1.083 ug/l
RT: 9.706 min Scan# 13
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 93 Resp: 1769

Ion	Ratio	Lower	Upper
93	100		
95	86.5	64.7	97.1
174	77.4	69.0	103.4



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

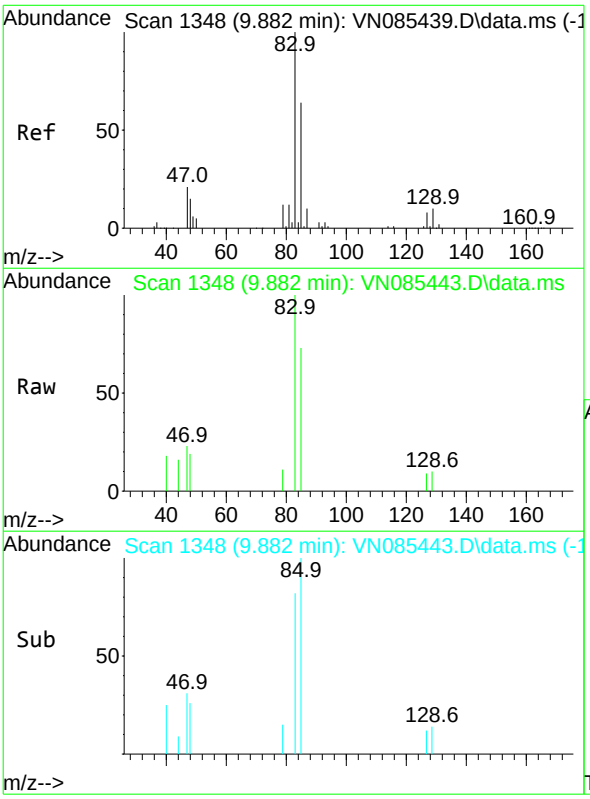

#47
Bromodichloromethane
Concen: 0.882 ug/l
RT: 9.882 min Scan# 1348
Delta R.T. 0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 83 Resp: 2935

Ion	Ratio	Lower	Upper
83	100		
85	72.9	51.2	76.8
127	9.0	6.5	9.7



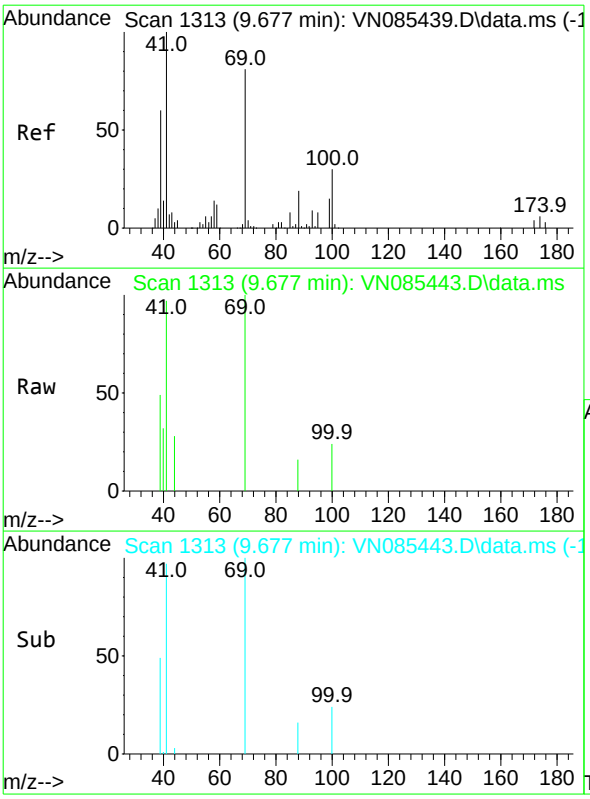

#48
Methyl methacrylate
Concen: 0.878 ug/l
RT: 9.677 min Scan# 13
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 41 Resp: 1886

Ion	Ratio	Lower	Upper
41	100		
69	76.2	64.7	97.1
39	62.8	49.0	73.6

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



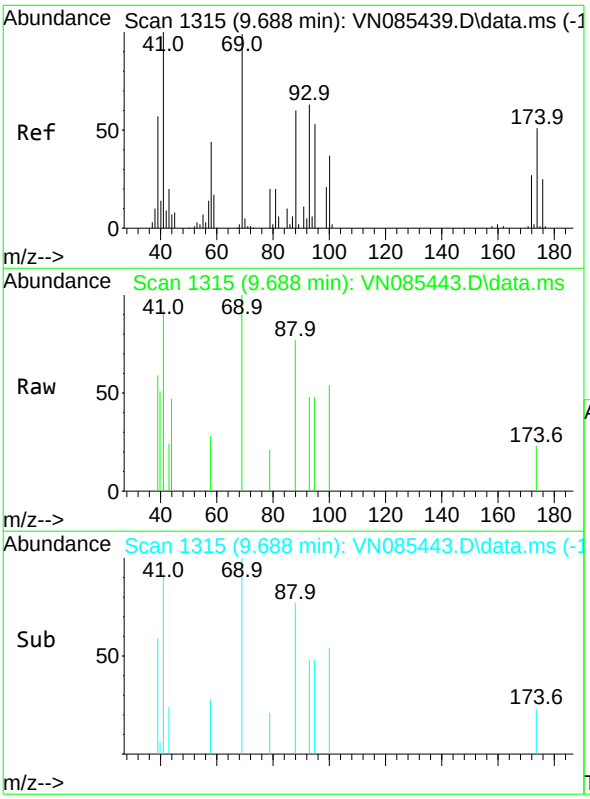

#49
1,4-Dioxane
Concen: 18.616 ug/l
RT: 9.688 min Scan# 1315
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 88 Resp: 673

Ion	Ratio	Lower	Upper
88	100		
43	0.0	26.6	39.8#
58	31.1	59.5	89.3#



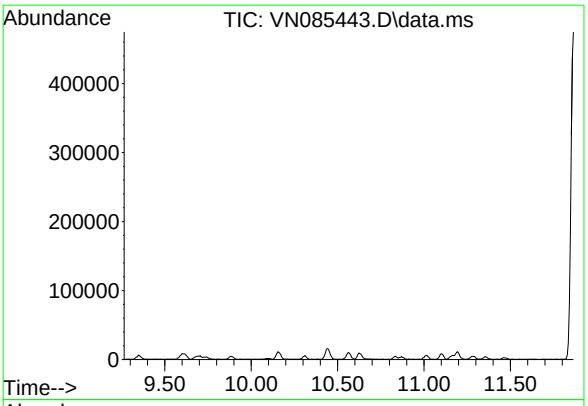

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.56 min

Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 98

Sig	Exp Ratio
98	100
100	65.3

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

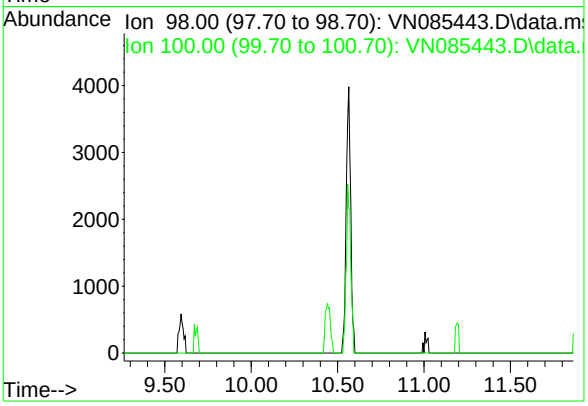

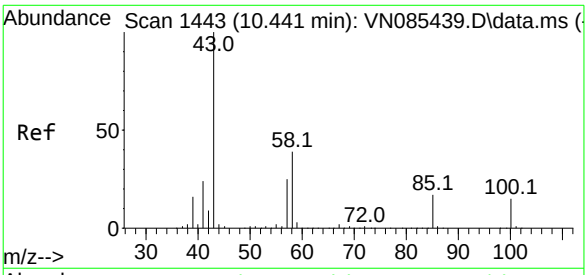

#51
4-Methyl-2-Pentanone
Concen: 4.163 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 11523

Ion	Ratio	Lower	Upper
43	100		
58	33.6	30.5	45.7

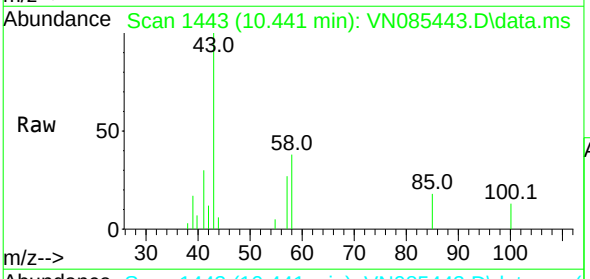

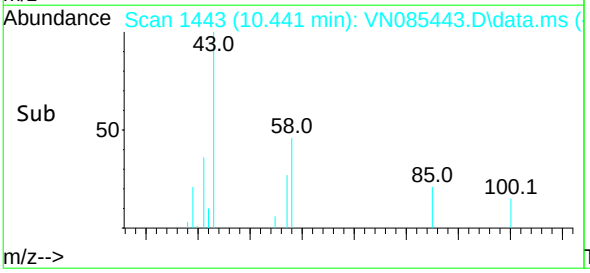



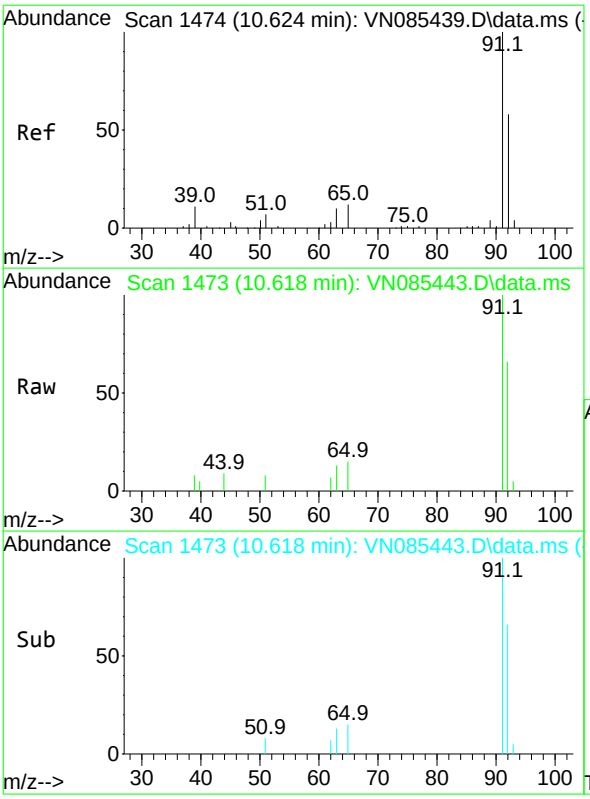

#52
Toluene
Concen: 0.814 ug/l
RT: 10.618 min Scan# 14
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 92 Resp: 4180

Ion	Ratio	Lower	Upper
92	100		
91	183.9	139.2	208.8



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

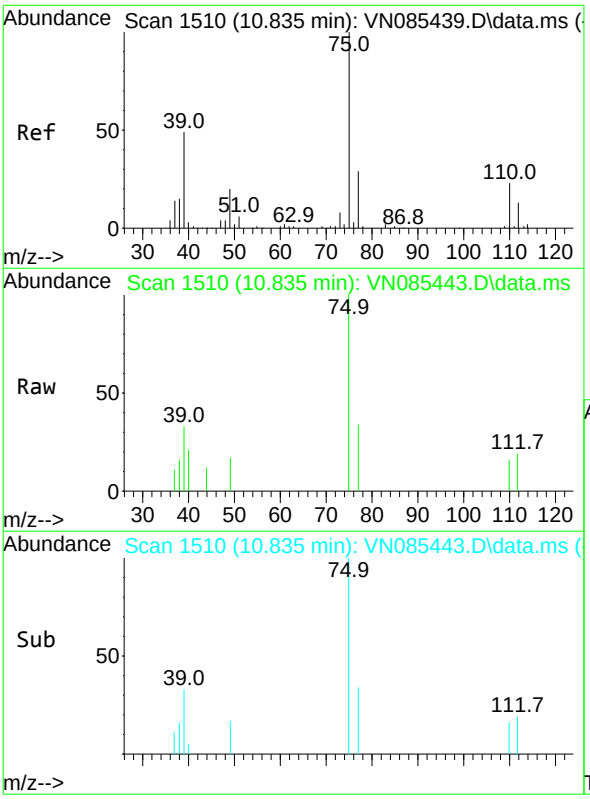

#53
t-1,3-Dichloropropene
Concen: 0.802 ug/l
RT: 10.835 min Scan# 1510
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 75 Resp: 2522

Ion	Ratio	Lower	Upper
75	100		
77	33.5	23.5	35.3



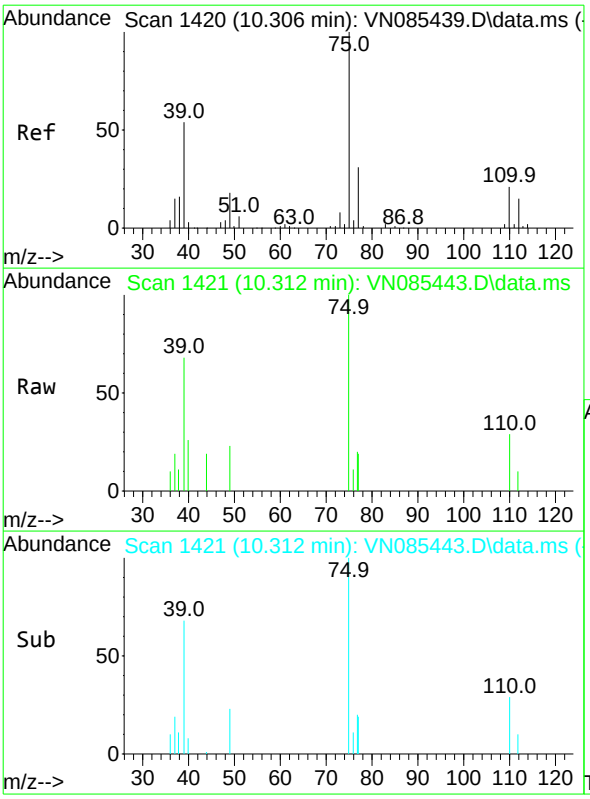

#54
cis-1,3-Dichloropropene
Concen: 0.811 ug/l
RT: 10.312 min Scan# 14
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 75 Resp: 2725

Ion	Ratio	Lower	Upper
75	100		
77	39.0	25.0	37.4#
39	67.6	43.1	64.7#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

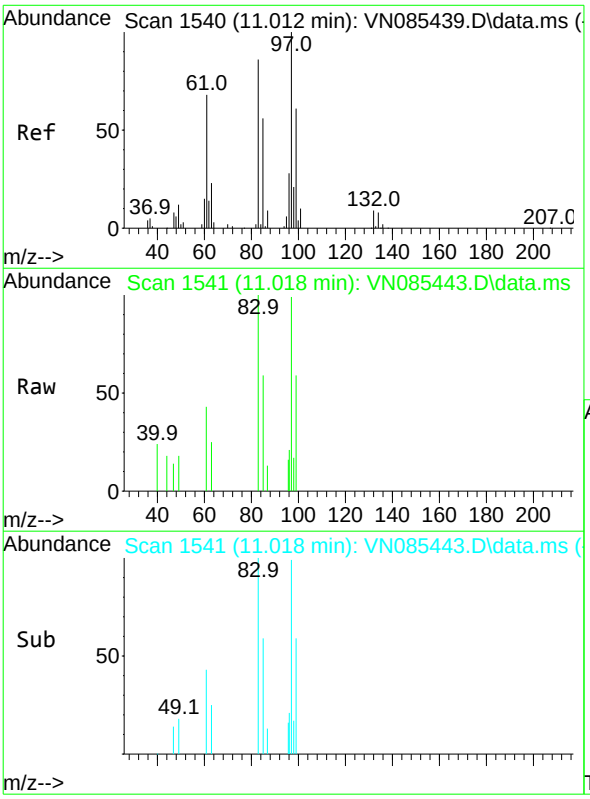

#55
1,1,2-Trichloroethane
Concen: 0.935 ug/l
RT: 11.018 min Scan# 1541
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 97 Resp: 1901

Ion	Ratio	Lower	Upper
97	100		
83	101.5	69.0	103.6
85	60.3	44.6	66.8
99	59.9	48.6	72.8



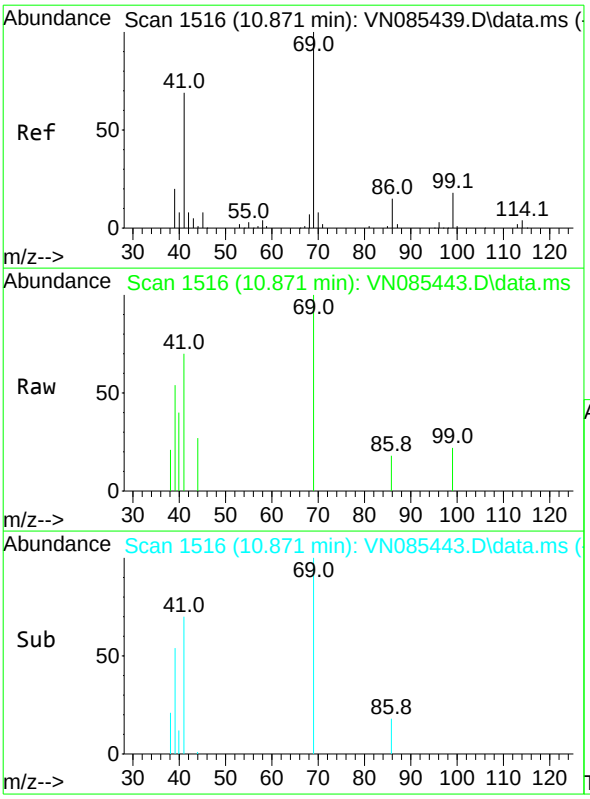

#56
Ethyl methacrylate
Concen: 2.471 ug/l
RT: 10.871 min Scan# 15
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 69 Resp: 1923

Ion	Ratio	Lower	Upper
69	100		
41	74.4	54.6	82.0
39	52.4	32.4	48.6#

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



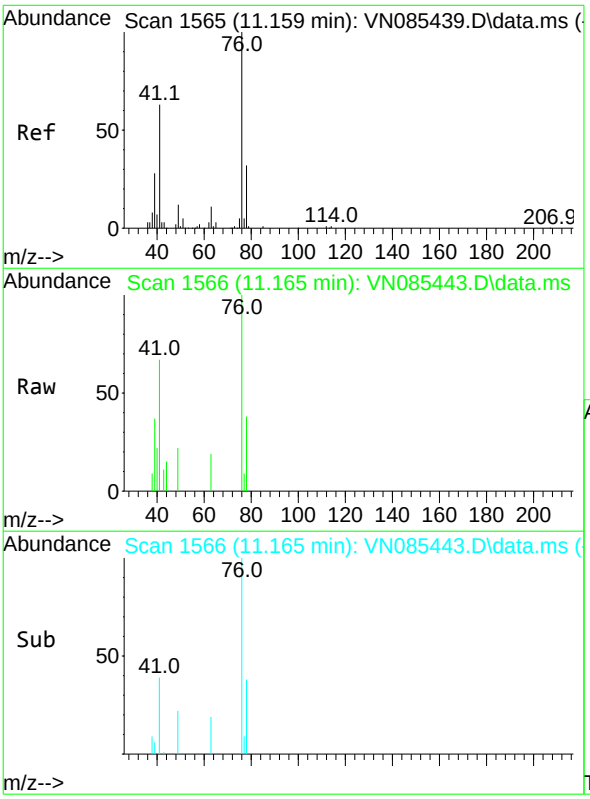

#57
1,3-Dichloropropane
Concen: 0.881 ug/l
RT: 11.165 min Scan# 1566
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 76 Resp: 3113

Ion	Ratio	Lower	Upper
76	100		
78	34.9	25.6	38.4



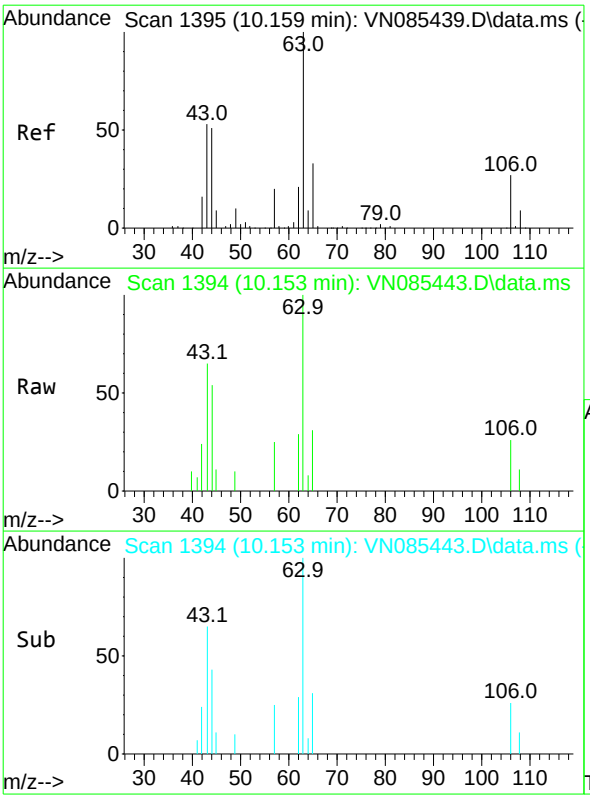

#58
2-Chloroethyl Vinyl ether
Concen: 3.822 ug/l
RT: 10.153 min Scan# 13
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 63 Resp: 4929

Ion	Ratio	Lower	Upper
63	100		
106	31.7	21.6	32.4

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



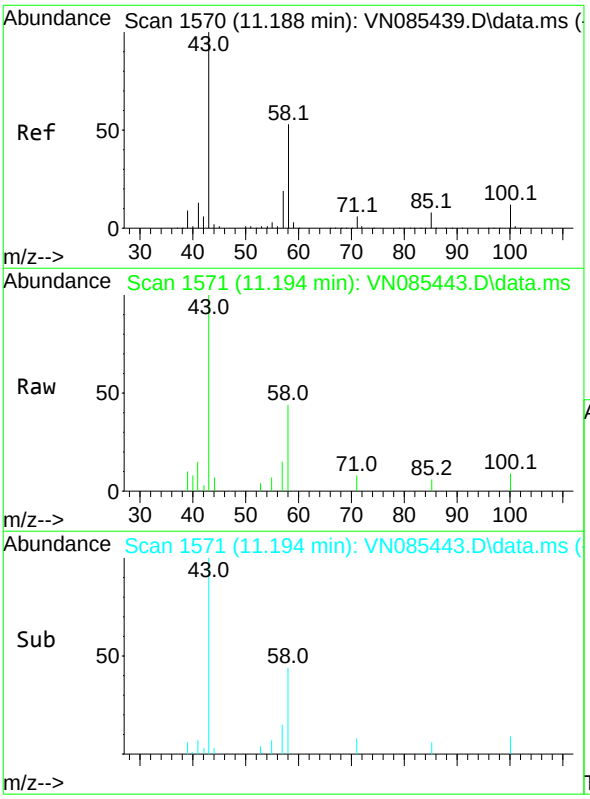

#59
2-Hexanone
Concen: 4.058 ug/l
RT: 11.194 min Scan# 1571
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 7905

Ion	Ratio	Lower	Upper
43	100		
58	42.9	26.2	78.6



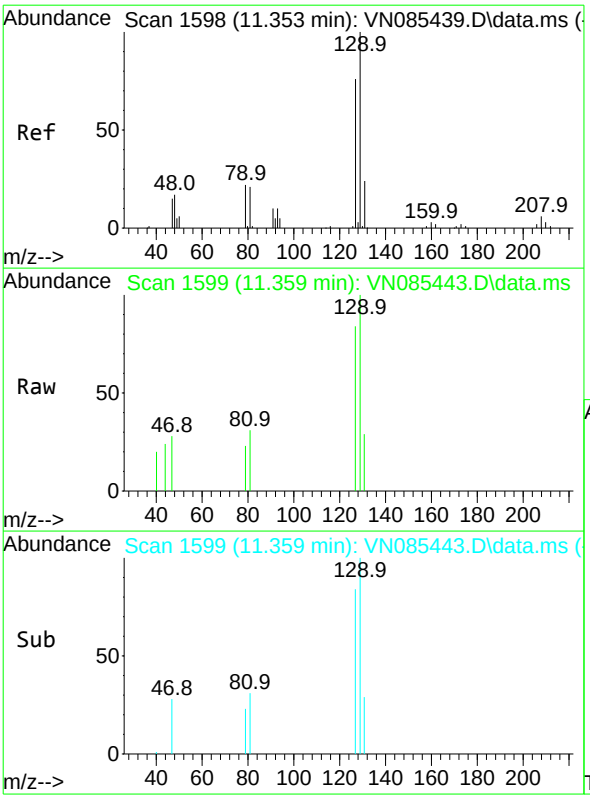

#60
Dibromochloromethane
Concen: 0.953 ug/l
RT: 11.359 min Scan# 15
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:129 Resp: 2339

Ion	Ratio	Lower	Upper
129	100		
127	78.9	38.6	115.8

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



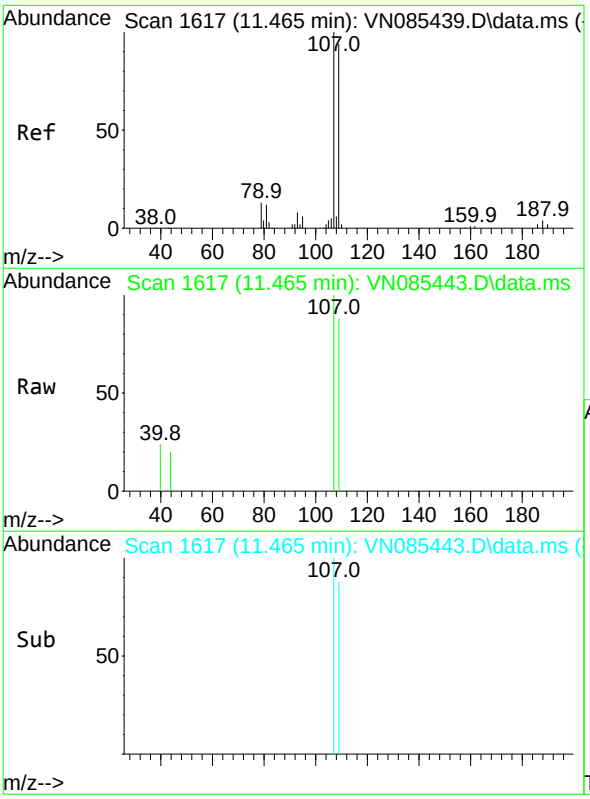

#61
1,2-Dibromoethane
Concen: 1.000 ug/l
RT: 11.465 min Scan# 1617
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:107 Resp: 2022

Ion	Ratio	Lower	Upper
107	100		
109	84.8	75.9	113.9



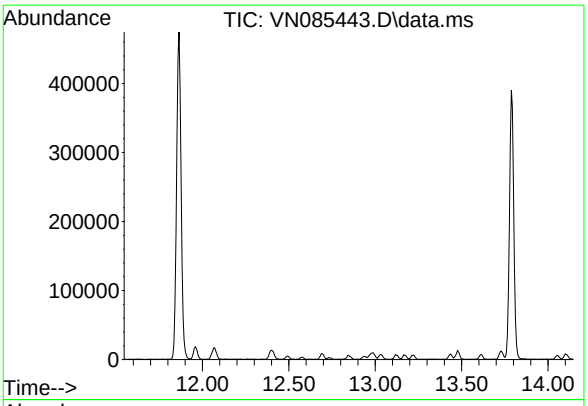

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.85 min

Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 95

Sig	Exp Ratio
95	100
174	72.5
176	71.2

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

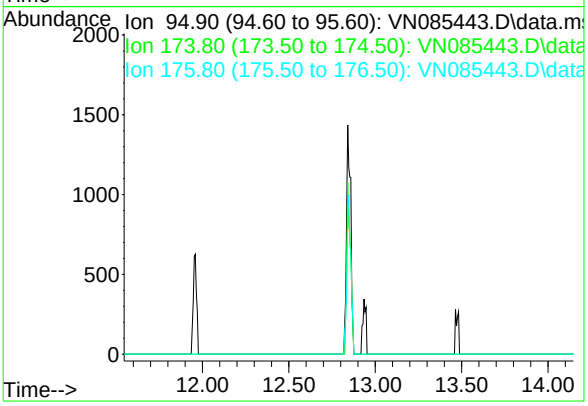

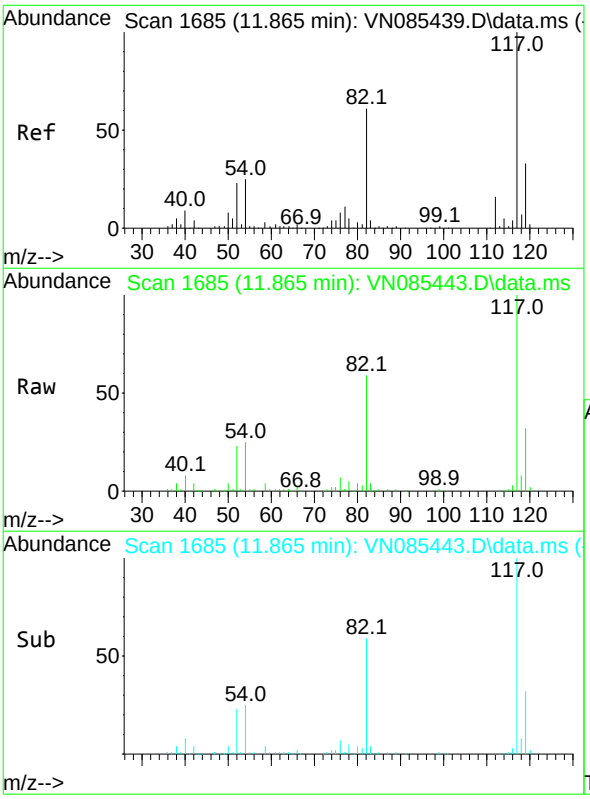

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:117 Resp: 256851

Ion	Ratio	Lower	Upper
117	100		
82	59.0	48.6	72.8
119	32.2	26.6	39.8

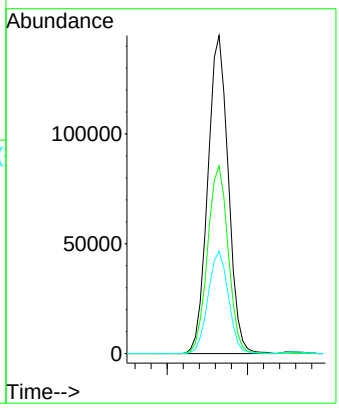

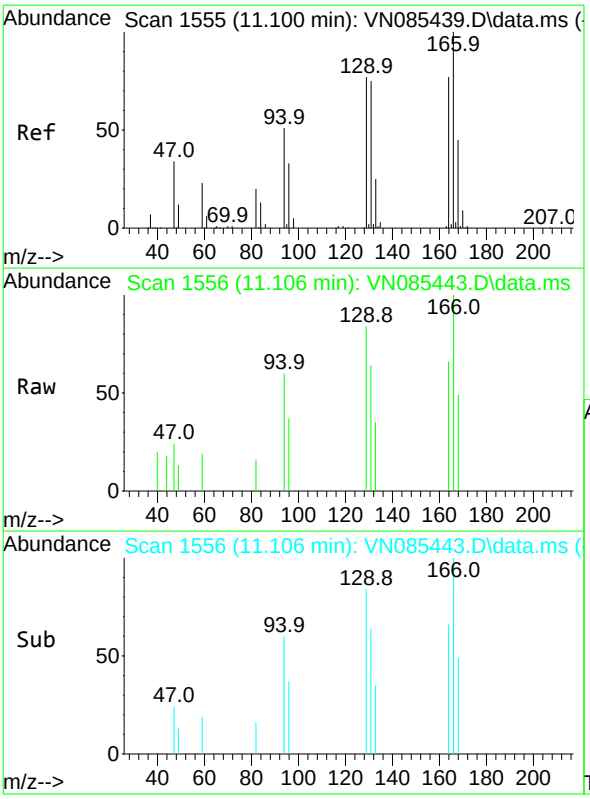

#64
Tetrachloroethene
Concen: 0.947 ug/l
RT: 11.106 min Scan# 15
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:164 Resp: 1658

Ion	Ratio	Lower	Upper
164	100		
166	152.1	103.4	155.2
129	128.3	79.2	118.8#
131	96.9	77.1	115.7



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

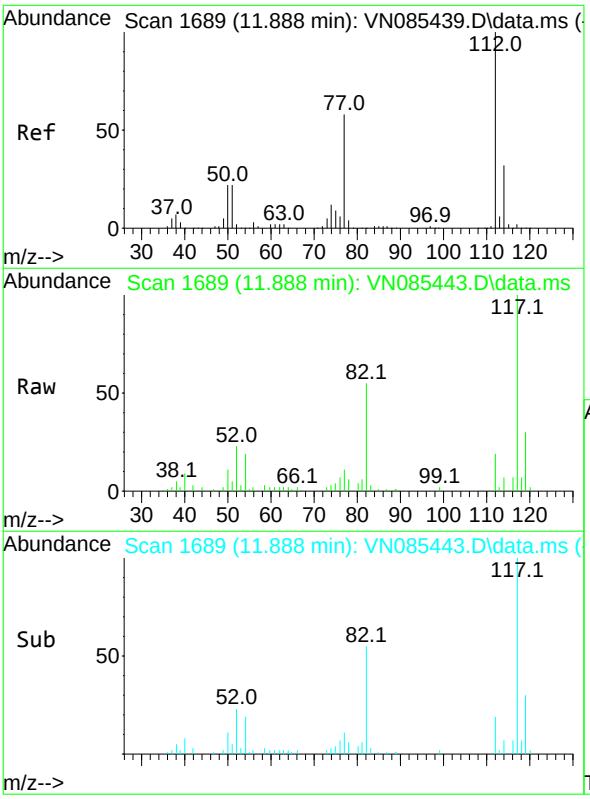

#65
Chlorobenzene
Concen: 0.960 ug/l
RT: 11.888 min Scan# 1689
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:112 Resp: 5401

Ion	Ratio	Lower	Upper
112	100		
114	35.3	25.3	37.9



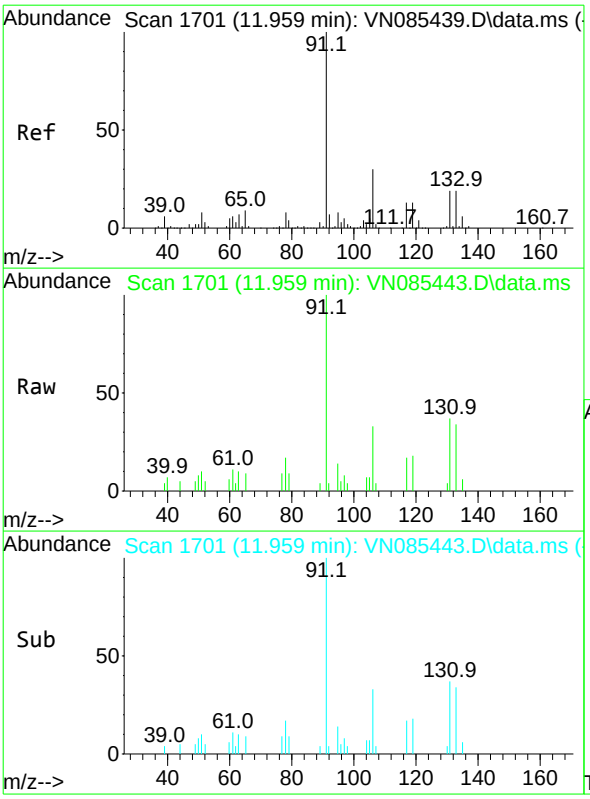

#66
1,1,1,2-Tetrachloroethane
Concen: 1.058 ug/l
RT: 11.959 min Scan# 17
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:131 Resp: 2185

Ion	Ratio	Lower	Upper
131	100		
133	97.7	47.4	142.3
119	0.0	33.1	99.5#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

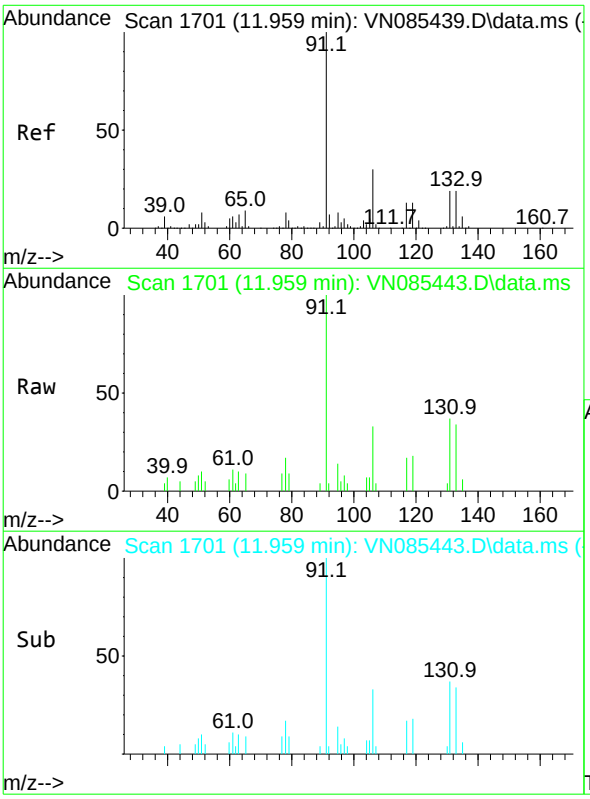

#67
Ethyl Benzene
Concen: 0.802 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 91 Resp: 7347

Ion	Ratio	Lower	Upper
91	100		
106	32.8	23.8	35.8



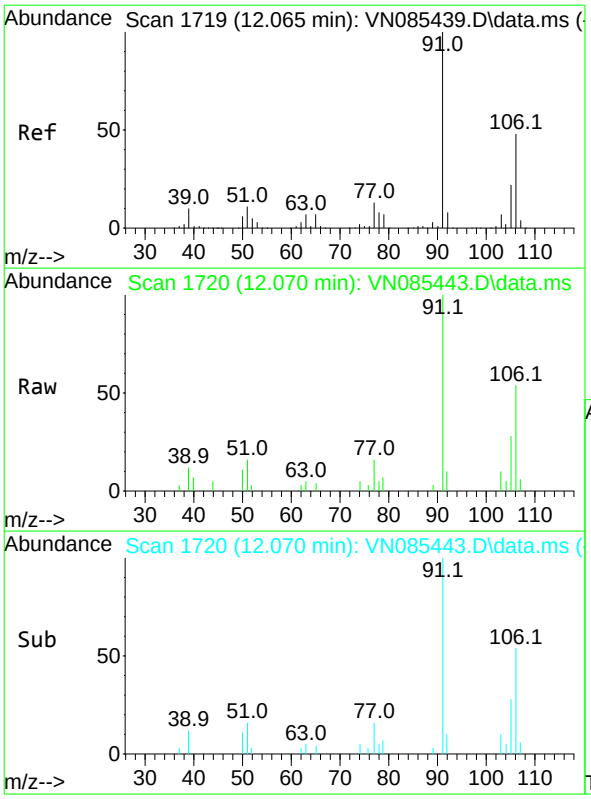

#68
m/p-Xylenes
Concen: 1.494 ug/l
RT: 12.070 min Scan# 17
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:106 Resp: 5059

Ion	Ratio	Lower	Upper
106	100		
91	209.3	167.7	251.5



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

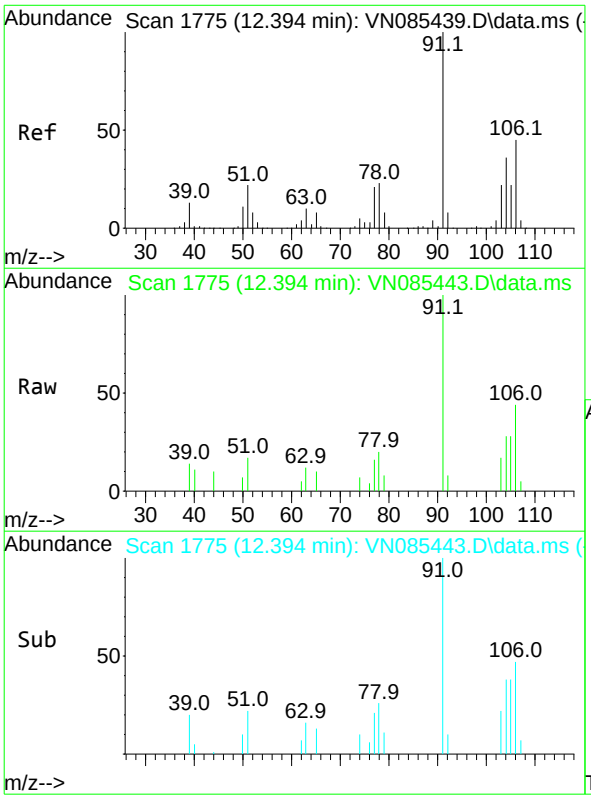

#69
o-Xylene
Concen: 0.766 ug/l
RT: 12.394 min Scan# 1775
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:106 Resp: 2478

Ion	Ratio	Lower	Upper
106	100		
91	225.4	110.4	331.2



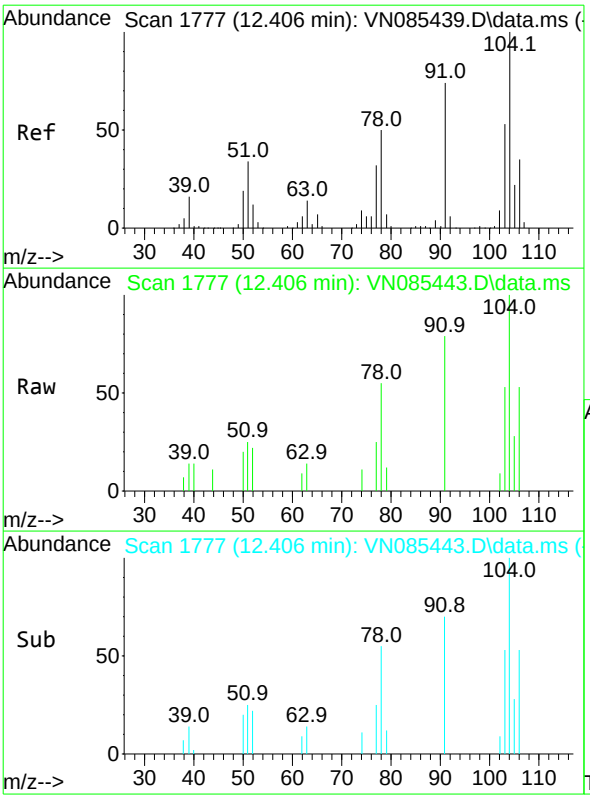

#70
Styrene
Concen: 0.712 ug/l
RT: 12.406 min Scan# 17
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:104 Resp: 3812

Ion	Ratio	Lower	Upper
104	100		
78	52.9	42.5	63.7
103	53.7	43.8	65.8



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

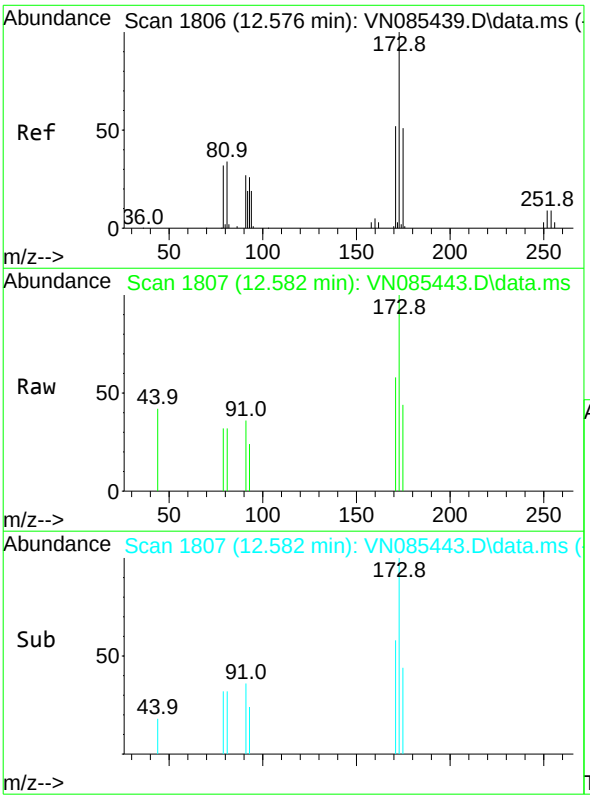

#71
Bromoform
Concen: 0.818 ug/l
RT: 12.582 min Scan# 1807
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:173 Resp: 1208

Ion	Ratio	Lower	Upper
173	100		
175	40.7	24.4	73.2
254	0.0	0.0	0.0



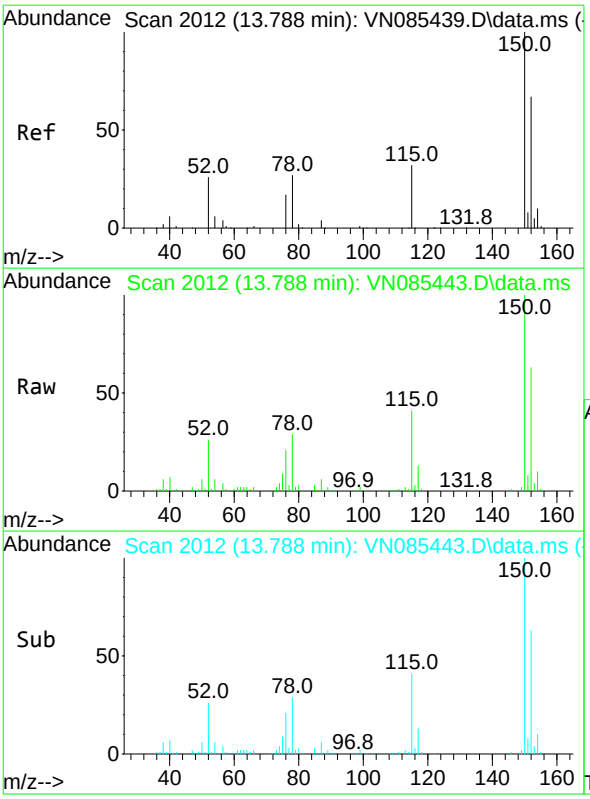

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:152 Resp: 99539

Ion	Ratio	Lower	Upper
152	100		
115	63.8	31.1	93.3
150	158.5	0.0	343.6

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



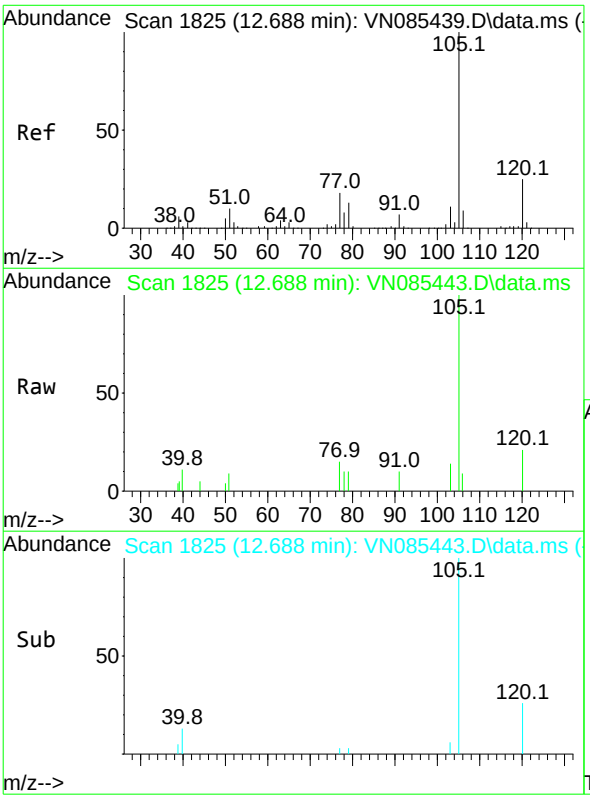

#73
Isopropylbenzene
Concen: 0.820 ug/l
RT: 12.688 min Scan# 1825
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:105 Resp: 5506

Ion	Ratio	Lower	Upper
105	100		
120	26.7	12.8	38.3



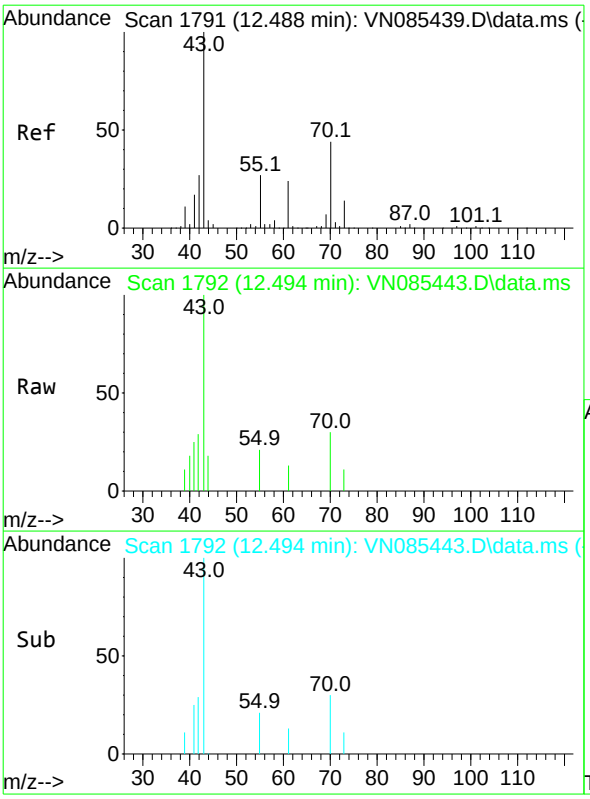

#74
N-amyl acetate
Concen: 0.899 ug/l
RT: 12.494 min Scan# 17
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 43 Resp: 2716

Ion	Ratio	Lower	Upper
43	100		
70	30.4	34.0	51.0#
55	24.2	21.4	32.2
61	17.6	19.0	28.4#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

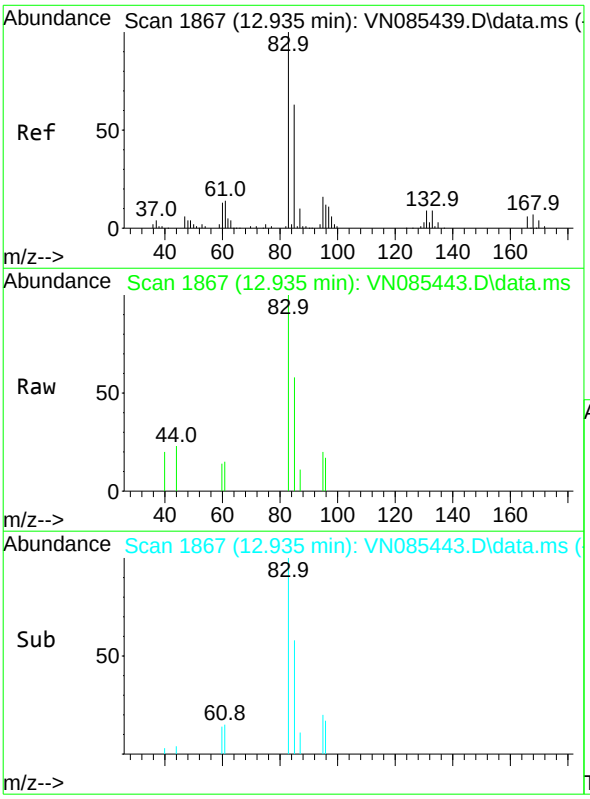

#75
1,1,2,2-Tetrachloroethane
Concen: 1.102 ug/l
RT: 12.935 min Scan# 1867
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 83 Resp: 2616

Ion	Ratio	Lower	Upper
83	100		
131	2.4	4.8	14.4#
85	65.7	32.2	96.6



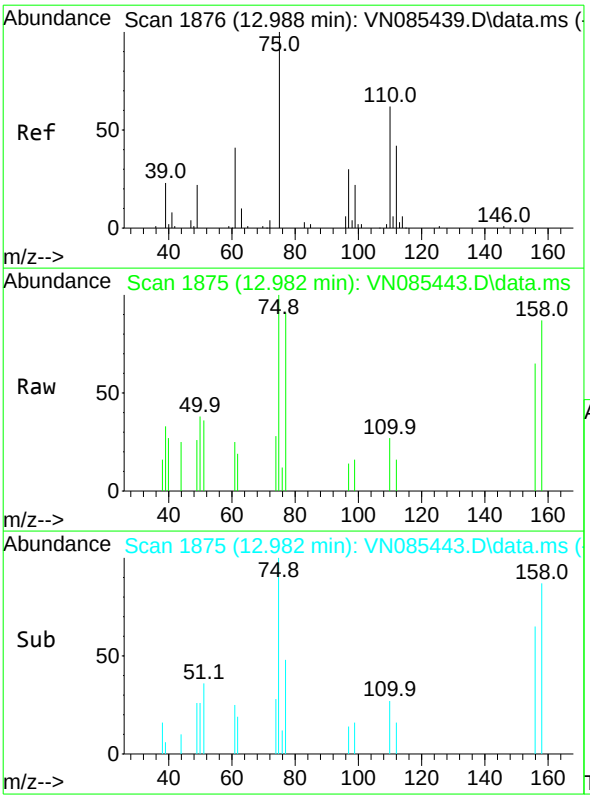

#76
1,2,3-Trichloropropane
Concen: 1.088 ug/l m
RT: 12.982 min Scan# 18
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 75 Resp: 2198

Ion	Ratio	Lower	Upper
75	100		
77	184.2	109.7	329.2



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

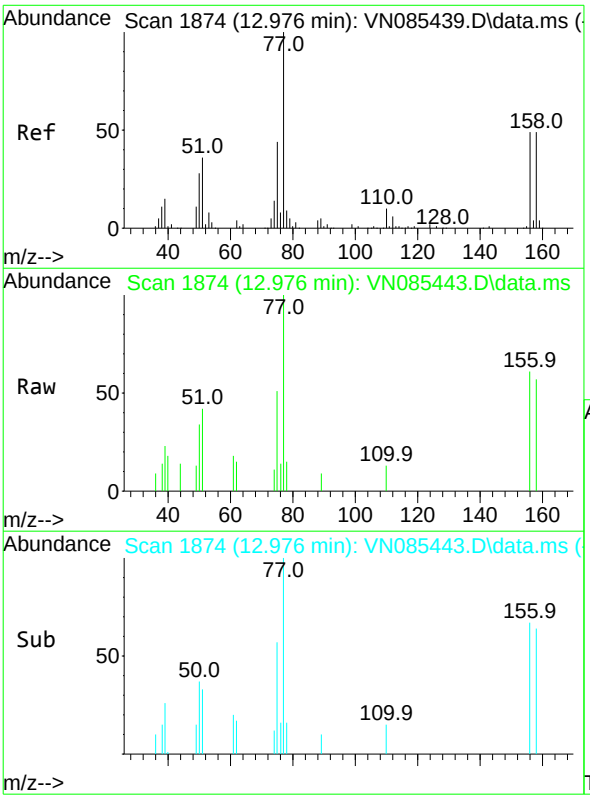

#77
Bromobenzene
Concen: 0.987 ug/l
RT: 12.976 min Scan# 1874
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:156 Resp: 1733

Ion	Ratio	Lower	Upper
156	100		
77	233.6	114.1	342.4
158	94.9	48.9	146.8



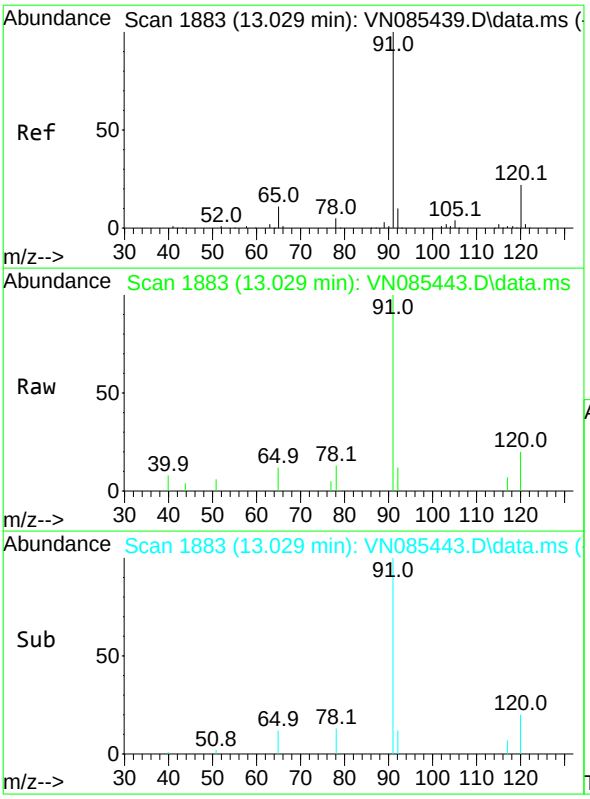

#78
n-propylbenzene
Concen: 0.808 ug/l
RT: 13.029 min Scan# 18
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 91 Resp: 6424

Ion	Ratio	Lower	Upper
91	100		
120	18.2	10.9	32.6

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



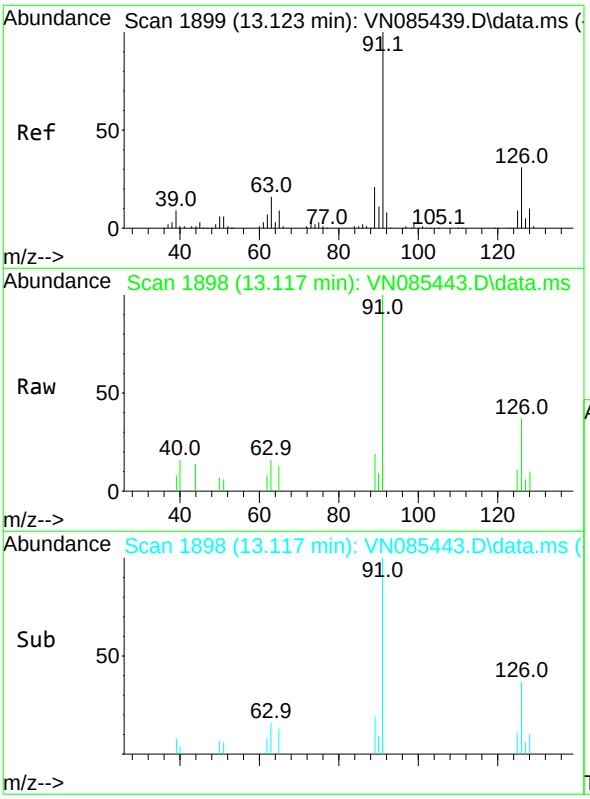

#79
2-Chlorotoluene
Concen: 0.871 ug/l
RT: 13.117 min Scan# 1898
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 91 Resp: 4483

Ion	Ratio	Lower	Upper
91	100		
126	32.9	15.7	47.1



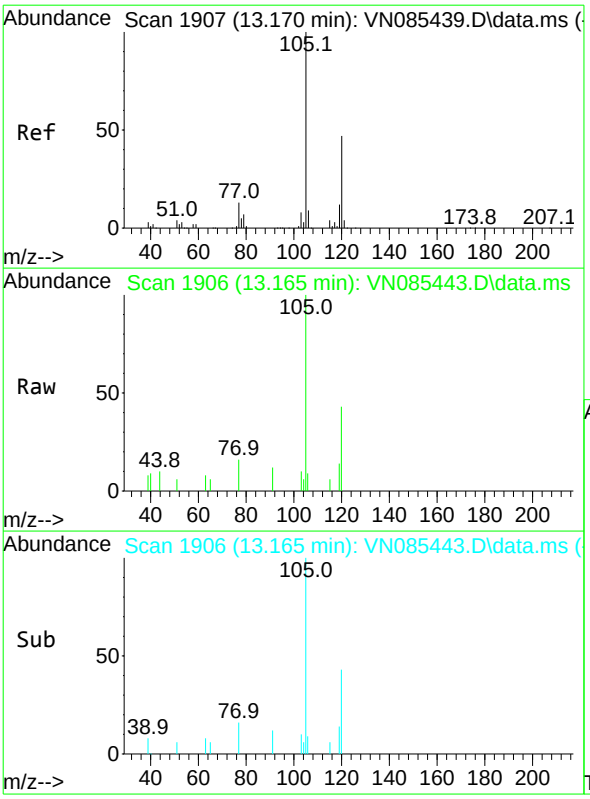

#80
1,3,5-Trimethylbenzene
Concen: 0.775 ug/l
RT: 13.165 min Scan# 19
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:105 Resp: 4301

Ion	Ratio	Lower	Upper
105	100		
120	41.2	23.9	71.7



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

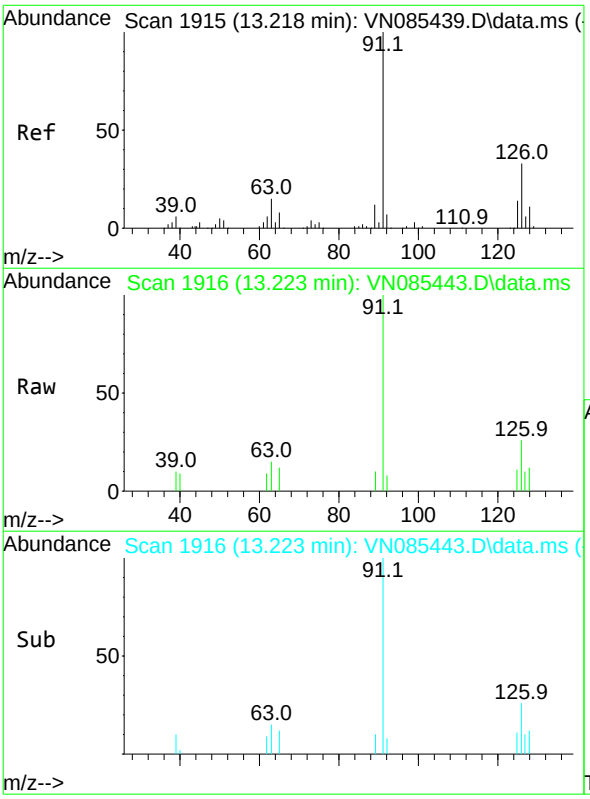

#82
4-Chlorotoluene
Concen: 0.833 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 91 Resp: 4268

Ion	Ratio	Lower	Upper
91	100		
126	31.0	15.9	47.7



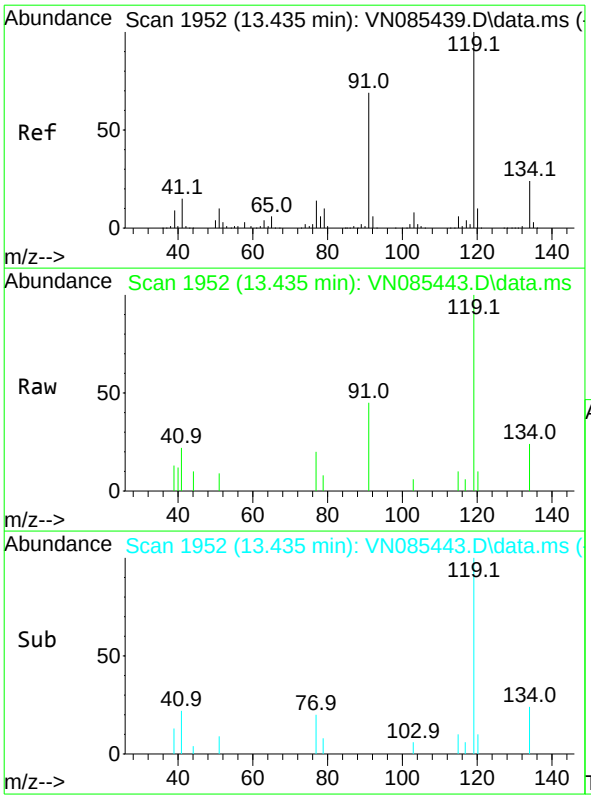

#83
tert-Butylbenzene
Concen: 0.805 ug/l
RT: 13.435 min Scan# 19
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:119 Resp: 3753

Ion	Ratio	Lower	Upper
119	100		
91	65.9	35.1	105.3
134	24.9	12.0	36.1

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



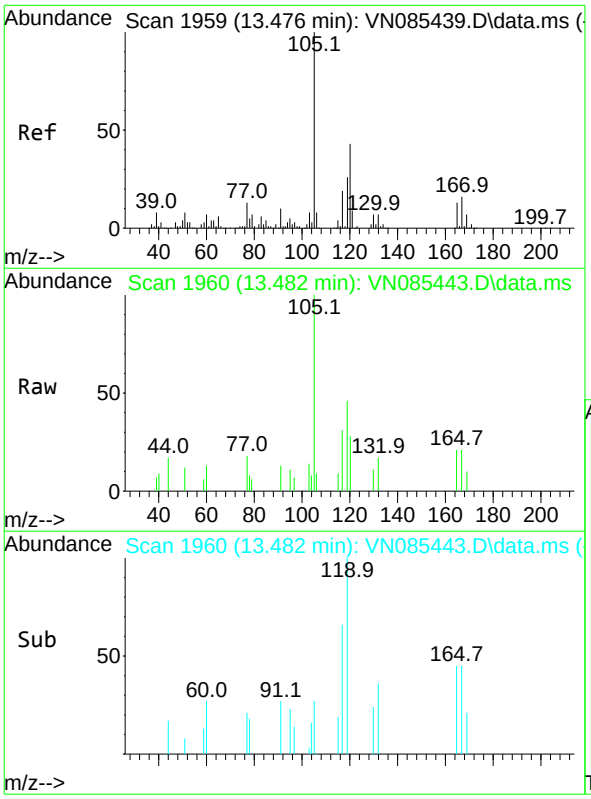

#84
1,2,4-Trimethylbenzene
Concen: 0.679 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:105 Resp: 3758

Ion	Ratio	Lower	Upper
105	100		
120	47.7	21.6	65.0



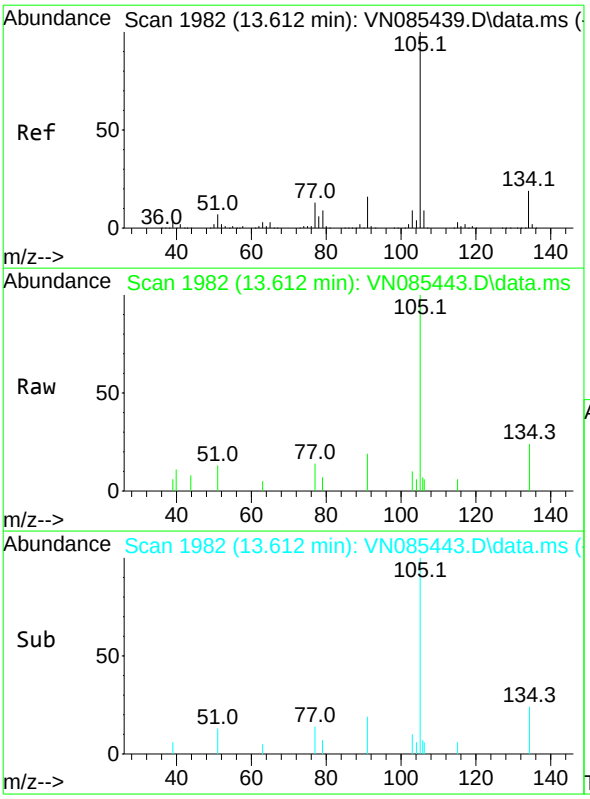

#85
sec-Butylbenzene
Concen: 0.714 ug/l
RT: 13.612 min Scan# 19
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:105 Resp: 4614

Ion	Ratio	Lower	Upper
105	100		
134	19.9	9.7	28.9



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

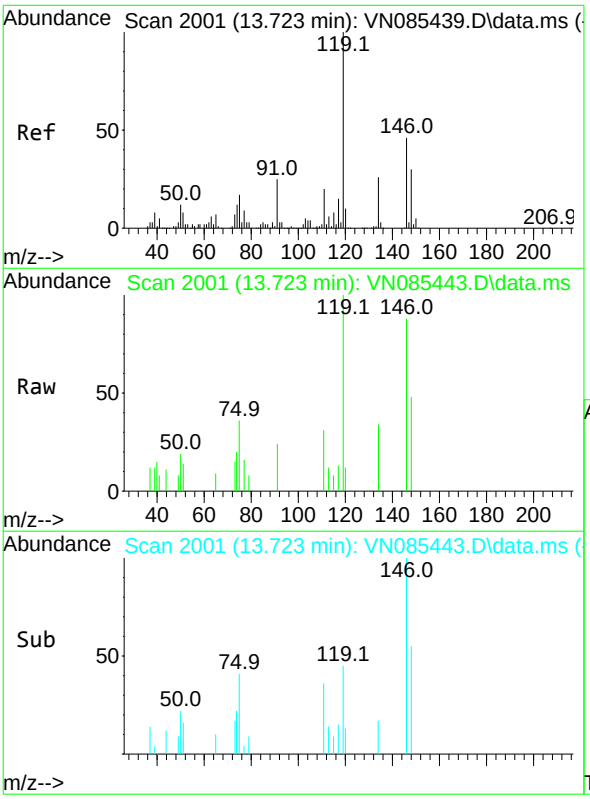

#86
p-Isopropyltoluene
Concen: 0.716 ug/l
RT: 13.723 min Scan# 2001
Delta R.T. 0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:119 Resp: 3538

Ion	Ratio	Lower	Upper
119	100		
134	25.6	12.7	38.0
91	23.2	12.7	38.1



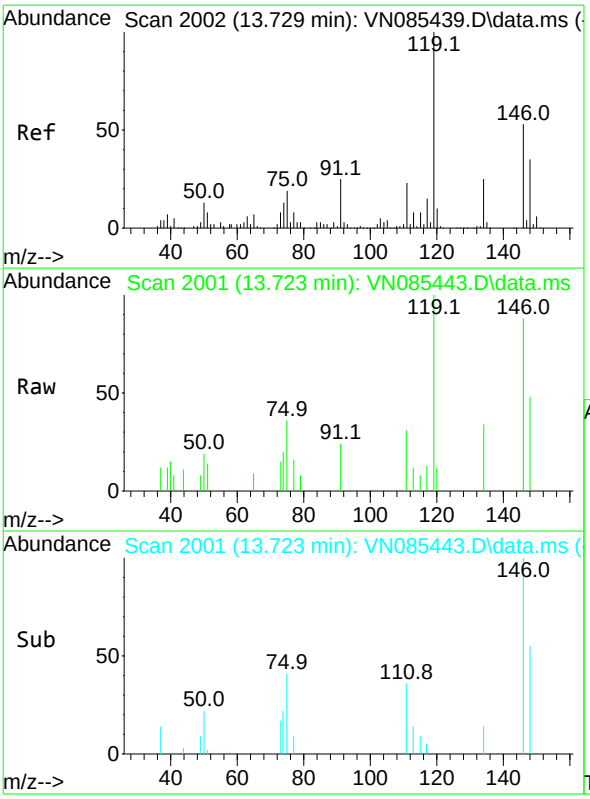

#87
1,3-Dichlorobenzene
Concen: 0.940 ug/l
RT: 13.723 min Scan# 20
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:146 Resp: 3038

Ion	Ratio	Lower	Upper
146	100		
111	43.0	21.4	64.3
148	70.9	32.3	96.9



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

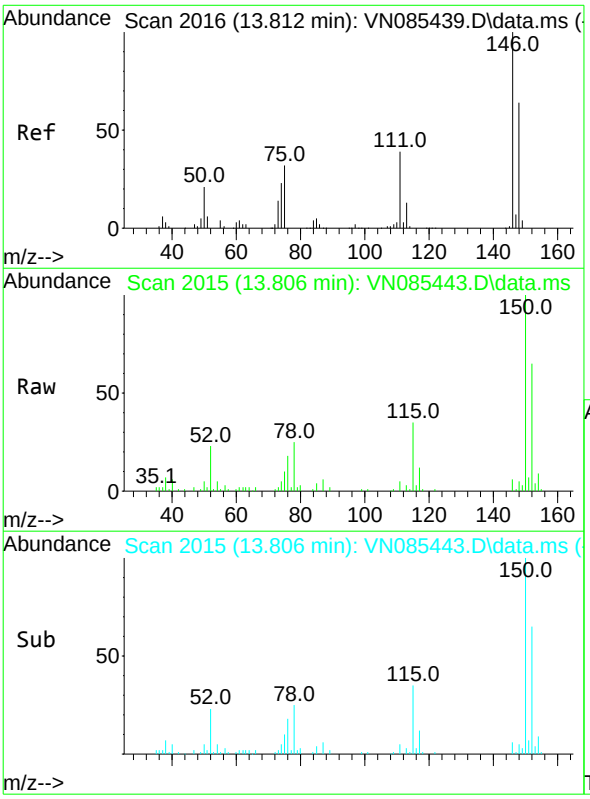

#88
1,4-Dichlorobenzene
Concen: 1.050 ug/l m
RT: 13.806 min Scan# 2015
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:146 Resp: 3517

Ion	Ratio	Lower	Upper
146	100		
111	37.2	21.3	63.7
148	61.2	32.4	97.0



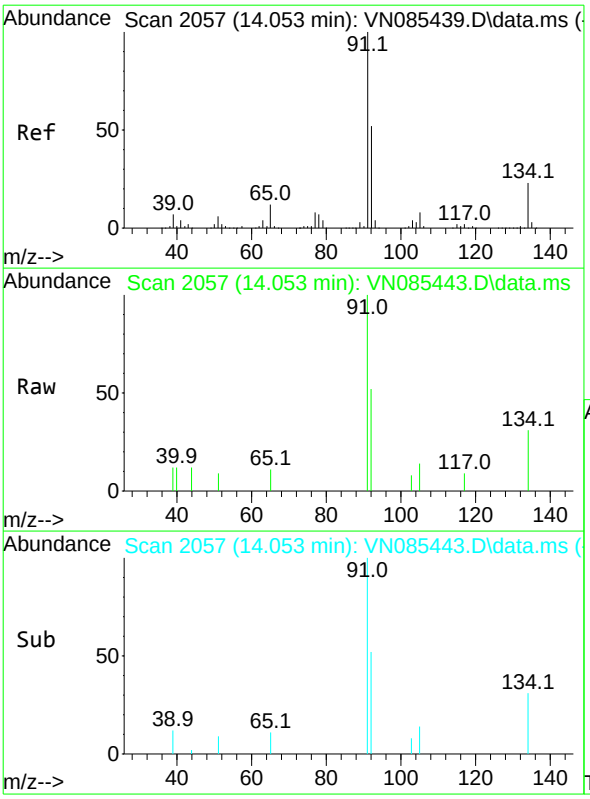

#89
n-Butylbenzene
Concen: 0.761 ug/l
RT: 14.053 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 91 Resp: 3527

Ion	Ratio	Lower	Upper
91	100		
92	57.2	25.8	77.3
134	25.5	11.7	35.1



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

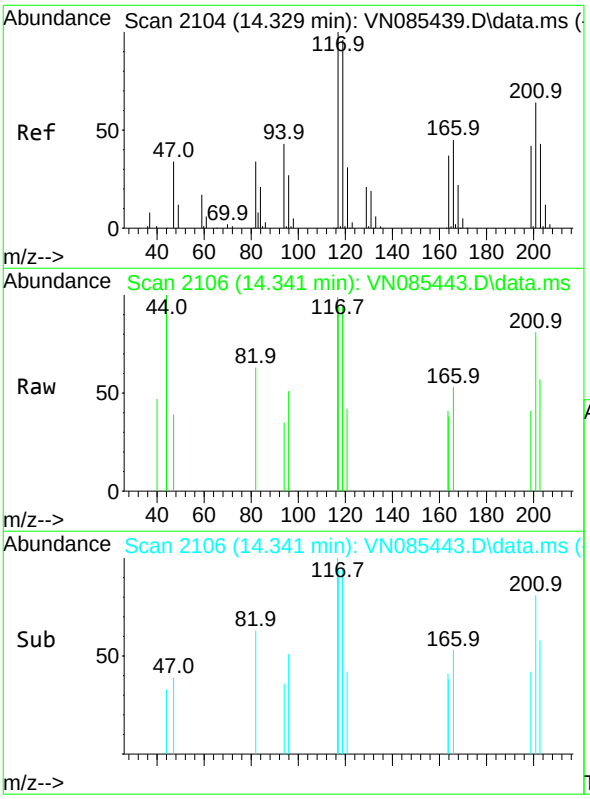

#90
Hexachloroethane
Concen: 1.102 ug/l
RT: 14.341 min Scan# 2106
Delta R.T. 0.012 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:117 Resp: 1355

Ion	Ratio	Lower	Upper
117	100		
201	66.5	33.7	101.0



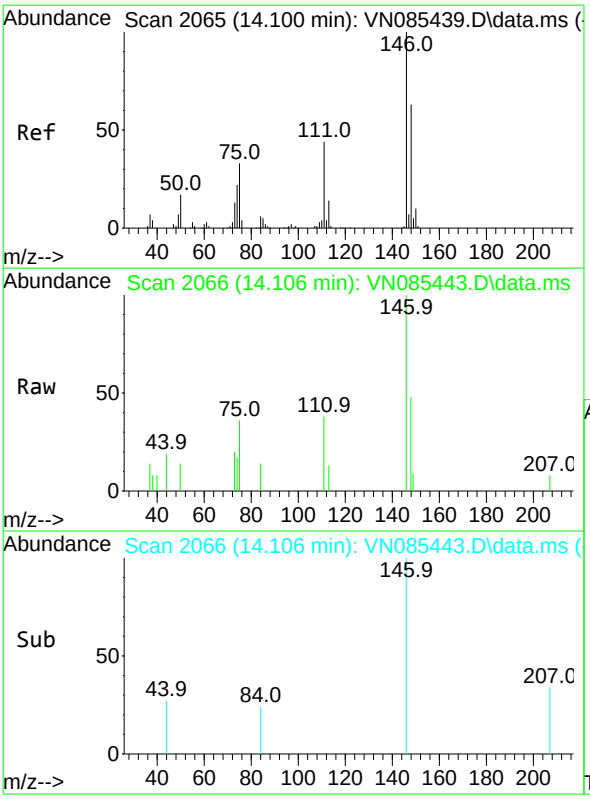

#91
1,2-Dichlorobenzene
Concen: 1.090 ug/l
RT: 14.106 min Scan# 20
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:146 Resp: 3515

Ion	Ratio	Lower	Upper
146	100		
111	43.4	21.7	65.1
148	57.8	31.4	94.2



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

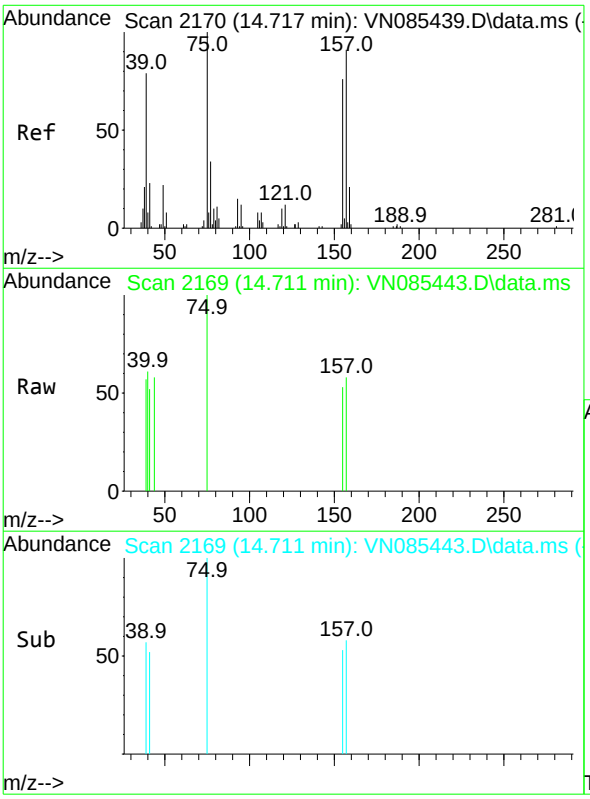

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.928 ug/l
RT: 14.711 min Scan# 2169
Delta R.T. -0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion: 75 Resp: 402

Ion	Ratio	Lower	Upper
75	100		
155	48.0	36.4	109.2
157	112.7	45.4	136.1



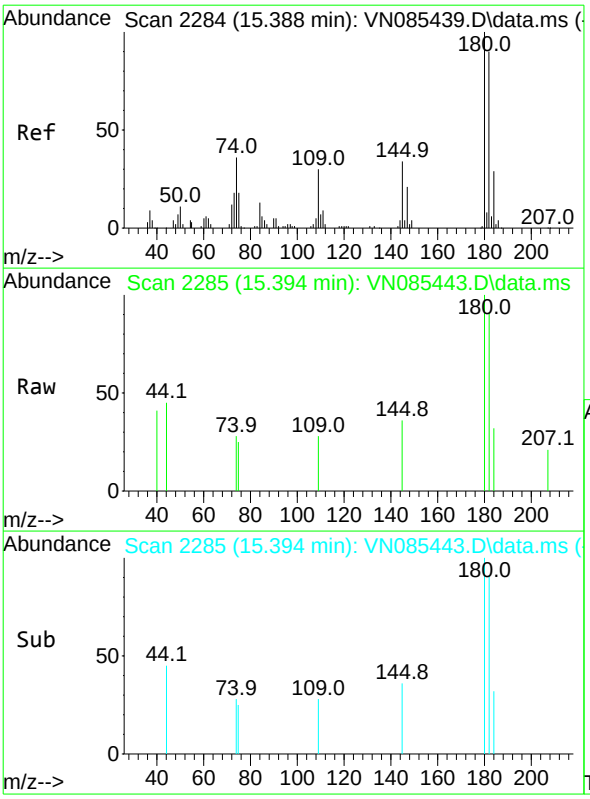

#93
1,2,4-Trichlorobenzene
Concen: 0.874 ug/l
RT: 15.394 min Scan# 22
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:180 Resp: 1310

Ion	Ratio	Lower	Upper
180	100		
182	106.3	46.8	140.3
145	9.7	16.0	48.0#



Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

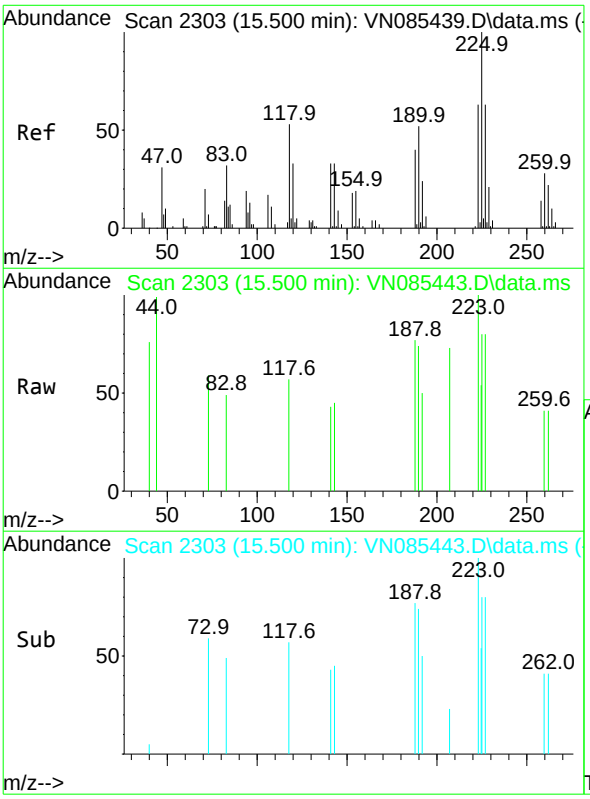

#94
Hexachlorobutadiene
Concen: 1.033 ug/l
RT: 15.500 min Scan# 2303
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:225 Resp: 822

Ion	Ratio	Lower	Upper
225	100		
223	50.7	30.7	92.1
227	55.7	30.9	92.5



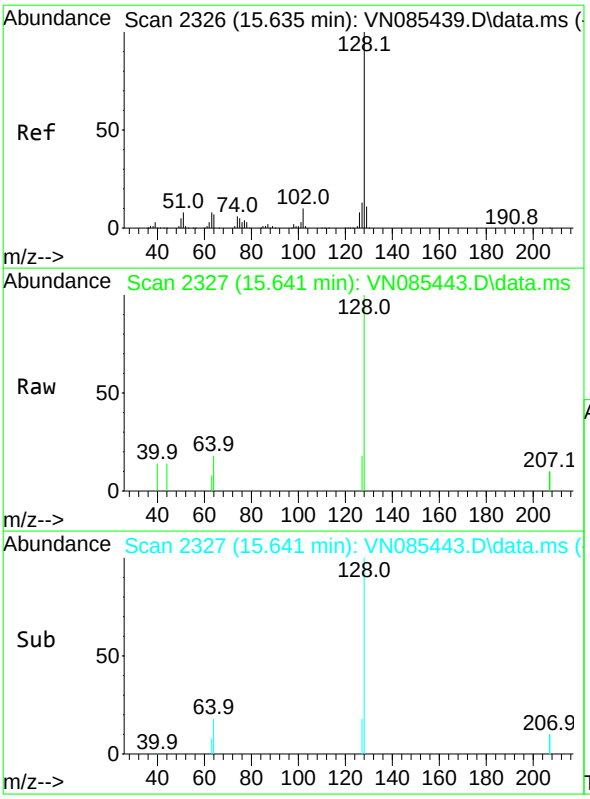

#95
Naphthalene
Concen: 0.941 ug/l
RT: 15.641 min Scan# 23
Delta R.T. 0.006 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:128 Resp: 4210

Ion	Ratio	Lower	Upper
128	100		
127	11.1	10.6	16.0
129	5.3	8.8	13.2#

Instrument :
MSVOA_N
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025



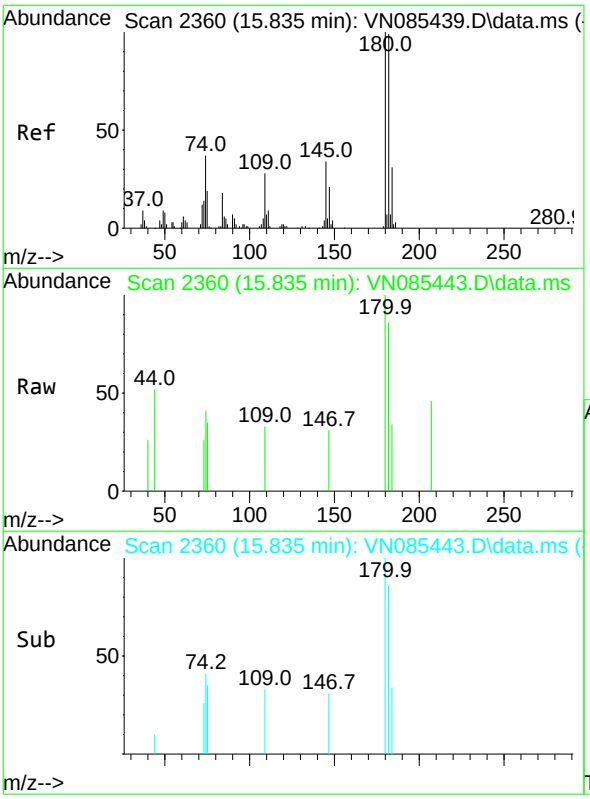

#96
1,2,3-Trichlorobenzene
Concen: 0.985 ug/l
RT: 15.835 min Scan# 2360
Delta R.T. -0.000 min
Lab File: VN085443.D
Acq: 14 Jan 2025 17:19

Tgt Ion:180 Resp: 1494

Ion	Ratio	Lower	Upper
180	100		
182	90.2	47.4	142.2
145	11.8	16.9	50.7#