
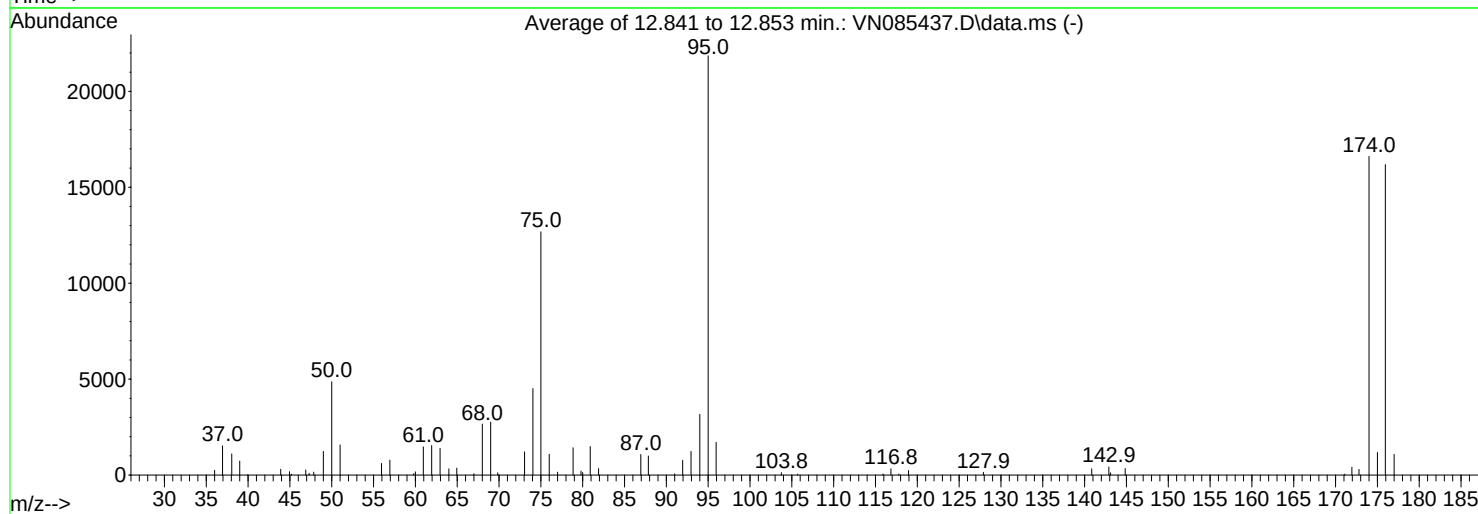


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011425\
Data File : VN085437.D
Acq On : 14 Jan 2025 14:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

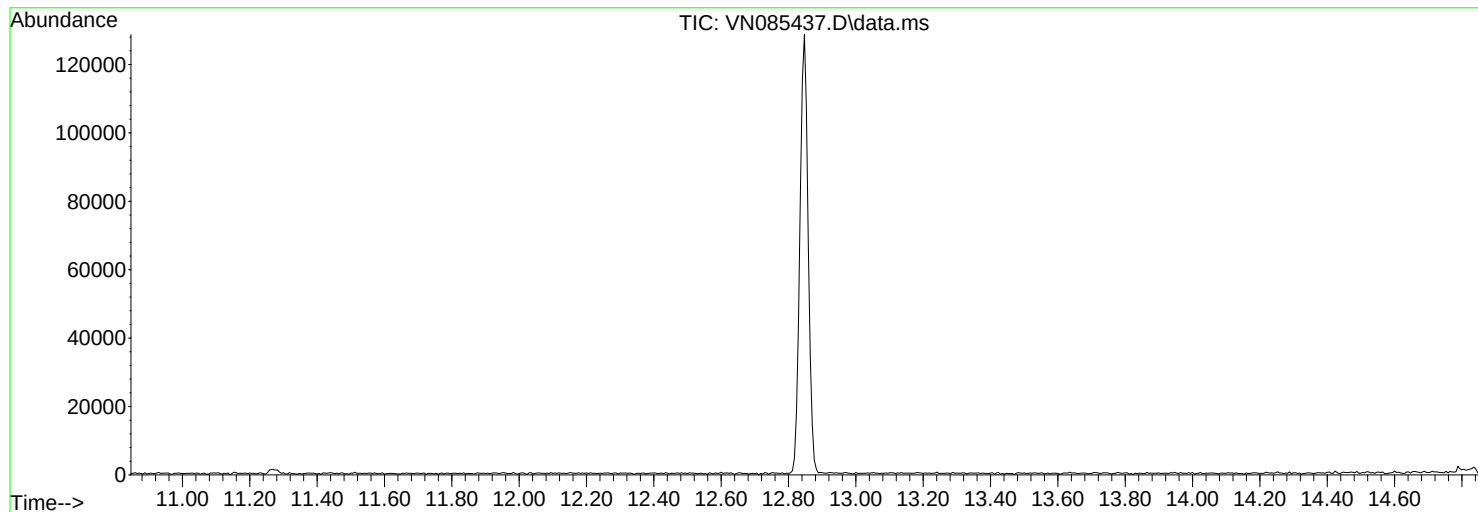

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	4864	PASS
75	95	30	60	58.0	12679	PASS
95	95	100	100	100.0	21856	PASS
96	95	5	9	7.8	1703	PASS
173	174	0.00	2	1.8	296	PASS
174	95	50	100	76.0	16613	PASS
175	174	5	9	7.1	1179	PASS
176	174	95	101	97.4	16185	PASS
177	176	5	9	6.7	1079	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	254	49.00	1237	64.95	364	79.80	211
36.95	1525	50.00	4864	67.00	71	80.00	136
38.05	1107	51.00	1571	68.00	2658	80.90	1487
39.00	730	55.95	608	69.00	2763	81.90	338
39.90	5	56.95	779	69.85	123	86.95	1072
43.90	302	59.80	76	73.05	1212	87.85	997
44.95	180	60.00	170	74.05	4514	91.00	68
45.20	50	60.95	1471	75.00	12679	91.95	773
46.90	269	61.95	1539	76.00	1086	92.95	1234
47.30	94	62.95	1390	77.00	153	94.00	3163
47.85	154	64.00	325	78.85	1426	95.00	21856

Average of 12.841 to 12.853 min.: VN085437.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.95	1703	144.85	346				
103.75	127	171.10	56				
105.70	51	171.95	407				
115.90	59	172.80	296				
116.85	327	174.00	16613				
117.80	58	175.00	1179				
118.95	233	175.95	16185				
127.90	145	177.00	1079				
140.85	328						
142.90	422						
143.10	115						

Instrument :

MSVOA_N

ClientSampleId :

BFB