


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011525\
Data File : BF141162.D
Acq On : 15 Jan 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

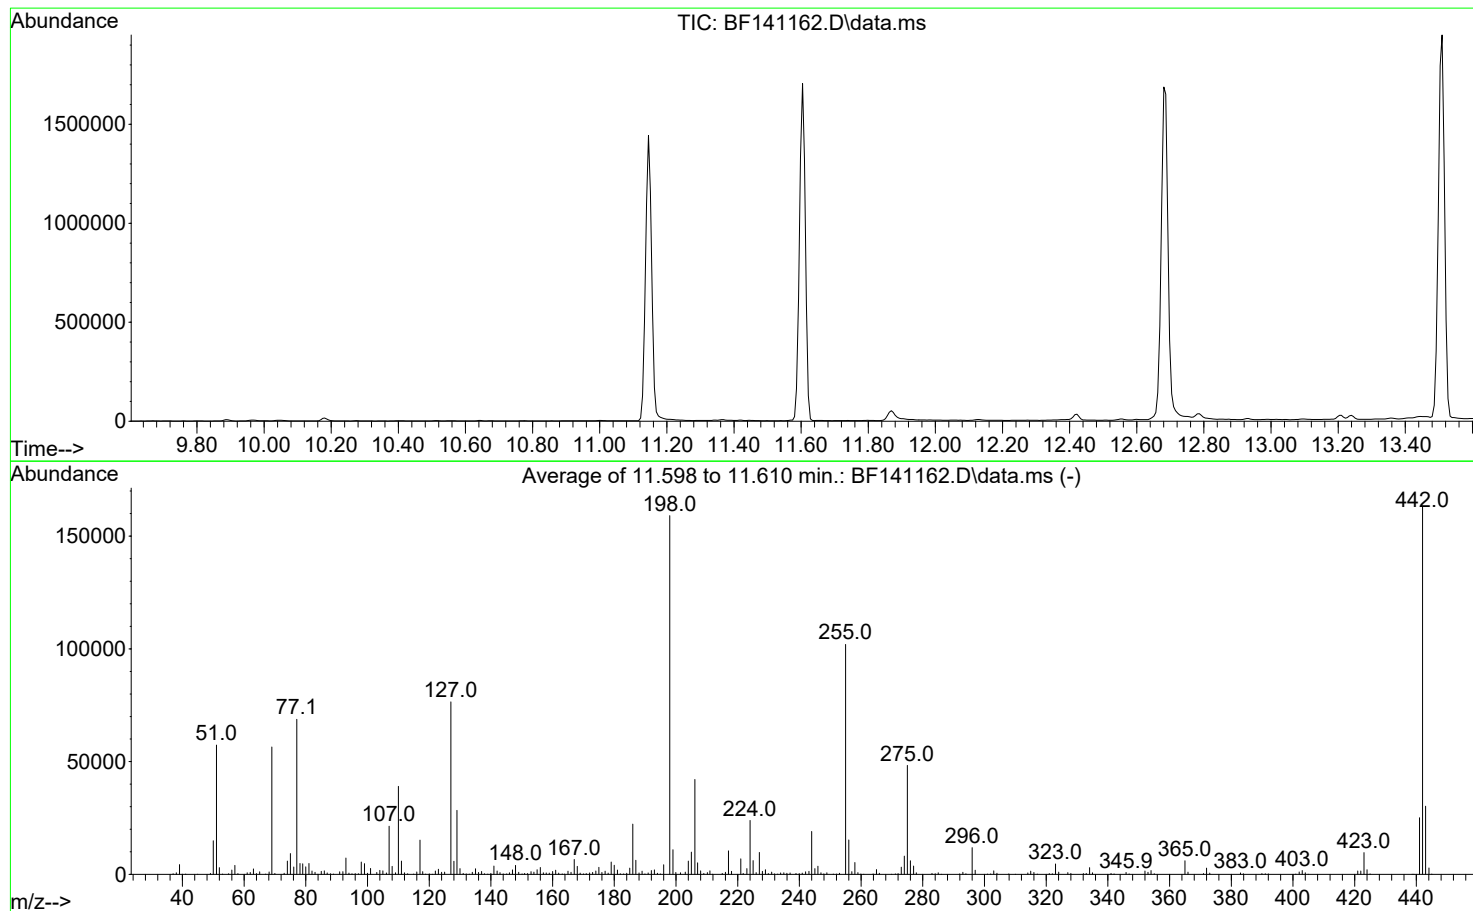

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	57307	PASS
68	69	0.00	2	1.9	1055	PASS
69	198	0.00	100	35.5	56501	PASS
70	69	0.00	2	0.8	449	PASS
127	198	10	80	48.1	76515	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159104	PASS
199	198	5	9	6.9	10934	PASS
275	198	10	60	30.4	48325	PASS
365	198	1	100	3.8	6020	PASS
441	198	0.01	100	15.8	25096	PASS
442	442	50	100	100.0	163141	PASS
443	442	15	24	18.5	30253	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/15/2025	BNA_F	<u>BF141162.D</u>
Compound Name	Response	Retention Time
DDT	495212	13.51
DDD	10841	13.21
DDE	490	12.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11331	506543	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011525\
Data File : BF141162.D
Acq On : 15 Jan 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 15 10:11:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

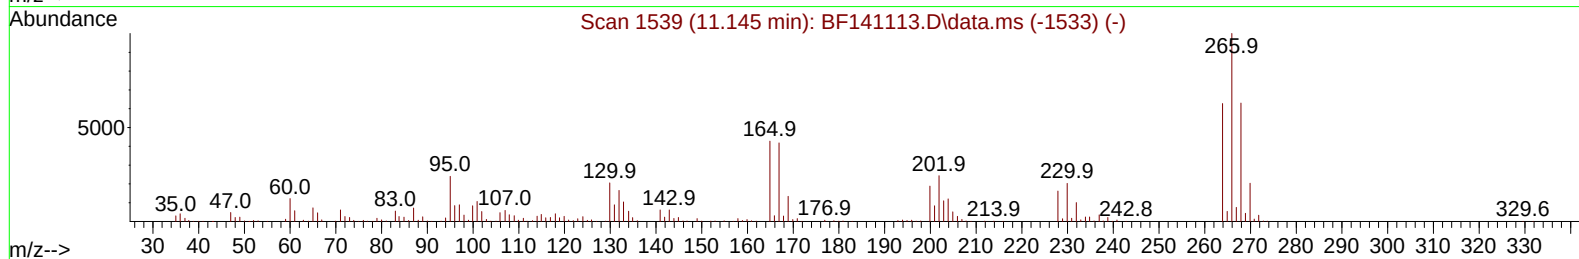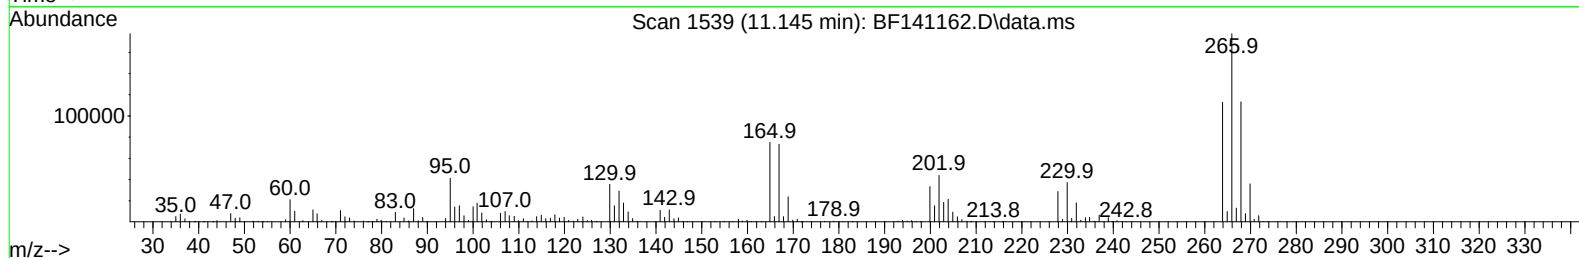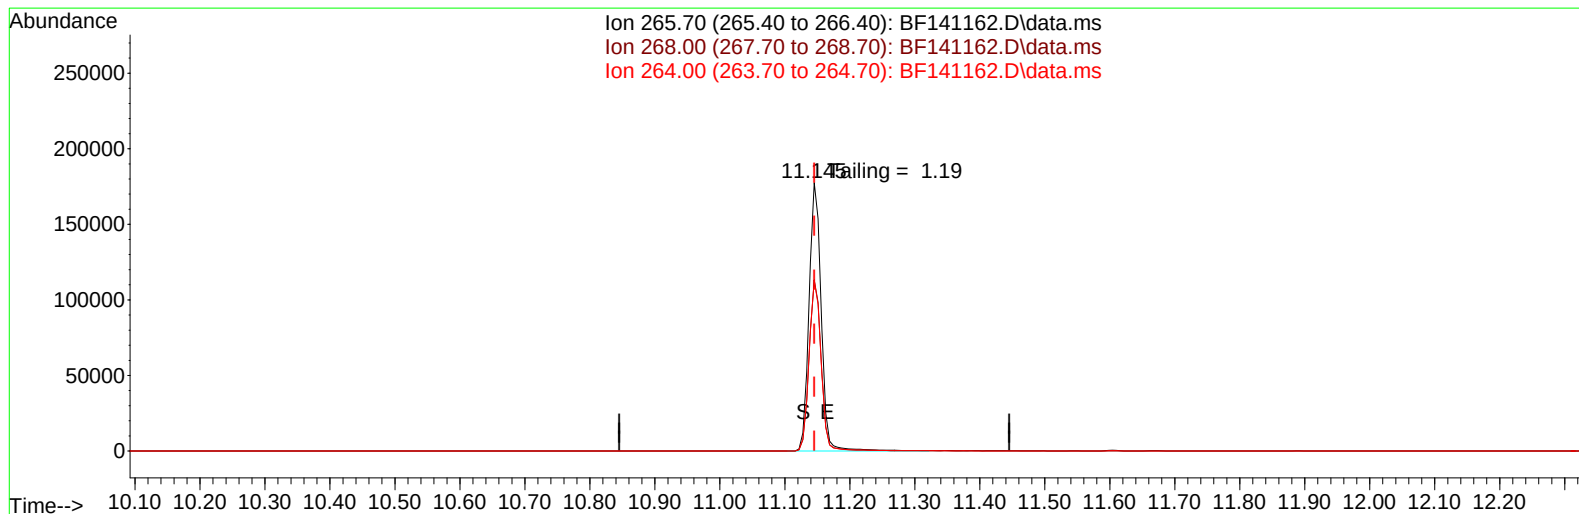

TIC: BF141162.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 17848.17 ng




response 232184

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.76
264.00	62.70	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011525\
Data File : BF141162.D
Acq On : 15 Jan 2025 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 15 10:11:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

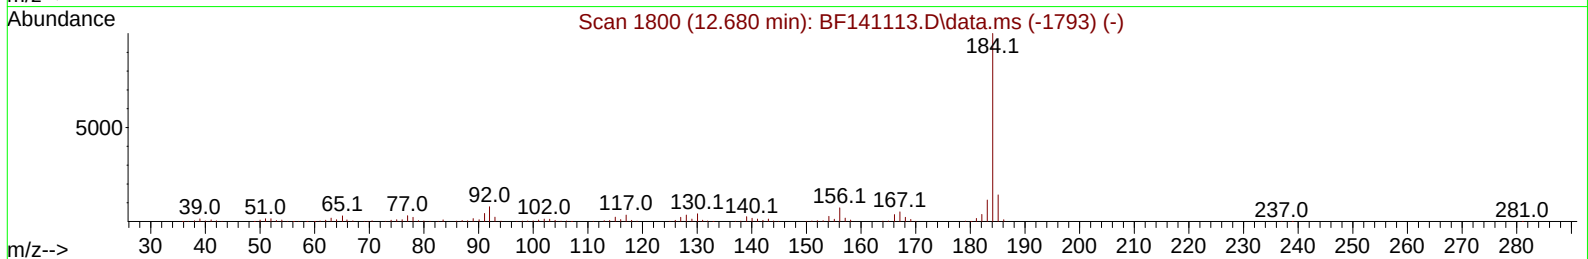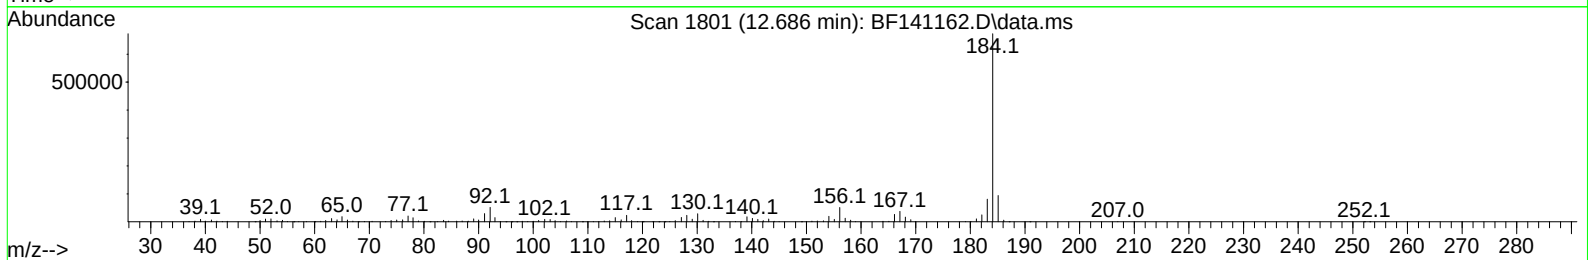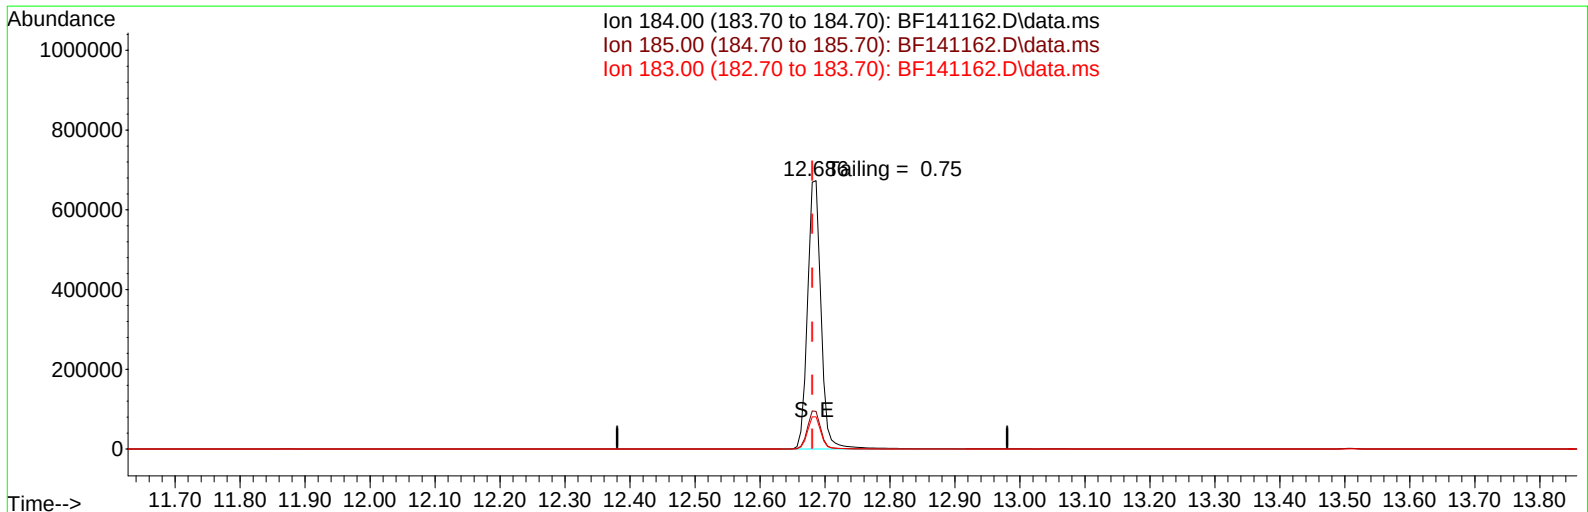

TIC: BF141162.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 34812.04 ng

response 973516

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.00
183.00	11.50	12.01
0.00	0.00	0.00