
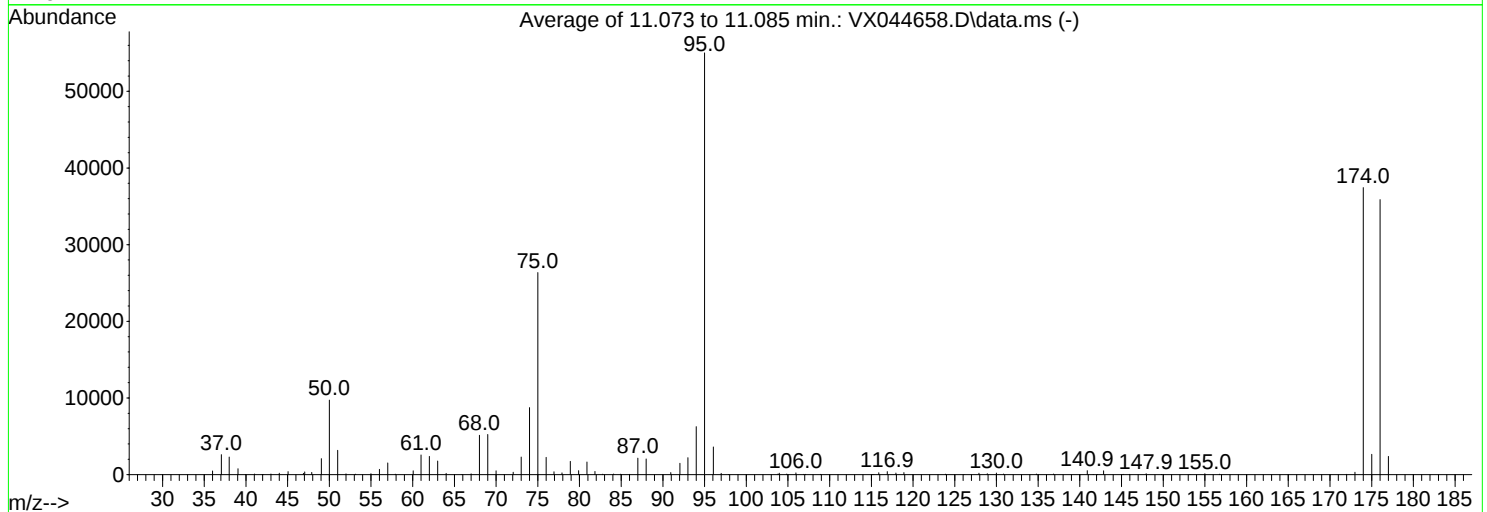


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011625\
Data File : VX044658.D
Acq On : 16 Jan 2025 08:02
Operator :
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Title : SW846 8260
Last Update : Mon Oct 28 13:41:34 2024

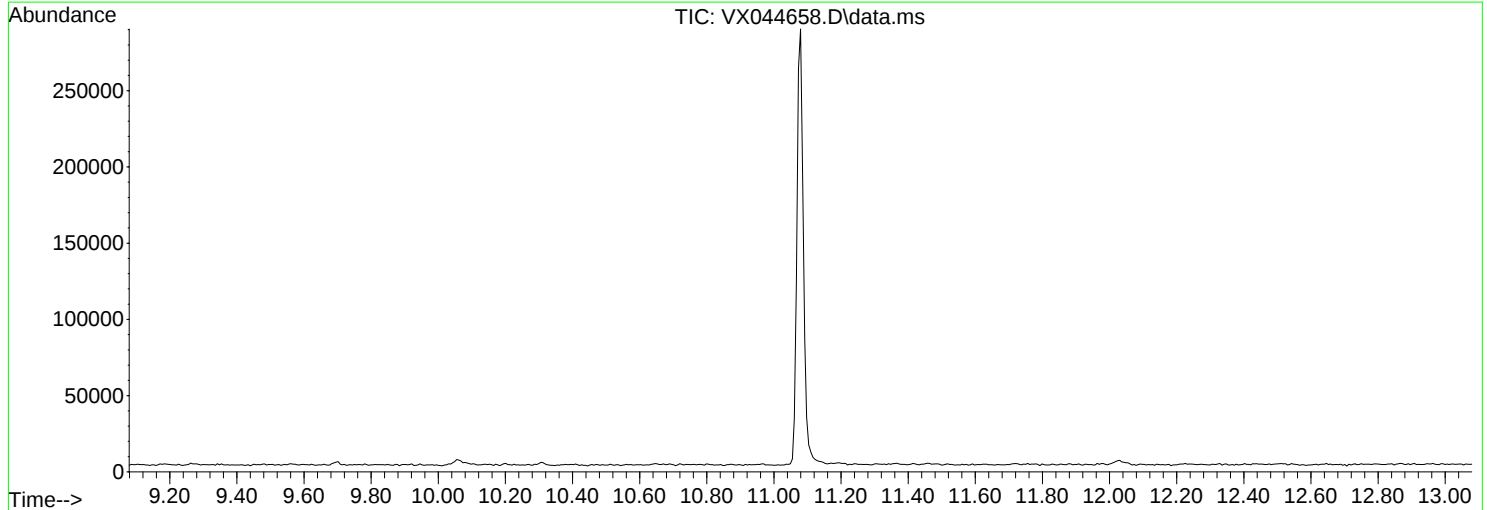

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	9723	PASS
75	95	30	60	47.9	26357	PASS
95	95	100	100	100.0	55021	PASS
96	95	5	9	6.6	3607	PASS
173	174	0.00	2	0.8	316	PASS
174	95	50	100	68.1	37445	PASS
175	174	5	9	7.1	2650	PASS
176	174	95	101	95.8	35883	PASS
177	176	5	9	6.6	2384	PASS