


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011025\
Data File : BF141108.D
Acq On : 10 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

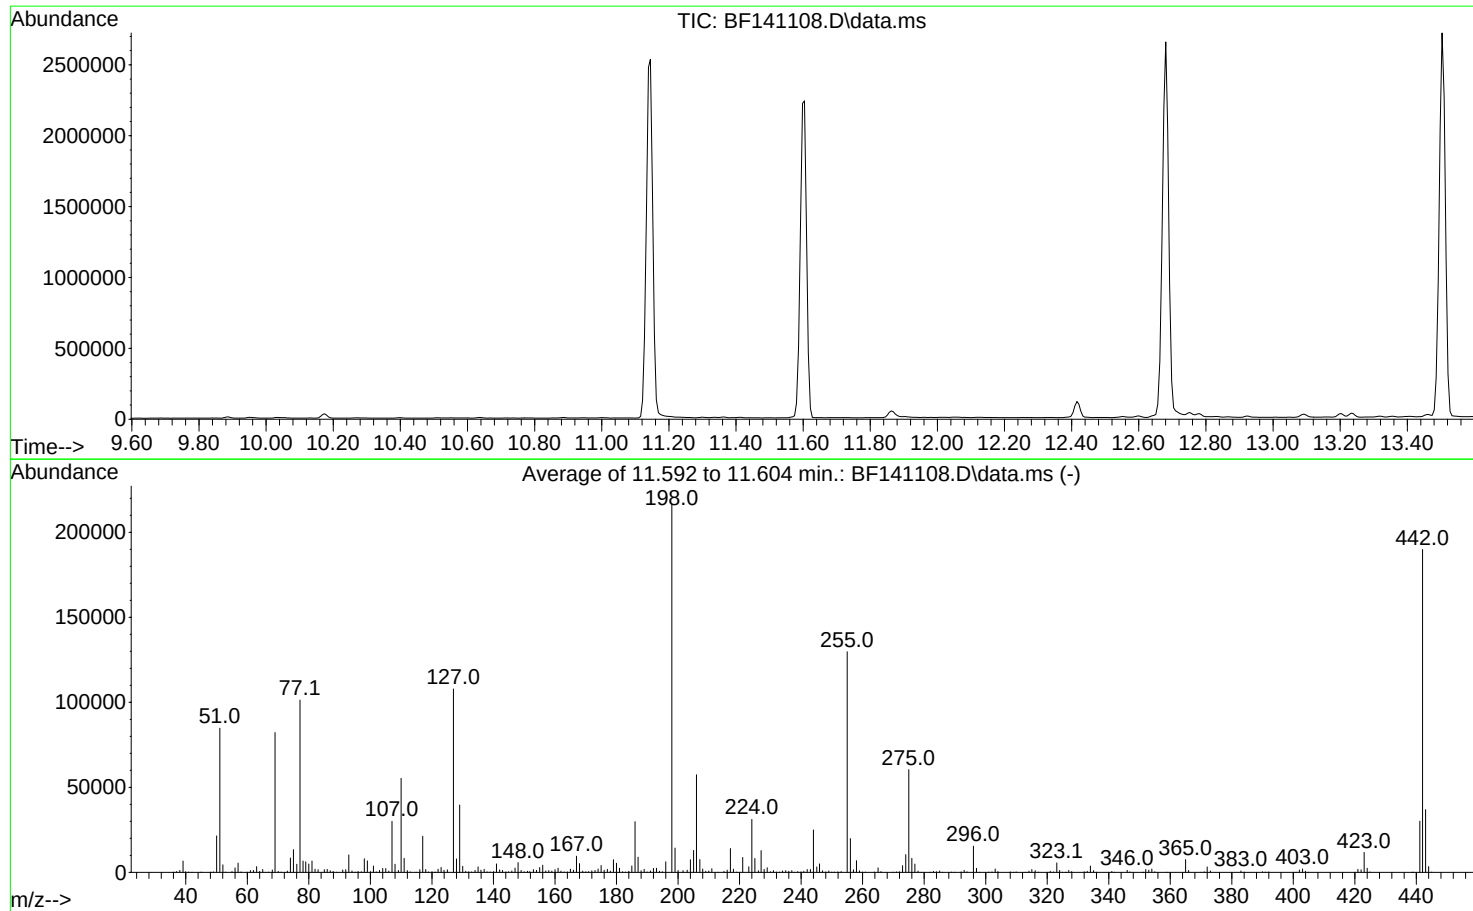

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	84750	PASS
68	69	0.00	2	1.8	1445	PASS
69	198	0.00	100	38.0	82278	PASS
70	69	0.00	2	0.7	551	PASS
127	198	10	80	49.8	107843	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	216341	PASS
199	198	5	9	6.6	14307	PASS
275	198	10	60	27.9	60421	PASS
365	198	1	100	3.5	7523	PASS
441	198	0.01	100	13.9	30123	PASS
442	442	50	100	100.0	189923	PASS
443	442	15	24	19.4	36936	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/10/2025	BNA_F	<u>BF141108.D</u>
Compound Name	Response	Retention Time
DDT	677363	13.504
DDD	13521	13.204
DDE	752	12.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14273	691636	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011025\
Data File : BF141108.D
Acq On : 10 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 12:08:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 12:07:52 2025
Response via : Initial Calibration

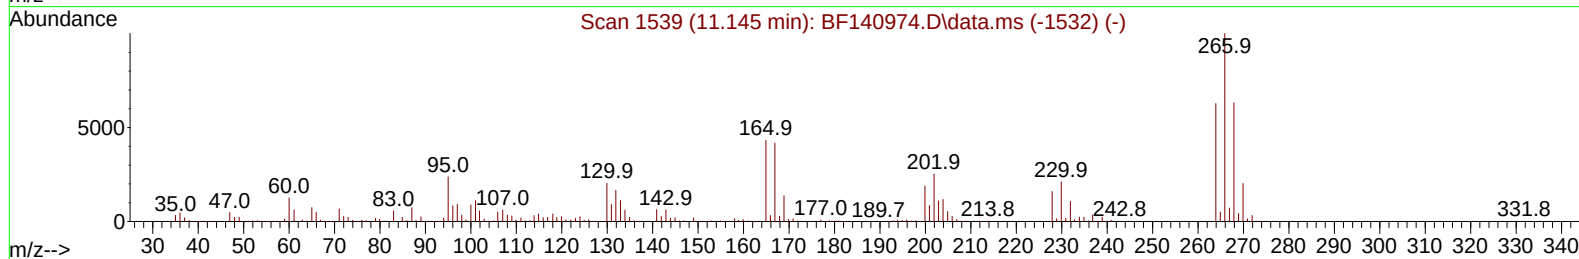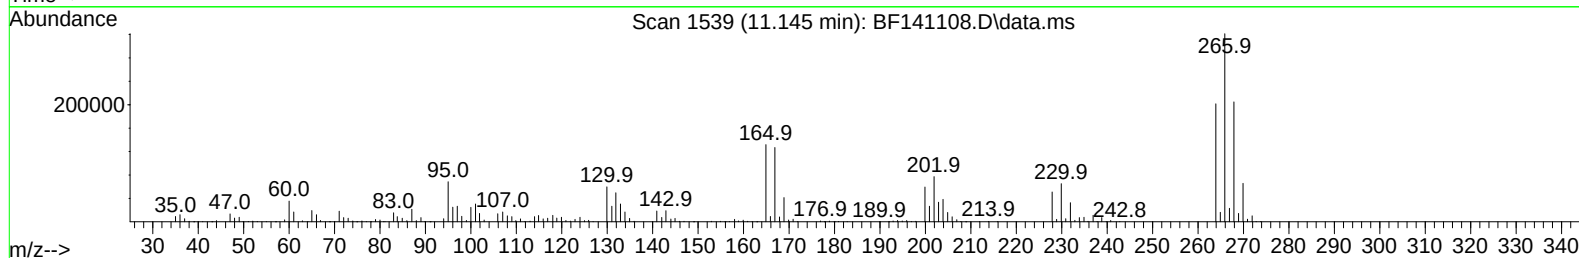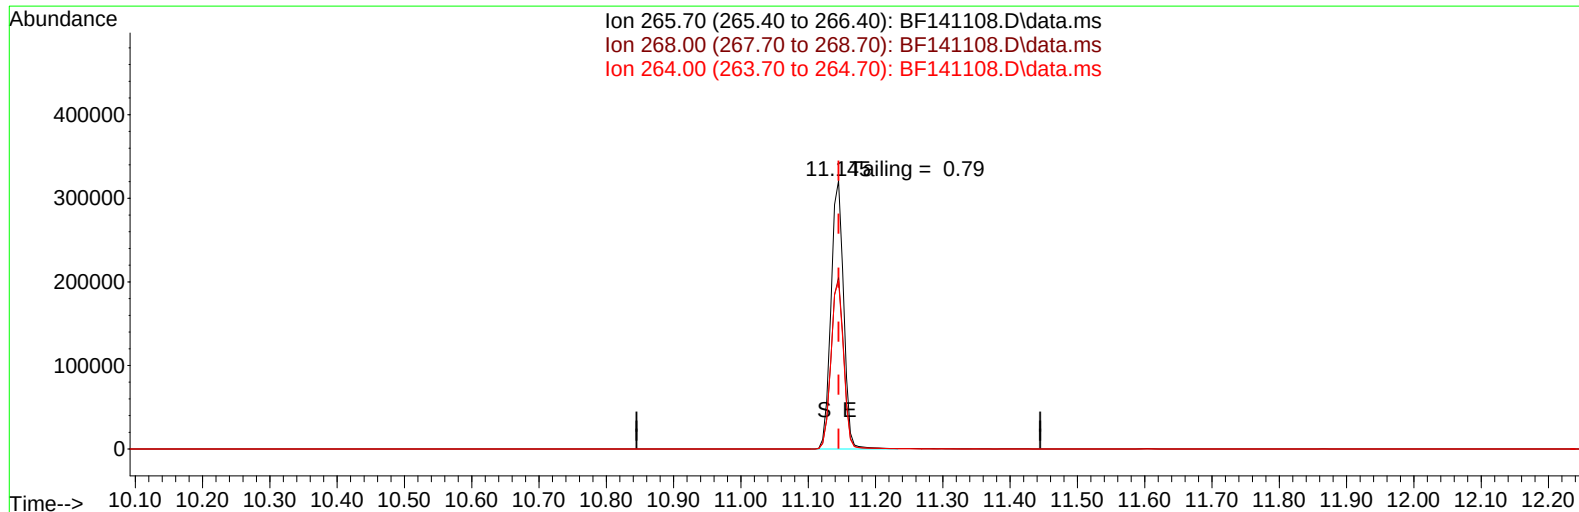

TIC: BF141108.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 27837.42 ng




response 420211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.79
264.00	62.80	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011025\
Data File : BF141108.D
Acq On : 10 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 12:08:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 12:07:52 2025
Response via : Initial Calibration

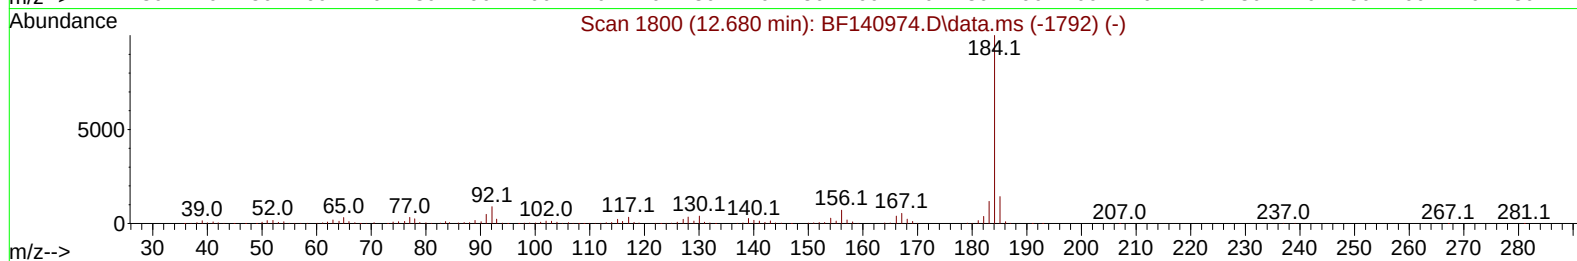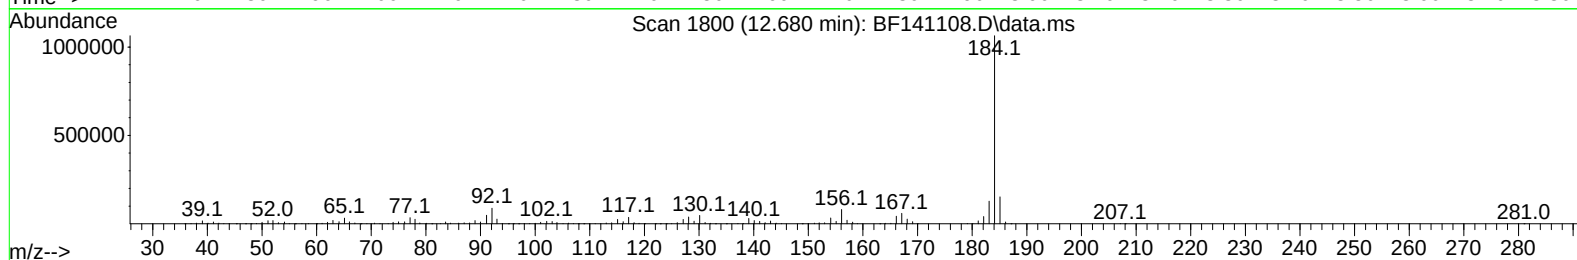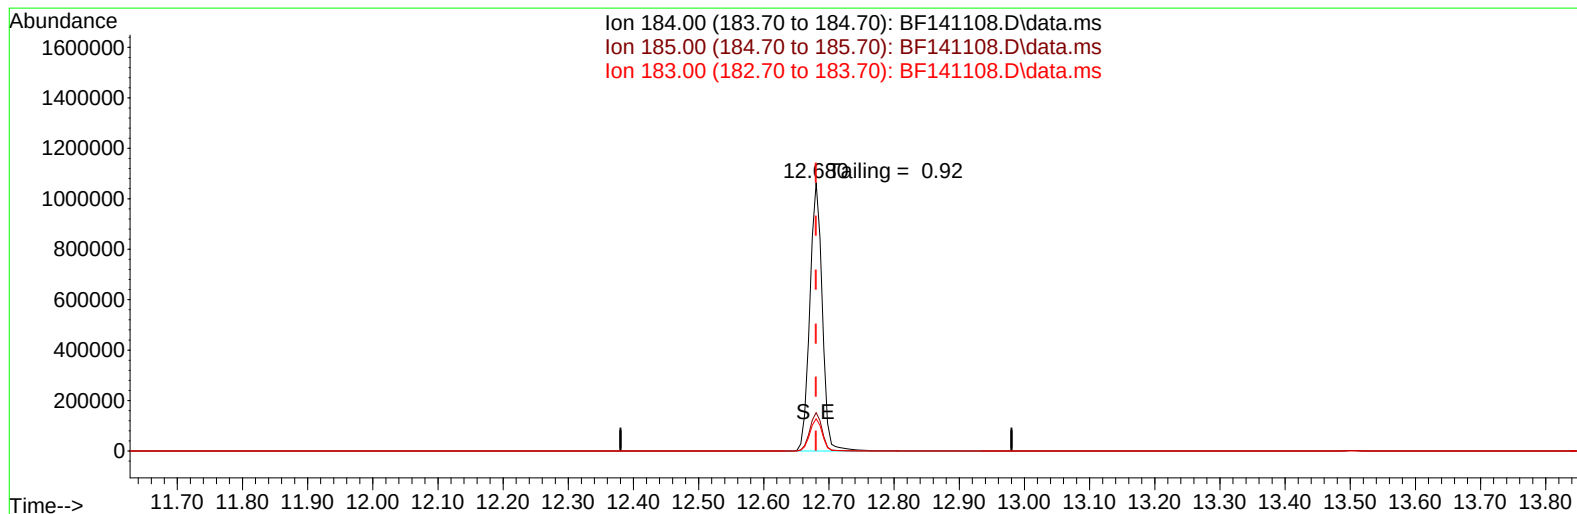

TIC: BF141108.D\data.ms

(77) Benzidine

12.680min (-0.000) 47053.75 ng

response 1415080

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.35
183.00	11.70	12.05
0.00	0.00	0.00