


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011725\
Data File : BF141192.D
Acq On : 17 Jan 2025 14:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

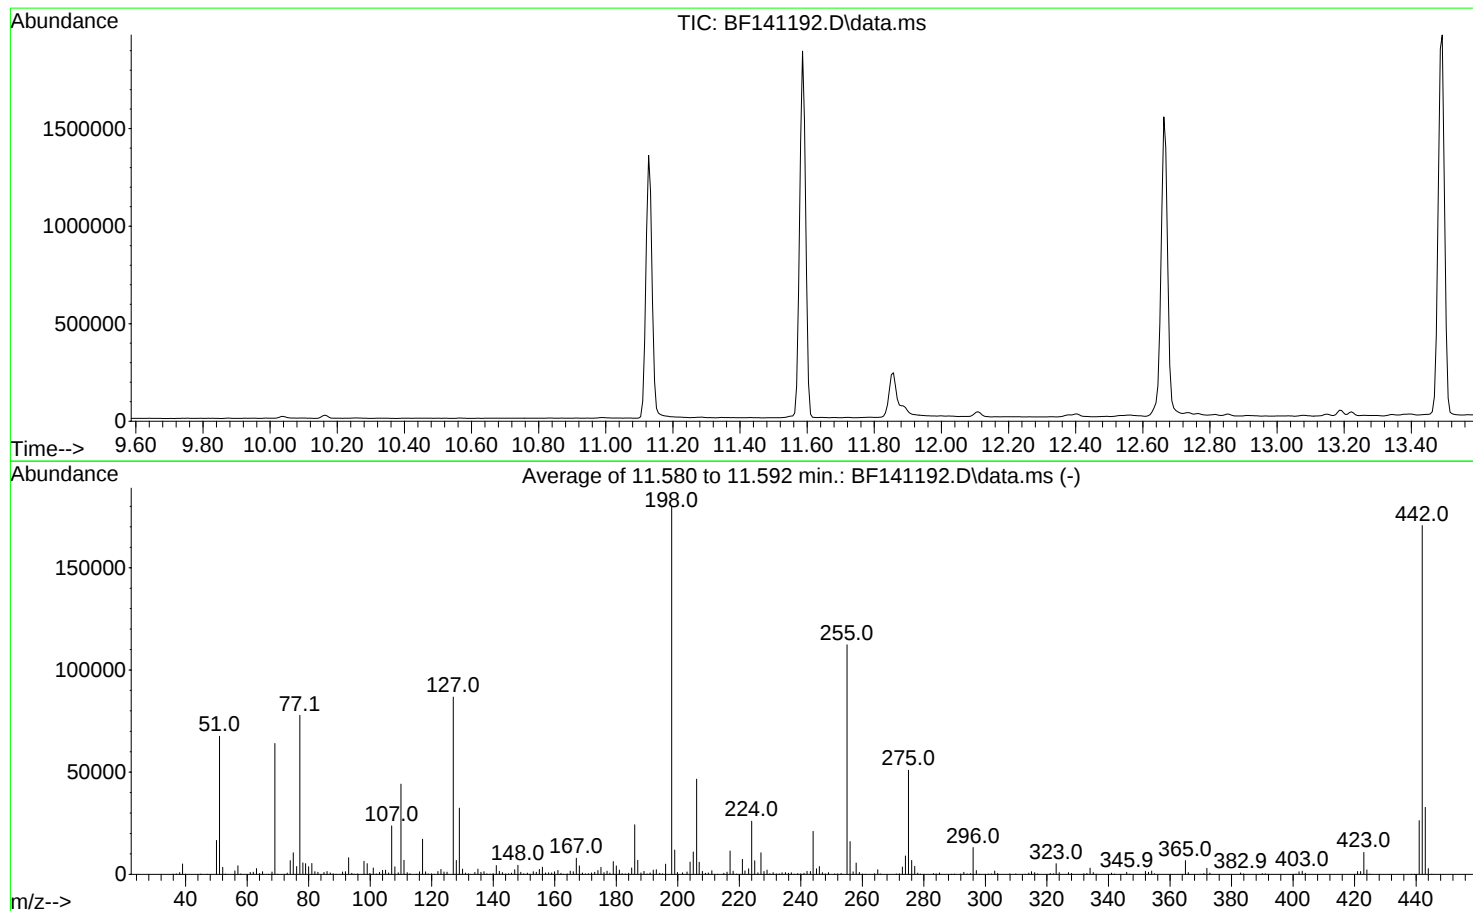

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	67540	PASS
68	69	0.00	2	1.8	1145	PASS
69	198	0.00	100	35.6	64039	PASS
70	69	0.00	2	0.1	63	PASS
127	198	10	80	48.2	86749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	179968	PASS
199	198	5	9	6.6	11915	PASS
275	198	10	60	28.3	50933	PASS
365	198	1	100	3.8	6771	PASS
441	198	0.01	100	14.6	26331	PASS
442	442	50	100	100.0	170675	PASS
443	442	15	24	19.2	32779	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/17/2025	BNA_F	<u>BF141192.D</u>
Compound Name	Response	Retention Time
DDT	489441	13.492
DDD	12774	13.192
DDE	1830	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14604	504045	2.90

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011725\
Data File : BF141192.D
Acq On : 17 Jan 2025 14:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 15:59:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

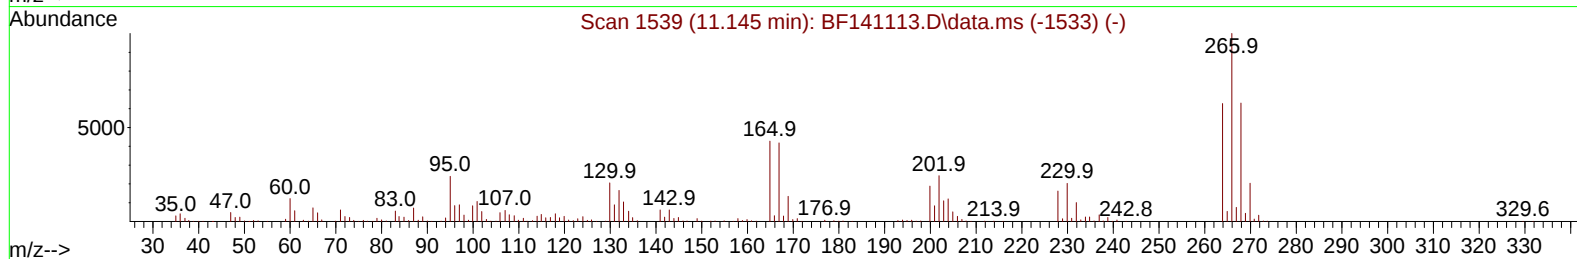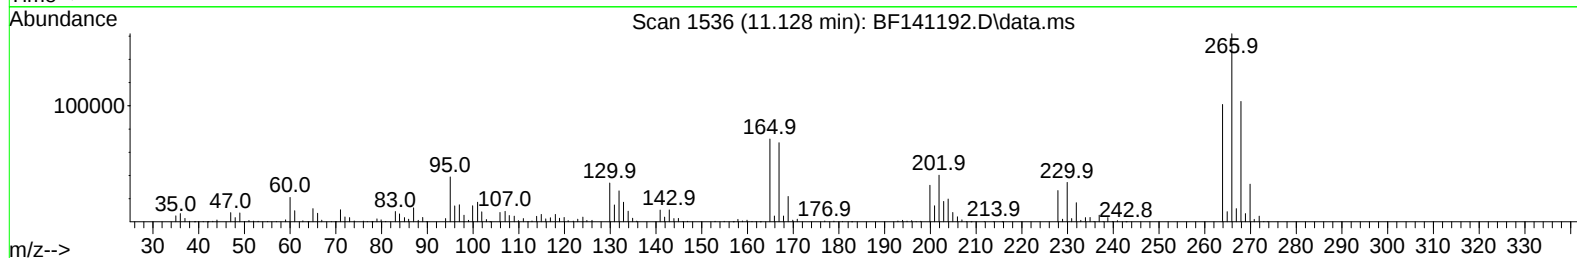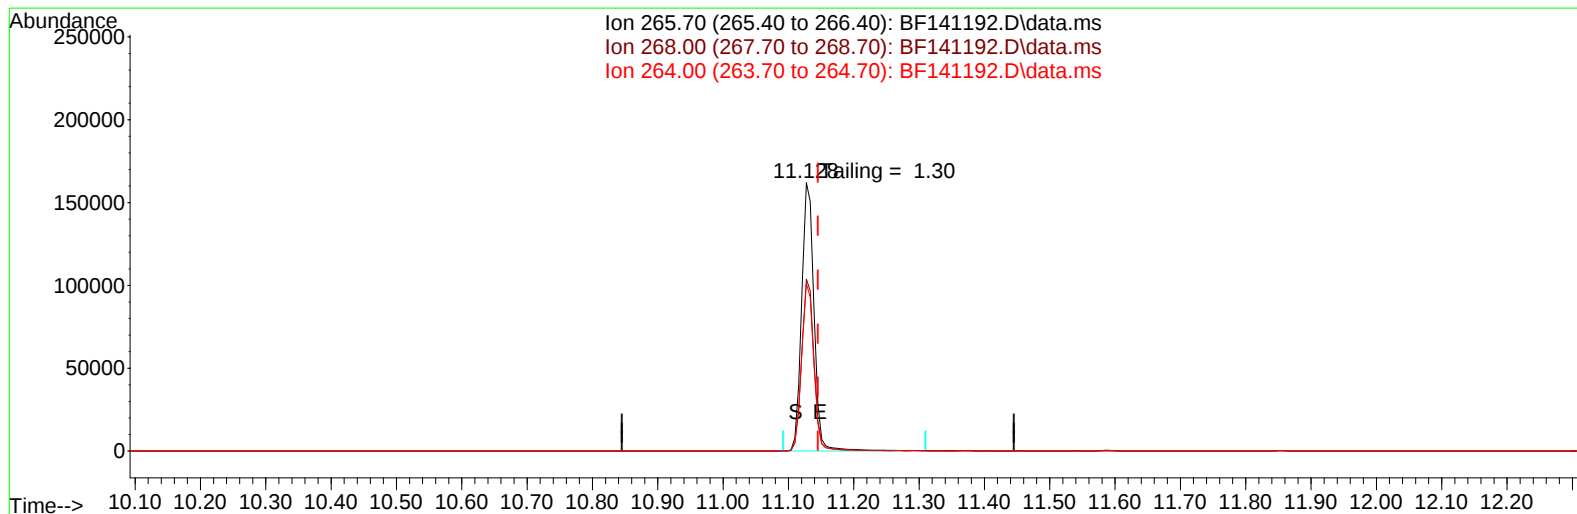

TIC: BF141192.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.018) 63009.31 ng




response 214616

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.07
264.00	62.70	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011725\
Data File : BF141192.D
Acq On : 17 Jan 2025 14:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 15:59:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

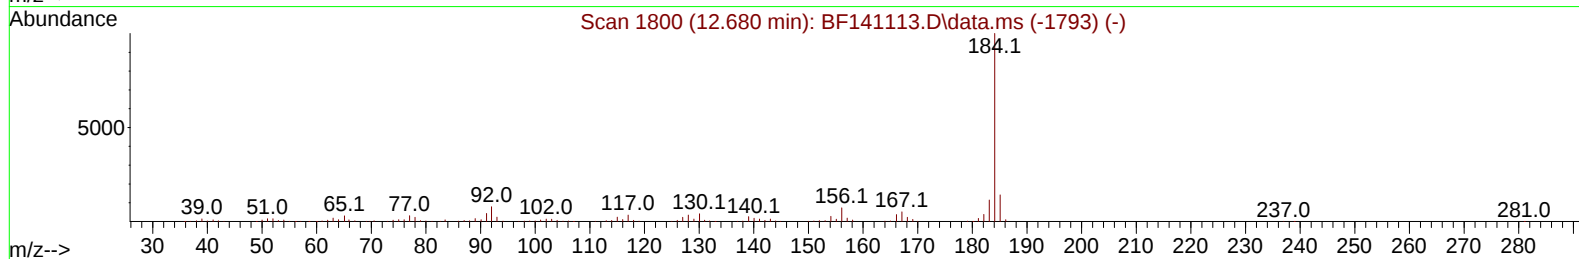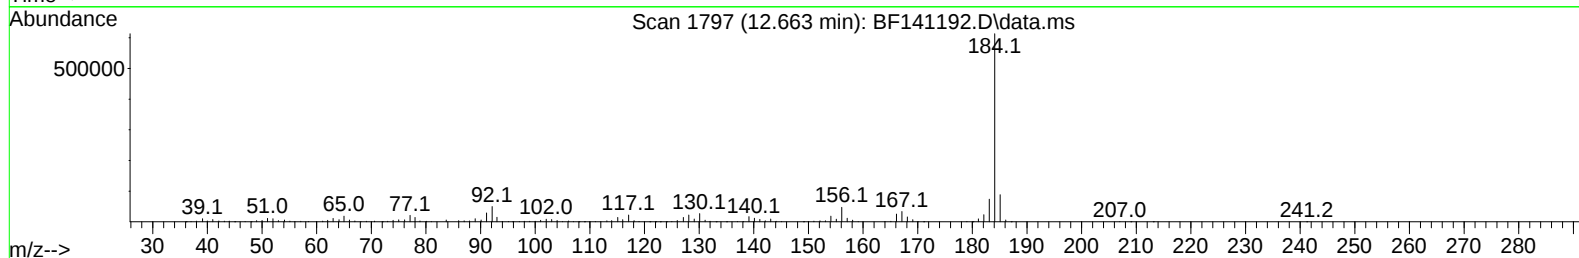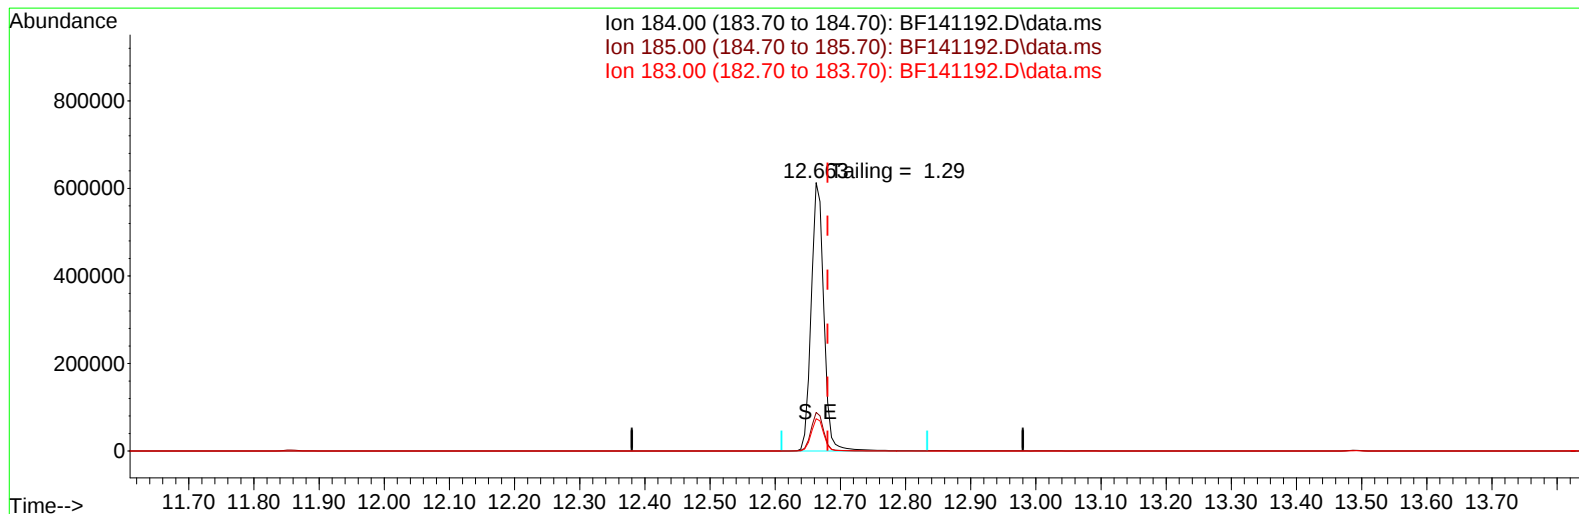

TIC: BF141192.D\data.ms

(77) Benzidine

12.663min (-0.018) 84932.11 ng

response 826882

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.40
183.00	11.50	12.05
0.00	0.00	0.00