


Ident	Instrument IC-1			Analyst :	NF	Method:	300.0 / 9056A		Initial wt/Fil
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name date time	
STD1	0	0	0	0	0	0	0	IC1-121824	12/18/2024 10:39
STD2	0.319	0.475	0.485	1.586	0.405	0.794	2.525	IC1-121824	12/18/2024 11:00
STD3	0.867	1.29	1.286	4.307	1.073	2.153	6.454	IC1-121824	12/18/2024 11:22
STD4	1.065	1.59	1.587	5.29	1.327	2.68	7.947	IC1-121824	12/18/2024 11:43
STD5	1.968	2.98	2.975	9.935	2.472	4.928	14.761	IC1-121824	12/18/2024 12:04
STD6	3.929	5.897	5.891	19.654	4.906	9.805	29.16	IC1-121824	12/18/2024 12:26
STD7	5.052	7.568	7.575	25.229	6.317	12.641	37.652	IC1-121824	12/18/2024 12:47
ICV	2.021	3.088	3.087	10.28	2.565	5.117	15.271	IC1-121824	12/18/2024 13:09
ICB	0	0	0	0	0	0	0	IC1-121824	12/18/2024 13:30
CCV	2.077	3.111	3.113	10.419	2.587	5.226	15.523	IC1-121824	1/17/2025 8:43
CCB	0	0	0	0	0	0	0	IC1-121824	1/17/2025 9:04
LB134320BLW	0	0	0	0	0	0	0	IC1-121824	1/17/2025 9:26
LB134320BSW	2.073	3.111	3.12	10.432	2.585	5.433	15.544	IC1-121824	1/17/2025 9:47
Q1120-01	0.148	128.178	0	0.693	0.194	0	29.758	IC1-121824	1/17/2025 10:09
Q1120-01MS	2.113	126.6	3.027	10.219	2.555	5.561	43.215	IC1-121824	1/17/2025 10:30
Q1120-01MSD	2.086	126.747	3.039	10.236	2.558	5.53	43.352	IC1-121824	1/17/2025 10:52
Q1120-01DLX50	0	2.002	0	0	0	0	1.708	IC1-121824	1/17/2025 11:13
CCV	2.108	3.115	3.123	10.457	2.597	5.441	15.572	IC1-121824	1/17/2025 11:35
CCB	0	0	0	0	0	0	0	IC1-121824	1/17/2025 11:56

Clear table

Instrument ID: IC-2									
Analyst : IZ				Method: 300.0 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0	0	0	0	0	0	0	0 IC1-121824	10 NF/IZ
STD2	0.319	0.475	0.485	1.586	0.405	0.794	2.525	IC1-121824	10 NF/IZ
STD3	0.867	1.29	1.286	4.307	1.073	2.153	6.454	IC1-121824	10 NF/IZ
STD4	1.065	1.59	1.587	5.29	1.327	2.68	7.947	IC1-121824	10 NF/IZ
STD5	1.968	2.98	2.975	9.935	2.472	4.928	14.761	IC1-121824	10 NF/IZ
STD6	3.929	5.897	5.891	19.654	4.906	9.805	29.16	IC1-121824	10 NF/IZ
STD7	5.052	7.568	7.575	25.229	6.317	12.641	37.652	IC1-121824	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1	-20.2500	-20.8333	-19.1667	-20.7000	-19.0000	-20.6000	-15.8333		
STD2	8.3750	7.5000	7.1667	7.6750	7.3000	7.6500	7.5667		
STD3	6.5000	6.0000	5.8000	5.8000	6.1600	7.2000	5.9600		
STD4	-1.6000	-0.6667	-0.8333	-0.6500	-1.1200	-1.4400	-1.5933		
STD5	-1.7750	-1.7167	-1.8167	-1.7300	-1.8800	-1.9500	-2.8000		
STD6	1.0400	0.9067	1.0000	0.9160	1.0720	1.1280	1.7622		

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

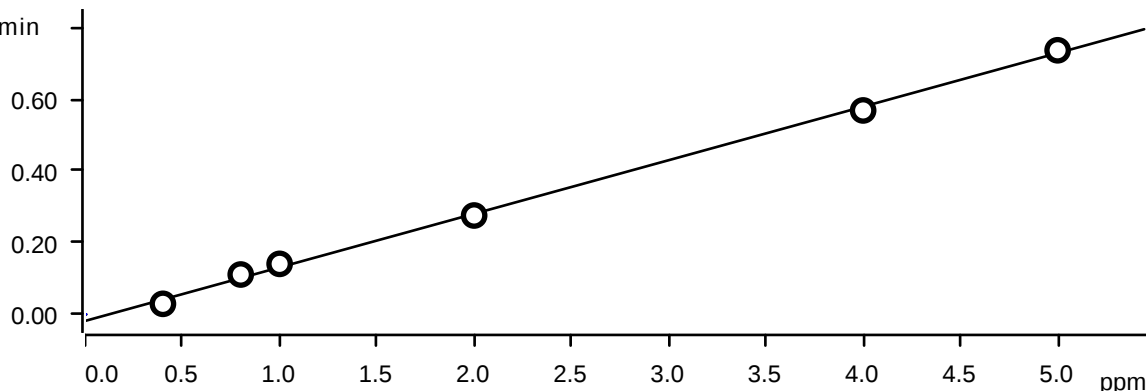

Function: $A = -0.0183596 + 0.0149351 \times Q$


Relative standard deviation 3.731557 %

Correlation coefficient 0.999324

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.400	10.0	1.0	1.0	0.029	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.276	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.568	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.736	STD7	2024-12-18 12:47:45 UTC-5	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

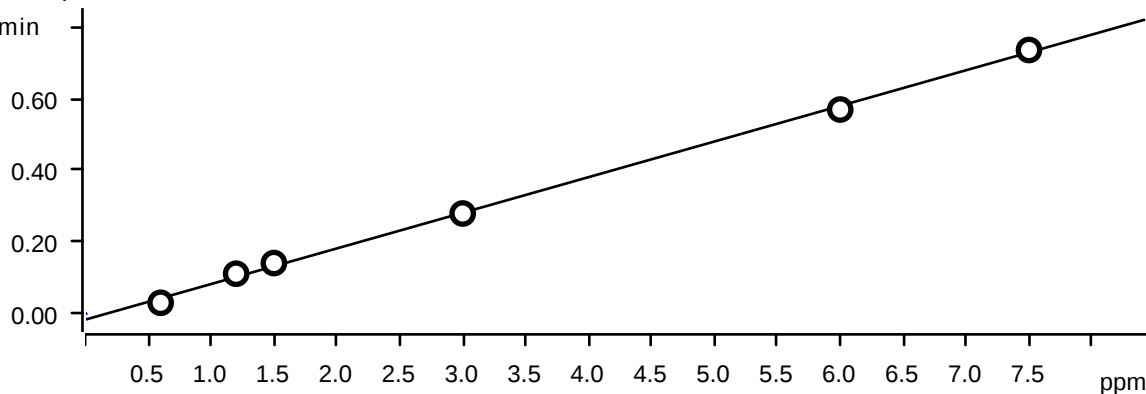


Function: $A = -0.0165562 + 9.93613E-3 \times Q$

Relative standard deviation 3.466087 %

Correlation coefficient 0.999410


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.031	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.569	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.735	STD7	2024-12-18 12:47:45 UTC-5	used

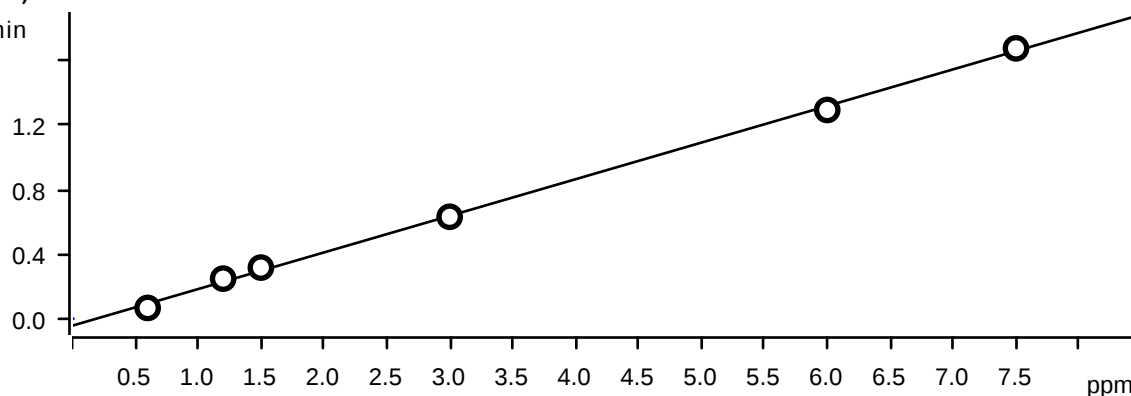Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0434679 + 0.0226901 \times Q$

Relative standard deviation 3.455351 %

Correlation coefficient 0.999423


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.067	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.317	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.632	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.293	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.675	STD7	2024-12-18 12:47:45 UTC-5	used

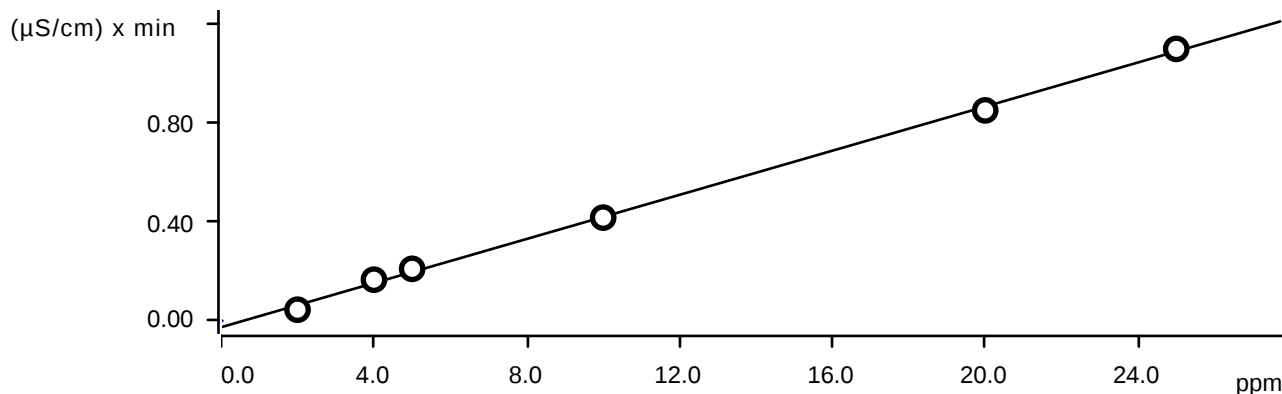Bromide (Anions)Function: $A = -0.0255661 + 4.44233E-3 \times Q$

Relative standard deviation 3.478545 %

Correlation coefficient 0.999408

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	2.000	10.0	1.0	1.0	0.045	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.166	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.416	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.848	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.095	STD7	2024-12-18 12:47:45 UTC-5	used

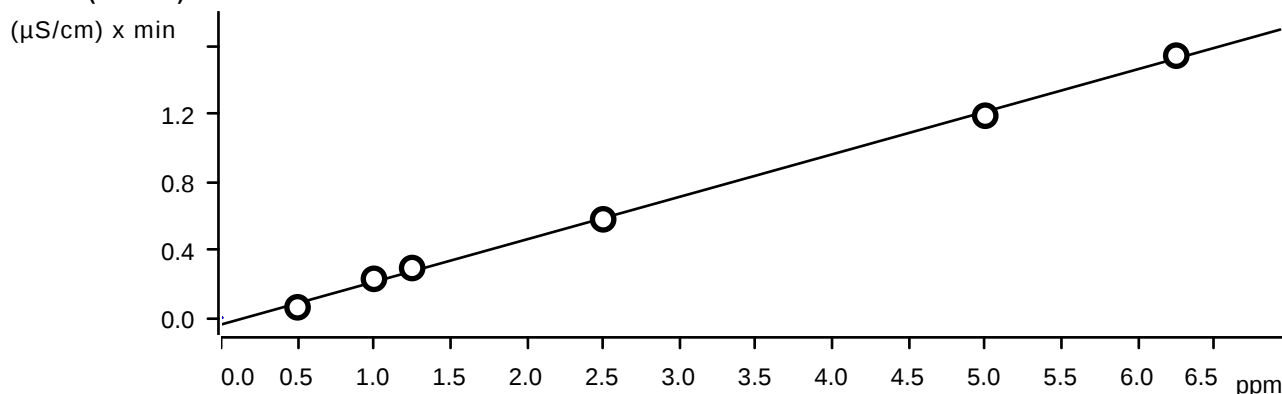
Nitrate (Anions)Function: $A = -0.0400484 + 0.0250507 \times Q$

Relative standard deviation 3.586984 %

Correlation coefficient 0.999378

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.500	10.0	1.0	1.0	0.061	STD2	2024-12-18 11:00:37 UTC-5	used

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.292	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.189	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.542	STD7	2024-12-18 12:47:45 UTC-5	used

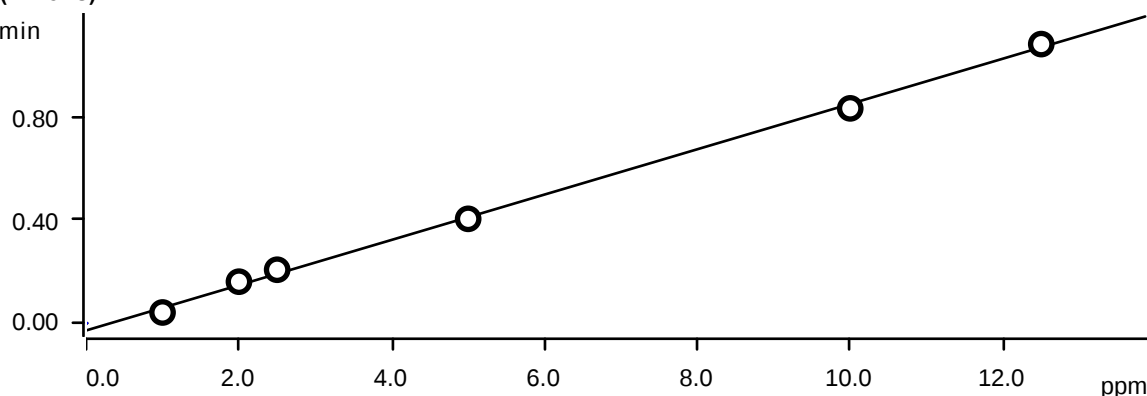
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0282076 + 8.77175E-3 \times Q$

Relative standard deviation 3.880200 %

Correlation coefficient 0.999273

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	1.000	10.0	1.0	1.0	0.041	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.207	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.404	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.832	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.081	STD7	2024-12-18 12:47:45 UTC-5	used

Sulfate (Anions)

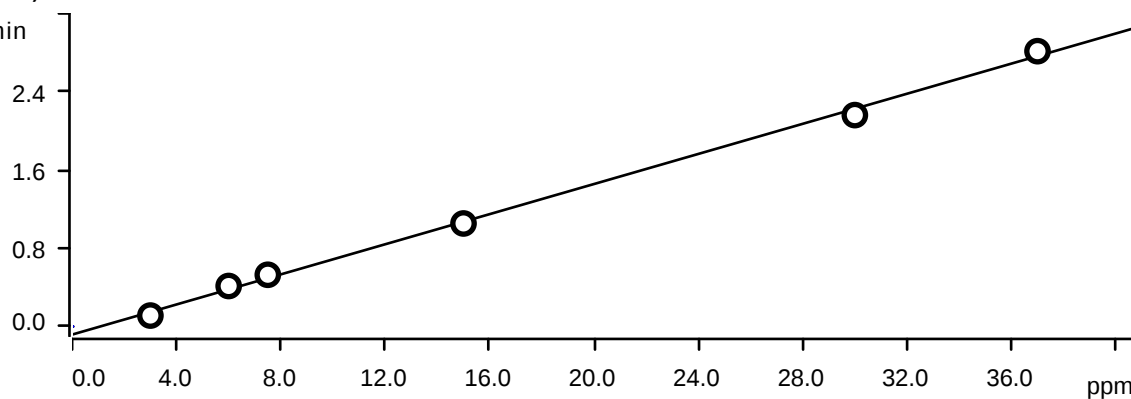 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0827937 + 7.69466E-3 \times Q$

Relative standard deviation 4.394299 %

Correlation coefficient 0.999072

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	3.000	10.0	1.0	1.0	0.112	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.414	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.529	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.053	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.161	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.814	STD7	2024-12-18 12:47:45 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-12-18 10:39:14 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

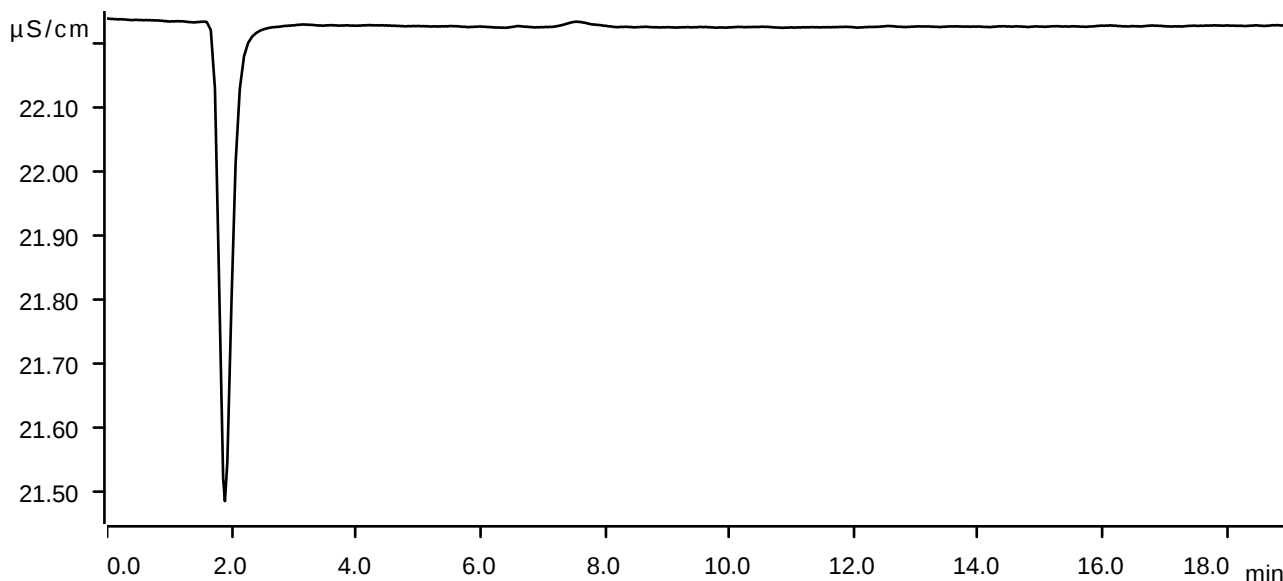


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-12-18 11:00:37 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

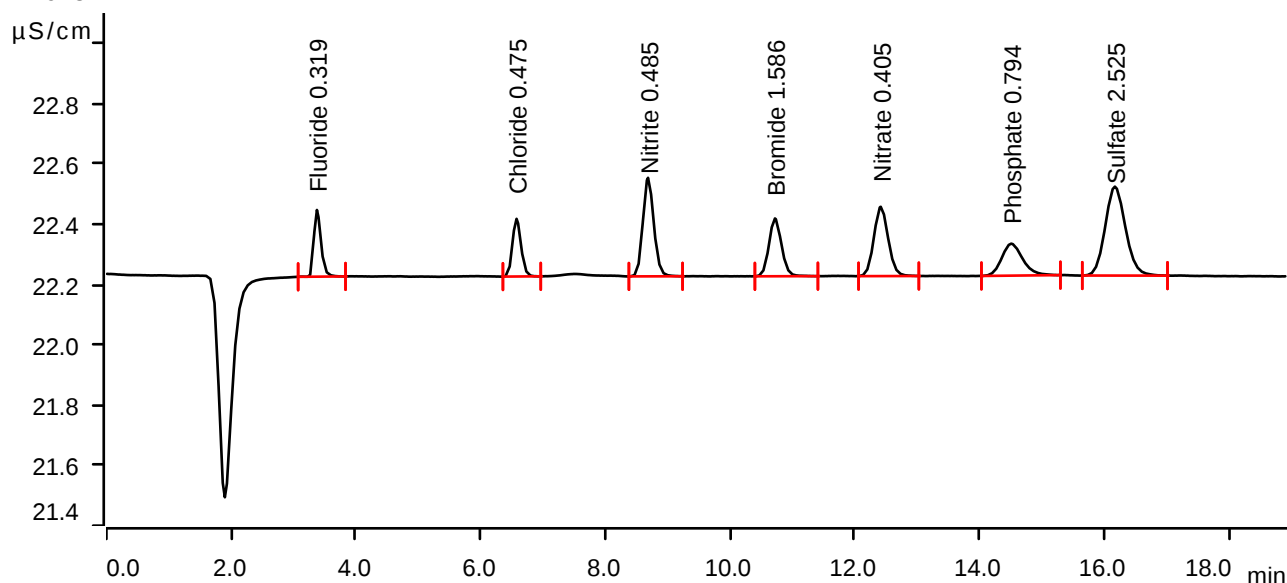

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.0293	0.221	0.319	Fluoride
2	6.577	0.0307	0.191	0.475	Chloride
3	8.685	0.0666	0.327	0.485	Nitrite
4	10.720	0.0449	0.192	1.586	Bromide
5	12.415	0.0613	0.230	0.405	Nitrate
6	14.510	0.0414	0.106	0.794	Phosphate
7	16.170	0.1115	0.295	2.525	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-12-18 11:22:01 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

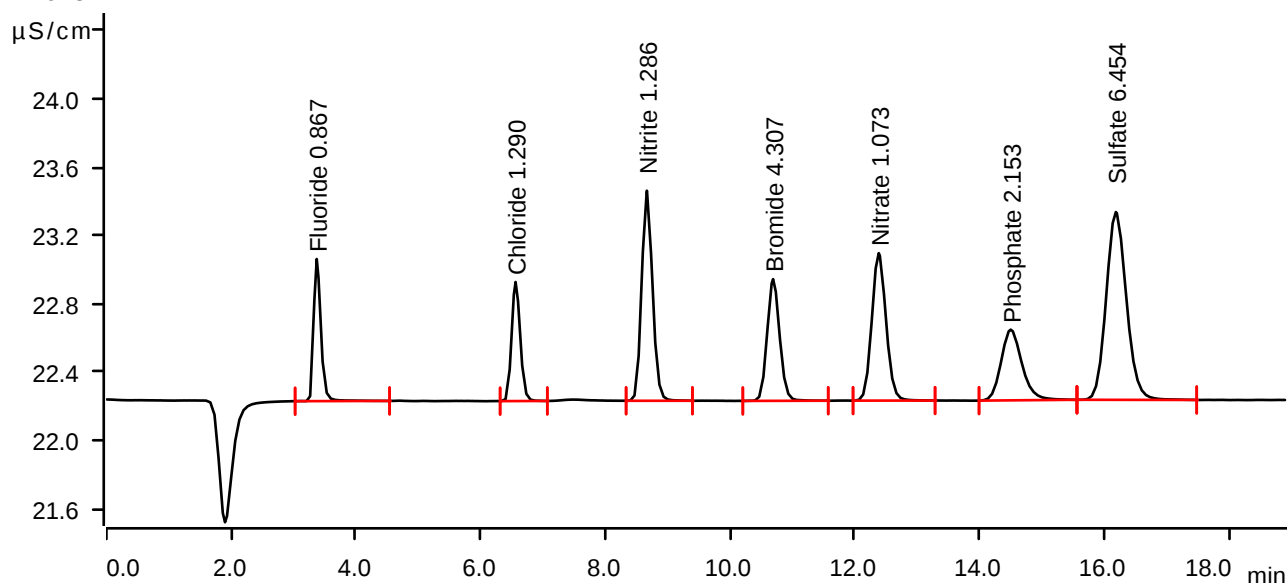

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.1111	0.832	0.867	Fluoride
2	6.562	0.1116	0.697	1.290	Chloride
3	8.665	0.2483	1.230	1.286	Nitrite
4	10.690	0.1658	0.713	4.307	Bromide
5	12.383	0.2288	0.864	1.073	Nitrate
6	14.500	0.1606	0.414	2.153	Phosphate
7	16.185	0.4138	1.100	6.454	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-12-18 11:43:26 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

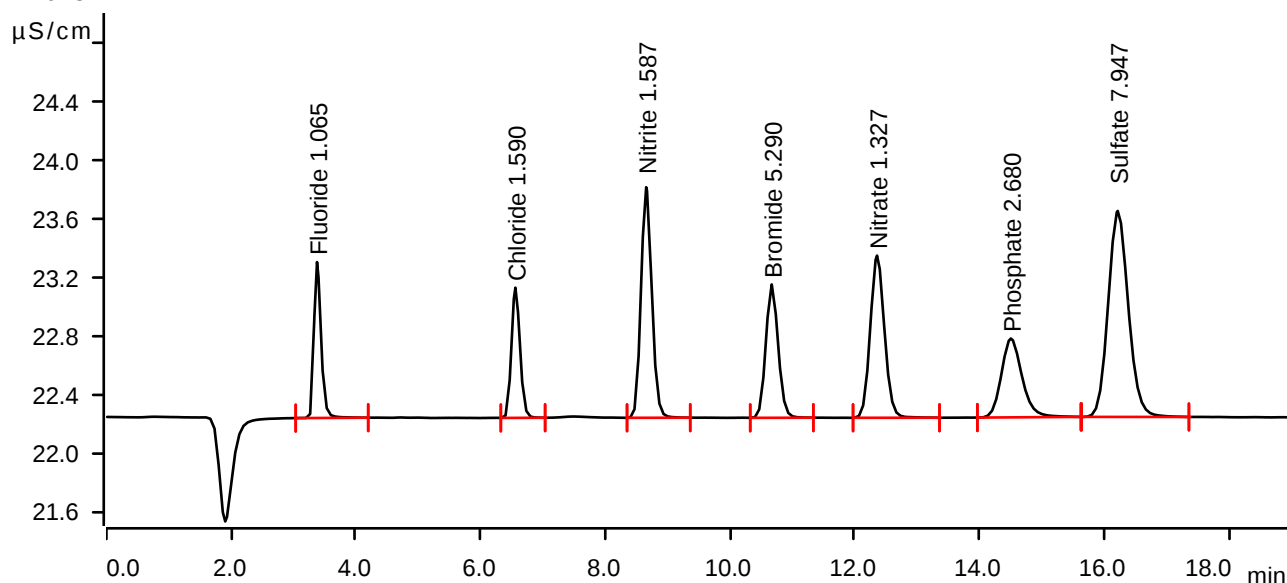

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.1407	1.065	1.065	Fluoride
2	6.558	0.1414	0.890	1.590	Chloride
3	8.655	0.3167	1.575	1.587	Nitrite
4	10.668	0.2094	0.911	5.290	Bromide
5	12.357	0.2924	1.108	1.327	Nitrate
6	14.502	0.2069	0.539	2.680	Phosphate
7	16.215	0.5287	1.408	7.947	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-12-18 12:04:52 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

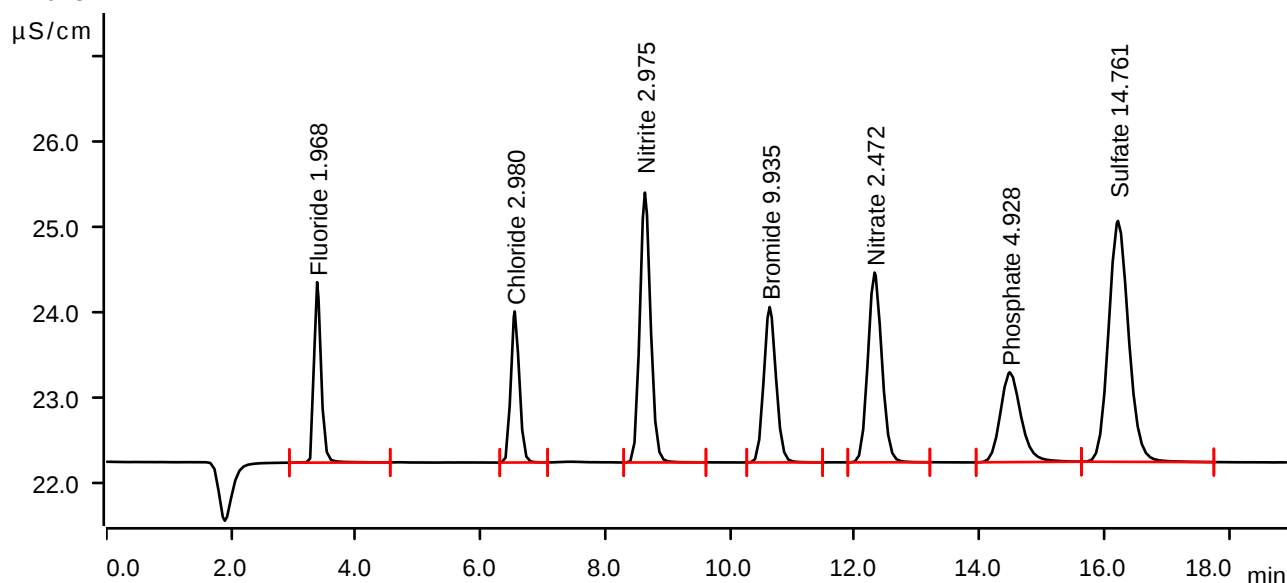

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.380	0.2755	2.114	1.968	Fluoride
2	6.548	0.2796	1.770	2.980	Chloride
3	8.635	0.6316	3.161	2.975	Nitrite
4	10.635	0.4158	1.820	9.935	Bromide
5	12.317	0.5791	2.223	2.472	Nitrate
6	14.485	0.4040	1.052	4.928	Phosphate
7	16.220	1.0530	2.822	14.761	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-12-18 12:26:18 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

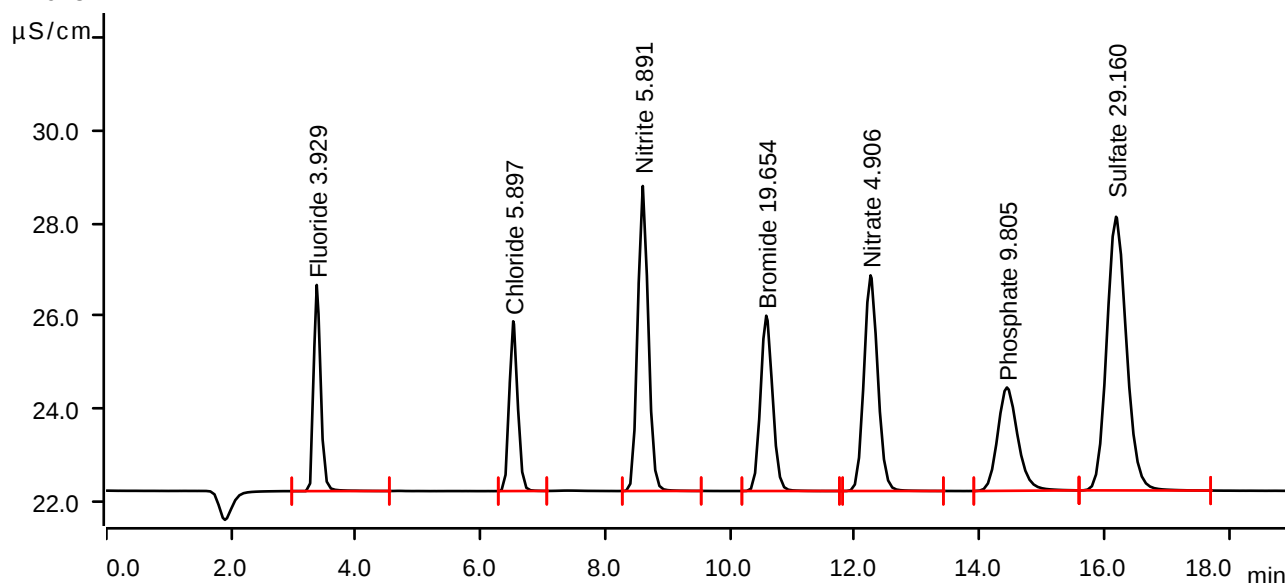

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.5685	4.427	3.929	Fluoride
2	6.523	0.5694	3.646	5.897	Chloride
3	8.602	1.2933	6.549	5.891	Nitrite
4	10.580	0.8475	3.765	19.654	Bromide
5	12.252	1.1889	4.631	4.906	Nitrate
6	14.438	0.8318	2.220	9.805	Phosphate
7	16.188	2.1610	5.877	29.160	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-12-18 12:47:45 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.75 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

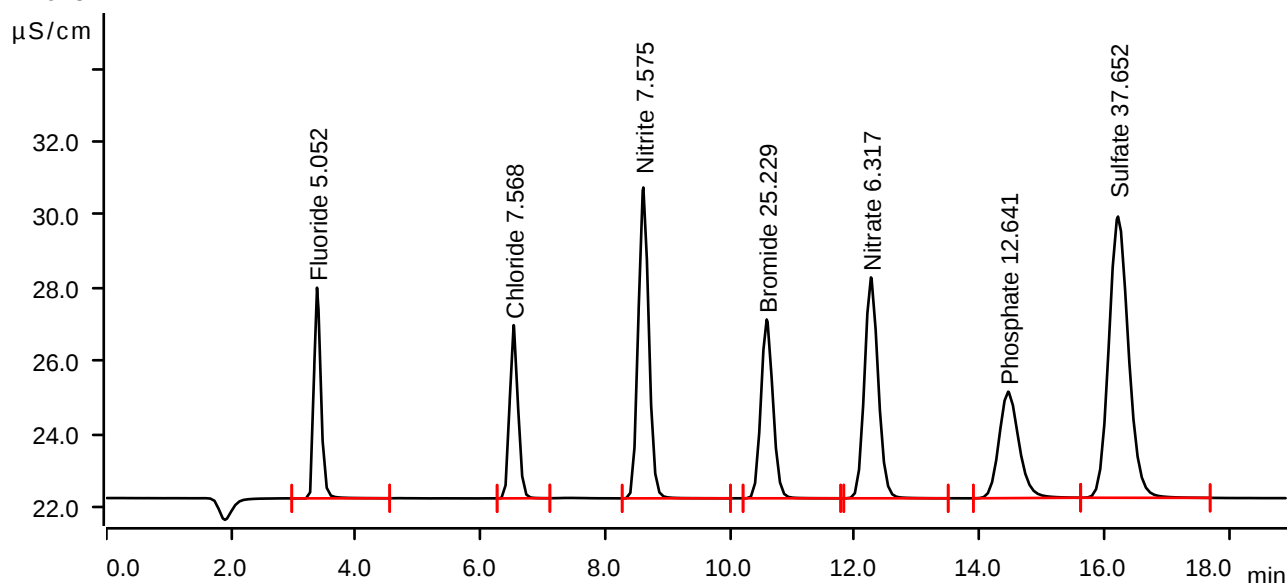

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.7362	5.758	5.052	Fluoride
2	6.530	0.7354	4.734	7.568	Chloride
3	8.610	1.6752	8.496	7.575	Nitrite
4	10.587	1.0952	4.888	25.229	Bromide
5	12.258	1.5424	6.037	6.317	Nitrate
6	14.458	1.0806	2.908	12.641	Phosphate
7	16.220	2.8144	7.686	37.652	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-12-18 13:09:13 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

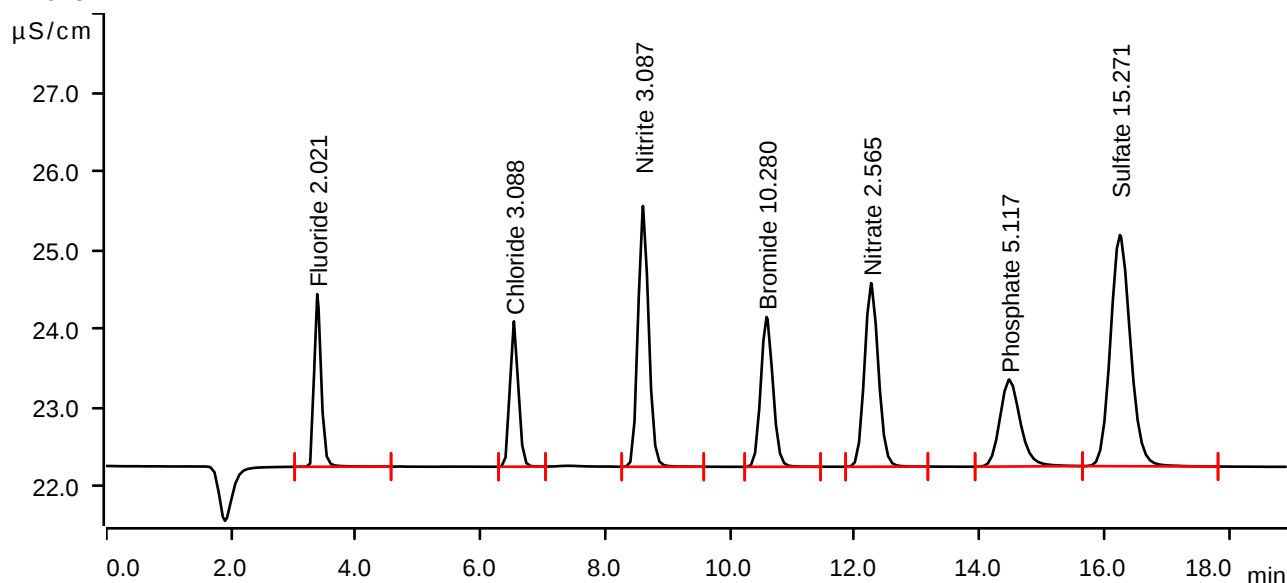


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.382	0.2835	2.190	2.021	Fluoride
2	6.533	0.2903	1.845	3.088	Chloride
3	8.605	0.6571	3.309	3.087	Nitrite
4	10.585	0.4311	1.902	10.280	Bromide
5	12.262	0.6024	2.329	2.565	Nitrate
6	14.477	0.4207	1.104	5.117	Phosphate
7	16.250	1.0923	2.934	15.271	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-12-18 13:30:41 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.64 MPa
Maximum pressure monitored yes
Temperature ---- °C

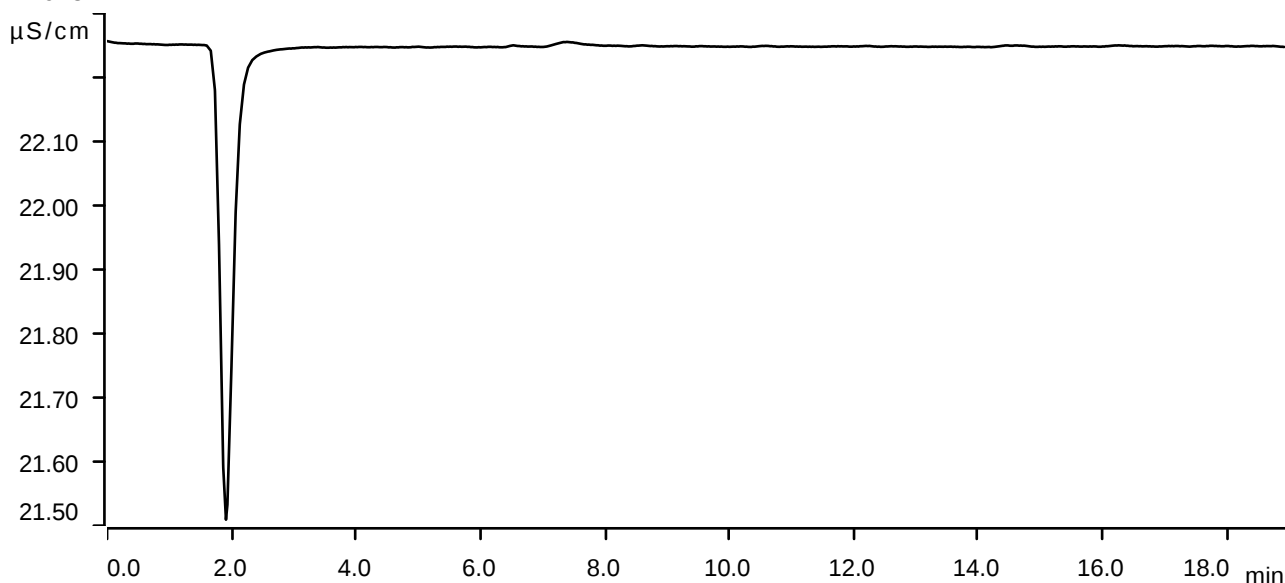Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-17 08:43:10 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

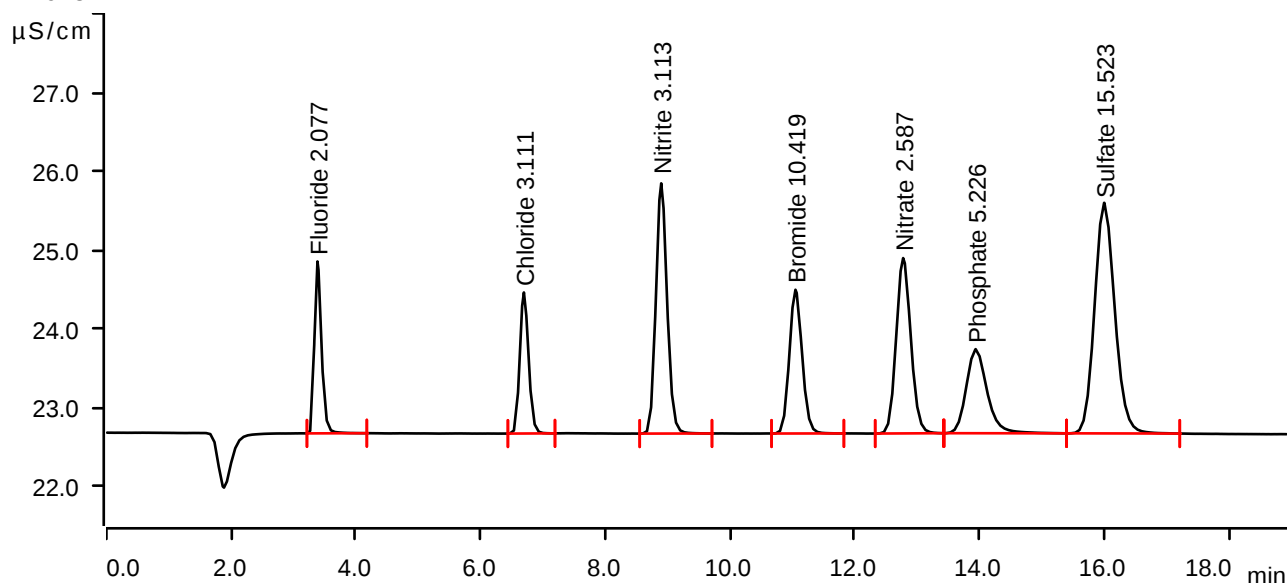

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.385	0.2869	2.181	2.077	Fluoride
2	6.695	0.2916	1.790	3.111	Chloride
3	8.897	0.6593	3.175	3.113	Nitrite
4	11.048	0.4339	1.824	10.419	Bromide
5	12.775	0.6034	2.225	2.587	Nitrate
6	13.938	0.4123	1.067	5.226	Phosphate
7	15.997	1.0999	2.926	15.523	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-17 09:04:40 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

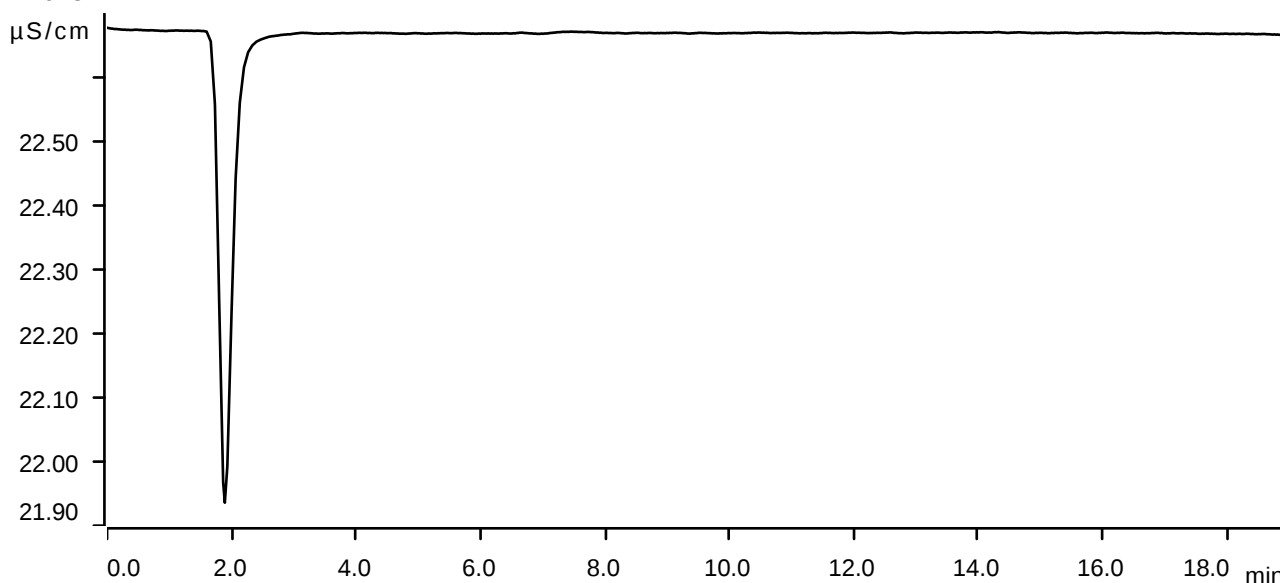


Sample data

Ident LB134320BLW
Sample type Sample
Determination start 2025-01-17 09:26:10 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

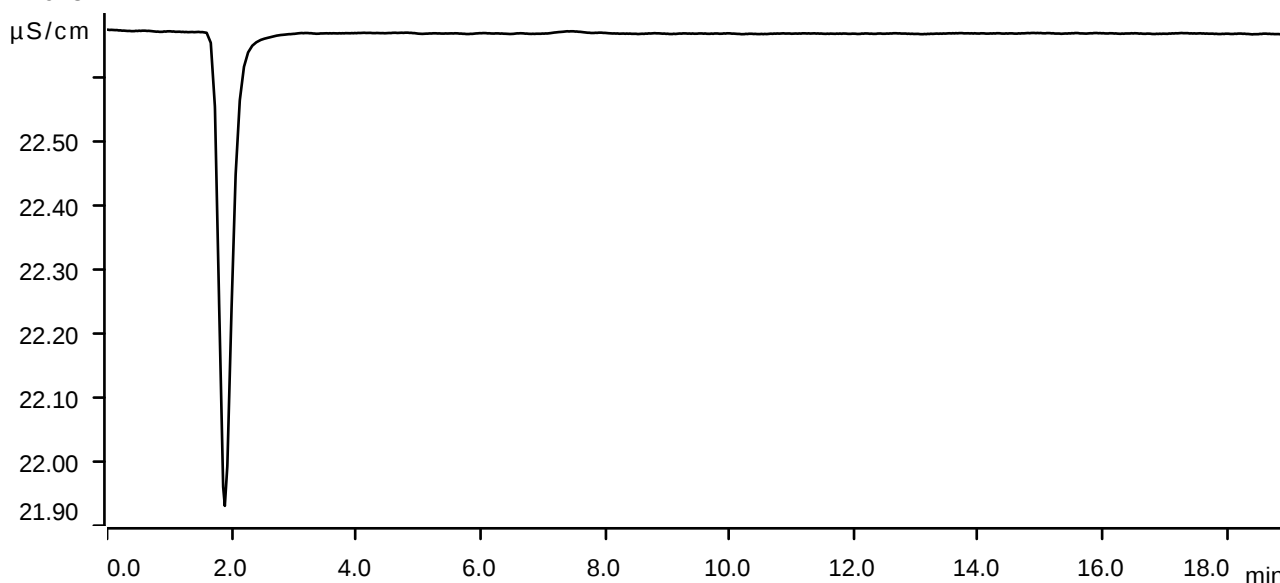


Sample data

Ident LB134320BSW
Sample type Sample
Determination start 2025-01-17 09:47:41 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

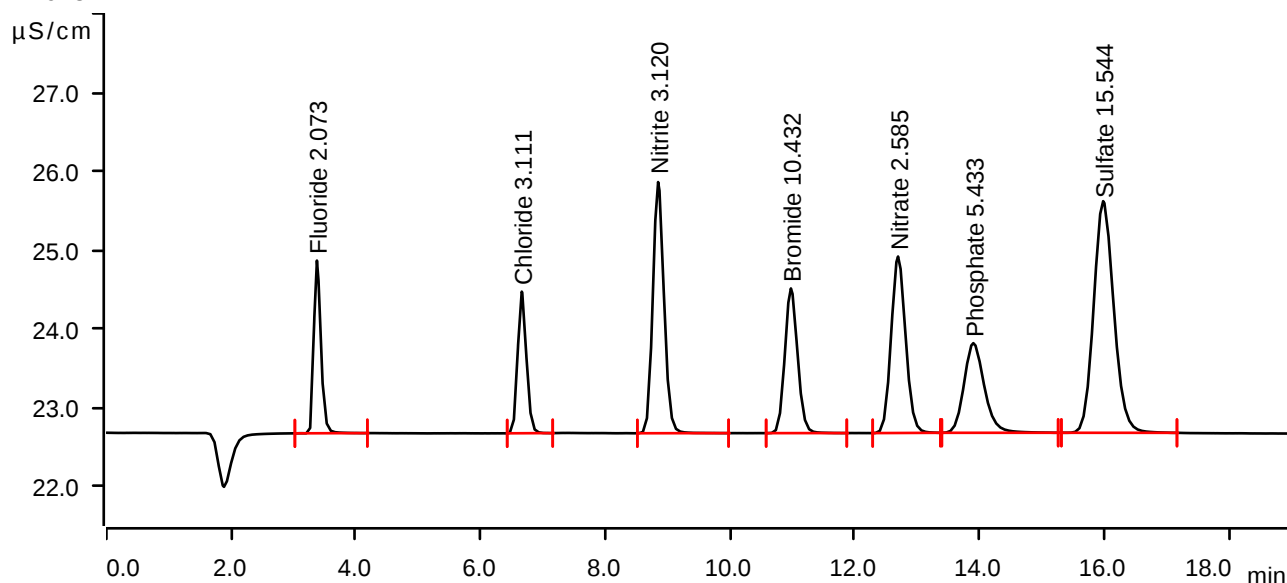

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.2863	2.191	2.073	Fluoride
2	6.660	0.2916	1.797	3.111	Chloride
3	8.847	0.6608	3.187	3.120	Nitrite
4	10.975	0.4344	1.836	10.432	Bromide
5	12.693	0.6029	2.240	2.585	Nitrate
6	13.900	0.4304	1.138	5.433	Phosphate
7	15.982	1.1015	2.939	15.544	Sulfate


Sample data

Ident Q1120-01
Sample type Sample
Determination start 2025-01-17 10:09:13 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

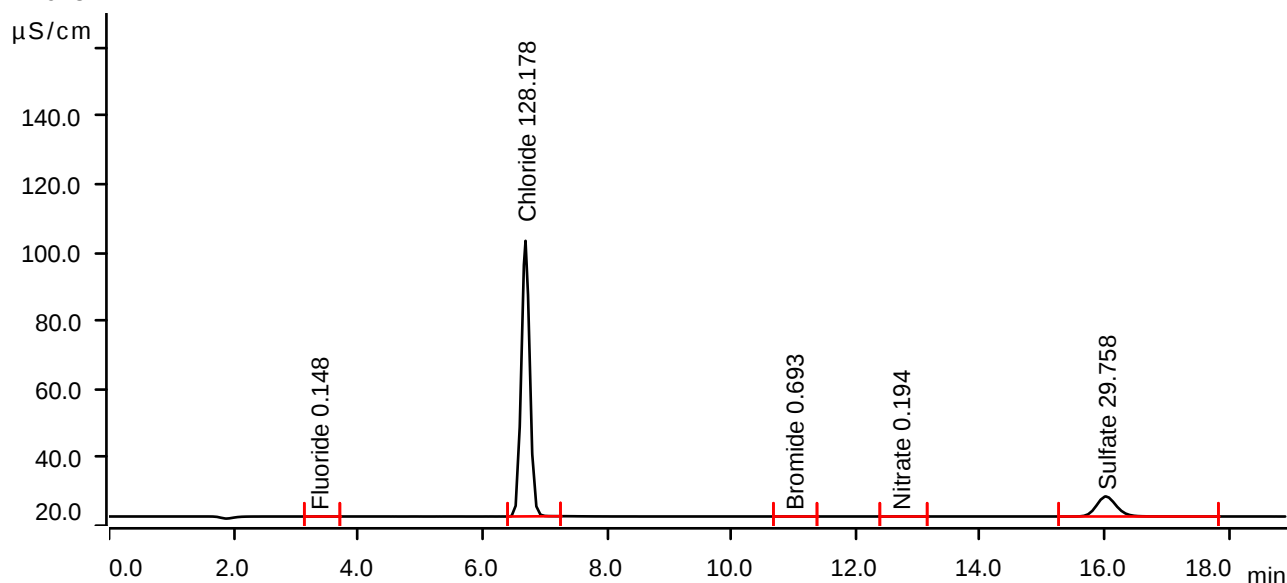

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.0021	0.013	0.148	Fluoride
2	6.693	12.6839	80.698	128.178	Chloride
3	10.997	0.0038	0.015	0.693	Bromide
4	12.712	0.0074	0.027	0.194	Nitrate
5	16.018	2.1896	5.878	29.758	Sulfate


Sample data

Ident Q1120-01MS
Sample type Sample
Determination start 2025-01-17 10:30:46 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

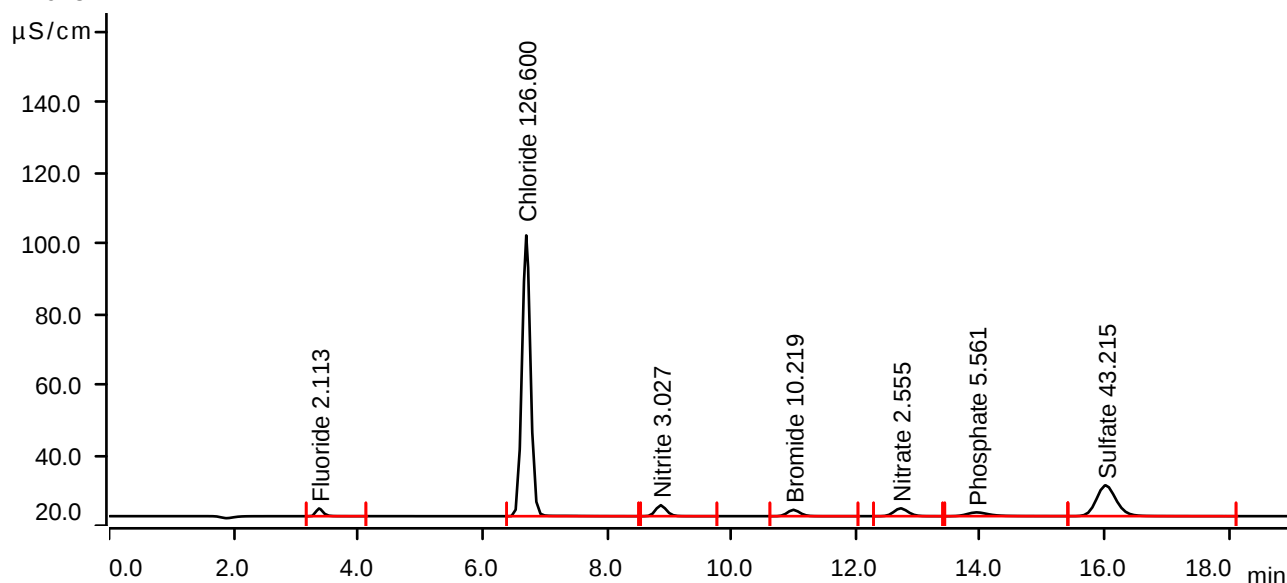

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.375	0.2922	2.192	2.113	Fluoride
2	6.705	12.5276	79.486	126.600	Chloride
3	8.867	0.6398	3.103	3.027	Nitrite
4	10.997	0.4250	1.792	10.219	Bromide
5	12.720	0.5955	2.208	2.555	Nitrate
6	13.942	0.4417	1.066	5.561	Phosphate
7	16.015	3.2197	8.721	43.215	Sulfate


Sample data

Ident Q1120-01MSD
Sample type Sample
Determination start 2025-01-17 10:52:19 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

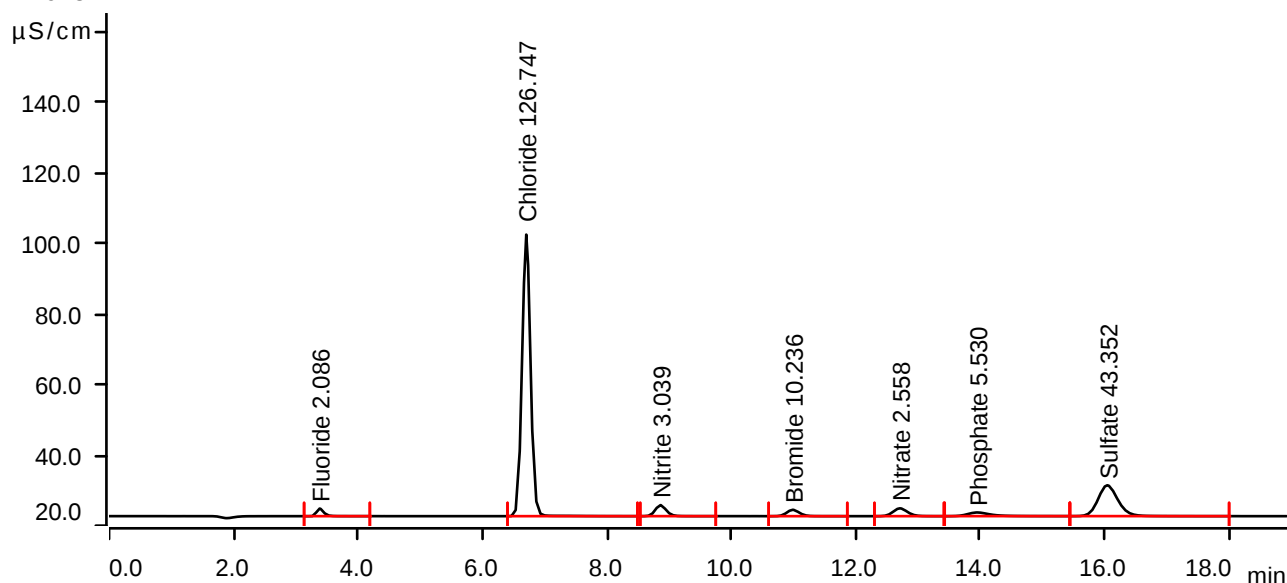

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.385	0.2883	2.158	2.086	Fluoride
2	6.705	12.5422	79.706	126.747	Chloride
3	8.862	0.6425	3.118	3.039	Nitrite
4	10.987	0.4258	1.801	10.236	Bromide
5	12.708	0.5963	2.215	2.558	Nitrate
6	13.952	0.4389	1.044	5.530	Phosphate
7	16.042	3.2301	8.738	43.352	Sulfate


Sample data

Ident Q1120-01DLX50
Sample type Sample
Determination start 2025-01-17 11:13:53 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

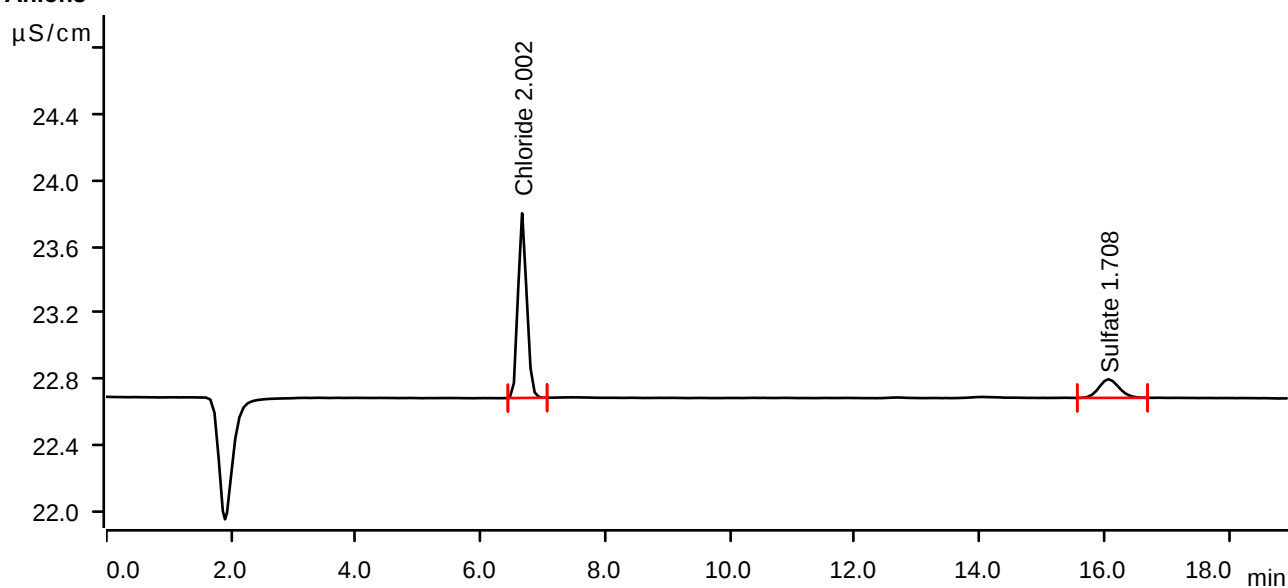

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.665	0.1816	1.118	2.002	Chloride
2	16.062	0.0424	0.113	1.708	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-17 11:35:28 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

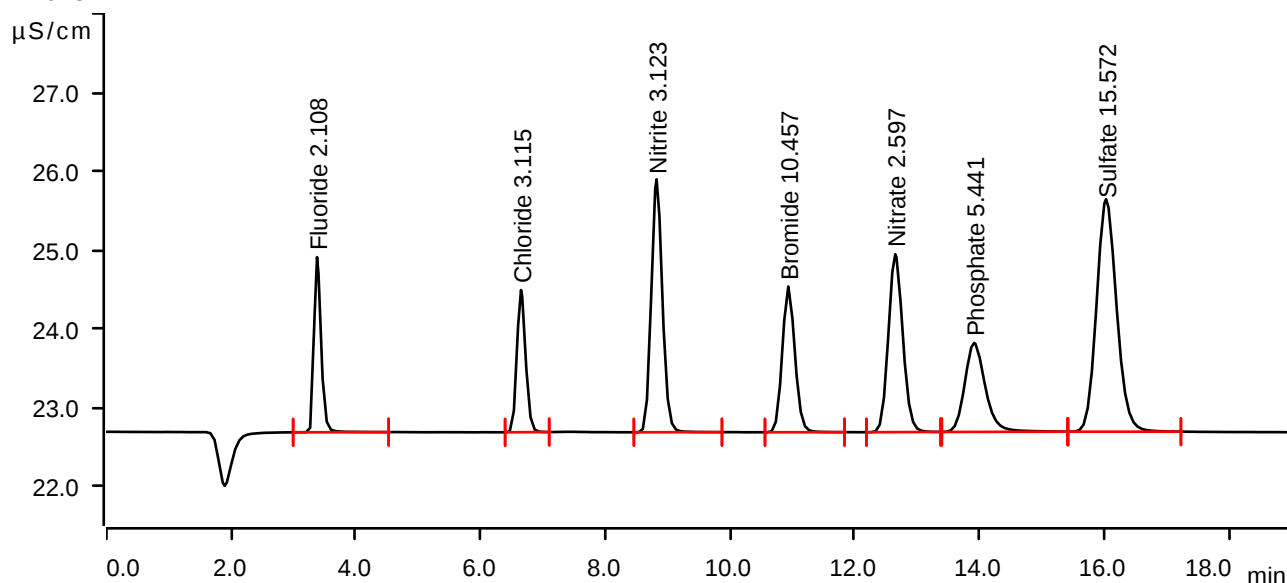


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.2916	2.222	2.108	Fluoride
2	6.648	0.2919	1.804	3.115	Chloride
3	8.822	0.6616	3.210	3.123	Nitrite
4	10.933	0.4355	1.849	10.457	Bromide
5	12.648	0.6059	2.257	2.597	Nitrate
6	13.913	0.4311	1.129	5.441	Phosphate
7	16.028	1.1037	2.950	15.572	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-17 11:56:58 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

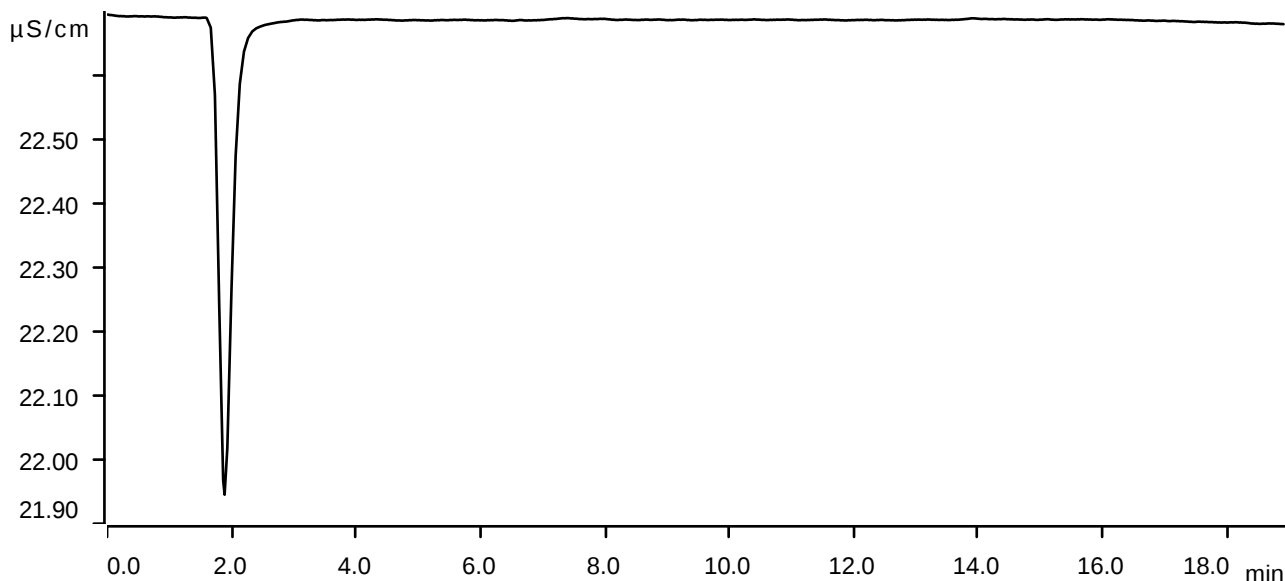Anions

LB134320

WORKLIST(Hardcopy Internal Chain)

WorkList Name : ANIONS-01172025

WorkList ID : 186969

Department : Wet-Chemistry

Date : 01-17-2025 08:00:06

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1120-01	RW10A-20250116	Water	Anions Group2		TETR06	M11	01/16/2025	300.0

Date/Time 01.17.2025, 09:00
Raw Sample Received by: NFWC
Raw Sample Relinquished by: NFWC

Date/Time 01.17.2025, 11:15
Raw Sample Received by: NFWC
Raw Sample Relinquished by: NFWC