

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010625\
 Data File : PP068920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2025 21:19
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 03:22:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 03:22:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.672	3.983	75140981	52106220	50.000	50.000
2) SA Decachlor...	10.525	9.112	57933955	62437321	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.873	4.197	8892583	6745743	500.000	500.000
9) L2 AR-1221-2	4.960	4.285	6435961	5189108	500.000	500.000
10) L2 AR-1221-3	5.036	4.362	19383914	15524592	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010625\
Data File : PP068920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2025 21:19
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 03:22:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 03:22:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

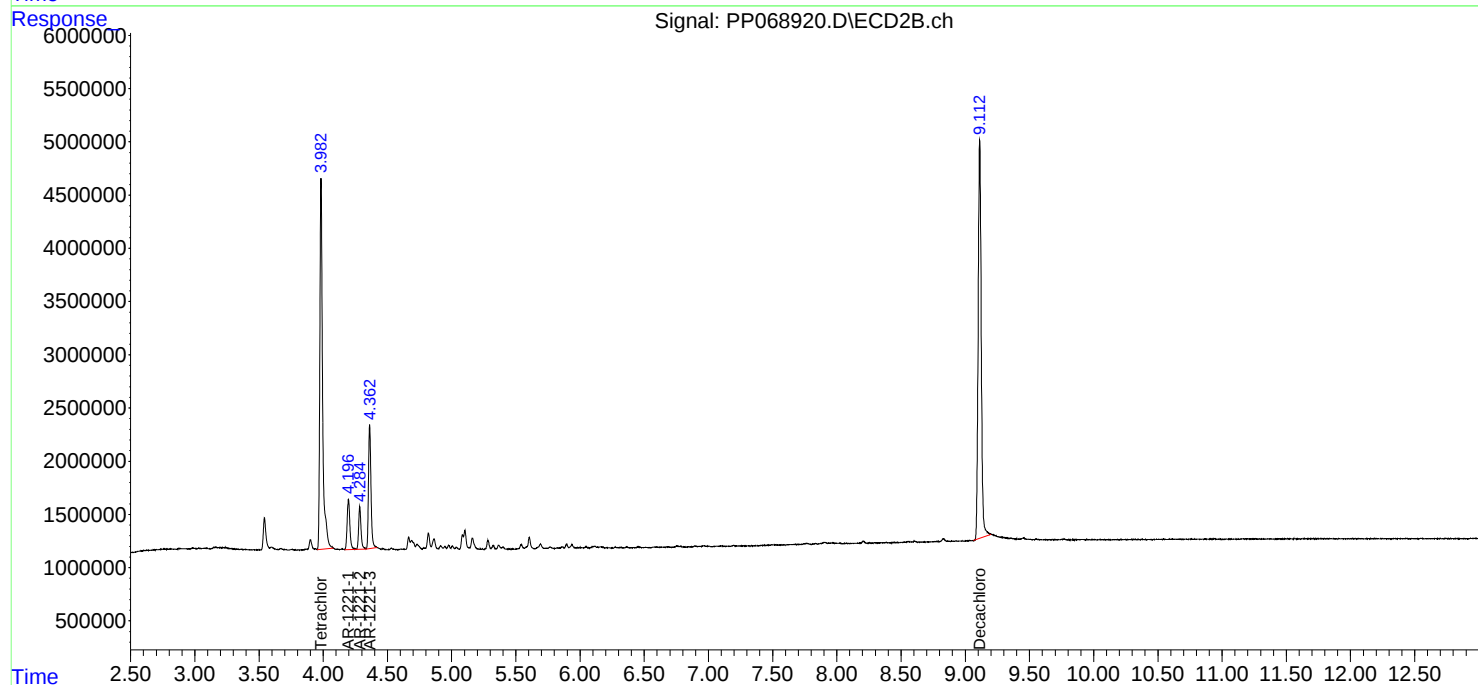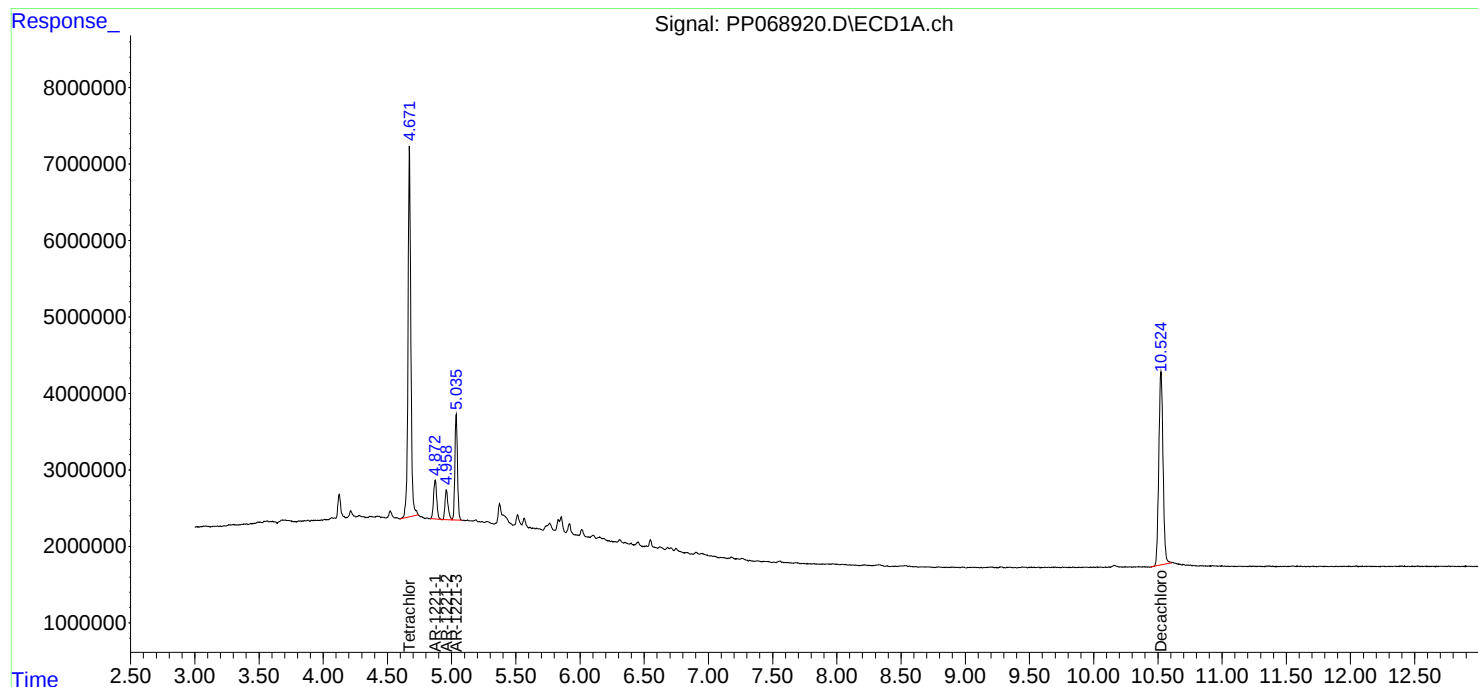


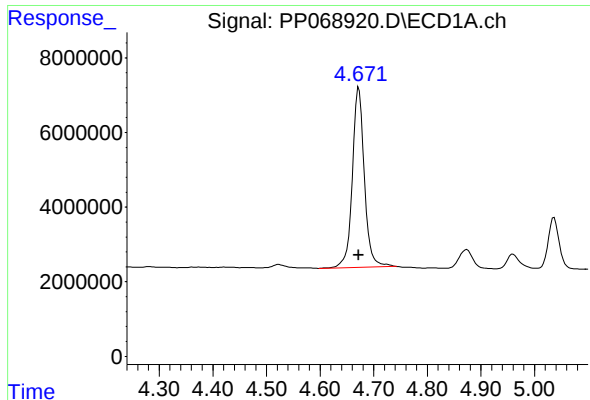

#1 Tetrachloro-m-xylene


R.T.: 4.672 min
Delta R.T.: 0.000 min
Response: 75140981
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

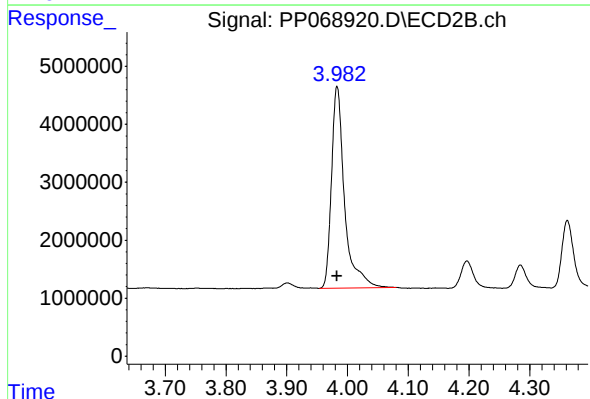


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 52106220
Conc: 50.00 ng/ml

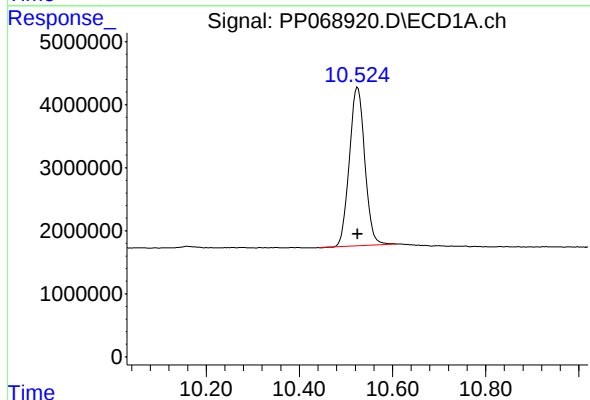


#2 Decachlorobiphenyl

R.T.: 10.525 min
Delta R.T.: 0.000 min
Response: 57933955
Conc: 50.00 ng/ml

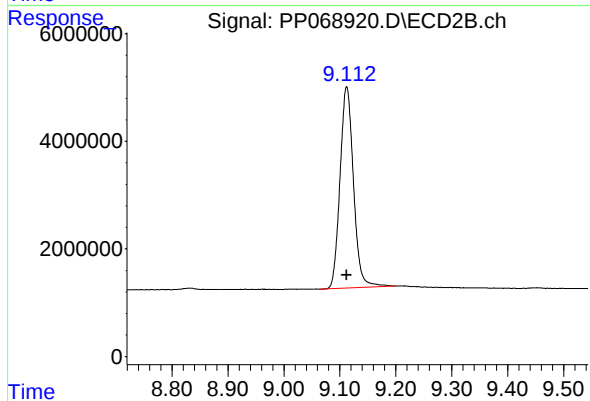

#2 Decachlorobiphenyl


R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 62437321
Conc: 50.00 ng/ml

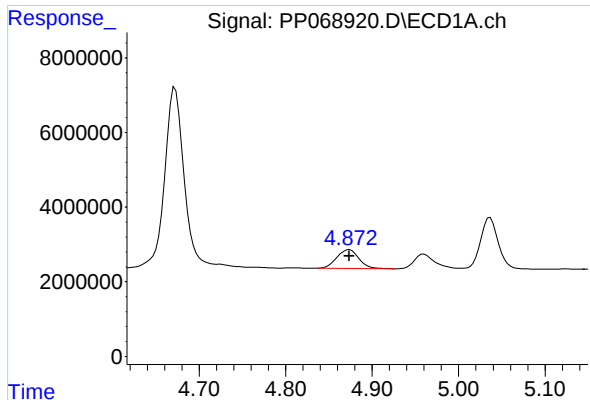

#8 AR-1221-1


R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 8892583
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

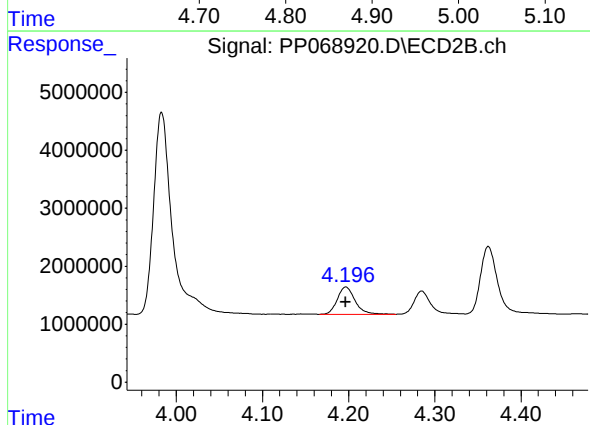


#8 AR-1221-1

R.T.: 4.197 min
Delta R.T.: 0.000 min
Response: 6745743
Conc: 500.00 ng/ml

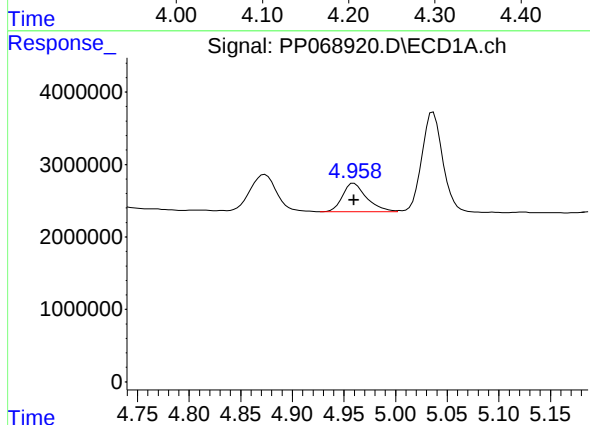


#9 AR-1221-2

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 6435961
Conc: 500.00 ng/ml

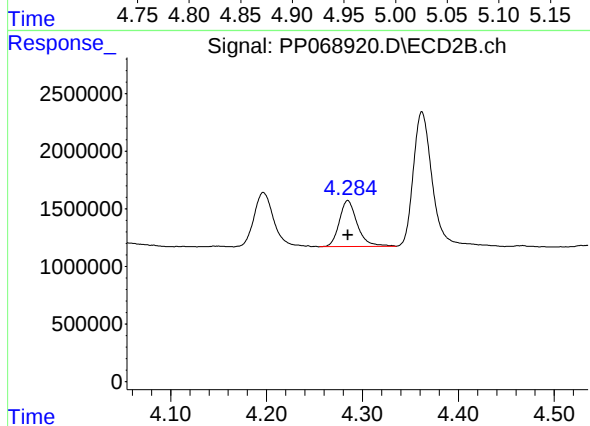

#9 AR-1221-2


R.T.: 4.285 min
Delta R.T.: 0.000 min
Response: 5189108
Conc: 500.00 ng/ml

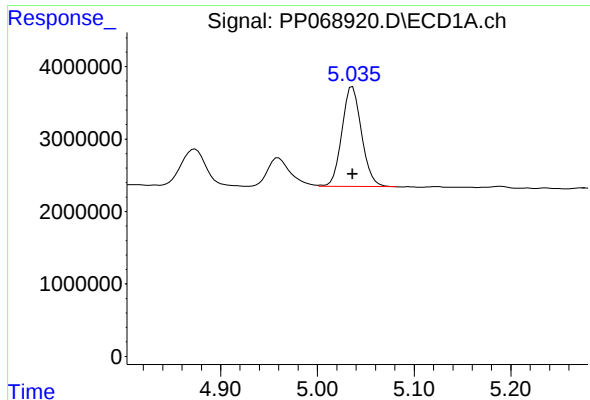

#10 AR-1221-3

R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 19383914
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

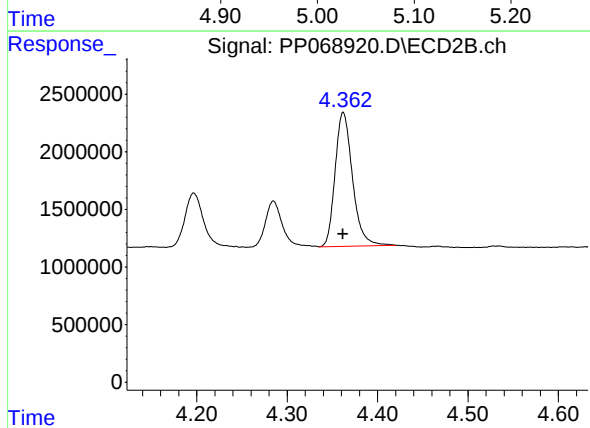

#10 AR-1221-3

R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 15524592
Conc: 500.00 ng/ml