


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012025\
Data File : BF141211.D
Acq On : 20 Jan 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

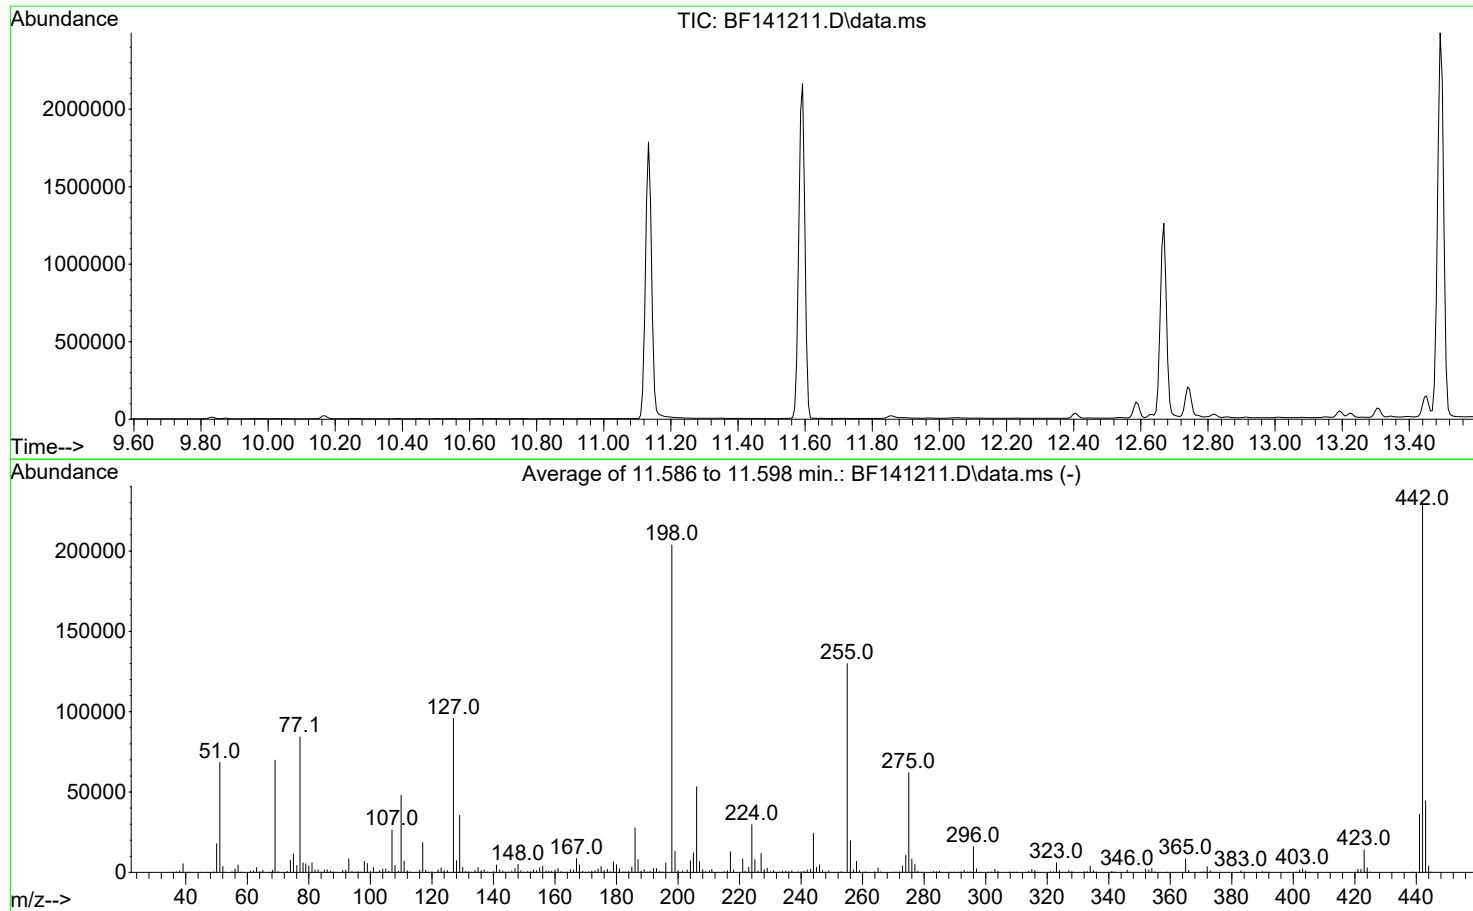

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	68317	PASS
68	69	0.00	2	2.0	1395	PASS
69	198	0.00	100	34.3	69851	PASS
70	69	0.00	2	0.6	440	PASS
127	198	10	80	47.0	95797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	203712	PASS
199	198	5	9	6.4	13092	PASS
275	198	10	60	30.5	62040	PASS
365	198	1	100	4.1	8447	PASS
441	198	0.01	100	17.7	36021	PASS
442	442	50	100	100.0	228949	PASS
443	442	15	24	19.5	44563	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/20/2025	BNA_F	<u>BF141211.D</u>
Compound Name	Response	Retention Time
DDT	626135	13.492
DDD	17930	13.192
DDE	1512	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19442	645577	3.01

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012025\
Data File : BF141211.D
Acq On : 20 Jan 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 20 10:54:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

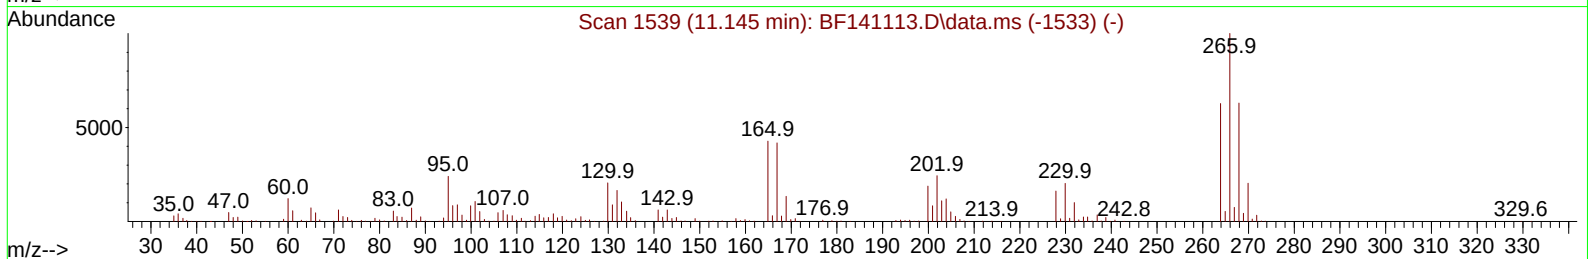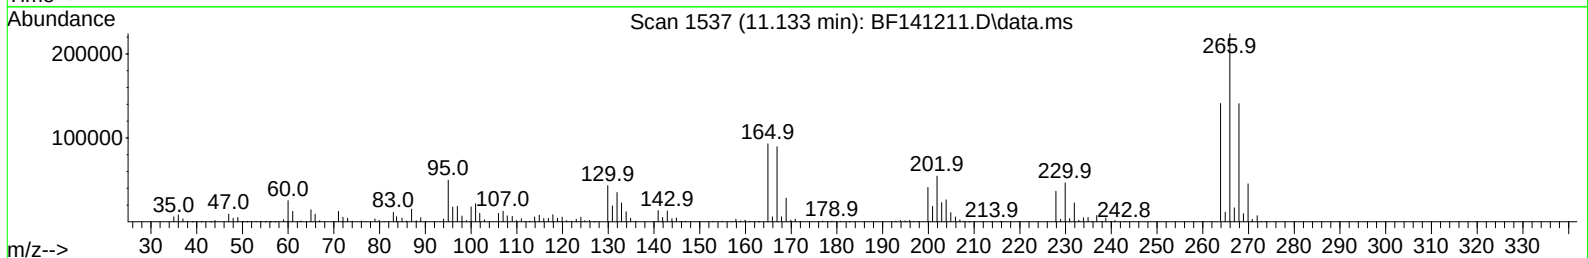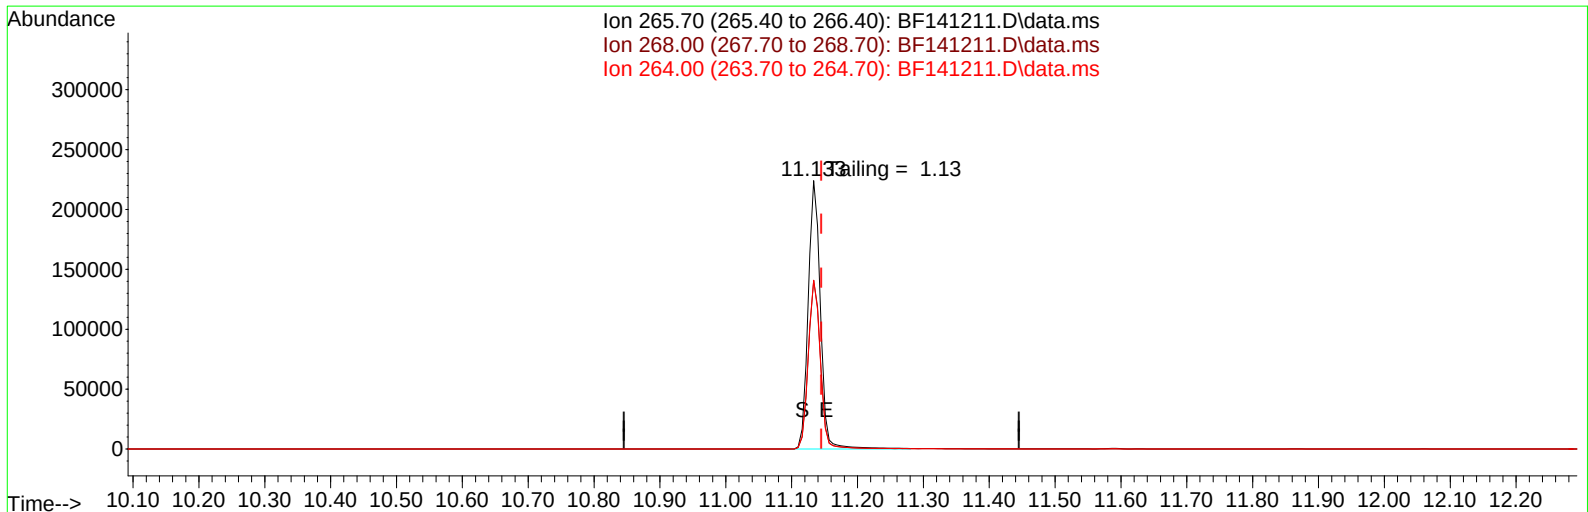

TIC: BF141211.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.012) 44495.62 ng




response 289966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.84
264.00	62.70	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012025\
Data File : BF141211.D
Acq On : 20 Jan 2025 09:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 20 10:54:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

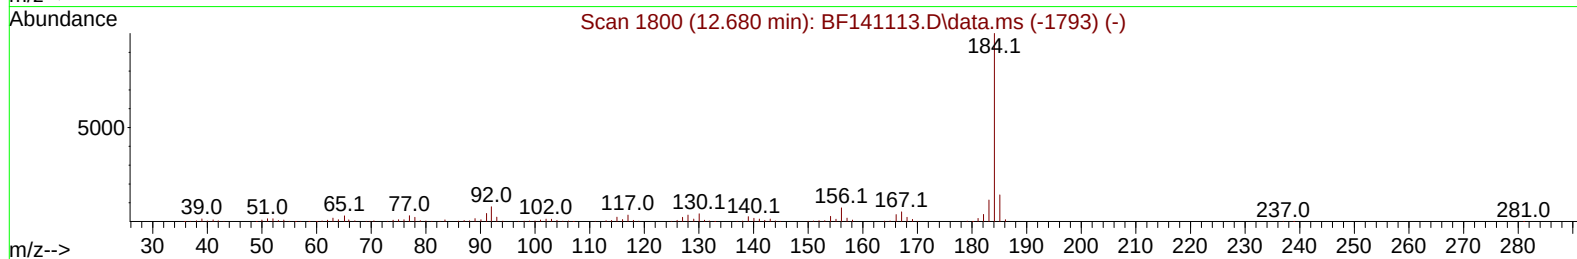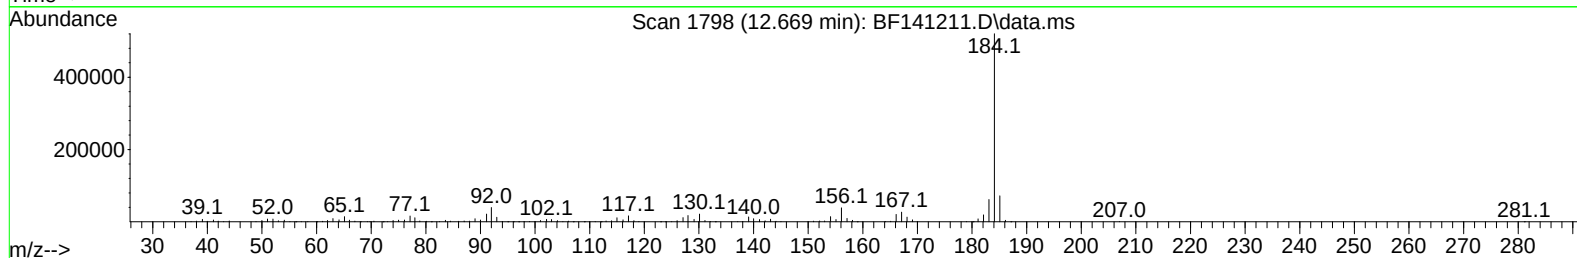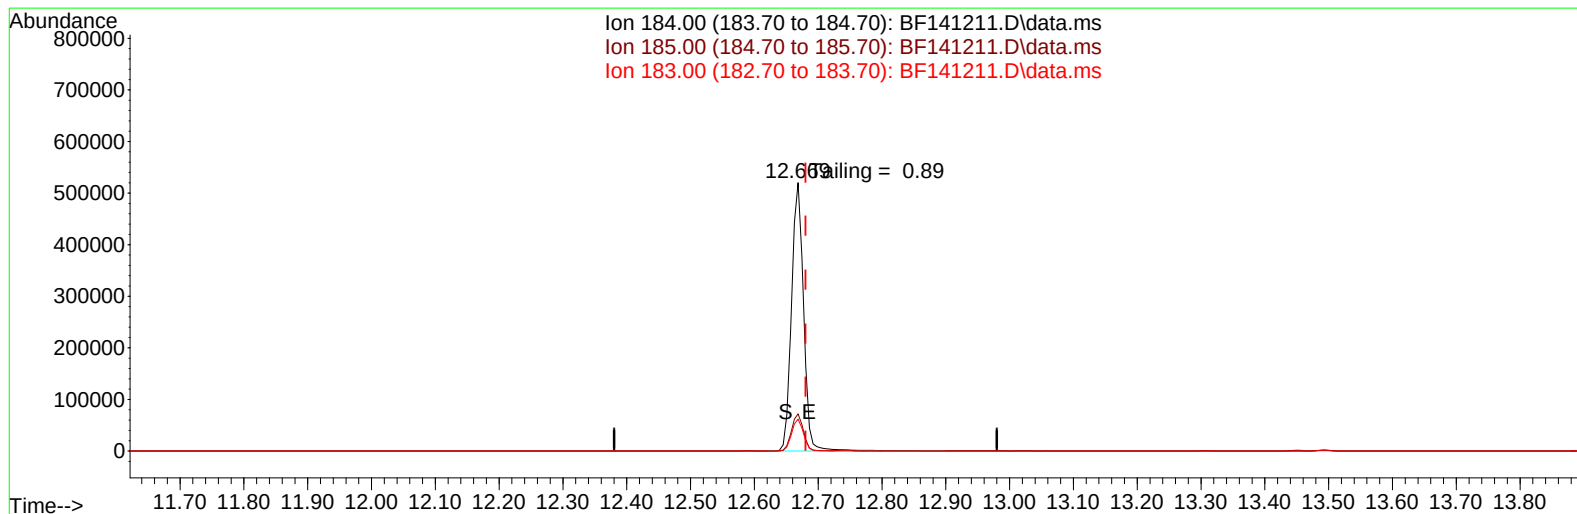

TIC: BF141211.D\data.ms

(77) Benzidine

12.669min (-0.012) 48437.63 ng

response 683565

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.84
183.00	11.50	11.90
0.00	0.00	0.00