
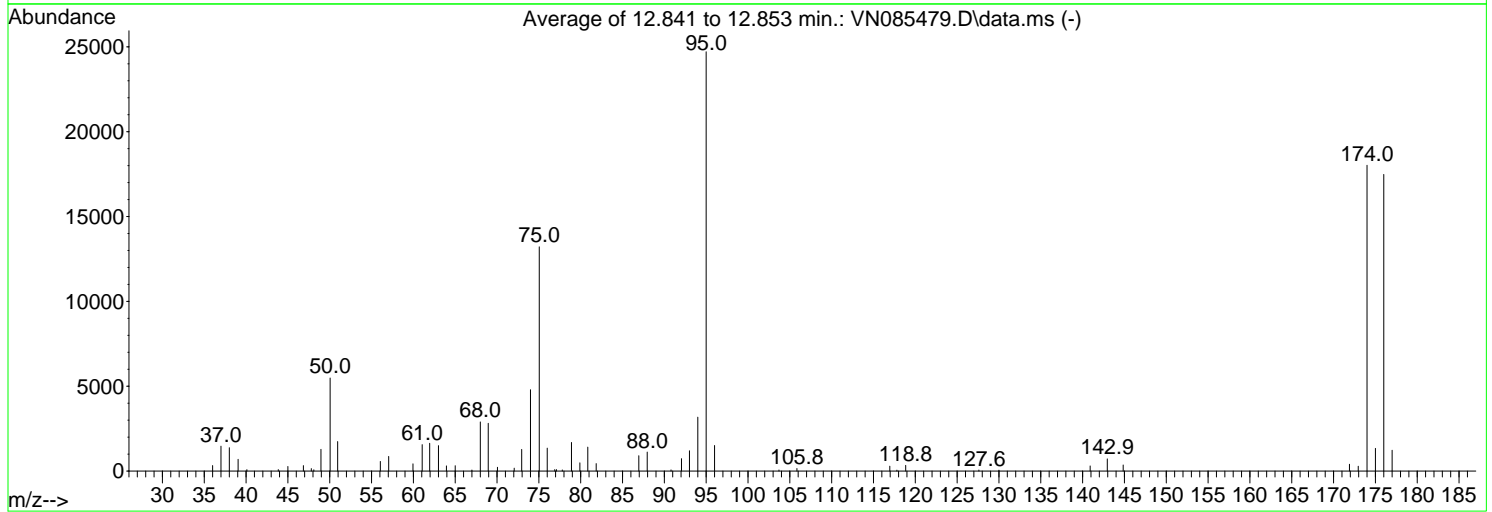


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN011725\  
 Data File : VN085479.D  
 Acq On : 17 Jan 2025 08:18  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N011425W.M  
 Title : SW846 8260  
 Last Update : Wed Jan 15 02:16:08 2025

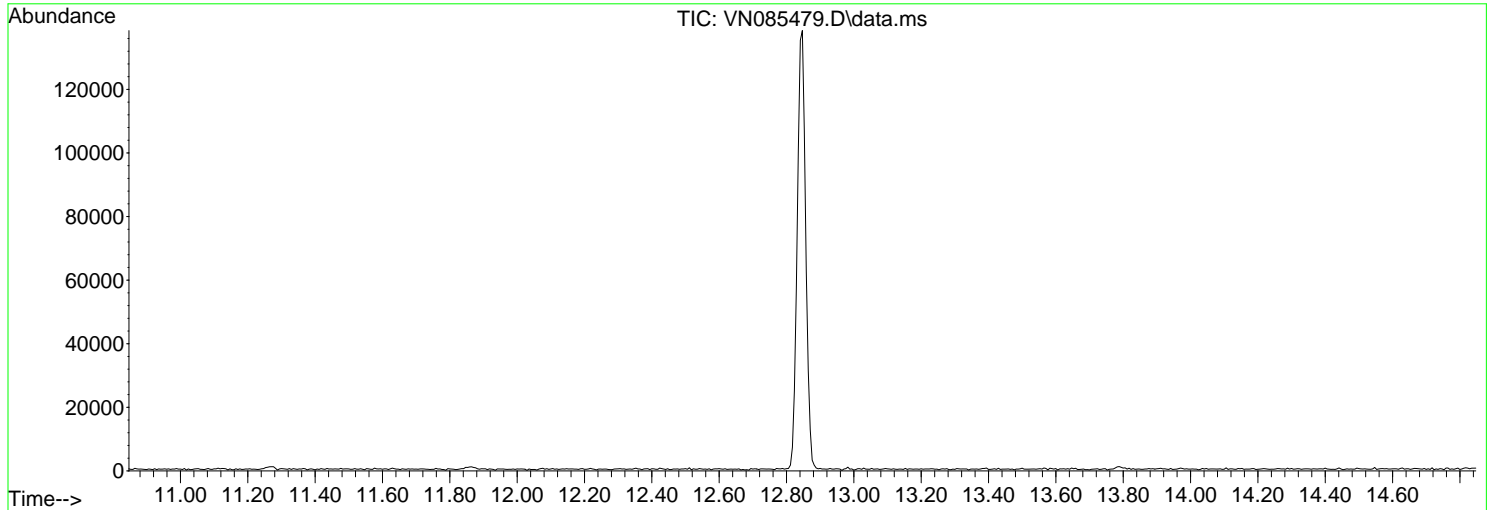

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	5485	PASS
75	95	30	60	53.5	13217	PASS
95	95	100	100	100.0	24712	PASS
96	95	5	9	6.1	1509	PASS
173	174	0.00	2	1.6	286	PASS
174	95	50	100	72.9	18023	PASS
175	174	5	9	7.4	1339	PASS
176	174	95	101	97.0	17481	PASS
177	176	5	9	7.0	1228	PASS

Average of 12.841 to 12.853 min.: VN085479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	326	50.05	5485	68.00	2897	78.90	1686
37.00	1469	50.95	1739	68.95	2815	79.90	486
38.00	1378	56.05	568	70.05	223	80.85	1412
39.05	693	57.05	862	72.05	173	81.85	440
40.10	84	59.95	426	72.95	1277	86.95	906
43.85	87	61.05	1559	74.00	4795	87.95	1121
45.00	272	61.95	1639	75.05	13217	90.80	72
46.85	323	63.00	1500	76.00	1351	92.05	734
47.80	146	63.95	306	76.90	87	93.00	1197
48.10	77	65.00	317	77.10	88	94.00	3178
48.95	1281	67.00	63	77.80	69	95.00	24712

Average of 12.841 to 12.853 min.: VN085479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.00	1509	171.90	401				
103.70	66	172.95	286				
105.85	153	174.00	18023				
116.95	288	175.00	1339				
117.80	56	176.00	17481				
118.85	336	177.00	1228				
127.60	62						
130.00	53						
140.90	303						
142.95	718						
144.85	358						

Instrument :

MSVOA\_N

ClientSampleId :

BFB