

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063229.D
 Acq On : 11 Feb 2025 11:14
 Operator : MD/SY
 Sample : VU0211WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0211WBL01

Quant Time: Feb 12 03:16:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 11 08:42:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	52216	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	13937	0.809	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	14680	0.820	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063229.D
Acq On : 11 Feb 2025 11:14
Operator : MD/SY
Sample : VU0211WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0211WBL01

Quant Time: Feb 12 03:16:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 11 08:42:19 2025
Response via : Initial Calibration




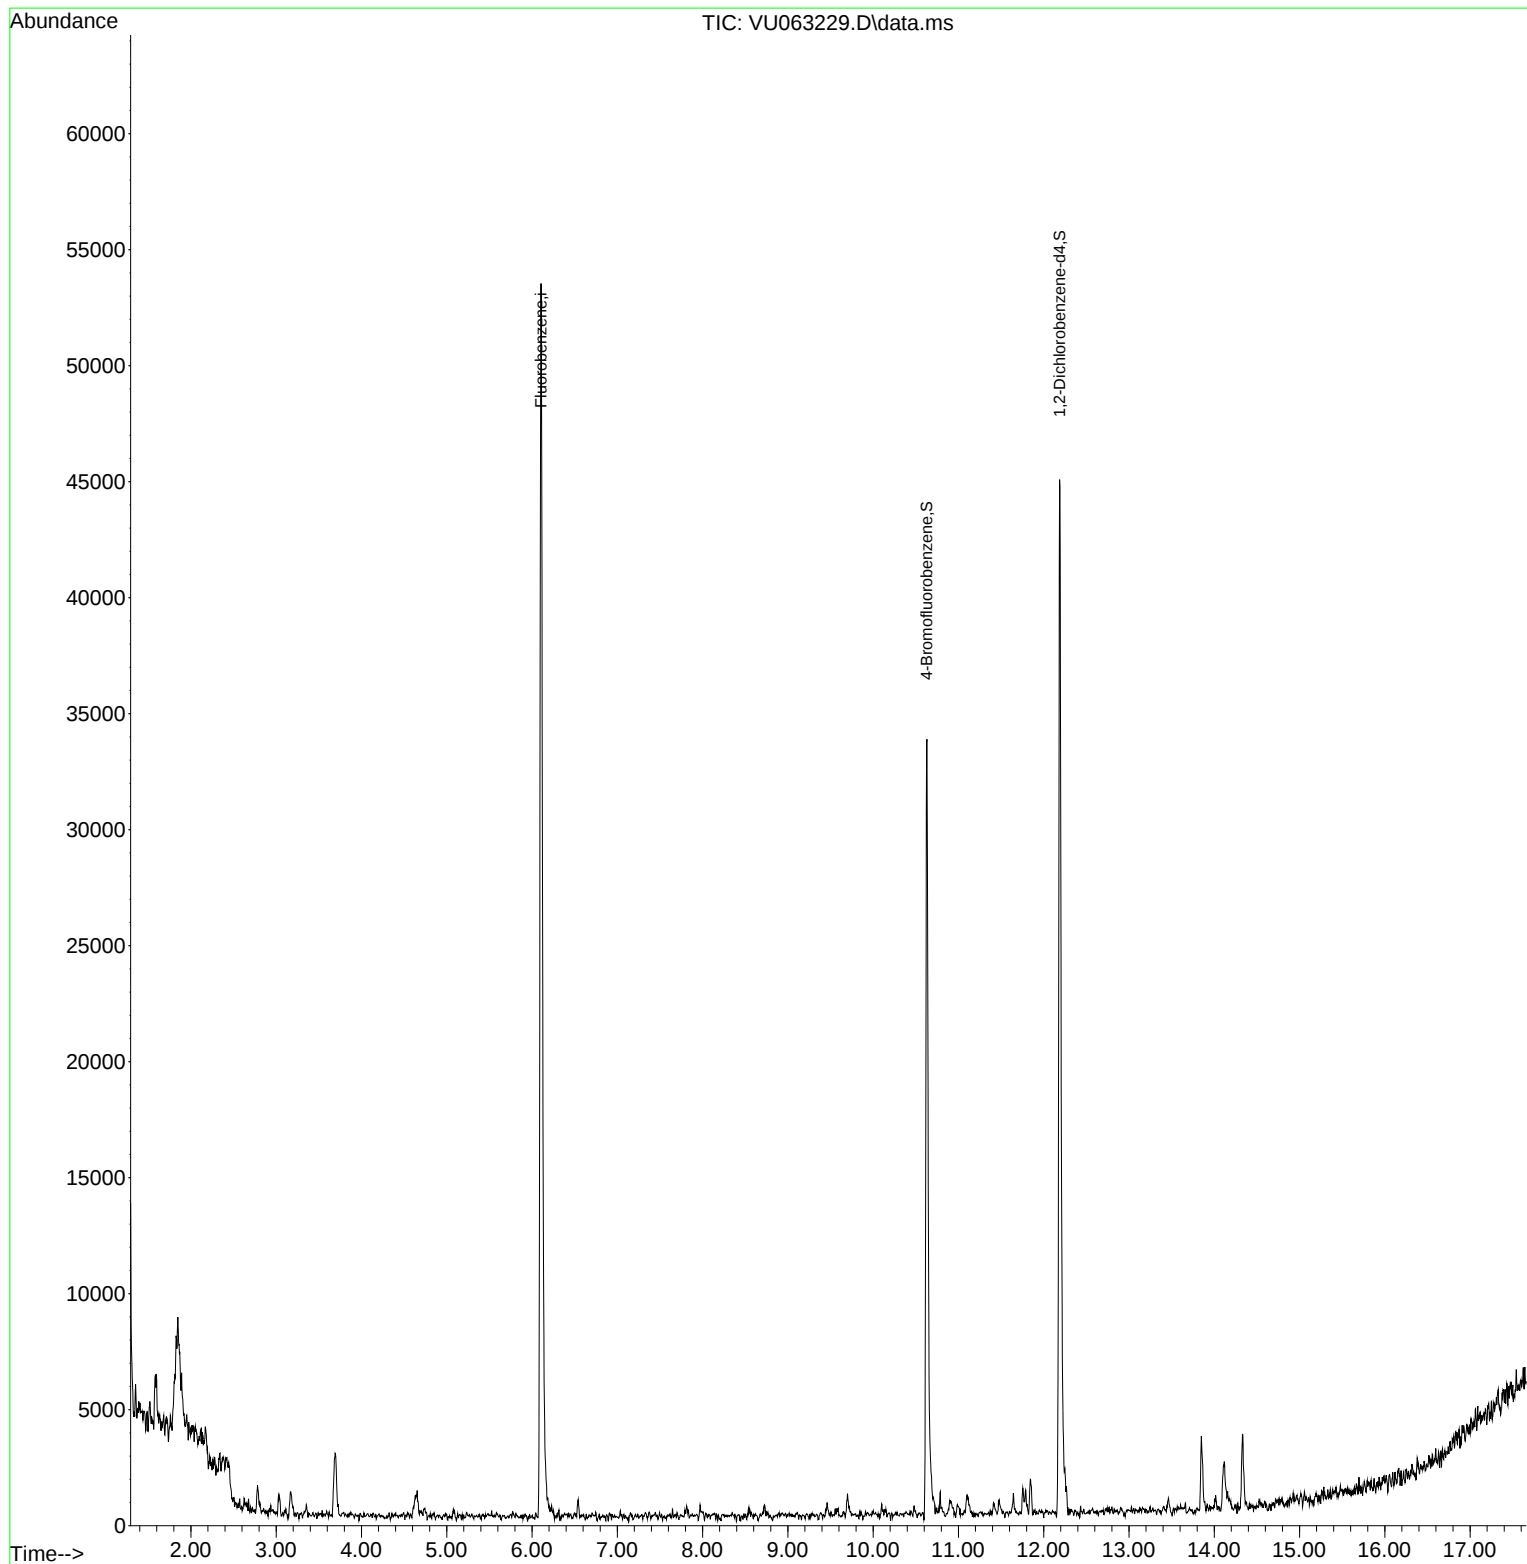


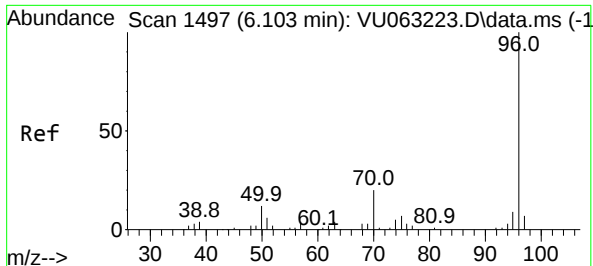

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1497
Delta R.T. 0.004 min
Lab File: VU063229.D
Acq: 11 Feb 2025 11:14




Instrument :
MSVOA_U
ClientSampleId :
VU0211WBL01


Tgt Ion: 96	Resp: 52216
Ion Ratio	Lower Upper
96 100	
70 20.0	15.6 23.4
95 9.2	7.3 10.9
97 6.4	0.0 0.0#

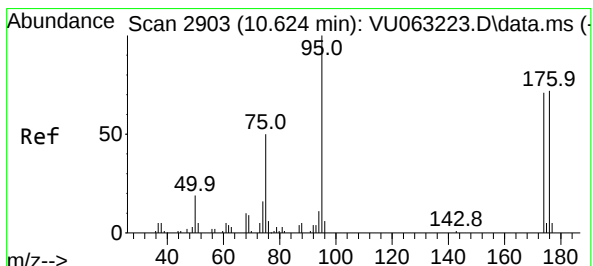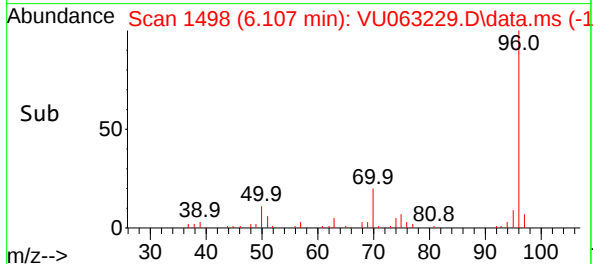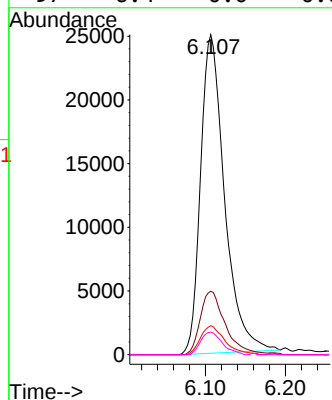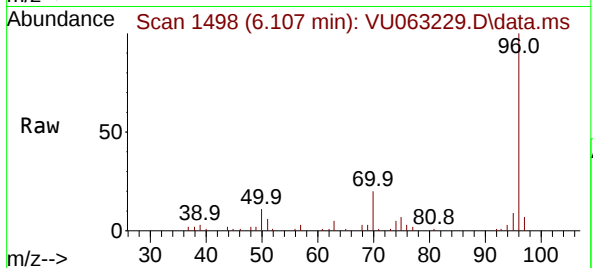

#57
4-Bromofluorobenzene
Concen: 0.809 ug/l
RT: 10.627 min Scan# 2904
Delta R.T. 0.003 min
Lab File: VU063229.D
Acq: 11 Feb 2025 11:14

Tgt Ion: 95	Resp: 13937
Ion Ratio	Lower Upper
95 100	
174 82.6	58.6 88.0
176 80.1	58.2 87.4

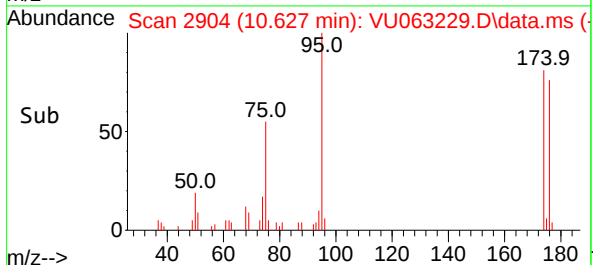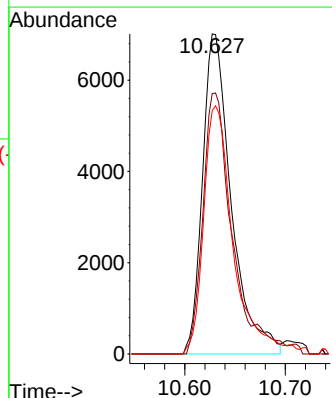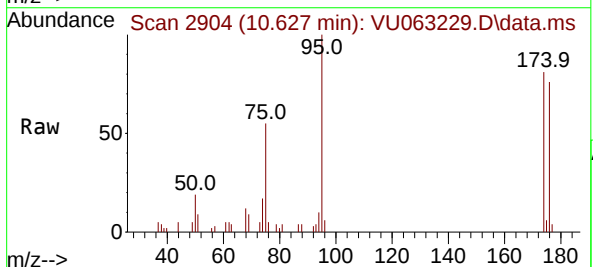

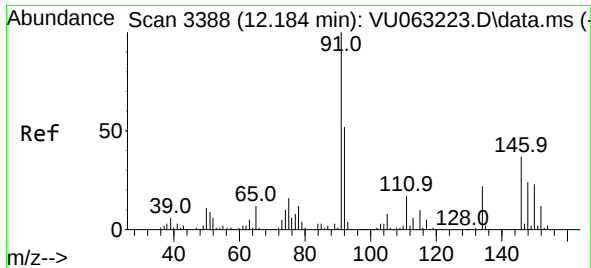

#68

1,2-Dichlorobenzene-d4

Concen: 0.820 ug/l

RT: 12.187 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU063229.D


Acq: 11 Feb 2025 11:14

Instrument :

MSVOA_U

ClientSampleId :

VU0211WBL01

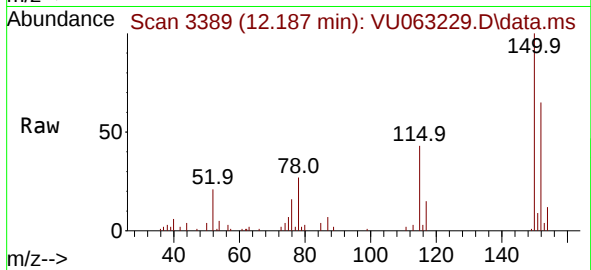

Tgt Ion:152 Resp: 14680

Ion Ratio Lower Upper

152 100

115 61.4 0.0 275.2

150 143.3 0.0 658.4

