


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020325\
Data File : BG063974.D
Acq On : 3 Feb 2025 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 04 02:51:00 2025

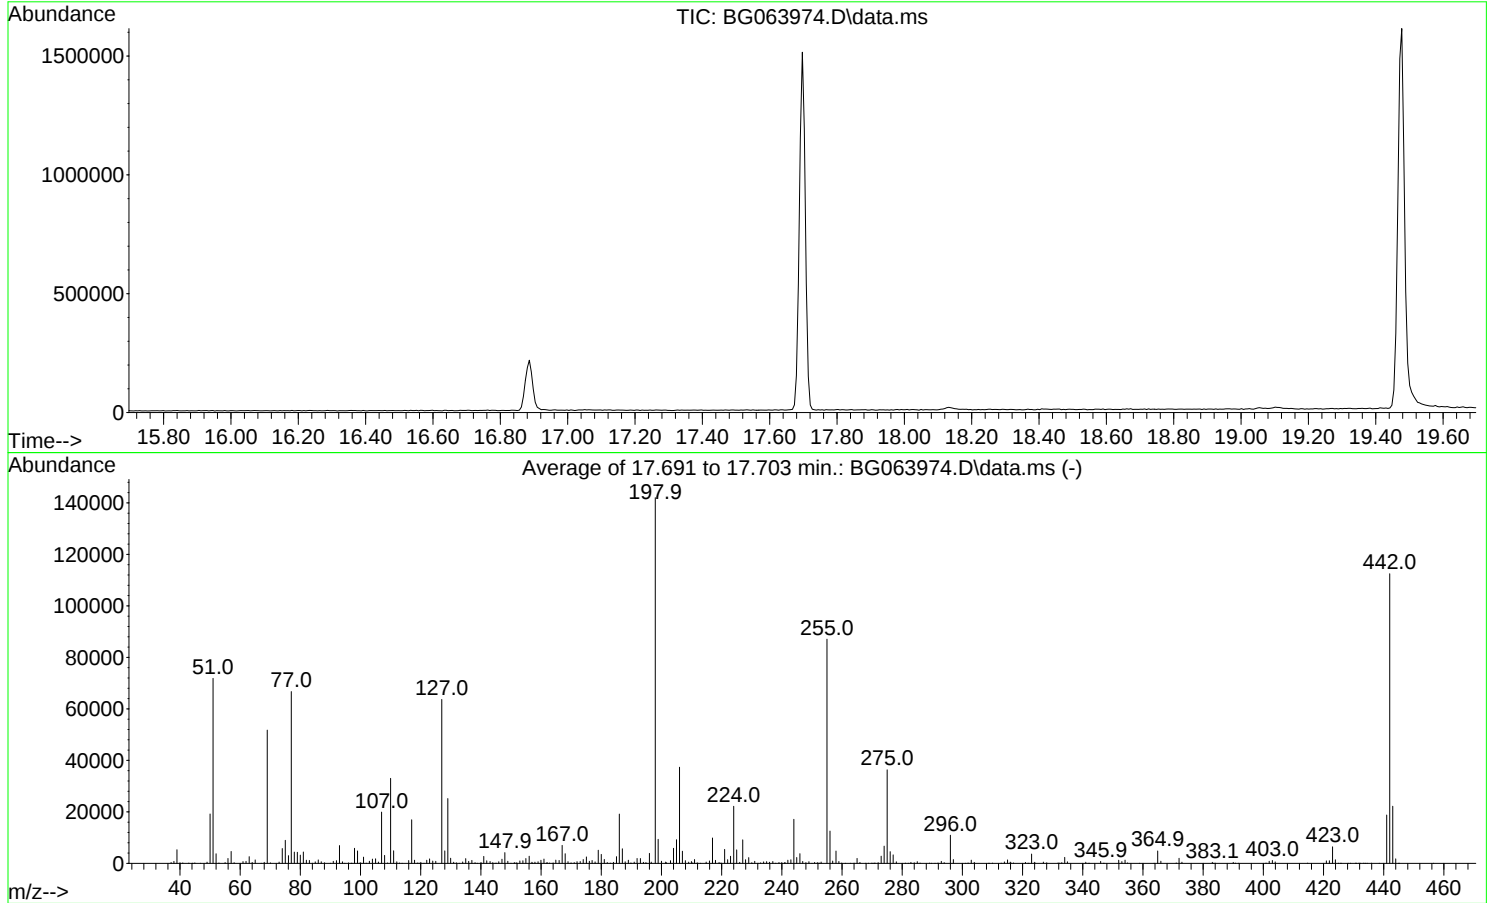




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	71845	PASS
68	69	0.00	2	0.8	422	PASS
69	198	0.00	100	36.4	51767	PASS
70	69	0.00	2	0.4	214	PASS
127	198	10	80	44.8	63667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	142024	PASS
199	198	5	9	6.6	9345	PASS
275	198	10	60	25.6	36341	PASS
365	198	1	100	3.4	4818	PASS
441	198	0.01	100	13.2	18774	PASS
442	442	50	100	100.0	112480	PASS
443	442	15	24	19.7	22199	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020325\
Data File : BG063974.D
Acq On : 3 Feb 2025 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 04 02:35:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:30:48 2025
Response via : Initial Calibration

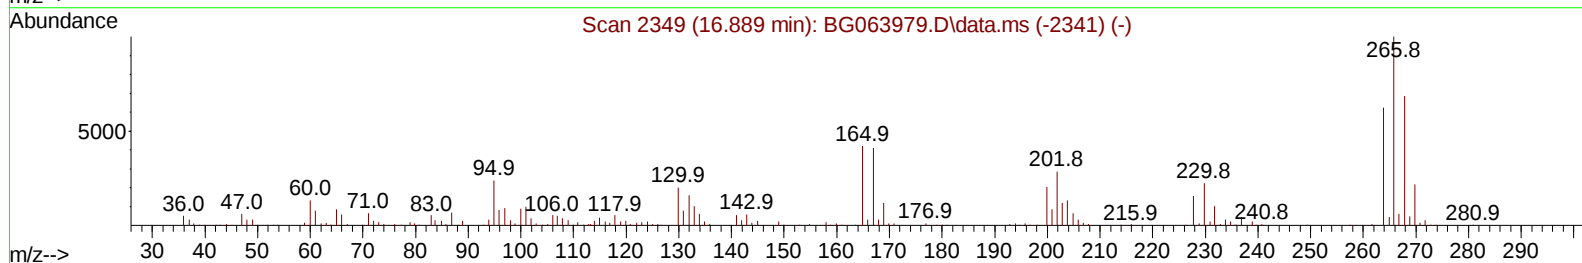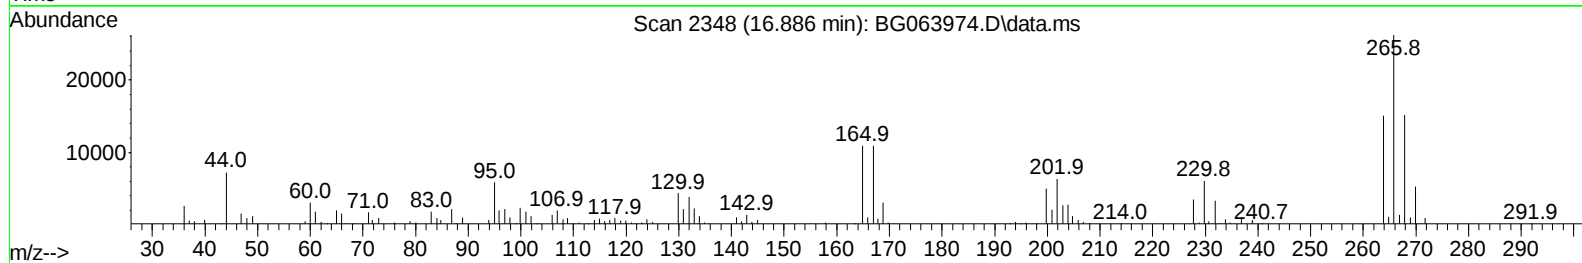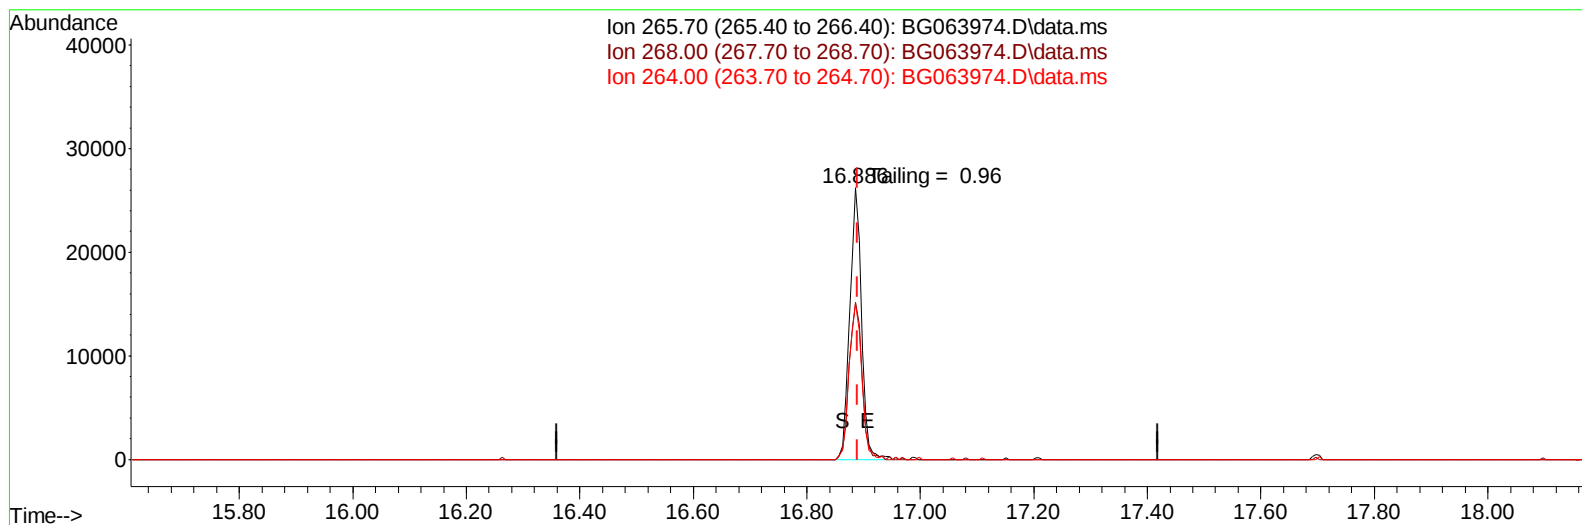

TIC: BG063974.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.003) 74371.74 ng




response 37632

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	57.98
264.00	62.50	57.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020325\
Data File : BG063974.D
Acq On : 3 Feb 2025 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 04 02:35:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:30:48 2025
Response via : Initial Calibration

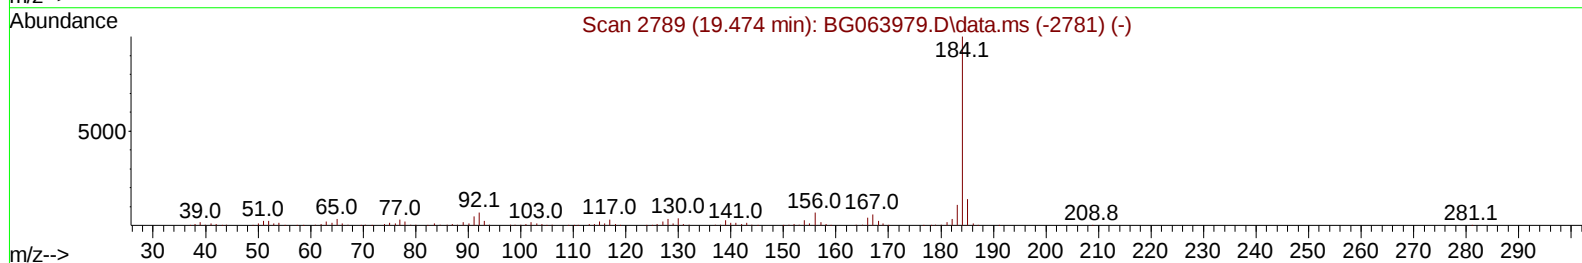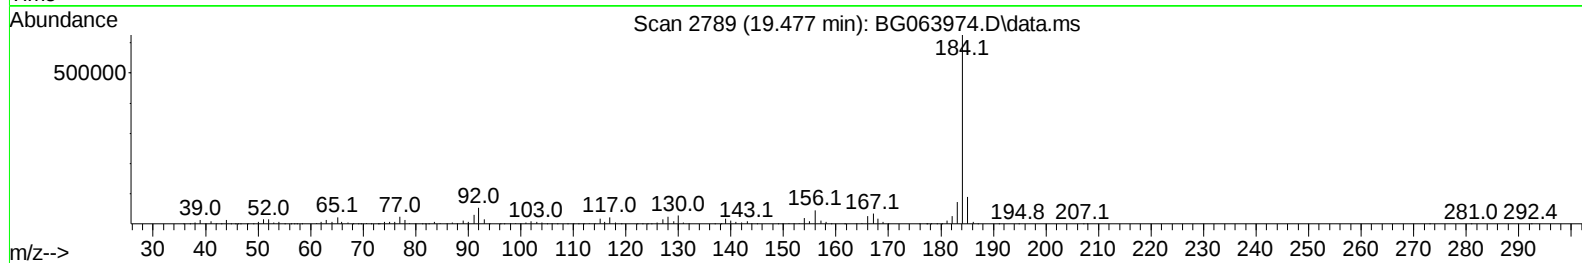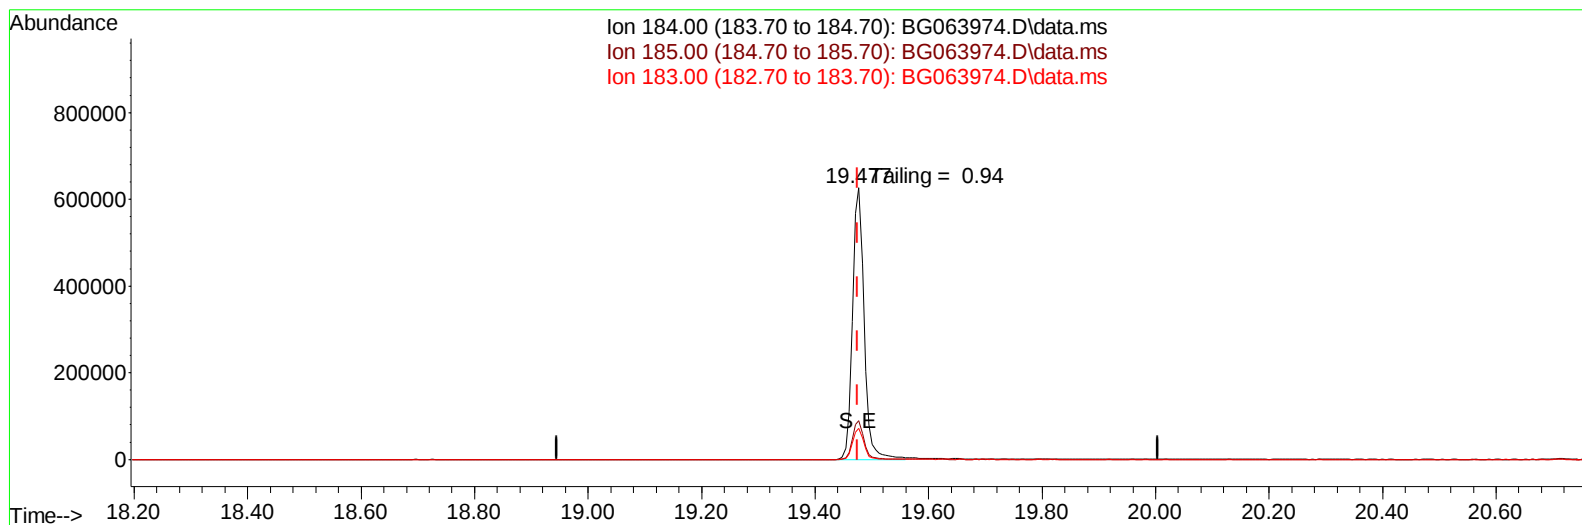

TIC: BG063974.D\data.ms

(77) Benzidine

19.477min (+ 0.003) 7478.24 ng

response 894155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.19
183.00	10.90	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2025	BNA_G	<u>BG063974.D</u>
Compound Name	Response	Retention Time
DDT	186437	20.711
DDD	3510	20.27
DDE	99	19.777
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3609	190046	1.90

Instrument :
BNA_G
ClientSampleId :
DFTPP