


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036111.D
Acq On : 29 Jan 2025 17:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 23 00:34:56 2025

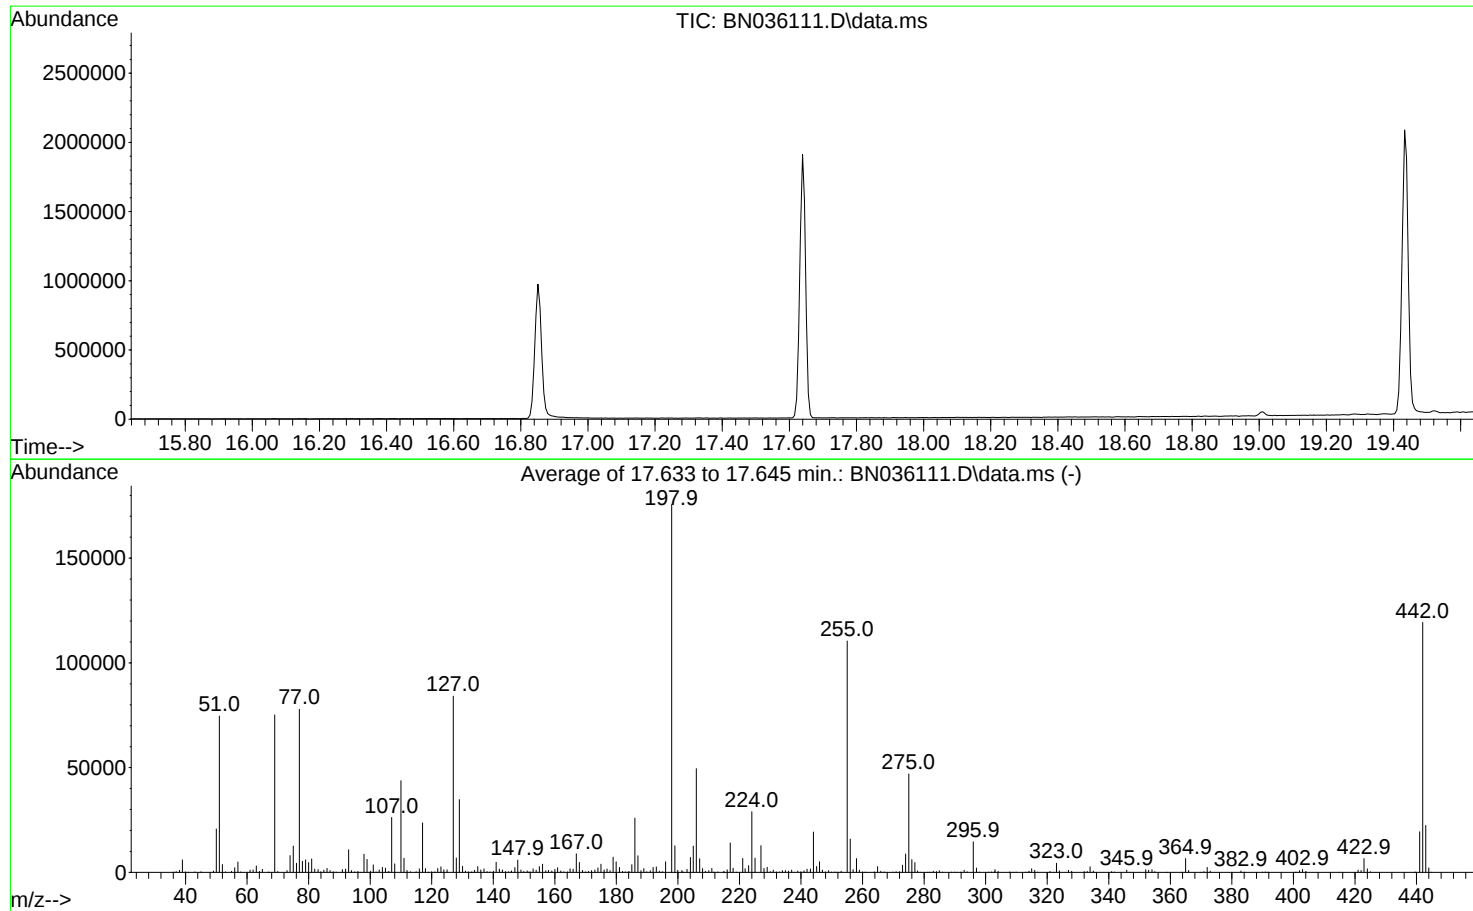

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	74616	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.8	75133	PASS
70	69	0.00	2	0.5	408	PASS
127	198	10	80	47.9	84115	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	175616	PASS
199	198	5	9	7.2	12719	PASS
275	198	10	60	26.8	46979	PASS
365	198	1	100	3.7	6563	PASS
441	198	0.01	100	11.1	19439	PASS
442	442	50	100	100.0	119304	PASS
443	442	15	24	18.8	22371	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/29/2025	BNA_N	<u>BN036111.D</u>
Compound Name	Response	Retention Time
DDT	544371	20.674
DDD	19172	20.233
DDE	1649	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20821	565192	3.68

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036111.D
Acq On : 29 Jan 2025 17:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 30 04:00:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

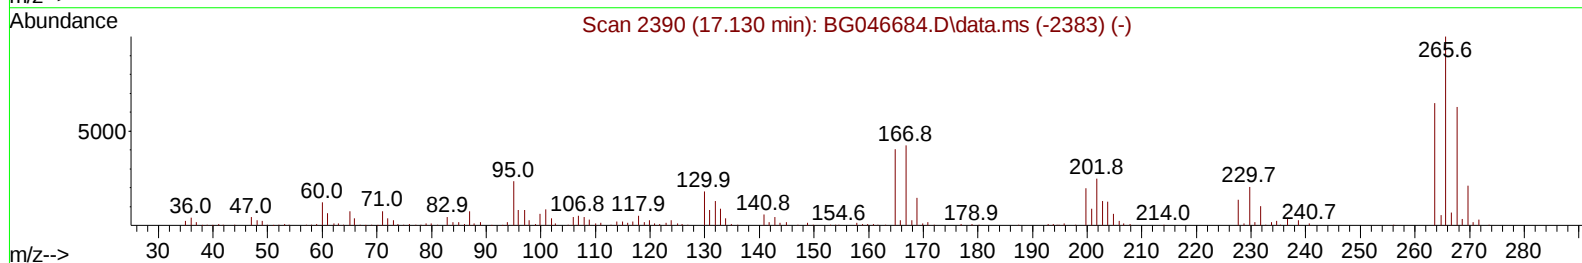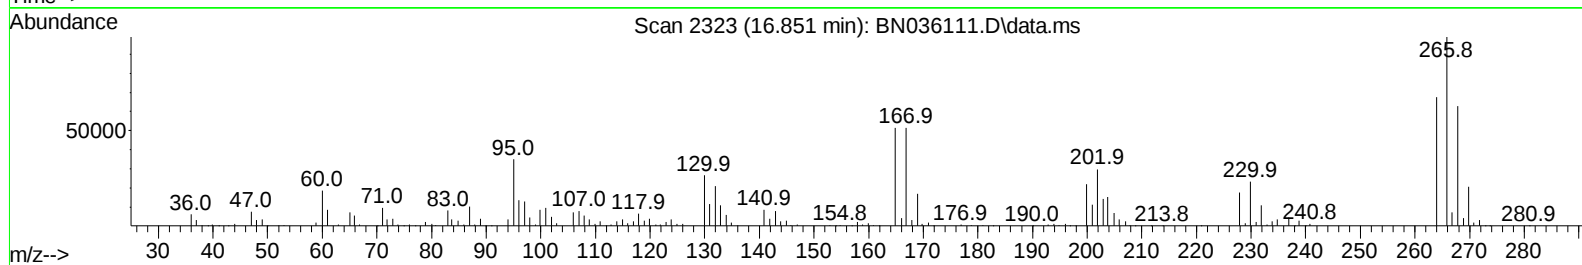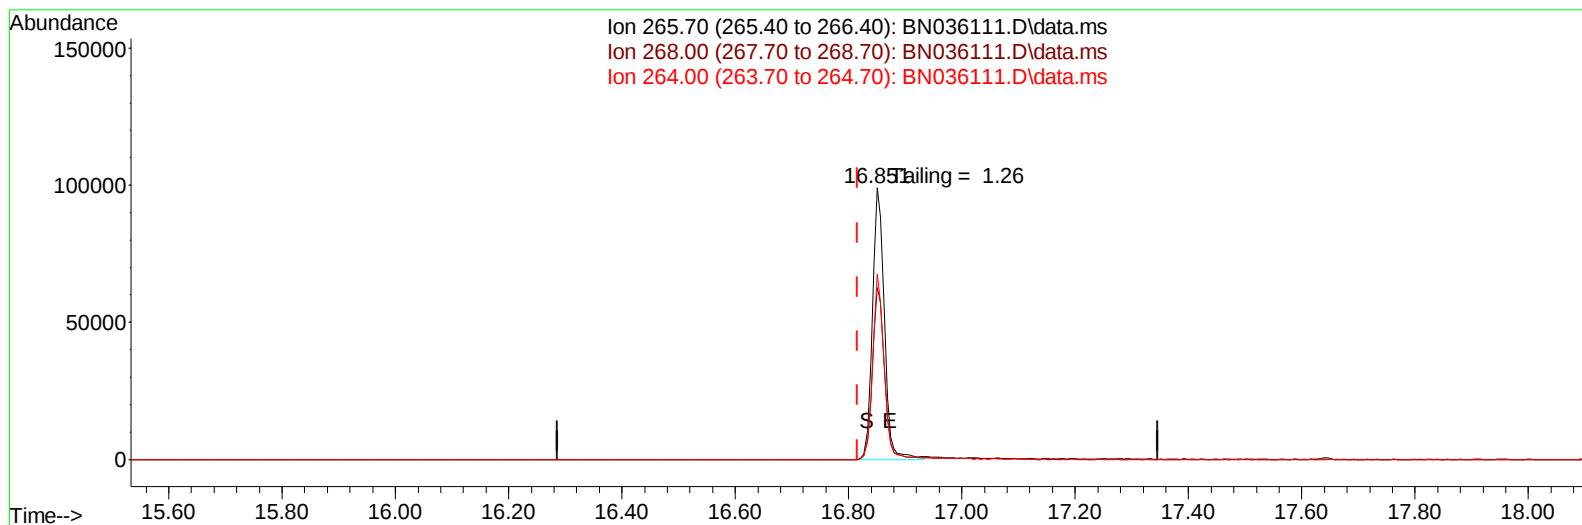

TIC: BN036111.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.035) 14413.06 ng




response 143876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.30
264.00	61.60	68.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036111.D
Acq On : 29 Jan 2025 17:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 30 04:00:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

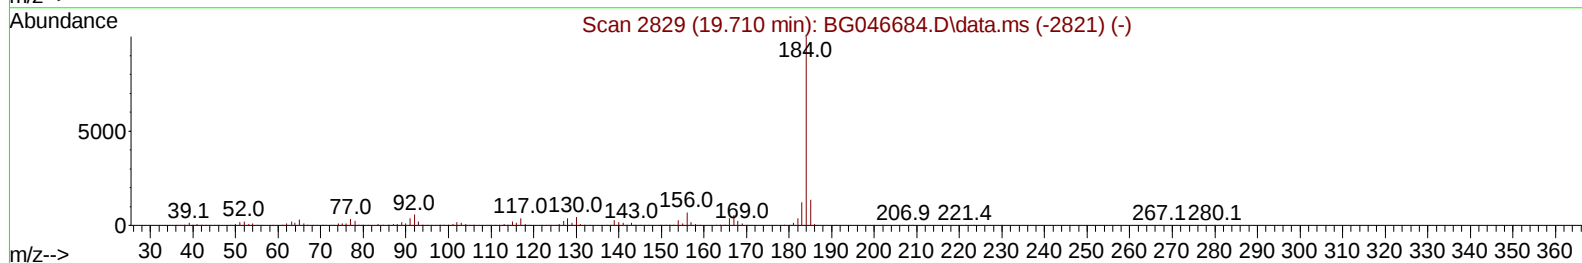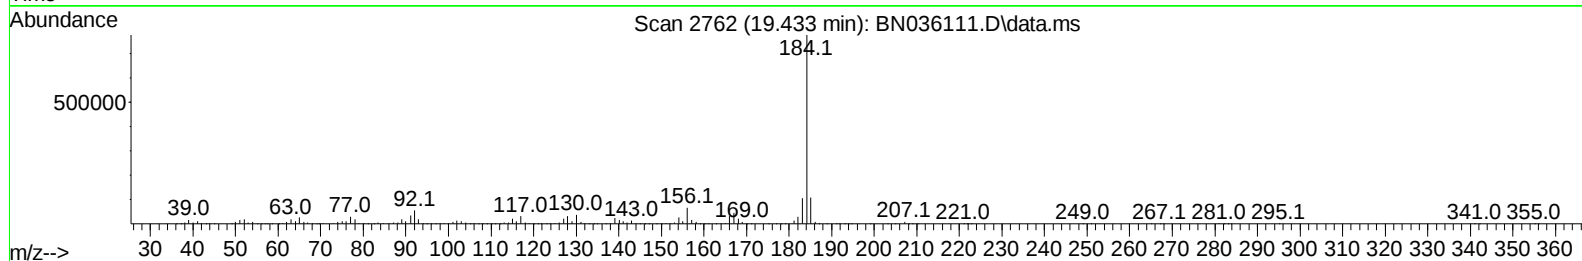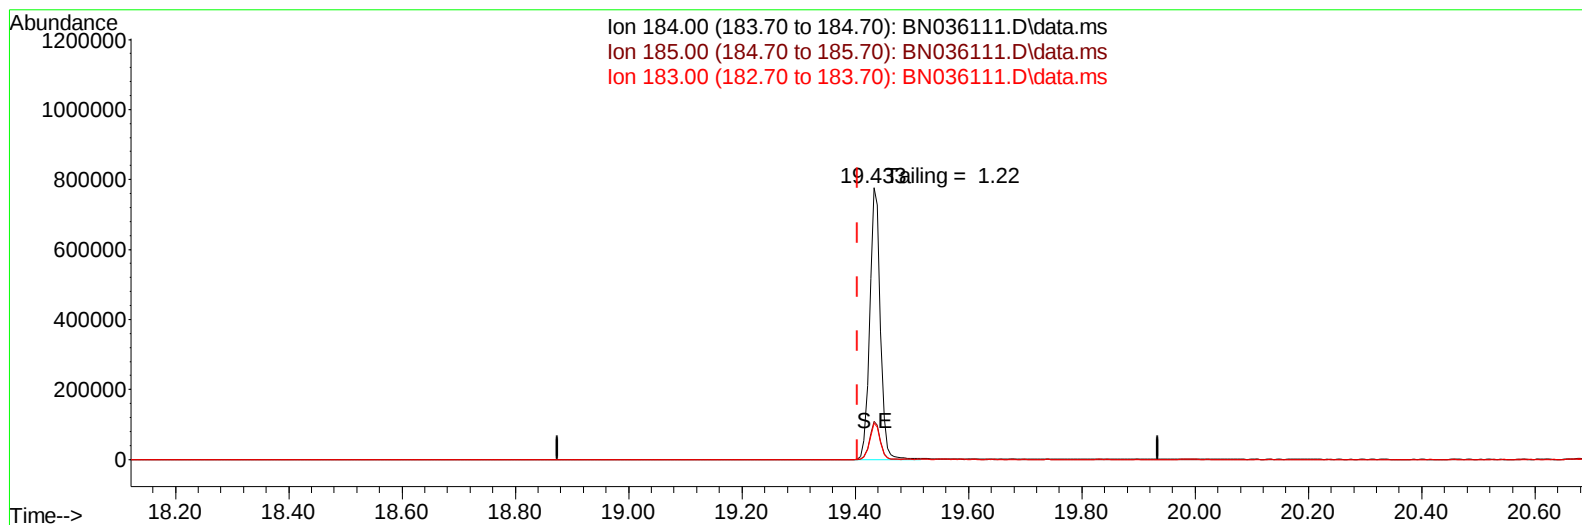

TIC: BN036111.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 611311.00 ng

response 1017570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	13.44
0.00	0.00	0.00