

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
 Data File : PL093735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2025 12:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 13:40:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 13:40:02 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.773	118.0E6	178.8E6	50.000	50.000
28) SA Decachlor...	9.053	7.909	91356144	160.3E6	50.000	50.000
Target Compounds						
23) Chlordane-1	4.700	3.771	55335446	61106259	500.000	500.000
24) Chlordane-2	5.229	4.347	55911116	70304921	500.000	500.000
25) Chlordane-3	5.939	4.977	183.8E6	213.9E6	500.000	500.000
26) Chlordane-4	6.021	5.039	220.6E6	206.1E6	500.000	500.000
27) Chlordane-5	6.870	5.935	42155882	74355315	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012125\
Data File : PL093735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2025 12:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 13:40:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 13:40:02 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

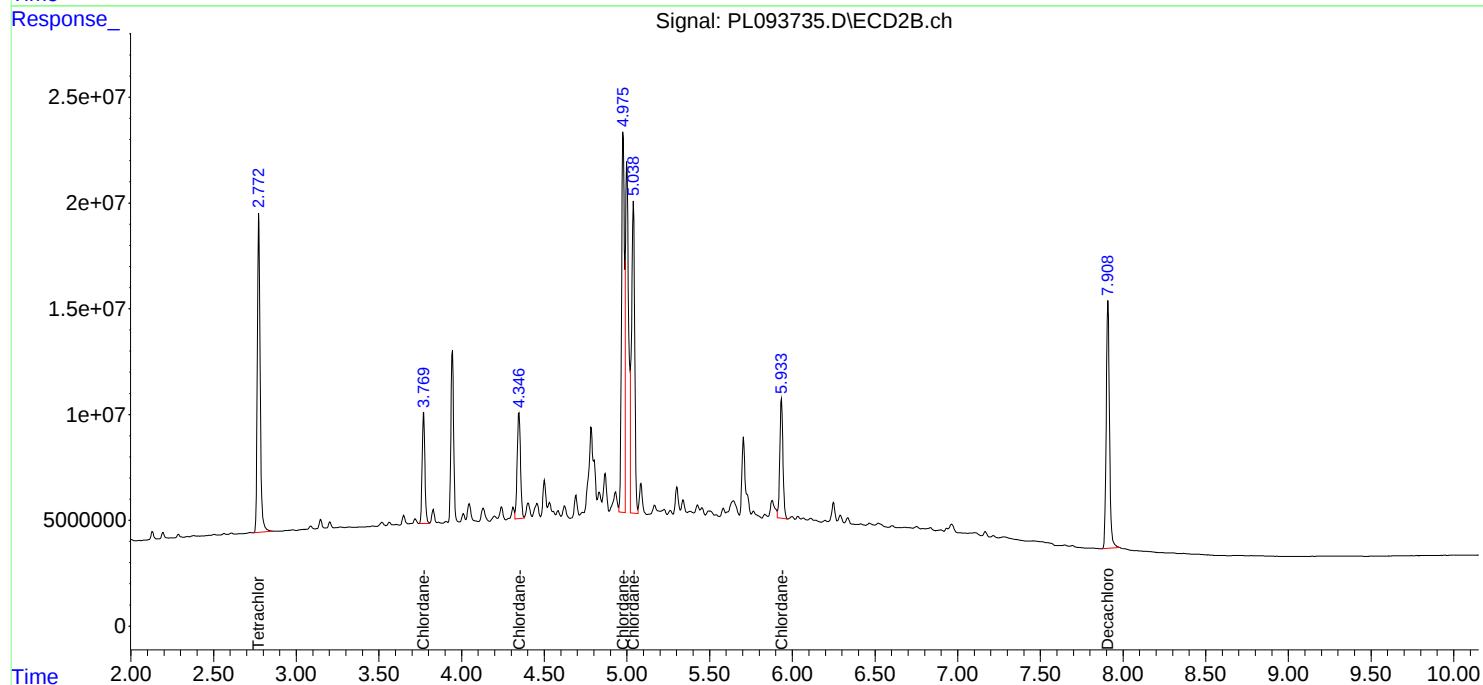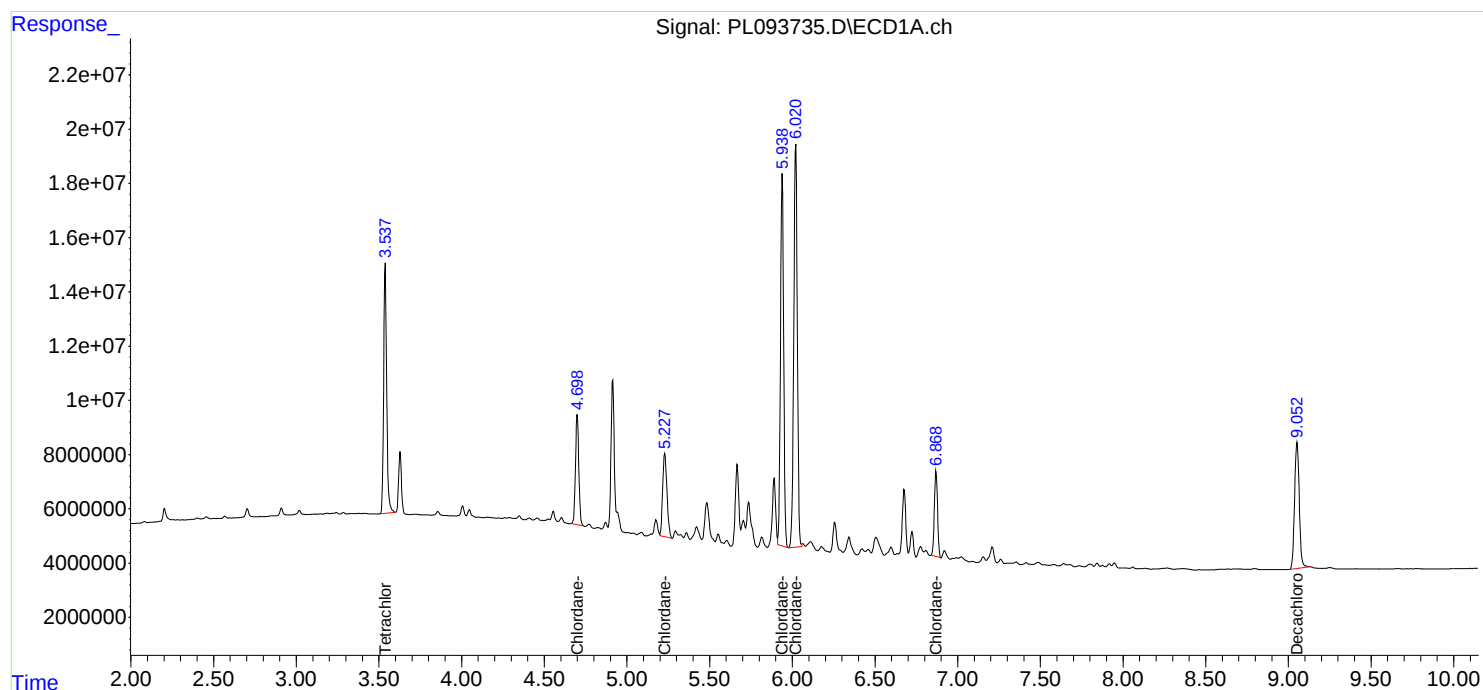


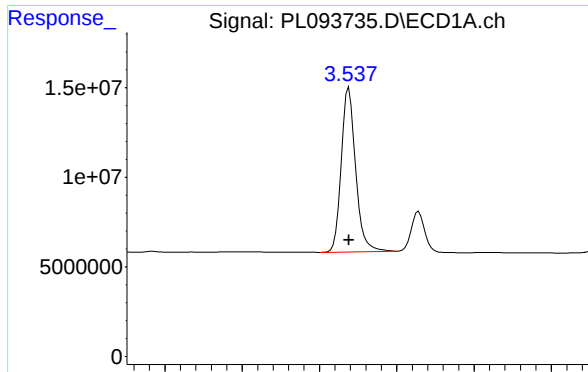

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 118044809
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

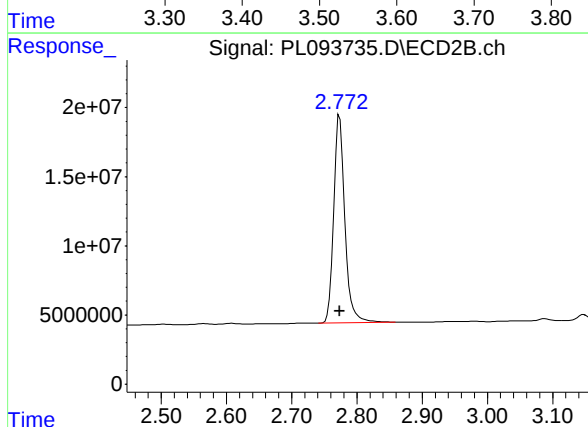


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 178786091
Conc: 50.00 ng/ml

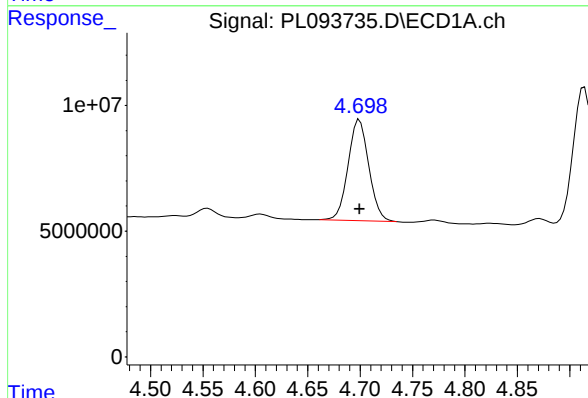


#23 Chlordane-1

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 55335446
Conc: 500.00 ng/ml

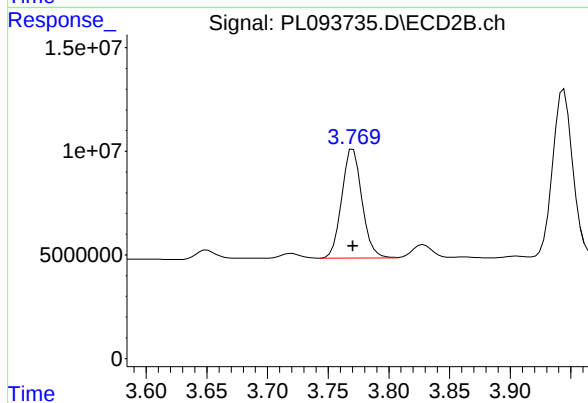

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 61106259
Conc: 500.00 ng/ml

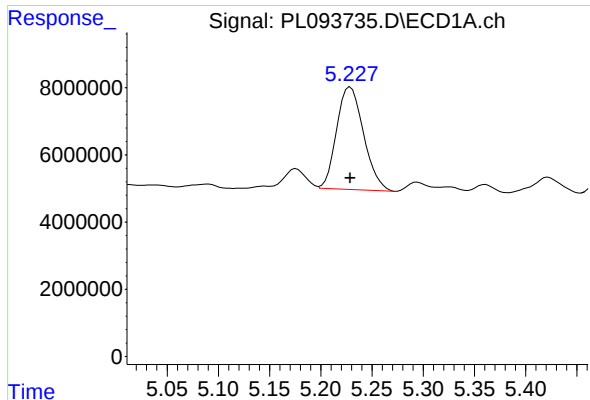

#24 Chlordane-2


R.T.: 5.229 min
Delta R.T.: 0.000 min
Response: 55911116
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

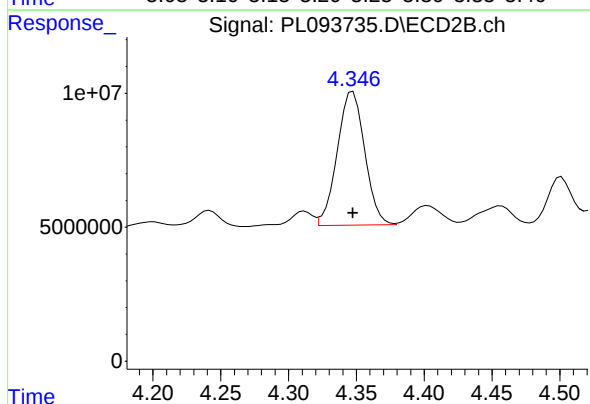


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 70304921
Conc: 500.00 ng/ml

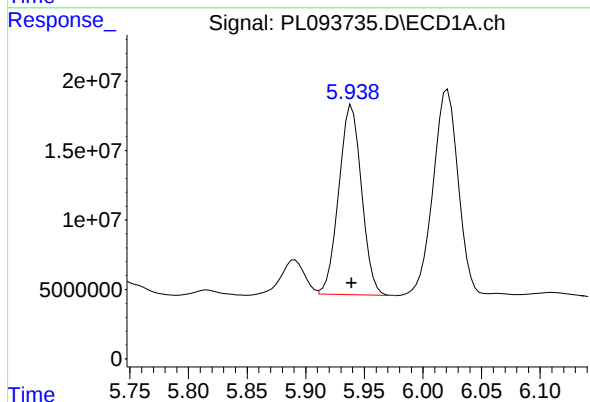


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 183782045
Conc: 500.00 ng/ml

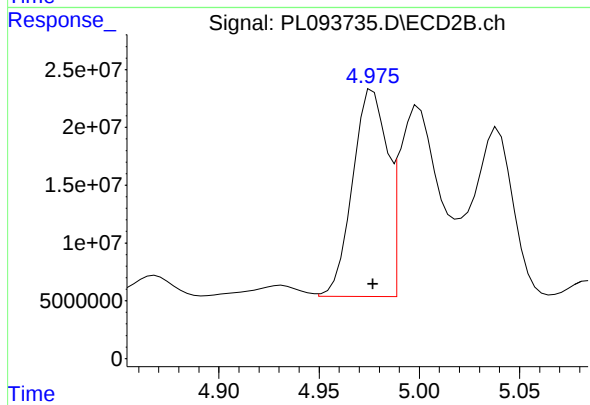

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 213941021
Conc: 500.00 ng/ml

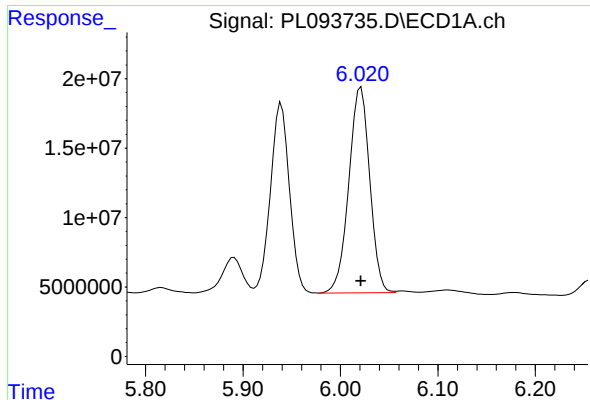

#26 Chlordane-4


R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 220583333
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

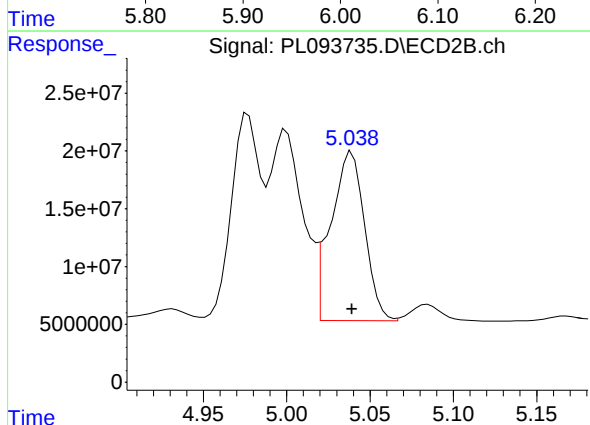


#26 Chlordane-4

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 206126766
Conc: 500.00 ng/ml

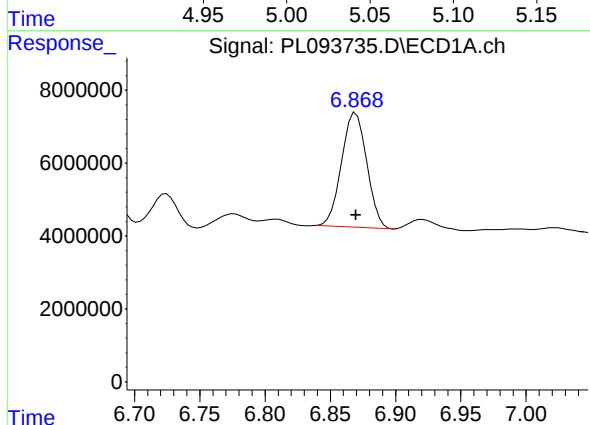


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 42155882
Conc: 500.00 ng/ml

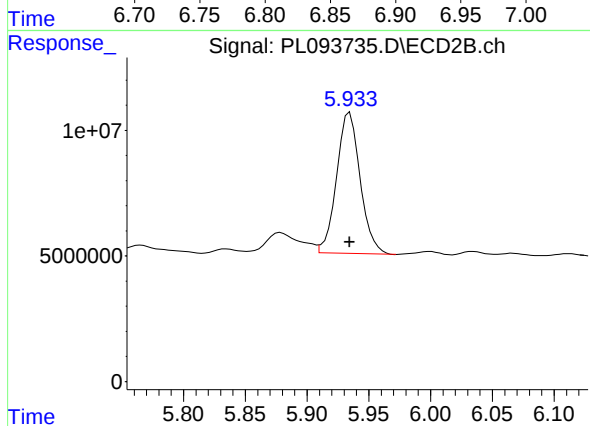

#27 Chlordane-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 74355315
Conc: 500.00 ng/ml

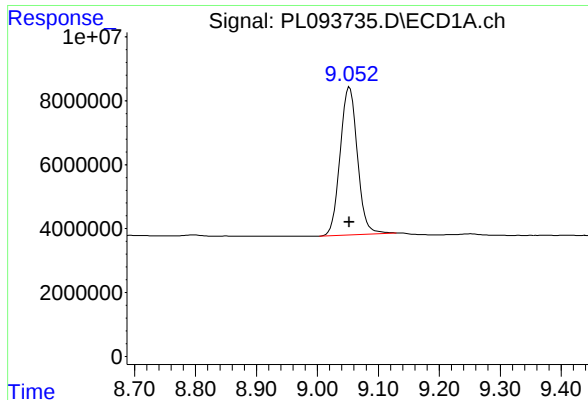

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 91356144
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

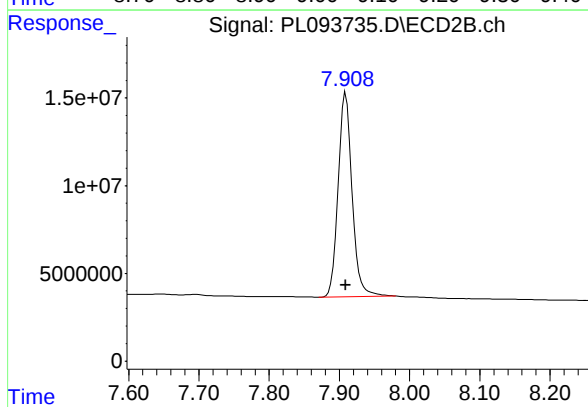

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 160259410
Conc: 50.00 ng/ml