

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
 Data File : BF141290.D
 Acq On : 29 Jan 2025 10:30
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC2.5

Quant Time: Jan 29 16:26:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 29 16:24:35 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.798	152	137039	20.000	ng	0.00
21) Naphthalene-d8	8.081	136	552749	20.000	ng	0.00
39) Acenaphthene-d10	9.833	164	301993	20.000	ng	0.00
64) Phenanthrene-d10	11.322	188	536934	20.000	ng	0.00
76) Chrysene-d12	13.963	240	311885	20.000	ng	0.00
86) Perylene-d12	15.427	264	276754	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0d	0.000	ng	
7) Phenol-d6	0.000	99	0d	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng	
79) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.198	70	18566	2.764	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141290.D
Acq On : 29 Jan 2025 10:30
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5

Quant Time: Jan 29 16:26:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 16:24:35 2025
Response via : Initial Calibration




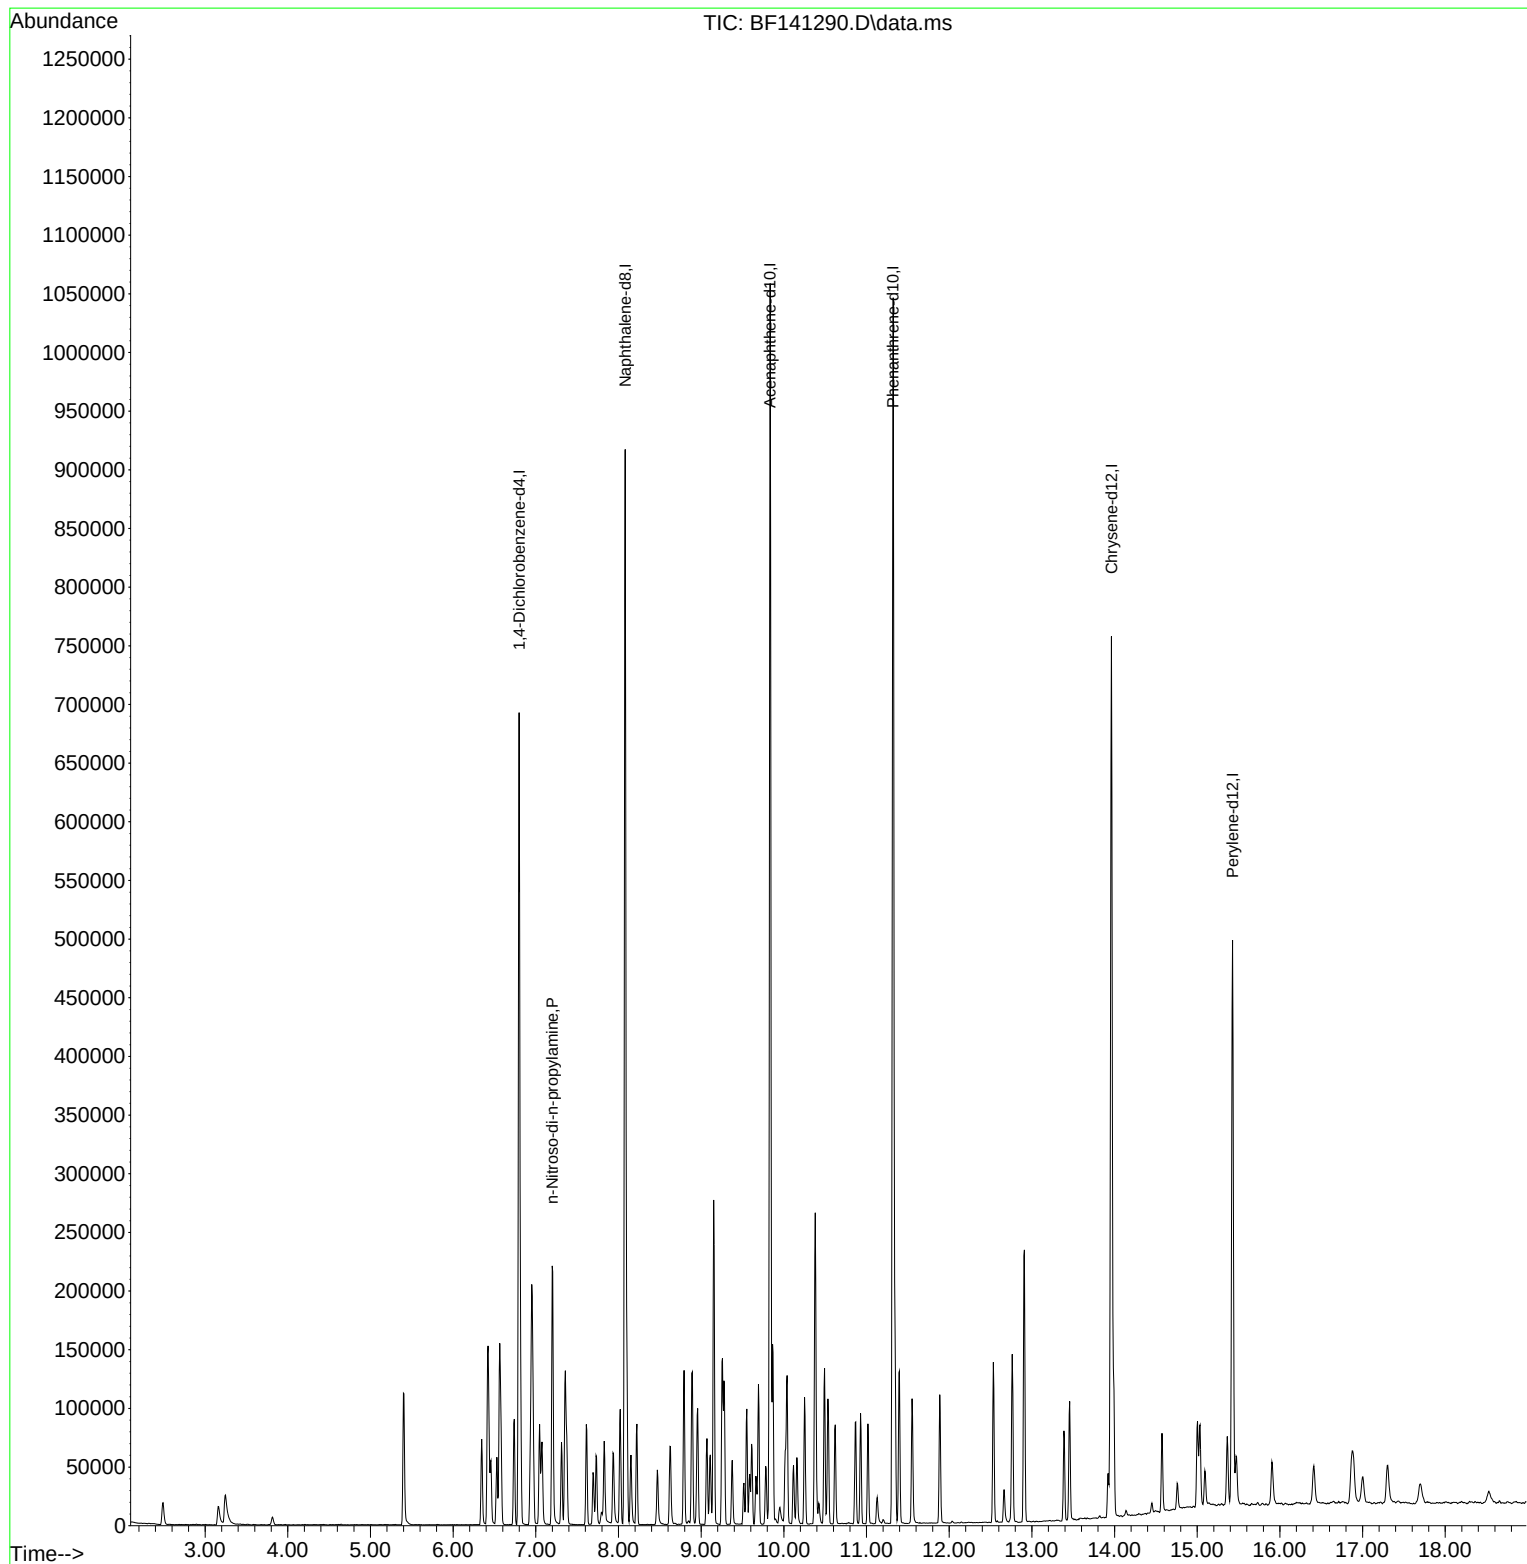


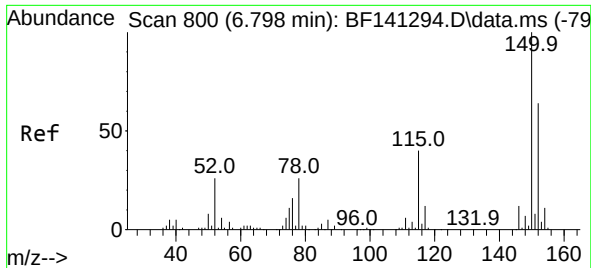

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.798 min Scan# 80
Delta R.T. 0.000 min
Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5


Tgt Ion:152 Resp: 137039
Ion Ratio Lower Upper
152 100
150 157.8 125.9 188.9
115 64.0 49.7 74.5

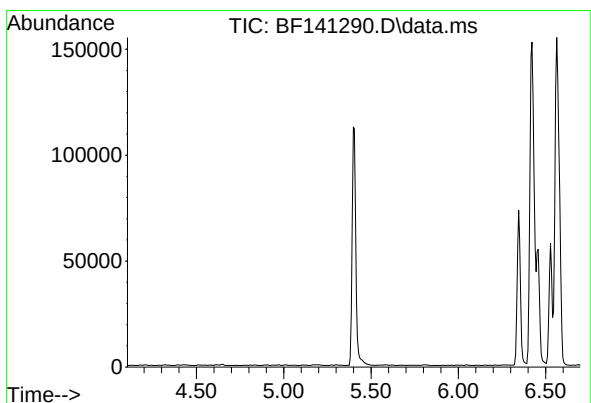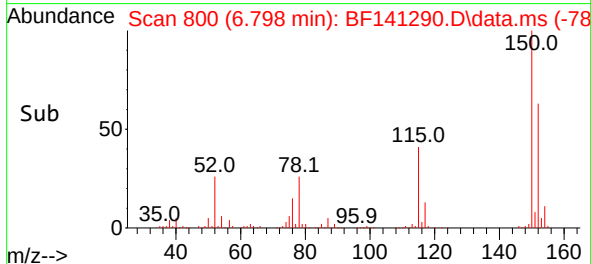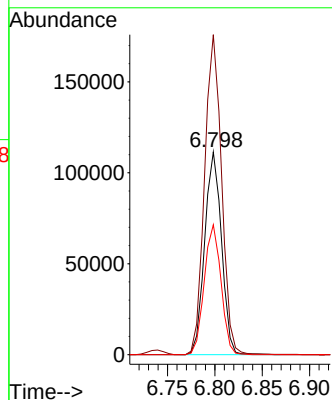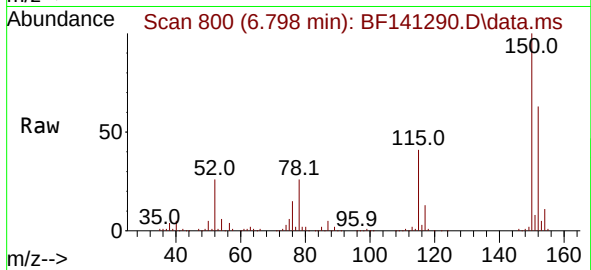


#5
2-Fluorophenol
Concen: 0.000 ng
Expected RT: 5.40 min

Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Tgt Ion: 112
Sig Exp Ratio
112 100
64 62.3
63 32.6

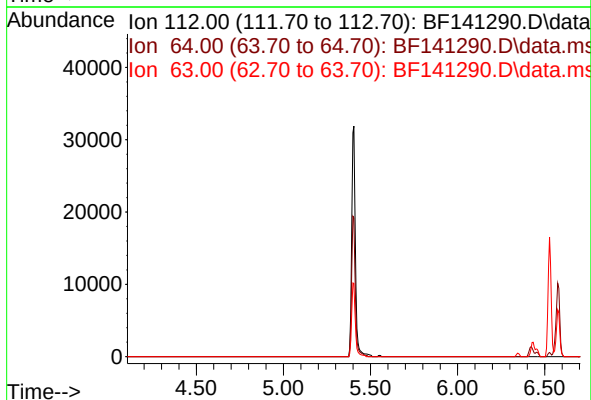


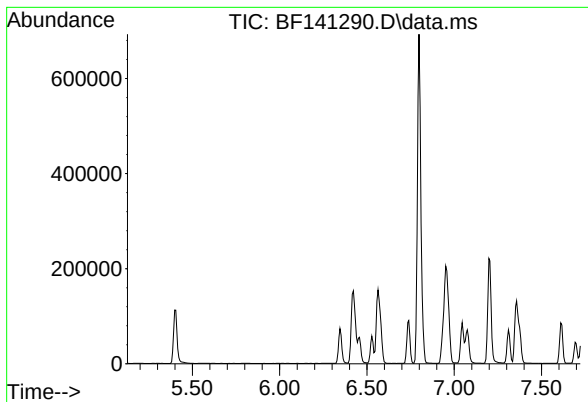


#7
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.43 min
 Lab File: BF141290.D
 Acq: 29 Jan 2025 10:30

Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC2.5

Tgt Ion: 99




Sig	Exp Ratio
99	100
42	21.4
71	33.6

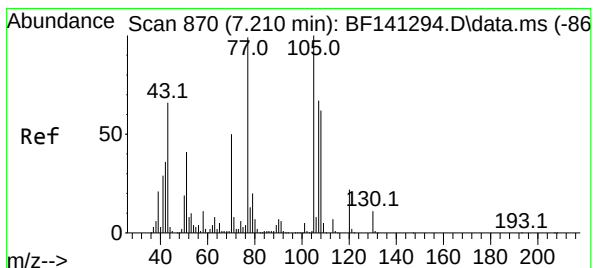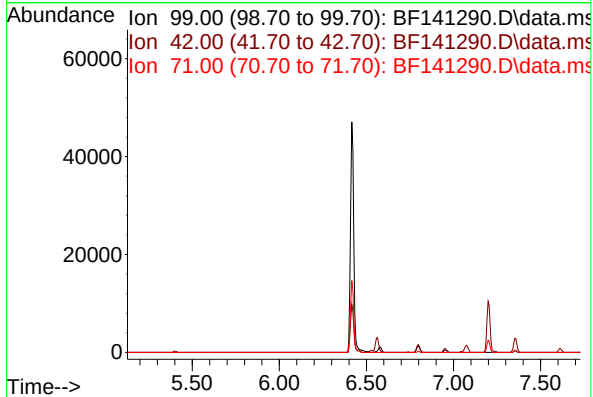


#19
 n-Nitroso-di-n-propylamine
 Concen: 2.764 ng
 RT: 7.198 min Scan# 868
 Delta R.T. -0.012 min
 Lab File: BF141290.D
 Acq: 29 Jan 2025 10:30

Tgt Ion: 70 Resp: 18566


Ion	Ratio	Lower	Upper
70	100		
42	71.6	56.8	85.2
101	9.0	7.7	11.5
130	20.1	16.8	25.2

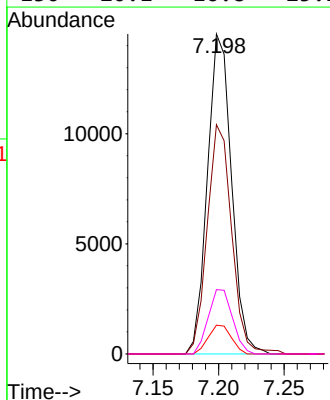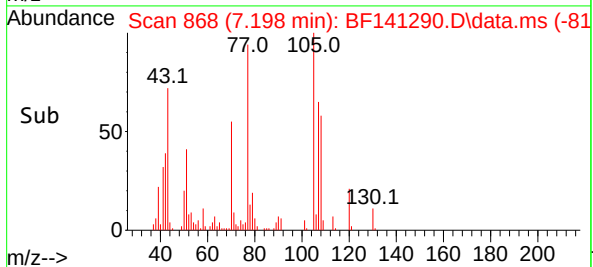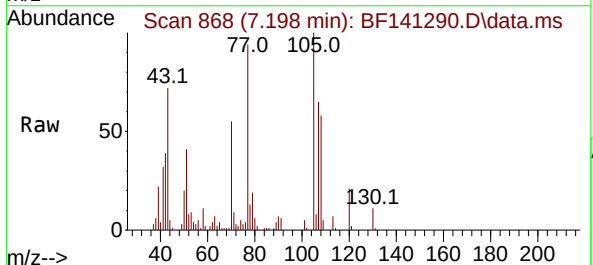



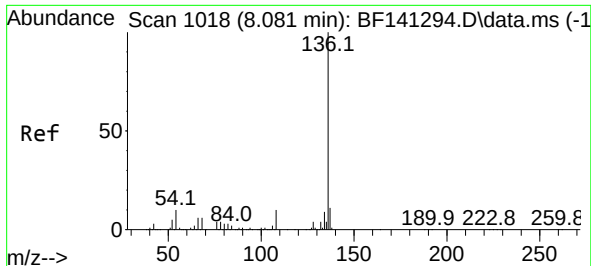


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1018
Delta R.T. 0.000 min
Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5

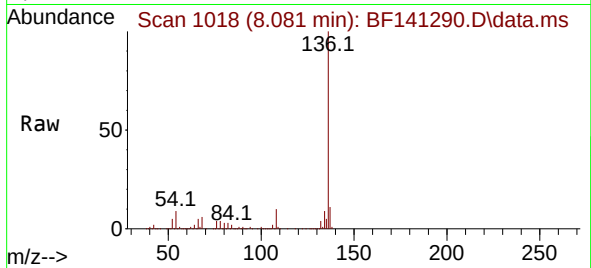


Tgt Ion:136 Resp: 552749
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 9.4 7.8 11.8
68 6.2 4.9 7.3

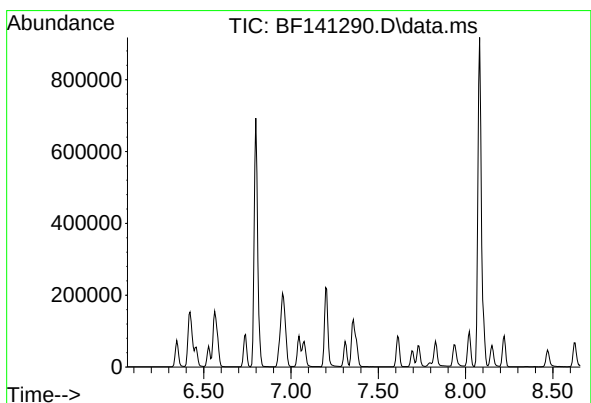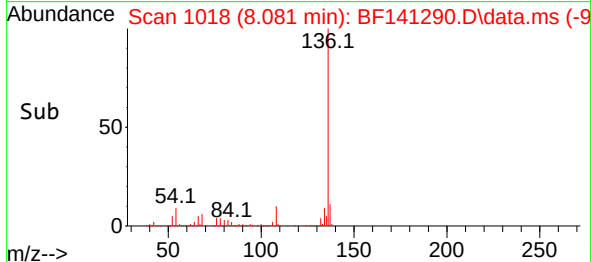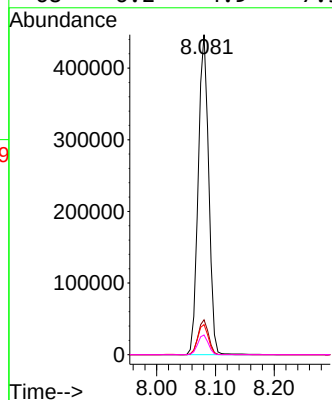


#23
Nitrobenzene-d5
Concen: 0.000 ng
Expected RT: 7.36 min

Lab File: BF141290.D
Acq: 29 Jan 2025 10:30


Tgt Ion: 82
Sig Exp Ratio
82 100
128 44.6
54 58.9

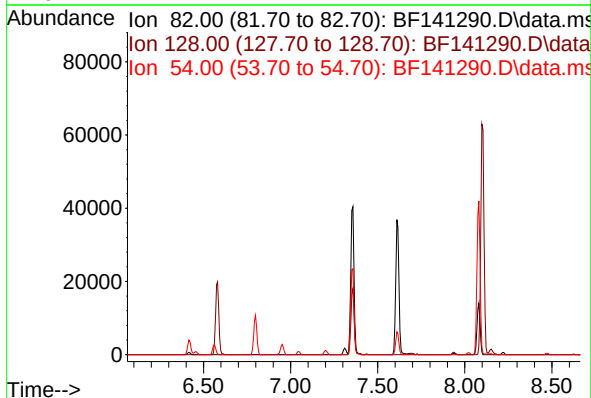



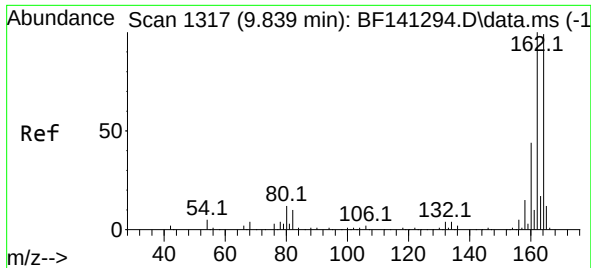


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.833 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5

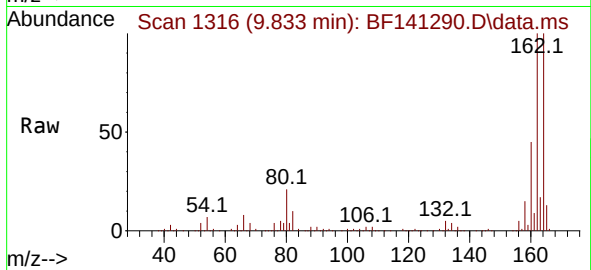


Tgt Ion:164 Resp: 301993
Ion Ratio Lower Upper
164 100
162 100.3 80.6 121.0
160 44.9 35.8 53.6

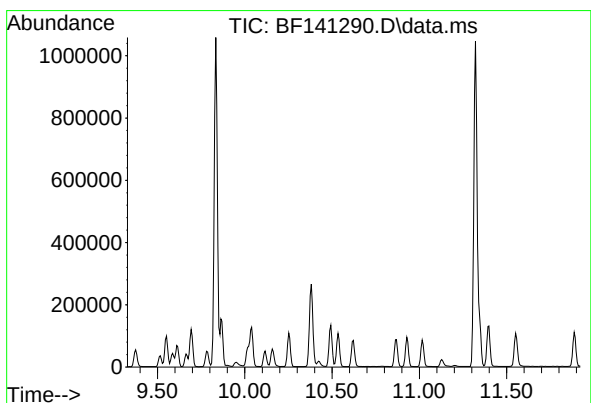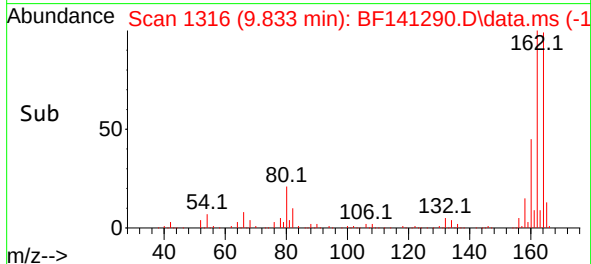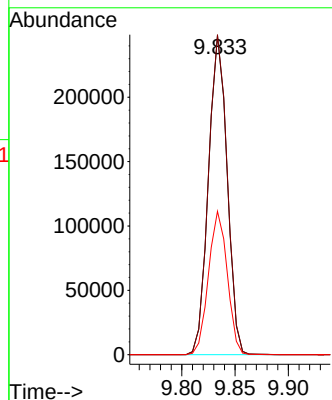


#42
2,4,6-Tribromophenol
Concen: 0.000 ng
Expected RT: 10.63 min

Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Tgt Ion: 330
Sig Exp Ratio
330 100
332 95.1
141 36.0


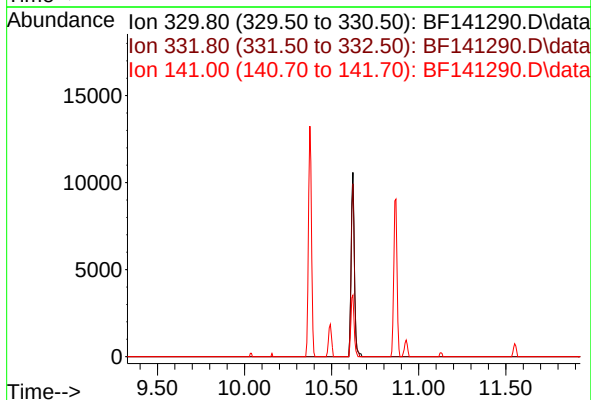


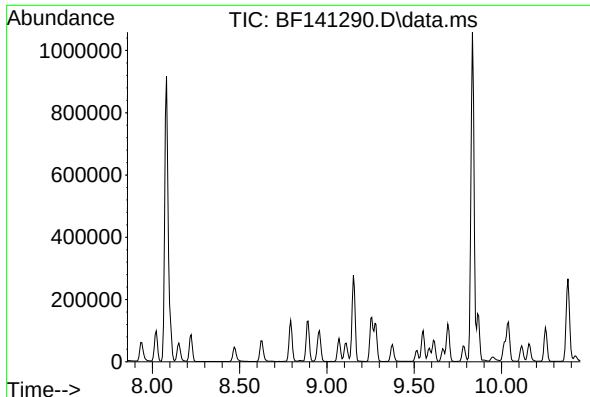

#45
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 9.16 min
 Lab File: BF141290.D
 Acq: 29 Jan 2025 10:30




Instrument :
 BNA_F
 ClientSampleId :
 SSTDICC2.5


Tgt Ion: 172
 Sig Exp Ratio
 172 100
 171 36.0
 170 23.8

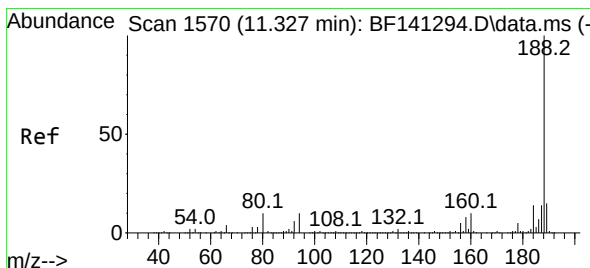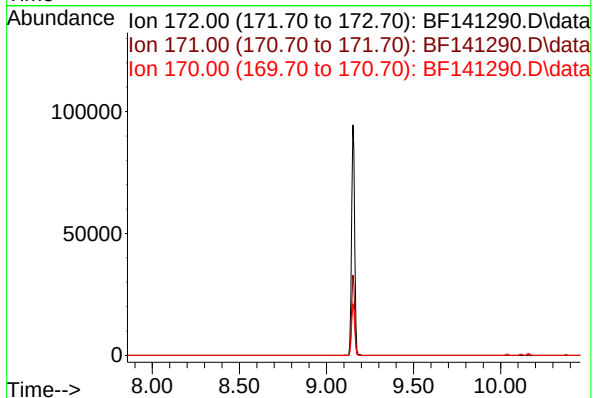

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.322 min Scan# 1569
 Delta R.T. -0.006 min
 Lab File: BF141290.D
 Acq: 29 Jan 2025 10:30

Tgt Ion: 188 Resp: 536934
 Ion Ratio Lower Upper
 188 100
 94 10.1 7.8 11.6
 80 10.6 8.2 12.4


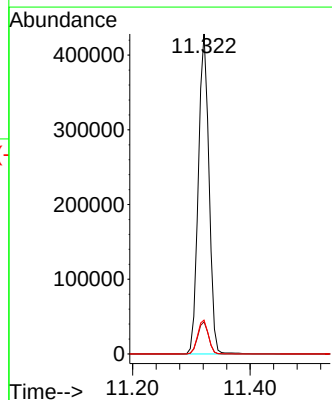
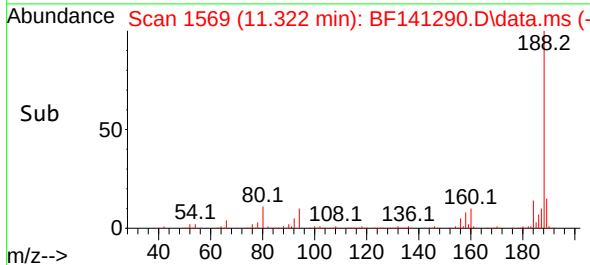
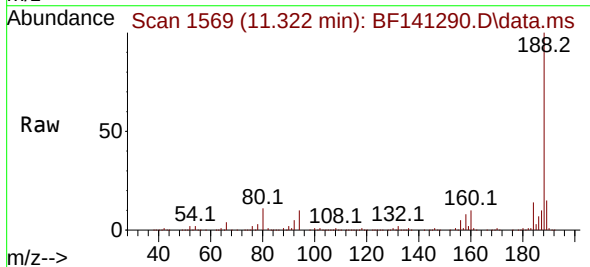


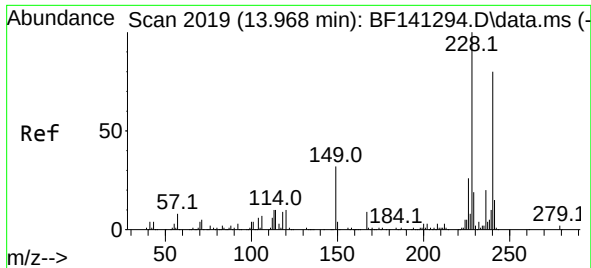

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 20
Delta R.T. -0.006 min
Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5


Tgt Ion:240 Resp: 311885
Ion Ratio Lower Upper
240 100
120 12.4 10.0 15.0
236 25.3 19.7 29.5

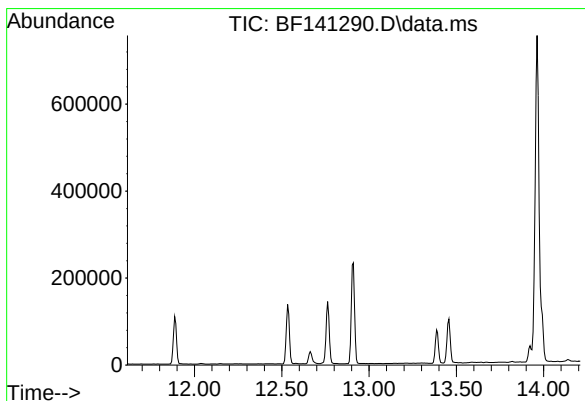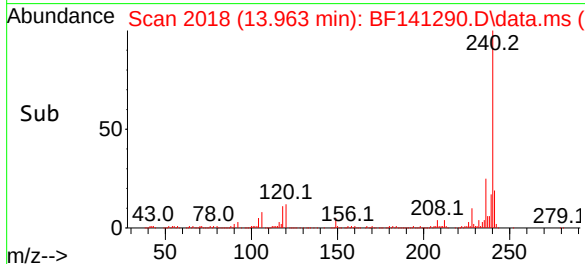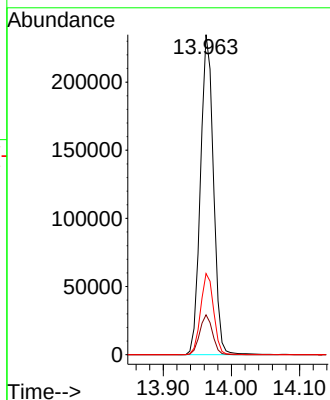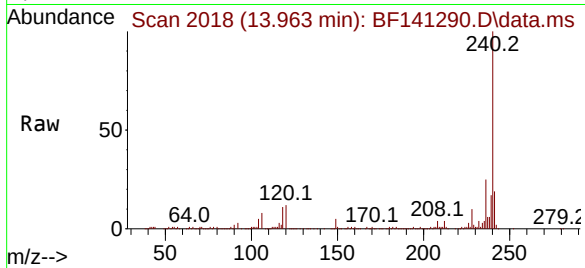


#79
Terphenyl-d14
Concen: 0.000 ng
Expected RT: 12.92 min

Lab File: BF141290.D
Acq: 29 Jan 2025 10:30


Tgt Ion: 244
Sig Exp Ratio
244 100
212 6.7
122 11.0

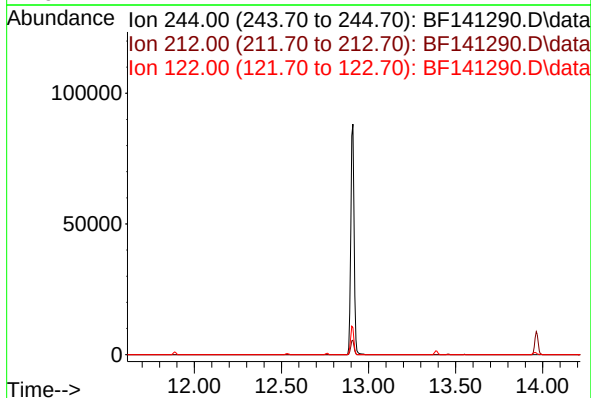

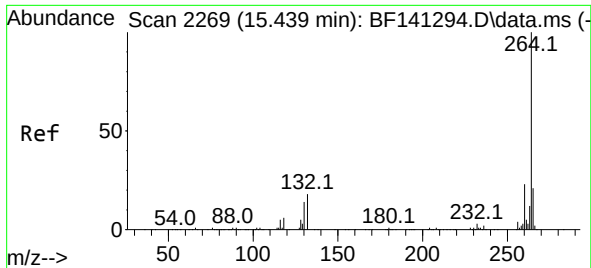

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.427 min Scan# 21
Delta R.T. -0.012 min
Lab File: BF141290.D
Acq: 29 Jan 2025 10:30

Instrument :
BNA_F
ClientSampleId :
SSTDICC2.5

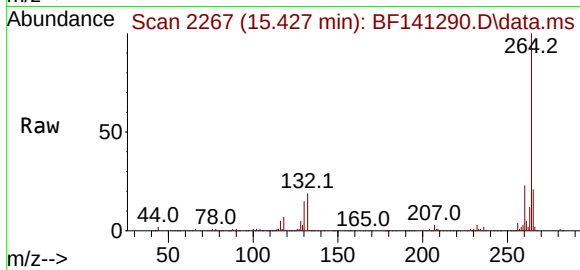

Tgt Ion:264 Resp: 276754

Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.6	27.8
265	21.2	16.7	25.1

