
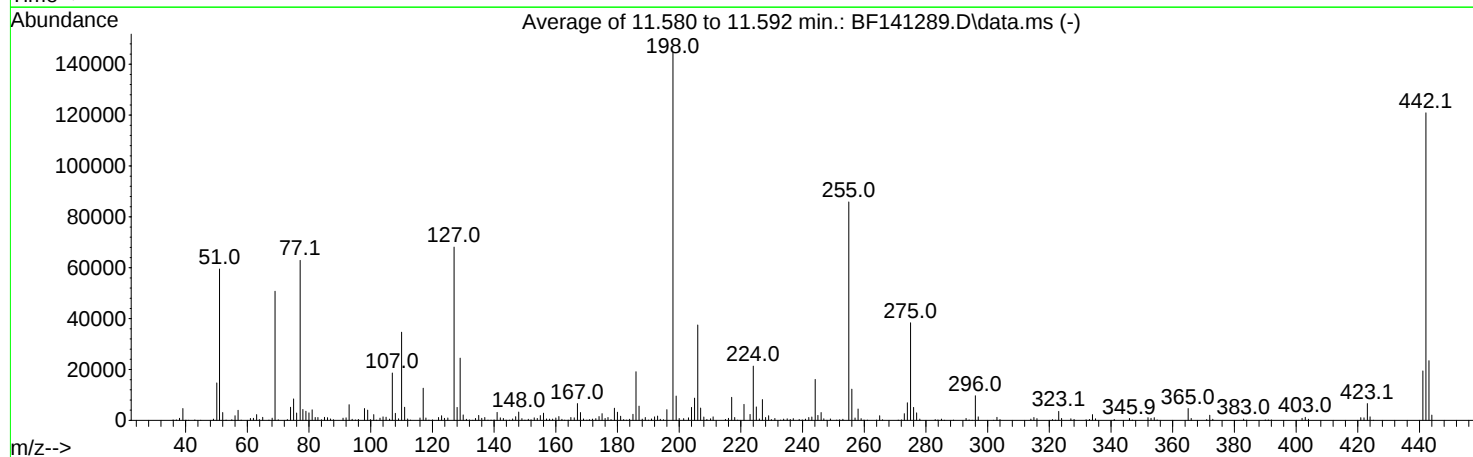


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141289.D
Acq On : 29 Jan 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

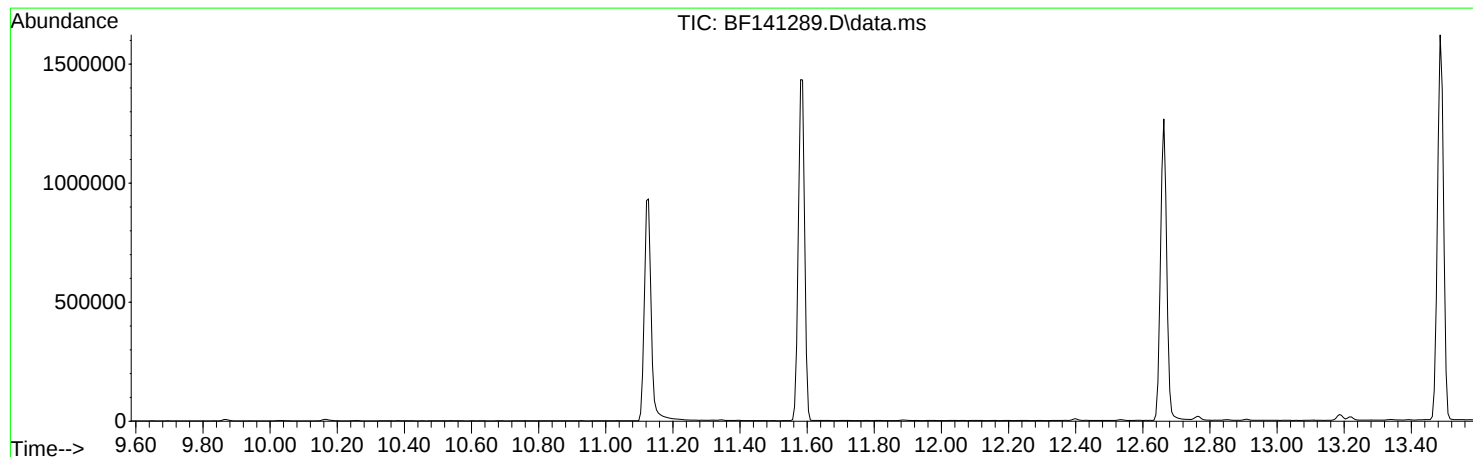




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	59504	PASS
68	69	0.00	2	1.7	874	PASS
69	198	0.00	100	35.1	50789	PASS
70	69	0.00	2	0.6	281	PASS
127	198	10	80	47.1	68133	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144613	PASS
199	198	5	9	6.6	9584	PASS
275	198	10	60	26.5	38371	PASS
365	198	1	100	3.2	4642	PASS
441	198	0.01	100	13.5	19467	PASS
442	442	50	100	100.0	120923	PASS
443	442	15	24	19.4	23456	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141289.D
Acq On : 29 Jan 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 29 13:18:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 13:12:40 2025
Response via : Initial Calibration

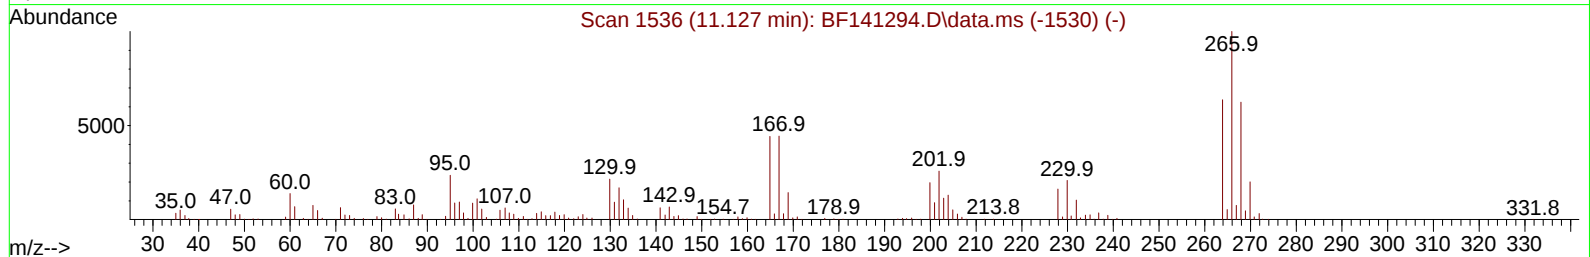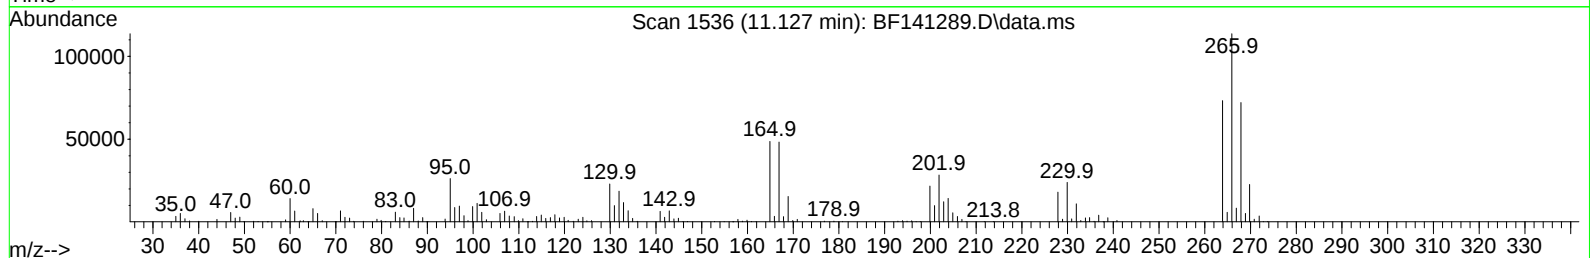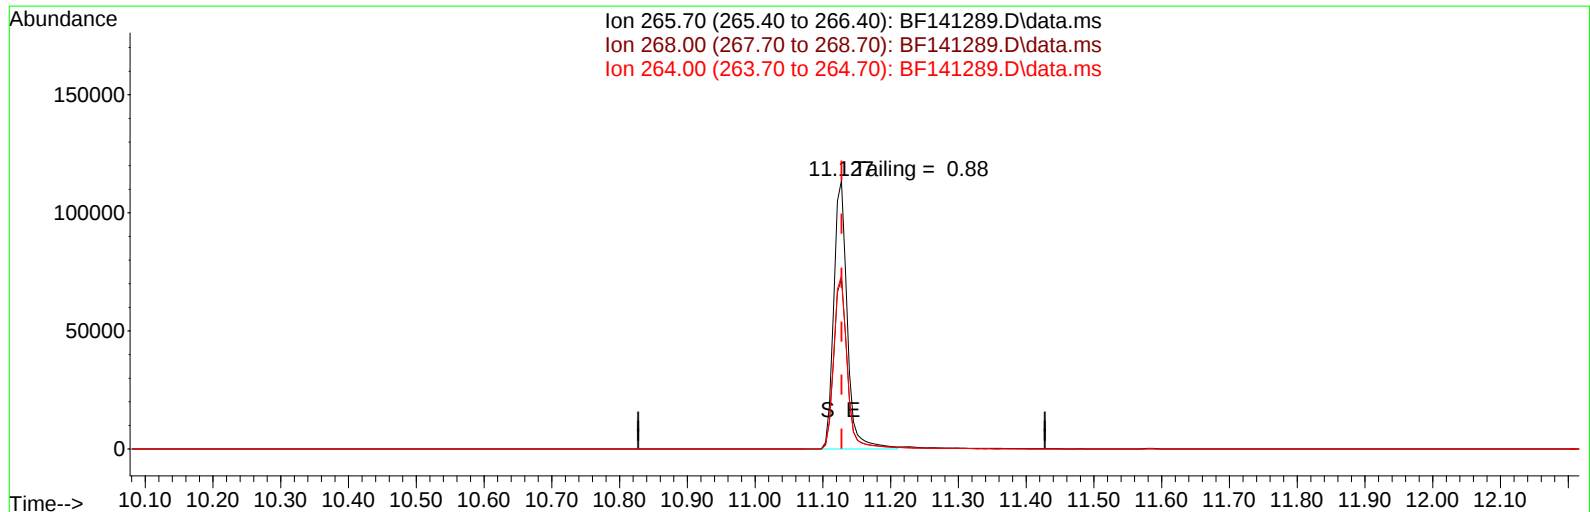

TIC: BF141289.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 18353.04 ng




response 157302

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.00	63.47
264.00	63.20	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141289.D
Acq On : 29 Jan 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 29 13:18:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 13:12:40 2025
Response via : Initial Calibration

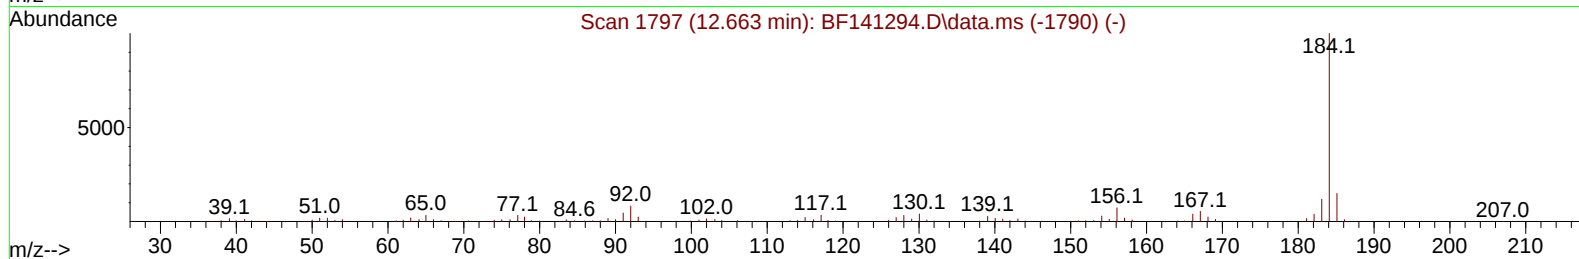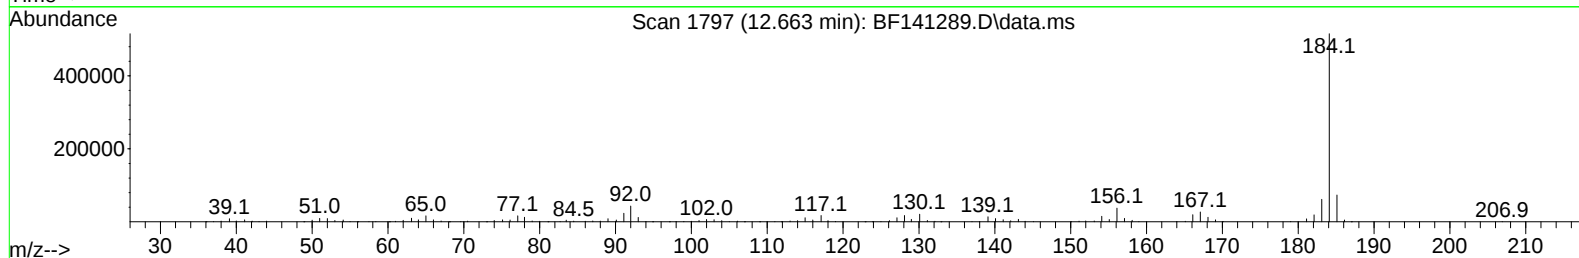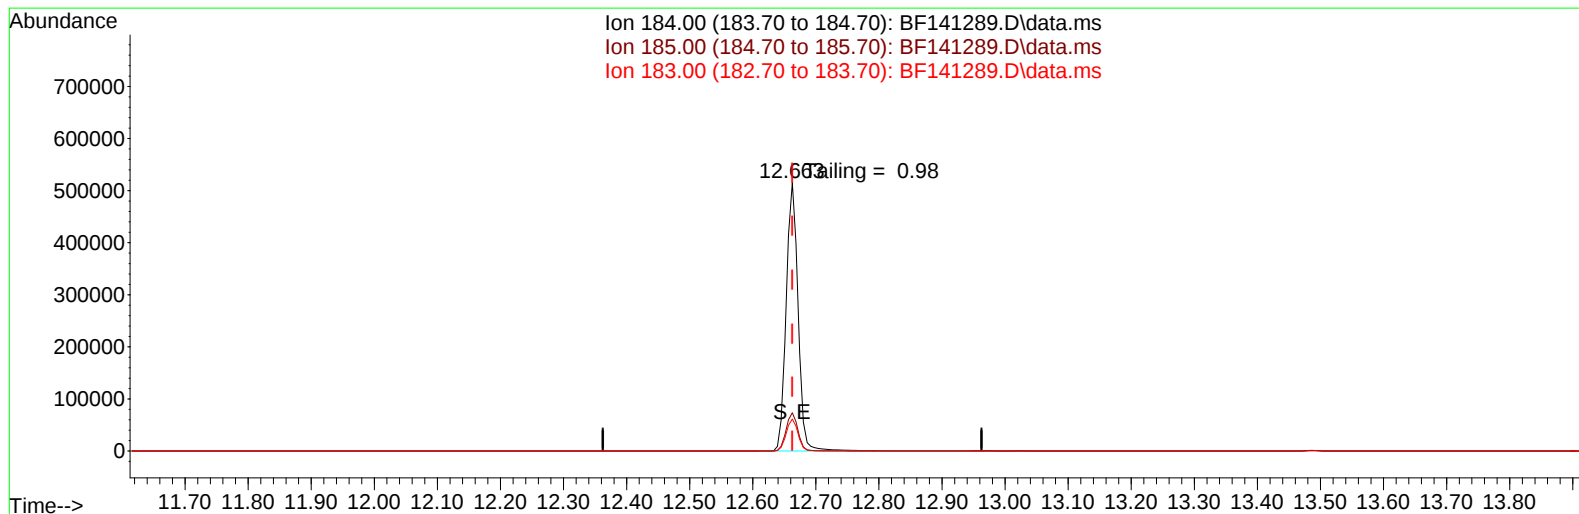

TIC: BF141289.D\data.ms

(77) Benzidine

12.663min (-0.000) 86413.53 ng

response 677498

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.27
183.00	11.70	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/29/2025	BNA_F	<u>BF141289.D</u>
Compound Name	Response	Retention Time
DDT	407437	13.486
DDD	11239	13.186
DDE	931	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12170	419607	2.90

Instrument :
BNA_F
ClientSampleId :
DFTPP