

DATA PACKAGE GENERAL CHEMISTRY

PROJECT NAME : FT MEADE TIPTON AIRFIELD PARCEL RI - PO 0111169

WESTON SOLUTIONS

1400 Weston Way

PO Box 2653

West Chester, PA - 19380

Phone No: 610-701-7400

ORDER ID : Q1211

ATTENTION : Nathan Fretz



Laboratory Certification ID # 20012



1) GENERAL CHEMISTRY DATA	2
2) Signature Page	3
3) Case Narrative	4
4) Qualifier Page	6
5) Conformance/Non Conformance	7
6) QA Checklist	8
7) Chronicle	9
8) Sample Data	10
8.1) TAPHHA-MW01-012825-00-T4	11
8.2) TAPHHA-MW01-012825-00-T4DL	12
8.3) TAPIAL2-MW03-012825-00-T3	13
9) QC Data Summary For Genchem	14
9.1) Initial and Continuing Calibration Verification	15
9.2) Initial and Continuing Calibration Blank Summary	19
9.3) Preparation Blank Summary	23
9.4) Matrix Spike Summary	24
9.5) Duplicate Sample Summary	28
9.6) Laboratory Control Sample Summary	31
10) GENCHEM RAW DATA	36
10.1) GENCHEM RAW DATA - ANALYTICAL	37
10.1.1) LB134464	37
10.1.2) LB134466	49
10.1.3) LB134473	51
10.1.4) LB134521	82
10.1.5) LB134532	85
10.2) GENCHEM RAW DATA - PREP	88
10.2.1) PB166477	88
11) Analytical Runlogs	91
12) Standard Prep Logs	100
13) Shipping Document	190
13.1) Chain Of Custody	191
13.2) Lab Certificate	192
13.3) Internal COC	193

Cover Page

Order ID : Q1211

Project ID : Ft Meade Tipton Airfield Parcel RI - PO 0111169

Client : Weston Solutions

Lab Sample Number

Q1211-01
Q1211-02
Q1211-03

Client Sample Number

TAPHHA-MW01-012825-00-T4
TAPIAL2-MW03-012825-00-T3
TAP-TB-02-012825-T4

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 2/4/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

Weston Solutions

Project Name: Ft Meade Tipton Airfield Parcel RI - PO 0111169

Project # N/A

Chemtech Project # Q1211

Test Name: Hexavalent Chromium, Oil and Grease, Anions Group5, TOC, Ammonia

A. Number of Samples and Date of Receipt:

3 Water samples were received on 01/29/2025.

B. Parameters:

According to the Chain of Custody document, the following analyses were requested: Ammonia, Anions Group5, Diesel Range Organics, Gasoline Range Organics, Hardness, Total, Hexavalent Chromium, Mercury, Metals ICP-TAL, METALS-TAL, Oil and Grease, PESTICIDE Group1, SVOC-TCL BNA -20, TOC and VOC-TCLVOA-10. This data package contains results for Hexavalent Chromium, Oil and Grease, Anions Group5, TOC, Ammonia.

C. Analytical Techniques:

The analysis of Oil and Grease was based on method 1664A, The analysis of Hexavalent Chromium was based on method 7196A, The analysis of Anions Group5 was based on method 9056A, The analysis of TOC was based on method 9060A and The analysis of Ammonia was based on method SM4500-NH3.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

Sample TAPHHA-MW01-012825-00-T4 was diluted due to high concentrations for Chloride.

The Blank Spike met requirements for all samples.

The Duplicate analysis met criteria for all samples.

The Matrix Spike analysis met criteria for all samples.

The Matrix Spike Duplicate analysis met criteria for all samples.

The Blank analysis did not indicate the presence of lab contamination.

The Calibration met the requirements.

E. Additional Comments:

As per method 1664A, MS/MSD is required to be performed with the sample analysis. However, Lab did not receive sufficient volume to perform the MS/MSD for Q1211, therefore Lab reported MS-MSD from Q1252.



I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

DATA REPORTING QUALIFIERS- INORGANIC

For reporting results, the following “ Results Qualifiers” are used:

J	Indicates the reported value was obtained from a reading that was less than the Contract Required Detection Limit (CRDL), but greater than or equal to the Instrument Detection Limit (IDL).
U	Indicates the analyte was analyzed for, but not detected.
ND	Indicates the analyte was analyzed for, but not detected
E	Indicates the reported value is estimated because of the presence of interference
M	Indicates Duplicate injection precision not met.
N	Indicates the spiked sample recovery is not within control limits.
S	Indicates the reported value was determined by the Method of Standard Addition (MSA).
*	Indicates that the duplicate analysis is not within control limits.
+	Indicates the correlation coefficient for the MSA is less than 0.995.
D	Indicates the reported value is from a secondary analysis with a dilution factor. The original analysis exceeded the calibration range.
M	Method qualifiers “P” for ICP instrument “PM” for ICP when Microwave Digestion is used “CV” for Manual Cold Vapor AA “AV” for automated Cold Vapor AA “CA” for MIDI-Distillation Spectrophotometric “AS” for Semi -Automated Spectrophotometric “C” for Manual Spectrophotometric “T” for Titrimetric “NR” for analyte not required to be analyzed
OR	Indicates the analyte’s concentration exceeds the calibrated range of the instrument for that specific analysis.
Q	Indicates the LCS did not meet the control limits requirements
H	Sample Analysis Out Of Hold Time

GENERAL CHEMISTRY CONFORMANCE/NON-CONFORMANCE SUMMARY

CHEMTECH PROJECT NUMBER: Q1211

MATRIX: Water

METHOD: 1664A,7196A,9056A,9060A,SM4500-NH3

	NA	NO	YES
1. Blank Contamination - If yes, list compounds and concentrations in each blank:		✓	
2. Matrix Spike Duplicate Recoveries Met Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable range.			
The Blank Spike met requirements for all samples.			
3. Sample Duplicate Analysis Met QC Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable range.			
4. Digestion Holding Time Met			✓
If not met, list number of days exceeded for each sample:			

ADDITIONAL COMMENTS:

As per method 1664A, MS/MSD is required to be performed with the sample analysis. However, Lab did not receive sufficient volume to perform the MS/MSD for Q1211, therefore Lab reported MS-MSD from Q1252.

QA REVIEW

Date

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q1211

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: SOHIL JODHANI

Date: 02/04/2025

LAB CHRONICLE

OrderID:	Q1211	OrderDate:	1/29/2025 10:10:00 AM
Client:	Weston Solutions	Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169
Contact:	Nathan Fretz	Location:	N31,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1211-01	TAPHHA-MW01-01282 5-00-T4	WATER			01/28/25 12:00			01/29/25
			Ammonia	SM4500-NH3		02/03/25	02/03/25 13:39	
			Anions Group5	9056A			01/29/25 12:41	
			Hexavalent Chromium	7196A			01/29/25 14:45	
			Oil and Grease	1664A			02/01/25 11:30	
			TOC	9060A			01/29/25 14:30	
Q1211-01DL	TAPHHA-MW01-01282 5-00-T4DL	WATER			01/28/25 12:00			01/29/25
			Anions Group5	9056A			01/29/25 14:07	
Q1211-02	TAPIAL2-MW03-0128 25-00-T3	WATER			01/28/25 14:55			01/29/25
			Ammonia	SM4500-NH3		02/03/25	02/03/25 13:50	
			Anions Group5	9056A			01/29/25 13:46	
			Hexavalent Chromium	7196A			01/29/25 14:49	
			Oil and Grease	1664A			02/01/25 11:30	
			TOC	9060A			01/29/25 15:47	



SAMPLE DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

Report of Analysis

Client:	Weston Solutions	Date Collected:	01/28/25 12:00
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Date Received:	01/29/25
Client Sample ID:	TAPHHA-MW01-012825-00-T4	SDG No.:	Q1211
Lab Sample ID:	Q1211-01	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Ammonia as N	0.080	U	1	0.045	0.080	0.10	mg/L	02/03/25 08:50	02/03/25 13:39	SM 4500-NH3 B plus G-11
Bromide	1.00	U	1	0.034	1.00	2.00	mg/L		01/29/25 12:41	9056A
Chloride	17.8	OR	1	0.011	0.30	0.60	mg/L		01/29/25 12:41	9056A
Fluoride	0.070	J	1	0.057	0.20	0.40	mg/L		01/29/25 12:41	9056A
Nitrite	0.30	U	1	0.011	0.30	0.60	mg/L		01/29/25 12:41	9056A
Nitrate	0.69		1	0.0034	0.25	0.50	mg/L		01/29/25 12:41	9056A
Sulfate	25.3		1	0.032	1.50	3.00	mg/L		01/29/25 12:41	9056A
Dissolved Hexavalent Chromium	0.0050	U	1	0.0030	0.0050	0.010	mg/L		01/29/25 14:45	7196A
Oil and Grease	2.00	U	1	0.40	2.00	5.00	mg/L		02/01/25 11:30	1664A
TOC	0.91	J	1	0.19	0.50	1.00	mg/L		01/29/25 14:30	9060A

Comments:

U = Not Detected
LOQ = Limit of Quantitation
MDL = Method Detection Limit
LOD = Limit of Detection
D = Dilution
Q = indicates LCS control criteria did not meet requirements
H = Sample Analysis Out Of Hold Time

J = Estimated Value
B = Analyte Found in Associated Method Blank
* = indicates the duplicate analysis is not within control limits.
E = Indicates the reported value is estimated because of the presence of interference.
OR = Over Range
N = Spiked sample recovery not within control limits

Report of Analysis

Client:	Weston Solutions	Date Collected:	01/28/25 12:00
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Date Received:	01/29/25
Client Sample ID:	TAPHHA-MW01-012825-00-T4DL	SDG No.:	Q1211
Lab Sample ID:	Q1211-01DL	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	16.7	D	5	0.055	1.50	3.00	mg/L		01/29/25 14:07	9056A

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

Report of Analysis

Client:	Weston Solutions	Date Collected:	01/28/25 14:55
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Date Received:	01/29/25
Client Sample ID:	TAPIAL2-MW03-012825-00-T3	SDG No.:	Q1211
Lab Sample ID:	Q1211-02	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Ammonia as N	0.40		1	0.045	0.080	0.10	mg/L	02/03/25 08:50	02/03/25 13:50	SM 4500-NH3 B plus G-11
Bromide	1.00	U	1	0.034	1.00	2.00	mg/L		01/29/25 13:46	9056A
Chloride	3.10		1	0.011	0.30	0.60	mg/L		01/29/25 13:46	9056A
Fluoride	0.076	J	1	0.057	0.20	0.40	mg/L		01/29/25 13:46	9056A
Nitrite	0.30	U	1	0.011	0.30	0.60	mg/L		01/29/25 13:46	9056A
Nitrate	0.25	U	1	0.0034	0.25	0.50	mg/L		01/29/25 13:46	9056A
Sulfate	30.7		1	0.032	1.50	3.00	mg/L		01/29/25 13:46	9056A
Dissolved Hexavalent Chromium	0.0050	U	1	0.0030	0.0050	0.010	mg/L		01/29/25 14:49	7196A
Oil and Grease	2.00	U	1	0.40	2.00	5.00	mg/L		02/01/25 11:30	1664A
TOC	7.30		1	0.19	0.50	1.00	mg/L		01/29/25 15:47	9060A

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

QC RESULT SUMMARY

Initial and Continuing Calibration Verification

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

RunNo.: LB134464

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: ICV1 TOC	mg/L	10.4	10	104	90-110	01/15/2025
Sample ID: CCV1 TOC	mg/L	9.8	10	98	90-110	01/29/2025
Sample ID: CCV2 TOC	mg/L	10.1	10	101	90-110	01/29/2025

Initial and Continuing Calibration Verification

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

RunNo.: LB134466

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: ICV Hexavalent Chromium	mg/L	0.503	0.5	101	90-110	01/29/2025
Sample ID: CCV1 Hexavalent Chromium	mg/L	0.499	0.5	100	90-110	01/29/2025
Sample ID: CCV2 Hexavalent Chromium	mg/L	0.504	0.5	101	90-110	01/29/2025

Initial and Continuing Calibration Verification

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

RunNo.: LB134473

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: ICV1						
Bromide	mg/L	10.3	10	103	90-110	01/20/2025
Chloride	mg/L	3.1	3	103	90-110	01/20/2025
Fluoride	mg/L	2.1	2	105	90-110	01/20/2025
Nitrite	mg/L	3.1	3	103	90-110	01/20/2025
Nitrate	mg/L	2.6	2.5	104	90-110	01/20/2025
Sulfate	mg/L	15.4	15	103	90-110	01/20/2025
Orthophosphate as P	mg/L	5.2	5	104	90-110	01/20/2025
Sample ID: CCV1						
Bromide	mg/L	9.9	10	99	90-110	01/29/2025
Chloride	mg/L	3	3	100	90-110	01/29/2025
Fluoride	mg/L	2	2	100	90-110	01/29/2025
Nitrite	mg/L	3	3	100	90-110	01/29/2025
Nitrate	mg/L	2.5	2.5	100	90-110	01/29/2025
Sulfate	mg/L	14.7	15	98	90-110	01/29/2025
Orthophosphate as P	mg/L	4.9	5	98	90-110	01/29/2025
Sample ID: CCV2						
Bromide	mg/L	10	10	100	90-110	01/29/2025
Chloride	mg/L	3	3	100	90-110	01/29/2025
Fluoride	mg/L	2	2	100	90-110	01/29/2025
Nitrite	mg/L	3	3	100	90-110	01/29/2025
Nitrate	mg/L	2.5	2.5	100	90-110	01/29/2025
Sulfate	mg/L	14.8	15	99	90-110	01/29/2025
Orthophosphate as P	mg/L	5	5	100	90-110	01/29/2025

Initial and Continuing Calibration Verification

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

RunNo.: LB134532

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: ICV1 Ammonia as N	mg/L	0.99	1	99	90-110	02/03/2025
Sample ID: CCV1 Ammonia as N	mg/L	0.94	1	94	90-110	02/03/2025
Sample ID: CCV2 Ammonia as N	mg/L	0.97	1	97	90-110	02/03/2025
Sample ID: CCV3 Ammonia as N	mg/L	0.95	1	95	90-110	02/03/2025
Sample ID: CCV4 Ammonia as N	mg/L	0.99	1	99	90-110	02/03/2025

Initial and Continuing Calibration Blank Summary

Client: Weston Solutions	SDG No.: Q1211
Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169	RunNo.: LB134464

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: ICB1 TOC	mg/L	0.2	0.5000	J	0.19	1	01/15/2025
Sample ID: CCB1 TOC	mg/L	0.26	0.5000	J	0.19	1	01/29/2025
Sample ID: CCB2 TOC	mg/L	0.26	0.5000	J	0.19	1	01/29/2025

Initial and Continuing Calibration Blank Summary

Client: Weston Solutions	SDG No.: Q1211
Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169	RunNo.: LB134466

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: ICB Hexavalent Chromium	mg/L	< 0.0050	0.0050	U	0.0027	0.01	01/29/2025
Sample ID: CCB1 Hexavalent Chromium	mg/L	< 0.0050	0.0050	U	0.0027	0.01	01/29/2025
Sample ID: CCB2 Hexavalent Chromium	mg/L	< 0.0050	0.0050	U	0.0027	0.01	01/29/2025

Initial and Continuing Calibration Blank Summary

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

RunNo.: LB134473

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: ICB1							
Bromide	mg/L	< 1.0000	1.0000	U	0.034	2	01/20/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/20/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.057	0.4	01/20/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/20/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.0034	0.5	01/20/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.032	3	01/20/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.079	1	01/20/2025
Sample ID: CCB1							
Bromide	mg/L	< 1.0000	1.0000	U	0.034	2	01/29/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.057	0.4	01/29/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.0034	0.5	01/29/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.032	3	01/29/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.079	1	01/29/2025
Sample ID: CCB2							
Bromide	mg/L	< 1.0000	1.0000	U	0.034	2	01/29/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.057	0.4	01/29/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.0034	0.5	01/29/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.032	3	01/29/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.079	1	01/29/2025

Initial and Continuing Calibration Blank Summary

Client: Weston Solutions	SDG No.: Q1211
Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169	RunNo.: LB134532

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: ICB1 Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025
Sample ID: CCB1 Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025
Sample ID: CCB2 Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025
Sample ID: CCB3 Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025
Sample ID: CCB4 Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025

Preparation Blank Summary

Client: Weston Solutions

SDG No.: Q1211

Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: LB134464BLW							
TOC	mg/L	0.26	0.5000	J	0.19	1	01/29/2025
Sample ID: lb134466BL							
Hexavalent Chromium	mg/L	< 0.0050	0.0050	U	0.003	0.01	01/29/2025
Sample ID: LB134473BLW							
Bromide	mg/L	< 1.0000	1.0000	U	0.034	2	01/29/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.057	0.4	01/29/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.011	0.6	01/29/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.0034	0.5	01/29/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.032	3	01/29/2025
Orthophosphate as P	mg/L	0.16	0.5000	J	0.079	1	01/29/2025
Sample ID: LB134521BL							
Oil and Grease	mg/L	< 2.5000	2.5000	U	0.4	5.0	02/01/2025
Sample ID: PB166477BL							
Ammonia as N	mg/L	< 0.0500	0.0500	U	0.045	0.1	02/03/2025

Matrix Spike Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1211-01
Client ID:	TAPHHA-MW01-012825-00-T4MS	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Ammonia as N	mg/L	75-125	1.10		0.045	U	1	1	110		02/03/2025
TOC	mg/L	75-125	10.4		0.91	J	10	1	95		01/29/2025
Hexavalent Chromium	mg/L	90-111	1.01		0.0030	U	1.0	2	101		01/29/2025
Bromide	mg/L	80-120	10.7		0.034	U	10	1	107		01/29/2025
Chloride	mg/L	80-120	20.6	OR	17.8	OR	3	1	93		01/29/2025
Fluoride	mg/L	80-120	2.20		0.070	J	2	1	107		01/29/2025
Nitrite	mg/L	80-120	3.20		0.011	U	3	1	107		01/29/2025
Nitrate	mg/L	80-120	3.30		0.69		2.5	1	104		01/29/2025
Sulfate	mg/L	80-120	40.8	OR	25.3		15	1	103		01/29/2025
Orthophosphate as P	mg/L	80-120	5.40		0.079	U	5	1	108		01/29/2025

Matrix Spike Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1211-01
Client ID:	TAPHHA-MW01-012825-00-T4MSD	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Ammonia as N	mg/L	75-125	1.10		0.045	U	1	1	110		02/03/2025
TOC	mg/L	75-125	10.2		0.91	J	10	1	93		01/29/2025
Hexavalent Chromium	mg/L	90-111	1.00		0.0030	U	1.0	2	100		01/29/2025
Bromide	mg/L	80-120	10.7		0.034	U	10	1	107		01/29/2025
Chloride	mg/L	80-120	20.6	OR	17.8	OR	3	1	93		01/29/2025
Fluoride	mg/L	80-120	2.20		0.070	J	2	1	107		01/29/2025
Nitrite	mg/L	80-120	3.20		0.011	U	3	1	107		01/29/2025
Nitrate	mg/L	80-120	3.30		0.69		2.5	1	104		01/29/2025
Sulfate	mg/L	80-120	40.9	OR	25.3		15	1	104		01/29/2025
Orthophosphate as P	mg/L	80-120	5.40		0.079	U	5	1	108		01/29/2025

Matrix Spike Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1252-01
Client ID:	EFFLUENTMS	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Oil and Grease	mg/L	78-114	31.9		12.0		20.0	1	100		02/01/2025

Matrix Spike Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1252-01
Client ID:	EFFLUENTMSD	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Oil and Grease	mg/L	78-114	32.2		12.0		20.0	1	101		02/01/2025

Duplicate Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1211-01
Client ID:	TPHHA-MW01-012825-00-T4DUP	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/AD	Qual	Analysis Date
Hexavalent Chromium	mg/L	+/-20	0.0030	U	0.0030	U	1	0		01/29/2025
Ammonia as N	mg/L	+/-20	0.045	U	0.045	U	1	0		02/03/2025

Duplicate Sample Summary

Client: Weston Solutions	SDG No.: Q1211
Project: Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID: Q1211-01
Client ID: TAPHHA-MW01-012825-00-T4MSD	Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/AD	Qual	Analysis Date
TOC	mg/L	+/-20	10.4		10.2		1	2		01/29/2025
Hexavalent Chromium	mg/L	+/-20	1.01		1.00		2	1		01/29/2025
Bromide	mg/L	+/-15	10.7		10.7		1	0		01/29/2025
Fluoride	mg/L	+/-15	2.20		2.20		1	0		01/29/2025
Nitrate	mg/L	+/-15	3.30		3.30		1	0		01/29/2025
Nitrite	mg/L	+/-15	3.20		3.20		1	0		01/29/2025
Orthophosphate as P	mg/L	+/-15	5.40		5.40		1	0		01/29/2025
Chloride	mg/L	+/-15	20.6	OR	20.6	OR	1	0		01/29/2025
Sulfate	mg/L	+/-15	40.8	OR	40.9	OR	1	0		01/29/2025
Ammonia as N	mg/L	+/-20	1.10		1.10		1	0		02/03/2025

Duplicate Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Sample ID:	Q1252-01
Client ID:	EFFLUENTMSD	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/AD	Qual	Analysis Date
Oil and Grease	mg/L	+/-18	31.9		32.2		1	0.94		02/01/2025

Laboratory Control Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Run No.:	LB134464

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	LB134464BSW							
TOC	mg/L	10	9.80		98	1	90-110	01/29/2025

Laboratory Control Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Run No.:	LB134466

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	lb134466BS							
Hexavalent Chromium	mg/L	0.5	0.51		102	1	90-111	01/29/2025

Laboratory Control Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Run No.:	LB134473

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	LB134473BSW							
Bromide	mg/L	10	9.90		99	1	90-110	01/29/2025
Chloride	mg/L	3	3.00		100	1	90-110	01/29/2025
Fluoride	mg/L	2	2.00		100	1	90-110	01/29/2025
Nitrite	mg/L	3	3.00		100	1	90-110	01/29/2025
Nitrate	mg/L	2.5	2.50		100	1	90-110	01/29/2025
Sulfate	mg/L	15	14.7		98	1	90-110	01/29/2025
Orthophosphate as P	mg/L	5	5.00		100	1	90-110	01/29/2025

Laboratory Control Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Run No.:	LB134521

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	LB134521BS							
Oil and Grease	mg/L	20.0	16.9		84	1	78-114	02/01/2025

Laboratory Control Sample Summary

Client:	Weston Solutions	SDG No.:	Q1211
Project:	Ft Meade Tipton Airfield Parcel RI - PO 0111169	Run No.:	LB134532

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	PB166477BS							
Ammonia as N	mg/L	1	0.97		97	1	90-110	02/03/2025



RAW DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

Sample ID	Result	Std. Dev.	RSD	Mode	ALT
CCV1	9.8484	0.1107	1.12	TOC	
CCB1	0.2595	0.0267	10.31	TOC	
LB134464BLW	0.2551	0.0472	18.49	TOC	
LB134464BSW.....	9.8044...	0.2674..	2.73...	TOC	..
Q1168-12	0.6055	0.0694	11.47	TOC	
Q1211-01	0.9104	0.1178	12.94	TOC	
Q1211-01MS.....	10.3715...	0.2208..	2.13...	TOC	..
Q1211-01MSD	10.1824	0.1057	1.04	TOC	
Q1211-02	7.2891	0.2899	3.98	TOC	
CCV2.....	10.0641...	0.1130..	1.12...	TOC	..
CCB2	0.2558	0.0563	22.02	TOC	

1

2

3

4

5

6

7

8

9

10

11

12

13

Method ID	Sample Type	Vial	Timestamp	Message
TOC 0 - 20 ppmC	Sample	11	2025/01/29 11:41	
TOC 0 - 20 ppmC	Sample	12	2025/01/29 12:05	Low Sample Detected
TOC 0 - 20 ppmC	Sample	13	2025/01/29 12:52	Low Sample Detected
TOC 0 - 20 ppmC	...Sample	.. 14..	2025/01/29 13:18	..
TOC 0 - 20 ppmC	Sample	16	2025/01/29 14:06	
TOC 0 - 20 ppmC	Sample	17	2025/01/29 14:30	
TOC 0 - 20 ppmC	...Sample	.. 18..	2025/01/29 14:55	..
TOC 0 - 20 ppmC	Sample	18	2025/01/29 15:20	
TOC 0 - 20 ppmC	Sample	19	2025/01/29 15:47	
TOC 0 - 20 ppmC	...Sample	.. 11..	2025/01/29 16:13	..
TOC 0 - 20 ppmC	Sample	13	2025/01/29 16:36	Low Sample Detected

1
2
3
4
5
6
7
8
9
10
11
12
13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

Sample ID: Q1168-12 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 14:06
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	0.5673	0.2836	22966	-2.534	-2.336	130
2	0.5435	0.2717	22002	-2.547	-2.350	130
3	0.7011	0.3506	28386	-2.596	-2.398	109
4	0.6101	0.3050	24698	-2.571	-2.371	127
<<<Statistics>>> Mean: 0.6055 Std Dev: 0.0694 RSD: 11.47						

Sample ID: Q1211-01 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 14:30
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	1.0551	0.5276	42716	-2.567	-2.369	135
2	0.9511	0.4755	38505	-2.548	-2.348	133
3	0.7872	0.3936	31869	-2.508	-2.309	121
4	0.8484	0.4242	34348	-2.520	-2.322	123
<<<Statistics>>> Mean: 0.9104 Std Dev: 0.1178 RSD: 12.94						

Sample ID: Q1211-01MS Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 14:55
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	10.5279	5.2640	426224	-2.499	-2.300	154
2	10.4070	5.2035	421329	-2.478	-2.279	153
3	10.0496	5.0248	406857	-2.484	-2.285	134
4	10.5017	5.2508	425161	-2.472	-2.278	153
<<<Statistics>>> Mean: 10.3715 Std Dev: 0.2208 RSD: 2.13						

Sample ID: Q1211-01MSD Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 15:20
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	10.2494	5.1247	414948	-2.448	-2.248	141
2	10.0427	5.0213	406577	-2.406	-2.207	142
3	10.1600	5.0800	411329	-2.374	-2.175	140
4	10.2774	5.1387	416082	-2.388	-2.189	142
<<<Statistics>>> Mean: 10.1824 Std Dev: 0.1057 RSD: 1.04						

Sample ID: Q1211-02 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 15:47

Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	7.1821	3.5910	290766	-2.416	-2.219	137
2	7.1193	3.5596	288224	-2.412	-2.216	168
3	7.1331	3.5665	288783	-2.389	-2.190	169
4	7.7221	3.8610	312629	-2.351	-2.156	165

<<<Statistics>>> Mean: 7.2891 Std Dev: 0.2899 RSD: 3.98

Sample ID: CCV2 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/29 16:13
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	10.1281	5.0641	410037	-2.343	-2.145	157
2	9.9175	4.9588	401510	-2.328	-2.128	155
3	10.0371	5.0185	406351	-2.314	-2.116	155
4	10.1736	5.0868	411876	-2.326	-2.126	157

<<<Statistics>>> Mean: 10.0641 Std Dev: 0.1130 RSD: 1.12

Sample ID: CCB2 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01291052
Cal. Curve: TOC
WATER 0-20PPM Timestamp: 2025/01/29 16:36
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	0.1828	0.0914	7402	-2.261	-2.128	120
2	0.2534	0.1267	10259	-2.302	-2.163	120
3	0.2675	0.1337	10830	-2.302	-2.156	120
4	0.3194	0.1597	12930	-2.321	-2.149	120

Last Message: Low Sample Detected
<<<Statistics>>> Mean: 0.2558 Std Dev: 0.0563 RSD: 22.02

Sample ID	Result	Std. Dev.	RSD	Mode	ALT
0.0PPM	6185	3006	48.60	TOC	
0.5PPM	27483	1110	4.04	TOC	
1.0PPM	48542	2267	4.67	TOC	
2.0PPM.....	88813...	1411..	1.59...	TOC	..
5.0PPM	211496	3458	1.64	TOC	
10.0PPM	411122	7732	1.88	TOC	
20.0PPM.....	817303...	2573..	0.31...	TOC	..
ICV1	10.3687	0.1121	1.08	TOC	
ICB1	0.2017	0.0756	37.49	TOC	
IC-20.....	0.1397...	0.0636..	45.51...	TOC	..
IC-R	0.1587	0.0461	29.04	TOC	

1

2

3

4

5

6

7

8

9

10

11

12

13

Method ID	Sample Type	Vial		Timestamp	Message
TOC 0 - 20 ppmC	TOC Standard	1	2025/01/15	12:17	Low Sample Detected
TOC 0 - 20 ppmC	TOC Standard	2	2025/01/15	12:42	
TOC 0 - 20 ppmC	TOC Standard	3	2025/01/15	13:07	
TOC 0 - 20 ppmC	...TOC Standard	.. 4..	2025/01/15	13:33	..
TOC 0 - 20 ppmC	TOC Standard	5	2025/01/15	13:59	
TOC 0 - 20 ppmC	TOC Standard	6	2025/01/15	14:26	
TOC 0 - 20 ppmC	...TOC Standard	.. 7..	2025/01/15	14:53	..
TOC 0 - 20 ppmC	Sample	6	2025/01/15	15:19	
TOC 0 - 20 ppmC	Sample	12	2025/01/15	15:43	Low Sample Detected
TOC 0 - 20 ppmC	...Sample	.. 13..	2025/01/15	16:07	..Low Sample Detected
TOC 0 - 20 ppmC	Sample	12	2025/01/15	16:30	Low Sample Detected

1
2
3
4
5
6
7
8
9
10
11
12
13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

Sample ID: 5.0PPM Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 13:59
Operator ID: NF IZ Sample Type: TOC Standard

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1			213032	-2.923	-2.726	159
2			206481	-2.832	-2.632	155
3			214311	-2.864	-2.669	157
4			212162	-2.841	-2.642	156

<<<Statistics>>> Mean: 211496 Std Dev: 3458 RSD: 1.64
=====

Sample ID: 10.0PPM Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 14:26
Operator ID: NF IZ Sample Type: TOC Standard

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1			400085	-2.807	-2.610	142
2			415561	-2.803	-2.603	162
3			411583	-2.777	-2.577	163
4			417257	-2.811	-2.611	164

<<<Statistics>>> Mean: 411122 Std Dev: 7732 RSD: 1.88
=====

Sample ID: 20.0PPM Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 14:53
Operator ID: NF IZ Sample Type: TOC Standard

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1			813925	-2.829	-2.632	177
2			819370	-2.836	-2.639	186
3			816671	-2.784	-2.585	170
4			819245	-2.792	-2.592	167

<<<Statistics>>> Mean: 817303 Std Dev: 2573 RSD: 0.31
=====

Sample ID: ICV1 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 15:19
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	10.3813	5.1906	420285	-2.799	-2.599	166
2	10.2898	5.1449	416583	-2.760	-2.560	165
3	10.2812	5.1406	416233	-2.764	-2.566	161
4	10.5226	5.2613	426009	-2.781	-2.584	161

<<<Statistics>>> Mean: 10.3687 Std Dev: 0.1121 RSD: 1.08
=====

Sample ID: ICB1 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 15:43
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	0.1020	0.0510	4131	-2.785	-2.738	120
2	0.2012	0.1006	8145	-2.809	-2.743	120
3	0.2187	0.1094	8855	-2.803	-2.725	120
4	0.2849	0.1425	11535	-2.810	-2.721	120

Last Message: Low Sample Detected

<<<Statistics>>> Mean: 0.2017 Std Dev: 0.0756 RSD: 37.49
=====

Sample ID: IC-20 Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 16:07
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	0.0727	0.0364	2944	-2.769	-2.766	120
2	0.1400	0.0700	5666	-2.789	-2.763	120
3	0.2250	0.1125	9108	-2.792	-2.701	120
4	0.1209	0.0605	4896	-2.763	-2.755	120

Last Message: Low Sample Detected

<<<Statistics>>> Mean: 0.1397 Std Dev: 0.0636 RSD: 45.51
=====

Sample ID: IC-R Mode: TOC
Method: TOC 0 - 20 ppmC Filename: 01151309
Cal. Curve: TOC WATER 0-20PPM Timestamp: 2025/01/15 16:30
Operator ID: NF IZ Sample Type: Sample

Rep #	ppm C	ug C	Raw Data	Beginning Baseline	Ending Baseline	Integration Time
1	0.0924	0.0462	3742	-2.733	-2.739	120
2	0.1992	0.0996	8064	-2.788	-2.739	120
3	0.1732	0.0866	7014	-2.775	-2.722	120
4	0.1700	0.0850	6884	-2.758	-2.719	120

Last Message: Low Sample Detected

<<<Statistics>>> Mean: 0.1587 Std Dev: 0.0461 RSD: 29.04
=====

Calibration Report Print Date/Time: 2025/01/15 14:57:01

Cal. Curve ID: TOC WATER 0-20PPM
Created: 2025/01/15 14:54
Calibration Factor (m): 8.097e+04
Y Intercept (b): 7467
r-squared: 0.99999

Re

Standard ID	Y Raw Data	X Expected ug C	Measured ug C	Message	Date & Time
0.0PPM	6185	0.000	-0.016		2025/01/15 12:17
0.5PPM	27483	0.250	0.247	-0.2	2025/01/15 12:42
1.0PPM	48542	0.500	0.507	1.4	2025/01/15 13:07
2.0PPM	88813	1.000	1.005	0.5	2025/01/15 13:33
5.0PPM	211497	2.500	2.520	0.8	2025/01/15 13:59
10.0PPM	411122	5.000	4.985	-0.3	2025/01/15 14:26
20.0PPM	817303	10.000	10.002	0.0	2025/01/15 14:53

NF

01.15.2025

LB1344 64

WORKLIST(Hardcopy Internal Chain)

WorkList Name : TOC MDL-01292025

WorkList ID : 187258

Department : Wet-Chemistry

Date : 01-29-2025 11:07:56

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1211-01	TPHHA-MW01-012825-00-T4	Water	TOC	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	9060A
Q1211-02	TAPIAL2-MW03-012825-00-T3	Water	TOC	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	9060A
Q1168-12	MDL-WATER-06-QT1-2025	Water	TOC	Conc H2SO4 to pH < 2	CHEM02	QA Of	01/23/2025	9060A

Date/Time01-29-2025, 11:10

Raw Sample Received by:NFL(wc)

Raw Sample Relinquished by:MLW01

Date/Time01-29-2025, 15:00

Raw Sample Received by:MLW01

Raw Sample Relinquished by:NFL(wc)



Analysis Method: 7196A

ANALYST: rubina

Parameter: ~~Hexavalent Chromium~~

SUPERVISOR REVIEW BY: Iwona

Run Number: LB134466

pH Meter ID: WC pH Meter-1

Reagent/Standard	Lot/Log #
Calibration Std. hexchrome 0.1 ppm	WP111683
Calibration Std. hexchrome 0.05 ppm	WP111682
calibration std. hexchrome 0.01 ppm	WP111680
calibration std. hexchrome 0 ppm	WP111679
hexavalent chromium color reagent	WP111659
5N sulfuric acid	WP110380
HEX LOD STD, 0.005PPM	WP111687
Calibration Std Hexachrome 0.025 ppm	WP111681
Hexavalent Chromium ICV-LCS Std	WP111686
Calibration and CCV std HexChrome 0.5PPM	WP111684
Calibration std HexChrome 1.0PPM	WP111685

Intercept: -0.0006

Slope: 0.7825

Regression: 0.999995

Seq	Lab ID	True Value (mg/l)	DF	Initial Vol (ml)	Final Vol (ml)	pH HN03	pH H2SO4	Absorb.at 540nm		Absorbance Difference	Result (mg/L)	%D	Anal Date	Anal Time
								Backgrnd	Color					
1	CAL1	0	1	100	100		1.74	0.000	0.000	0.000	0.000		01/29/2025	14:30
2	CAL2	0.01	1	100	100		1.85	0.000	0.006	0.006	0.008	-20	01/29/2025	14:31
3	CAL3	0.025	1	100	100		1.87	0.000	0.018	0.018	0.023	-8	01/29/2025	14:32
4	CAL4	0.05	1	100	100		1.89	0.000	0.039	0.039	0.050	0	01/29/2025	14:33
5	CAL5	0.1	1	100	100		1.89	0.000	0.079	0.079	0.101	1	01/29/2025	14:34
6	CAL6	0.5	1	100	100		1.85	0.000	0.390	0.390	0.499	-0.2	01/29/2025	14:35
7	CAL7	1	1	100	100		1.88	0.000	0.782	0.782	1.000	0	01/29/2025	14:36

Analysis Method: 7196A

ANALYST:rubina

Parameter: Hexavalent Chromium

SUPERVISOR REVIEW BY:Iwona

Run Number: LB134466

pH Meter ID:WC pH Meter-1

Seq	Lab ID	True Value	DF	Initial Vol (ml/gm)	Final Vol (ml)	pH HN03	pH H2SO4	Absorb.at540nm		Absorbance Difference	Intermediate Result (mg/L)	Anal Date	Anal Time
								Backgrnd	Color				
1	ICV	0.5	1	100	100		1.91	0.000	0.393	0.393	0.503	01/29/2025	14:37
2	ICB		1	100	100		1.76	0.000	0.000	0.000	0.001	01/29/2025	14:38
3	CCV1	0.5	1	100	100		1.93	0.000	0.390	0.390	0.499	01/29/2025	14:39
4	CCB1		1	100	100		1.80	0.000	0.001	0.001	0.002	01/29/2025	14:40
5	RL Check	0.01	1	100	100		1.90	0.000	0.007	0.007	0.010	01/29/2025	14:41
6	lb134466BL		1	100	100		1.74	0.000	0.001	0.001	0.002	01/29/2025	14:42
7	lb134466BS	0.5	1	100	100		1.93	0.000	0.400	0.400	0.512	01/29/2025	14:43
8	Q1168-09		1	100	100		2.02	0.000	0.005	0.005	0.007	01/29/2025	14:44
9	Q1211-01		1	100	100		2.08	0.000	0.000	0.000	0.001	01/29/2025	14:45
10	Q1211-01DU		1	100	100		2.10	0.000	0.000	0.000	0.001	01/29/2025	14:46
11	Q1211-01MS	1	2	100	100		2.10	0.000	0.395	0.395	0.506	01/29/2025	14:47
12	Q1211-01MS	1	2	100	100		2.11	0.000	0.392	0.392	0.502	01/29/2025	14:48
13	Q1211-02		1	100	100		2.06	0.000	0.000	0.000	0.001	01/29/2025	14:49
14	CCV2	0.5	1	100	100		1.92	0.000	0.394	0.394	0.504	01/29/2025	14:50
15	CCB2		1	100	100		1.78	0.000	0.001	0.001	0.002	01/29/2025	14:51

Instrument ID		IC-1	Analyst :		NF		Method: 00.0 / 9056A				
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	wt/Fir	Analyst
STD1	0	0	0	0	0	0	0	IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ
ICV	2.059	3.086	3.062	10.267	2.569	5.158	15.361	IC1-012025	1/20/2025 13:44	10	NF/IZ
ICB	0	0	0	0	0	0	0	IC1-012025	1/20/2025 14:06	10	NF/IZ
CCV	1.993	2.971	2.961	9.92	2.473	4.899	14.669	IC1-012025	1/29/2025 11:15	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-012025	1/29/2025 11:37	10	NF/IZ
LB134473BLW	0	0	0	0	0	0.161	0	IC1-012025	1/29/2025 11:58	10	NF/IZ
LB134473BSW	1.978	2.97	2.97	9.935	2.473	4.976	14.719	IC1-012025	1/29/2025 12:20	10	NF/IZ
Q1211-01	0.07	17.774	0	0	0.685	0	25.293	IC1-012025	1/29/2025 12:41	10	NF/IZ
Q1211-01MS	2.185	20.594	3.185	10.716	3.297	5.351	40.776	IC1-012025	1/29/2025 13:03	10	NF/IZ
Q1211-01MSD	2.189	20.627	3.192	10.712	3.298	5.406	40.871	IC1-012025	1/29/2025 13:24	10	NF/IZ
Q1211-02	0.076	3.071	0	0	0	0	30.679	IC1-012025	1/29/2025 13:46	10	NF/IZ
Q1211-01DLX5	0	3.332	0	0	0.184	0	5.246	IC1-012025	1/29/2025 14:07	10	NF/IZ
CCV	1.992	2.985	2.982	9.979	2.483	4.991	14.76	IC1-012025	1/29/2025 14:29	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-012025	1/29/2025 14:51	10	NF/IZ

1
2
3
4
5
6
7
8
9
10
11
12
13

Clear table


Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0	0 IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	-1.0000	0.3333	2.1667	0.9500	2.2000	-0.6000	3.0000
STD2	4.3750	4.8333	4.5000	4.6000	4.7000	4.4500	5.4000
STD3	-3.3000	-2.4667	-2.2667	-2.4200	-2.3200	-1.2400	-2.6800
STD4	-0.2000	-0.9000	-1.3667	-0.8800	-1.2800	-1.2800	-1.7267
STD5	0.4000	-0.3833	-0.4500	-0.5650	-0.7200	-0.3000	-0.7067
STD6	-0.2000	0.3600	0.4667	0.4760	0.6240	0.3360	0.6973

Fluoride (Anions)

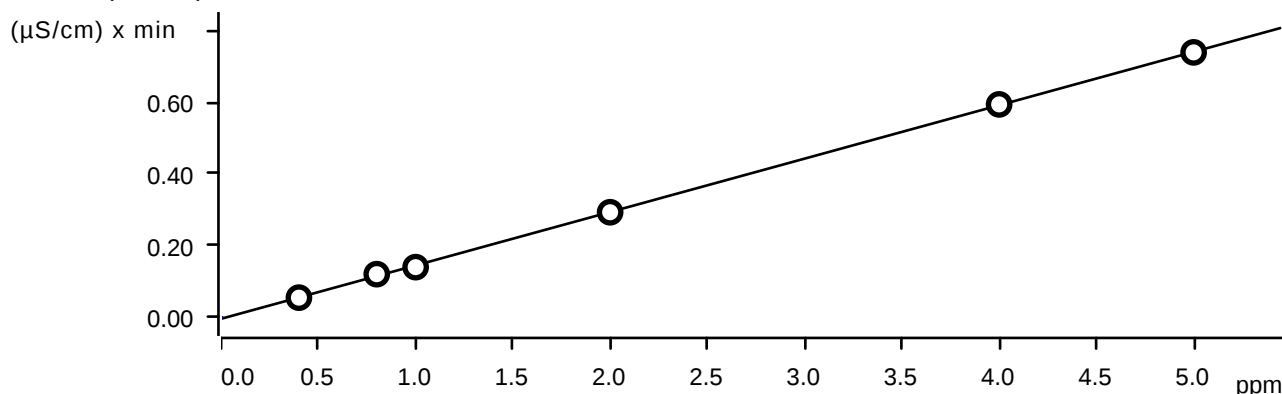
Function: $A = -4.02271E-3 + 0.0148839 \times Q$

Relative standard deviation 1.203859 %

Correlation coefficient 0.999923

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.120	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.140	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.594	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.739	STD7	2025-01-20 13:23:08 UTC-5	used

Chloride (Anions)

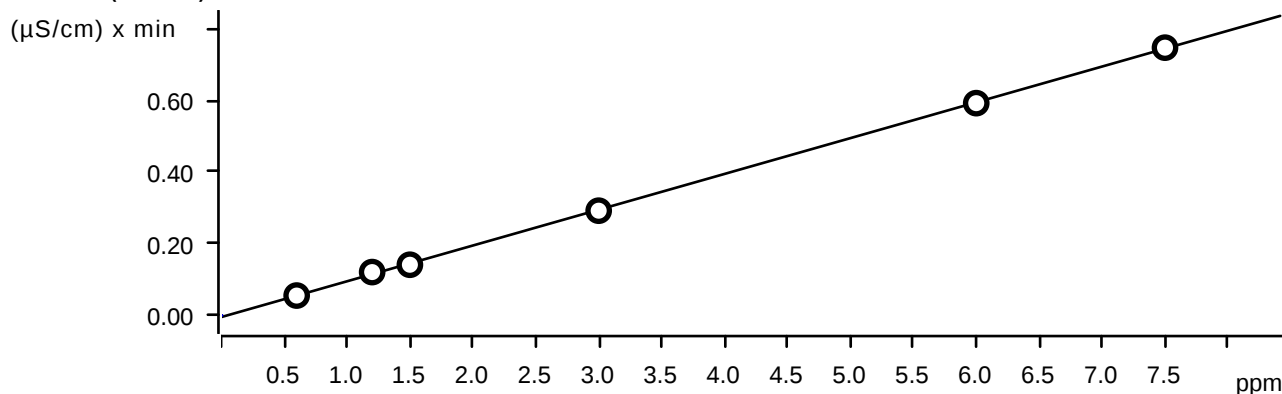Function: $A = -4.62538E-3 + 9.98029E-3 \times Q$


Relative standard deviation 1.261416 %

Correlation coefficient 0.999916

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.292	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.592	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrite (Anions)

(μS/cm) x min

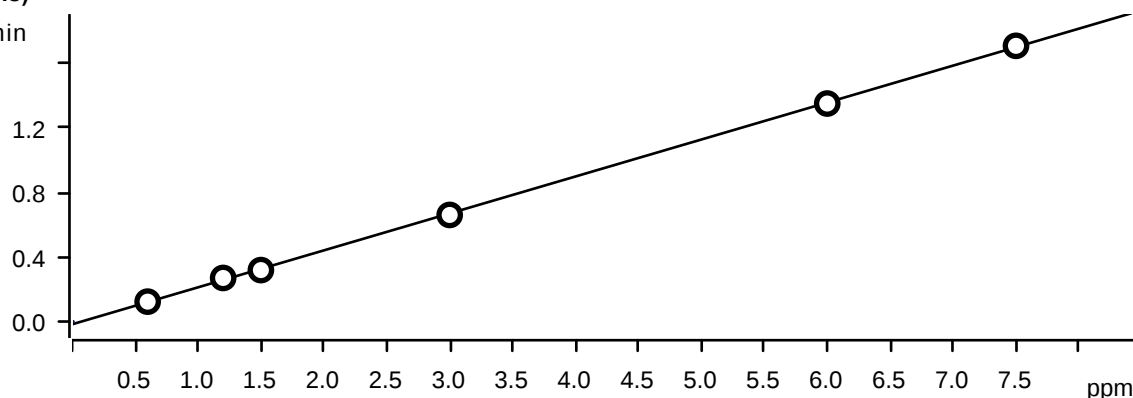Function: $A = -0.0179856 + 0.0228967 \times Q$


Relative standard deviation 1.369596 %

Correlation coefficient 0.999903

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.269	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.660	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.350	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.707	STD7	2025-01-20 13:23:08 UTC-5	used

Bromide (Anions)

($\mu\text{S/cm}$) $\times$ min

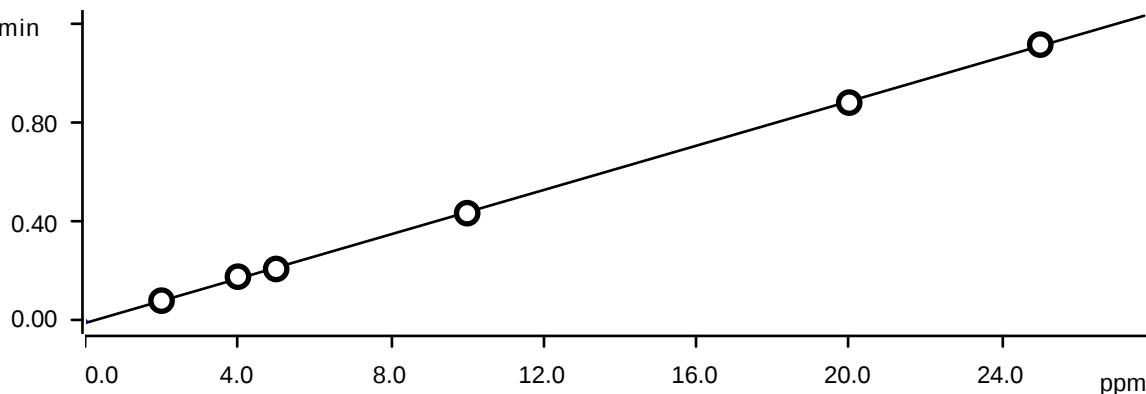

Function: $A = -8.89651E-3 + 4.46429E-3 \times Q$


Relative standard deviation: 1.338167 %

Correlation coefficient: 0.999906

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.178	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.434	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.879	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrate (Anions)

($\mu\text{S/cm}$) $\times$ min

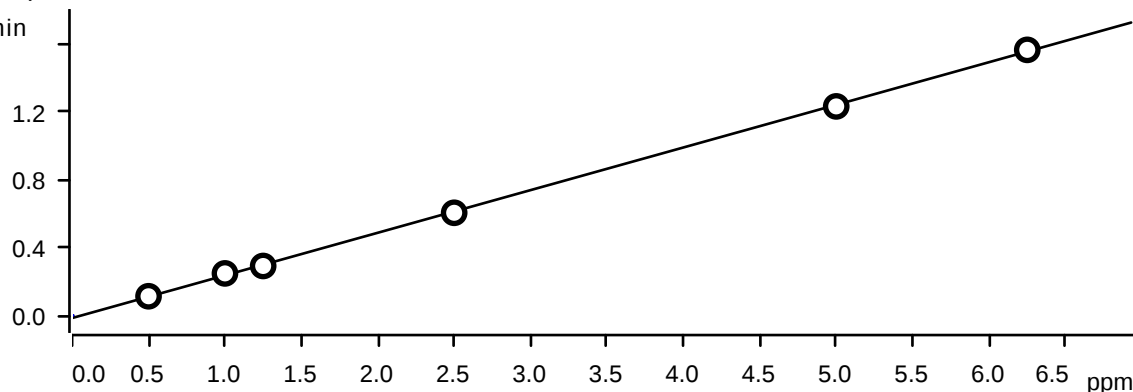


Function: $A = -0.0155875 + 0.0250988 \times Q$

Relative standard deviation: 1.561944 %

Correlation coefficient 0.999873

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.247	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.291	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.604	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.230	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.563	STD7	2025-01-20 13:23:08 UTC-5	used

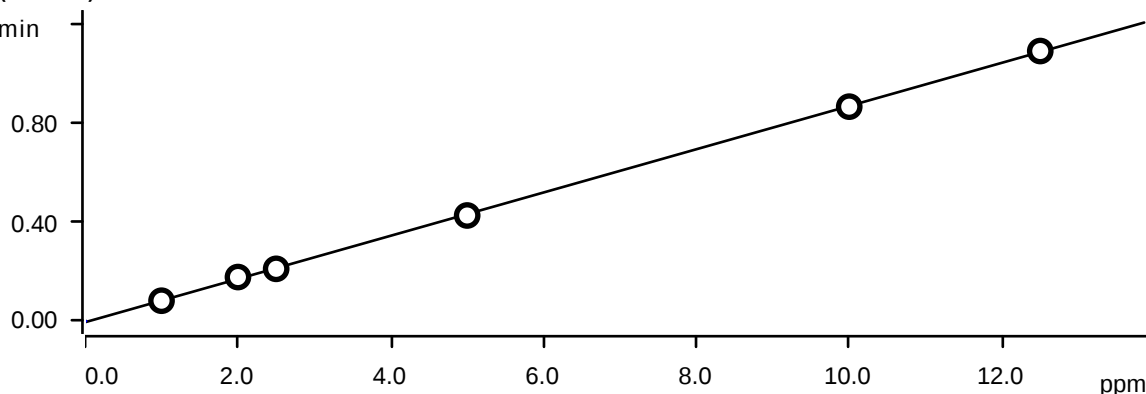
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -4.38887E-3 + 8.70711E-3 \times Q$

Relative standard deviation 1.148005 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.211	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.425	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-01-20 13:23:08 UTC-5	used

Sulfate (Anions)

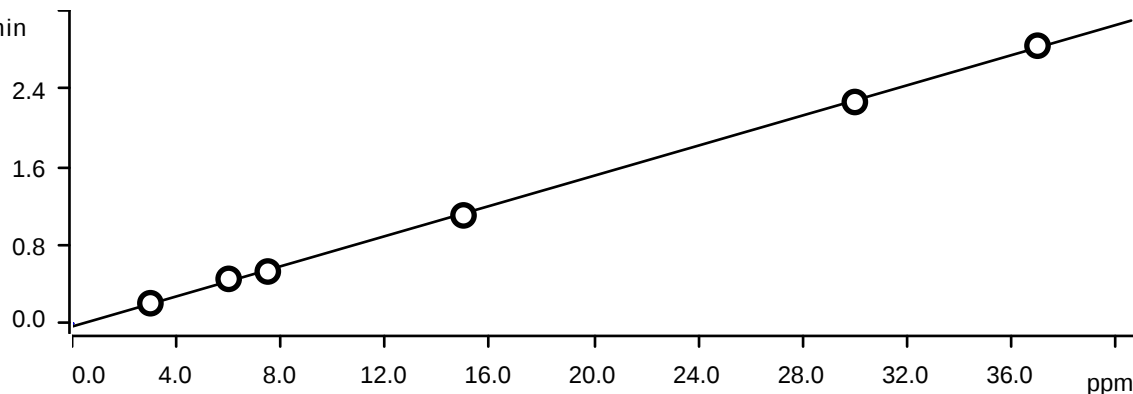 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0310554 + 7.70543E-3 \times Q$

Relative standard deviation 1.797524 %

Correlation coefficient 0.999831

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.456	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.105	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.264	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.840	STD7	2025-01-20 13:23:08 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-01-20 11:14:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

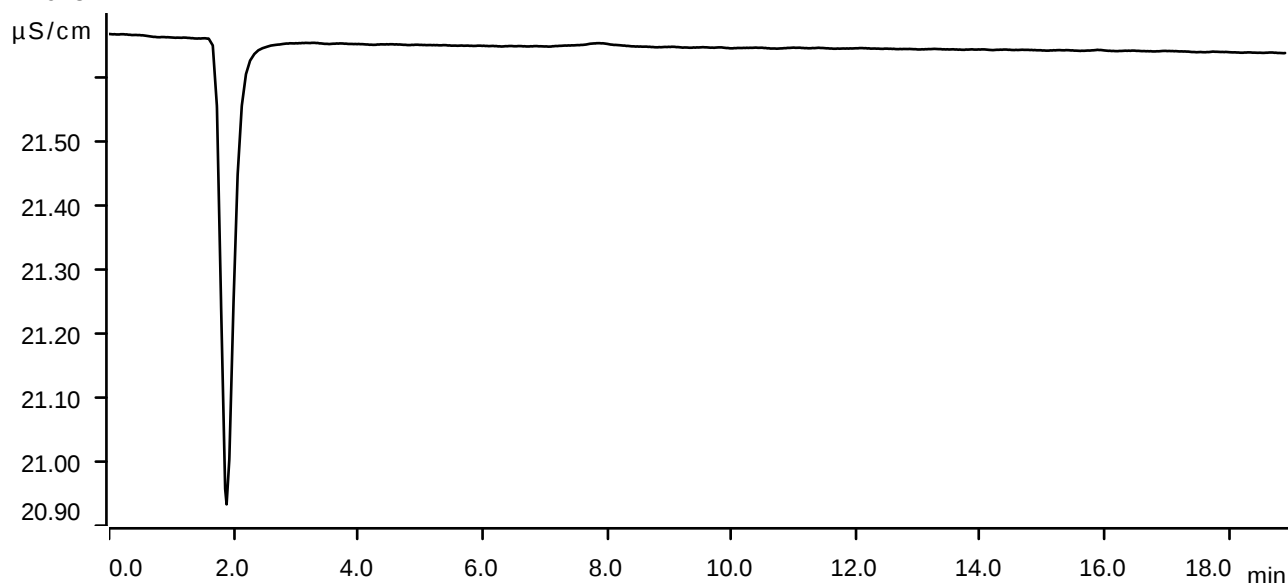


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-01-20 11:36:02 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

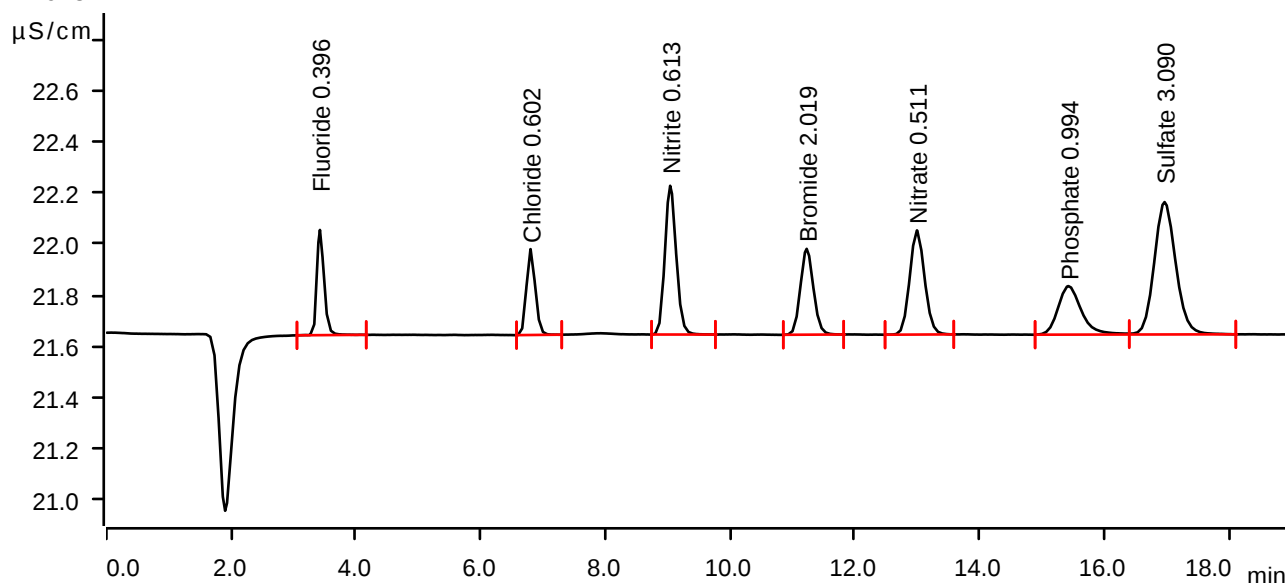

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.0549	0.411	0.396	Fluoride
2	6.802	0.0555	0.335	0.602	Chloride
3	9.040	0.1223	0.581	0.613	Nitrite
4	11.228	0.0813	0.335	2.019	Bromide
5	12.995	0.1126	0.407	0.511	Nitrate
6	15.423	0.0822	0.190	0.994	Phosphate
7	16.967	0.2070	0.517	3.090	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-01-20 11:57:26 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

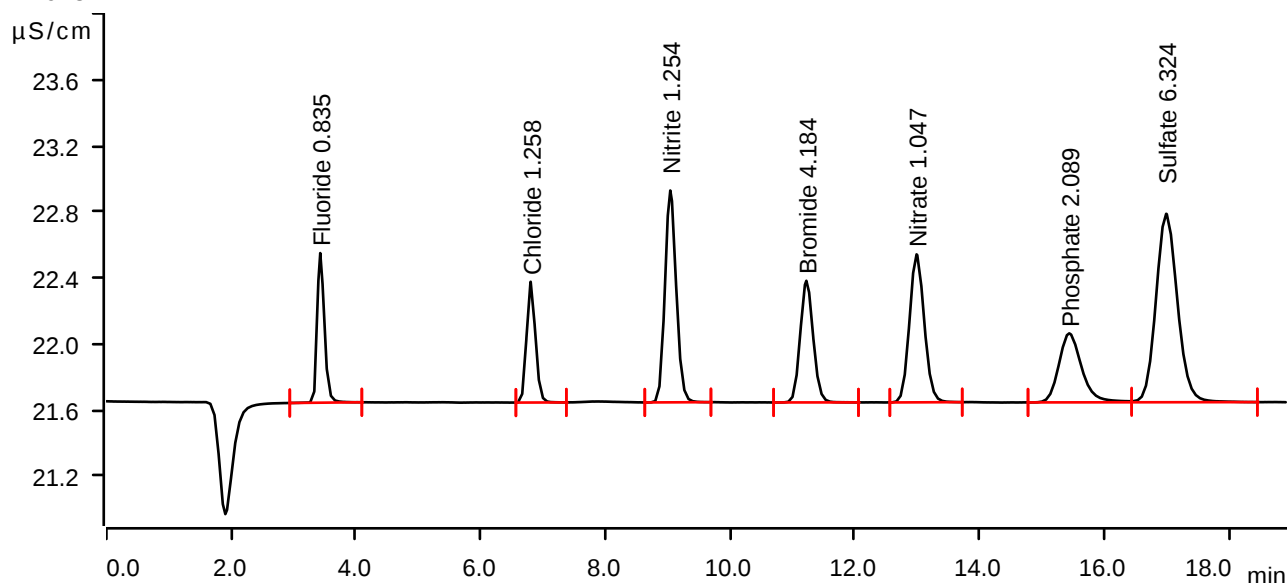

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1203	0.906	0.835	Fluoride
2	6.803	0.1209	0.731	1.258	Chloride
3	9.042	0.2691	1.282	1.254	Nitrite
4	11.223	0.1779	0.736	4.184	Bromide
5	12.990	0.2472	0.896	1.047	Nitrate
6	15.438	0.1775	0.418	2.089	Phosphate
7	16.992	0.4562	1.141	6.324	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-01-20 12:18:50 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

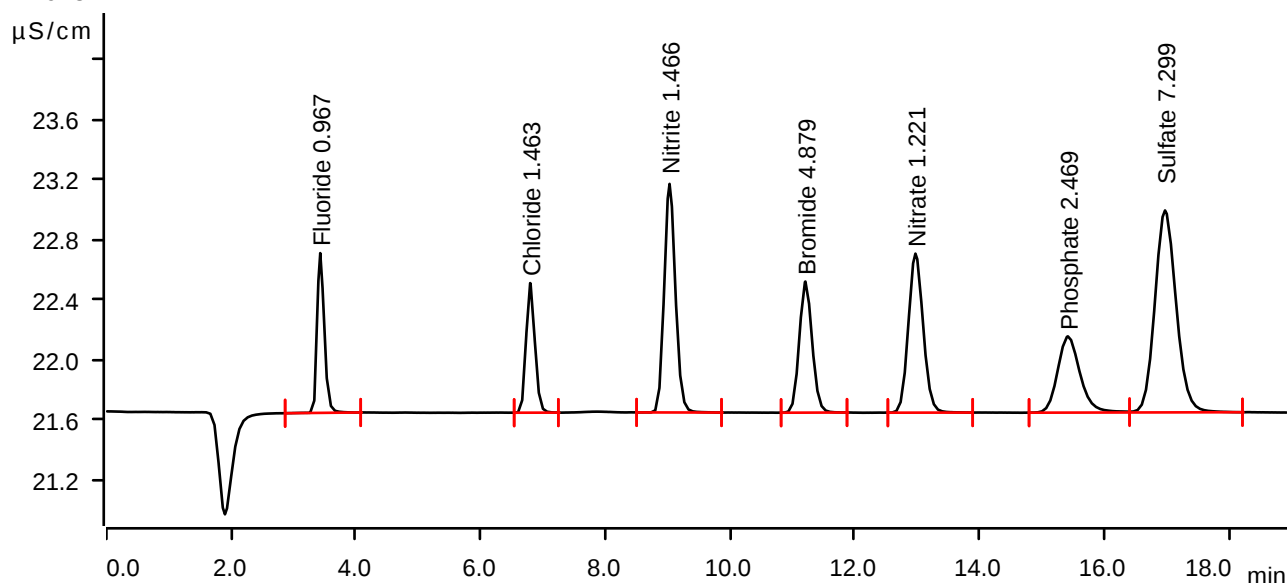

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1399	1.061	0.967	Fluoride
2	6.795	0.1414	0.860	1.463	Chloride
3	9.030	0.3178	1.517	1.466	Nitrite
4	11.208	0.2089	0.870	4.879	Bromide
5	12.972	0.2908	1.056	1.221	Nitrate
6	15.417	0.2105	0.506	2.469	Phosphate
7	16.973	0.5314	1.341	7.299	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-01-20 12:40:15 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

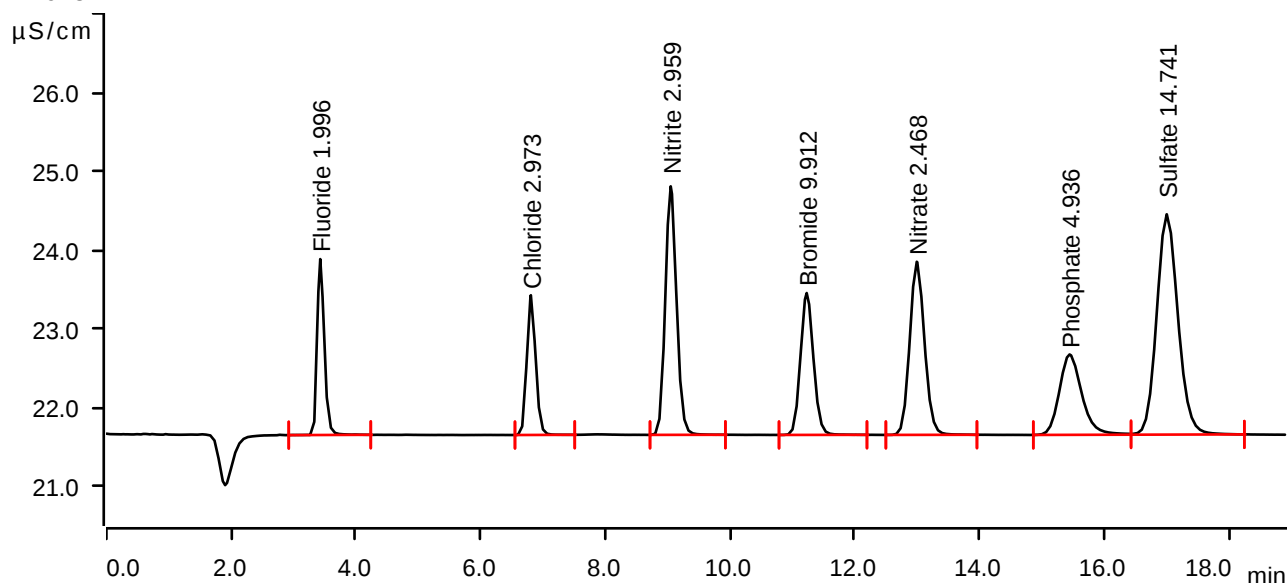

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2930	2.233	1.996	Fluoride
2	6.807	0.2921	1.773	2.973	Chloride
3	9.048	0.6595	3.154	2.959	Nitrite
4	11.228	0.4336	1.801	9.912	Bromide
5	12.993	0.6039	2.197	2.468	Nitrate
6	15.443	0.4254	1.020	4.936	Phosphate
7	17.002	1.1048	2.795	14.741	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-01-20 13:01:41 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

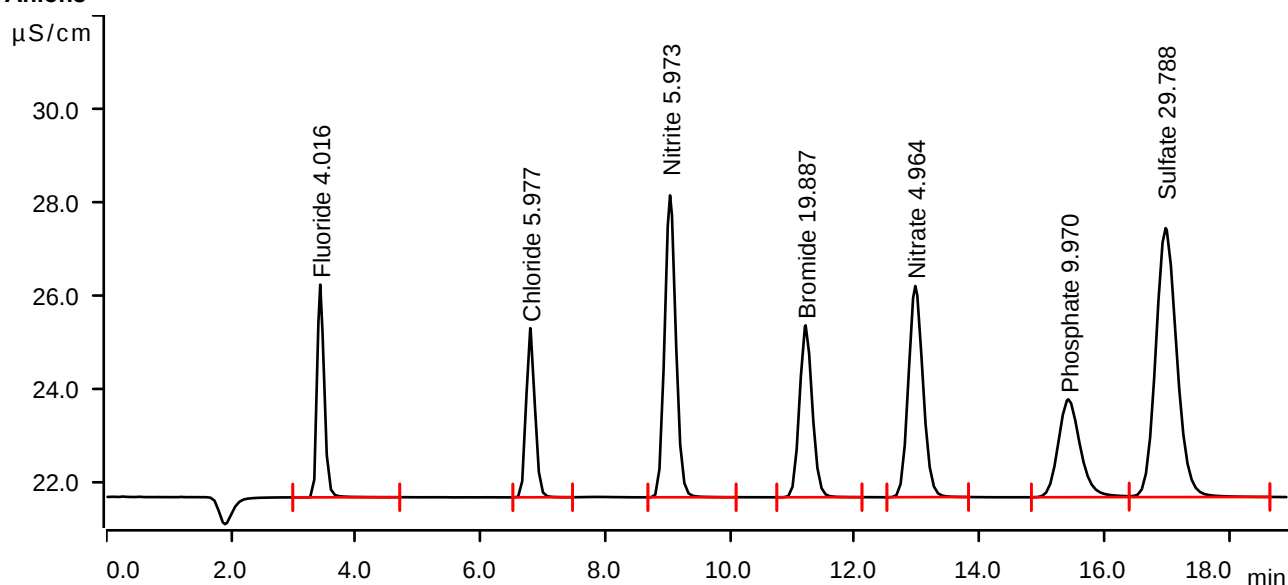

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.5937	4.568	4.016	Fluoride
2	6.797	0.5919	3.633	5.977	Chloride
3	9.038	1.3497	6.484	5.973	Nitrite
4	11.212	0.8789	3.691	19.887	Bromide
5	12.970	1.2302	4.535	4.964	Nitrate
6	15.423	0.8637	2.101	9.970	Phosphate
7	16.983	2.2643	5.777	29.788	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-01-20 13:23:08 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

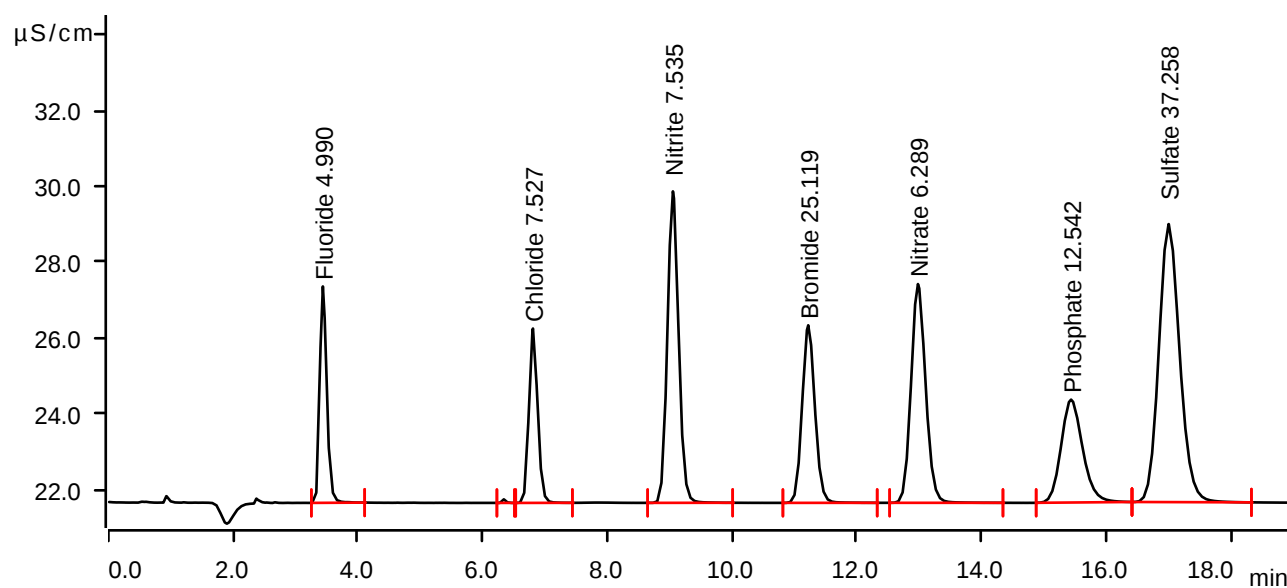

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.440	0.7387	5.703	4.990	Fluoride
2	6.342	0.0051	0.093	invalid	
3	6.808	0.7466	4.595	7.527	Chloride
4	9.052	1.7073	8.209	7.535	Nitrite
5	11.222	1.1125	4.681	25.119	Bromide
6	12.980	1.5629	5.766	6.289	Nitrate
7	15.435	1.0877	2.713	12.542	Phosphate
8	16.998	2.8398	7.327	37.258	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-01-20 13:44:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

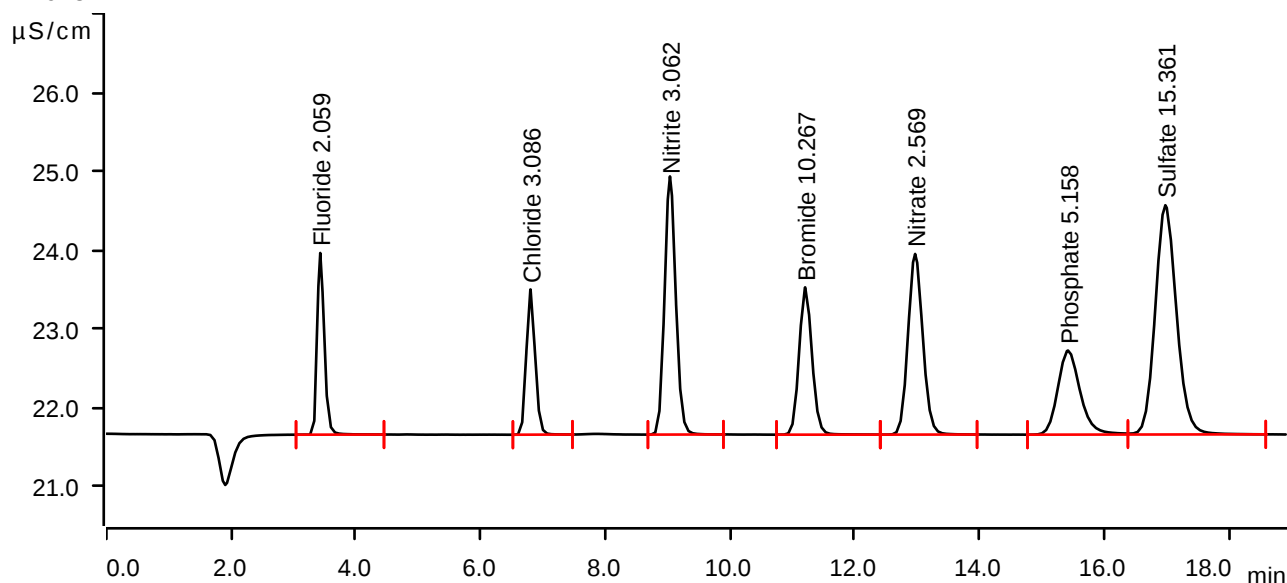

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.3025	2.306	2.059	Fluoride
2	6.798	0.3033	1.843	3.086	Chloride
3	9.037	0.6832	3.276	3.062	Nitrite
4	11.205	0.4495	1.869	10.267	Bromide
5	12.967	0.6293	2.293	2.569	Nitrate
6	15.418	0.4447	1.067	5.158	Phosphate
7	16.978	1.1525	2.909	15.361	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-01-20 14:06:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

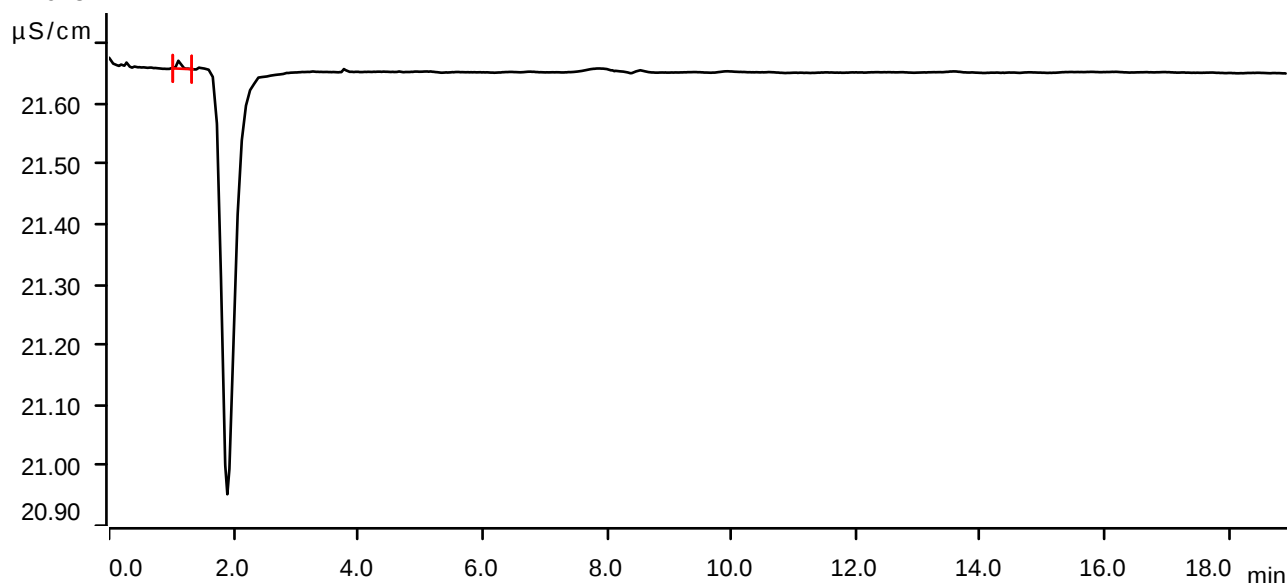

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.115	0.0010	0.013	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-29 11:15:35 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

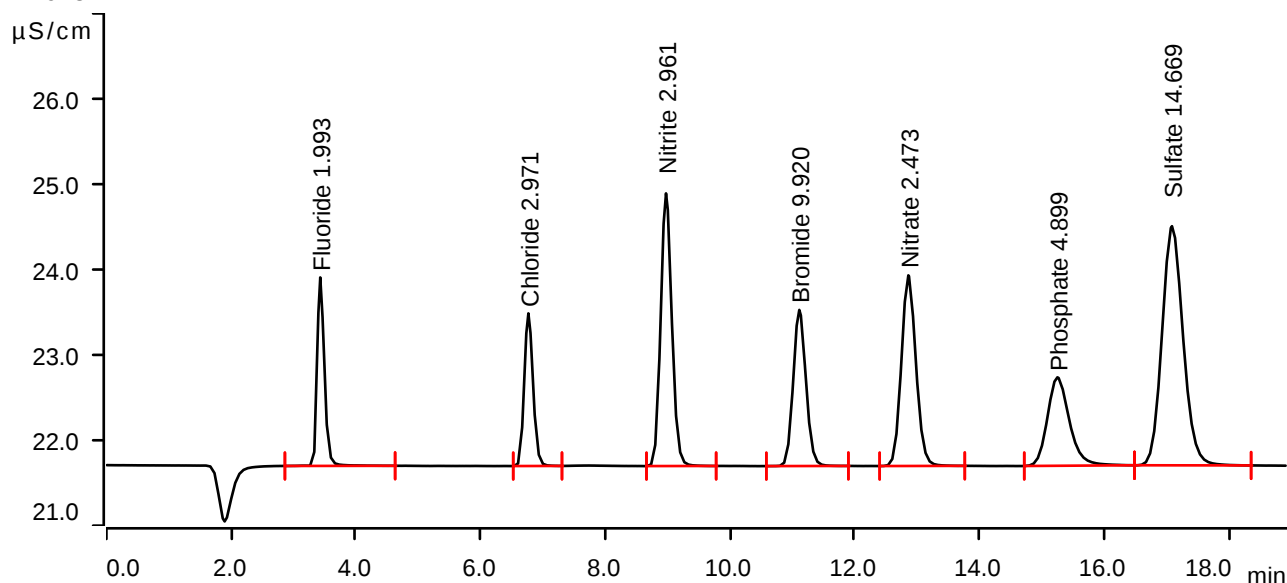

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2926	2.208	1.993	Fluoride
2	6.767	0.2919	1.788	2.971	Chloride
3	8.973	0.6599	3.194	2.961	Nitrite
4	11.110	0.4340	1.829	9.920	Bromide
5	12.858	0.6052	2.233	2.473	Nitrate
6	15.248	0.4222	1.036	4.899	Phosphate
7	17.085	1.0993	2.801	14.669	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-29 11:37:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

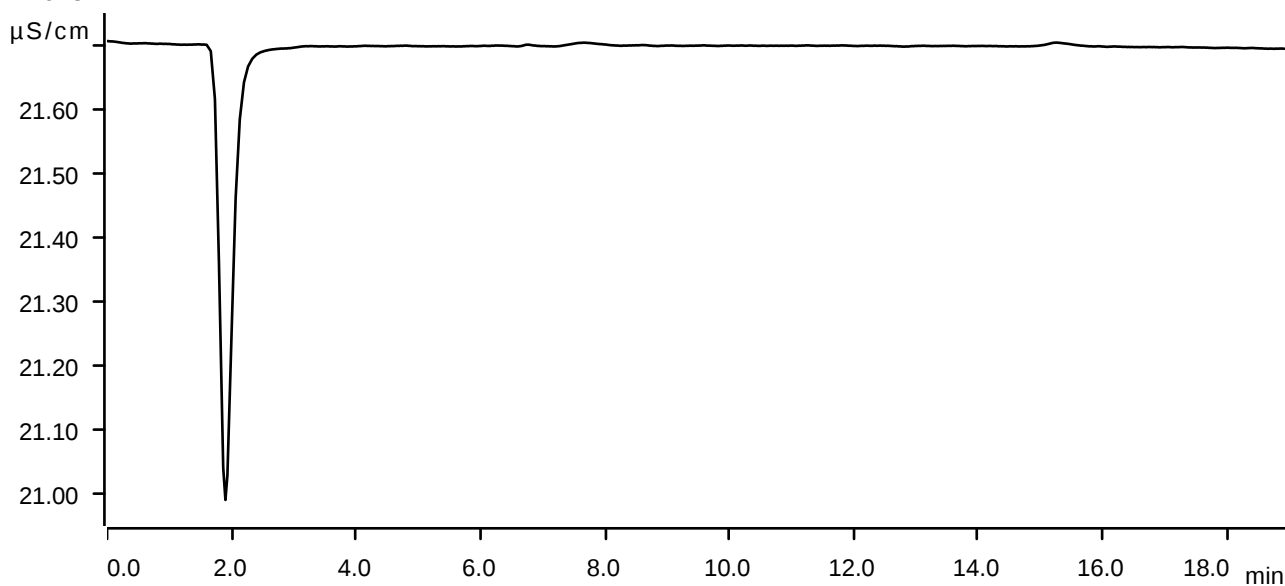


Sample data

Ident LB134473BLW
Sample type Sample
Determination start 2025-01-29 11:58:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

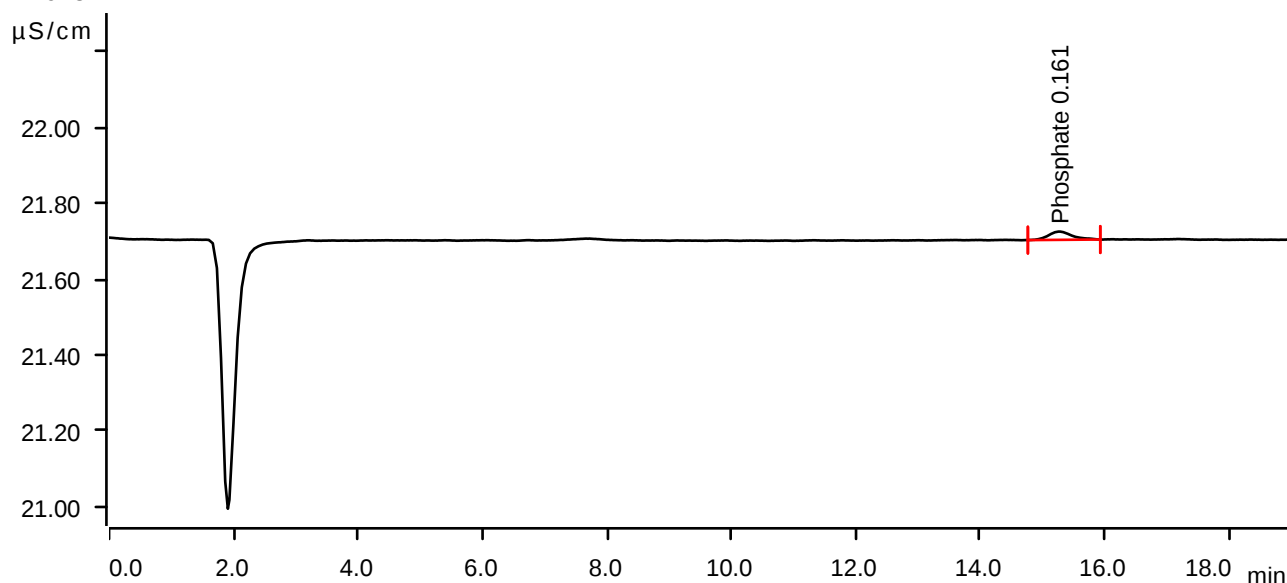

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	15.255	0.0096	0.022	0.161	Phosphate


Sample data

Ident LB134473BSW
Sample type Check standard 1
Determination start 2025-01-29 12:20:07 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

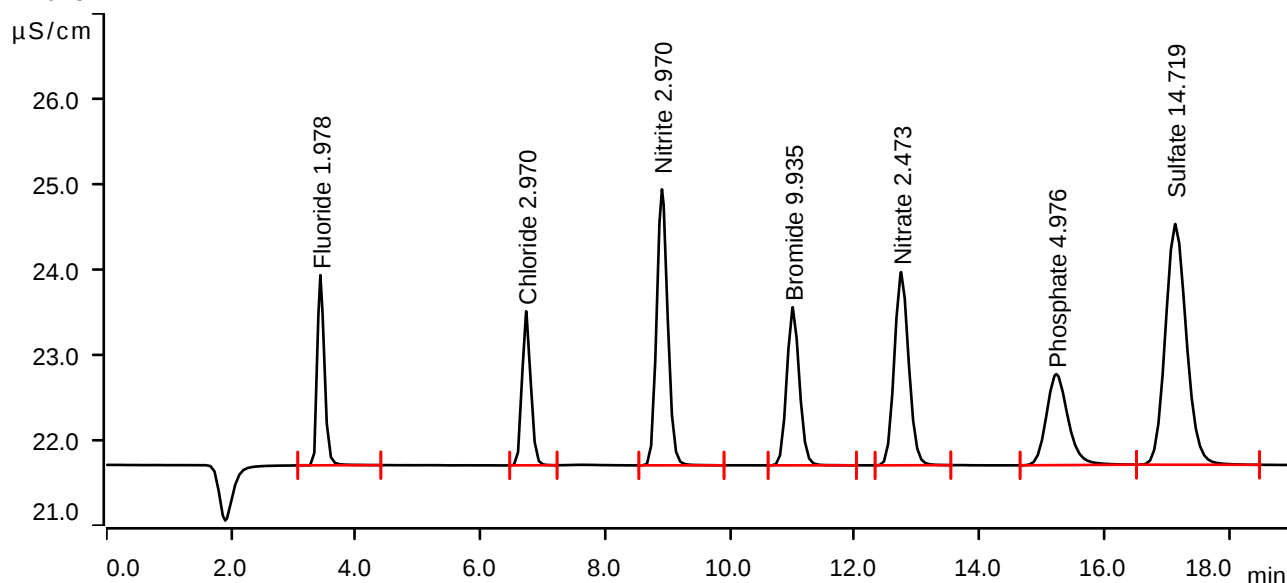

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.432	0.2904	2.227	1.978	Fluoride
2	6.730	0.2918	1.805	2.970	Chloride
3	8.908	0.6621	3.233	2.970	Nitrite
4	11.005	0.4346	1.852	9.935	Bromide
5	12.743	0.6052	2.263	2.473	Nitrate
6	15.230	0.4288	1.067	4.976	Phosphate
7	17.138	1.1031	2.820	14.719	Sulfate


Sample data

Ident Q1211-01
Sample type Sample
Determination start 2025-01-29 12:41:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

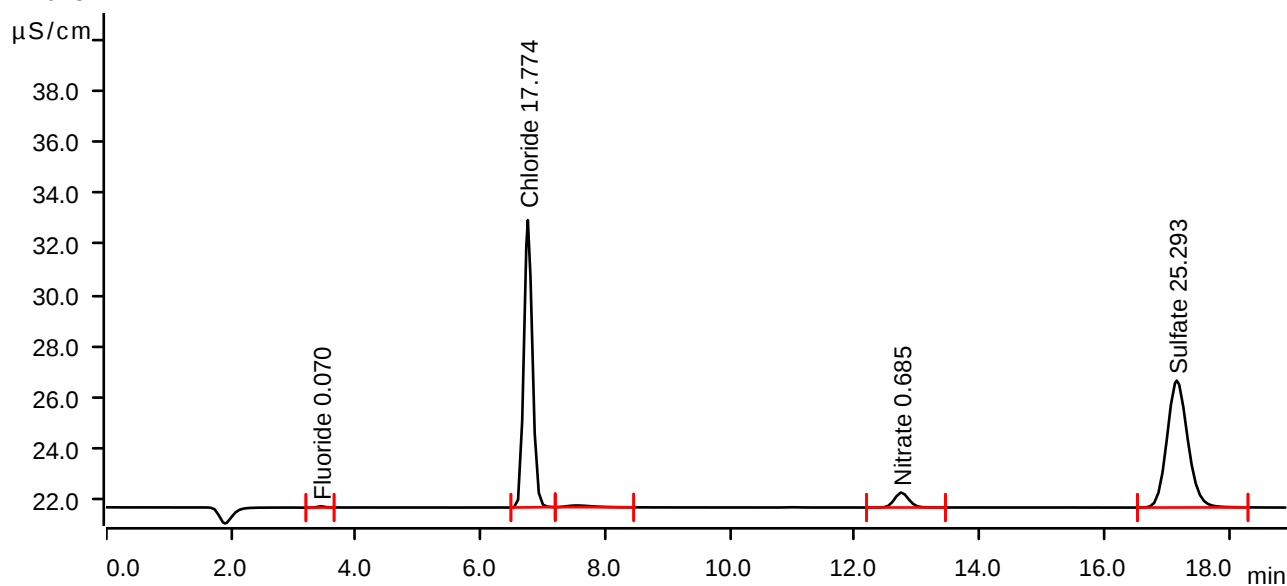

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.437	0.0065	0.048	0.070	Fluoride
2	6.758	1.7693	11.215	17.774	Chloride
3	7.532	0.0305	0.064	invalid	
4	12.745	0.1565	0.582	0.685	Nitrate
5	17.162	1.9178	4.954	25.293	Sulfate


Sample data

Ident Q1211-01MS
Sample type Sample
Determination start 2025-01-29 13:03:12 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

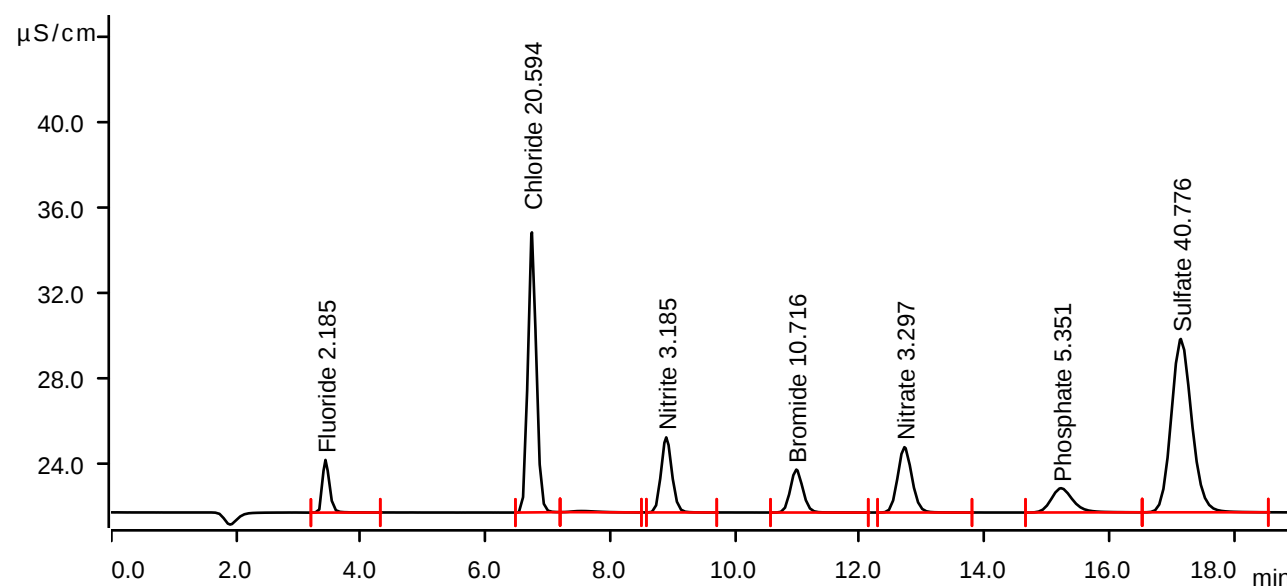

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.433	0.3212	2.468	2.185	Fluoride
2	6.743	2.0507	13.120	20.594	Chloride
3	7.532	0.0266	0.057	invalid	
4	8.897	0.7112	3.517	3.185	Nitrite
5	10.982	0.4695	2.013	10.716	Bromide
6	12.715	0.8120	3.063	3.297	Nitrate
7	15.227	0.4615	1.138	5.351	Phosphate
8	17.147	3.1109	8.122	40.776	Sulfate


Sample data

Ident Q1211-01MSD
Sample type Sample
Determination start 2025-01-29 13:24:46 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

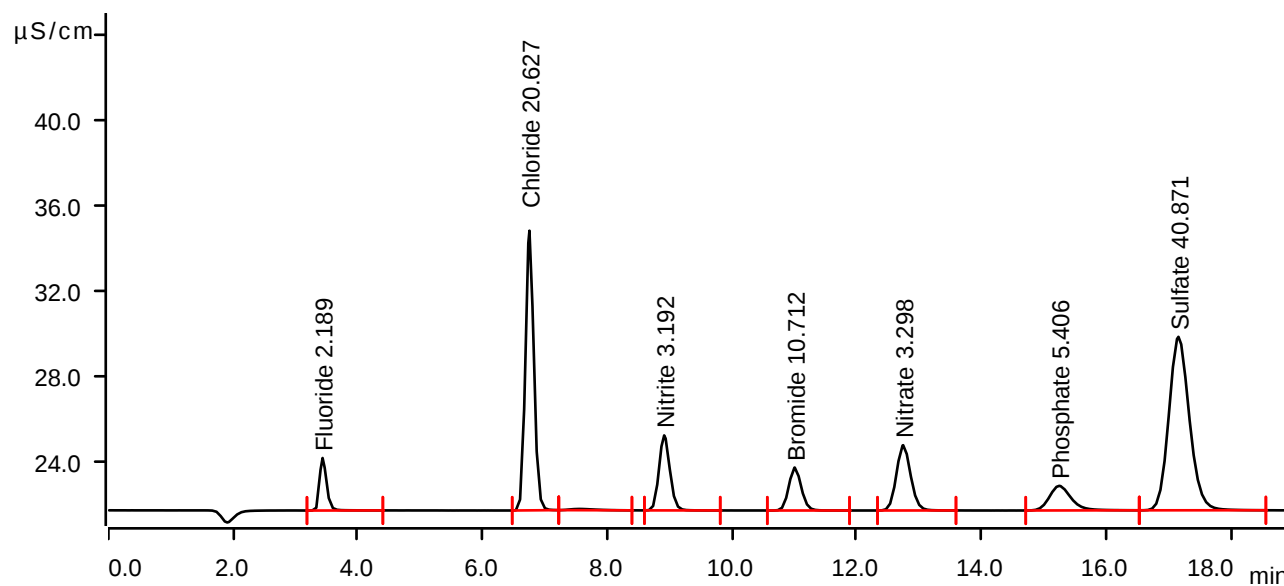

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.435	0.3218	2.461	2.189	Fluoride
2	6.752	2.0540	13.103	20.627	Chloride
3	7.552	0.0273	0.058	invalid	
4	8.912	0.7130	3.514	3.192	Nitrite
5	11.005	0.4693	2.011	10.712	Bromide
6	12.743	0.8121	3.059	3.298	Nitrate
7	15.245	0.4663	1.153	5.406	Phosphate
8	17.157	3.1182	8.128	40.871	Sulfate


Sample data

Ident Q1211-02
Sample type Sample
Determination start 2025-01-29 13:46:20 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

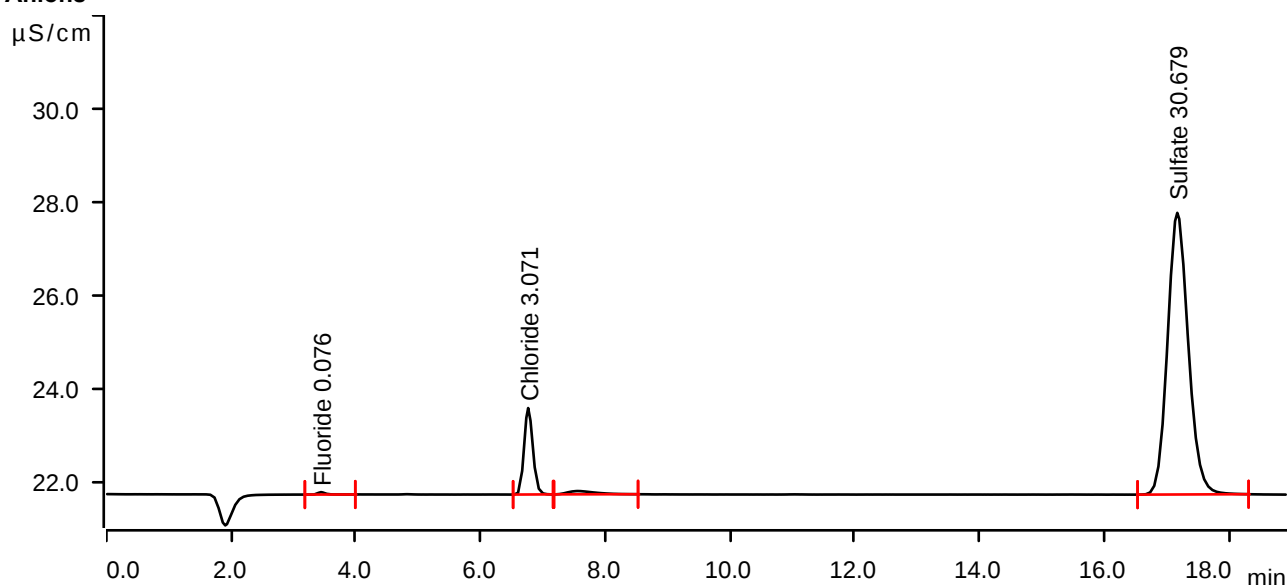

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.442	0.0072	0.051	0.076	Fluoride
2	6.763	0.3019	1.856	3.071	Chloride
3	7.555	0.0362	0.071	invalid	
4	17.170	2.3329	6.048	30.679	Sulfate


Sample data

Ident Q1211-01DLX5
Sample type Sample
Determination start 2025-01-29 14:07:55 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

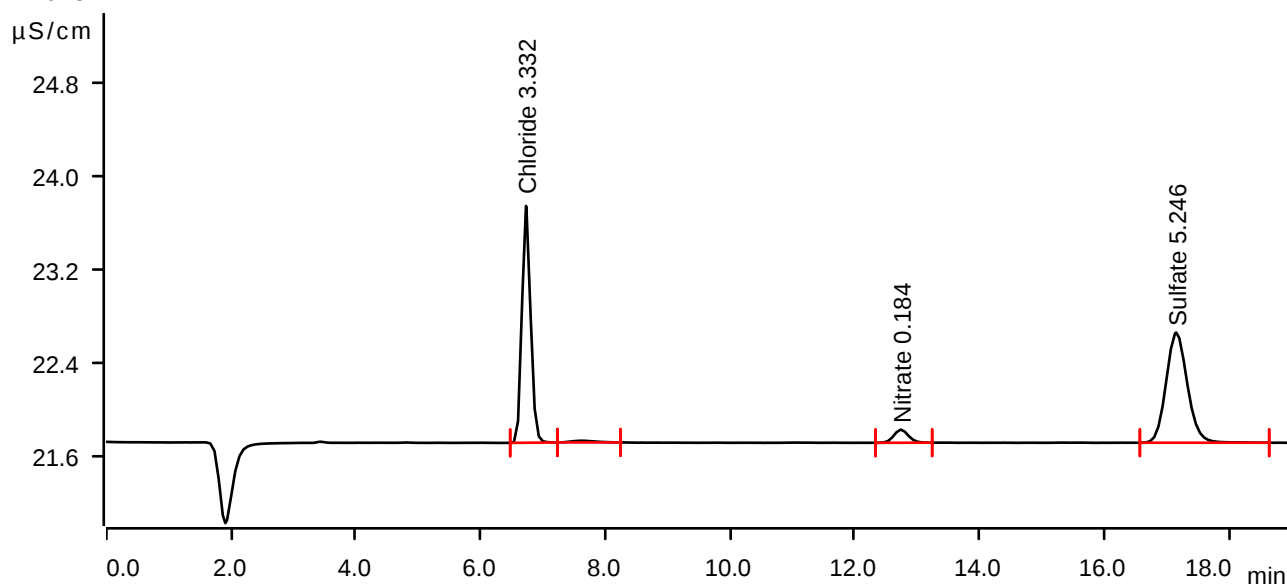

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.728	0.3279	2.034	3.332	Chloride
2	7.607	0.0066	0.015	invalid	
3	12.740	0.0306	0.113	0.184	Nitrate
4	17.152	0.3732	0.946	5.246	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-29 14:29:30 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

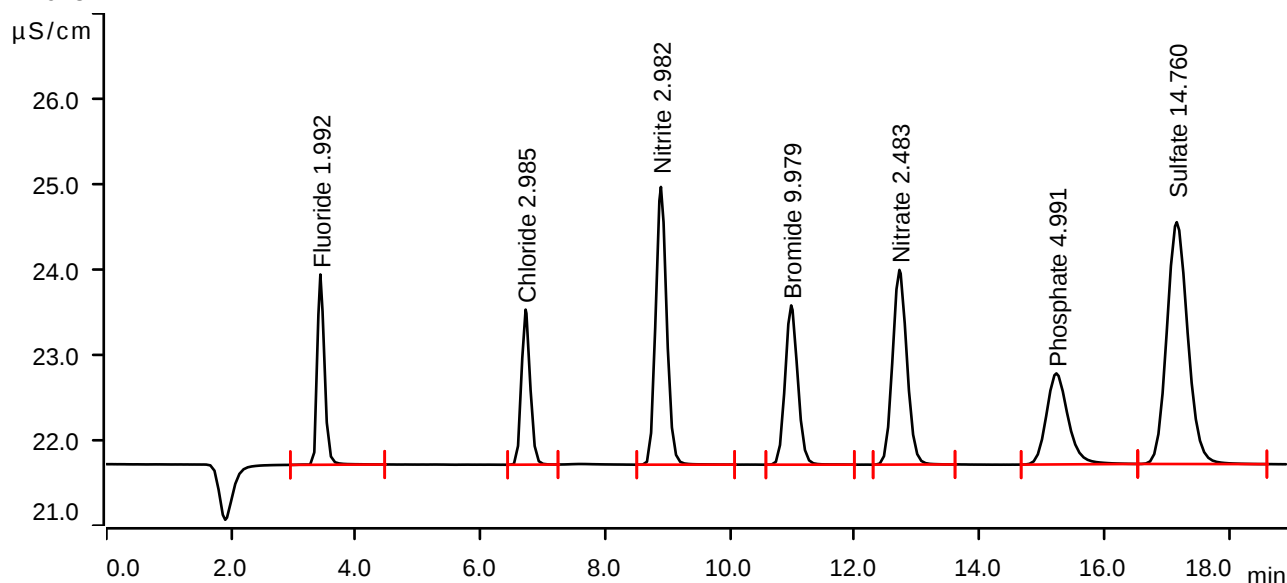

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.432	0.2925	2.229	1.992	Fluoride
2	6.722	0.2932	1.816	2.985	Chloride
3	8.892	0.6649	3.253	2.982	Nitrite
4	10.980	0.4366	1.866	9.979	Bromide
5	12.715	0.6076	2.280	2.483	Nitrate
6	15.232	0.4302	1.066	4.991	Phosphate
7	17.162	1.1062	2.833	14.760	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-29 14:51:00 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

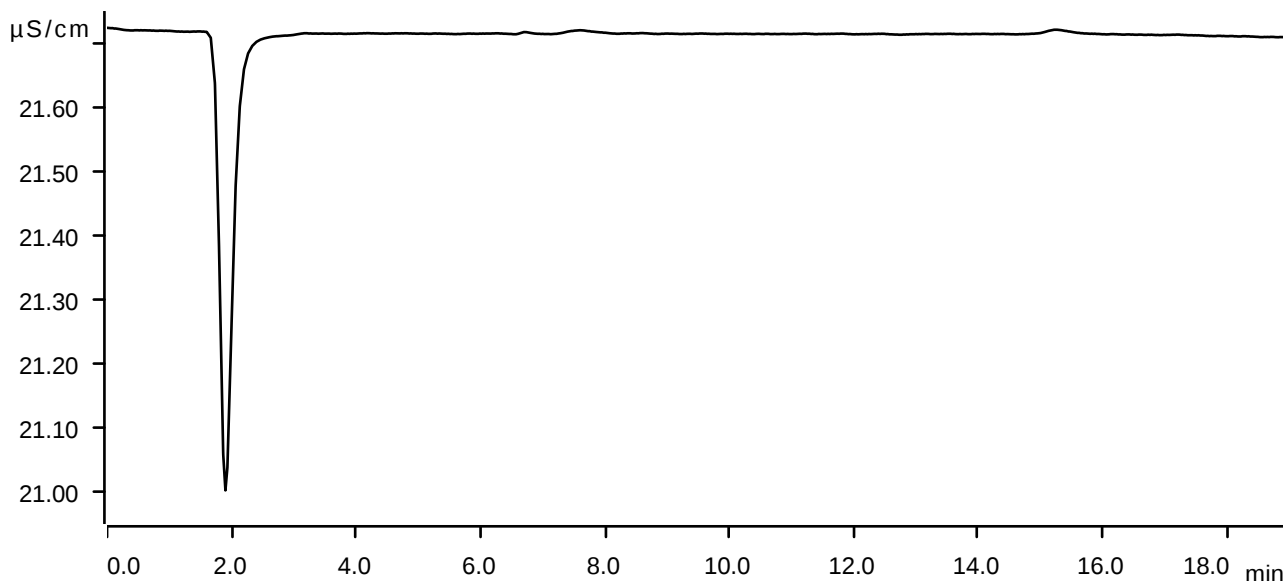

WORKLIST(Hardcopy Internal Chain)

LB134473

WorkList Name : ANIONS-01292025

WorkList ID : 187264

Department : Wet-Chemistry

Date : 01-29-2025 12:03:28

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1211-01	TPHHA-MW01-012825-00-T4	Water	Anions Group5	Cool 4 deg C	WEST04	N31	01/28/2025	9056A
Q1211-02	TAPIAL2-MW03-012825-00-T3	Water	Anions Group5	Cool 4 deg C	WEST04	N31	01/28/2025	9056A

Date/Time 01.29.2025 12:05
Raw Sample Received by: NFWC
Raw Sample Relinquished by: JFWC

Date/Time 01.29.2025 14:15
Raw Sample Received by: JFWC
Raw Sample Relinquished by: NFWC

Extraction and Analytical Summary Report

Analysis Method: 1664A
Test: Oil and Grease
Run Number: LB134521
Analysis Date: 02/01/2025
BalanceID: WC SC-6
OvenID: EXT OVEN-3

ANALYST: jignesh
REVIEWED BY: Iwona
Extraction Date: 02/01/2025
Extraction IN Time: 10:10
Extraction OUT Time: 10:48
Thermometer ID: EXT OVEN#3

Dish #	Lab ID	Client ID	Matrix	pH	Sample Vol (ml)	Final Volume (ml)	Empty Dish Weight (g)	Final Empty Dish Weight (g)	Silica Gel Weight (g)	Weight After Drying (g)	Final Weight After Drying (g)	Change Weight (g)	Result in ppm
1	LB134521BL	LB134521BL	WATER	1.3	1000	100	3.0263	3.0263	0	3.0264	3.0264	0.0001	0.1
2	LB134521BS	LB134521BS	WATER	1.3	1000	100	3.1788	3.1788	0	3.1957	3.1957	0.0169	16.9
3	Q1168-07	LOD-MDL-WATER-01-QT1-2	WATER	1.3	1000	100	2.9631	2.9631	0	2.9652	2.9652	0.0021	2.1
4	Q1168-08	LOQ-WATER-02-QT1-2025	WATER	1.3	1000	100	2.7481	2.7481	0	2.7538	2.7538	0.0057	5.7
5	Q1211-01	TPHHA-MW01-012825-00-T	WATER	1.3	1000	100	3.0878	3.0878	0	3.0879	3.0879	0.0001	0.1
6	Q1211-02	TAPIAL2-MW03-012825-00	WATER	1.3	1000	100	3.0320	3.0320	0	3.0323	3.0323	0.0003	0.3
7	Q1252-01	EFFLUENT	WATER	1.6	1000	100	3.0521	3.0521	0	3.0641	3.0641	0.0120	12
8	Q1252-02	Q1252-01MS	WATER	1.6	1000	100	3.1485	3.1485	0	3.1804	3.1804	0.0319	31.9
9	Q1252-03	Q1252-01MSD	WATER	1.6	1000	100	2.9903	2.9903	0	3.0225	3.0225	0.0322	32.2

QC Batch# LB134521 Test: Oil and Grease Analysis Date: 02/01/2025

Chemicals Used:

Chemical Name	Chemical Lot #
HEXANE	W3153
pH Paper 0-14	M6069
Sodium Sulfate	EP2580
1:1 HCL	WP110826
Silica Gel	NA
Sand	NA

Standards Used:

Standard Name	Amount Used	Standard Lot #
LCSW	2.5 ML	WP100827
LCSWD	NA	NA
MS/MSD	2.5 ML	WP100828

BALANCE CALIBRATION / OVEN Dessicator Data

Analytical Balance ID # : WC SC-6

Before Analysis

0.0020 gram Balance: 0.0018 (0.0018-0.0022) In OVEN TEMP1 : 71 °C Dessicator Time In1 : 12:26
 1.0000 gram Balance: 1.0004 (0.9950-1.0050) In Time1: 11:30
 Bal Check Time: 10:30 Out OVEN TEMP1: 71 °C Dessicator Time Out1: 13:10
 Out Time1: 12:25

After Analysis

0.0020 gram Balance: 0.0021 (0.0018-0.0022) In OVEN TEMP2 : 70 °C Dessicator Time In2 : 14:31
 1.0000 gram Balance: 1.0005 (0.9950-1.0050) In Time2: 14:00
 Bal Check Time: 15:15 Out OVEN TEMP2: 70 °C Dessicator Time Out2: 15:10
 Out Time2: 14:30

WORKLIST(Hardcopy Internal Chain)

134521

WorkList Name : oil & grease p1211

WorkList ID : 187391

Department : Wet-Chemistry

Date : 02-01-2025 09:58:54

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1168-07	LOD-MDL-WATER-01-QT1-202	Water	Oil and Grease	Conc H2SO4 to pH < 2	CHEM02	QA Of	01/23/2025	1664A
Q1168-08	LOQ-WATER-02-QT1-2025	Water	Oil and Grease	Conc H2SO4 to pH < 2	CHEM02	QA Of	01/23/2025	1664A
Q1211-01	TPHHA-MW01-012825-00-T4	Water	Oil and Grease	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	1664A
Q1211-02	TAPIAL2-MW03-012825-00-T3	Water	Oil and Grease	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	1664A
Q1252-01	EFFLUENT	Water	Oil and Grease	Conc H2SO4 to pH < 2	HOLL01	E11	01/31/2025	1664A
Q1252-02	Q1252-01MS	Water	Oil and Grease	Conc H2SO4 to pH < 2	HOLL01	E11	01/31/2025	1664A
Q1252-03	Q1252-01MSD	Water	Oil and Grease	Conc H2SO4 to pH < 2	HOLL01	E11	01/31/2025	1664A

Date/Time 02/01/25 10:00
 Raw Sample Received by: SA (Edt-Val)
 Raw Sample Relinquished by: RJ (Edt-Val)

Date/Time 02/01/25

Raw Sample Received by: RJ (Edt-Val)

Raw Sample Relinquished by: SA (Edt-Val)

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

2/3/2025 14:33

Reviewed by : RM

Instrument ID : Konelab

Test: Ammonia-N

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.992	0.0	0.148	
ICB1	-0.009	0.0	0.014	
CCV1	0.938	0.0	0.141	
CCB1	-0.002	0.0	0.015	
RL CHECK	0.084	0.0	0.027	
PB166477BL	-0.009	0.0	0.014	
PB166477BS	0.971	0.0	0.145	
Q1168-07	0.074	0.0	0.025	
Q1168-08	0.090	0.0	0.027	
Q1211-01	0.004	0.0	0.016	
Q1211-01DUP	0.005	0.0	0.016	
Q1211-01MS	1.060	0.0	0.157	
Q1211-01MSD	1.068	0.0	0.158	
Q1211-02	0.402	0.0	0.069	
CCV2	0.968	0.0	0.145	
CCB2	0.001	0.0	0.016	
Q1252-01	10.844	0.0	1.466	Test limit high
Q1252-05	2.050	0.0	0.290	Test limit high
PB166478BL	0.007	0.0	0.016	
PB166478BS	1.020	0.0	0.152	
Q1168-01	0.071	0.0	0.025	
Q1168-02	0.103	0.0	0.029	
CCV3	0.945	0.0	0.142	
CCB3	-0.004	0.0	0.015	
Q1252-01DLX10	1.074	0.0	0.159	
Q1252-05DLX2	0.966	0.0	0.145	
CCV4	0.994	0.0	0.148	
CCB4	-0.005	0.0	0.015	
N	28			
Mean	0.882			
SD	2.0295			
CV%	230.06			

84% (50-150)
02/03/2025
RM

Test limit high
Test limit high

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 03 12:51:07 2025

Mon Feb 03 14:31:08 2025

Sample Id	Sam/Ctr/c	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Ammonia-1 P		0.0029	mg/l	2/3/2025 12:51:07	
0.1PPM	A	Ammonia-1 P		0.1004	mg/l	2/3/2025 12:51:08	
0.2PPM	A	Ammonia-1 P		0.202	mg/l	2/3/2025 12:51:09	
0.4PPM	A	Ammonia-1 P		0.3808	mg/l	2/3/2025 12:51:10	
1.0PPM	A	Ammonia-1 P		0.986	mg/l	2/3/2025 12:51:11	
1.3PPM	A	Ammonia-1 P		1.3854	mg/l	2/3/2025 12:51:12	
2.0PPM	A	Ammonia-1 P		1.9759	mg/l	2/3/2025 12:51:13	
ICV1	S	Ammonia-1 P		0.9918	mg/l	2/3/2025 13:28:52	
ICB1	S	Ammonia-1 P		-0.0086	mg/l	2/3/2025 13:28:54	
CCV1	S	Ammonia-1 P		0.938	mg/l	2/3/2025 13:28:56	
CCB1	S	Ammonia-1 P		-0.0025	mg/l	2/3/2025 13:28:58	
RL CHECK	S	Ammonia-1 P		0.0838	mg/l	2/3/2025 13:29:01	
PB166477BL	S	Ammonia-1 P		-0.0091	mg/l	2/3/2025 13:29:03	
PB166477BS	S	Ammonia-1 P		0.9708	mg/l	2/3/2025 13:39:37	
Q1168-07	S	Ammonia-1 P		0.0741	mg/l	2/3/2025 13:39:40	
Q1168-08	S	Ammonia-1 P		0.0897	mg/l	2/3/2025 13:39:42	
Q1211-01	S	Ammonia-1 P		0.0041	mg/l	2/3/2025 13:39:43	
Q1211-01DUP	S	Ammonia-1 P		0.0054	mg/l	2/3/2025 13:39:45	
Q1211-01MS	S	Ammonia-1 P		1.0604	mg/l	2/3/2025 13:39:47	
Q1211-01MSD	S	Ammonia-1 P		1.0684	mg/l	2/3/2025 13:50:20	
Q1211-02	S	Ammonia-1 P		0.4024	mg/l	2/3/2025 13:50:21	
CCV2	S	Ammonia-1 P		0.9677	mg/l	2/3/2025 13:50:22	
CCB2	S	Ammonia-1 P		0.0007	mg/l	2/3/2025 13:50:24	
Q1252-01	S	Ammonia-1 P		10.8436	mg/l	2/3/2025 13:50:26	
Q1252-05	S	Ammonia-1 P		2.0496	mg/l	2/3/2025 13:50:27	
PB166478BL	S	Ammonia-1 P		0.007	mg/l	2/3/2025 13:50:28	
PB166478BS	S	Ammonia-1 P		1.0198	mg/l	2/3/2025 13:59:53	
Q1168-01	S	Ammonia-1 P		0.0712	mg/l	2/3/2025 13:59:54	
Q1168-02	S	Ammonia-1 P		0.1027	mg/l	2/3/2025 13:59:57	
CCV3	S	Ammonia-1 P		0.9453	mg/l	2/3/2025 13:59:58	
CCB3	S	Ammonia-1 P		-0.0039	mg/l	2/3/2025 14:00:00	
Q1252-01DLX10	S	Ammonia-1 P		1.0743	mg/l	2/3/2025 14:31:01	
Q1252-05DLX2	S	Ammonia-1 P		0.9658	mg/l	2/3/2025 14:31:04	
CCV4	S	Ammonia-1 P		0.9936	mg/l	2/3/2025 14:31:05	
CCB4	S	Ammonia-1 P		-0.0054	mg/l	2/3/2025 14:31:08	

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

2/3/2025 12:53


Test Ammonia-N

Accepted 2/3/2025 12:53

Factor 7.476
Bias 0.015

Coeff. of det. 0.998852

Errors

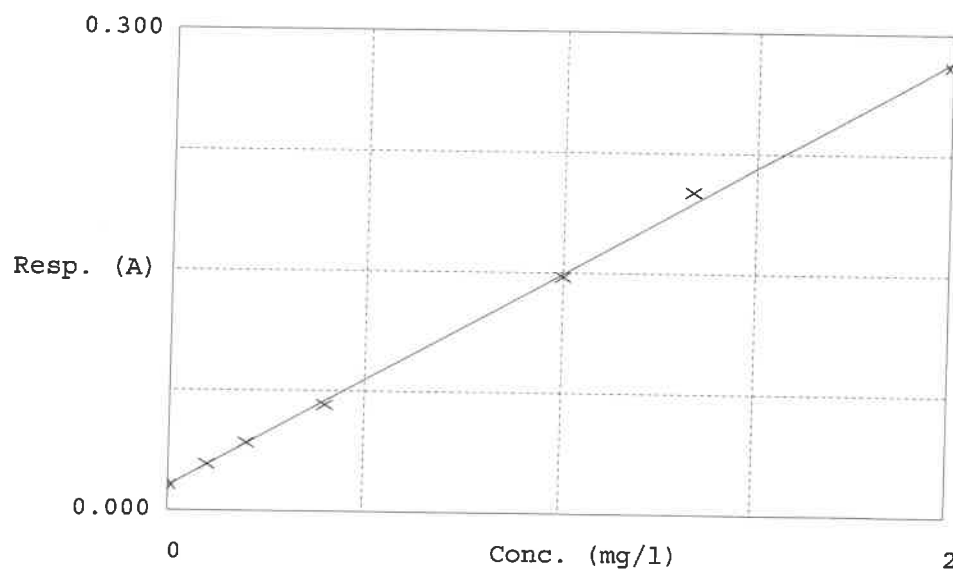

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.016	0.0029	0.0000	-
2	NH3-2PPM	0.029	0.1004	0.1000	0.4
3	NH3-2PPM	0.042	0.2020	0.2000	1.0
4	NH3-2PPM	0.066	0.3808	0.4000	-4.8
5	NH3-2PPM	0.147	0.9860	1.0000	-1.4
6	NH3-2PPM	0.201	1.3854	1.3333	6.6
7	NH3-2PPM	0.280	1.9759	2.0000	-1.2

02/03/2025
RM

SOP ID : MSM4500-NH3 B,G-Ammonia-17

SDG No : N/A

Matrix : WATER

Pipette ID : WC

Balance ID : N/A

Hood ID : HOOD#2

Block ID : WC-DIST-BLOCK-1

Weigh By : N/A

Start Digest Date: 02/03/2025 Time : 08:50 Temp : 150 °C

End Digest Date: 02/03/2025 Time : 09:50 Temp : 160 °C

 5 batch 02/03/2025 10:15 160°C
 02/03/2025 11:15 160°C

Digestion tube ID : M5595

Block Thermometer ID : WC CYANIDE

Filter paper ID : N/A

Prep Technician Signature: RM

pH Meter ID : N/A

Supervisor Signature: 12

Standard Name	MLS USED	STD REF. # FROM LOG
LCSW	1.0ML	WP111420
MS/MSD SPIKE SOL.	1.0ML	WP111419
PBW	50.0ML	W3112
RL CHECK	0.1ML	WP111419
LOD	0.8ML	WP111744

Chemical Used	ML/SAMPLE USED	Lot Number
BORATE BUFFER	2.5ML	WP111325
NAOH 6N	0.5-2.0ML	WP111318
H2SO4 0.04N	5.0ML	WP110335
pH strip-Ammonia	N/A	W3133
KI-starch paper	N/A	W3155
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

 ALL GLASSWEAR ARE STEAMED OUT AND THERE WERE NO TRACE OF AMMONIA USING NESLER REAGENT
 WP111604, Due to bad matrix and client history 1ML was taken as an initial volume for Q1252-01,05, LOQ WP111744

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
02/03/2025 10:10	RM CWG	RM CWG
	Preparation Group	Analysis Group

Lab Sample ID	Client Sample ID	Initial Vol (ml)	Final Vol (ml)	pH	Sulfide	Oxidizing	Nitrate/ Nitrite	Comment	Prep Pos
PB166477BL	PBW477	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
PB166477BS	LCS477	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1168-07	LOD-MDL-WATER-01-QT1-20 25	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1168-08	LOQ-WATER-02-QT1-2025	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1211-01	TPHHA-MW01-012825-00-T4	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1211-01DUP	TPHHA-MW01-012825-00-T4 DUP	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1211-01MS	TPHHA-MW01-012825-00-T4 MS	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1211-01MSD	TPHHA-MW01-012825-00-T4 MSD	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1211-02	TAPIAL2-MW03-012825-00-T 3	50	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1252-01	EFFLUENT	1	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A
Q1252-05	INFLUENT	1	50	<2	N/A	Negative	N/A	AFTER ADDING 6N NAOH PH IS 9.5	N/A

WORKLIST(Hardcopy Internal Chain)

WorkList Name : AMMONIA-W-2-3

WorkList ID : 187400

Department : Distillation

Date : 02-03-2025 08:14:01

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1168-07	LOD-MDL-WATER-01-QT1-202	Water	Ammonia	Conc H2SO4 to pH < 2	CHEM02	QA Of	01/23/2025	SM4500-NH3
Q1168-08	LOQ-WATER-02-QT1-2025	Water	Ammonia	Conc H2SO4 to pH < 2	CHEM02	QA Of	01/23/2025	SM4500-NH3
Q1211-01	TPHHA-MW01-012825-00-T4	Water	Ammonia	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	SM4500-NH3
Q1211-02	TAPIAL2-MW03-012825-00-T3	Water	Ammonia	Conc H2SO4 to pH < 2	WEST04	N31	01/28/2025	SM4500-NH3
Q1252-01	EFFLUENT	Water	Ammonia	Conc H2SO4 to pH < 2	HOLL01	E11	01/31/2025	SM4500-NH3
Q1252-05	INFLUENT	Water	Ammonia	Conc H2SO4 to pH < 2	HOLL01	E11	01/31/2025	SM4500-NH3

Date/Time 02/03/2025 08:20
 Raw Sample Received by: RM CWC
 Raw Sample Relinquished by: [Signature]

Date/Time 02/03/2025 10:30
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

Instrument ID: TOC

Daily Analysis Runlog For Sequence/QC Batch ID # LB134464

Review By	Niha	Review On	1/31/2025 9:24:04 AM
Supervise By	Iwona	Supervise On	1/31/2025 11:12:58 AM
SubDirectory	LB134464	Test	TOC
STD. NAME	STD REF.#		
ICAL Standard	WP111441,WP111442,WP111443,WP111444,WP111445,WP111446		
ICV Standard	WP111448		
CCV Standard	WP111580		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP111581		
Chk Standard	WP111453,WP111454,WP109953,WP111676,WP111677		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	0.0PPM	0.0PPM	CAL1	01/15/25 12:17		NF IZ	OK
2	0.5PPM	0.5PPM	CAL2	01/15/25 12:42		NF IZ	OK
3	1.0PPM	1.0PPM	CAL3	01/15/25 13:07		NF IZ	OK
4	2.0PPM	2.0PPM	CAL4	01/15/25 13:33		NF IZ	OK
5	5.0PPM	5.0PPM	CAL5	01/15/25 13:59		NF IZ	OK
6	10.0PPM	10.0PPM	CAL6	01/15/25 14:26		NF IZ	OK
7	20.0PPM	20.0PPM	CAL7	01/15/25 14:53		NF IZ	OK
8	ICV1	ICV1	ICV	01/15/25 15:19		NF IZ	OK
9	ICB1	ICB1	ICB	01/15/25 15:43		NF IZ	OK
10	IC-20	IC-20	SAM	01/15/25 16:07		NF IZ	OK
11	IC-R	IC-R	SAM	01/15/25 16:30		NF IZ	OK
12	CCV1	CCV1	CCV	01/29/25 11:41		NF IZ	OK
13	CCB1	CCB1	CCB	01/29/25 12:05		NF IZ	OK
14	LB134464BLW	LB134464BLW	MB	01/29/25 12:52		NF IZ	OK
15	LB134464BSW	LB134464BSW	LCS	01/29/25 13:18		NF IZ	OK
16	Q1168-12	MDL-WATER-06-QT1	SAM	01/29/25 14:06		NF IZ	OK
17	Q1211-01	TAPHHA-MW01-0128	SAM	01/29/25 14:30		NF IZ	OK
18	Q1211-01MS	TAPHHA-MW01-0128	MS	01/29/25 14:55	2.0ml WP111578 +38.0ml Sample	NF IZ	OK

Instrument ID: TOC

Daily Analysis Runlog For Sequence/QC Batch ID # LB134464

Review By	Niha	Review On	1/31/2025 9:24:04 AM
Supervise By	Iwona	Supervise On	1/31/2025 11:12:58 AM
SubDirectory	LB134464	Test	TOC
STD. NAME	STD REF.#		
ICAL Standard	WP111441,WP111442,WP111443,WP111444,WP111445,WP111446		
ICV Standard	WP111448		
CCV Standard	WP111580		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP111581		
Chk Standard	WP111453,WP111454,WP109953,WP111676,WP111677		

19	Q1211-01MSD	TAPHHA-MW01-0128	MSD	01/29/25 15:20	2.0ml WP111578 +38.0ml Sample	NF IZ	OK
20	Q1211-02	TAPIAL2-MW03-0128	SAM	01/29/25 15:47		NF IZ	OK
21	CCV2	CCV2	CCV	01/29/25 16:13		NF IZ	OK
22	CCB2	CCB2	CCB	01/29/25 16:36		NF IZ	OK

Instrument ID: SPECTROPHOTOMETER-1

Daily Analysis Runlog For Sequence/QC Batch ID # LB134466

Review By	rubina	Review On	1/29/2025 3:52:22 PM
Supervise By	Iwona	Supervise On	1/29/2025 4:19:53 PM
SubDirectory	LB134466	Test	Hexavalent Chromium
STD. NAME	STD REF.#		
ICAL Standard	N/A		
ICV Standard	N/A		
CCV Standard	N/A		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	N/A		
Chk Standard	WP111683,WP111682,WP111680,WP111679,WP111659,WP110380,WP111687,WP111681,WP111686,WP111684,WI		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	CAL1	CAL1	CAL	01/29/25 14:30		rubina	OK
2	CAL2	CAL2	CAL	01/29/25 14:31		rubina	OK
3	CAL3	CAL3	CAL	01/29/25 14:32		rubina	OK
4	CAL4	CAL4	CAL	01/29/25 14:33		rubina	OK
5	CAL5	CAL5	CAL	01/29/25 14:34		rubina	OK
6	CAL6	CAL6	CAL	01/29/25 14:35		rubina	OK
7	CAL7	CAL7	CAL	01/29/25 14:36		rubina	OK
8	ICV	ICV	ICV	01/29/25 14:37		rubina	OK
9	ICB	ICB	ICB	01/29/25 14:38		rubina	OK
10	CCV1	CCV1	CCV	01/29/25 14:39		rubina	OK
11	CCB1	CCB1	CCB	01/29/25 14:40		rubina	OK
12	RL Check	RL Check	SAM	01/29/25 14:41		rubina	OK
13	Ib134466BL	Ib134466BL	MB	01/29/25 14:42		rubina	OK
14	Ib134466BS	Ib134466BS	LCS	01/29/25 14:43		rubina	OK
15	Q1168-09	MDL-WATER-03-QT1	SAM	01/29/25 14:44		rubina	OK
16	Q1211-01	TAPHHA-MW01-0128	SAM	01/29/25 14:45		rubina	OK
17	Q1211-01DUP	TAPHHA-MW01-0128	DUP	01/29/25 14:46		rubina	OK
18	Q1211-01MS	TAPHHA-MW01-0128	MS	01/29/25 14:47		rubina	OK

Instrument ID: SPECTROPHOTOMETER-1

Daily Analysis Runlog For Sequence/QC Batch ID # LB134466

Review By	rubina	Review On	1/29/2025 3:52:22 PM
Supervise By	Iwona	Supervise On	1/29/2025 4:19:53 PM
SubDirectory	LB134466	Test	Hexavalent Chromium

STD. NAME	STD REF.#
ICAL Standard	N/A
ICV Standard	N/A
CCV Standard	N/A
ICSA Standard	N/A
CRI Standard	N/A
LCS Standard	N/A
Chk Standard	WP111683,WP111682,WP111680,WP111679,WP111659,WP110380,WP111687,WP111681,WP111686,WP111684,WI

19	Q1211-01MSD	TAPHHA-MW01-0128	MSD	01/29/25 14:48		rubina	OK
20	Q1211-02	TAPIAL2-MW03-0128	SAM	01/29/25 14:49		rubina	OK
21	CCV2	CCV2	CCV	01/29/25 14:50		rubina	OK
22	CCB2	CCB2	CCB	01/29/25 14:51		rubina	OK

Instrument ID: IC-2

Daily Analysis Runlog For Sequence/QC Batch ID # LB134473

Review By	Niha	Review On	1/31/2025 9:14:39 AM
Supervise By	Iwona	Supervise On	1/31/2025 11:12:22 AM
SubDirectory	LB134473	Test	Anions
STD. NAME	STD REF.#		
ICAL Standard	WP111484,WP111485,WP111486,WP111487,WP111488,WP111489,WP111490		
ICV Standard	WP111491		
CCV Standard	WP111689		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP111690		
Chk Standard	WP111492,WP111493		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	STD1	STD1	CAL1	01/20/25 11:14	All standards, samples, and	NF/IZ	OK
2	STD2	STD2	CAL2	01/20/25 11:36	QC are filtered through	NF/IZ	OK
3	STD3	STD3	CAL3	01/20/25 11:57	0.45um, filter lot W3160	NF/IZ	OK
4	STD4	STD4	CAL4	01/20/25 12:18		NF/IZ	OK
5	STD5	STD5	CAL5	01/20/25 12:40		NF/IZ	OK
6	STD6	STD6	CAL6	01/20/25 13:01		NF/IZ	OK
7	STD7	STD7	CAL7	01/20/25 13:23		NF/IZ	OK
8	ICV1	ICV1	ICV	01/20/25 13:44		NF/IZ	OK
9	ICB1	ICB1	ICB	01/20/25 14:06		NF/IZ	OK
10	CCV1	CCV1	CCV	01/29/25 11:15		NF/IZ	OK
11	CCB1	CCB1	CCB	01/29/25 11:37		NF/IZ	OK
12	LB134473BLW	LB134473BLW	MB	01/29/25 11:58		NF/IZ	OK
13	LB134473BSW	LB134473BSW	LCS	01/29/25 12:20		NF/IZ	OK
14	Q1211-01	TAPHHA-MW01-0128	SAM	01/29/25 12:41		NF/IZ	OK
15	Q1211-01MS	TAPHHA-MW01-0128	MS	01/29/25 13:03	9.5ml of sample, 0.5mL W3091	NF/IZ	OK
16	Q1211-01MSD	TAPHHA-MW01-0128	MSD	01/29/25 13:24	9.5ml of sample, 0.5mL W3091	NF/IZ	OK
17	Q1211-02	TAPIAL2-MW03-0128	SAM	01/29/25 13:46		NF/IZ	OK
18	Q1211-01DL	TAPHHA-MW01-0128	SAM	01/29/25 14:07		NF/IZ	OK

Instrument ID: IC-2

Daily Analysis Runlog For Sequence/QC Batch ID # LB134473

Review By	Niha	Review On	1/31/2025 9:14:39 AM
Supervise By	Iwona	Supervise On	1/31/2025 11:12:22 AM
SubDirectory	LB134473	Test	Anions

STD. NAME	STD REF.#
ICAL Standard	WP111484,WP111485,WP111486,WP111487,WP111488,WP111489,WP111490
ICV Standard	WP111491
CCV Standard	WP111689
ICSA Standard	N/A
CRI Standard	N/A
LCS Standard	WP111690
Chk Standard	WP111492,WP111493

19	CCV2	CCV2	CCV	01/29/25 14:29		NF/IZ	OK
20	CCB2	CCB2	CCB	01/29/25 14:51		NF/IZ	OK

Instrument ID: WC SC-3

Daily Analysis Runlog For Sequence/QC Batch ID # LB134521

Review By	jignesh	Review On	2/1/2025 10:36:11 AM
Supervise By	Iwona	Supervise On	2/3/2025 9:31:42 AM
SubDirectory	LB134521	Test	Oil and Grease
STD. NAME	STD REF.#		
ICAL Standard	N/A		
ICV Standard	N/A		
CCV Standard	N/A		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	N/A		
Chk Standard	W3153,M6069,EP2580,WP110826,NA,NA,WP100827,NA,WP100828		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	LB134521BL	LB134521BL	MB	02/01/25 11:30		jignesh	OK
2	LB134521BS	LB134521BS	LCS	02/01/25 11:30		jignesh	OK
3	Q1168-07	LOD-MDL-WATER-01	SAM	02/01/25 11:30	ADD 0.25 WP110827	jignesh	OK
4	Q1168-08	LOQ-WATER-02-QT1	SAM	02/01/25 11:30	ADD 0.0625 WP110828	jignesh	OK
5	Q1211-01	TAPHHA-MW01-0128	SAM	02/01/25 11:30		jignesh	OK
6	Q1211-02	TAPIAL2-MW03-0128	SAM	02/01/25 11:30		jignesh	OK
7	Q1252-01	EFFLUENT	SAM	02/01/25 11:30		jignesh	OK
8	Q1252-02	Q1252-01MS	MS	02/01/25 11:30		jignesh	OK
9	Q1252-03	Q1252-01MSD	MSD	02/01/25 11:30		jignesh	OK

Instrument ID: KONELAB

Daily Analysis Runlog For Sequence/QC Batch ID # LB134532

Review By	rubina	Review On	2/4/2025 8:35:17 AM
Supervise By	Iwona	Supervise On	2/4/2025 10:15:39 AM
SubDirectory	LB134532	Test	Ammonia
STD. NAME	STD REF.#		
ICAL Standard	WP111741		
ICV Standard	WP111743		
CCV Standard	WP111742		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP111420		
Chk Standard	WP110416,WP111745,WP111385,WP111660,WP111744		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	0.0PPM	0.0PPM	CAL1	02/03/25 12:51		rubina	OK
2	0.1PPM	0.1PPM	CAL2	02/03/25 12:51		rubina	OK
3	0.2PPM	0.2PPM	CAL3	02/03/25 12:51		rubina	OK
4	0.4PPM	0.4PPM	CAL4	02/03/25 12:51		rubina	OK
5	1.0PPM	1.0PPM	CAL5	02/03/25 12:51		rubina	OK
6	1.3PPM	1.3PPM	CAL6	02/03/25 12:51		rubina	OK
7	2.0PPM	2.0PPM	CAL7	02/03/25 12:51		rubina	OK
8	ICV1	ICV1	ICV	02/03/25 13:28		rubina	OK
9	ICB1	ICB1	ICB	02/03/25 13:28		rubina	OK
10	CCV1	CCV1	CCV	02/03/25 13:28		rubina	OK
11	CCB1	CCB1	CCB	02/03/25 13:28		rubina	OK
12	RL	RL	SAM	02/03/25 13:29		rubina	OK
13	PB166477BL	PB166477BL	MB	02/03/25 13:29		rubina	OK
14	PB166477BS	PB166477BS	LCS	02/03/25 13:39		rubina	OK
15	Q1168-07	LOD-MDL-WATER-01	SAM	02/03/25 13:39		rubina	OK
16	Q1168-08	LOQ-WATER-02-QT1	LOQ	02/03/25 13:39		rubina	OK
17	Q1211-01	TAPHHA-MW01-0128	SAM	02/03/25 13:39		rubina	OK
18	Q1211-01DUP	TAPHHA-MW01-0128	DUP	02/03/25 13:39		rubina	OK

Instrument ID: KONELAB

Daily Analysis Runlog For Sequence/QC Batch ID # LB134532

Review By	rubina	Review On	2/4/2025 8:35:17 AM
Supervise By	Iwona	Supervise On	2/4/2025 10:15:39 AM
SubDirectory	LB134532	Test	Ammonia
STD. NAME	STD REF.#		
ICAL Standard	WP111741		
ICV Standard	WP111743		
CCV Standard	WP111742		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP111420		
Chk Standard	WP110416,WP111745,WP111385,WP111660,WP111744		

19	Q1211-01MS	TAPHHA-MW01-0128	MS	02/03/25 13:39		rubina	OK
20	Q1211-01MSD	TAPHHA-MW01-0128	MSD	02/03/25 13:50		rubina	OK
21	Q1211-02	TAPIAL2-MW03-0128	SAM	02/03/25 13:50		rubina	OK
22	CCV2	CCV2	CCV	02/03/25 13:50		rubina	OK
23	CCB2	CCB2	CCB	02/03/25 13:50		rubina	OK
24	Q1252-01	EFFLUENT	SAM	02/03/25 13:50	High	rubina	Dilution
25	Q1252-05	INFLUENT	SAM	02/03/25 13:50	High	rubina	Dilution
26	PB166478BL	PB166478BL	MB	02/03/25 13:50		rubina	OK
27	PB166478BS	PB166478BS	LCS	02/03/25 13:59		rubina	OK
28	Q1168-01	LOD-MDL-SOIL-01-Q	SAM	02/03/25 13:59		rubina	OK
29	Q1168-02	LOQ-SOIL-02-QT1-20	LOQ	02/03/25 13:59		rubina	OK
30	CCV3	CCV3	CCV	02/03/25 13:59		rubina	OK
31	CCB3	CCB3	CCB	02/03/25 14:00		rubina	OK
32	Q1252-01DL	EFFLUENTDL	SAM	02/03/25 14:31	Report 10X	rubina	Confirms
33	Q1252-05DL	INFLUENTDL	SAM	02/03/25 14:31	Report 2X	rubina	Confirms
34	CCV4	CCV4	CCV	02/03/25 14:31		rubina	OK
35	CCB4	CCB4	CCB	02/03/25 14:31		rubina	OK

Prep Standard - Chemical Standard Summary

Order ID : Q1211

Test : Ammonia, Anions Group5, Hexavalent Chromium, Oil and Grease, TOC

Prepbatch ID : PB166477,

Sequence ID/Qc Batch ID: LB134464, LB134466, LB134473, LB134521, LB134532,

Standard ID :

EP2580, WP100827, WP100828, WP109953, WP110149, WP110150, WP110259, WP110335, WP110380, WP110416, WP110767, WP110826, WP111315, WP111316, WP111317, WP111318, WP111325, WP111385, WP111419, WP111420, WP111436, WP111437, WP111439, WP111441, WP111442, WP111443, WP111444, WP111445, WP111446, WP111448, WP111449, WP111450, WP111451, WP111452, WP111453, WP111454, WP111484, WP111485, WP111486, WP111487, WP111488, WP111489, WP111490, WP111491, WP111492, WP111493, WP111578, WP111579, WP111580, WP111581, WP111659, WP111660, WP111676, WP111677, WP111678, WP111679, WP111680, WP111681, WP111682, WP111683, WP111684, WP111685, WP111686, WP111687, WP111689, WP111690, WP111741, WP111742, WP111743, WP111744, WP111745, WP99896,

Chemical ID :

E3551, E3854, M5501, M5673, M6041, M6069, M6121, W1992, W1993, W2606, W2647, W2651, W2652, W2666, W2700, W2783, W2784, W2800, W2845, W2858, W2860, W2898, W2979, W3016, W3017, W3020, W3022, W3058, W3062, W3063, W3112, W3113, W3132, W3133, W3153, W3155, W3167, W3169, W3174,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2580	01/17/2025	07/01/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 01/17/2025
FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
114	hexavalent chromium color reagent	WP100827	02/02/2023	02/09/2023	Rubina Mughal	WETCHEM_S CALE_5 (WC SC-5)	None	Iwona Zarych 02/02/2023
FROM 0.25000gram of W2979 + 50.00000ml of W2783 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3456	Cyanide Intermediate Working Std, 5PPM	WP100828	02/02/2023	02/03/2023	Iwona Zarych	None	WETCHEM_FIPETTE_3 (WC)	Sohil Jodhani 02/07/2023
FROM 0.25000ml of W2898 + 49.75000ml of WP99896 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
613	Phosphoric acid reagent	WP109953	09/25/2024	03/25/2025	Niha Farheen Shaik	None	None	Iwona Zarych 09/27/2024
FROM 150.00000ml of W3112 + 50.00000ml of W2860 = Final Quantity: 200.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
153	Ammonia Stock Std. (1000 ppm)	WP110149	10/11/2024	04/08/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 10/14/2024
FROM 3.81900gram of W1993 + 996.18100ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1895	Ammonia Stock Std, 1000PPM-SS	WP110150	10/11/2024	04/08/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 10/14/2024
FROM 3.81900gram of W1992 + 996.18100ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4035	IC ELUENT CONCENTRATE FOR IC-1	WP110259	10/16/2024	04/16/2025	Iwona Zarych	WETCHEM_SCALE_5 (WC SC-5)	None	Jignesh Parikh
FROM 2.10000gram of W2647 + 84.75000gram of W3058 + 913.15000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1597	0.04 N H2SO4	WP110335	10/22/2024	04/22/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych
FROM 1.00000ml of M5673 + 999.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
126	5N sulfuric acid	WP110380	10/24/2024	04/24/2025	Rubina Mughal	None	None	Iwona Zarych
								10/24/2024

FROM 140.00000ml of M5673 + 860.00000ml of W3112 = Final Quantity: 1.000 L

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
740	sodium nitroferricyanide for ammonia	WP110416	10/25/2024	04/25/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych
								10/25/2024

FROM 0.05000gram of W2666 + 99.95000ml of W3112 = Final Quantity: 100.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3886	Inorganic carbon stock solution, 1000ppm	WP110767	11/20/2024	05/20/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC SC-5)	None	Mohan Bera
FROM 3.49700gram of W2647 + 4.41220gram of W3058 + 993.00000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
229	1:1 HCL	WP110826	11/22/2024	05/13/2025	Jignesh Parikh	None	None	Iwona Zarych
FROM 500.00000ml of M6121 + 500.00000ml of W3112 = Final Quantity: 1.000 L								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1993	HEXAVALENTCHROMIUM STOCK STD 1, 50PPM	WP111315	01/09/2025	07/09/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 01/09/2025
FROM 0.14140gram of W2651 + 1000.00000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1994	HEXAVALENTCHROMIUM STOCK STD 2, 50PPM	WP111316	01/09/2025	07/09/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 01/09/2025
FROM 0.14140gram of W2652 + 1000.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1796	NaOH, 0.1N	WP111317	01/09/2025	07/09/2025	Rubina Mughal	WETCHEM_SCALE_7 (WC SC-6)	None	Iwona Zarych 01/09/2025
FROM 4.00000gram of W3113 + 996.00000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1471	NaOH Solution, 6N	WP111318	01/09/2025	07/09/2025	Rubina Mughal	WETCHEM_SCALE_7 (WC SC-6)	None	Iwona Zarych 01/09/2025
FROM 240.00000gram of W3113 + 760.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1494	BORATE BUFFER	WP111325	01/09/2025	07/09/2025	Rubina Mughal	None	None	Iwona Zarych
								01/09/2025

FROM 100.00000L of W3112 + 9.50000gram of W2700 + 88.00000ml of WP111317 = Final Quantity: 100.000 L

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
290	Phenol reagent for Ammonia	WP111385	01/13/2025	07/13/2025	Rubina Mughal	WETCHEM_SCALE_8 (WC SC-7)	None	Iwona Zarych
								01/13/2025

FROM 3.20000gram of W3113 + 8.30000gram of W2858 + 88.80000ml of W3112 = Final Quantity: 100.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1322	Ammonia Intermediate Std, 50PPM	WP111419	01/16/2025	02/16/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 95.00000ml of W3112 + 5.00000ml of WP110149 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1639	Ammonia Intermediate Std-Second source, 50PPM	WP111420	01/16/2025	02/16/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 95.00000ml of W3112 + 5.00000ml of WP110150 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2050	TOC STOCK STD, 4000PPM	WP111436	01/15/2025	07/15/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC)	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 5.00000ml of W2860 + 8.51200gram of W3169 + 990.00000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2051	TOC STOCK STD-SS, 4000PPM	WP111437	01/15/2025	06/30/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC)	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 5.00000ml of W2860 + 8.51200gram of W2784 + 990.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3888	TOC Water Intermediate std-200ppm	WP111439	01/15/2025	01/22/2025	Niha Farheen Shaik	None	None	Iwona Zarych 01/16/2025
FROM 95.00000ml of W3112 + 5.00000ml of WP111436 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
304	TOC CAL 0.00ppm	WP111441	01/15/2025	01/22/2025	Niha Farheen Shaik	None	None	Iwona Zarych 01/16/2025
FROM 100.00000ml of W3112 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
305	TOC CAL 0.5ppm	WP111442	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 99.75000ml of W3112 + 0.25000ml of WP111439 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
306	TOC CAL 1.0PPM	WP111443	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 99.50000ml of W3112 + 0.50000ml of WP111439 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
307	TOC CAL 2.0PPM	WP111444	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 99.00000ml of W3112 + 1.00000ml of WP111439 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
308	TOC CAL 5.0PPM	WP111445	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 97.50000ml of W3112 + 2.50000ml of WP111439 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
310	TOC CAL 20.0PPM	WP111446	01/15/2025	01/22/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/16/2025

FROM 90.00000ml of W3112 + 10.00000ml of WP111439 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2819	TOC ICV-LCSS, 1000PPM	WP111448	01/15/2025	01/22/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/16/2025

FROM 15.00000ml of W3112 + 5.00000ml of WP111437 = Final Quantity: 20.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4003	Solution A	WP111449	01/15/2025	07/15/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 01/16/2025
FROM 1000.00000ml of W3112 + 2.56500gram of W3167 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4004	Solution B	WP111450	01/15/2025	07/15/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 01/16/2025
FROM 0.24800gram of W3020 + 0.28100gram of M5501 + 0.28300gram of W2800 + 0.59400gram of W1992 + 1000.00000ml of W3112 + 2.05000gram of W3017 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4005	Solution C	WP111451	01/15/2025	07/15/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych
FROM 0.70500gram of W3016 + 1000.00000ml of W3112 + 2.80600gram of W2647 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4006	Solution D	WP111452	01/15/2025	07/15/2025	Niha Farheen Shaik	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych
FROM 1.86200gram of W3022 + 1000.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4007	IC-removal check solution	WP111453	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 0.04000ml of M6041 + 10.00000ml of WP111449 + 10.00000ml of WP111450 + 10.00000ml of WP111451 + 10.00000ml of WP111452 = Final Quantity: 40.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3887	Inorganic carbon solution, 20ppm	WP111454	01/15/2025	01/22/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/16/2025
FROM 49.00000ml of W3112 + 1.00000ml of WP110767 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2487	Anions 300/9056 calibration standard 1	WP111484	01/20/2025	01/21/2025	Niha Farheen Shaik	None	None	Iwona Zarych 01/20/2025
FROM 100.00000ml of W3112 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
24	Anions 300/9056 calibration standard 2	WP111485	01/20/2025	01/21/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/20/2025
FROM 0.20000ml of W3063 + 9.80000ml of W3112 = Final Quantity: 10.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
25	Anions 300/9056 calibration standard 3	WP111486	01/20/2025	01/21/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/20/2025
FROM 0.40000ml of W3063 + 9.60000ml of W3112 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
26	Anions 300/9056 calibration standard 4	WP111487	01/20/2025	01/21/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/20/2025
FROM 0.50000ml of W3063 + 9.50000ml of W3112 = Final Quantity: 10.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3680	Anions 300/9056 calibration standard 5-CCV	WP111488	01/20/2025	01/21/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025

FROM 45.00000ml of W3112 + 5.00000ml of W3063 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3679	Anions 300/9056 calibration standard 6	WP111489	01/20/2025	01/21/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025

FROM 2.00000ml of W3063 + 8.00000ml of W3112 = Final Quantity: 10.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3681	Anions 300/9056 calibration standard 7	WP111490	01/20/2025	01/21/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025

FROM 2.50000ml of W3063 + 7.50000ml of W3112 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3233	Anions 300/9056 ICV-LCS std	WP111491	01/20/2025	01/21/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025

FROM 45.00000ml of W3112 + 5.00000ml of W3062 = Final Quantity: 50.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4036	IC ELUENT FOR IC-1	WP111492	01/20/2025	02/20/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025
FROM 1980.00000ml of W3112 + 20.00000ml of WP110259 = Final Quantity: 2000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4037	IC H2SO4 FOR IC-1	WP111493	01/20/2025	02/20/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/20/2025
FROM 5.60000ml of M6041 + 994.40000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3888	TOC Water Intermediate std-200ppm	WP111578	01/23/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/28/2025
FROM 95.00000ml of W3112 + 5.00000ml of WP111436 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3889	TOC Water Intermediate std SS-200ppm	WP111579	01/23/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/28/2025
FROM 95.00000ml of W3112 + 5.00000ml of WP111437 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3331	TOC CAL-CCV std, 10PPM	WP111580	01/23/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/28/2025
FROM 190.00000ml of W3112 + 10.00000ml of WP111578 = Final Quantity: 200.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1650	TOC ICV/LCS STD. 10PPM	WP111581	01/23/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/28/2025
FROM 190.00000ml of W3112 + 10.00000ml of WP111579 = Final Quantity: 200.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
114	hexavalent chromium color reagent	WP111659	01/27/2025	02/03/2025	Rubina Mughal	WETCHEM_SCALE_5 (WC SC-5)	None	Iwona Zarych 01/28/2025
FROM 0.25000gram of W2979 + 50.00000ml of E3854 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
635	EDTA BUFFER FOR AMMONIA	WP111660	01/28/2025	07/28/2025	Rubina Mughal	WETCHEM_SCALE_8 (WC SC-7)	None	Iwona Zarych 01/28/2025
FROM 5.50000gram of W3113 + 50.00000gram of W3132 + 950.00000ml of W3112 = Final Quantity: 1000.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3893	TOC MDL-LOD std, 0.5ppm	WP111676	01/28/2025	01/30/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.75000ml of W3112 + 0.25000ml of WP111578 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3892	TOC Water LOQ std 1.0ppm	WP111677	01/28/2025	01/30/2025	Niha Farheen Shaik	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.50000ml of W3112 + 0.50000ml of WP111578 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1103	HEX CHROME INTERMEDIATE STD SOURCE 1 (5PPM)	WP111678	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_F IPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 9.00000ml of W3112 + 1.00000ml of WP111315 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
110	calibration std. hexchrome 0 ppm	WP111679	01/29/2025	01/30/2025	Rubina Mughal	None	None	Iwona Zarych 01/30/2025
FROM 100.00000ml of W3112 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
109	calibration std. hexchrome 0.01 ppm	WP111680	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.80000ml of W3112 + 0.20000ml of WP111678 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3800	Calibration Std Hexachrome 0.025 ppm	WP111681	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.50000ml of W3112 + 0.50000ml of WP111678 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
108	Calibration Std. hexchrome 0.05 ppm	WP111682	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.00000ml of W3112 + 1.00000ml of WP111678 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
107	Calibration Std. hexchrome 0.1 ppm	WP111683	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.80000ml of W3112 + 0.20000ml of WP111315 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3808	Calibration and CCV std HexChrome 0.5PPM	WP111684	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.00000ml of W3112 + 1.00000ml of WP111315 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3809	Calibration std HexChrome 1.0PPM	WP111685	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 98.00000ml of W3112 + 2.00000ml of WP111315 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3804	Hexavalent Chromium ICV-LCS Std	WP111686	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.00000ml of W3112 + 1.00000ml of WP111316 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1986	HEX LOD STD, 0.005PPM	WP111687	01/29/2025	01/30/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 01/30/2025
FROM 99.90000ml of W3112 + 0.10000ml of WP111678 = Final Quantity: 100.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3680	Anions 300/9056 calibration standard 5-CCV	WP111689	01/29/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/30/2025
FROM 45.00000ml of W3112 + 5.00000ml of W3063 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3233	Anions 300/9056 ICV-LCS std	WP111690	01/29/2025	01/30/2025	Niha Farheen Shaik	None	Glass Pipette-A	Iwona Zarych 01/30/2025
FROM 45.00000ml of W3112 + 5.00000ml of W3062 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
275	Ammonia Calibration Std. (2 ppm)	WP111741	02/03/2025	02/04/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 02/03/2025
FROM 48.00000ml of W3112 + 2.00000ml of WP111419 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
285	Ammonia CCV Std. (1 ppm)	WP111742	02/03/2025	02/04/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 02/03/2025
FROM 49.00000ml of W3112 + 1.00000ml of WP111419 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
286	Ammonia ICV Std. (1 ppm)	WP111743	02/03/2025	02/04/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 02/03/2025
FROM 49.00000ml of W3112 + 1.00000ml of WP111420 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3906	Ammonia MDL-LOD-LOQ spiking solution -5ppm	WP111744	02/03/2025	02/04/2025	Rubina Mughal	None	WETCHEM_FIPETTE_3 (WC)	Iwona Zarych 02/03/2025
FROM 45.00000ml of W3112 + 5.00000ml of WP111419 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
289	Sodium Hypochlorite for Ammonia	WP111745	02/03/2025	07/31/2025	Rubina Mughal	None	None	Iwona Zarych 02/03/2025
FROM 50.00000ml of W3112 + 50.00000ml of W3174 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
11	Sodium hydroxide absorbing solution 0.25 N	WP99896	11/15/2022	05/15/2023	Jignesh Parikh	WETCHEM_SCALE_4 (WC SC-4)	None	Iwona Zarych 11/15/2022
FROM 21.00000L of W2606 + 210.00000gram of W2845 = Final Quantity: 21.000 L								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	1234	03/25/2025	10/30/2024 / Rajesh	10/22/2024 / Rajesh	E3854

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3624-05 / Sodium Chloride, Crystal (cs/4x2.5kg)	0000281938	07/06/2026	07/24/2023 / mohan	04/14/2023 / mohan	M5501

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	23D2462010	03/20/2028	09/21/2023 / mohan	09/05/2023 / mohan	M5673

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	23D2462010	03/20/2028	08/16/2024 / mohan	08/16/2024 / mohan	M6041

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	140440 / TEST PAPERS,PH,0-2.5,.2SENSI, 100PK	80A0441	02/29/2028	09/03/2024 / jignesh	08/19/2024 / Jaswal	M6069

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	0000275677	05/13/2025	11/13/2024 / Eman	10/13/2024 / Eman	M6121

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J0660-1 / AMMONIUM CHLORIDE, ACS, 500G	WL13B	04/08/2025	04/08/2015 / apatel	04/08/2015 / apatel	W1992

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J0660-1 / AMMONIUM CHLORIDE, ACS, 500G	XE09B	04/08/2025	04/08/2015 / apatel	04/08/2015 / apatel	W1993

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	10/24/2024	10/24/2019 / apatel	10/24/2019 / apatel	W2606

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J3506-5 / SODIUM BICARBONATE, PWD, ACS, 2.5KG	0000240594	06/03/2026	02/24/2020 / AMANDEEP	01/20/2020 / apatel	W2647

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	AA13450-36 / Potassium Dichromate, 500g(NEW)	T15F019	01/24/2030	01/24/2020 / apatel	01/24/2020 / apatel	W2651

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	P188-500 / Potassium Dichromate, 500g(new-2nd lot)	194664	01/24/2030	01/24/2020 / apatel	01/24/2020 / apatel	W2652

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	87683 / Sodium Nitroferricyanide 250g	W12F013	02/10/2030	02/10/2020 / apatel	02/10/2020 / apatel	W2666

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J3568-1 / Sodium Borate, 500 gms	2019111354	04/23/2025	04/23/2020 / apatel	03/11/2020 / apatel	W2700

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	0000263246	06/17/2023	12/23/2020 / ketankumar	12/23/2020 / ketankumar	W2783

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	P243-500 / Potassium Hydrogen Phthalate, 500 gms	201089	06/30/2025	12/23/2020 / apatel	12/16/2020 / apatel	W2784

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J3040-1 / POTASSIUM CHLORIDE, CRYST, ACS, 500G	198947	09/30/2025	03/08/2021 / apatel	03/08/2021 / apatel	W2800

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19510-7 / Sodium Hydroxide Pellets 12 Kg	21C2456604	01/31/2024	03/30/2022 / JIGNESH	06/24/2021 / apatel	W2845

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	P1060-10 / PHENOL, ACS, 500G	M13H048	01/07/2026	07/07/2021 / apatel	07/07/2021 / apatel	W2858

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J0260-3 / Phosphoric Acid, 2.5 L	0000278313	01/31/2026	07/12/2021 / apatel	07/12/2021 / apatel	W2860

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Supelco	90157 / Cyanide Standard, 1000ppm from Supelco	HC03107133	06/30/2023	01/24/2022 / apatel	01/24/2022 / apatel	W2898

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	31390 / 1,5-Diphenylcarbazine	MKCR6636	12/09/2027	12/09/2022 / lwona	12/09/2022 / lwona	W2979

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
SIGMA ALDRICH	S9390-100G / Sodium phosphate dibasic heptahydrate	SLCP6576	11/30/2025	04/03/2023 / lwona	04/03/2023 / lwona	W3016

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
SIGMA ALDRICH	C7902-500G / Calcium chloride dihydrate - 500G	SLCP4280	08/31/2025	04/03/2023 / lwona	04/03/2023 / lwona	W3017

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Thermo Fisher Scientific	012364.36 / Calcium nitrate tetrahydrate, ACS, 99.0-103.0%	MKCS4612	09/30/2025	04/03/2023 / lwona	04/03/2023 / lwona	W3020

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
SIGMA ALDRICH	S4392-250G / Sodium metasilicate nonahydrate	SLCM8472	03/31/2025	04/05/2023 / lwona	04/05/2023 / lwona	W3022

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	EM-SX0395-3 / SODIUM CARBONATE ANHYDR 2.5KG	2023012653	10/19/2028	09/03/2024 / jignesh	10/19/2023 / lwona	W3058

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	300-CAL-A-500ML / 300.0 Calibration Standard, 500 ml	T2-MEB716667	02/12/2025	02/12/2024 / lwona	10/30/2023 / lwona	W3062

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	300-CAL-A-500ML / 300.0 Calibration Standard, 500 ml	U2-MEB735684	04/09/2025	04/09/2024 / lwona	11/16/2023 / lwona	W3063

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19510-7 / Sodium Hydroxide Pellets 12 Kg	23B1556310	12/31/2025	07/08/2024 / lwona	07/08/2024 / lwona	W3113

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC05050-1 / EDTA, disodium salt, dihydrate 1 lb	2ND0156	07/10/2026	07/26/2024 / lwona	07/26/2024 / lwona	W3132

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	140476 / Test Paper,PH Short Range 9.0/10.0	L23	08/22/2029	08/22/2024 / lwona	08/22/2024 / lwona	W3133

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	11/25/2024 / jignesh	11/21/2024 / jignesh	W3153

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	140730 / TEST PAPER,POT.IOD-STRCH,P K100,CS12	14-860	12/02/2029	12/02/2024 / lwona	12/02/2024 / lwona	W3155

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J2500-1 / MAGNESIUM SULFATE 7-HYDRATE CRYSTALS 500G	24J2856877	05/29/2027	01/03/2025 / lwona	01/03/2025 / lwona	W3167

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	P243-500 / Potassium Hydrogen Phthalate, 500 gms	24H0956262	04/28/2026	01/03/2025 / lwona	01/03/2025 / lwona	W3169

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J9416-1 / Sodium Hypochlorite 500 ml	2501J28	07/31/2025	01/24/2025 / lwona	01/24/2025 / lwona	W3174

Certificate of Analysis



Date of Release: 12/18/2013

Product: Ammonium Chloride GR ACS

Catalog No.: AX1270 all
size codes

Grade: Meets ACS Specifications

CAS #: 12125-02-9

Country of Origin: India

FW: 53.49

Lot No.: WL13B



Characteristic	Requirement		Results	UOM
	Minimum	Maximum		
Assay (argentometric)	99.5		99.9	%
Calcium (Ca)		0.001	0.0001	%
Form	White crystals		White crystals	
Heavy metals (as Pb)		5	5	ppm
Identification	To pass test		Passes	
Insoluble matter		0.005	0.002	%
Iron (Fe)		2	2	ppm
Loss on drying (105 C)		0.5	0.21	%
Magnesium (Mg)		5	0.6	ppm
pH of a 5% solution at 25 C	4.5	5.5	4.76	
Phosphate (PO4)		2	2	ppm
Residue after ignition		0.01	0.002	%
Sulfate (SO4)		0.002	0.002	%

Joe Schoellkopf

Quality Control Manager

This document has been produced electronically and is valid without a signature.

Certificate of Analysis



Date of Release: 5/12/2014

Product: Ammonium Chloride GR ACS

Catalog No.: AX1270 all
size codes

Grade: Meets ACS Specifications

CAS #: 12125-02-9

Country of Origin: India

FW: 53.49

Lot No.: XE09B



Characteristic	Requirement		Results	UOM
	Minimum	Maximum		
Assay (argentometric)	99.5		99.8	%
Calcium (Ca)		0.001	0.0001	%
Form	White crystals		White crystals	
Heavy metals (as Pb)		5	5	ppm
Identification	To pass test		Passes	
Insoluble matter		0.005	0.002	%
Iron (Fe)		2	2	ppm
Loss on drying (105 C)		0.5	0.22	%
Magnesium (Mg)		5	0.7	ppm
pH of a 5% solution at 25 C	4.5	5.5	4.95	
Phosphate (PO4)		2	2	ppm
Residue after ignition		0.01	0.002	%
Sulfate (SO4)		0.002	0.002	%

Joe Schoellkopf

Quality Control Manager

This document has been produced electronically and is valid without a signature.



Certificate of Analysis

1.19533.0500 Cyanide standard solution traceable to SRM from NIST $K_2[Zn(CN)_4]$ in H_2O
1000 mg/l CN Certipur®
Batch HC03107133

Batch Values

Concentration	β (CN ⁻)	1002	mg/l
---------------	----------------------------	------	------

Determination method: Argentometric titration.

The content of this solution was determined with silver nitrate standard solution (article number 1.09081) standardized against volumetric standard sodium chloride (article number 1.02406). The expanded measurement uncertainty is $\pm 0.7\%$ ($k=2$ coverage factor for 95% coverage probability). The certified value is traceable to primary standard NIST SRM 999c (NIST: National Institute of Standards and Technology, USA) by means of volumetric standard sodium chloride, measured in the accredited calibration laboratory of Merck KGaA, Darmstadt, Germany in accordance to DIN EN ISO/IEC 17025.

Date of release (DD.MM.YYYY) 02.07.2020

Minimum shelf life (DD.MM.YYYY) 30.06.2023

Ayfer Yildirim

Responsible laboratory manager quality control

This document has been produced electronically and is valid without a signature.

Product No.: 13450
Product: Potassium dichromate, ACS, 99.0% min
Lot No.: T15F019

Test	Limits	Results
Appearance	Orange-red crystals	Orange-red crystals
Identification	To Pass	Passes
Purity	99.0 % min	99.67 %
Insoluble matter	0.005 % max	0.004 %
Loss on drying	0.05 % max	0.03 %
Chloride	0.001 % max	< 0.001 %
Sulfate	0.005 % max	< 0.005 %
Iron	0.001 % max	< 0.001 %
Calcium	0.003 % max	0.0012 %
Sodium	0.02 % max	0.0047 %

Order our products online [alfa.com](https://www.thermofisher.com)

This document has been electronically generated and does not require a signature.

This is to certify that units of the lot number above were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the purchaser, formulator or those performing further manufacturing to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The above information is the actual analytical results obtained.

Sodium Bicarbonate, Powder
BAKER ANALYZED® A.C.S. Reagent

(sodium hydrogen carbonate)



Material No.: 3506-05
Batch No.: 0000240594
Manufactured Date: 2019/06/05
Retest Date: 2026/06/03
Revision No: 1

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay (NaHCO ₃) (dried basis)	99.7 – 100.3 %	100.1
Insoluble Matter	<= 0.015 %	< 0.002
Chloride (Cl)	<= 0.003 %	0.003
Phosphate (PO ₄)	<= 0.001 %	0.001
Sulfur Compounds (as SO ₄)	<= 0.003 %	0.003
Calcium (Ca)	<= 0.02 %	0.02
Trace Impurities – Iron (Fe)	<= 0.001 %	0.001
Magnesium (Mg)	<= 0.005 %	0.005
Potassium (K)	<= 0.005 %	0.005
Ammonium (NH ₄)	<= 5 ppm	5
Trace Impurities – ACS – Heavy Metals (as Pb)	<= 5 ppm	5

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

James Ethier
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Acetone
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 0000263246
Manufactured Date: 2020/06/17
Expiration Date: 2023/06/17
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.7
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0000 ppm	0.1000
Substances Reducing Permanganate	Passes Test	PT
Titration Acid (µeq/g)	<= 0.3	0.1
Titration Base (µeq/g)	<= 0.6	< 0.1
Water (H ₂ O)	<= 0.5 %	0.3
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	5

For Laboratory, Research or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: US
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

W2858 Received by AP on 07/07/2021

Product No.: 33213
Product: Phenol, ACS, 99+%, stab.
Lot No.: M13H048

Test	Limits	Results
Assay	99.0 % min	99.8 %
Freezing point	40.5°C min	40.5 °C
Clarity of solution	To pass test	Passes
Residue after evaporation	0.05 % max	< 0.05 %
Water	0.5 % max	0.2 %

Retest date: January 7, 2026

Order our products online [alfa.com](https://www.alfa.com)

This document has been electronically generated and does not require a signature.

This is to certify that units of the lot number above were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the purchaser, formulator or those performing further manufacturing to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The above information is the actual analytical results obtained.

Phosphoric Acid
BAKER ANALYZED® A.C.S. Reagent

(orthophosphoric acid)



Material No.: 0260-03
Batch No.: 0000278313
Manufactured Date: 2021/02/01
Retest Date: 2026/01/31
Revision No: 2

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay (H ₃ PO ₄) (by acidimetry)	85.0 – 87.0 %	85.8
Calcium (Ca)	<= 0.002 %	< 0.001
Color (APHA)	<= 10	5
Insoluble Matter	<= 0.001 %	< 0.001
ACS – Magnesium (Mg)	<= 0.002 %	<0.002
Sulfate (SO ₄)	<= 12 ppm	< 4
Volatile Acids (as CH ₃ COOH)	<= 0.001 %	0.001
Reducing Substances	Passes Test	PT
Chloride (Cl)	<= 3 ppm	< 1
Nitrate (NO ₃)	<= 5 ppm	< 2
Trace Impurities – Antimony (Sb)	<= 20.000 ppm	0.007
Trace Impurities – Arsenic (As)	<= 0.500 ppm	< 0.001
Trace Impurities – Iron (Fe)	<= 10.000 ppm	< 1.000
Heavy Metals (as Pb)	<= 8 ppm	< 3
Trace Impurities – Manganese (Mn)	<= 0.500 ppm	0.005
Trace Impurities – Potassium (K)	<= 40.000 ppm	< 0.001
Trace Impurities – Sodium (Na)	<= 200.000 ppm	0.082

For Laboratory, Research or Manufacturing Use

Exceeds A.C.S. Specifications

Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

W2666 Recived on 02/10/2020 by AP

Product No.: 87683
 Product: Sodium pentacyanonitrosylferrate(III) dihydrate, ACS, 99.0-102.0%
 Lot No.: W12F013

Test	Limits	Results
Assay	99.0 - 102.0 %	99.67 %
Insoluble	0.01 % max	0.0079 %
Chloride	0.02 % max	Not detected
Sulfate	To pass test	Passes test
Aqueous solubility	To pass test	Passes test
Limit on Ferricyanide	To pass test	Passes test
Limit on Ferrocyanide	To pass test	Passes test

 Order our products online [alfa.com](https://www.alfa.com)

This document has been electronically generated and does not require a signature.

This is to certify that units of the lot number above were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the purchaser, formulator or those performing further manufacturing to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The above information is the actual analytical results obtained.

W 3016
Rec 04/03/23 12

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.comEmail USA: techserv@sial.comOutside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:

Sodium phosphate dibasic heptahydrate - ACS reagent, 98.0-102.0%

Product Number: S9390
Batch Number: SLCP6576
Brand: SIGALD
CAS Number: 7782-85-6
MDL Number: MFCD00149180
Formula: $\text{HNa}_2\text{O}_4\text{P} \cdot 7\text{H}_2\text{O}$
Formula Weight: 268.07 g/mol
Quality Release Date: 02 NOV 2022
Recommended Retest Date: NOV 2025

 $\text{Na}_2\text{HPO}_4 \cdot 7\text{H}_2\text{O}$

Test	Specification	Result
Appearance (Color)	White	White
Appearance (Form)	Powder	Powder
Assay	98.0 - 102.0 %	99.8 %
Insoluble Matter	≤ 0.005 %	0.003 %
Chloride (Cl) < or = 0.001%	Pass	Pass
Sulfate < or = 0.005%	Pass	Pass
Iron (Fe) < or = 0.001%	Pass	Pass
Heavy Metals by ICP	< = 0.001%	< 0.001%
pH of 5% solution at 25 deg C	8.7 - 9.3	9.2
Note ACS Tests		



Brian Dulle, Supervisor
Quality Assurance
St. Louis, Missouri US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



W 3017
Rec 4/3/23 12

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.comEmail USA: techserv@sial.comOutside USA: eurtechserv@sial.com

Product Name:

Certificate of Analysis

Calcium chloride dihydrate - BioReagent, suitable for cell culture, suitable for insect cell culture, suitable for plant cell culture, $\geq 99.0\%$

Product Number: C7902



Batch Number: SLCP4280

Brand: SIGMA

CAS Number: 10035-04-8

MDL Number: MFCD00149613

Formula: $\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$

Formula Weight: 147.01 g/mol

Quality Release Date: 14 NOV 2022

Recommended Retest Date: AUG 2025

Test	Specification	Result
Appearance (Color)	White	White
Appearance (Form)	Powder	Powder
Solubility (Color)	Colorless	Colorless
Solubility (Turbidity)	Clear	Clear
294 mg/mL, H ₂ O		
Titration with EDTA	99.0 - 105.0 %	103.3 %
Cell Culture Test	Pass	Pass
Insect Cell Test	Pass	Pass
Plant Cell Culture Test	Pass	Pass



Brian Dulle, Supervisor
Quality Assurance
St. Louis, Missouri US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



W 3020
Rec. 4/3/23

12

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.comEmail USA: techserv@sial.comOutside USA: eurtechserv@sial.com

Product Name:

Certificate of Analysis**Calcium nitrate tetrahydrate - ACS reagent, 99%**

Product Number: 237124
Batch Number: MKCS4612
Brand: SIGALD
CAS Number: 13477-34-4
MDL Number: MFCD00149604
Formula: $\text{CaN}_2\text{O}_6 \cdot 4\text{H}_2\text{O}$
Formula Weight: 236.15 g/mol
Quality Release Date: 27 FEB 2023
Recommended Retest Date: SEP 2025

 $\text{Ca}(\text{NO}_3)_2 \cdot 4\text{H}_2\text{O}$

Test	Specification	Result
Appearance (Color)	White	White
Appearance (Form)	Conforms to Requirements	Crystals
Granular Powder or Crystals or Flakes		
Complexometric EDTA	99.0 - 103.0 %	99.6 %
X-Ray Diffraction	Conforms to Structure	Conforms
pH	5.0 - 7.0	5.4
c = 5%, Water, 25 Deg C		
Insoluble Matter	$\leq 0.005 \%$	$< 0.001 \%$
c = 10%, Water		
Chloride Content	$\leq 0.005 \%$	$< 0.005 \%$
Nitrite (NO_2)	$\leq 0.001 \%$	$< 0.001 \%$
Sulfate (SO_4)	$\leq 0.002 \%$	$< 0.002 \%$
Barium	$\leq 0.005 \%$	$< 0.001 \%$
Heavy Metals	$\leq 5.0 \text{ ppm}$	$< 1.0 \text{ ppm}$
by ICP-OES		
Iron (Fe)	$\leq 5.0 \text{ ppm}$	$< 1.0 \text{ ppm}$
Magnesium (Mg)	$\leq 0.05 \%$	$< 0.01 \%$
Potassium (K)	$\leq 0.005 \%$	$< 0.001 \%$
Sodium (Na)	$\leq 0.01 \%$	$< 0.01 \%$
Strontium (Sr)	$\leq 0.05 \%$	$< 0.01 \%$
Meets ACS Requirements	Current ACS Specification	Conforms

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



W3020

Sigma-Aldrich

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com

Email USA: techserv@sial.com

Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Number: 237124
Batch Number: MKCS4612

Test	Specification	Result
Recommended Retest Period 3 Years		



Larry Coers, Director
Quality Control
Milwaukee, WI US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



W 3022

Rec. 4/5/23 12

3050 Spruce Street, Saint Louis, MO 63103, USA


Website: www.sigmaaldrich.comEmail USA: techserv@sial.comOutside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:

Sodium metasilicate nonahydrate - $\geq 98\%$

Product Number: S4392
Batch Number: SLCM8472
Brand: ALDRICH
CAS Number: 13517-24-3
MDL Number: MFCD00149175
Formula: $\text{Na}_2\text{O}_3\text{Si} \cdot 9\text{H}_2\text{O}$
Formula Weight: 284.20 g/mol
Quality Release Date: 14 MAR 2022
Recommended Retest Date: MAR 2025



Test	Specification	Result
Appearance (Color)	White	White
Appearance (Form)	Powder	Powder
Solubility (Color)	Colorless	Colorless
Solubility (Turbidity)	Clear	Clear
50 mg/ml, H ₂ O		
Titration with HCl	$\geq 98\%$	100 %



Brian Dulle, Supervisor
Quality Assurance
St. Louis, Missouri US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



Certificate Of Analysis



W 3058

Re. 10/19/23 12

Date of Release: 1/27/2023

Name: **Sodium Carbonate, Anhydrous**

Powder, ACS

Item No: **SX0395 All Sizes**

Lot / Batch No: **2023012653**

Country of Origin: **India**

Item	Specifications	Analysis
Assay (calculated on dried substance)	99.5% min.	100.2%
Calcium (Ca)	0.03% max.	0.004%
Chloride (Cl)	0.001% max.	<0.001%
Color	White	Passes Test
Form	Powder	Passes Test
Heavy metals (by ICP-OES)	5 ppm max.	<5 ppm
Insoluble Matter	0.01% max.	0.003%
Iron (Fe)	5 ppm max.	<5 ppm
Loss on heating at 285C	1.0% max.	0.1%
Magnesium (Mg)	0.005% max.	0.0008%
Phosphate (PO ₄)	0.001% max.	<0.001%
Potassium (K)	0.005% max.	0.003%
Silica (SiO ₂)	0.005% max.	<0.005%
Sulfur compounds (as SO ₄)	0.003% max.	<0.003%

Joe Schoellkopf

Quality Control Manager

This document has been produced electronically and is valid without a signature.

EMD Millipore is a division of Merck KGaA, Darmstadt, Germany

EMD Millipore Corporation

400 Summit Drive
Burlington, MA 01803
U.S.A.

Form number: 00005624CA, Rev. 2.0

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

N 3062

rec on 10/30/23
12

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Ion Chromatography Solution
Catalog Number: 300-CAL-A
Lot Number: T2-MEB716667
Matrix: H₂O
Value / Analyte(s):
150 µg/mL ea:
Sulfate,
100 µg/mL ea:
Bromide,
50 µg/mL ea:
o-Phosphate as P,
30 µg/mL ea:
Chloride, Nitrite as N,
25 µg/mL ea:
Nitrate as N,
20 µg/mL ea:
Fluoride

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Bromide, Br	100.0 ± 0.5 µg/mL	Chloride, Cl	30.00 ± 0.13 µg/mL
Fluoride, F-	20.00 ± 0.06 µg/mL	Nitrate as N, NNO ₃ -	25.00 ± 0.09 µg/mL
Nitrite as N, NNO ₂ -	30.00 ± 0.15 µg/mL	o-Phosphate as P, PPO ₄	50.00 ± 0.30 µg/mL
Sulfate, SO ₄	150.0 ± 0.9 µg/mL		

Density: 0.999 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Br	IC Assay	3184	151130
Br	Fajans	999c	999c
Cl	IC Assay	3182	060925
Cl	Fajans	999c	999c
Cl	Calculated		See Sec. 4.2
F-	IC Assay	3183	140203
NNO3-	IC Assay	3185	050517
NNO2-	IC Assay		traceable to 40h
PPO4	IC Assay	3186	170606
SO4	IC Assay	3181	080603

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum (1/(u_{char i}^2)))$$

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum ((w_i)^2 (u_{char i}^2))]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k (u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 CHROMATOGRAM

N/A

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

March 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **March 17, 2027**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

W3063
rec. 11/16/23 12

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Ion Chromatography Solution
Catalog Number: 300-CAL-A
Lot Number: U2-MEB735684
Matrix: H₂O
Value / Analyte(s):
150 µg/mL ea:
Sulfate,
100 µg/mL ea:
Bromide,
50 µg/mL ea:
o-Phosphate as P,
30 µg/mL ea:
Chloride, Nitrite as N,
25 µg/mL ea:
Nitrate as N,
20 µg/mL ea:
Fluoride

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Bromide, Br	100.0 ± 0.5 µg/mL	Chloride, Cl	30.00 ± 0.14 µg/mL
Fluoride, F-	20.00 ± 0.06 µg/mL	Nitrate as N, NNO ₃ -	25.00 ± 0.09 µg/mL
Nitrite as N, NNO ₂ -	30.00 ± 0.15 µg/mL	o-Phosphate as P, PPO ₄	50.00 ± 0.18 µg/mL
Sulfate, SO ₄	150.0 ± 0.8 µg/mL		

Density: 0.999 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Br	IC Assay	3184	151130
Br	Fajans	999c	999c
Cl	IC Assay	3182	190830
Cl	Fajans	999c	999c
F-	IC Assay	3183	140203
NNO3-	IC Assay	3185	170309
NNO2-	IC Assay		traceable to 40h
PPO4	IC Assay	3186	170606
SO4	IC Assay	3181	080603

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum(1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k(u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum(w_i)^2(u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a)(u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k(u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 CHROMATOGRAM

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

August 10, 2023

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **August 10, 2028**

- The date after which this CRM/RM should not be used.
- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____
- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0

NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Justin Dirico
Stock Processing Supervisor



Certificate Approved By:

Nicholas Plymale
Custom VSM Coordinator



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate Of Analysis



Date of Release: 11/14/2019

W2700 Recived by AP on 3/11/2020

Name: **Sodium Borate, Decahydrate**
ACS

Item No: **SX0355 All Sizes**

Lot / Batch No: **2019111354**

Country of Origin: **India**

Item	Specifications	Analysis
Assay (Na ₂ B ₄ O ₇ • 10H ₂ O)	99.5 - 105.0%	101.7%
Calcium (Ca)	0.005% max.	0.003%
Chloride (Cl)	0.001% max.	<0.001%
Color	White	Passes Test
Form	Crystals	Passes Test
Heavy Metals (as Pb)	0.001% max.	<0.001%
Insoluble Matter	0.005% max.	0.002%
Iron (Fe)	5 ppm max.	<5 ppm
pH of a 0.01 M solution at 25C	9.15 - 9.20	9.17
Phosphate (PO ₄)	0.001% max.	<0.001%
Sulfate (SO ₄)	0.005% max.	<0.005%

Joe Schoellkopf

Quality Control Manager

This document has been produced electronically and is valid without a signature .

EMD Millipore is a division of Merck KGaA, Darmstadt, Germany

EMD Millipore Corporation

400 Summit Drive
Burlington, MA 01803
U.S.A.

Form number: 00005624CA, Rev. 2.0

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120632

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	P217	Quality Test / Release Date	09/03/2020
Lot Number	198947		
Description	POTASSIUM CHLORIDE, A.C.S.		
Country of Origin	United States	Suggested Retest Date	Sep/2025
Chemical Origin	Inorganic-non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	White crystals
ASSAY	%	Inclusive Between 99.0 - 100.5	99.7
BARIUM (Ba)	PASS/FAIL	= P.T. (ABOUT 0.001%)	P.T. (ABOUT 0.001%)
BROMIDE	%	<= 0.01	<0.01
CALCIUM	%	<= 0.002	<0.002
CHLORATE & NITRATE	%	<= 0.003	<0.001
HEAVY METALS (as Pb)	ppm	<= 5	<5
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
INSOLUBLE MATTER	%	<= 0.005	<0.005
IODIDE	%	<= 0.002	<0.002
IRON (Fe)	ppm	<= 2	<1
MAGNESIUM	%	<= 0.001	<0.0005
PH 5% SOLUTION @ 25 DEG C		Inclusive Between 5.4 - 8.6	6.0
PHOSPHATE (PO4)	ppm	<= 5	<5
SODIUM (Na)	%	<= 0.005	<0.005
SULFATE (SO4)	%	<= 0.001	<0.001

Julian Burton

Julian Burton - Quality Control Manager – Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
 If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.



Certificate of Analysis

1 Reagent Lane
Fair Lawn, NJ 07410
201.796.7100 tel
201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120632

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	P188	Quality Test / Release Date	08/12/2019
Lot Number	194664		
Description	POTASSIUM DICHROMATE, A.C.S.		
Country of Origin	United States	Suggested Retest Date	Aug/2024
Chemical Origin	Inorganic-non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		
Chemical Comment			

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Fine, orange-red crystals
ASSAY	%	>= 99	99.2
CALCIUM	%	<= 0.003	<0.003
CHLORIDE	%	<= 0.001	<0.001
LOSS ON DRYING @ 105 C	%	<= 0.05	<0.05
SULFATE (SO4)	%	<= 0.005	<0.005
INSOLUBLE MATTER	%	<= 0.005	0.003
IRON (Fe)	%	<= 0.001	<0.001
SODIUM (Na)	%	<= 0.02	<0.02
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST

Jerusa Bailey-Wyche

Quality Assurance Specialist - Certificate of Analysis Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Certificate of Analysis

ThermoFisher
SCIENTIFIC

Certificate of Analysis

1 Reagent Lane
Fair Lawn, NJ 07410
201.796.7100 tel
201.796.1329 faxThermo Fisher Scientific's Quality System has been found to conform to Quality Management System
Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120632

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	P243	Quality Test / Release Date	06/19/2020
Lot Number	201089		
Description	POTASSIUM HYDROGEN PHTHALATE, ACIDIMETRIC STANDARD, A.C.S.		
Country of Origin	Spain	Suggested Retest Date	Jun/2025
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	WHITE CRYSTALS
ASSAY POTASSIUM HYDROGEN PHTHALATE	%	Inclusive Between 99.95 - 100.05	100.03
CHLORINE COMPOUNDS	%	<= 0.003	<0.003
HEAVY METALS (as Pb)	ppm	<= 5	<5
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
INSOLUBLE MATTER	%	<= 0.005	<0.005
IRON (Fe)	ppm	<= 5	<5
PH OF 0.05M SOLUTION		Inclusive Between 4.00 - 4.02	4.00
SODIUM (Na)	%	<= 0.005	<0.005
SULFUR COMPOUNDS	%	<= 0.002	<0.002%
TRACEABLE TO NIST	SOD CARBONATE	= LOT 351a	351a
TRACEABLE TO NIST KHP STD	POT. ACID PHTHALATE	= LOT 84L	84L



Julian Burton - Quality Control Manager – Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %
COMMENTS		
QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Sodium Chloride, Crystal
BAKER ANALYZED® A.C.S. Reagent



M5497 - M5508
And on 4/14/23
063

Material No.: 3624-01

Batch No.: 0000281938

Manufactured Date: 2021-06-07


Retest Date: 2026-06-07

Revision No.: 2

Certificate of Analysis

Test	Specification	Result
Assay (NaCl) (by Ag titrn)	≥ 99.0 %	100.0 %
pH of 5% Solution at 25°C	5.0 - 9.0	6.3
Insoluble Matter	≤ 0.005 %	0.003 %
Iodide (I)	≤ 0.002 %	< 0.002 %
Bromide (Br)	≤ 0.01 %	< 0.01 %
Chlorate and Nitrate (as NO ₃)	≤ 0.003 %	< 0.001 %
ACS - Phosphate (PO ₄)	≤ 5 ppm	< 5 ppm
Sulfate (SO ₄)	≤ 0.004 %	< 0.004 %
Barium (Ba)	Passes Test	Passes Test
ACS - Heavy Metals (as Pb)	≤ 5 ppm	< 5 ppm
Iron (Fe)	≤ 2 ppm	< 1 ppm
Calcium (Ca)	≤ 0.002 %	< 0.001 %
Magnesium (Mg)	≤ 0.001 %	< 0.001 %
Potassium (K)	≤ 0.005 %	0.001 %

For Laboratory, Research, or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs
Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

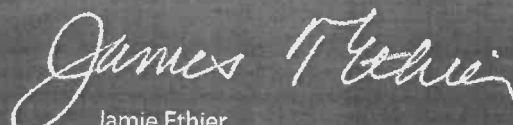
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



Material No.: 9673-33
Batch No.: 23D2462010
Manufactured Date: 2023-03-22
Retest Date: 2028-03-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.1 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO ₂)	≤ 2 ppm	< 2 ppm
Ammonium (NH ₄)	≤ 1 ppm	1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO ₃)	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO ₄)	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	8.5 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	0.5 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	1.3 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.8 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	< 0.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	31.5 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium




Material No.: 9673-33
Batch No.: 23D2462010

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	5.4 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 0.2 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.4 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

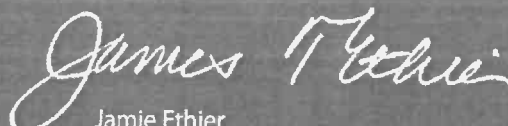
Jamie Ethier
Vice President Global Quality

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



M 6041-4b
MS

Material No.: 9673-33
Batch No.: 23D2462010
Manufactured Date: 2023-03-22
Retest Date: 2028-03-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.1 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO ₂)	≤ 2 ppm	< 2 ppm
Ammonium (NH ₄)	≤ 1 ppm	1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO ₃)	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO ₄)	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	8.5 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	0.5 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	1.3 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.8 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	< 0.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	31.5 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

 **avantor™**




Material No.: 9673-33
Batch No.: 23D2462010

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	5.4 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 0.2 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.4 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

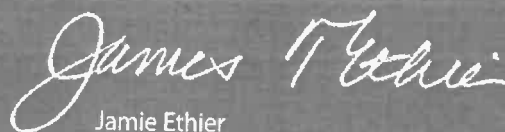

Jamie Ethier
Vice President Global Quality

Certificate of Analysis

Product information

Product	pH-Fix 0.3-2.3
REF	92180
LOT	80A0441
Expiration date:	29.02.2028
Date of examination:	23.01.2024
Gradation:	pH 0.3-0.7-1.0-1.3-1.6-1.9-2.3

Confirmation

Hereby we confirm, that the above mentioned product has successfully passed our quality control system in accordance with ISO 9001 and meets the specific quality criteria.

This document has been produced electronically and is valid without a signature.

Hydrochloric Acid, 36.5-38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



R → 16/13/24
Met dig

M 6121

Material No.: 9530-33
Batch No.: 0000275677
Manufactured Date: 2020/12/16
Retest Date: 2025/12/15
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 - 38.0 %	37.6
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Specific Gravity at 60°/60°F	1.185 - 1.192	1.190
ACS - Bromide (Br)	<= 0.005 %	< 0.005
ACS - Extractable Organic Substances	<= 5 ppm	1
ACS - Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities - Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities - Aluminum (Al)	<= 10.0 ppb	< 0.2
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities - Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities - Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	29.7
Trace Impurities - Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	< 0.2
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	< 1
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.1
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.3
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use
Product Information (not specifications):
Appearance (clear, fuming liquid)
Meets ACS Specifications

Country of Origin: US
Packaging Site: Phillipsburg Mfg Ctr & DC

James Ethier
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

W 2979

Rec: 12/09/22

exp. 12/09/27

Product Name:

1,5-Diphenylcarbazide - ACS reagent

Product Number:

259225

Batch Number:

MKCR6636

Brand:

SIAL

CAS Number:

140-22-7

MDL Number:

MFCD00003013

Formula:

C₁₃H₁₄N₄O


Formula Weight:

242.28 g/mol

Quality Release Date:

02 JUN 2022

Certificate of Analysis



Test	Specification	Result
Appearance (Color)	Conforms to Requirements	Pink
Off-White to Pink, Light Purple or Tan		
Appearance (Form)	Powder or Chunks	Powder
Melting Point	173.0 - 176.0 °C	173.0 °C
Infrared Spectrum	Conforms to Structure	Conforms
Residue on ignition (Ash)	≤ 0.05 %	0.01 %
15 minutes, 800 Degrees Celsius		
Solubility	Pass	Pass
Sensitivity Test	Pass	Pass
Meets ACS Requirements	Current ACS Specification	Conforms



Larry Coers, Director
Quality Control
Milwaukee, WI US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



Sodium Hydroxide (Pellets)

Material: 0583
Grade: ACS GRADE
Batch Number: 23B1556310

Chemical Formula: NaOH
Molecular Weight: 40
CAS #: 1310-73-2
Appearance:

Manufacture Date: 12/14/2022
Expiration Date: 12/31/2025

Storage: Room Temperature

Pellets

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Calcium	<= 0.005 %	<0.005 %	PASS
Chloride	<= 0.005 %	0.002 %	PASS
Heavy Metals	<= 0.002 %	<0.002 %	PASS
Iron	<= 0.001 %	<0.001 %	PASS
Magnesium	<= 0.002 %	<0.002 %	PASS
Mercury	<= 0.1 ppm	<0.1 ppm	PASS
Nickel	<= 0.001 %	<0.001 %	PASS
Nitrogen Compounds	<= 0.001 %	<0.001 %	PASS
Phosphate	<= 0.001 %	<0.001 %	PASS
Potassium	<= 0.02 %	<0.02 %	PASS
Purity	>= 97.0 %	99.2 %	PASS
Sodium Carbonate	<= 1.0 %	0.5 %	PASS
Sulfate	<= 0.003 %	<0.003 %	PASS

Internal ID #: 710

Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.



Sodium Hydroxide (Pellets)

Material: 0583
Grade: ACS GRADE
Batch Number: 23B1556310

Chemical Formula: NaOH
Molecular Weight: 40
CAS #: 1310-73-2
Appearance:

Manufacture Date: 12/14/2022
Expiration Date: 12/31/2025

Storage: Room Temperature

Pellets

Spec Set: 0583ACS

Internal ID #: 710

Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.

Item Number	ED150	Lot Number	2ND0156
Item	Edetate Disodium, Dihydrate, USP	CAS Number	6381-92-6
Molecular Formula	C ₁₀ H ₁₄ N ₂ Na ₂ O ₈ •2H ₂ O	Molecular Weight	372.24

TEST	SPECIFICATION		RESULT
	MIN	MAX	
ASSAY (DRIED BASIS)	99.0	101.0 %	99.5 %
pH OF A 5% SOLUTION @ 25°C	4.0	6.0	4.6
LOSS ON DRYING	8.7	11.4 %	8.90 %
CALCIUM (Ca)	NO PRECIPITATE IS FORMED		NO PRECIPITATE IS FORMED
ELEMENTAL IMPURITIES:			.
NICKEL (Ni)	AS REPORTED		<0.3 ppm
CHROMIUM (Cr)	AS REPORTED		<0.3 ppm
NITRILOTRIACETIC ACID[n[(HOCOCH ₂) ₃ N]		0.1 %	<0.10 %
IDENTIFICATION A	MATCHES REFERENCE		MATCHES REFERENCE
IDENTIFICATION B	RED COLOR IS DISCHARGED, LEAVING A YELLOWISH SOLUTION		RED COLOR IS DISCHARGED, LEAVING A YELLOWISH SOLUTION
IDENTIFICATION C	MEETS THE REQUIREMENTS FOR SODIUM		MEETS THE REQUIREMENTS FOR SODIUM
CERTIFIED HALAL			CERTIFIED HALAL
EXPIRATION DATE			10-JUL-2026
DATE OF MANUFACTURE			11-JUL-2023
APPEARANCE			WHITE CRYSTALLINE POWDER
RESIDUAL SOLVENTS		AS REPORTED	NO RESIDUAL SOLVENTS PRESENT
MONOGRAPH EDITION			USP 2024

Certificate of Analysis Results Entered By:

CACEVEDO
Charmian Acevedo
22-MAY-24 08:12:30

Spectrum Chemical Mfg Corp
755 Jersey Avenue
New Brunswick 08901 NJ



Certificate of Analysis Results Approved By:

GHERRERA
Genaro Herrera
22-MAY-24 12:32:01

All pharmaceutical ingredients are tested using current edition of applicable pharmacopeia.

Read and understand label and SDS before handling any chemicals. All Spectrum's chemicals are for manufacturing, processing, repacking or research purposes by experienced personnel only. It is the customer's responsibility to provide adequate hazardous material training and ensure that appropriate Personal Protective Equipment (PPE) is used before handling any chemical.

The Elemental Impurities standards implemented by USP and other Pharmaceutical Compendia reflect a growing understanding of the toxicology of trace levels of elemental impurities that can remain in drug substances originating from either raw materials or manufacturing processes. Identifying and quantifying impurities can be critical to predicting the best possible patient outcomes. Elemental Impurities has been a requirement of all products meeting USP/NF, EP and BP monographs since January 1, 2018. More information can be found in USP sections <232> Elemental Impurities – Limits and <233> Elemental Impurities – Procedures. Data for drug substances furnished by Spectrum Chemical Mfg. Corp can be used to ensure that patient daily exposures by oral administration to the selected elements are not exceeded in the formulation of pharmaceutical products.

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



WJ3153
SB
0844e. 11/25/2024
SB

Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Magnesium Sulfate Heptahydrate

Material: 0662
Grade: ACS GRADE
Batch Number: 24J2856877

Chemical Formula: $\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$
Molecular Weight: 246.48
CAS #: 10034-99-8
Appearance:

Manufacture Date: 05/29/2023
Reassay Date: 05/29/2027

Storage: Room Temperature

White powder

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Ammonium	$\leq 0.002 \%$	$< 0.001 \%$	PASS
Calcium	$\leq 0.02 \%$	$< 0.0005 \%$	PASS
Chloride	$\leq 0.0005 \%$	0.0001%	PASS
Heavy Metals (as Pb)	$\leq 0.0005 \%$	$< 0.0001 \%$	PASS
Insolubles	$\leq 0.005 \%$	$< 0.0002 \%$	PASS
Iron	$\leq 0.0005 \%$	$< 0.00001 \%$	PASS
Manganese	$\leq 0.0005 \%$	$< 0.0001 \%$	PASS
Nitrate	$\leq 0.002 \%$	$< 0.001 \%$	PASS
pH (5%, Water) @25C	5.0 - 8.2	6.3	PASS
Potassium	$\leq 0.005 \%$	$< 0.001 \%$	PASS
Purity	98.0 - 102.0 %	100.1 %	PASS
Sodium	$\leq 0.005 \%$	$< 0.001 \%$	PASS
Strontium	$\leq 0.005 \%$	$< 0.00001 \%$	PASS

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits. Product meets analytical specifications of the grades listed.



Magnesium Sulfate Heptahydrate

Material: 0662
Grade: ACS GRADE
Batch Number: 24J2856877

Chemical Formula: $\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$
Molecular Weight: 246.48
CAS #: 10034-99-8
Appearance:

Manufacture Date: 05/29/2023
Reassay Date: 05/29/2027

Storage: Room Temperature

White powder

Spec Set: 0662ACS

Internal ID #: 793

Signature	Additional Information
We certify that this batch conforms to the specifications listed.	Analysis may have been rounded to significant digits in specification limits.
This document has been electronically produced and is valid without a signature.	Product meets analytical specifications of the grades listed.
Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	





Material	BDH9260-500G
Material Description	BDH POTASS HYDRGN PHTHLTE 500G
Grade	ACS GRADE
Batch	24H0956262
Reassay Date	04/28/2026
CAS Number	877-24-7
Molecular Formula	HOCC6H4COOK
Molecular Mass	204.22
Date of Manufacture	04/29/2023
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	White crystals.	White crystals.
Assay (dried basis)	99.95 - 100.05 %	99.98 %
Chlorine Compounds	<= 0.003 %	<0.003 %
Heavy Metals (as Pb)	<= 5 ppm	<5 ppm
Insoluble Matter	<= 0.005 %	0.003 %
Iron	<= 5 ppm	<5 ppm
pH (0.05M, Water) @25C	4.00 - 4.02	4.00
Sodium	<= 0.005 %	<0.005 %
Sulfur Compounds	<= 0.002 %	<0.002 %

Internal ID #: 322

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.

Certificate of Analysis

Sodium Hypochlorite Solution, 5% available Chlorine

Lot Number: 2501J28

Product Number: 7495.5

Manufacture Date: JAN 17, 2025

Expiration Date: JUL 2025

This solution is subject to slow decomposition upon exposure to air. Keep container tightly capped. Refrigeration may improve stability.
When used in the Phenate method for Ammonia, APHA recommends replacing this solution about every 2 months.

Name	CAS#	Grade
Water	7732-18-5	Commercial
Sodium Hypochlorite	7681-52-9	Commercial

Test	Specification	Result	NIST SRM#
Appearance	Colorless to greenish-yellow liquid	Passed	
Assay (vs. Sodium Thiosulfate/Starch)	4.75-5.25 % (w/w) Cl ₂	5.17 % (w/w) Cl ₂	136

Specification	Reference
Sodium Hypochlorite, 5%	APHA (4500-NH3 F)
Sodium Hypochlorite	ASTM (D 4785)

Volumetric glassware complies with Class A tolerance requirements of ASTM E 288 and NIST Circular 434; it is calibrated before first use and recalibrated regularly in accordance with ASTM E 542 and NIST Procedure NBSIR 74-461. Balances are calibrated regularly with weights certified traceable to the NIST national mass standard. Thermometers and temperature probes are calibrated before first use and recalibrated regularly with a thermometer traceable to NIST standards. All products are prepared according to master documents that assure manufacture according to validated methods. Batch records document raw material traceability and production and testing history for each lot manufactured.

Part Number	Size / Package Type	Shelf Life (Unopened Container)
7495.5-1	4 L black poly	6 months
7495.5-16	500 mL amber poly	6 months
7495.5-32	1 L amber poly	6 months
7495.5-8	250 mL amber poly	6 months

Recommended Storage: 15°C - 30°C (59°F - 86°F)



Jose Pena (01/17/2025)
Operations Manager

This test report shall not be reproduced, except in full, without the written approval of Ricca Chemical Company.



SHIPPING DOCUMENTS

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13

Q1211



Weston COC ID
Weston_20250128_1605

Chain of Custody Record/Lab Work Request

Page	1	of	1
------	---	----	---

Client:	Weston Solutions, Inc.		
Project Manager:	David Sembrot		
Street Address:	1400 Weston Way	City:	West Chester
Phone:	610-314-5456	ST, ZIP:	PA, 19038
e-mail:	david.sembrot@westonsolutions.com		
Sampled By:	Cheyenne Harrington		

Project Name:	Fort Meade RI	Project POC:	Nathan Fretz
PO Number	0111169	Phone:	484-524-5665
W.O. #:		POC e-mail:	nathan.fretz@westonsolutions.com
Lab:	CHEMTECH	Lab POC:	Yazmeen Gomez
TAT (days):	21	Lab Phone:	908-728-3144
Lab Address:	284 Sheffield Street Mountainside, NJ 07092		

Matrix Codes
SS - Soil
SE - Sediment
SO - Solid
SL - Sludge
GW - Groundwater
W - Water
SB - Soil Boring
A - Air
DS - Drum Solids
DL - Drum Liquids
L - EP/TCLP Leachate
WI - Wipe
X - Other
F - Fish

Lab Use Only		
Temperature of cooler when received (°C)		
COC Tape was present and unbroken on outer package?	Y	N
Samples received in good condition?	Y	N
Labels indicate properly preserved?	Y	N
Received within holding times?	Y	N
Discrepancies between sample labels and COC record?	Y	N

Analyses Requested:	DRO by EPA 8015D	Pesticides by EPA 8081B	SVOCs by EPA 8270E	O&G by EPA 1664A	Hardness by EPA 200	Anions by EPA 9056A	TOC by EPA 9060A/Lloyd Kahn	GRO by EPA 8015D	VOCs by EPA 8260D	Hex Cr by EPA	Ammonia by SM4500-NH3 B P	Metals w/ Hg by EPA 6020B/17470A
Container Type:	Amber	Amber	Amber	Glass	Plastic	Plastic	Vial	Vial	Vial	Plastic	Plastic	Plastic
Container Size:	1 L	1 L	1 L	1 L	1 L	1 L	40 mL	40 mL	40 mL	500 mL	500 mL	500 mL
Preservative:	Ice to 0-6	Ice to 0-6	Ice to 0-6	H2SO4 to <	HNO3 to pH	Ice to 0-6	H2SO4 to <	HCL to PH	HCL to Ph	Ammonium	H2SO4: Ice	HNO3 to pH

#	Sample ID	G/C	Matrix	# Cont	MS/MSD	Date Collected	Time Collected													Special Instructions/Comments
1	TAPHHA-MW01-012825-00-T4	g	GW	19	no	1/28/2025	12:00	X	X	X	X	X	X	X	X	X	X	X	X	
2	TAPIAL2-MW03-012825-00-T3	g	GW	19	no	1/28/2025	14:55	X	X	X	X	X	X	X	X	X	X	X	X	
3	TAP-TB-02-012825-T4	g	W	2	no	1/28/2025	12:05								X					
4																				
5																				
6																				
7																				
8																				
9																				
10																				
11																				
12																				

Shipping Airbill Number: 77173295 4230, 77173295 4240						Cooler Number: 1/2 of 2		
Relinquished By		Date	Time	Received By		Date	Time	Additional Comments
1.)	[Signature]	1/28/25	1710	[Signature]		1-29-25	10:00	
2.)								
3.)								

2.1", 2.3"

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1211	WEST04	Order Date : 1/29/2025 10:10:00 AM	Project Mgr :
Client Name : Weston Solutions		Project Name : Ft Meade Tipton Airfield Pa	Report Type : Level 4
Client Contact : Nathan Fretz		Receive DateTime : 1/29/2025 10:00:00 AM	EDD Type : SEDD 2A
Invoice Name : Weston Solutions		Purchase Order :	Hard Copy Date :
Invoice Contact : Nathan Fretz			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1211-01	TPHHA-MW01-012825-00-T4 TAPHHA YG 02/04/25	Water	01/28/2025	12:00	VOC-TCLVOA-10		8260D	10 Bus. Days	
Q1211-02	TAPIAL2-MW03-012825-00-T3	Water	01/28/2025	14:55	VOC-TCLVOA-10		8260D	10 Bus. Days	
Q1211-03	TAP-TB-02-012825-T4	Water	01/28/2025	12:05	VOC-TCLVOA-10		8260D	10 Bus. Days	

Relinquished By : CP

Date / Time : 1-29-25 1125

Received By : Sams

Date / Time : 1/29/25 11:25 NGH 5

Storage Area : VOA Refridgerator Room