


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141318.D
Acq On : 31 Jan 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

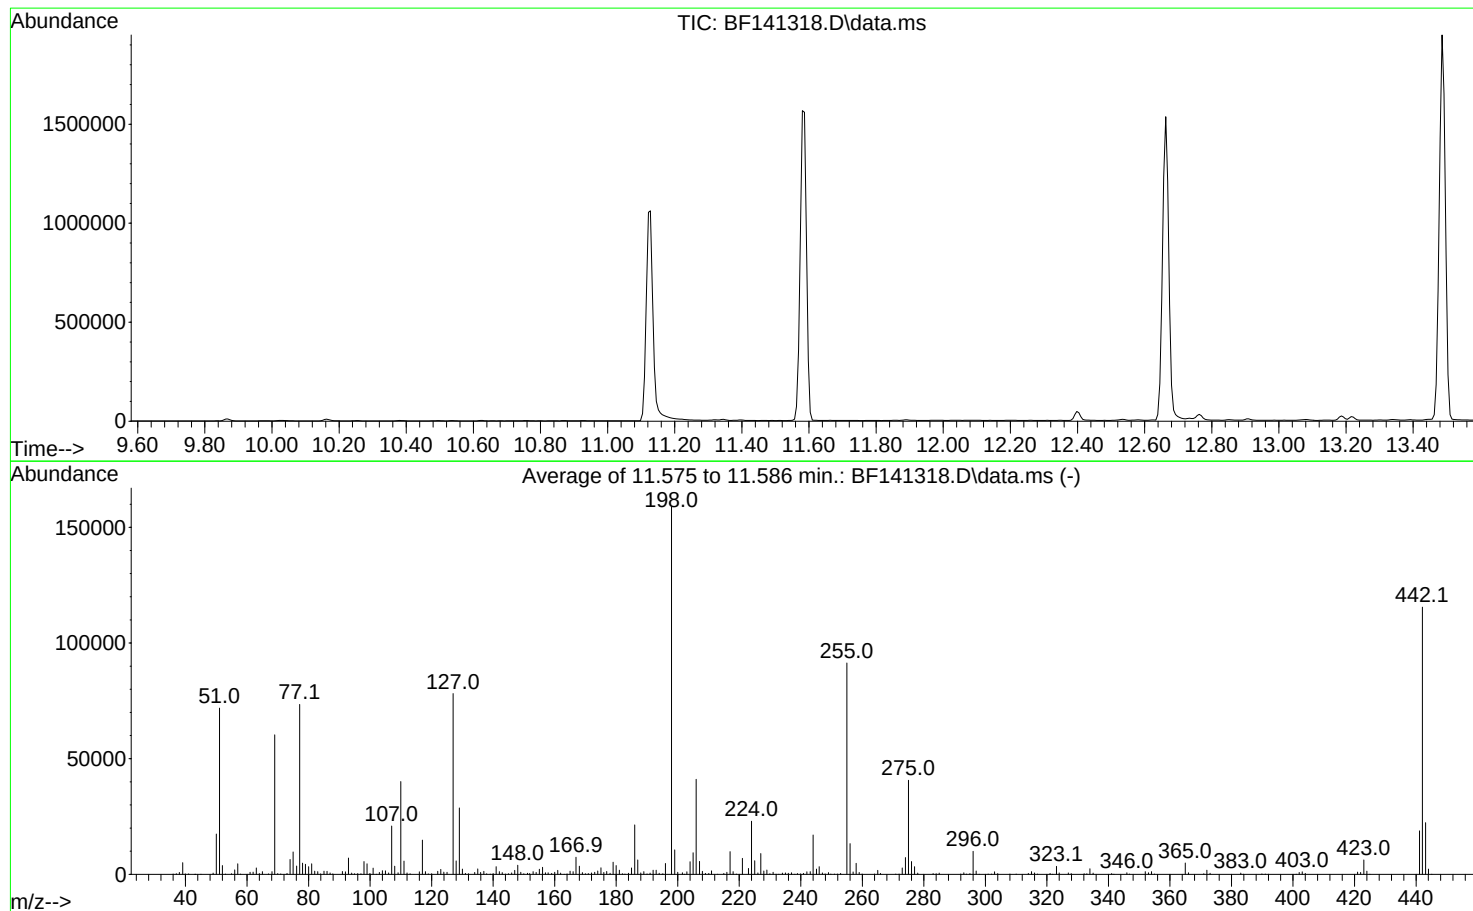

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	71840	PASS
68	69	0.00	2	1.9	1161	PASS
69	198	0.00	100	37.9	60326	PASS
70	69	0.00	2	0.6	349	PASS
127	198	10	80	49.2	78163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159005	PASS
199	198	5	9	6.7	10584	PASS
275	198	10	60	25.6	40664	PASS
365	198	1	100	3.1	4901	PASS
441	198	0.01	100	11.8	18814	PASS
442	442	50	100	100.0	115523	PASS
443	442	15	24	19.4	22359	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/31/2025	BNA_F	<u>BF141318.D</u>
Compound Name	Response	Retention Time
DDT	492165	13.486
DDD	11226	13.186
DDE	822	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12048	504213	2.39

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141318.D
Acq On : 31 Jan 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 10:52:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

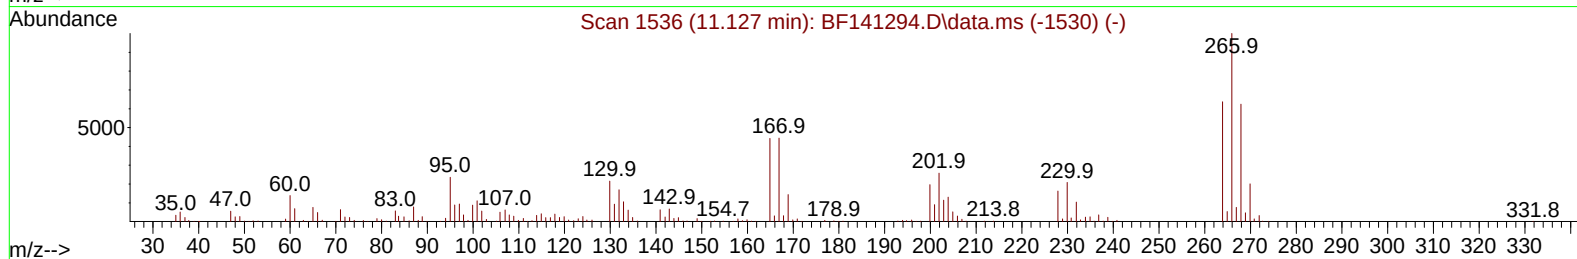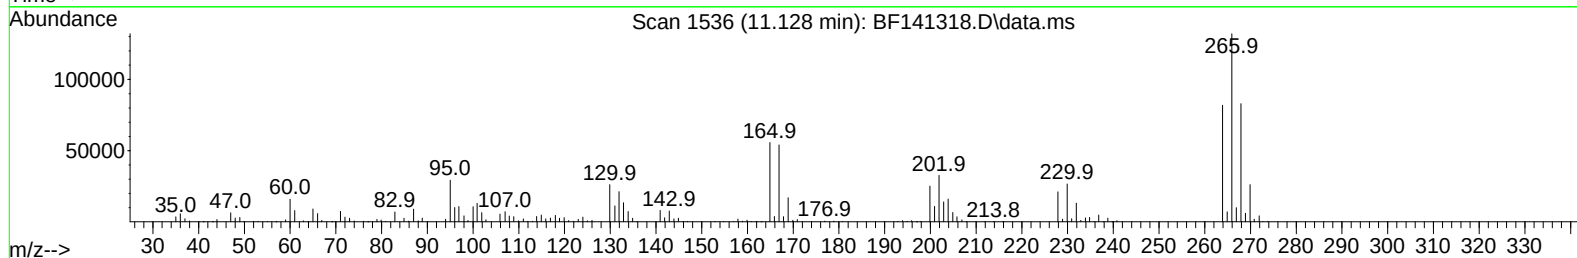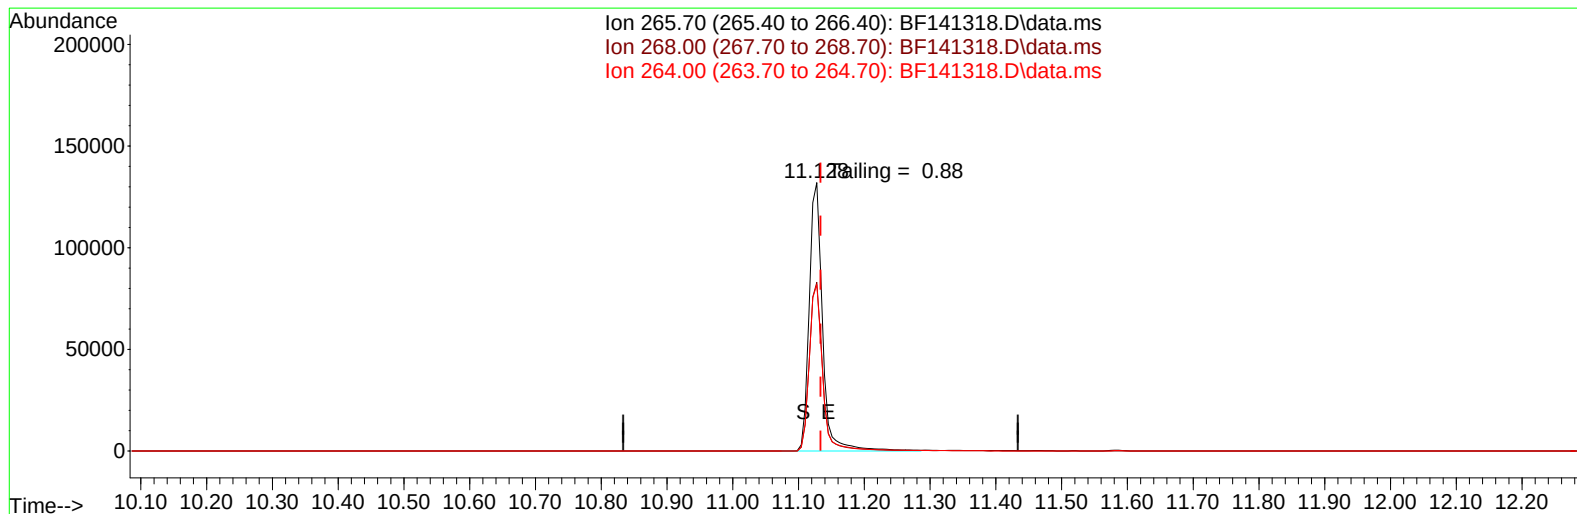

TIC: BF141318.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.006) 13648.97 ng

response 185655

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.83
264.00	63.70	62.03
0.00	0.00	0.00

