
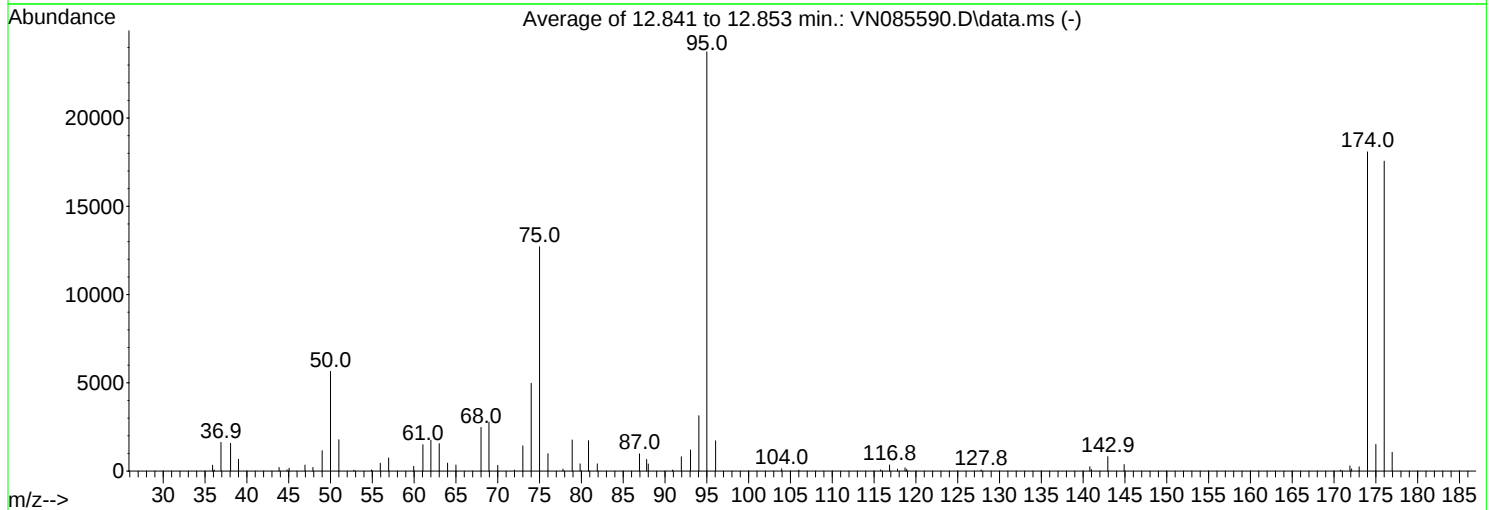


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013125\
Data File : VN085590.D
Acq On : 31 Jan 2025 09:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Title : SW846 8260
Last Update : Thu Jan 16 01:16:09 2025

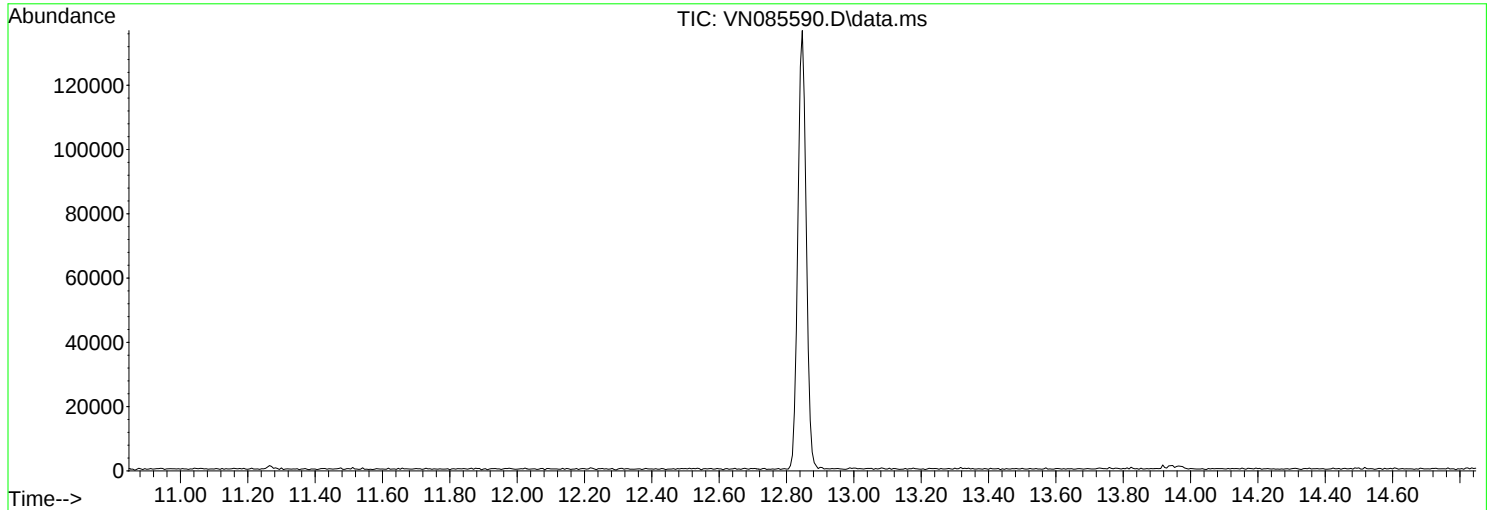

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	5647	PASS
75	95	30	60	53.5	12707	PASS
95	95	100	100	100.0	23757	PASS
96	95	5	9	7.2	1718	PASS
173	174	0.00	2	1.4	245	PASS
174	95	50	100	76.1	18083	PASS
175	174	5	9	8.3	1508	PASS
176	174	95	101	97.1	17560	PASS
177	176	5	9	6.0	1060	PASS