

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013025\
 Data File : P0109280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 13:06
 Operator : YP/AJ
 Sample : Q1215-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JPP-29.1-012825

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/31/2025
 Supervised By :Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 14:30:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 22 03:46:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	130.4E6	92572592	17.251m	17.270m
2) SA Decachlor...	8.755	8.707	94913407	45892733	13.700	13.346m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO013025\
Data File : PO109280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 13:06
Operator : YP/AJ
Sample : Q1215-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JPP-29.1-012825


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 14:30:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 22 03:46:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

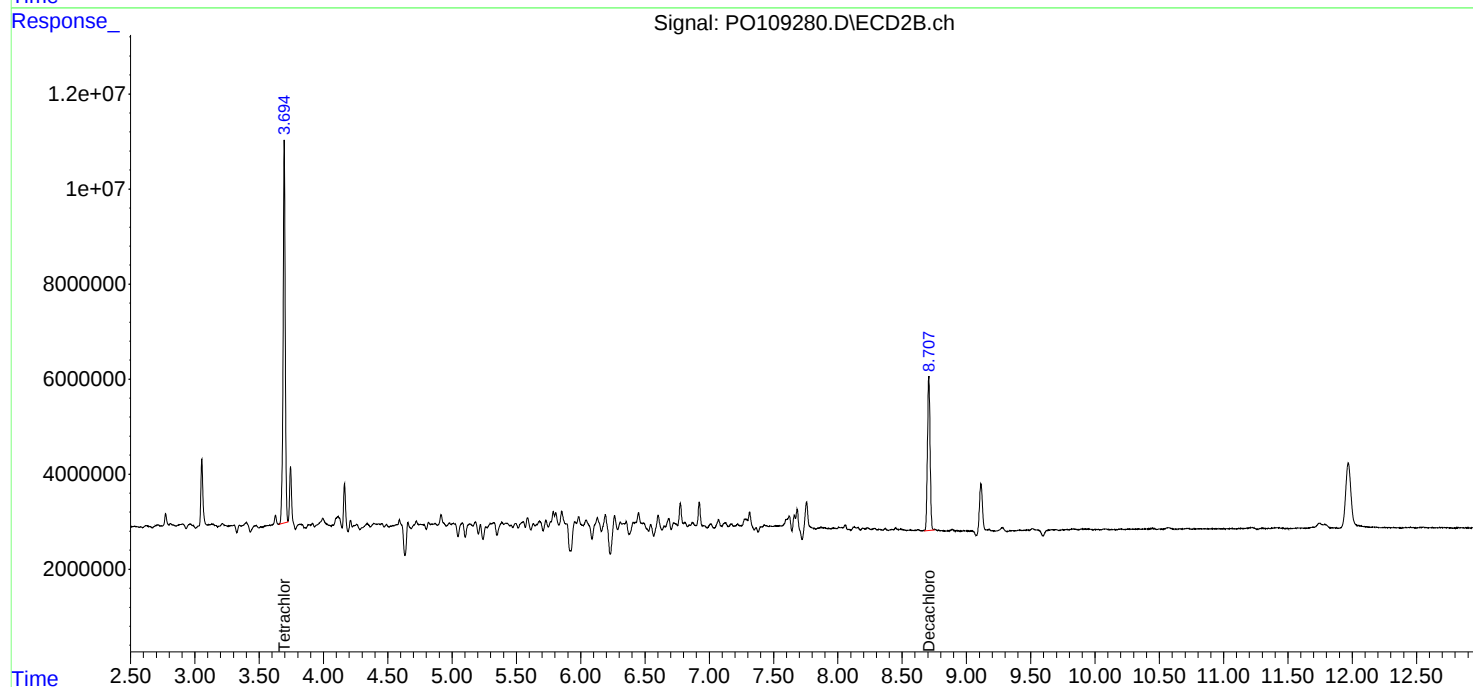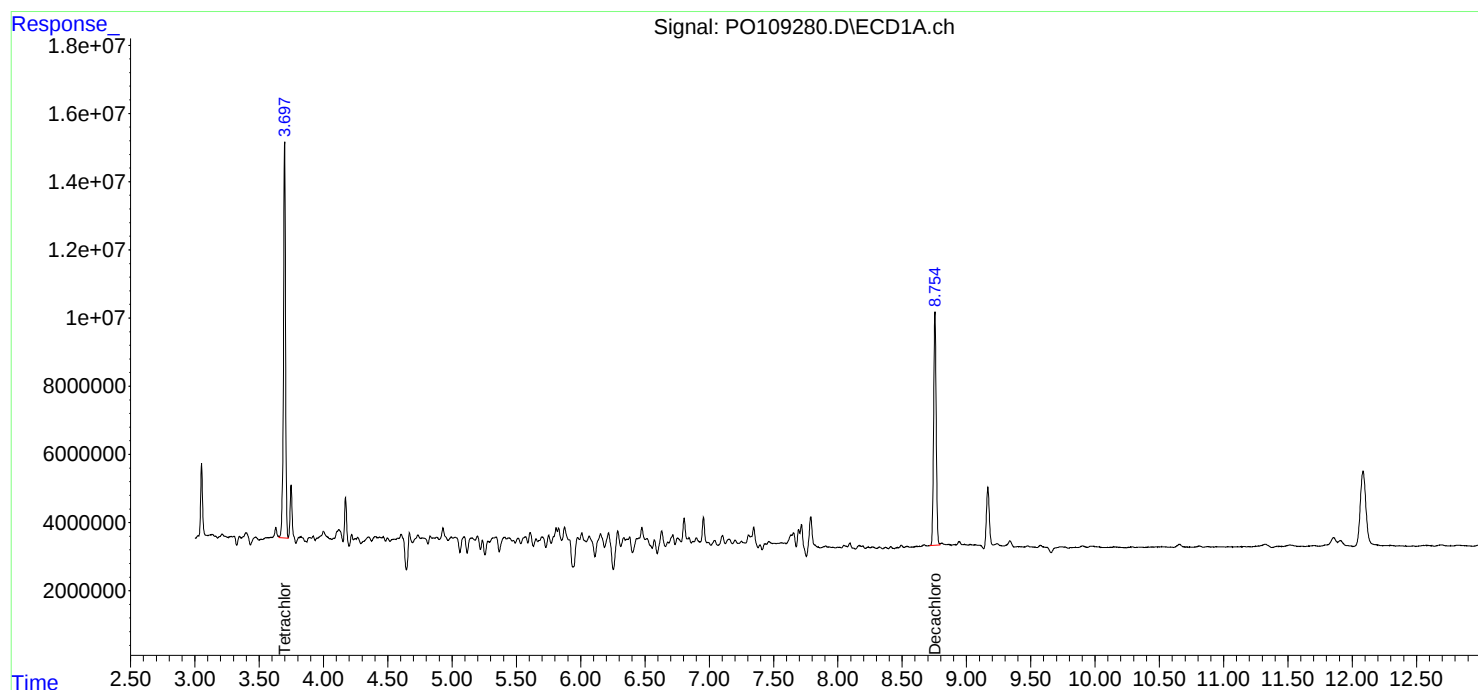

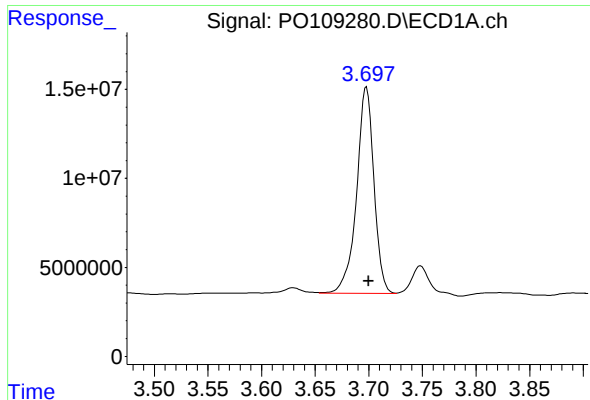


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: -0.003 min
Response: 130359314
Conc: 17.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
JPP-29.1-012825


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

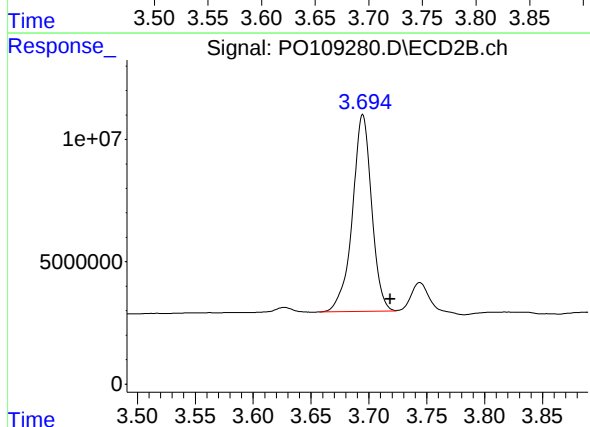


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: -0.024 min
Response: 92572592
Conc: 17.27 ng/ml m

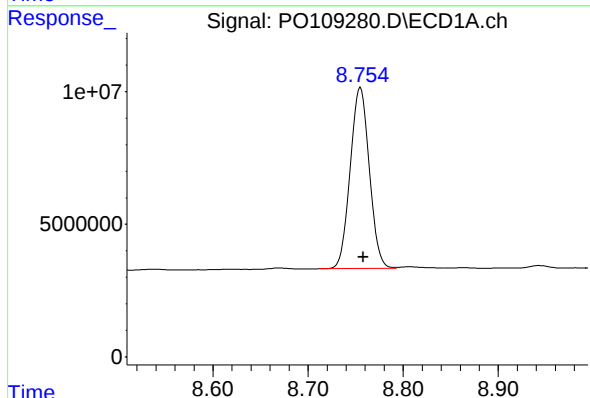

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.003 min
Response: 94913407
Conc: 13.70 ng/ml

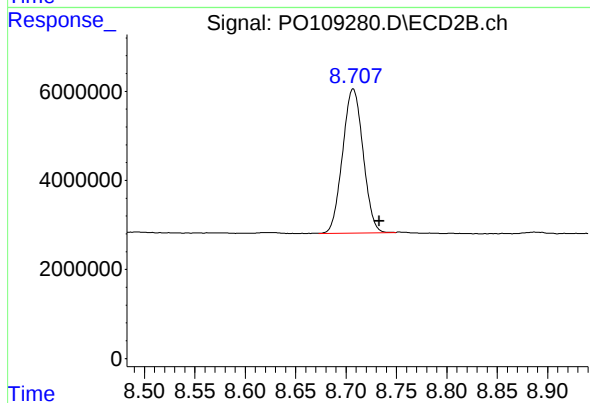

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: -0.026 min
Response: 45892733
Conc: 13.35 ng/ml m