
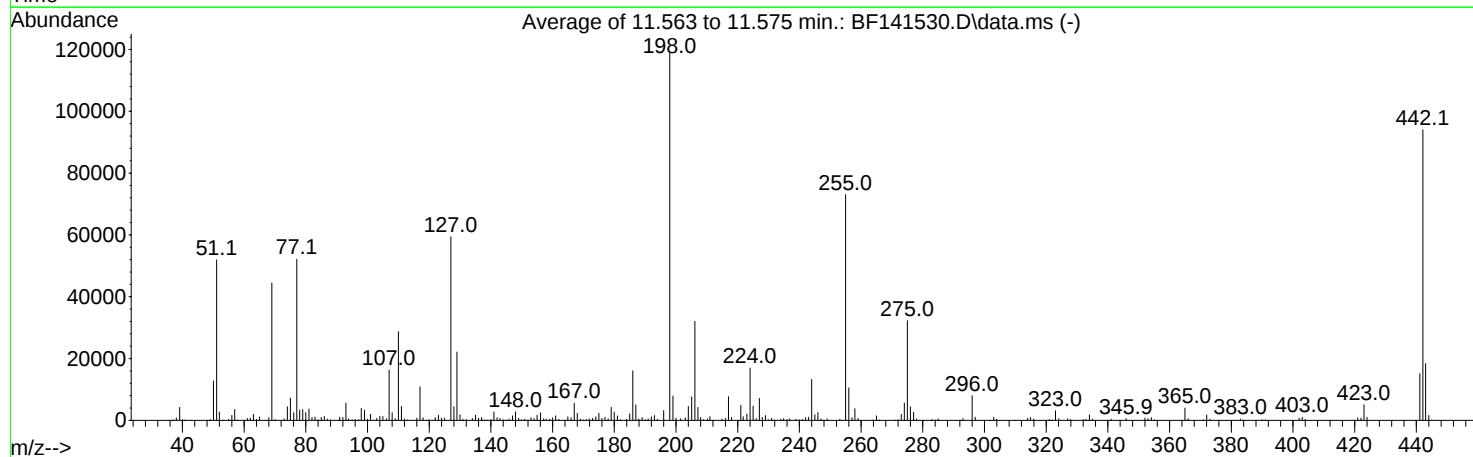


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141530.D
Acq On : 10 Feb 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

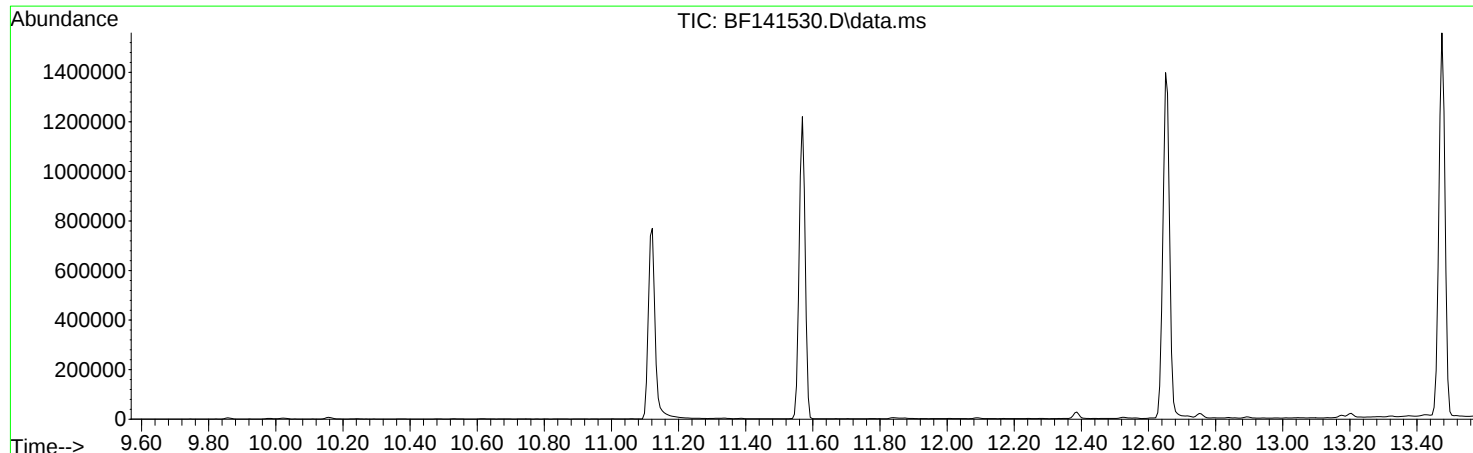

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	51904	PASS
68	69	0.00	2	1.9	860	PASS
69	198	0.00	100	37.3	44448	PASS
70	69	0.00	2	0.5	238	PASS
127	198	10	80	49.9	59352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119008	PASS
199	198	5	9	6.6	7849	PASS
275	198	10	60	27.1	32248	PASS
365	198	1	100	3.4	3990	PASS
441	198	0.01	100	12.7	15136	PASS
442	442	50	100	100.0	94021	PASS
443	442	15	24	19.5	18358	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/10/2025	BNA_F	<u>BF141530.D</u>
Compound Name	Response	Retention Time
DDT	386356	13.474
DDD	7404	13.204
DDE	837	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8241	394597	2.09

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141530.D
Acq On : 10 Feb 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 12:29:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

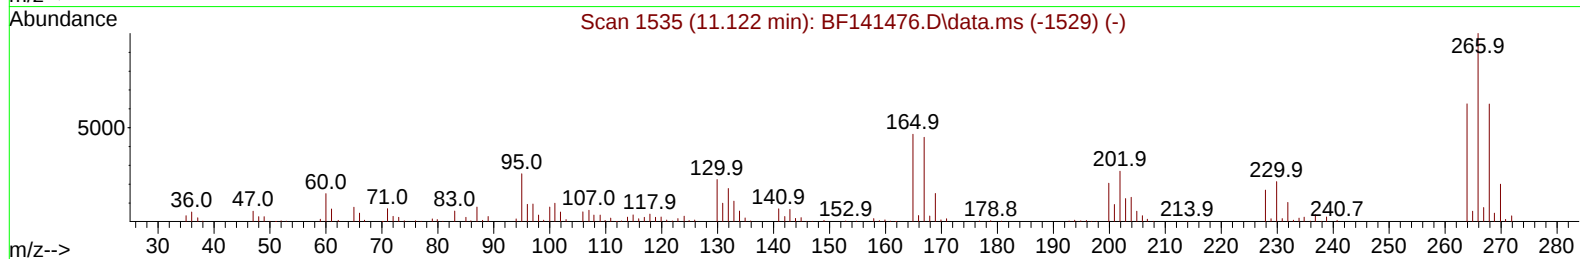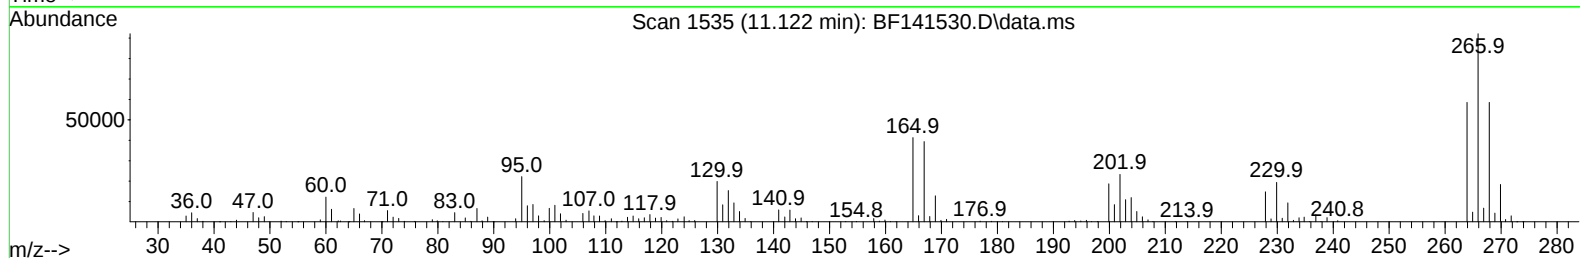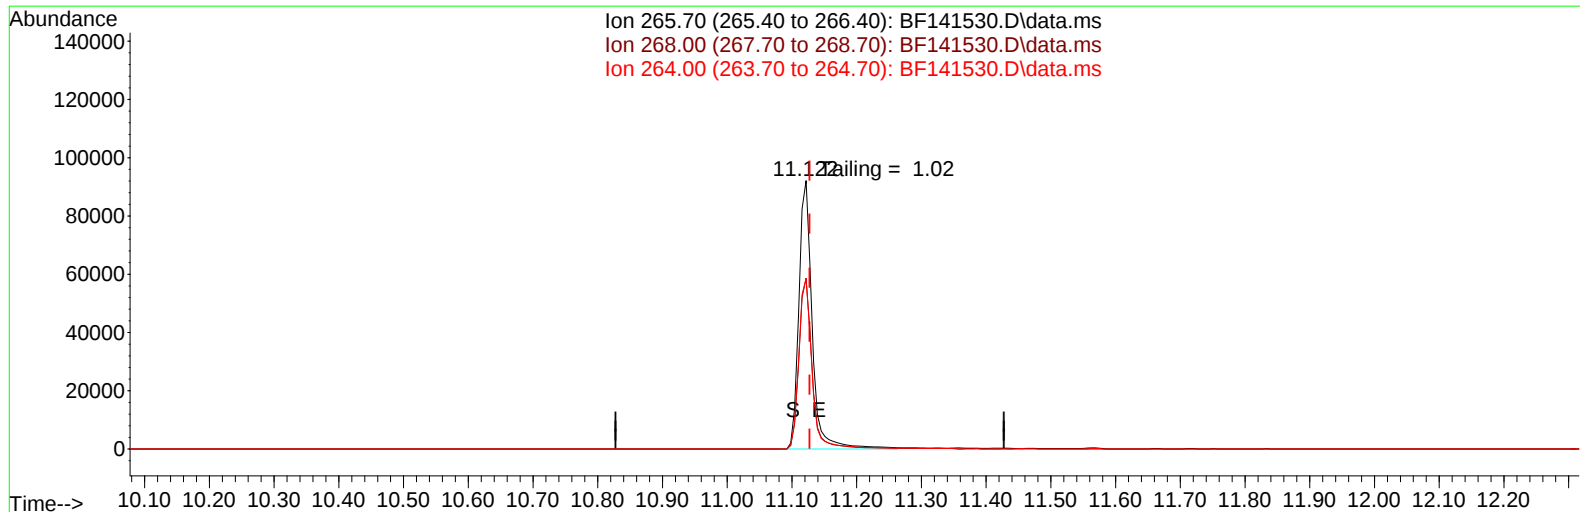

TIC: BF141530.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 15920.77 ng




response 133560

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.58
264.00	62.60	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141530.D
Acq On : 10 Feb 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 12:29:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

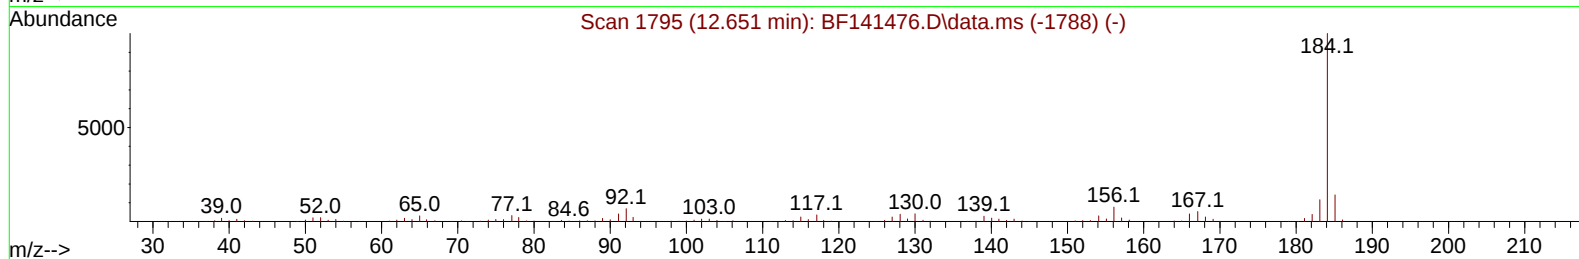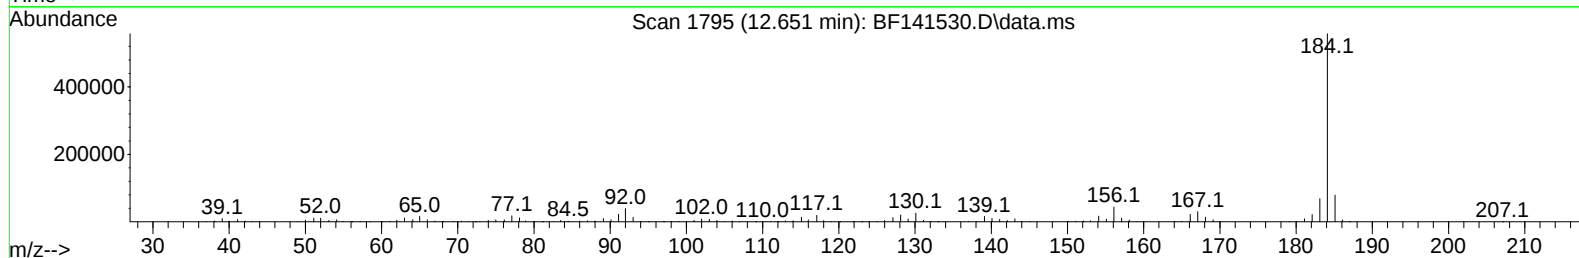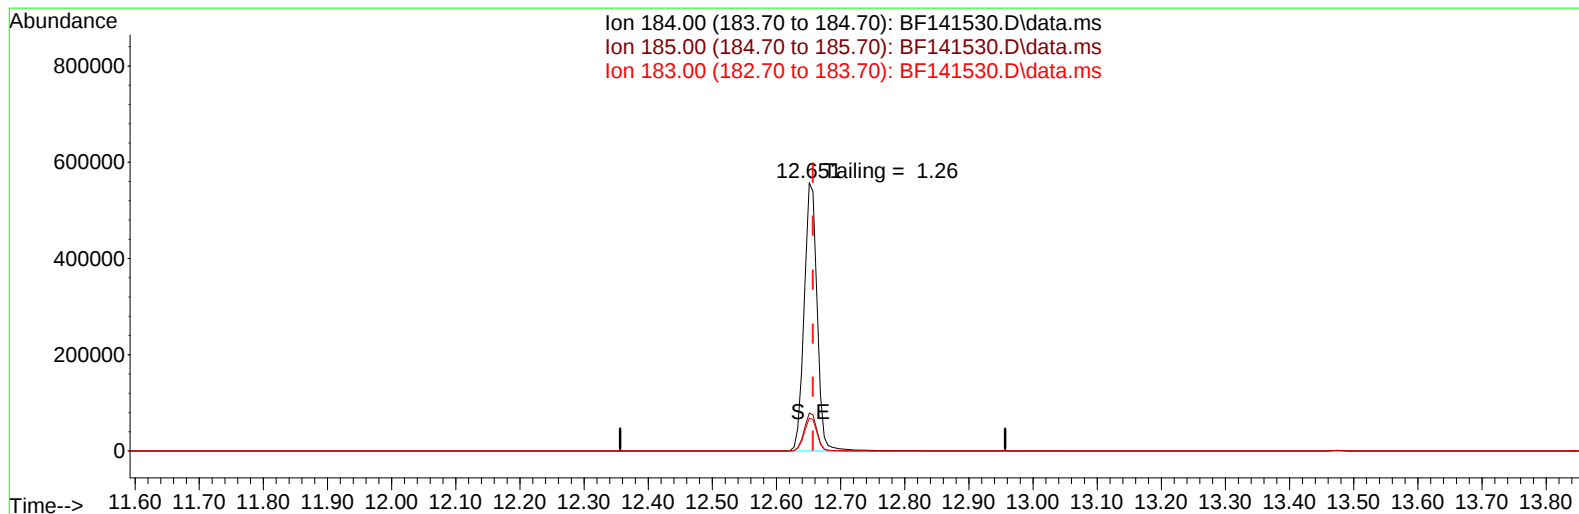

TIC: BF141530.D\data.ms

(77) Benzidine

12.651min (-0.006) 32112.35 ng

response 784704

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.14
183.00	11.60	12.25
0.00	0.00	0.00