


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021125\  
Data File : BF141550.D  
Acq On : 11 Feb 2025 10:02  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Feb 06 16:58:59 2025

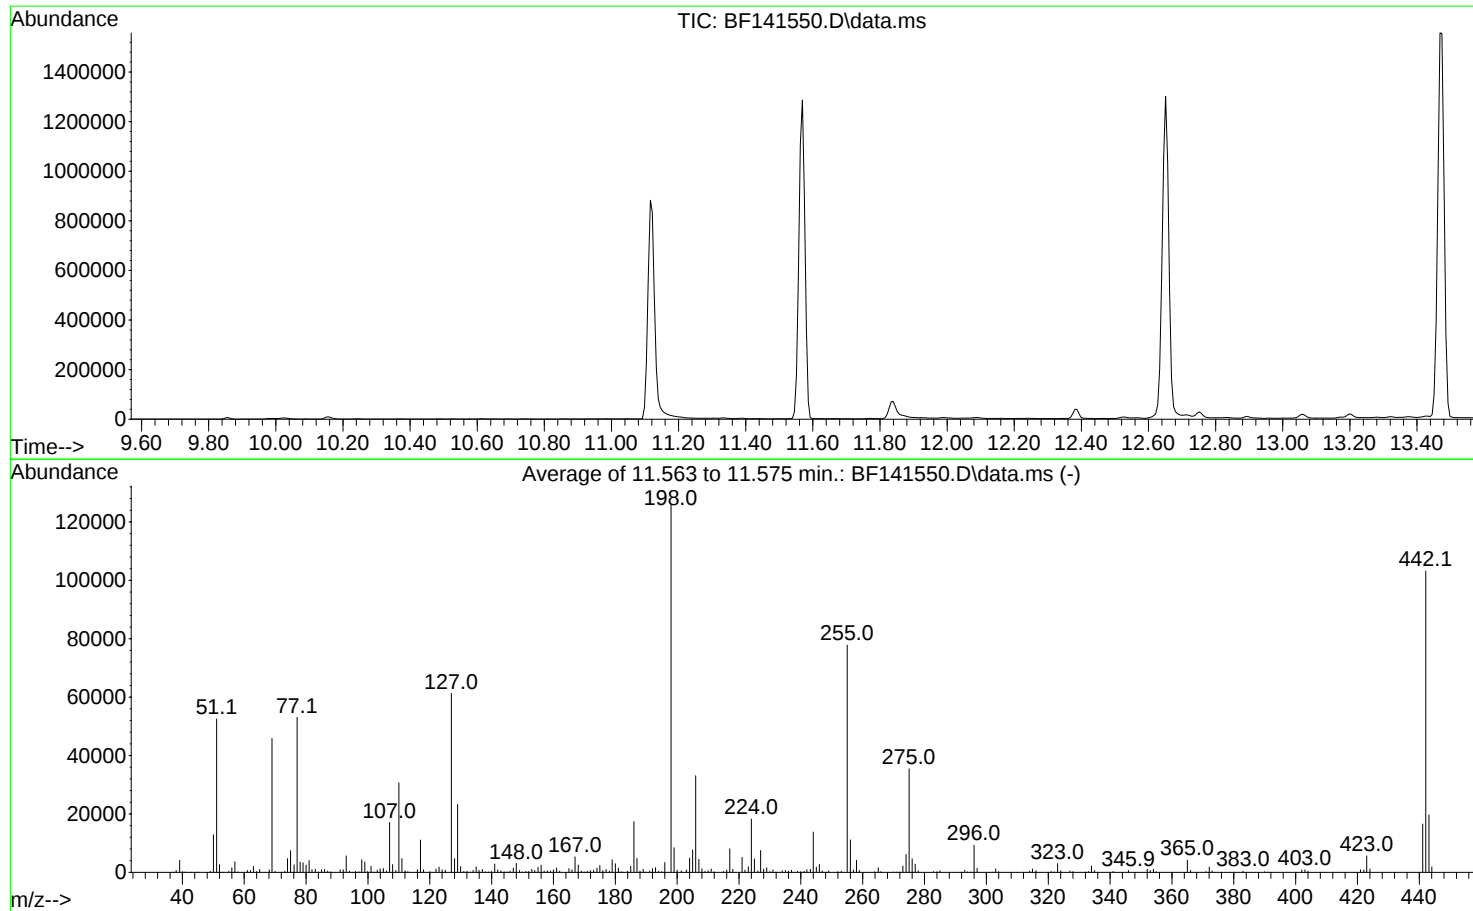

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.7         | 52576      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 880        | PASS                |
| 69             | 198             | 0.00            | 100             | 36.4         | 45864      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 312        | PASS                |
| 127            | 198             | 10              | 80              | 48.6         | 61283      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 125976     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 8465       | PASS                |
| 275            | 198             | 10              | 60              | 28.2         | 35464      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 4164       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 16543      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 103163     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 19671      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/11/2025     | BNA_F            | <u>BF141550.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 411059           | 13.474             |
| DDD           | 6230             | 13.204             |
| DDE           | 573              | 12.839             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 6803          | 417862           | 1.63               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021125\  
Data File : BF141550.D  
Acq On : 11 Feb 2025 10:02  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 11 10:57:59 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 06 16:58:59 2025  
Response via : Initial Calibration

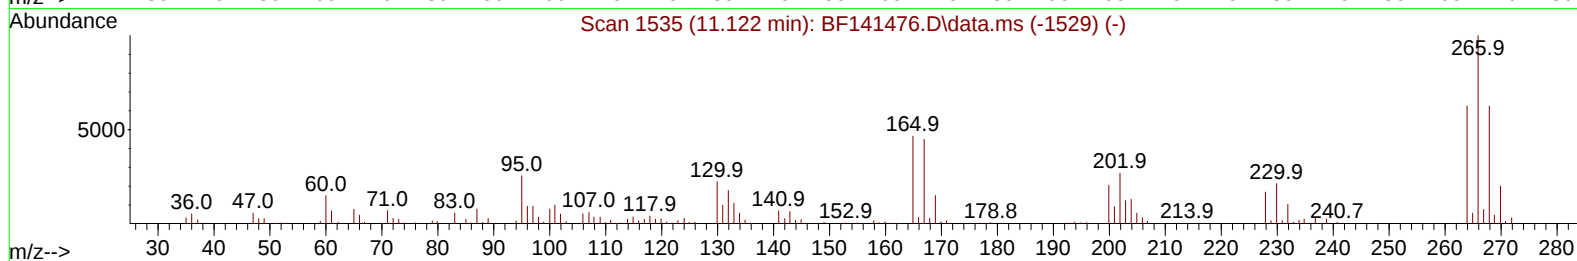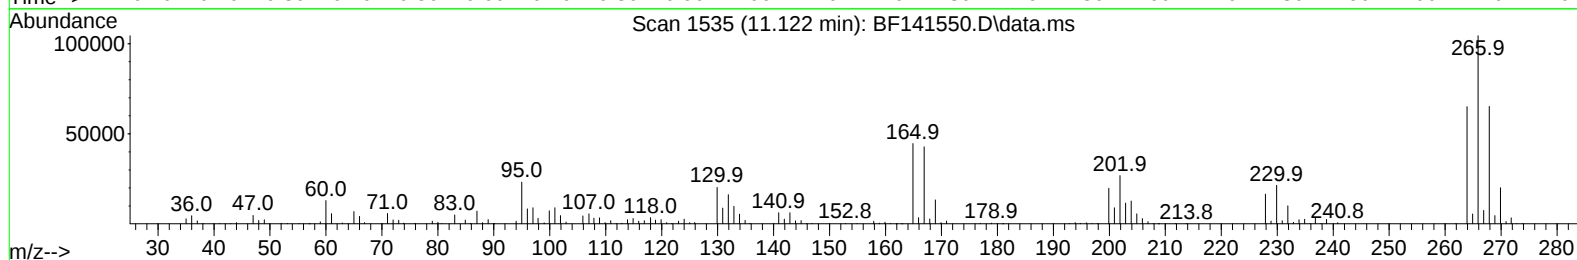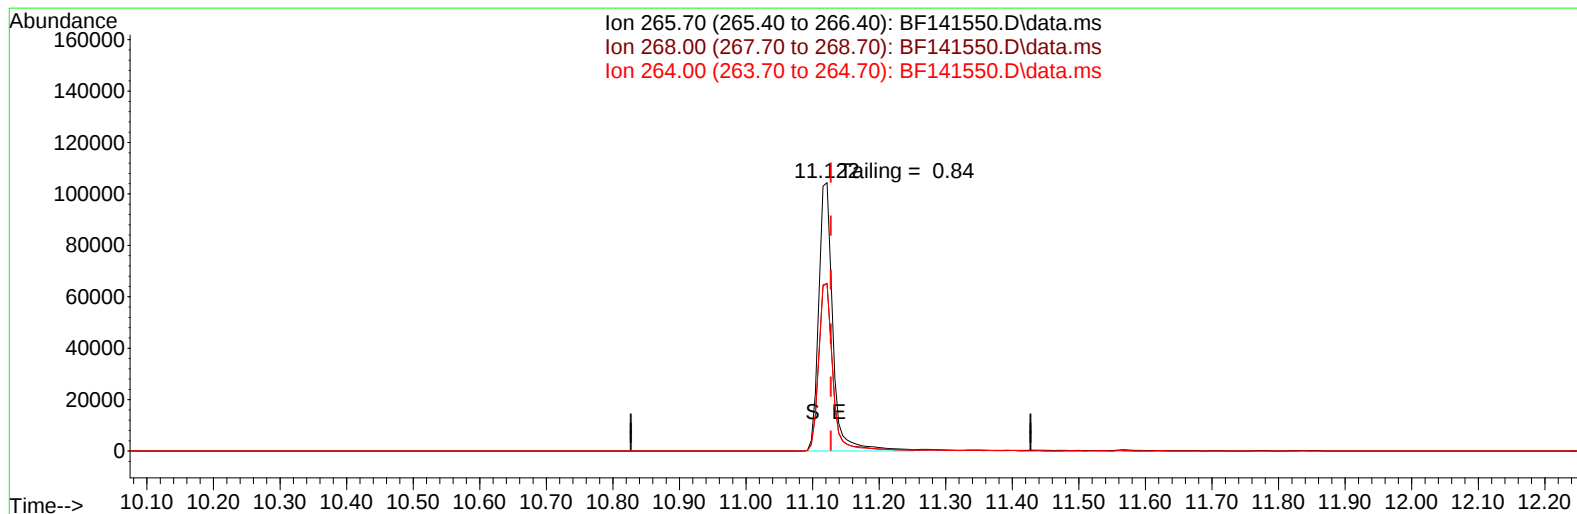

TIC: BF141550.D\data.ms

**(70) Pentachlorophenol (C)**

**11.122min (-0.006) 16244.81 ng**




**response 154688**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 62.47  |
| 264.00 | 62.60  | 62.37  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021125\  
Data File : BF141550.D  
Acq On : 11 Feb 2025 10:02  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 11 10:57:59 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 06 16:58:59 2025  
Response via : Initial Calibration

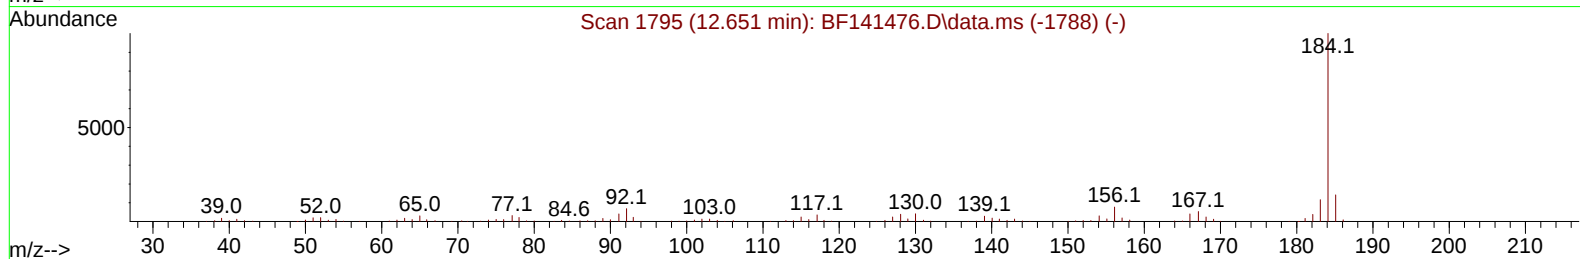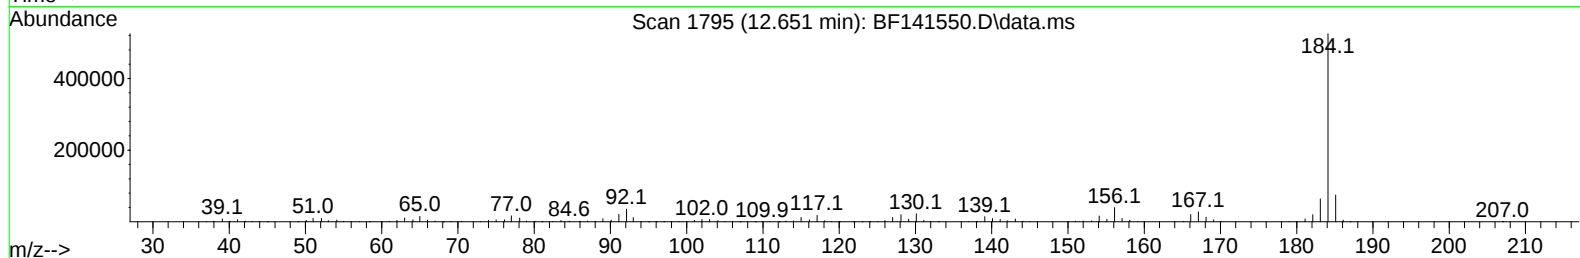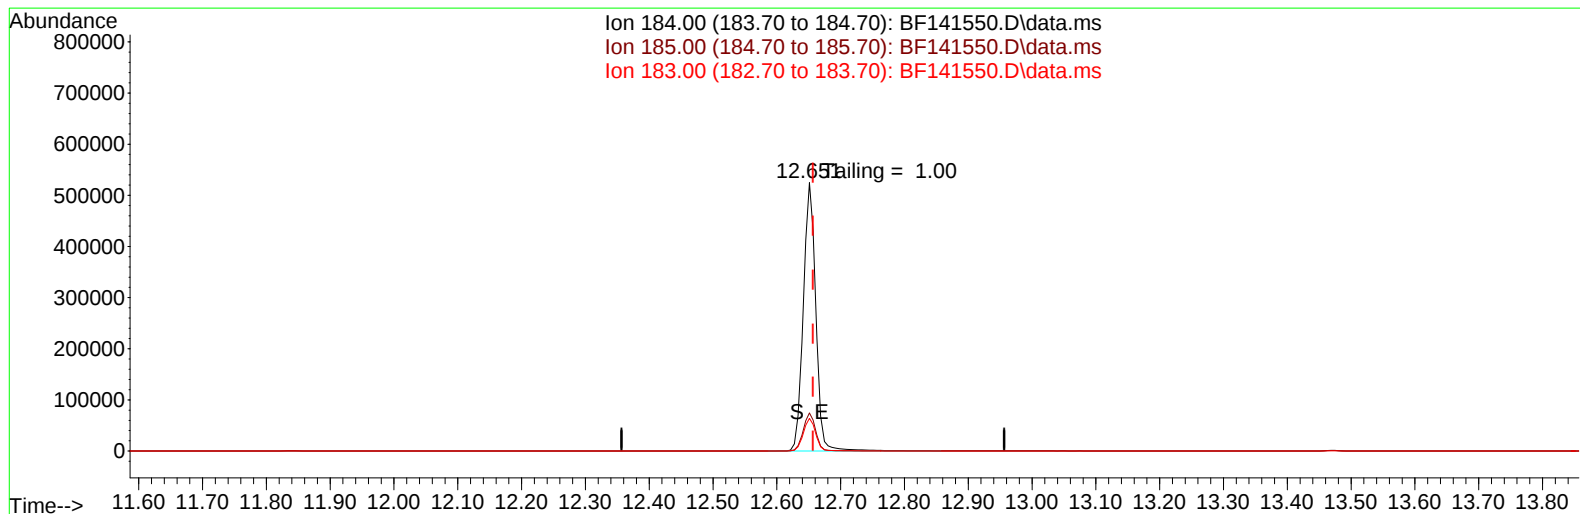

TIC: BF141550.D\data.ms

(77) Benzidine

12.651min (-0.006) 26925.30 ng

response 718522

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.23  |
| 183.00 | 11.60  | 12.19  |
| 0.00   | 0.00   | 0.00   |