


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012225\
Data File : BN036009.D
Acq On : 22 Jan 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 23 00:34:56 2025

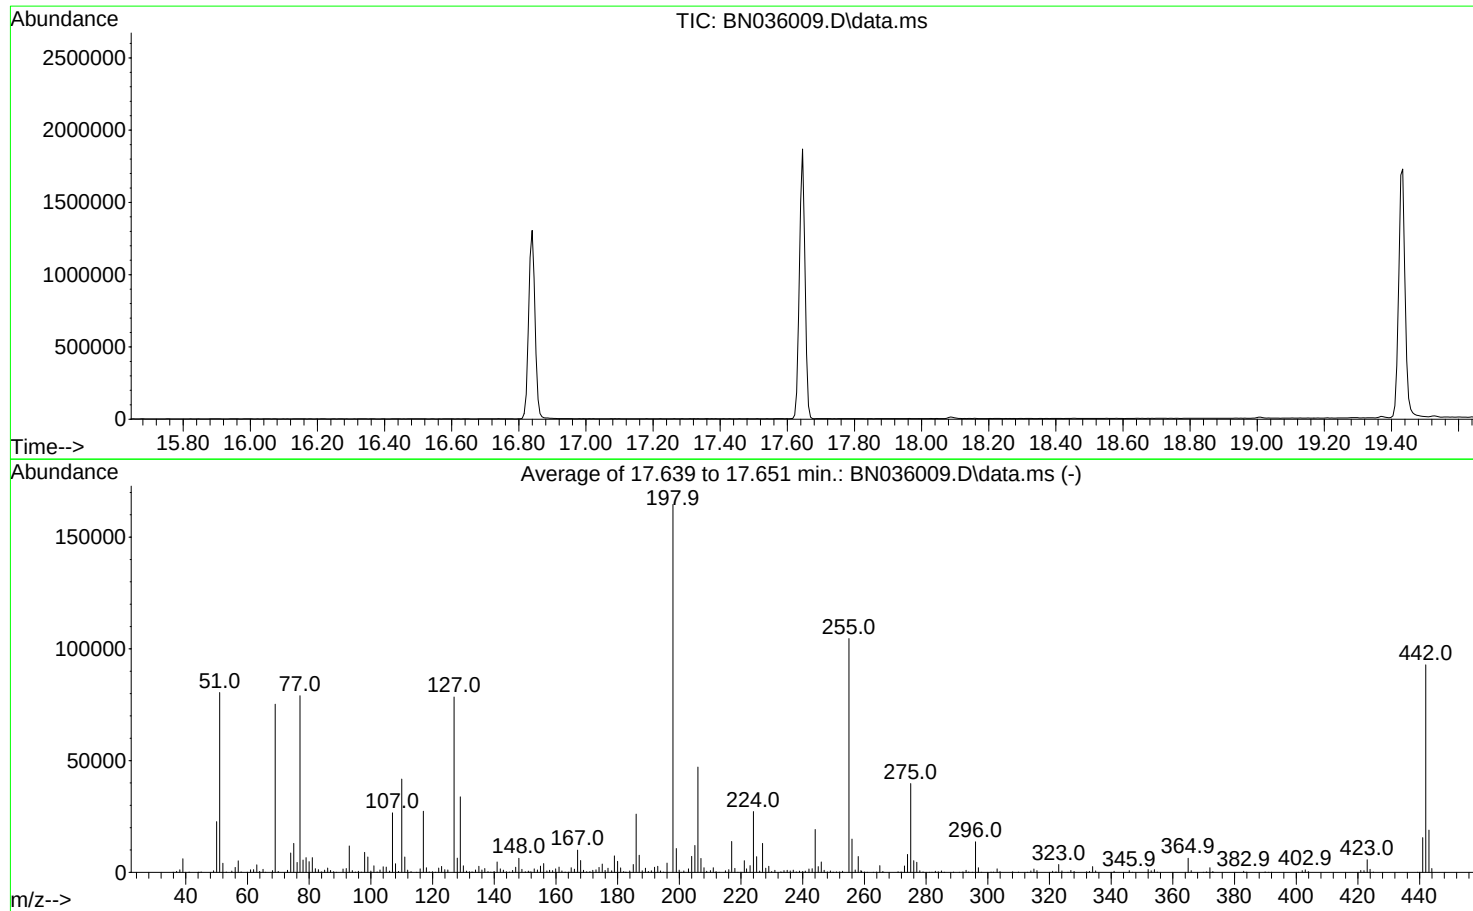




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	80440	PASS
68	69	0.00	2	1.1	792	PASS
69	198	0.00	100	45.7	75224	PASS
70	69	0.00	2	0.6	433	PASS
127	198	10	80	47.7	78488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	164608	PASS
199	198	5	9	6.5	10652	PASS
275	198	10	60	24.1	39749	PASS
365	198	1	100	3.8	6294	PASS
441	198	0.01	100	9.4	15532	PASS
442	442	50	100	100.0	92893	PASS
443	442	15	24	20.4	18924	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012225\
Data File : BN036009.D
Acq On : 22 Jan 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 23 00:54:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

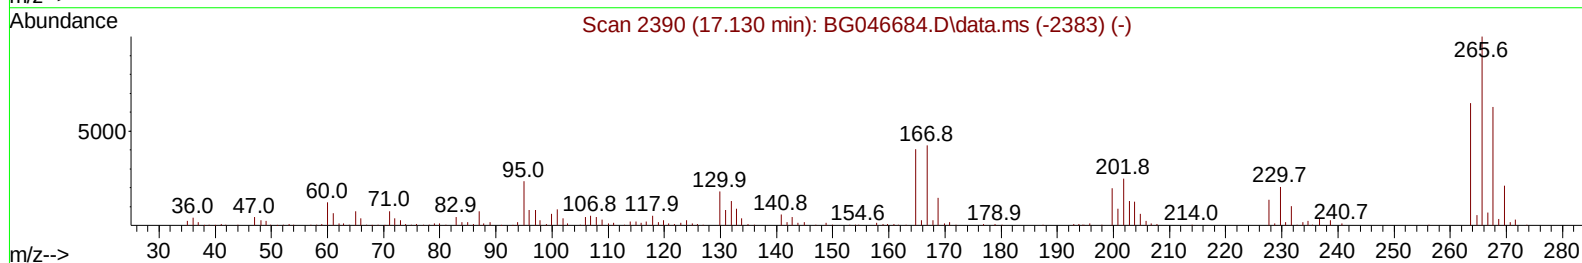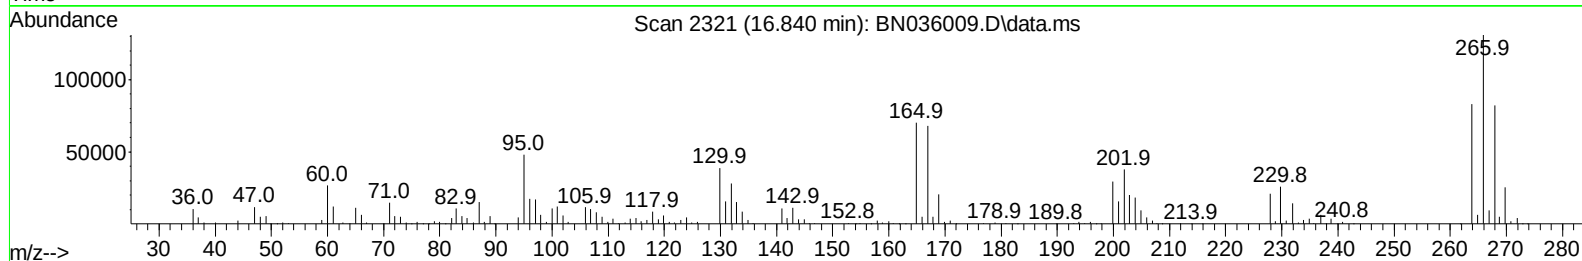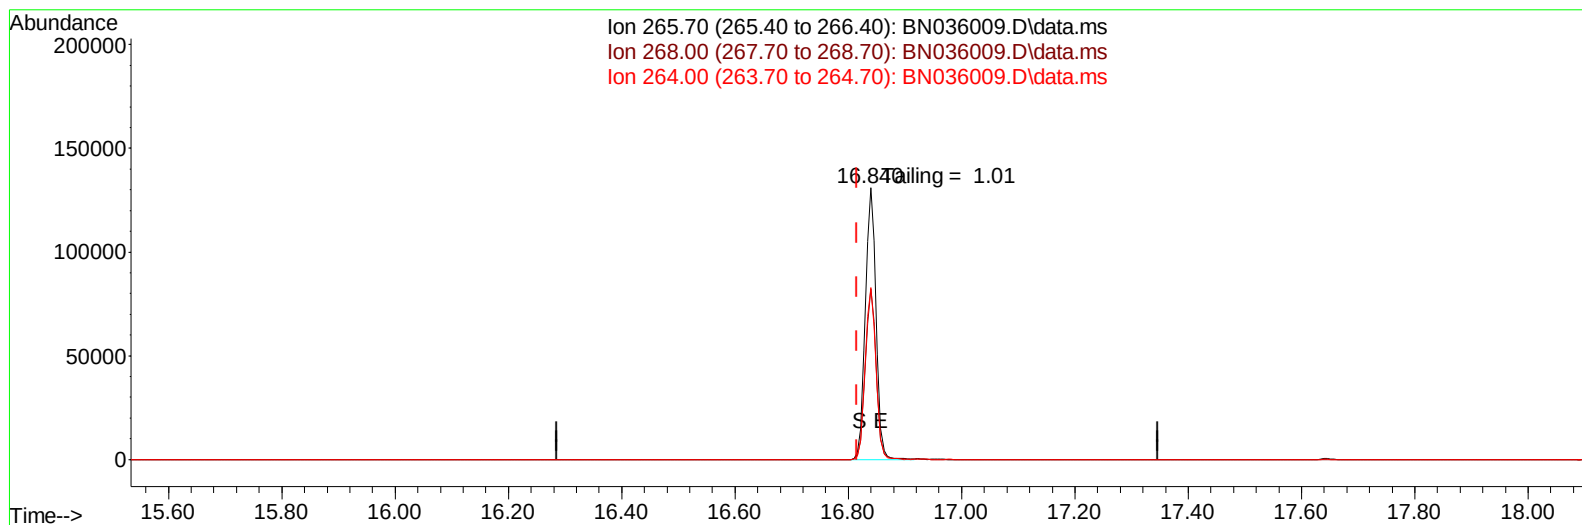

TIC: BN036009.D\data.ms

(70) Pentachlorophenol (C)

16.840min (+ 0.024) 21048.35 ng




response 172285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.84
264.00	61.60	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012225\
Data File : BN036009.D
Acq On : 22 Jan 2025 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 23 00:54:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

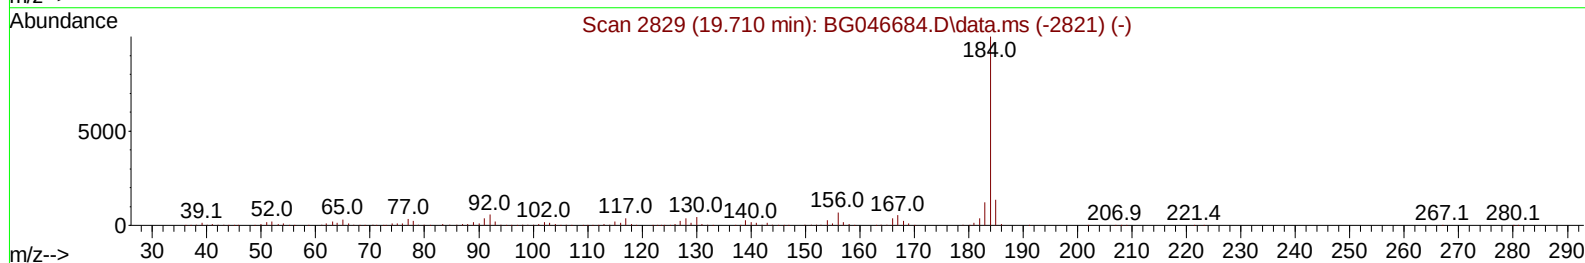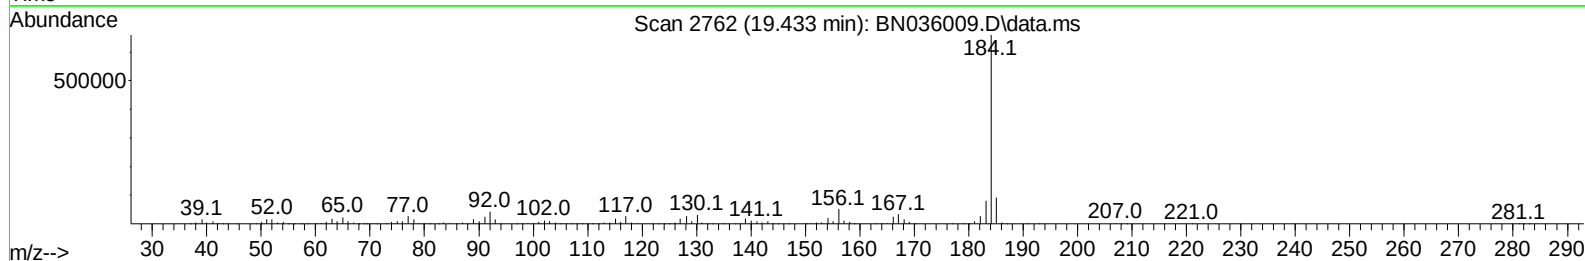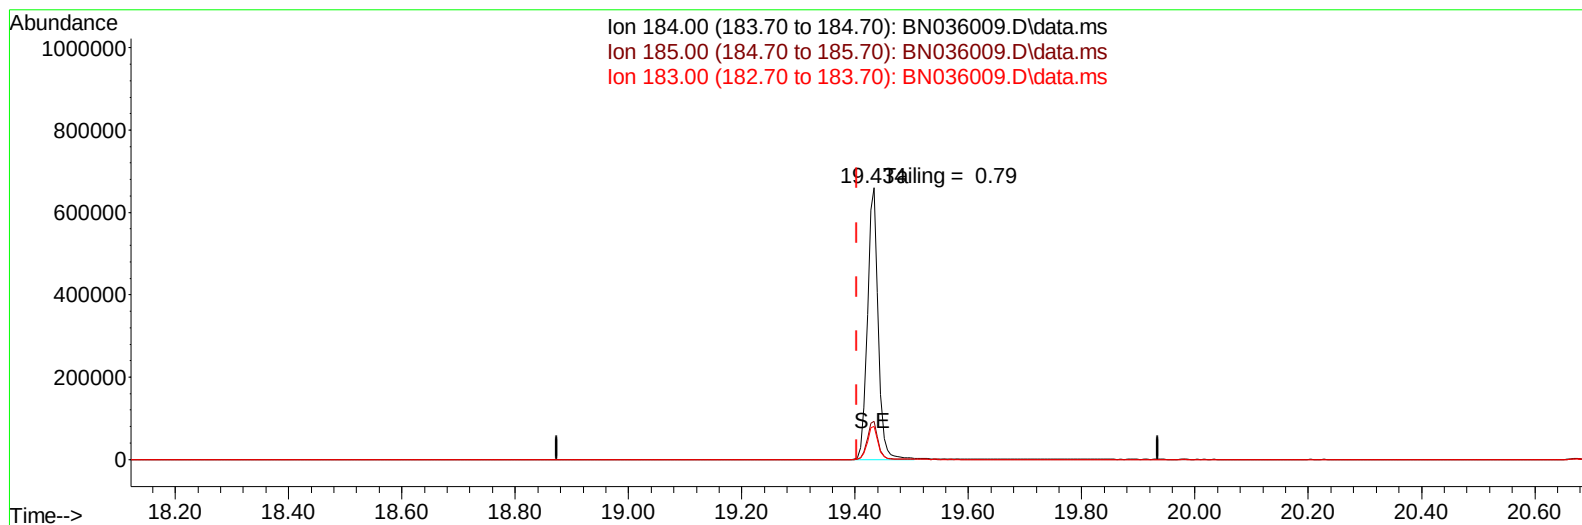

TIC: BN036009.D\data.ms

(77) Benzidine

19.433min (+ 0.029) 0.00 ng

response 875464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/22/2025	BNA_N	<u>BN036009.D</u>
Compound Name	Response	Retention Time
DDT	507361	20.675
DDD	11555	20.233
DDE	890	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12445	519806	2.39

Instrument :
BNA_N
ClientSampleId :
DFTPP