


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036319.D
Acq On : 06 Feb 2025 05:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 01:04:09 2025

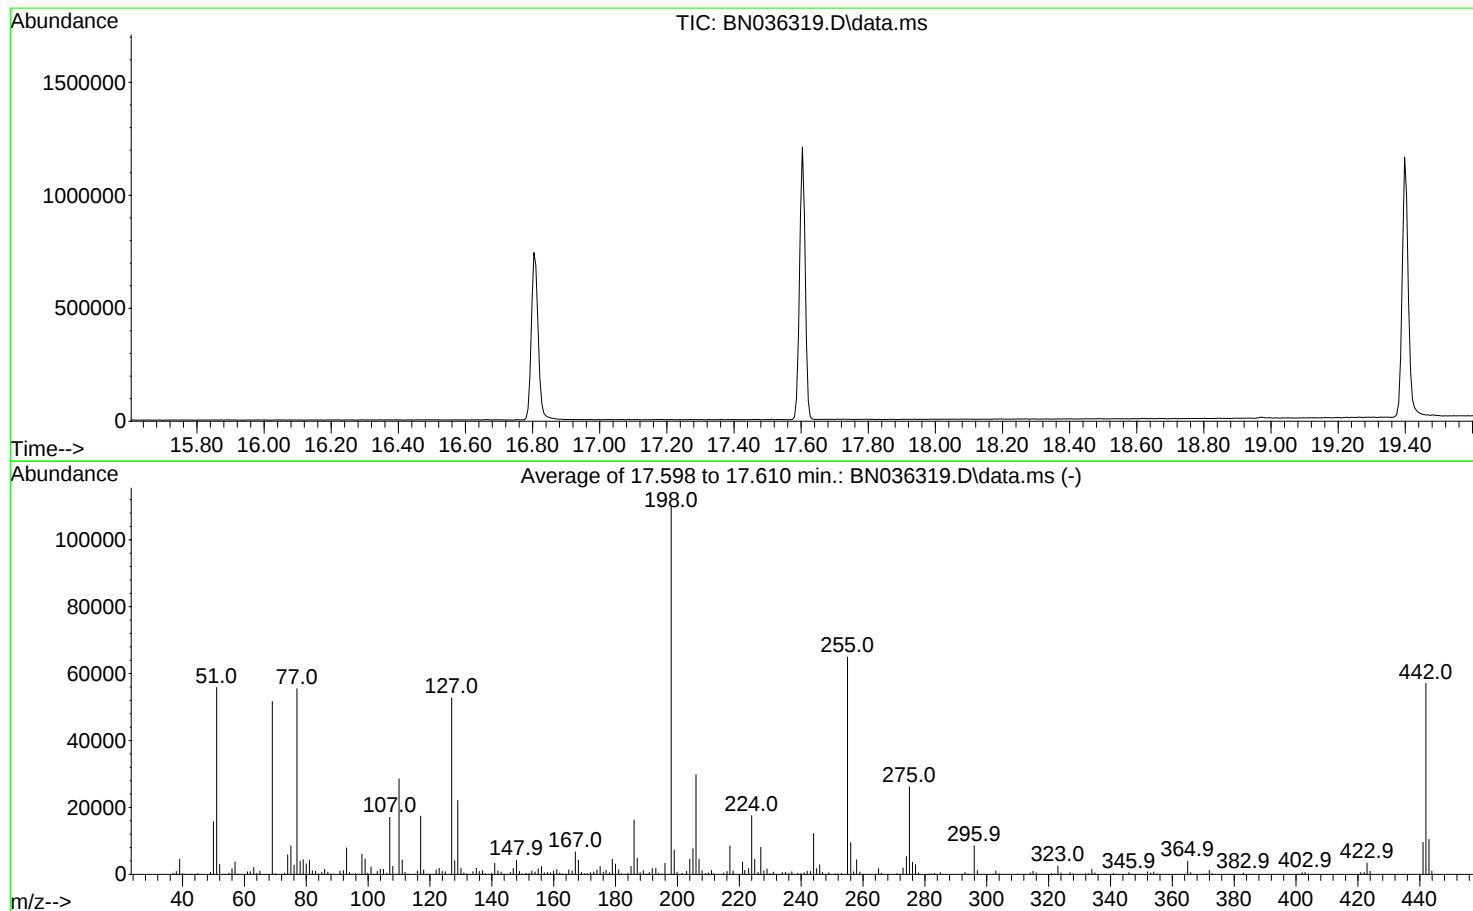

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	55883	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.0	51659	PASS
70	69	0.00	2	0.4	209	PASS
127	198	10	80	48.0	52773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109947	PASS
199	198	5	9	6.6	7267	PASS
275	198	10	60	23.8	26152	PASS
365	198	1	100	3.6	3930	PASS
441	198	0.01	100	8.7	9577	PASS
442	442	50	100	100.0	57093	PASS
443	442	15	24	18.3	10429	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/5/2025	BNA_N	<u>BN036319.D</u>
Compound Name	Response	Retention Time
DDT	307936	20.639
DDD	16912	20.198
DDE	720	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17632	325568	5.42

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036319.D
Acq On : 06 Feb 2025 05:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 07:50:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

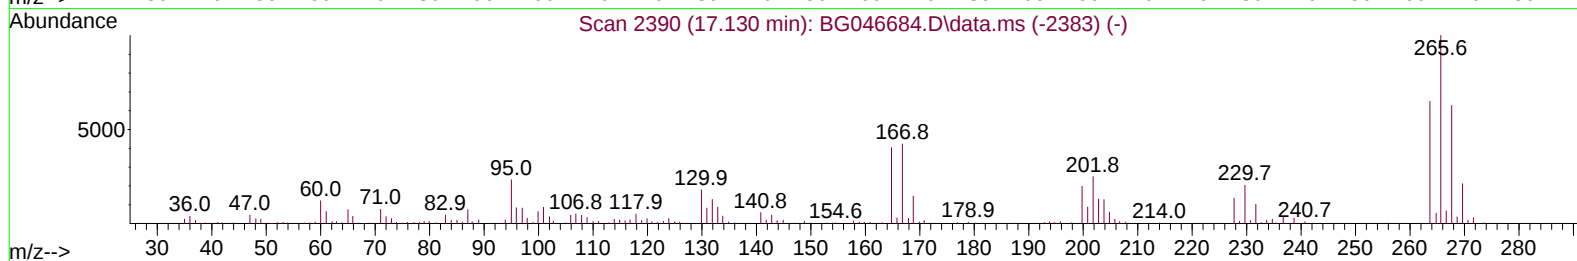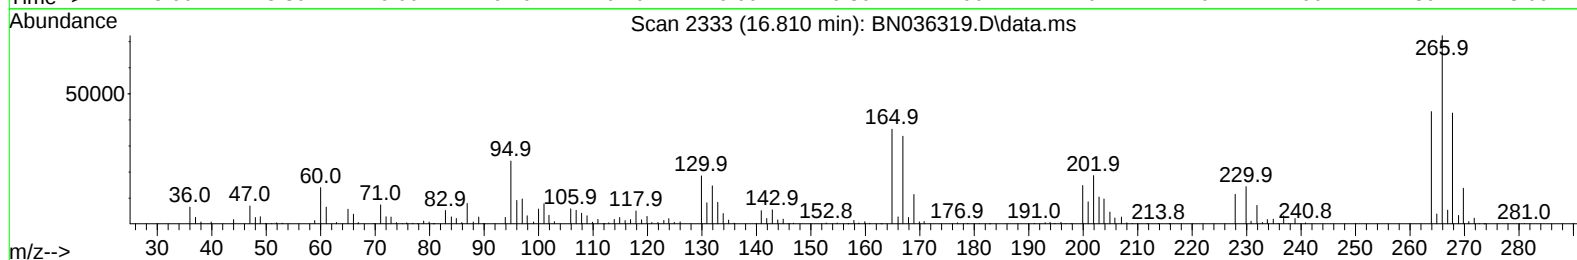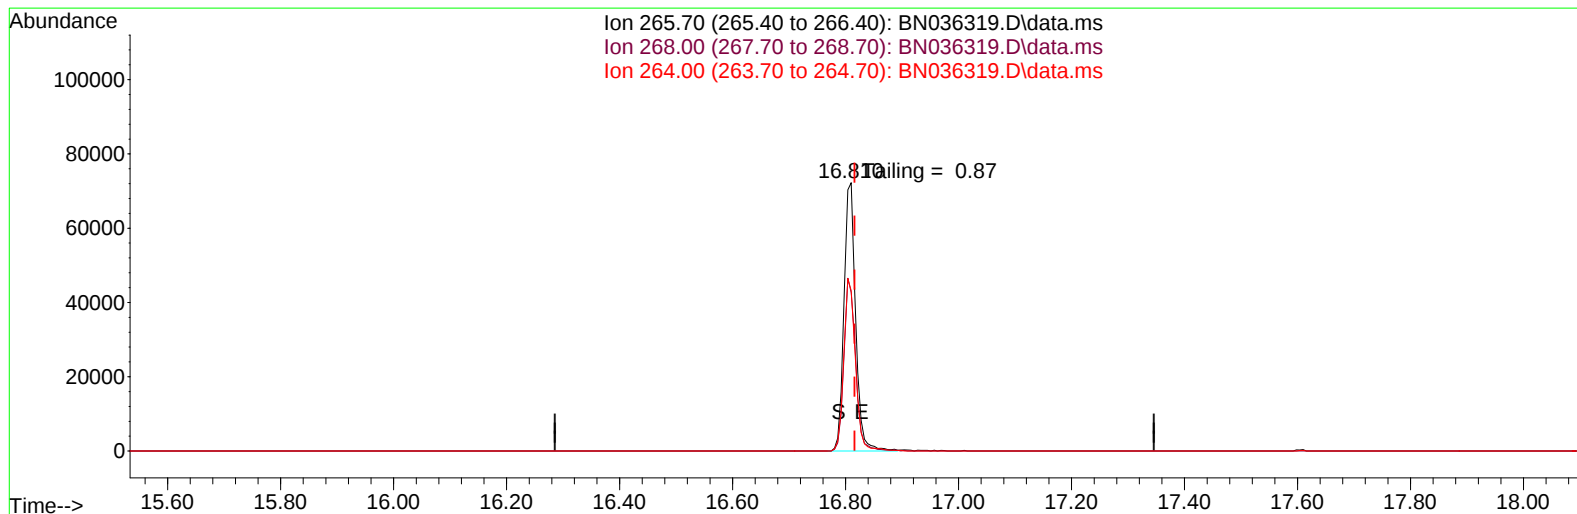

TIC: BN036319.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.006) 17584.32 ng




response 103084

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.02
264.00	61.60	59.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036319.D
Acq On : 06 Feb 2025 05:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 07:50:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

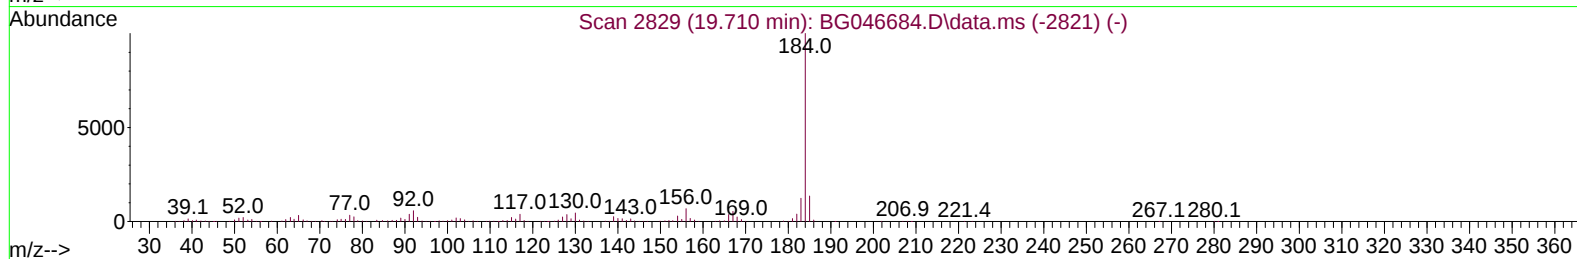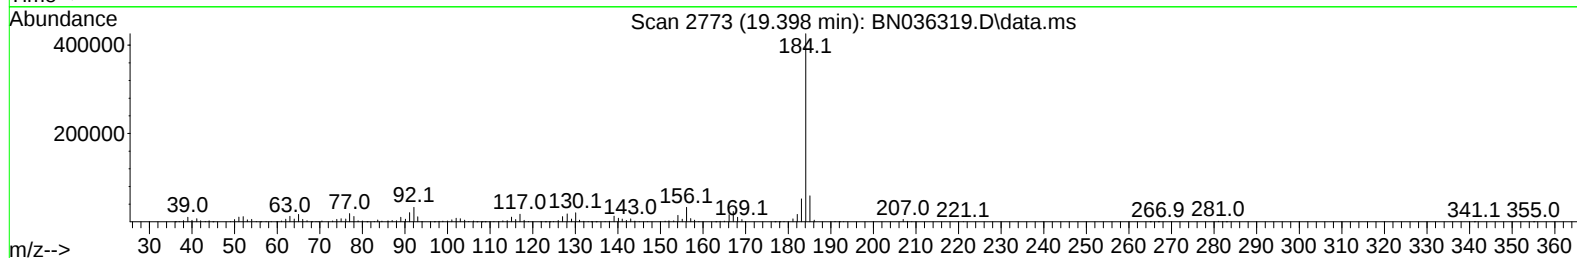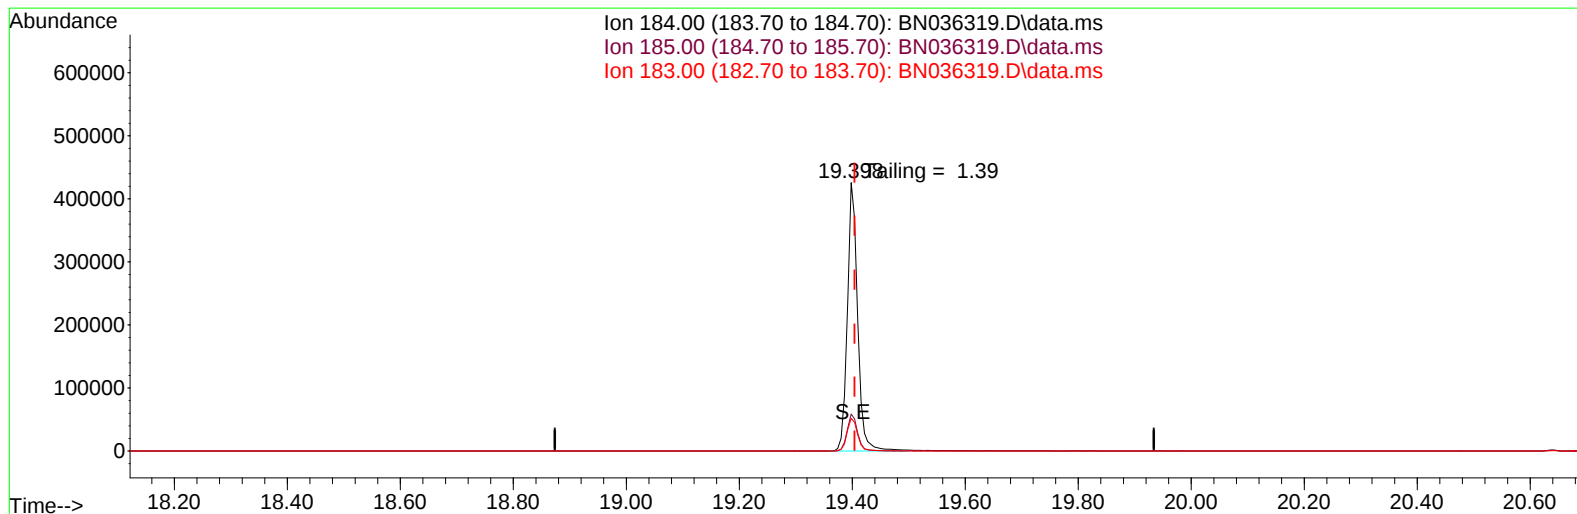

TIC: BN036319.D\data.ms

(77) Benzidine

19.398min (-0.006) 0.00 ng

response 542068

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	12.17
0.00	0.00	0.00