

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013125\
 Data File : P0109354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2025 01:46
 Operator : YP/AJ
 Sample : Q1232-15
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JPP-42.2-012925

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/10/2025
 Supervised By :Ankita Jodhani 02/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 05:22:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 22 03:46:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.699	3.696	171.4E6	126.4E6	22.677m	23.579m
2) SA Decachlor...	8.761	8.712	113.4E6	61750325	16.367	17.957

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO013125\
Data File : PO109354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2025 01:46
Operator : YP/AJ
Sample : Q1232-15
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JPP-42.2-012925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/10/2025
Supervised By :Ankita Jodhani 02/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 05:22:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 22 03:46:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

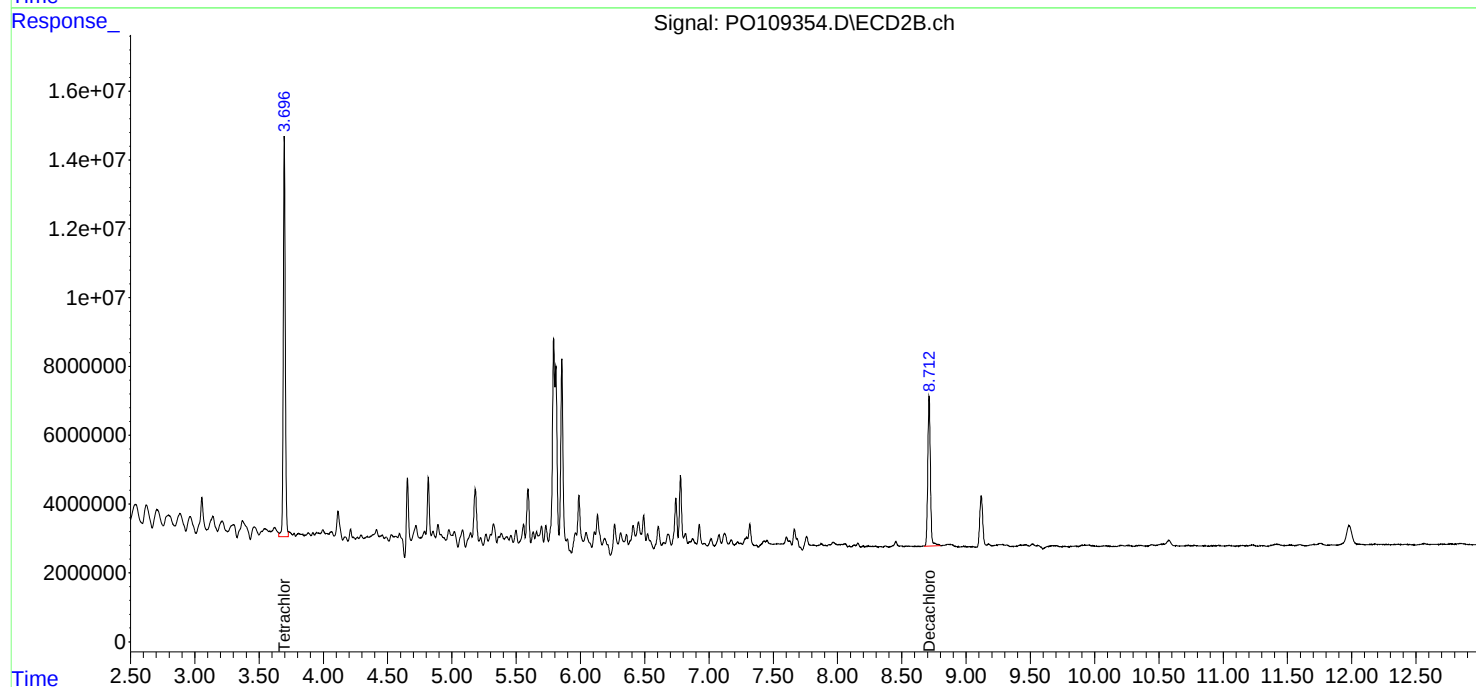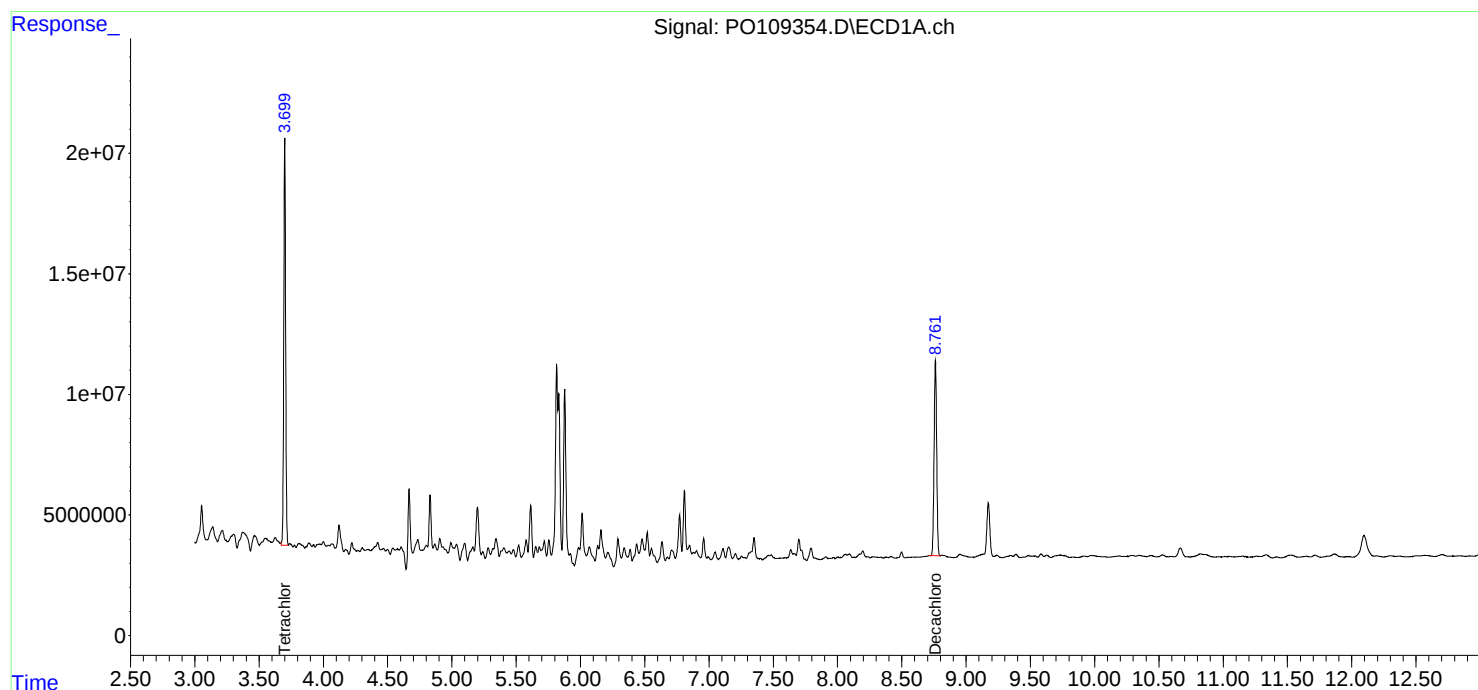

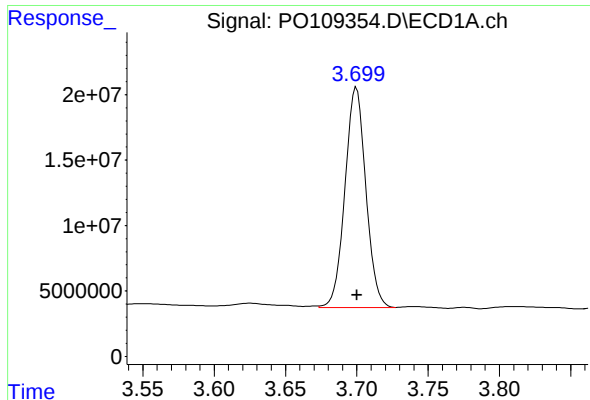


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 171356950
Conc: 22.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
JPP-42.2-012925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/10/2025
Supervised By :Ankita Jodhani 02/10/2025

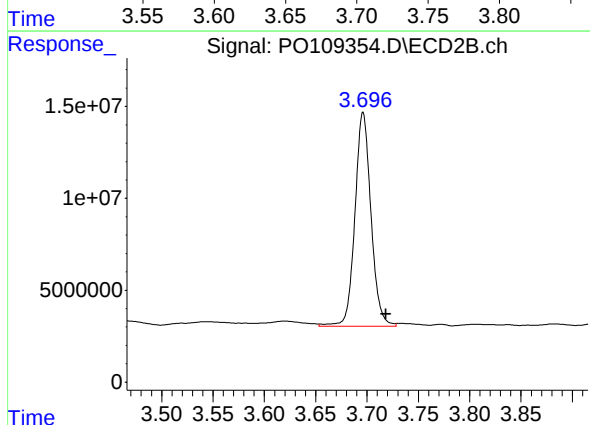


#1 Tetrachloro-m-xylene

R.T.: 3.696 min
Delta R.T.: -0.023 min
Response: 126392367
Conc: 23.58 ng/ml

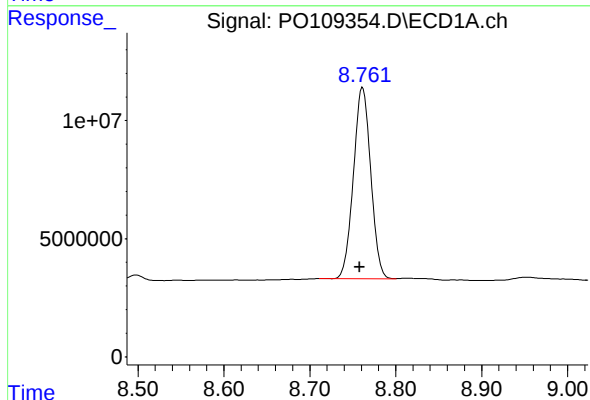

#2 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: 0.003 min
Response: 113389265
Conc: 16.37 ng/ml

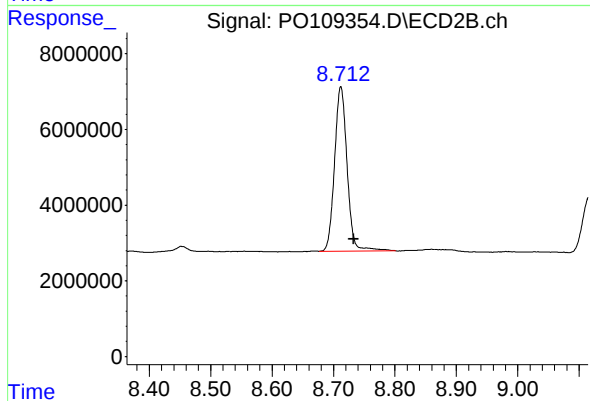

#2 Decachlorobiphenyl

R.T.: 8.712 min
Delta R.T.: -0.021 min
Response: 61750325
Conc: 17.96 ng/ml