


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141434.D
Acq On : 05 Feb 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

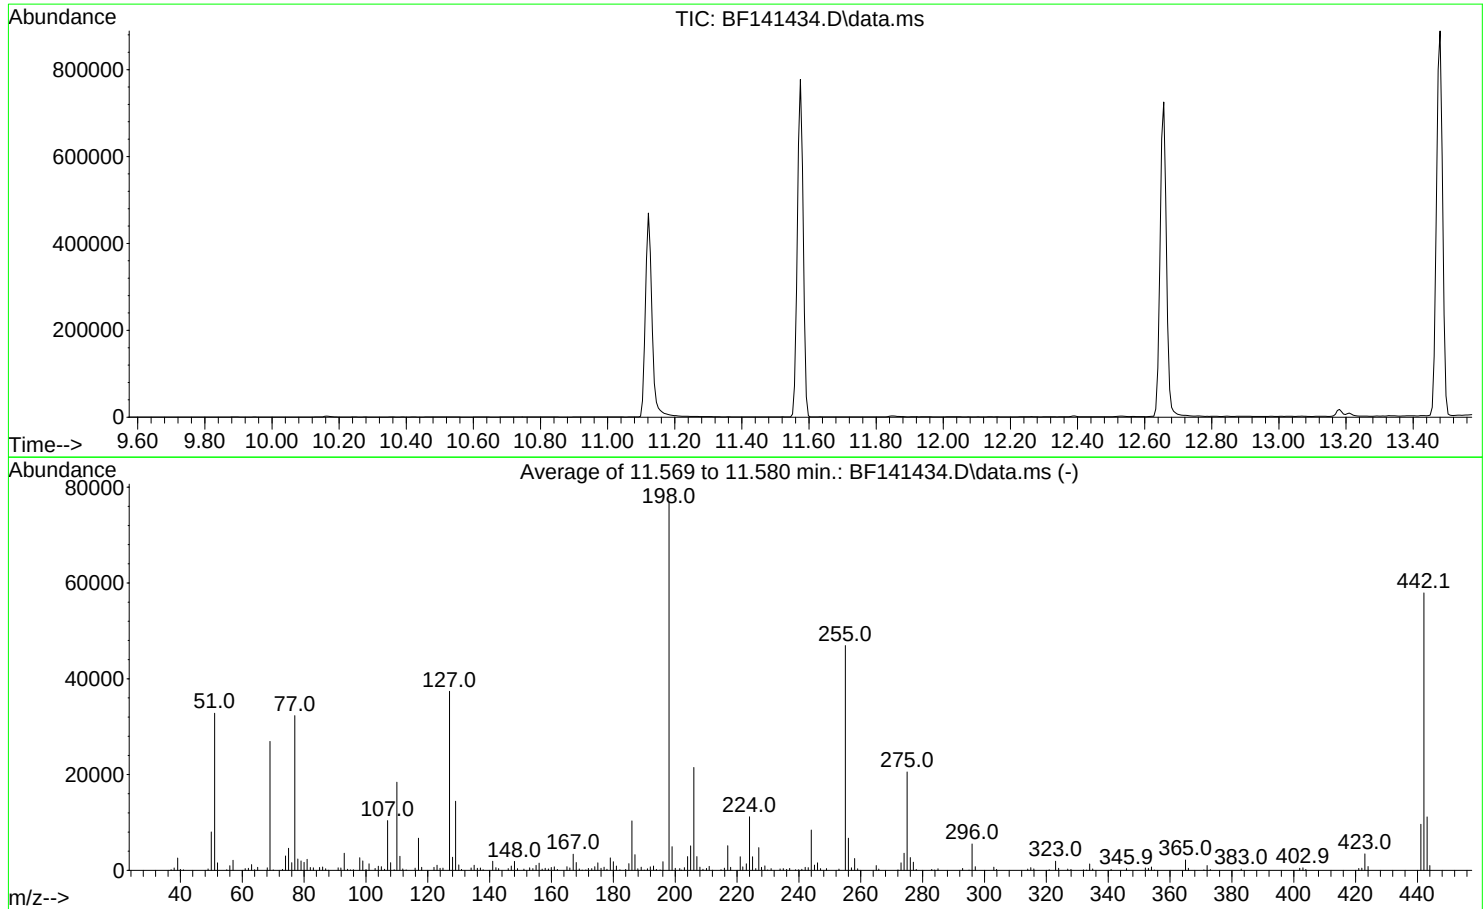

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	42.7	32805	PASS
68	69	0.00	2	2.0	529	PASS
69	198	0.00	100	35.1	26925	PASS
70	69	0.00	2	0.4	108	PASS
127	198	10	80	48.7	37376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76800	PASS
199	198	5	9	6.4	4937	PASS
275	198	10	60	26.8	20563	PASS
365	198	1	100	2.8	2166	PASS
441	198	0.01	100	12.5	9611	PASS
442	442	50	100	100.0	57928	PASS
443	442	15	24	19.2	11149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/5/2025	BNA_F	<u>BF141434.D</u>
Compound Name	Response	Retention Time
DDT	219771	13.48
DDD	7608	13.18
DDE	480	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8088	227859	3.55

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141434.D
Acq On : 05 Feb 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 05 10:46:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

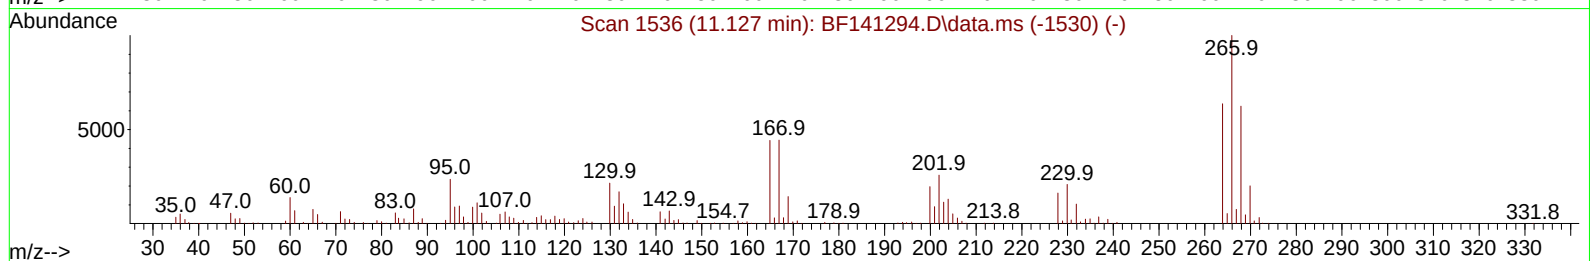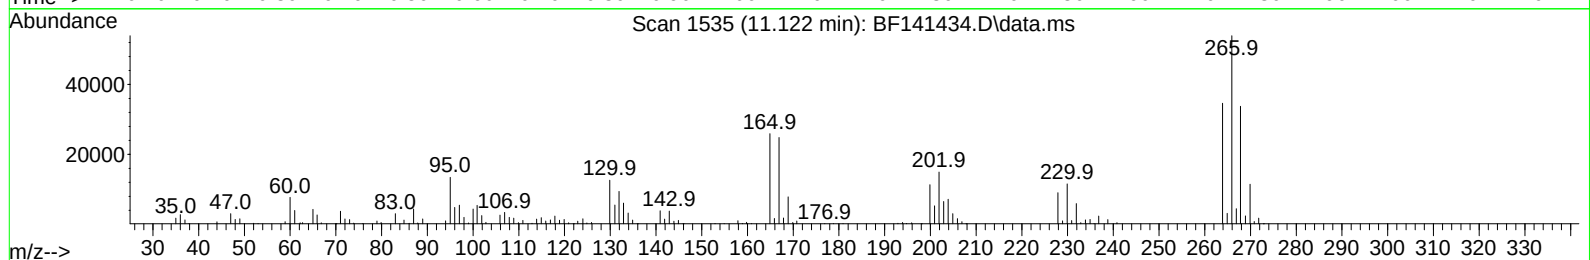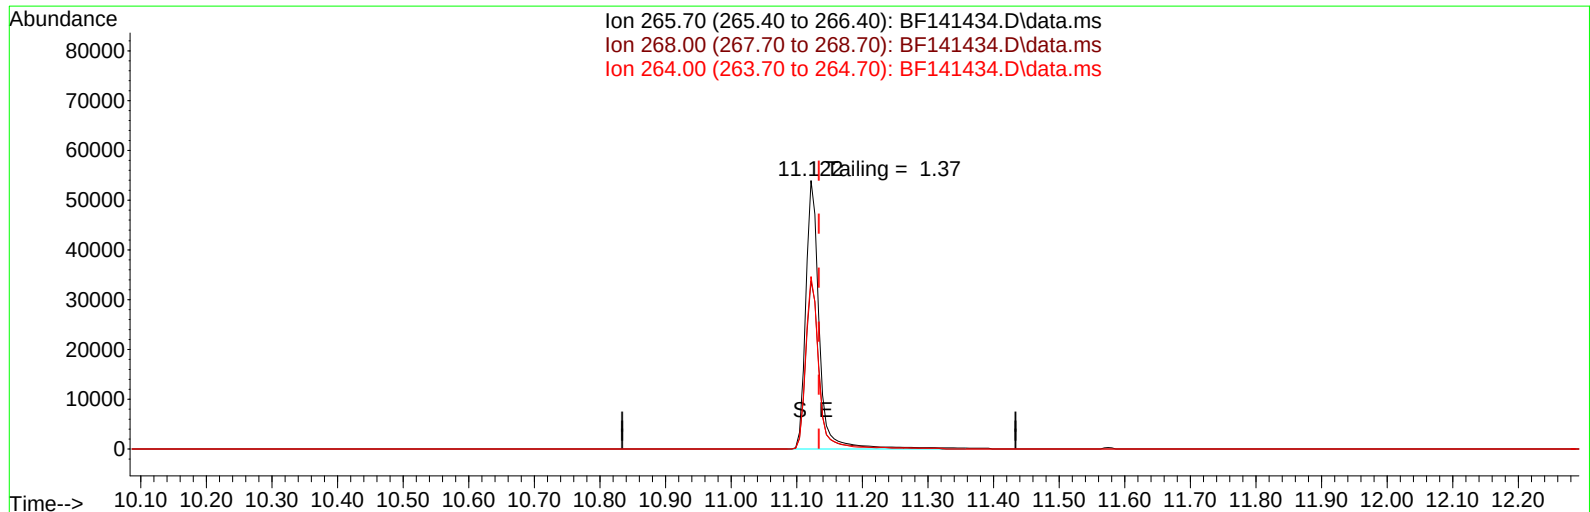

TIC: BF141434.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.012) 27136.66 ng




response 77371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.57
264.00	63.70	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141434.D
Acq On : 05 Feb 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 05 10:46:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

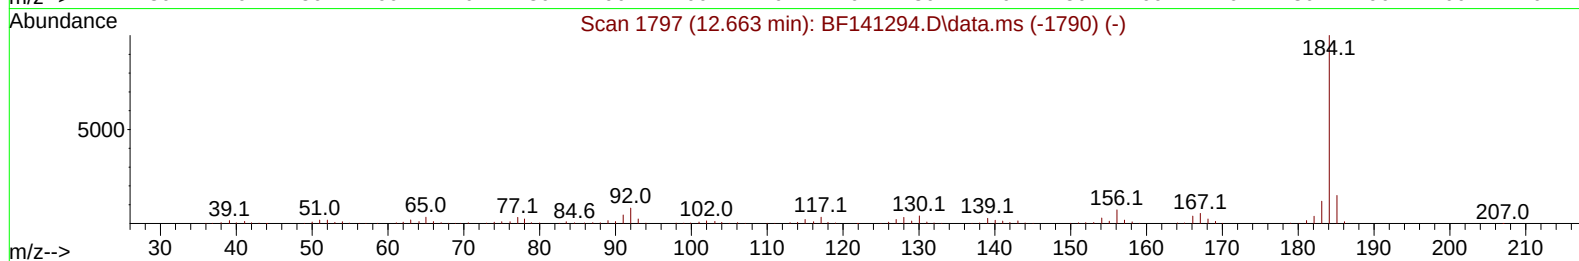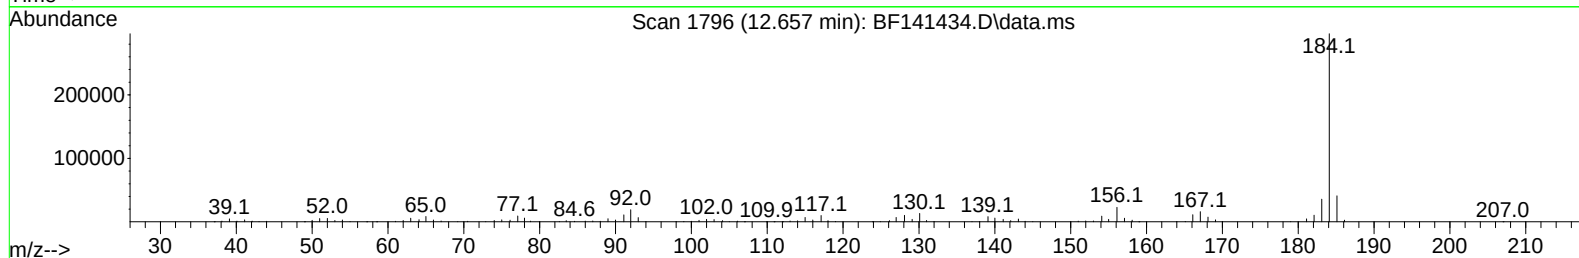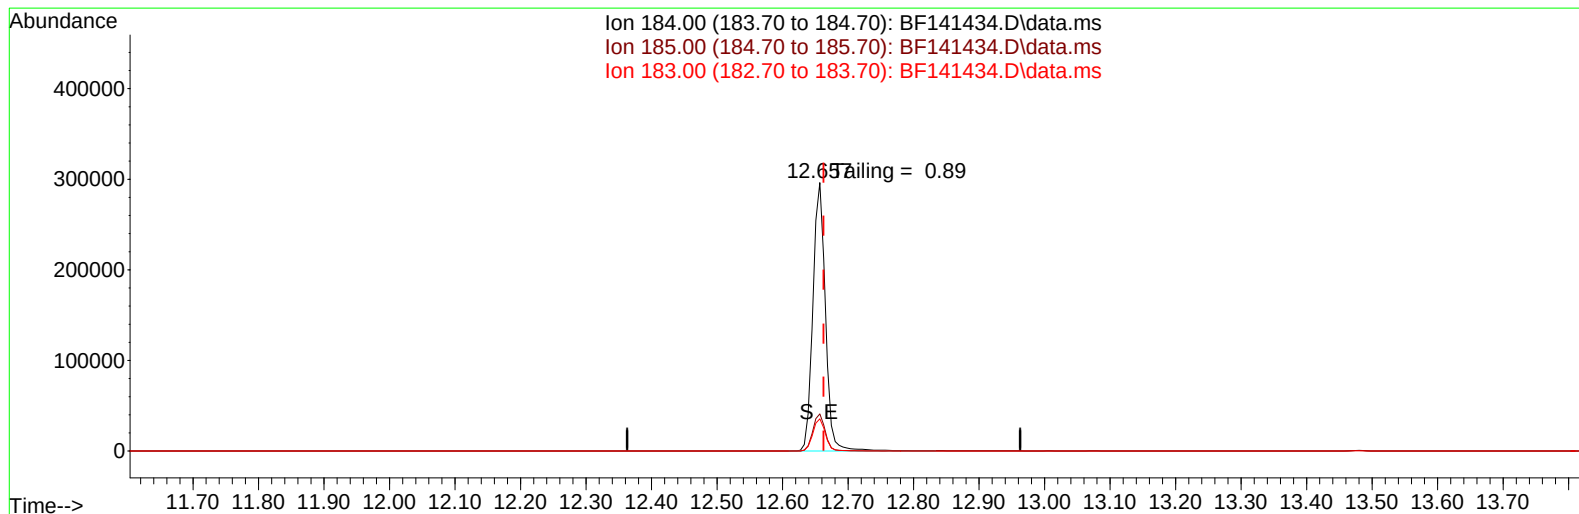

TIC: BF141434.D\data.ms

(77) Benzidine

12.657min (-0.006) 0.00 ng

response 393319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.83
183.00	11.90	12.02
0.00	0.00	0.00