
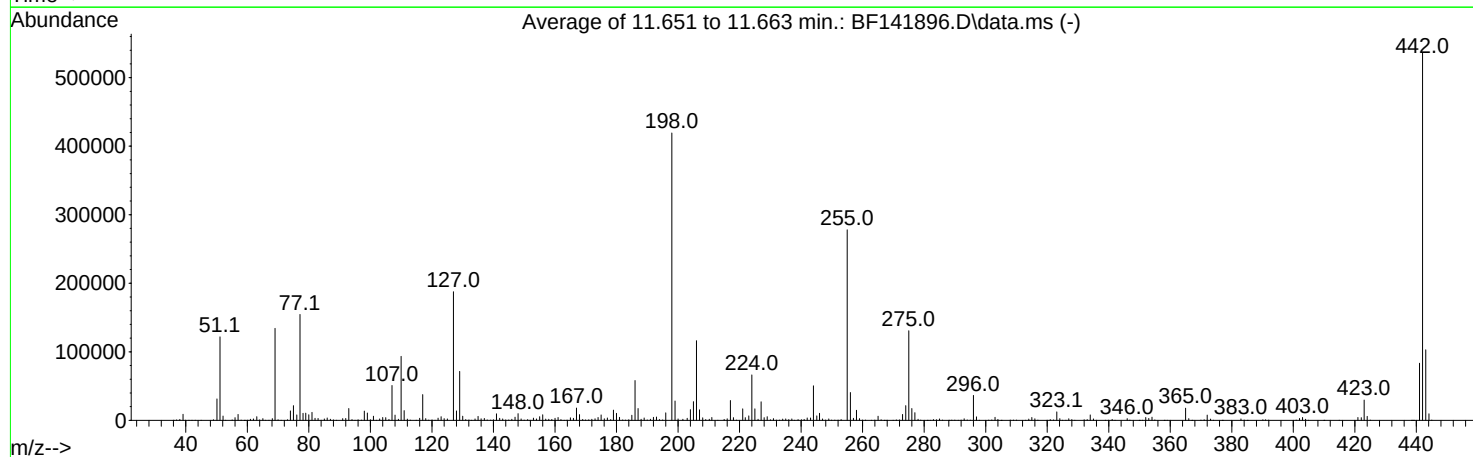


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

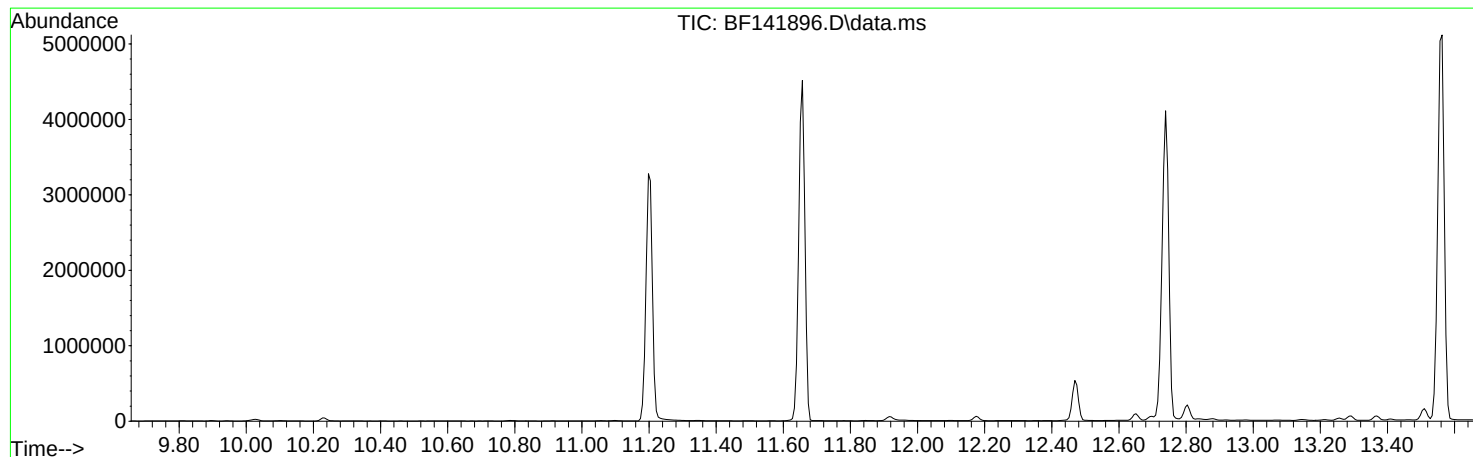

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	121957	PASS
68	69	0.00	2	1.9	2599	PASS
69	198	0.00	100	32.0	134239	PASS
70	69	0.00	2	0.7	949	PASS
127	198	10	80	44.8	187627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	419221	PASS
199	198	5	9	6.7	28280	PASS
275	198	10	60	31.2	130819	PASS
365	198	1	100	4.2	17803	PASS
441	198	0.01	100	19.9	83389	PASS
442	442	50	100	100.0	536640	PASS
443	442	15	24	19.2	102888	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/10/2025	BNA_F	<u>BF141896.D</u>
Compound Name	Response	Retention Time
DDT	1358235	13.562
DDD	20094	13.292
DDE	930	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21024	1379259	1.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

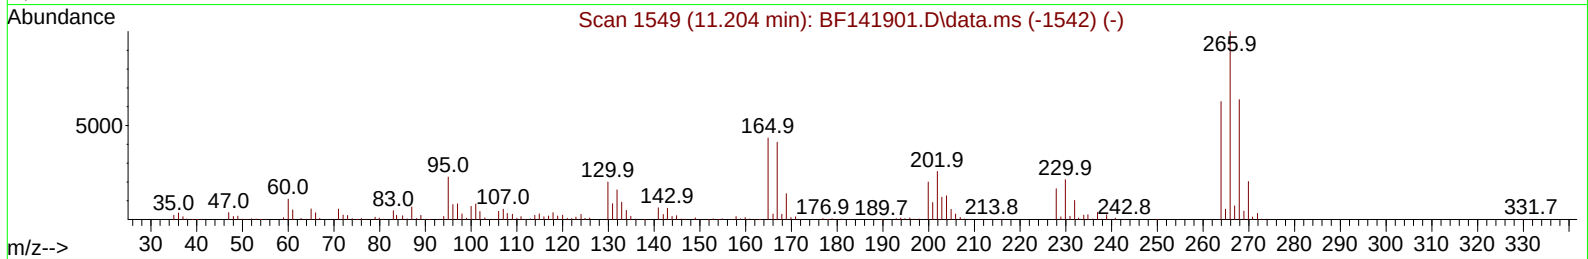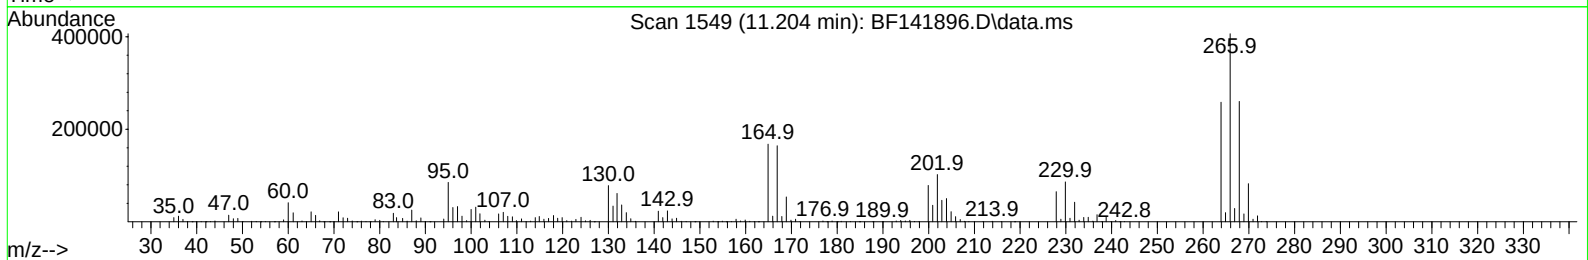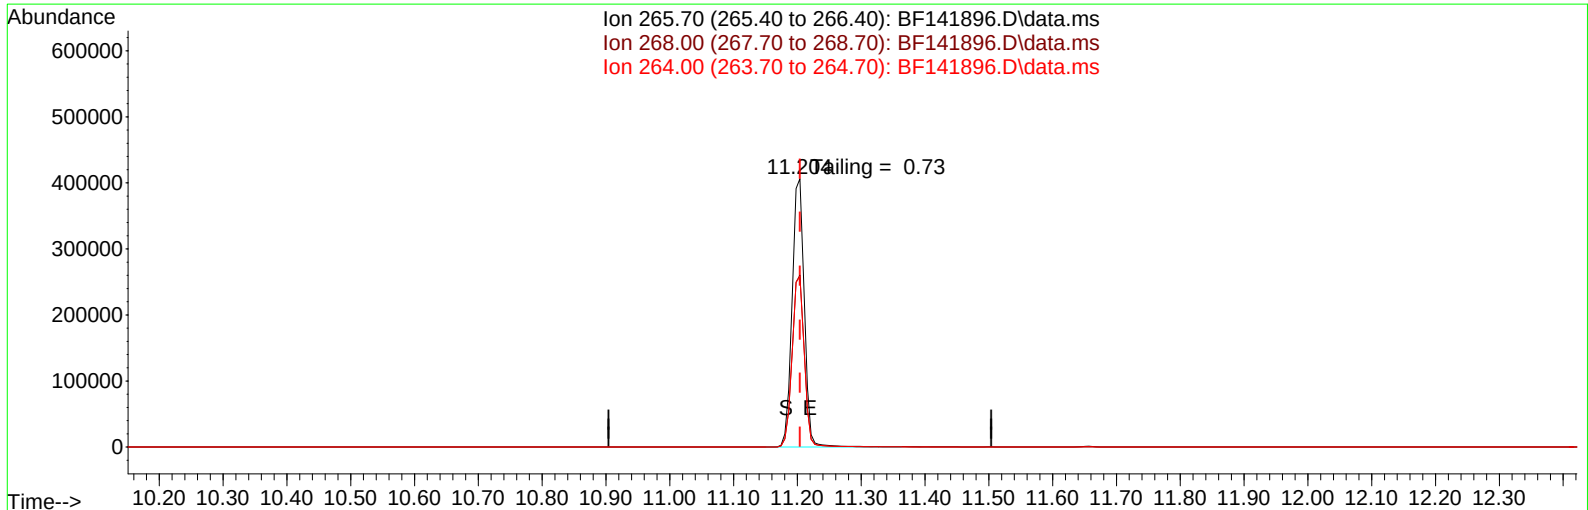

TIC: BF141896.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 118650.09 ng




response 544757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.05
264.00	62.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

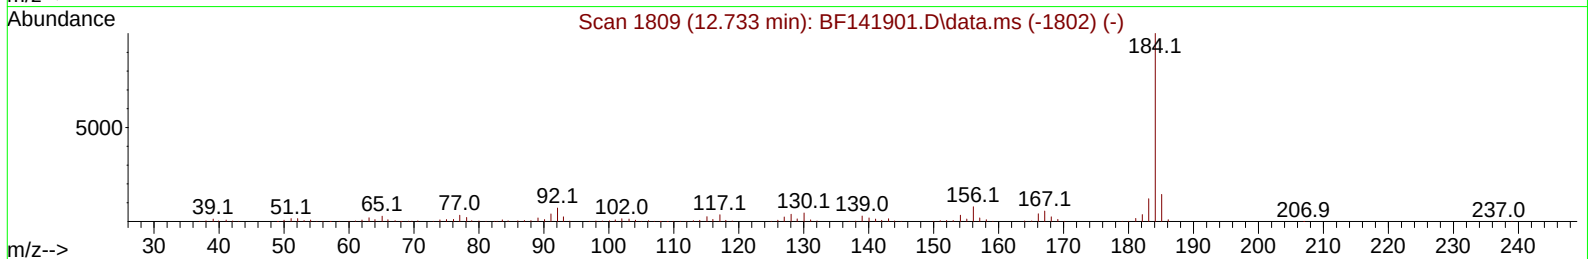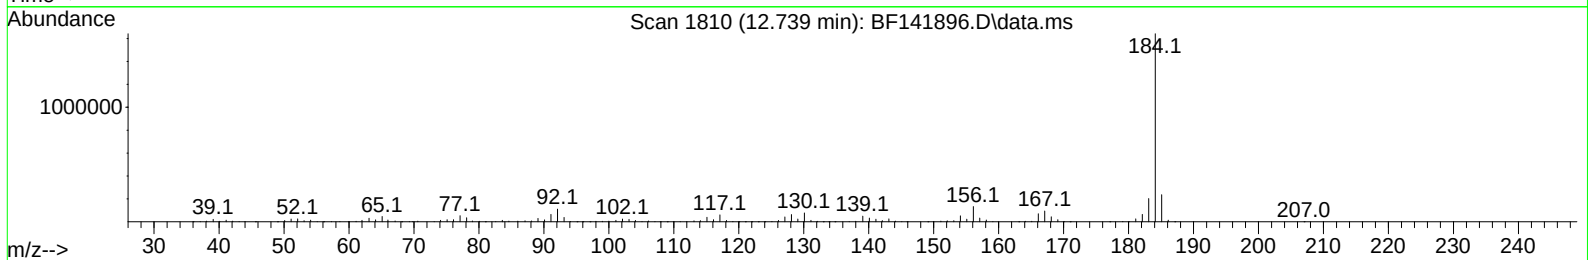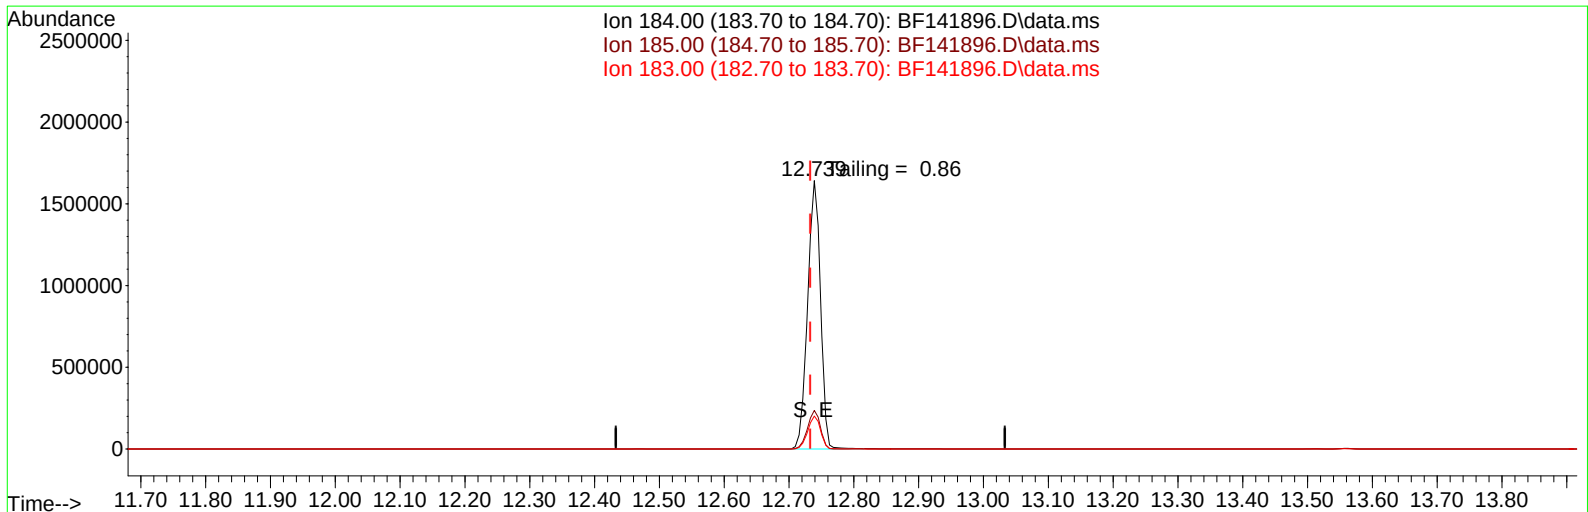

TIC: BF141896.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 203796.44 ng

response 2274676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.38
183.00	12.10	12.32
0.00	0.00	0.00