

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
 Data File : BF141382.D
 Acq On : 03 Feb 2025 21:17
 Operator : RC/JU
 Sample : Q1232-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JPP-42.1-012925

Quant Time: Feb 04 00:19:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 29 17:41:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	89109	20.000	ng	-0.01
21) Naphthalene-d8	8.075	136	351714	20.000	ng	-0.01
39) Acenaphthene-d10	9.827	164	188139	20.000	ng	-0.01
64) Phenanthrene-d10	11.316	188	319169	20.000	ng	-0.01
76) Chrysene-d12	13.957	240	226990	20.000	ng	-0.02
86) Perylene-d12	15.409	264	160771	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	781568	134.651	ng	0.02
7) Phenol-d6	6.439	99	943996	127.845	ng	0.00
23) Nitrobenzene-d5	7.357	82	700084	104.932	ng	-0.01
42) 2,4,6-Tribromophenol	10.622	330	280292	162.507	ng	-0.01
45) 2-Fluorobiphenyl	9.151	172	1259480	103.040	ng	-0.01
79) Terphenyl-d14	12.910	244	1391951	94.570	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020325\
Data File : BF141382.D
Acq On : 03 Feb 2025 21:17
Operator : RC/JU
Sample : Q1232-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JPP-42.1-012925

Quant Time: Feb 04 00:19:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration




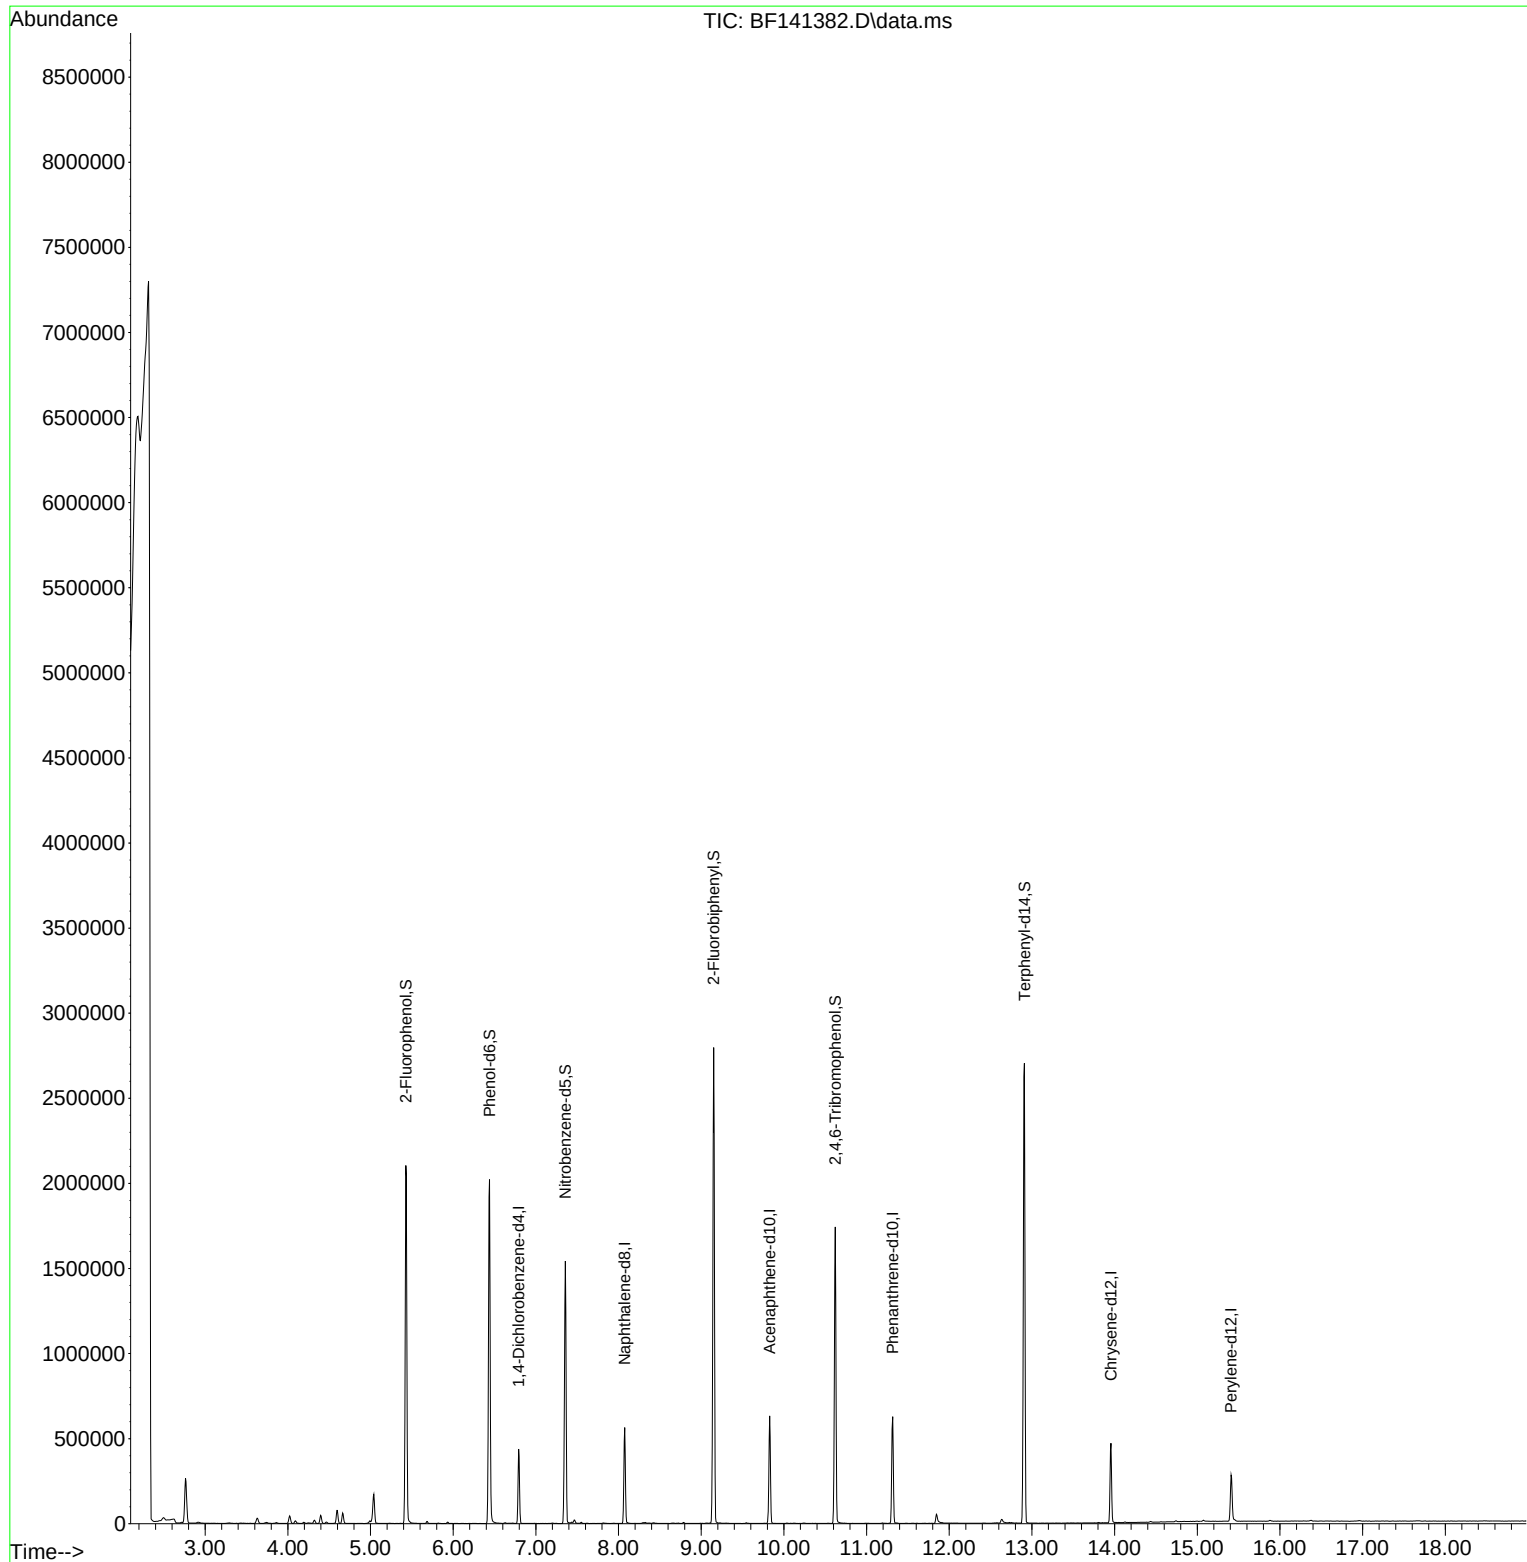


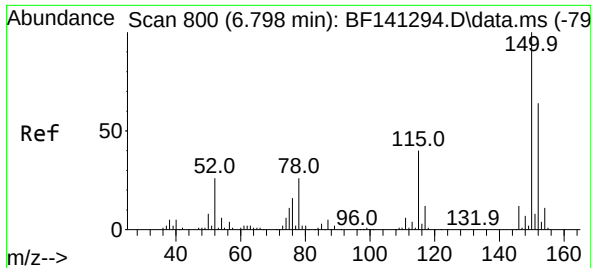

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.792 min Scan# 79
 Delta R.T. -0.012 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17




Instrument :
 BNA_F
 ClientSampleId :
 JPP-42.1-012925


Tgt Ion:152 Resp: 89109
 Ion Ratio Lower Upper
 152 100
 150 153.5 125.9 188.9
 115 63.0 49.7 74.5

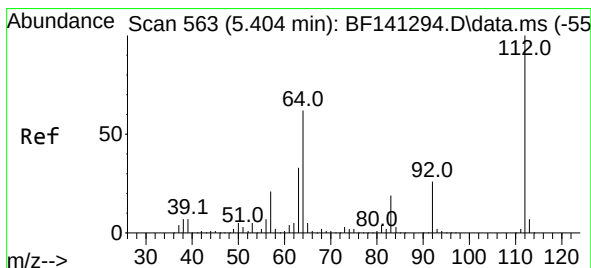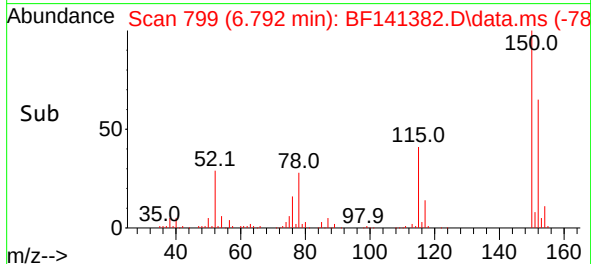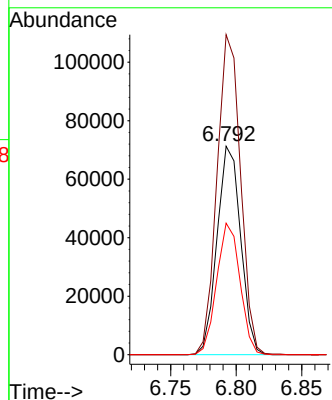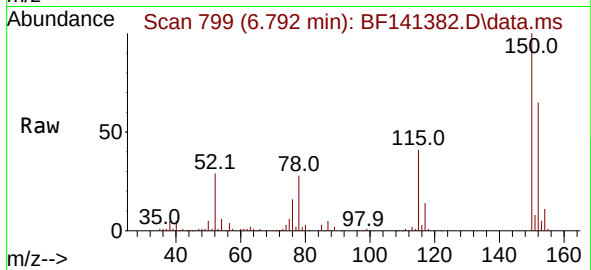

#5
 2-Fluorophenol
 Concen: 134.651 ng
 RT: 5.428 min Scan# 567
 Delta R.T. 0.017 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17

Tgt Ion:112 Resp: 781568
 Ion Ratio Lower Upper
 112 100
 64 64.4 49.8 74.8
 63 34.9 26.1 39.1


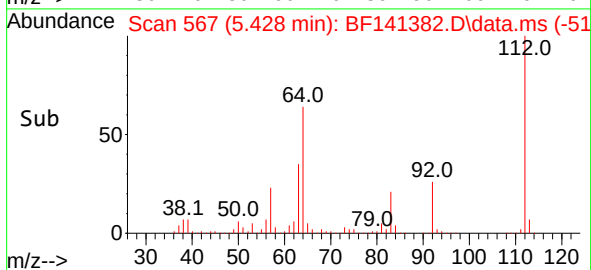
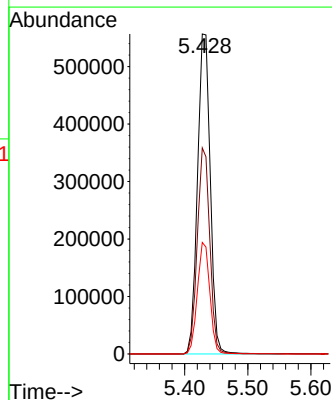
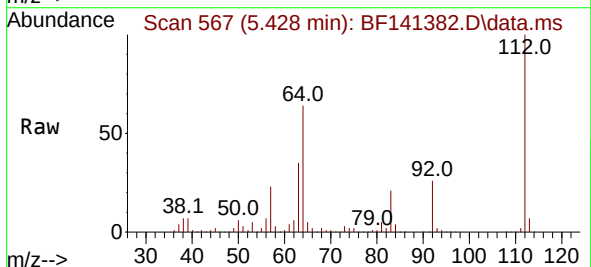


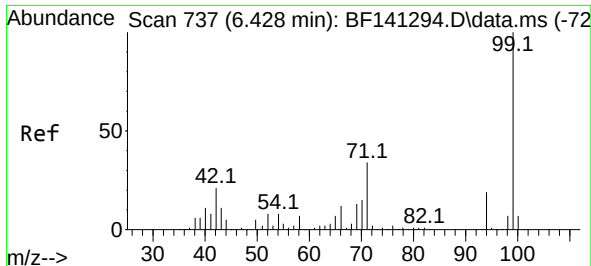

#7
Phenol-d6
Concen: 127.845 ng
RT: 6.439 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF141382.D
Acq: 03 Feb 2025 21:17




Instrument :
BNA_F
ClientSampleId :
JPP-42.1-012925


Tgt Ion: 99 Resp: 943996
Ion Ratio Lower Upper
99 100
42 22.2 17.1 25.7
71 37.3 26.9 40.3

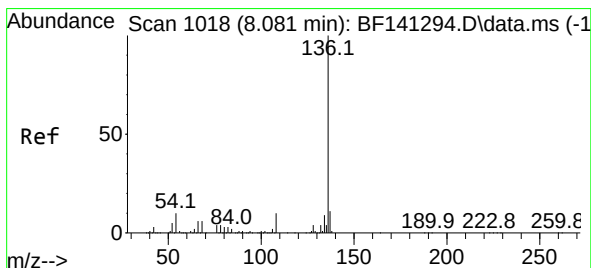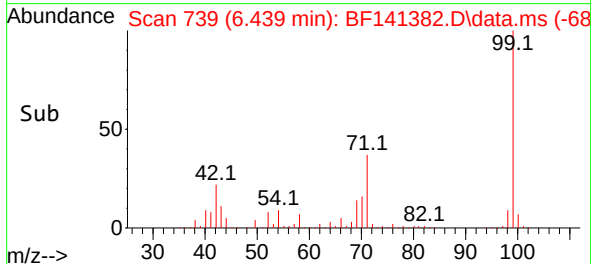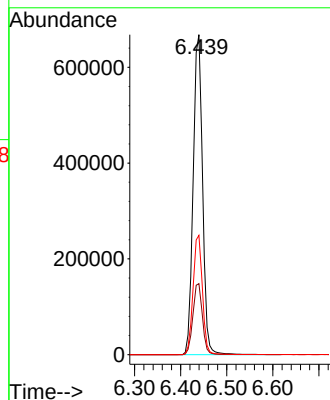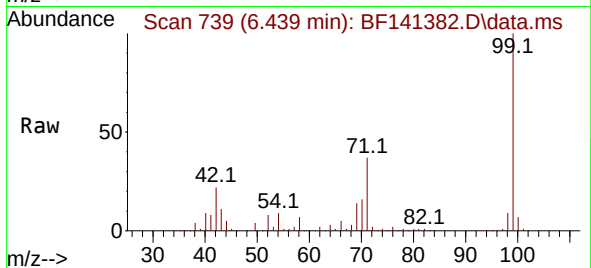

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.075 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF141382.D
Acq: 03 Feb 2025 21:17

Tgt Ion: 136 Resp: 351714
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 9.0 7.8 11.8
68 5.0 4.9 7.3


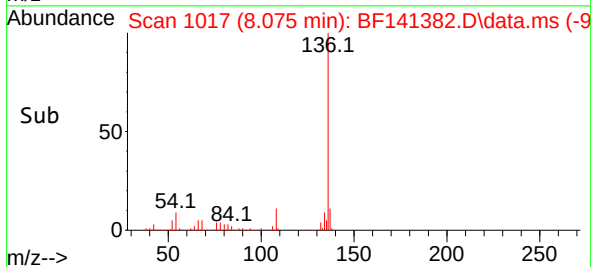
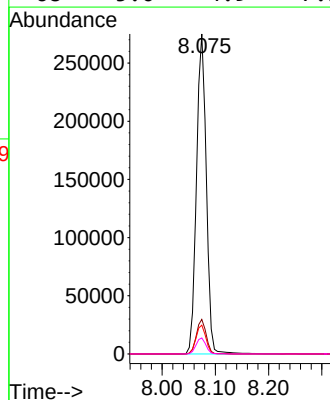
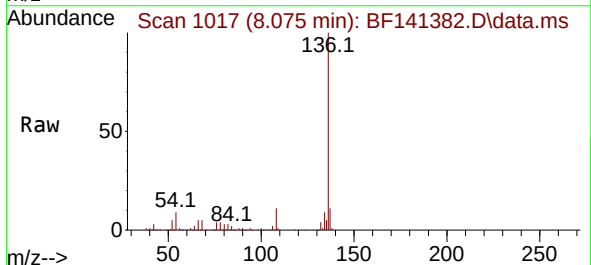


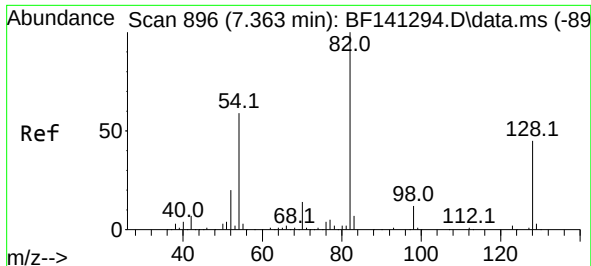

#23
 Nitrobenzene-d5
 Concen: 104.932 ng
 RT: 7.357 min Scan# 895
 Delta R.T. -0.012 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17




Instrument :
 BNA_F
 ClientSampleId :
 JPP-42.1-012925


Tgt Ion: 82 Resp: 700084
 Ion Ratio Lower Upper
 82 100
 128 43.4 35.7 53.5
 54 58.8 47.1 70.7

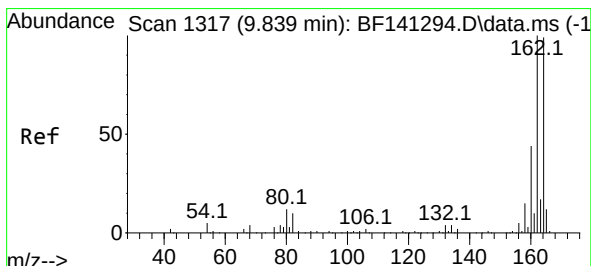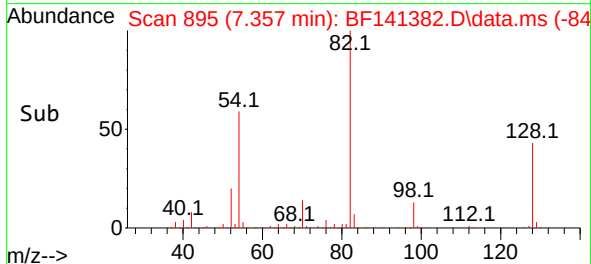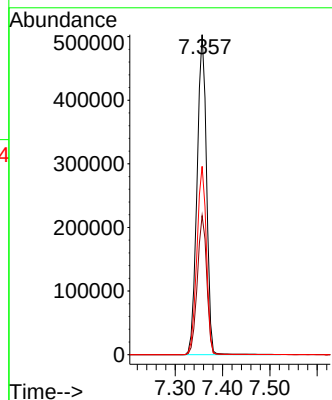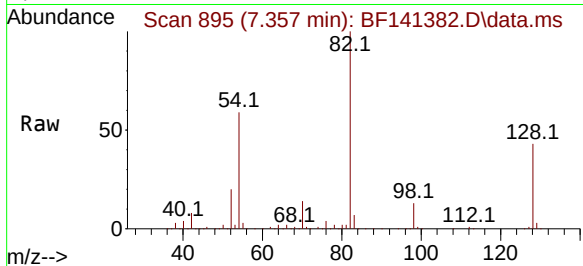

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.827 min Scan# 1315
 Delta R.T. -0.012 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17

Tgt Ion:164 Resp: 188139
 Ion Ratio Lower Upper
 164 100
 162 103.1 80.6 121.0
 160 45.2 35.8 53.6

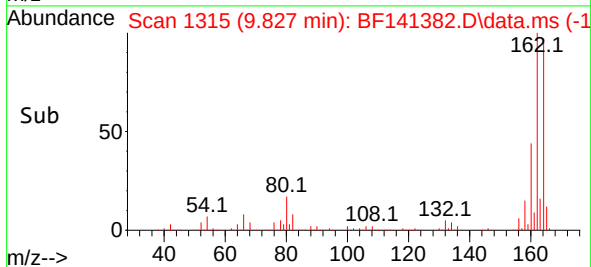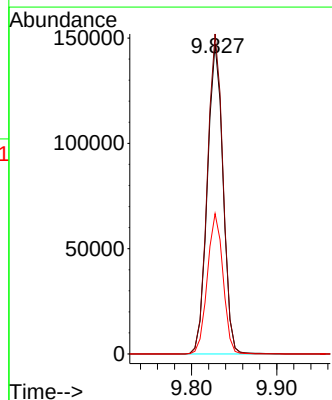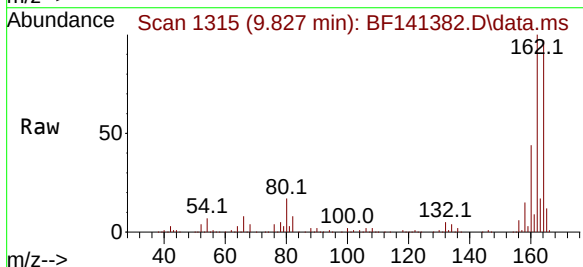

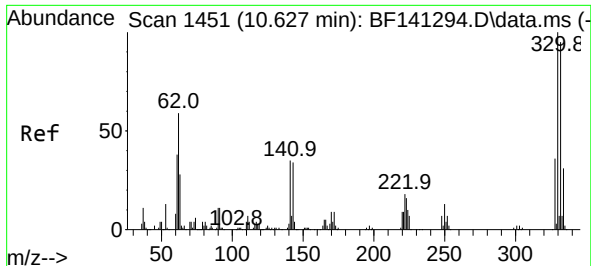

#42

2,4,6-Tribromophenol

Concen: 162.507 ng

RT: 10.622 min Scan# 1451

Delta R.T. -0.012 min

Lab File: BF141382.D


Acq: 03 Feb 2025 21:17

Instrument :

BNA_F

ClientSampleId :

JPP-42.1-012925

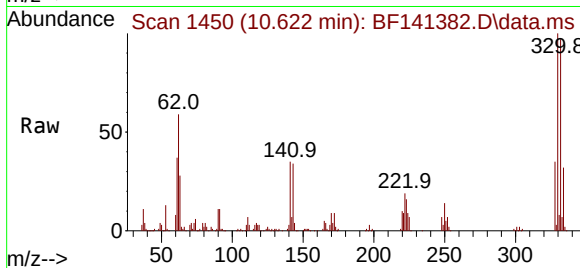




Tgt Ion:330 Resp: 280292

Ion Ratio Lower Upper

330 100

332 96.8 76.1 114.1

141 36.0 28.8 43.2

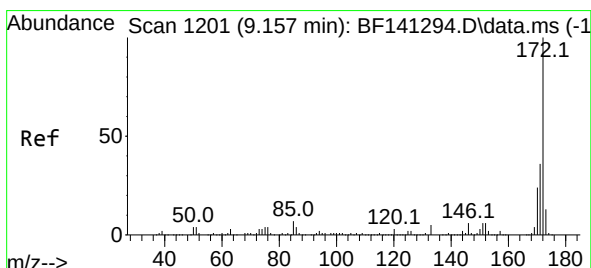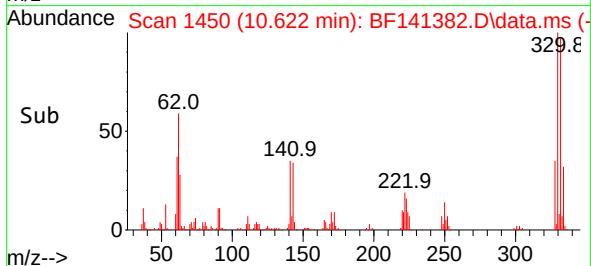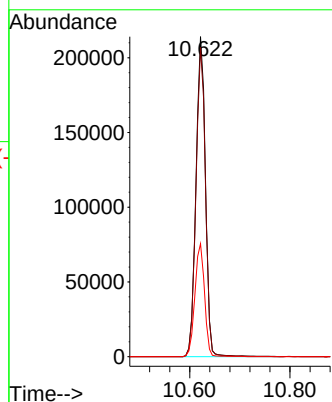

#45

2-Fluorobiphenyl

Concen: 103.040 ng

RT: 9.151 min Scan# 1200

Delta R.T. -0.012 min

Lab File: BF141382.D

Acq: 03 Feb 2025 21:17




Tgt Ion:172 Resp: 1259480


Ion Ratio Lower Upper

172 100

171 35.8 28.8 43.2


170 23.8 19.0 28.6

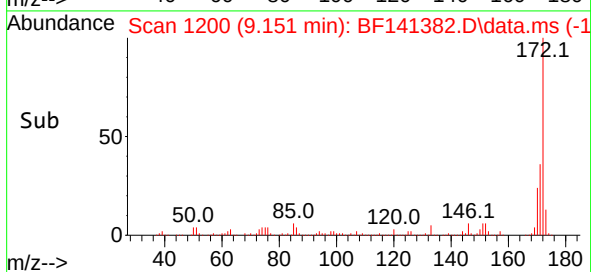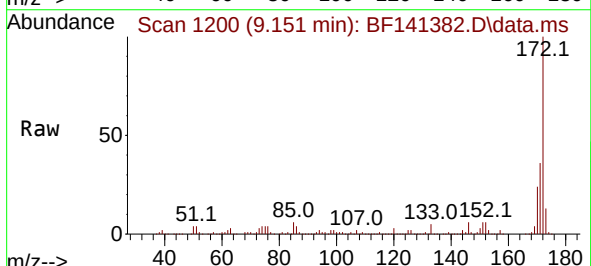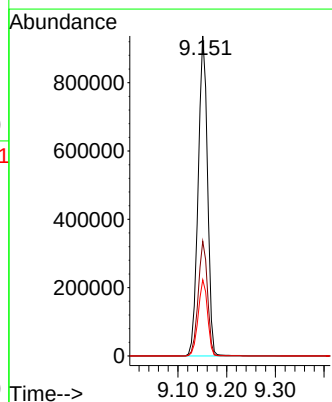



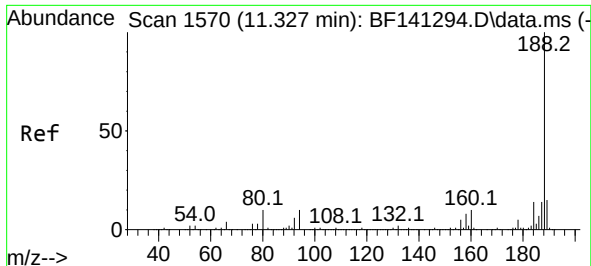


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.316 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF141382.D
Acq: 03 Feb 2025 21:17

Instrument :
BNA_F
ClientSampleId :
JPP-42.1-012925



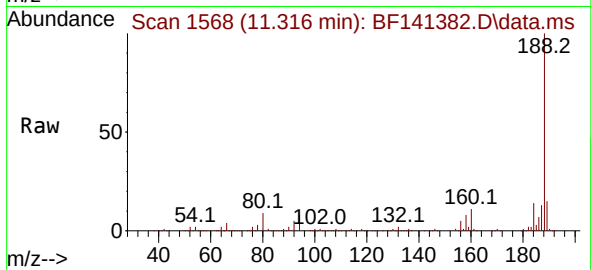



Tgt Ion:188 Resp: 319169
Ion Ratio Lower Upper
188 100
94 8.5 7.8 11.6
80 9.1 8.2 12.4

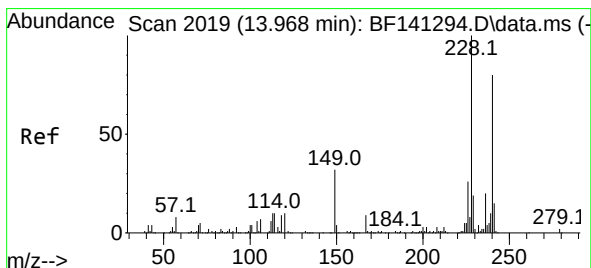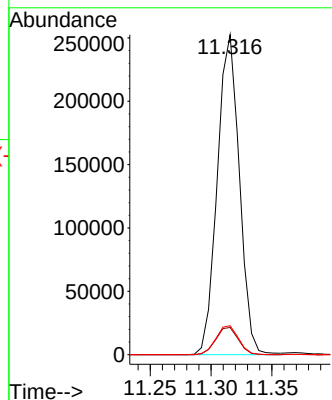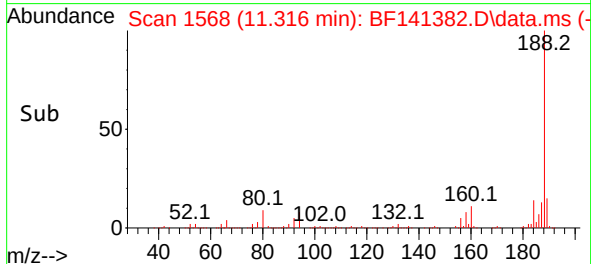

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 2017
Delta R.T. -0.018 min
Lab File: BF141382.D
Acq: 03 Feb 2025 21:17


Tgt Ion:240 Resp: 226990
Ion Ratio Lower Upper
240 100
120 10.7 10.0 15.0
236 25.4 19.7 29.5

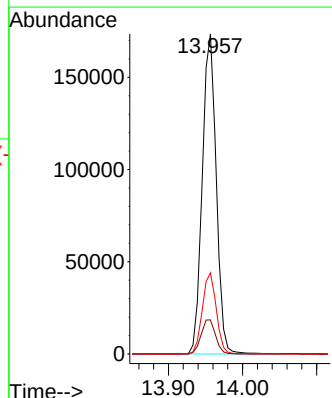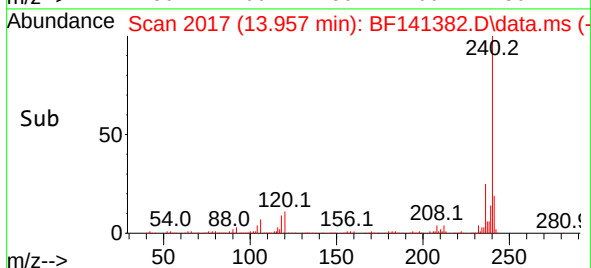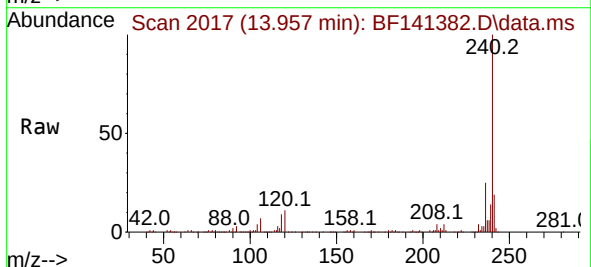



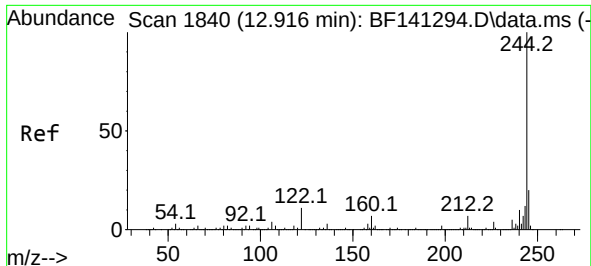


#79
 Terphenyl-d14
 Concen: 94.570 ng
 RT: 12.910 min Scan# 1839
 Delta R.T. -0.006 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17


Instrument :
 BNA_F
 ClientSampleId :
 JPP-42.1-012925

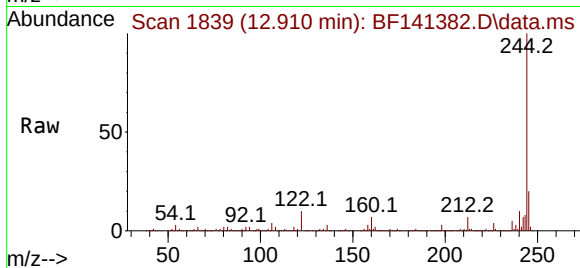

Tgt Ion:244 Resp: 1391951
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 10.5 8.8 13.2

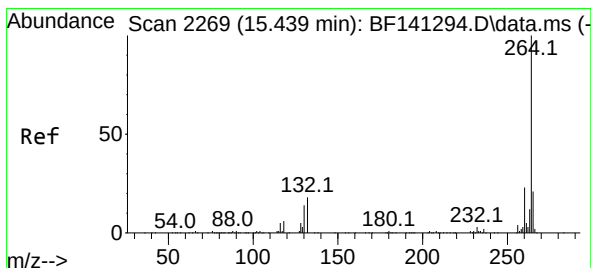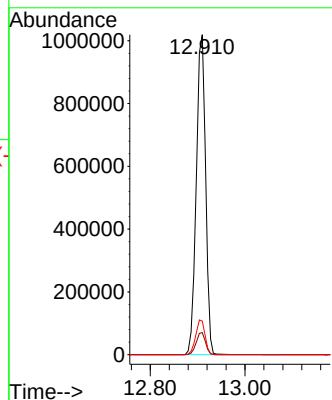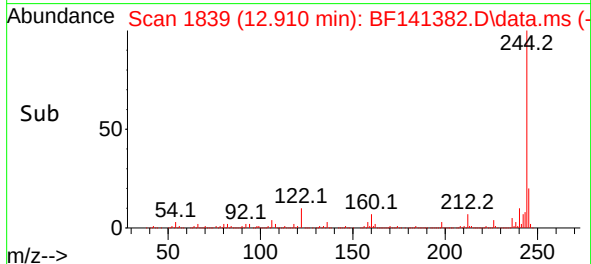

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.409 min Scan# 2264
 Delta R.T. -0.030 min
 Lab File: BF141382.D
 Acq: 03 Feb 2025 21:17

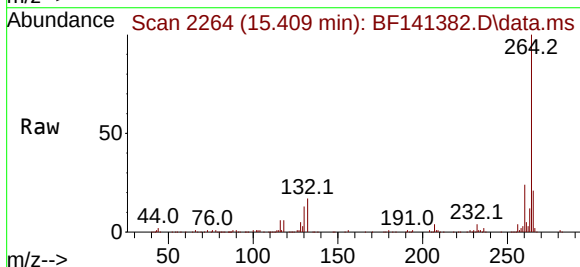

Tgt Ion:264 Resp: 160771
 Ion Ratio Lower Upper
 264 100
 260 23.7 18.6 27.8
 265 21.1 16.7 25.1

