

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012325\
 Data File : FE052030.D
 Signal(s) : FID1B.ch
 Acq On : 24 Jan 2025 00:06
 Operator : YP\AJ
 Sample : 10 TRPH STD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 10 TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 24 03:02:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
 Quant Title :
 QLast Update : Fri Jan 24 03:00:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.253	1061033	11.396 ug/ml
Target Compounds			
1) N-OCTANE	2.412	889828	11.012 ug/ml
2) N-DECANE	4.906	959030	11.079 ug/ml
3) N-DODECANE	7.033	1052037	11.161 ug/ml
4) N-TETRADECANE	8.839	1077547	11.283 ug/ml
5) N-HEXADECANE	10.432	1131977	11.345 ug/ml
6) N-OCTADECANE	11.865	1193205	11.371 ug/ml
7) N-EICOSANE	13.167	1184917	11.402 ug/ml
8) N-DOCOSANE	14.358	1182709	11.434 ug/ml
10) N-TETRACOSANE	15.456	1180708	11.429 ug/ml
11) N-HEXACOSANE	16.473	1163260	11.428 ug/ml
12) N-OCTACOSANE	17.419	1147105	11.391 ug/ml
13) N-TRIACONTANE	18.304	1137270	11.430 ug/ml
14) N-DOTRIACONTANE	19.134	1110748	11.493 ug/ml
15) N-TETRATRIACONTANE	19.915	1019077	11.732 ug/ml
16) N-HEXATRIACONTANE	20.653	911856	12.238 ug/ml
17) N-OCTATRIACONTANE	21.439	859350	12.480 ug/ml
18) N-TETRACONTANE	22.441	882539	13.114 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012325\
Data File : FE052030.D
Signal(s) : FID1B.ch
Acq On : 24 Jan 2025 00:06
Operator : YP\AJ
Sample : 10 TRPH STD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

Integration File: autoint1.e
Quant Time: Jan 24 03:02:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:00:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

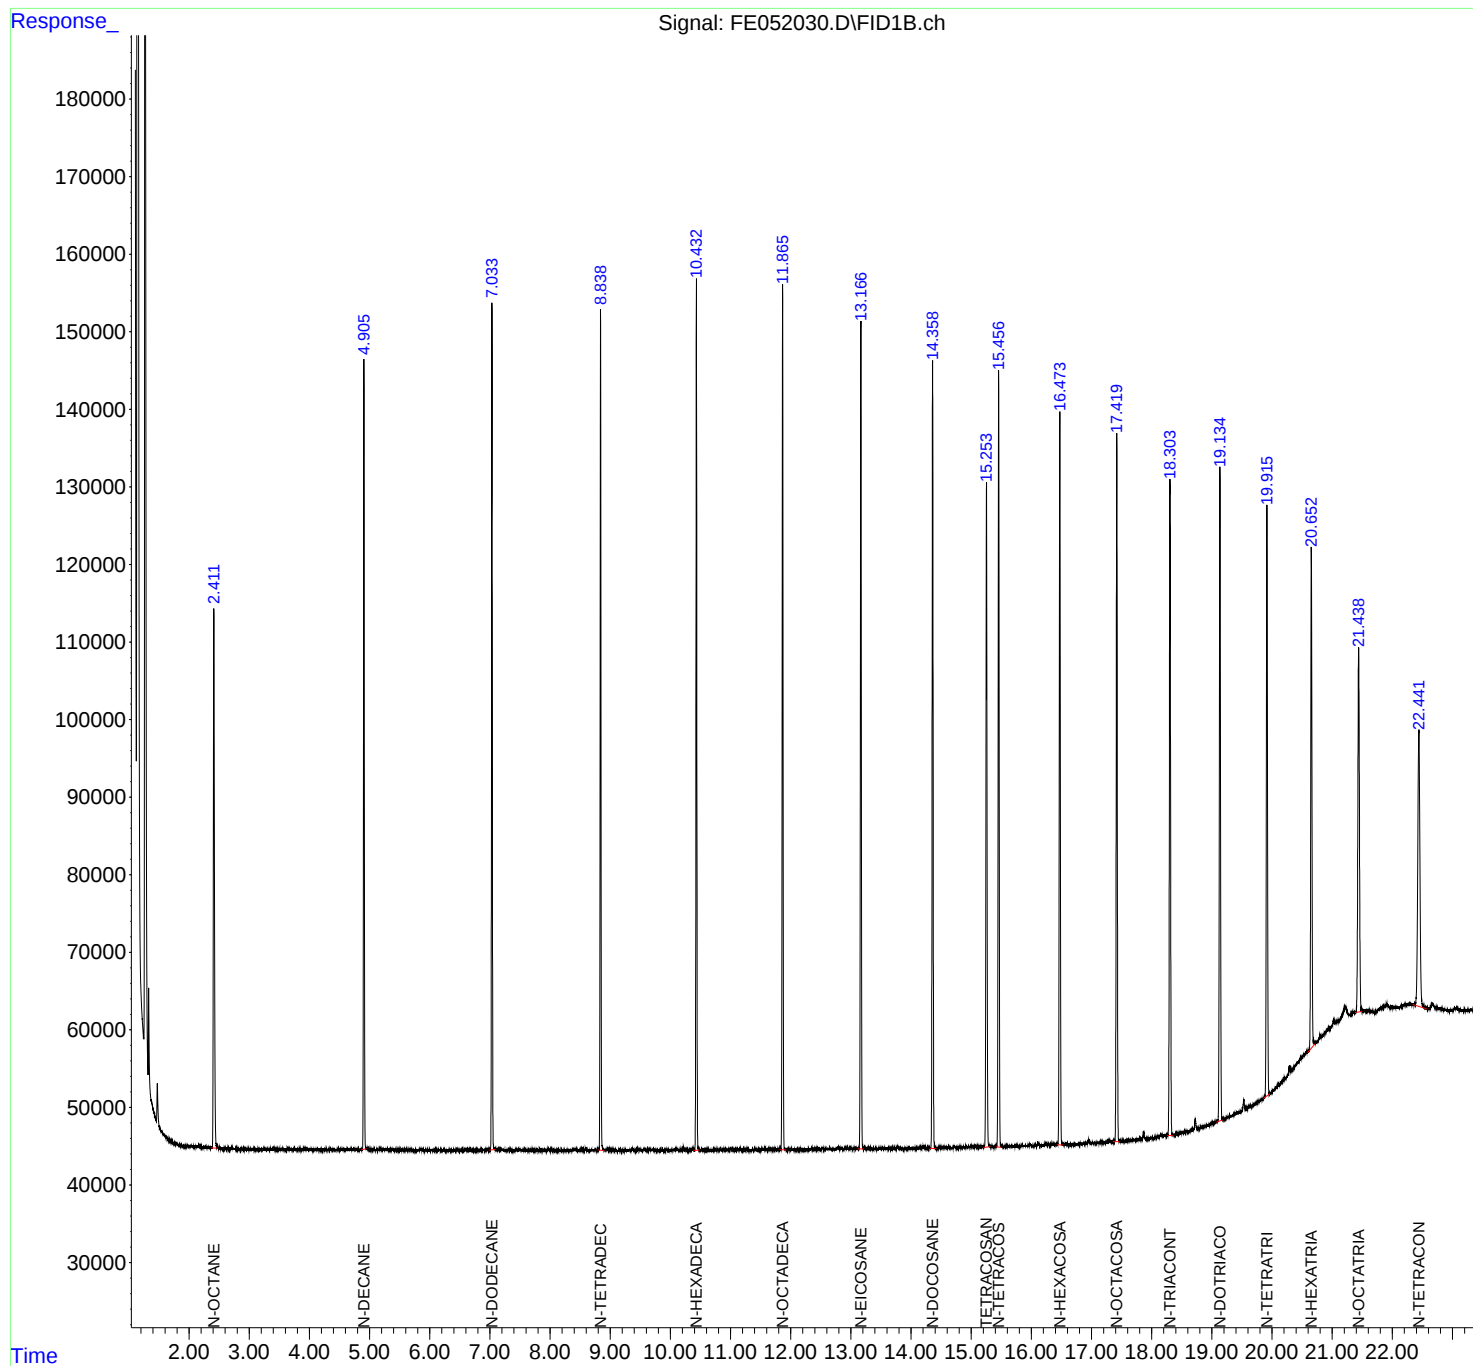


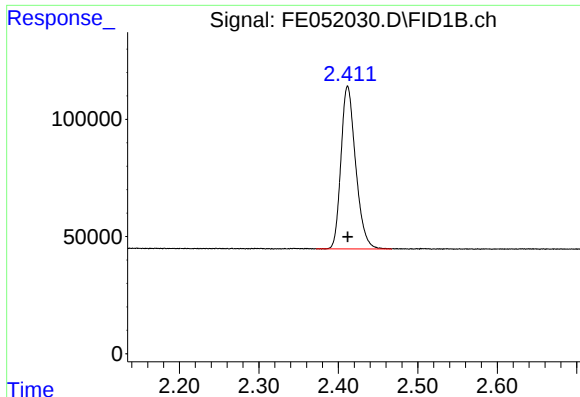

#1 N-OCTANE


R.T.: 2.412 min
Delta R.T.: 0.000 min
Response: 889828
Conc: 11.01 ug/ml

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

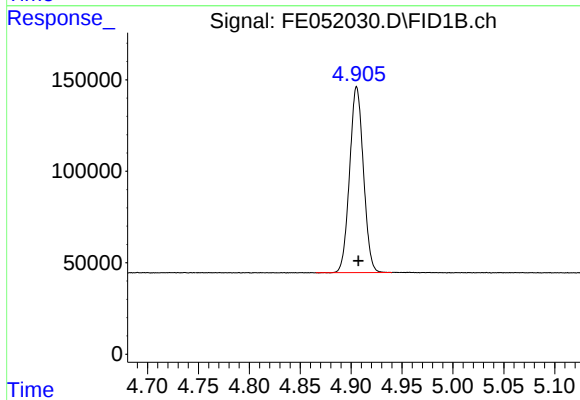


#2 N-DECANE

R.T.: 4.906 min
Delta R.T.: -0.002 min
Response: 959030
Conc: 11.08 ug/ml

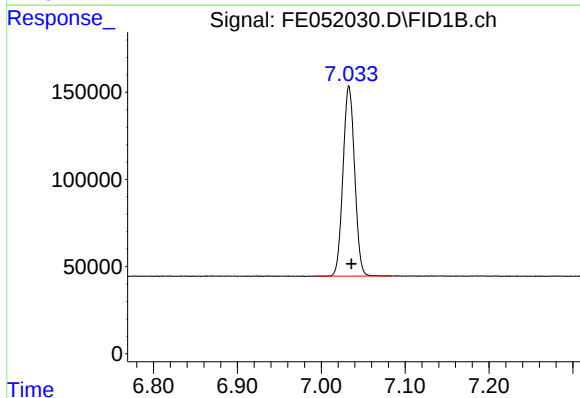


#3 N-DODECANE

R.T.: 7.033 min
Delta R.T.: -0.003 min
Response: 1052037
Conc: 11.16 ug/ml

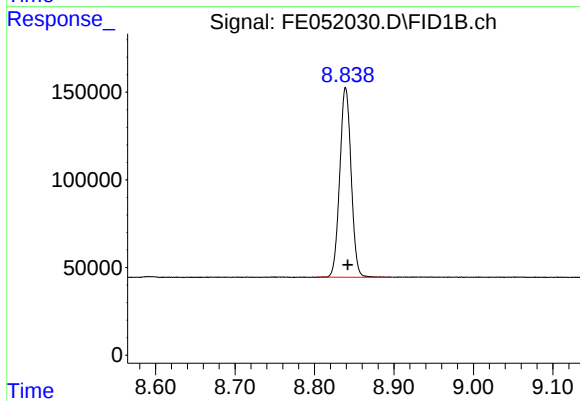

#4 N-TETRADECANE


R.T.: 8.839 min
Delta R.T.: -0.003 min
Response: 1077547
Conc: 11.28 ug/ml

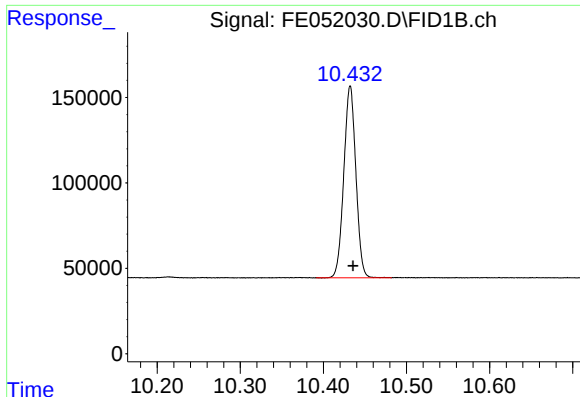

#5 N-HEXADECANE


R.T.: 10.432 min
Delta R.T.: -0.003 min
Response: 1131977
Conc: 11.34 ug/ml

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

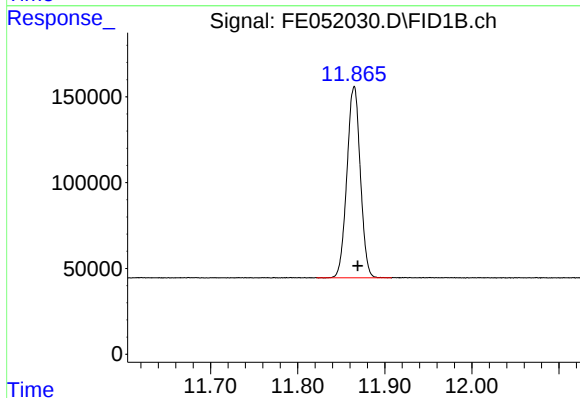


#6 N-OCTADECANE

R.T.: 11.865 min
Delta R.T.: -0.004 min
Response: 1193205
Conc: 11.37 ug/ml

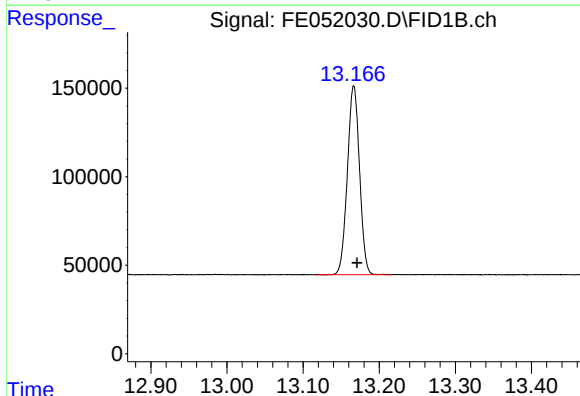


#7 N-EICOSANE

R.T.: 13.167 min
Delta R.T.: -0.004 min
Response: 1184917
Conc: 11.40 ug/ml

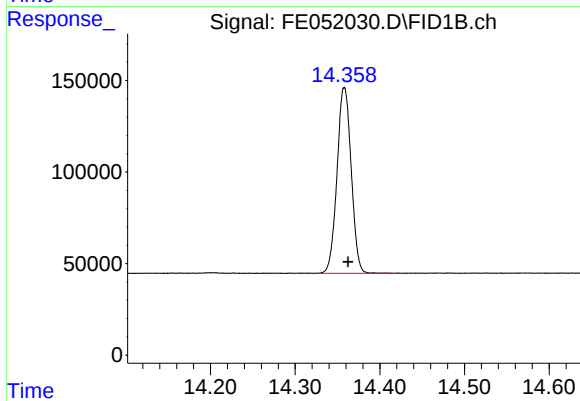

#8 N-DOCOSANE


R.T.: 14.358 min
Delta R.T.: -0.004 min
Response: 1182709
Conc: 11.43 ug/ml

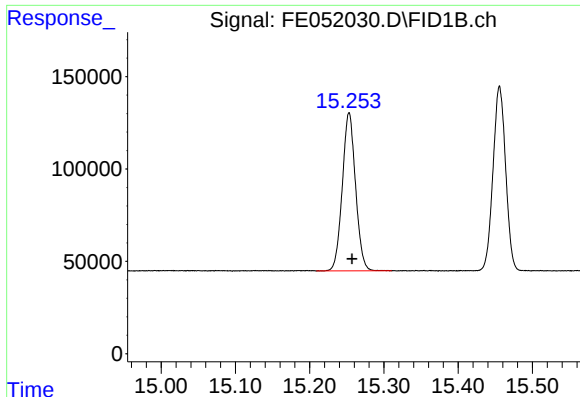

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.253 min
Delta R.T.: -0.004 min
Response: 1061033
Conc: 11.40 ug/ml

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

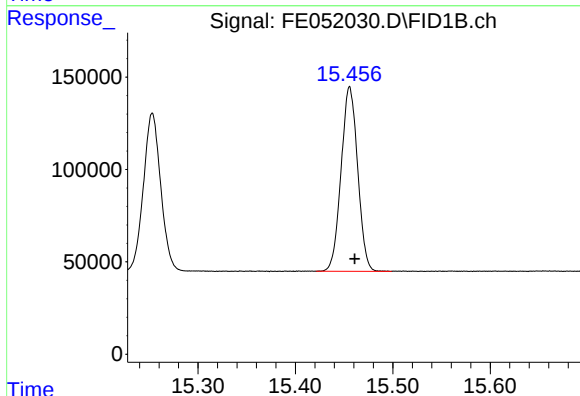


#10 N-TETRACOSANE

R.T.: 15.456 min
Delta R.T.: -0.005 min
Response: 1180708
Conc: 11.43 ug/ml

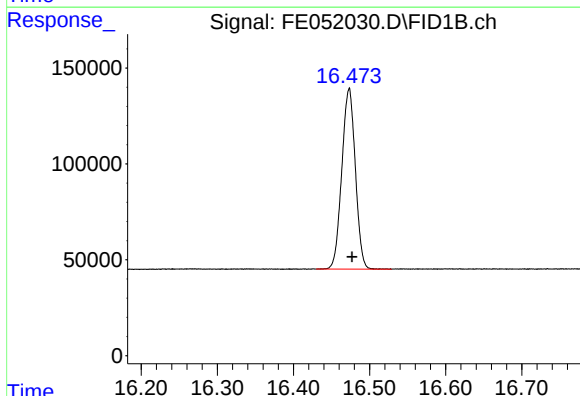


#11 N-HEXACOSANE

R.T.: 16.473 min
Delta R.T.: -0.004 min
Response: 1163260
Conc: 11.43 ug/ml

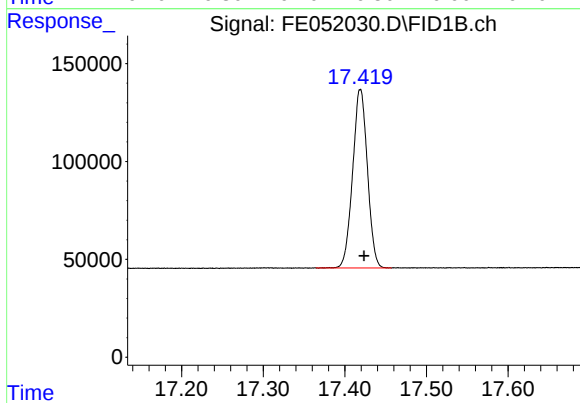

#12 N-OCTACOSANE


R.T.: 17.419 min
Delta R.T.: -0.005 min
Response: 1147105
Conc: 11.39 ug/ml

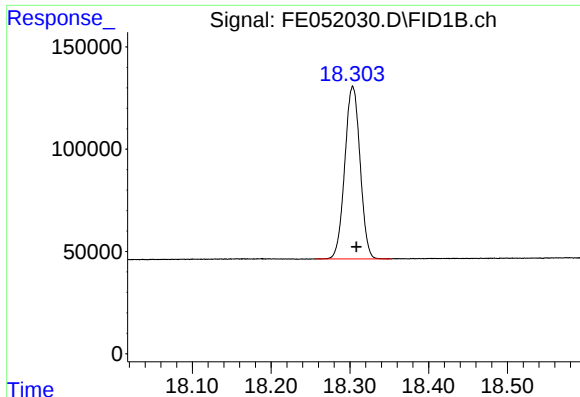

#13 N-TRIACONTANE


R.T.: 18.304 min
Delta R.T.: -0.004 min
Response: 1137270
Conc: 11.43 ug/ml

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

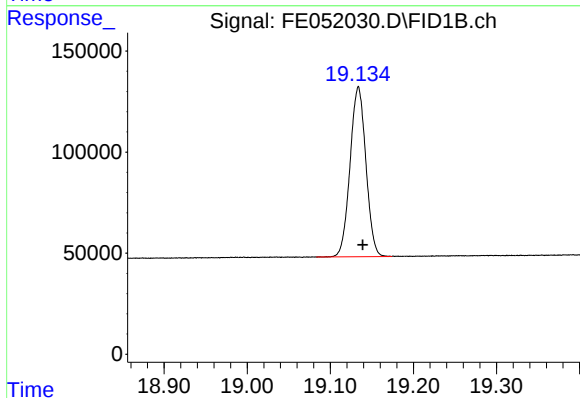


#14 N-DOTRIACONTANE

R.T.: 19.134 min
Delta R.T.: -0.005 min
Response: 1110748
Conc: 11.49 ug/ml

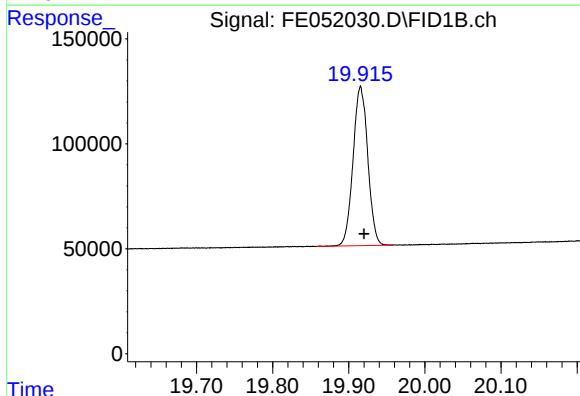


#15 N-TETRATRIACONTANE

R.T.: 19.915 min
Delta R.T.: -0.005 min
Response: 1019077
Conc: 11.73 ug/ml

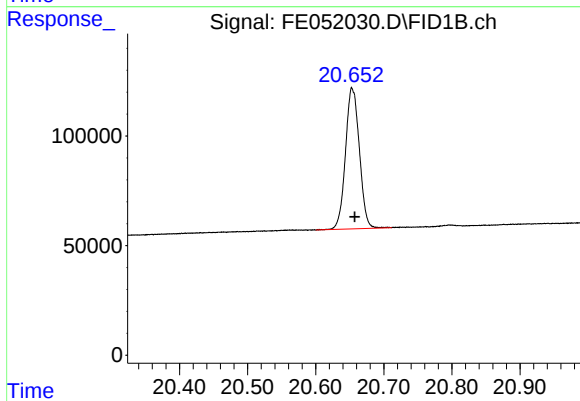

#16 N-HEXATRIACONTANE


R.T.: 20.653 min
Delta R.T.: -0.004 min
Response: 911856
Conc: 12.24 ug/ml

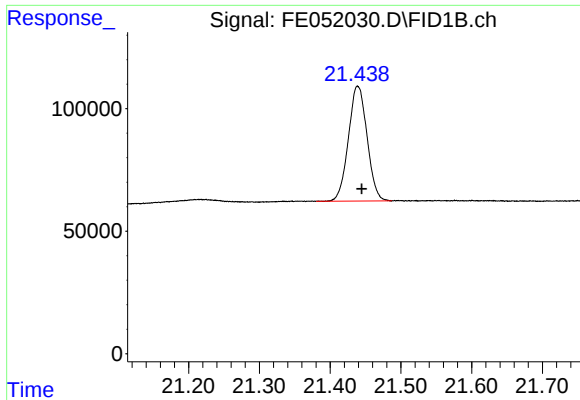

#17 N-OCTATRIACONTANE

R.T.: 21.439 min
Delta R.T.: -0.006 min
Response: 859350
Conc: 12.48 ug/ml

Instrument :
FID_E
ClientSampleId :
10 TRPH STD

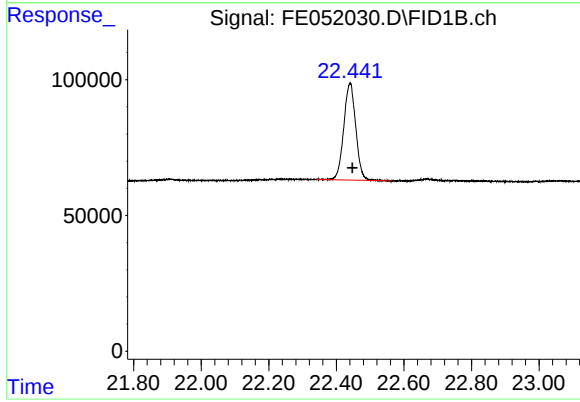

#18 N-TETRACONTANE

R.T.: 22.441 min
Delta R.T.: -0.006 min
Response: 882539
Conc: 13.11 ug/ml