

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012325\
 Data File : FE052031.D
 Signal(s) : FID1B.ch
 Acq On : 24 Jan 2025 00:36
 Operator : YP\AJ
 Sample : 5 TRPH STD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 5 TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 24 03:02:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
 Quant Title :
 QLast Update : Fri Jan 24 03:00:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.253	535796	5.755 ug/ml
Target Compounds			
1) N-OCTANE	2.412	447517	5.538 ug/ml
2) N-DECANE	4.906	479458	5.539 ug/ml
3) N-DODECANE	7.033	524622	5.565 ug/ml
4) N-TETRADECANE	8.839	538294	5.636 ug/ml
5) N-HEXADECANE	10.432	566935	5.682 ug/ml
6) N-OCTADECANE	11.864	597723	5.696 ug/ml
7) N-EICOSANE	13.166	599565	5.769 ug/ml
8) N-DOCOSANE	14.358	599958	5.800 ug/ml
10) N-TETRACOSANE	15.456	594003	5.750 ug/ml
11) N-HEXACOSANE	16.473	585191	5.749 ug/ml
12) N-OCTACOSANE	17.418	583549	5.795 ug/ml
13) N-TRIACONTANE	18.303	588228	5.912 ug/ml
14) N-DOTRIACONTANE	19.133	573000	5.929 ug/ml
15) N-TETRATRIACONTANE	19.915	509659	5.868 ug/ml
16) N-HEXATRIACONTANE	20.654	427588	5.739 ug/ml
17) N-OCTATRIACONTANE	21.439	394101	5.724 ug/ml
18) N-TETRACONTANE	22.438	382667	5.686 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012325\
Data File : FE052031.D
Signal(s) : FID1B.ch
Acq On : 24 Jan 2025 00:36
Operator : YP\AJ
Sample : 5 TRPH STD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

Integration File: autoint1.e
Quant Time: Jan 24 03:02:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:00:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

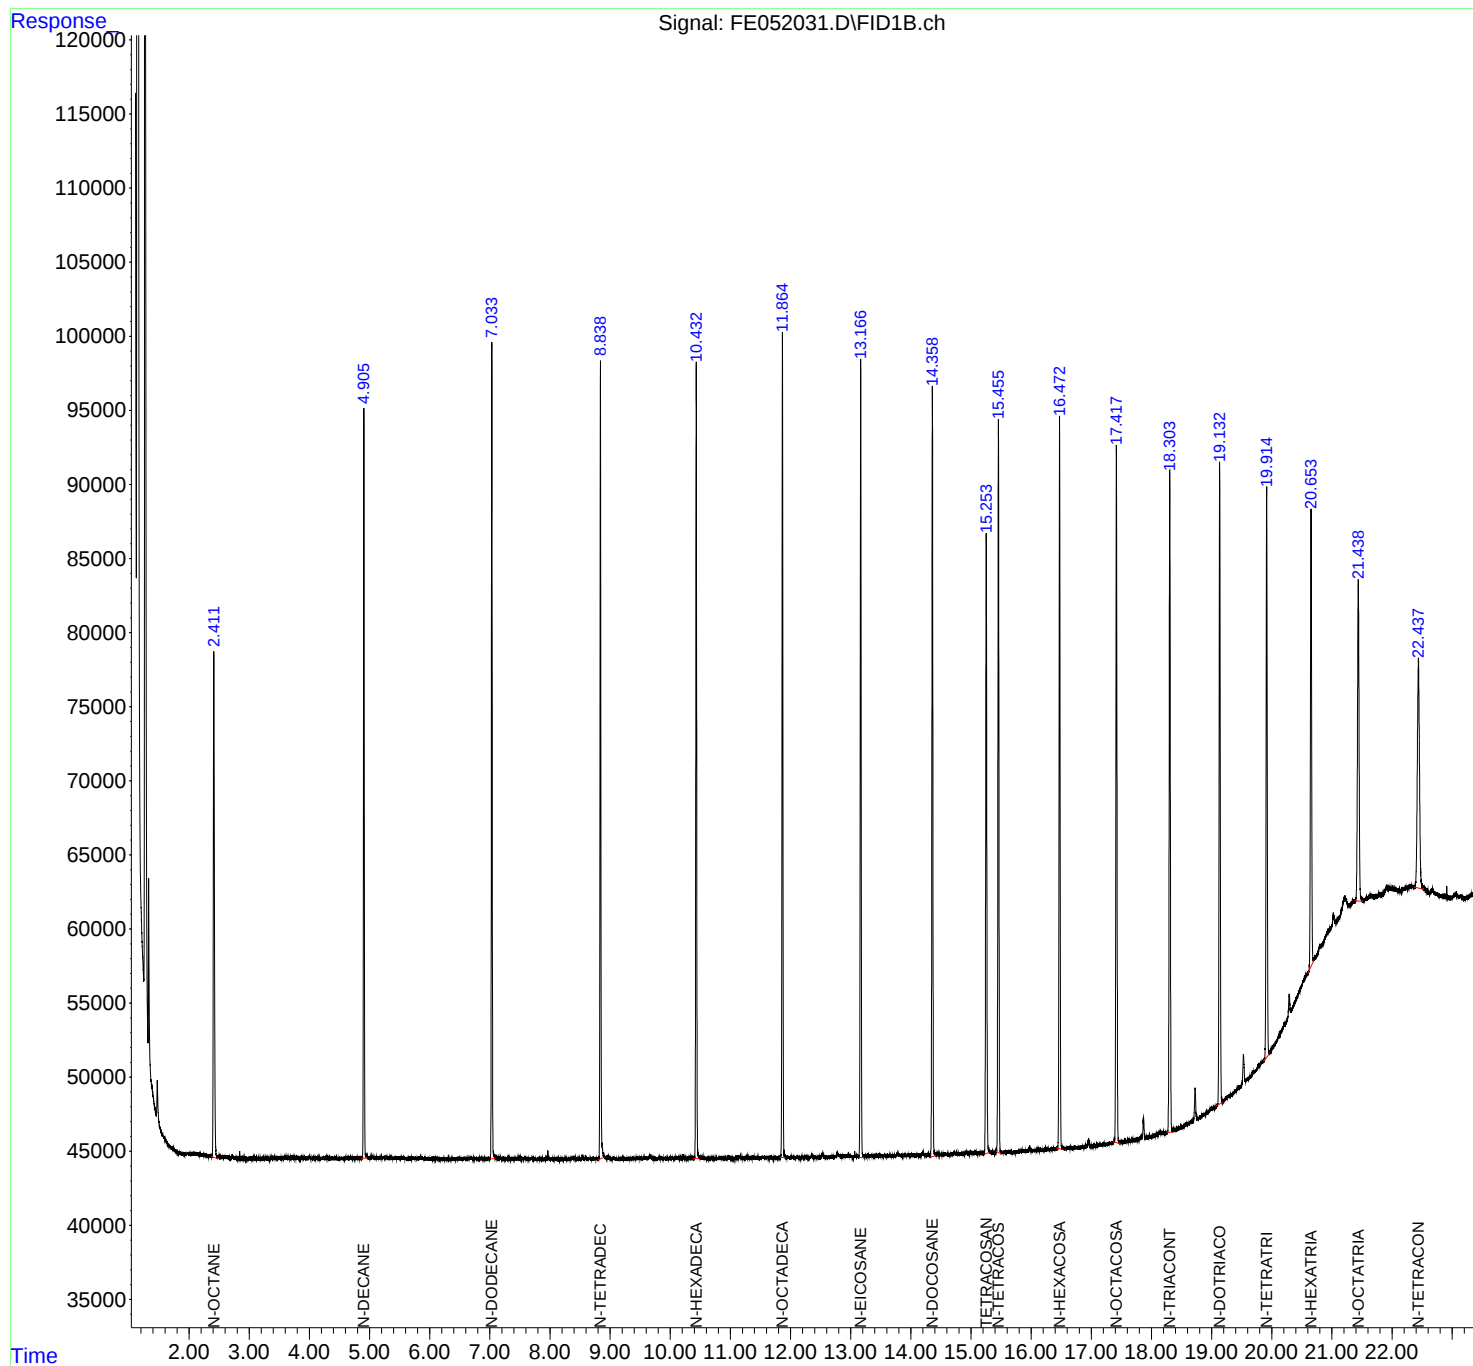


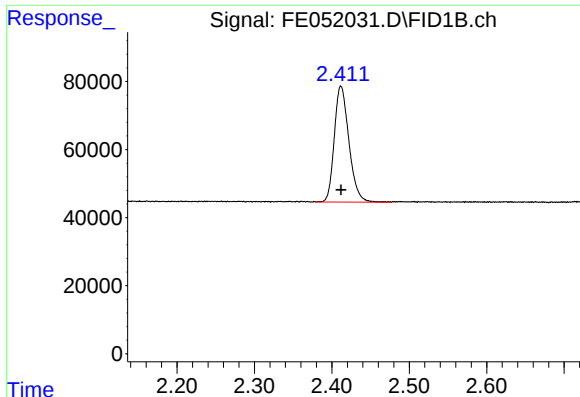

#1 N-OCTANE


R.T.: 2.412 min
Delta R.T.: 0.000 min
Response: 447517
Conc: 5.54 ug/ml

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

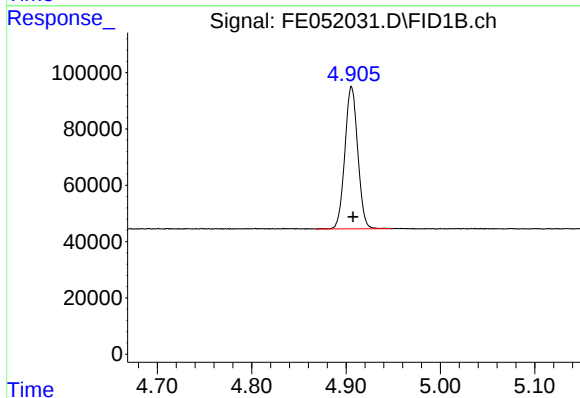


#2 N-DECANE

R.T.: 4.906 min
Delta R.T.: -0.001 min
Response: 479458
Conc: 5.54 ug/ml

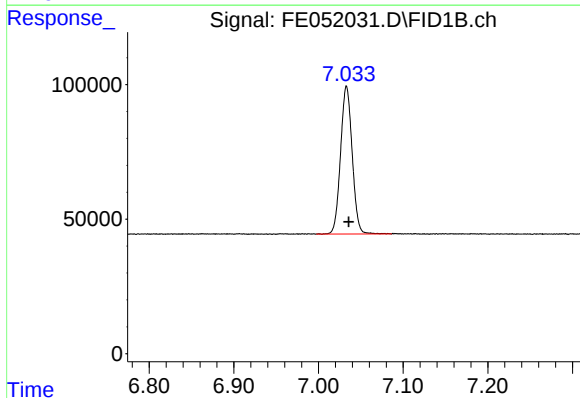


#3 N-DODECANE

R.T.: 7.033 min
Delta R.T.: -0.003 min
Response: 524622
Conc: 5.57 ug/ml

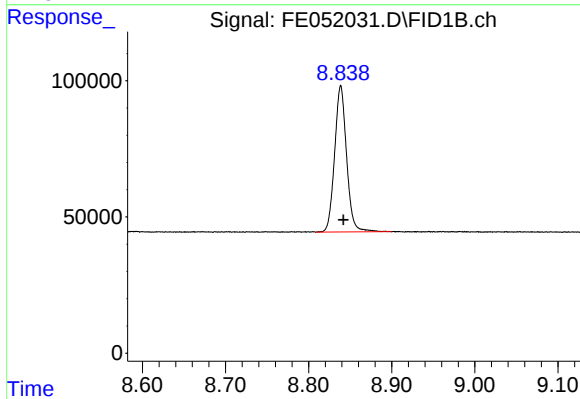

#4 N-TETRADECANE


R.T.: 8.839 min
Delta R.T.: -0.003 min
Response: 538294
Conc: 5.64 ug/ml

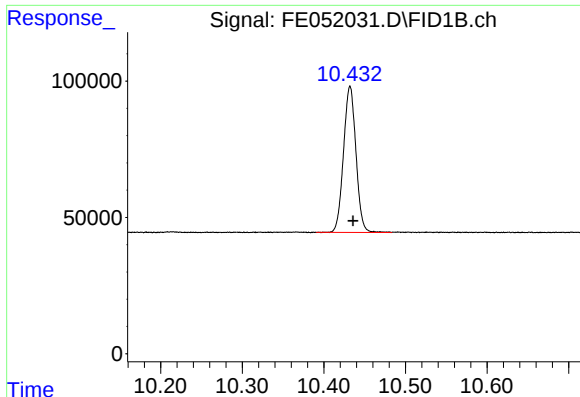

#5 N-HEXADECANE


R.T.: 10.432 min
Delta R.T.: -0.003 min
Response: 566935
Conc: 5.68 ug/ml

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

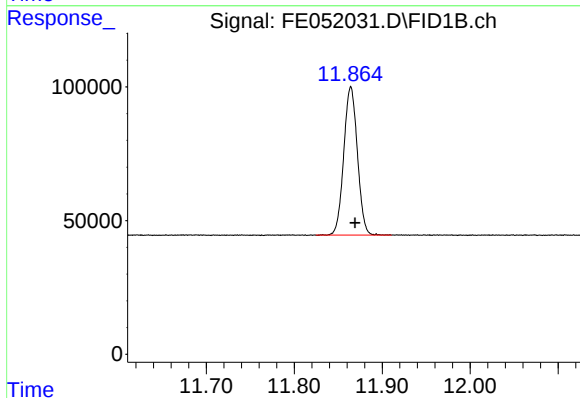


#6 N-OCTADECANE

R.T.: 11.864 min
Delta R.T.: -0.005 min
Response: 597723
Conc: 5.70 ug/ml

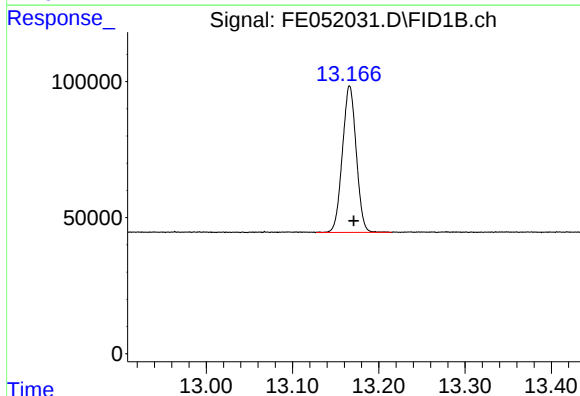


#7 N-EICOSANE

R.T.: 13.166 min
Delta R.T.: -0.005 min
Response: 599565
Conc: 5.77 ug/ml

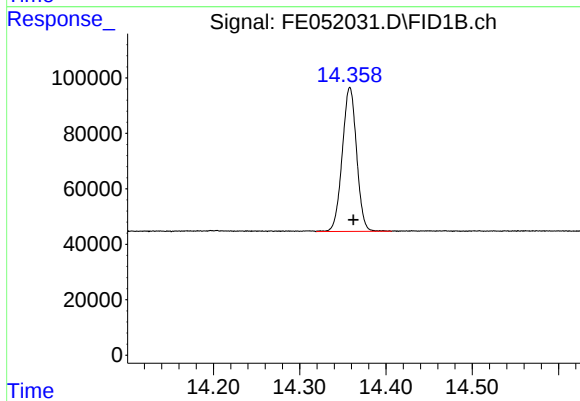

#8 N-DOCOSANE


R.T.: 14.358 min
Delta R.T.: -0.004 min
Response: 599958
Conc: 5.80 ug/ml

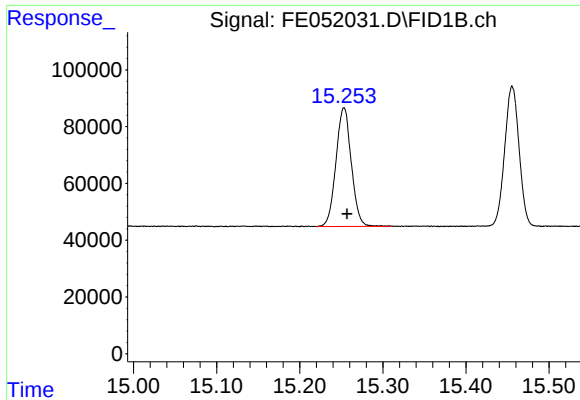

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.253 min
Delta R.T.: -0.004 min
Response: 535796
Conc: 5.75 ug/ml

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

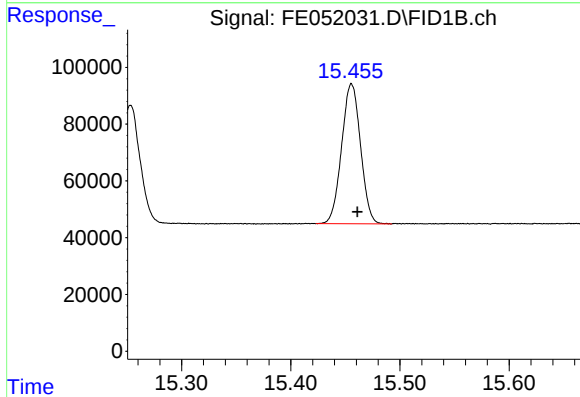


#10 N-TETRACOSANE

R.T.: 15.456 min
Delta R.T.: -0.005 min
Response: 594003
Conc: 5.75 ug/ml

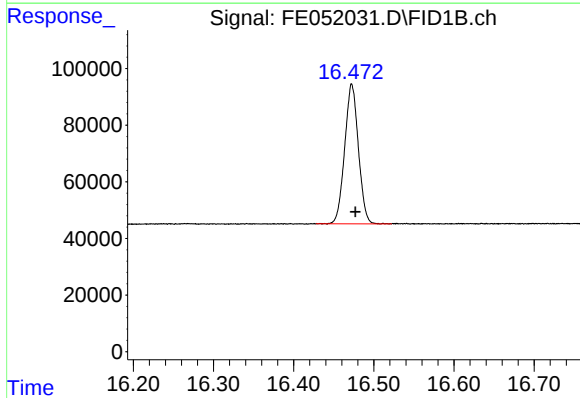


#11 N-HEXACOSANE

R.T.: 16.473 min
Delta R.T.: -0.004 min
Response: 585191
Conc: 5.75 ug/ml

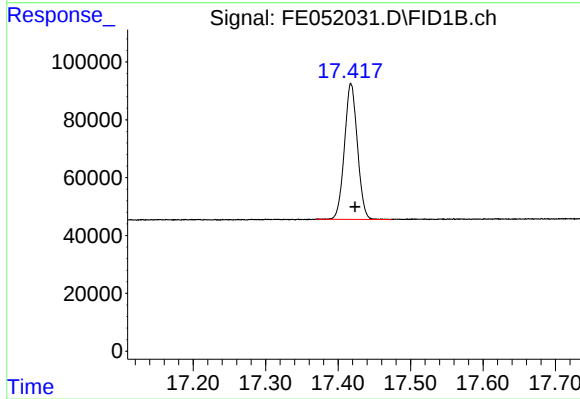

#12 N-OCTACOSANE


R.T.: 17.418 min
Delta R.T.: -0.006 min
Response: 583549
Conc: 5.79 ug/ml

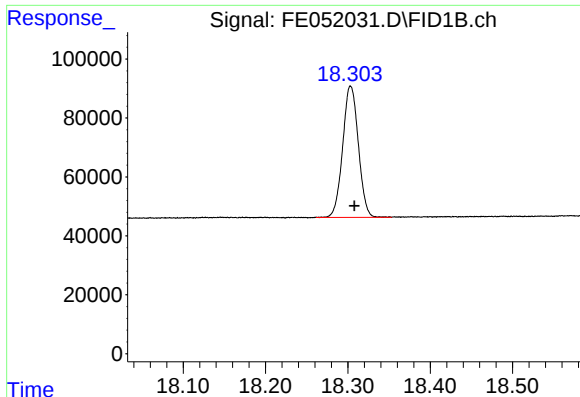

#13 N-TRIACONTANE


R.T.: 18.303 min
Delta R.T.: -0.005 min
Response: 588228
Conc: 5.91 ug/ml

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

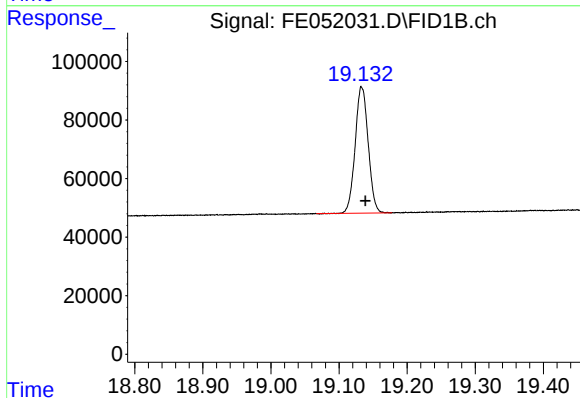


#14 N-DOTRIACONTANE

R.T.: 19.133 min
Delta R.T.: -0.006 min
Response: 573000
Conc: 5.93 ug/ml

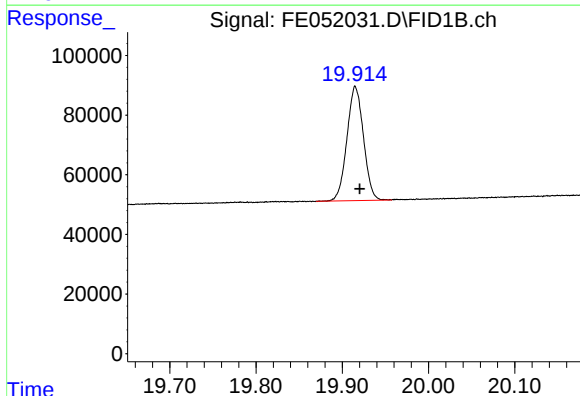


#15 N-TETRATRIACONTANE

R.T.: 19.915 min
Delta R.T.: -0.005 min
Response: 509659
Conc: 5.87 ug/ml

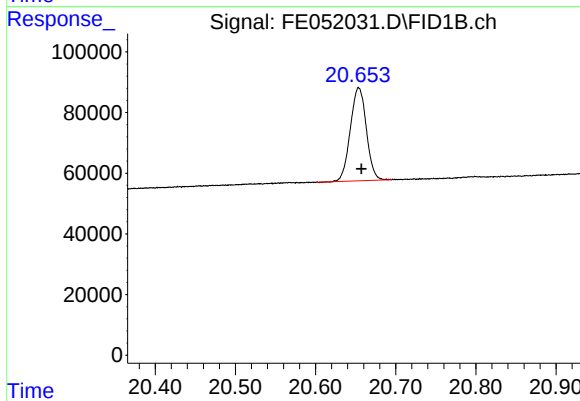

#16 N-HEXATRIACONTANE


R.T.: 20.654 min
Delta R.T.: -0.004 min
Response: 427588
Conc: 5.74 ug/ml

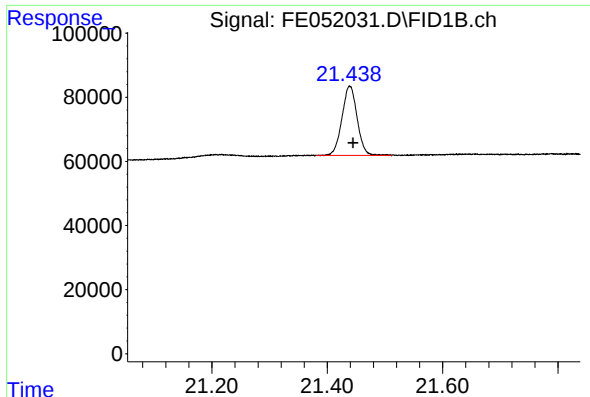

#17 N-OCTATRIACONTANE

R.T.: 21.439 min
Delta R.T.: -0.006 min
Response: 394101
Conc: 5.72 ug/ml

Instrument :
FID_E
ClientSampleId :
5 TRPH STD

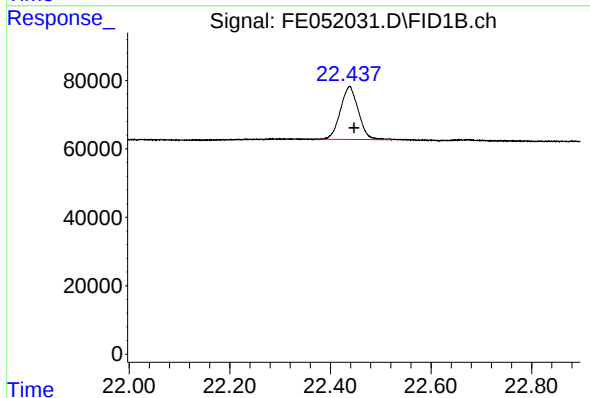

#18 N-TETRACONTANE

R.T.: 22.438 min
Delta R.T.: -0.009 min
Response: 382667
Conc: 5.69 ug/ml