


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141335.D
Acq On : 31 Jan 2025 16:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

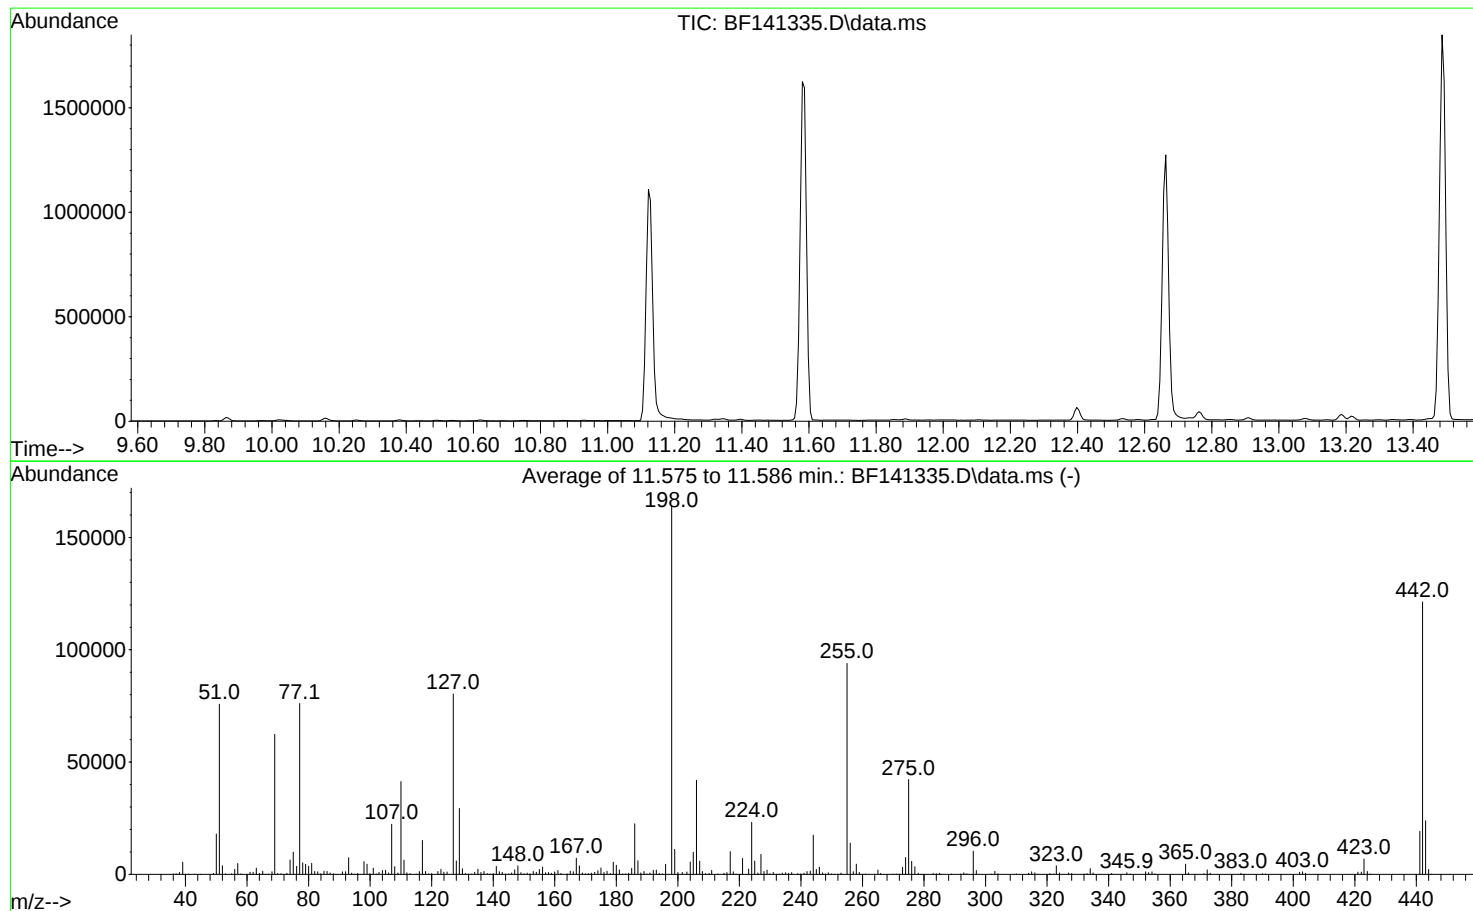

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	75704	PASS
68	69	0.00	2	1.9	1195	PASS
69	198	0.00	100	38.1	62342	PASS
70	69	0.00	2	0.7	436	PASS
127	198	10	80	49.0	80267	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	163789	PASS
199	198	5	9	6.8	11100	PASS
275	198	10	60	25.8	42219	PASS
365	198	1	100	2.8	4575	PASS
441	198	0.01	100	11.7	19173	PASS
442	442	50	100	100.0	121349	PASS
443	442	15	24	19.7	23847	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/31/2025	BNA_F	<u>BF141335.D</u>
Compound Name	Response	Retention Time
DDT	464959	13.486
DDD	12206	13.186
DDE	750	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12956	477915	2.71

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141335.D
Acq On : 31 Jan 2025 16:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 17:41:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

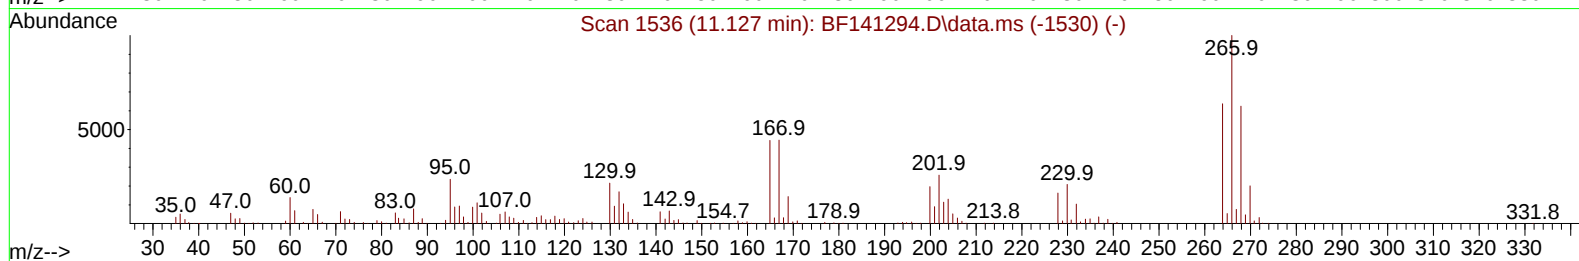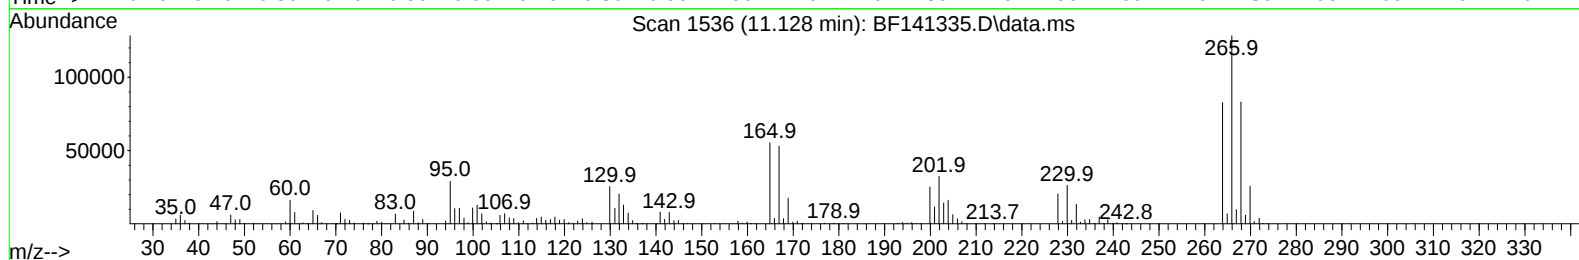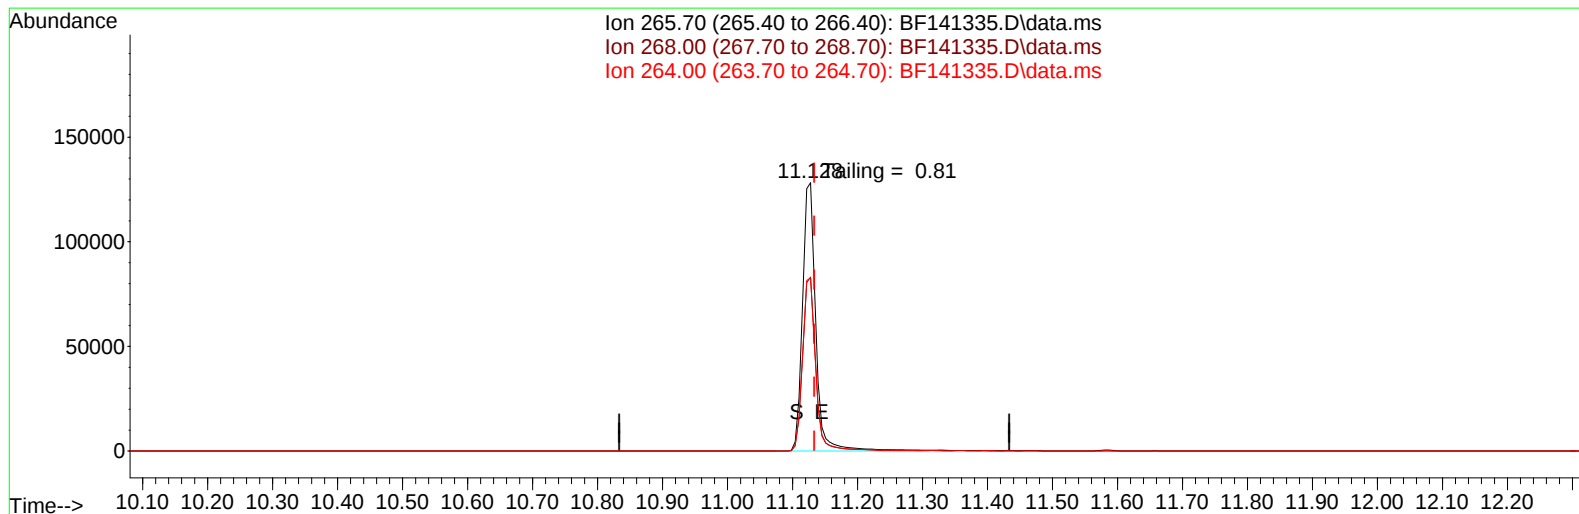

TIC: BF141335.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.006) 9273.56 ng




response 183922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.82
264.00	63.70	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141335.D
Acq On : 31 Jan 2025 16:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 17:41:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

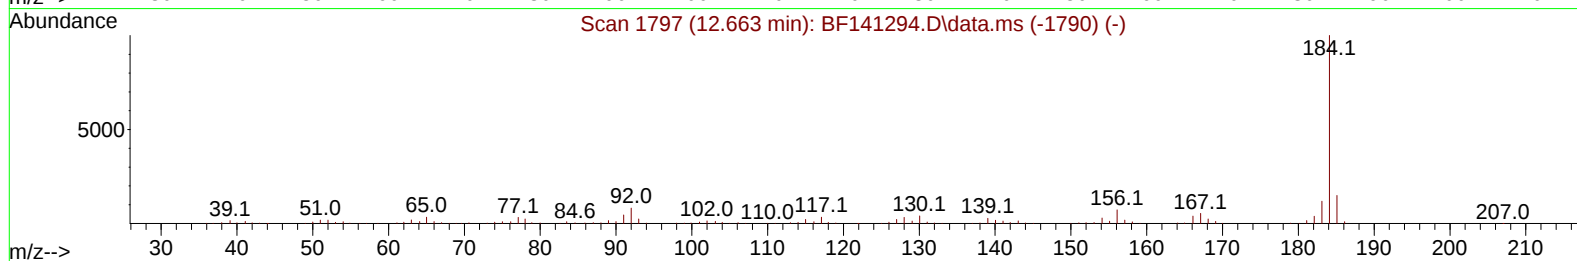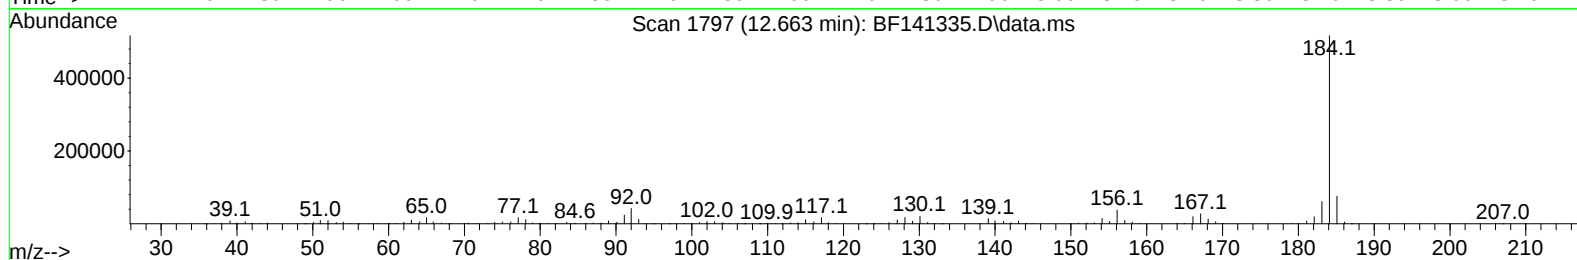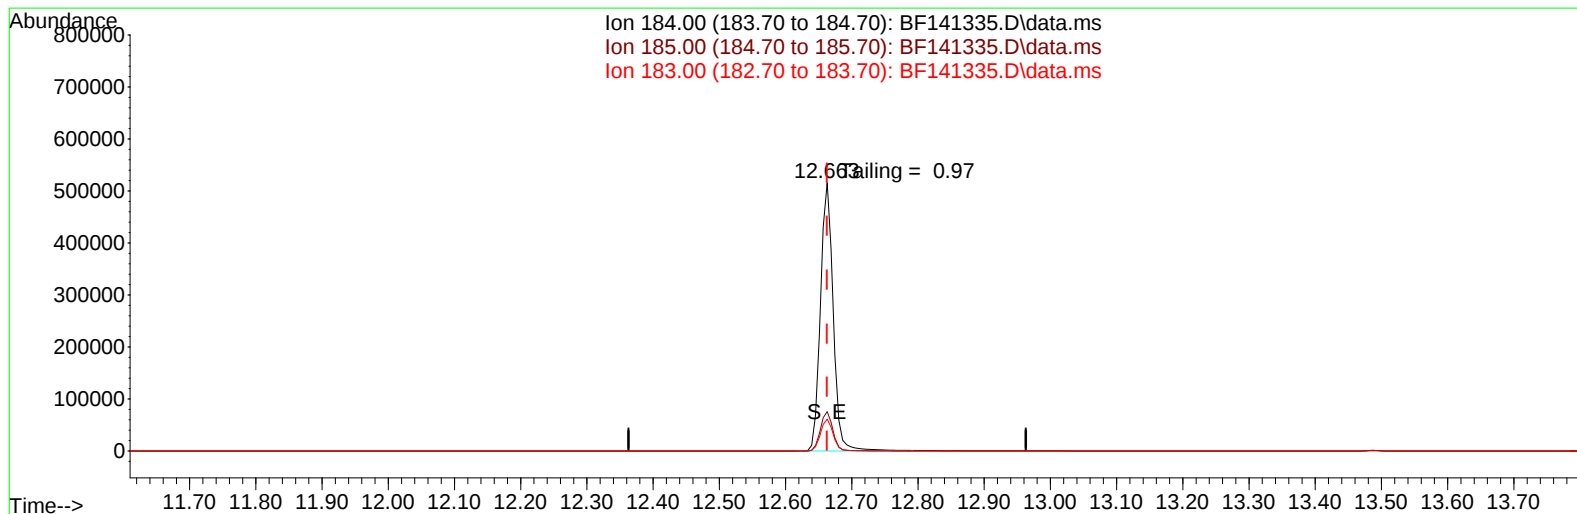

TIC: BF141335.D\data.ms

(77) Benzidine

12.663min (-0.000) 12340.55 ng

response 693915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.67
183.00	11.90	11.87
0.00	0.00	0.00