

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052174.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 13:38
Operator : YP\AJ
Sample : Q1241-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-5.3-013025

Integration File: autoint1.e
Quant Time: Feb 03 00:09:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.286	1842824	18.503 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052174.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 13:38
Operator : YP\AJ
Sample : Q1241-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-5.3-013025

Integration File: autoint1.e
Quant Time: Feb 03 00:09:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

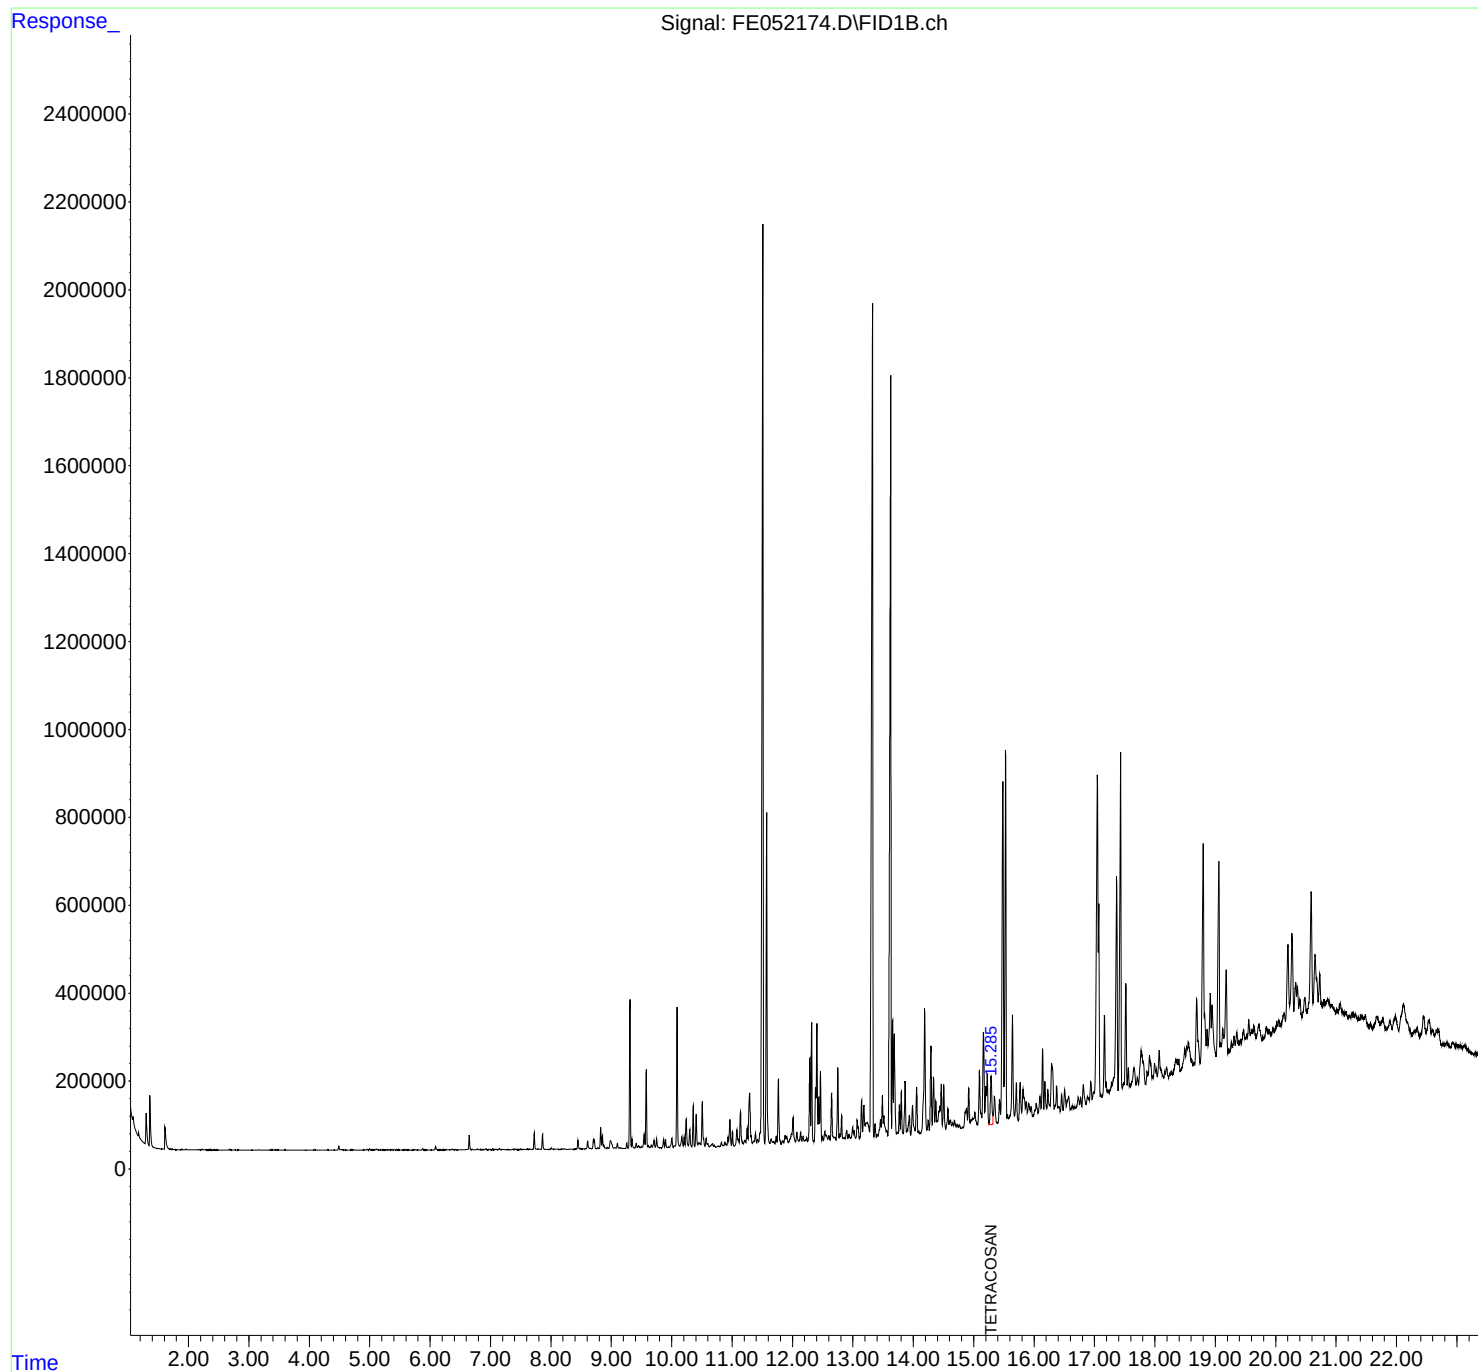

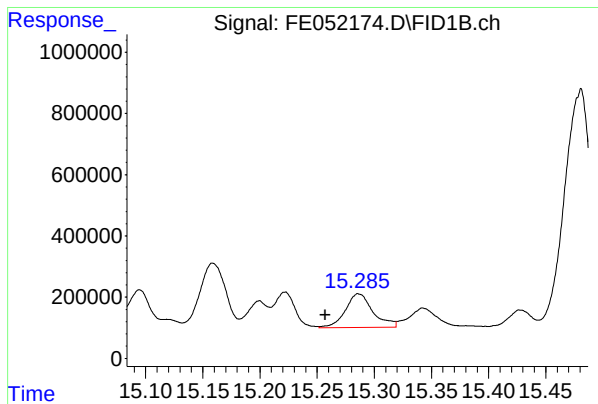

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.286 min
Delta R.T.: 0.029 min
Response: 1842824
Conc: 18.50 ug/ml

Instrument :
FID_E
ClientSampleId :
JPP-5.3-013025