

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052183.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 18:11
Operator : YP\AJ
Sample : Q1241-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-3.5-013025

Integration File: autoint1.e
Quant Time: Feb 03 00:12:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.234	262321	2.634 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052183.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 18:11
Operator : YP\AJ
Sample : Q1241-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-3.5-013025

Integration File: autoint1.e
Quant Time: Feb 03 00:12:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

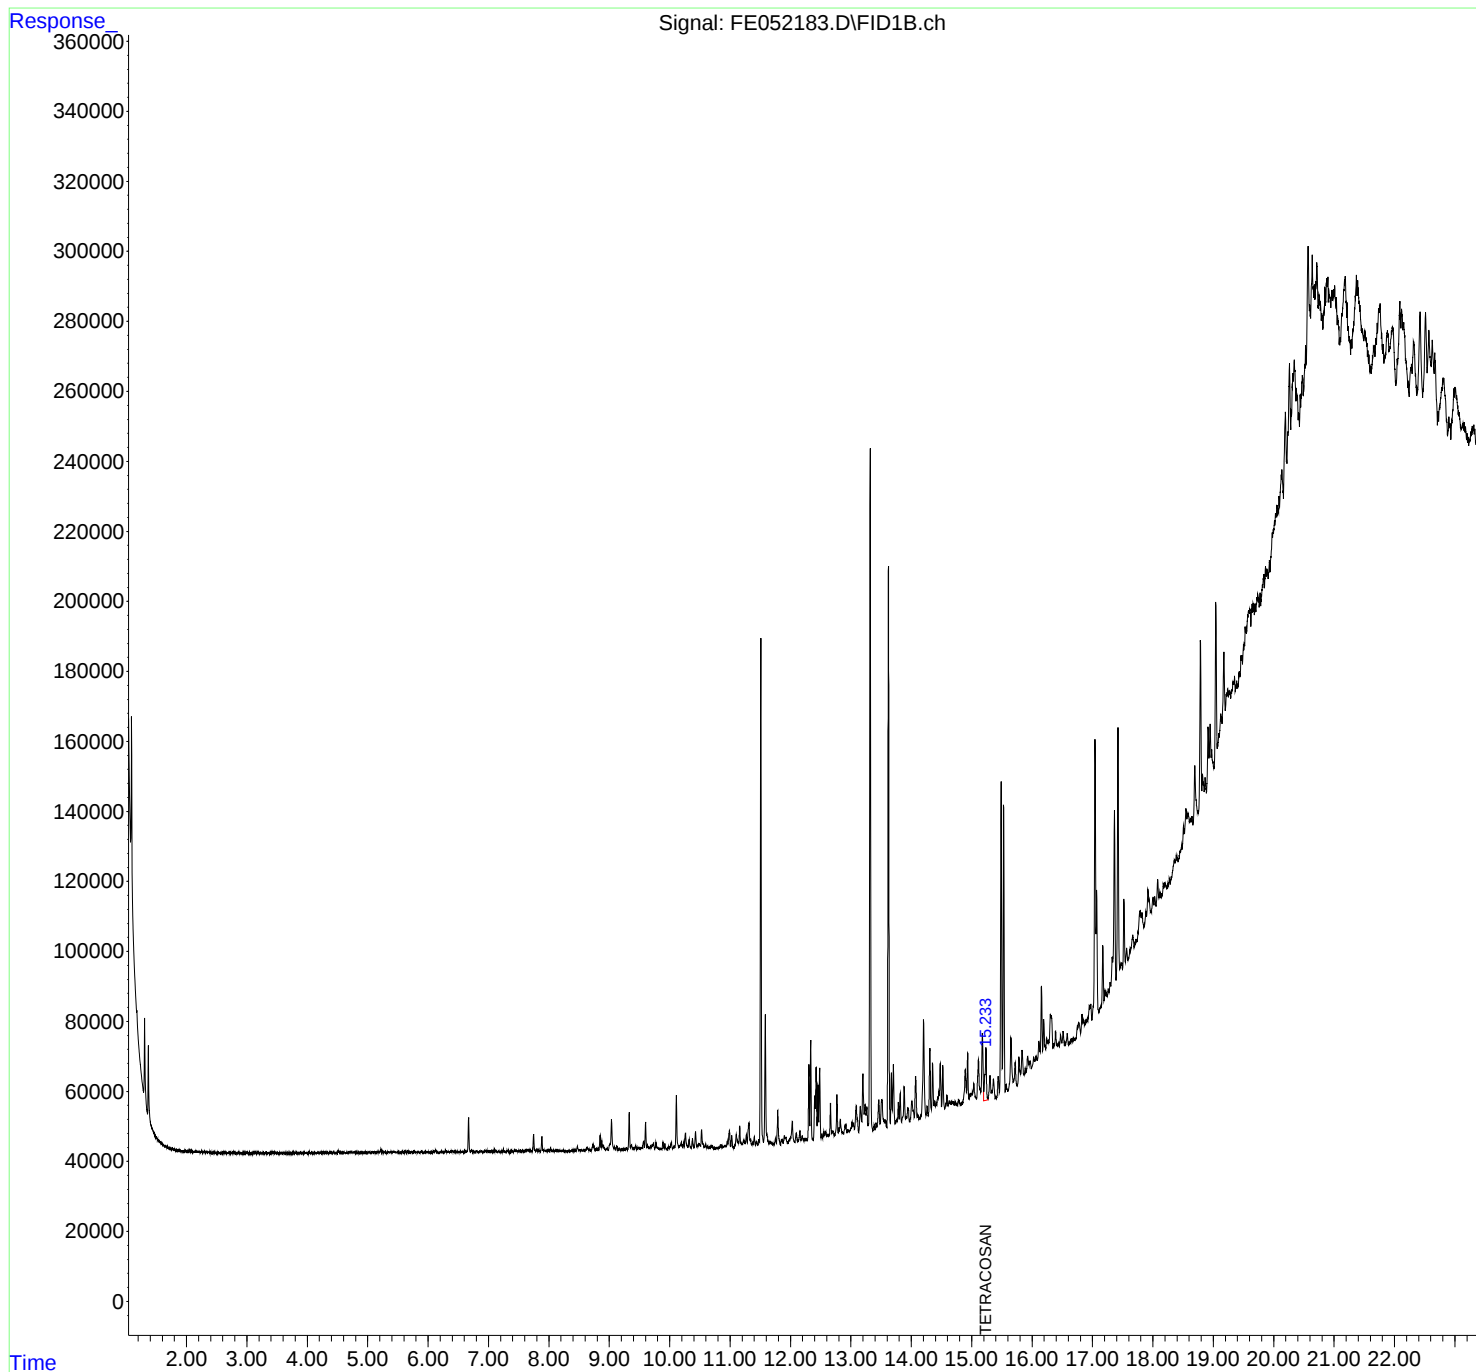

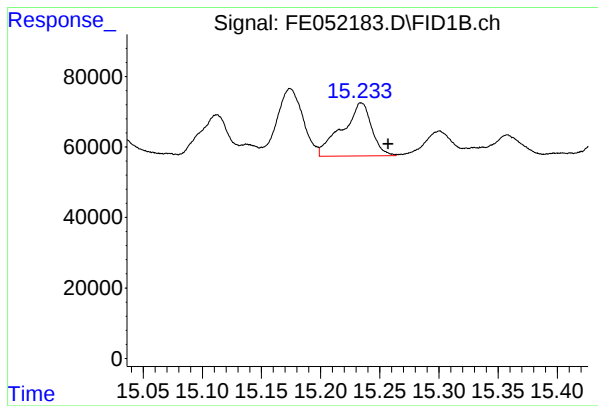

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.234 min
Delta R.T.: -0.023 min
Response: 262321
Conc: 2.63 ug/ml

Instrument :
FID_E
ClientSampleId :
JPP-3.5-013025