

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020425\
 Data File : P0109416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 11:54
 Operator : YP/AJ
 Sample : Q1241-03RE
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JPP-3.5-013025RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/05/2025
 Supervised By :Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:46:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 04 08:55:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.695	139.7E6	86935631	18.438m	16.278
2) SA Decachlor...	8.756	8.708	163.6E6	84323270	25.247	27.059

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020425\
Data File : PO109416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 11:54
Operator : YP/AJ
Sample : Q1241-03RE
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JPP-3.5-013025RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/05/2025
Supervised By :Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:46:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO020325.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 04 08:55:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

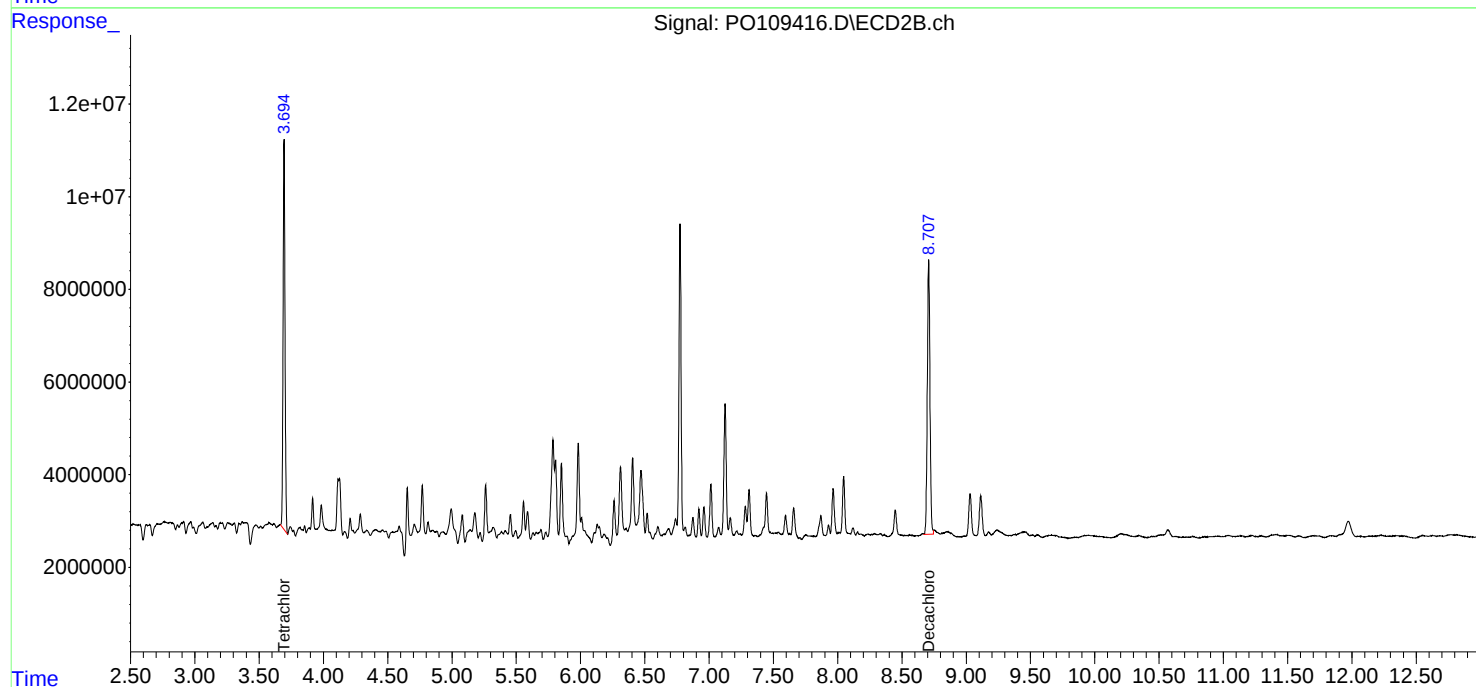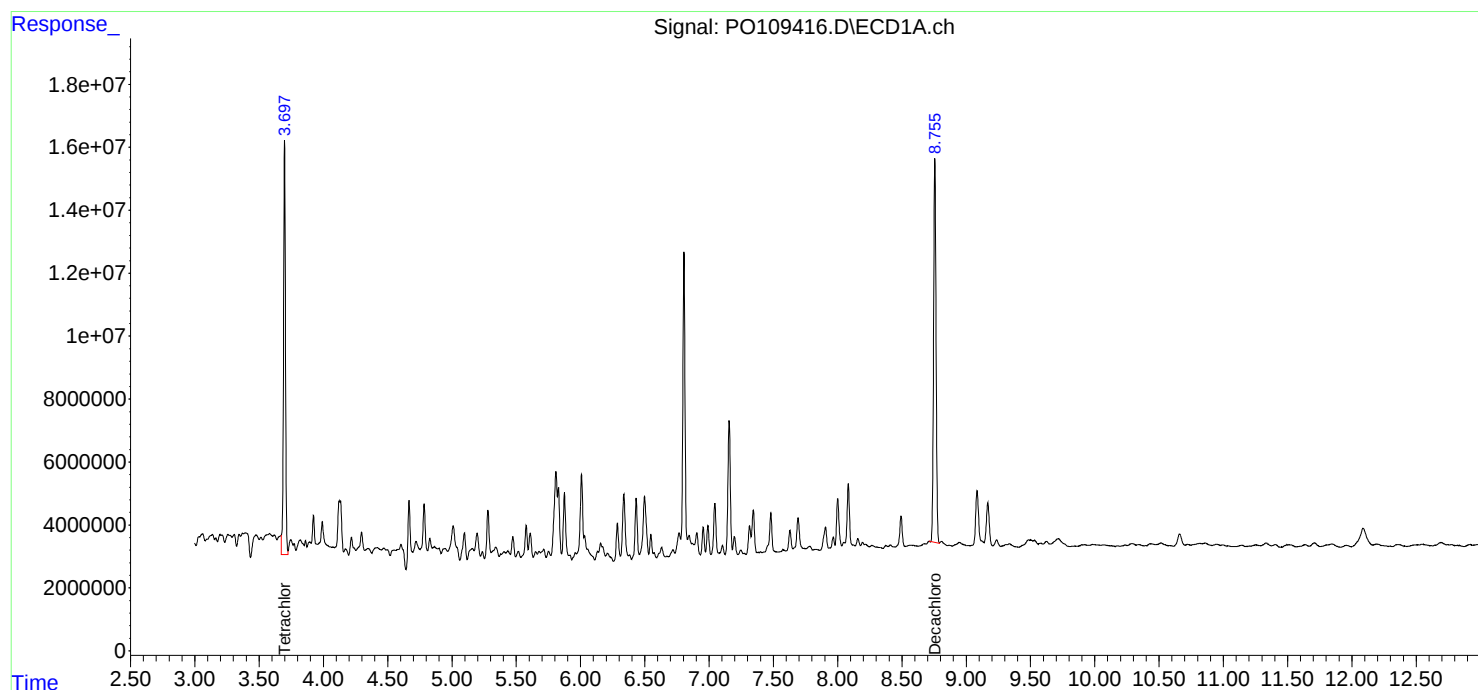

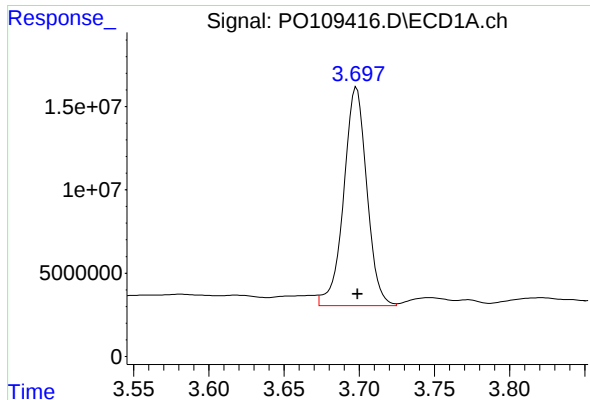


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: -0.002 min
Response: 139741288
Conc: 18.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
JPP-3.5-013025RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/05/2025
Supervised By :Ankita Jodhani 02/05/2025

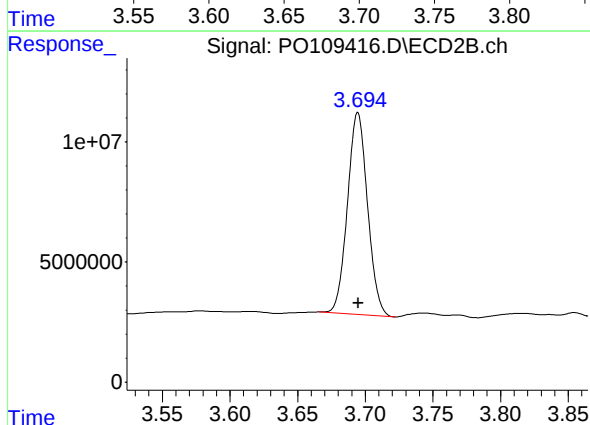


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 86935631
Conc: 16.28 ng/ml

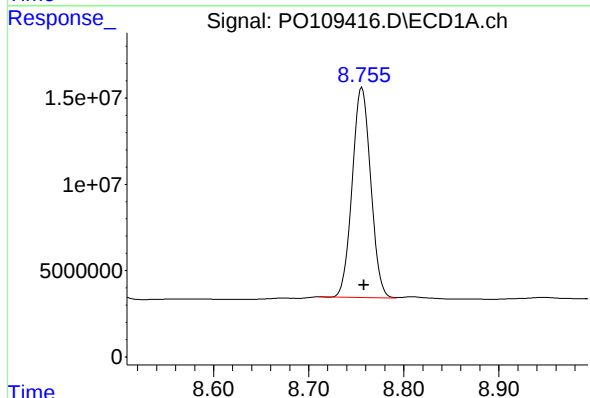

#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: -0.002 min
Response: 163634773
Conc: 25.25 ng/ml

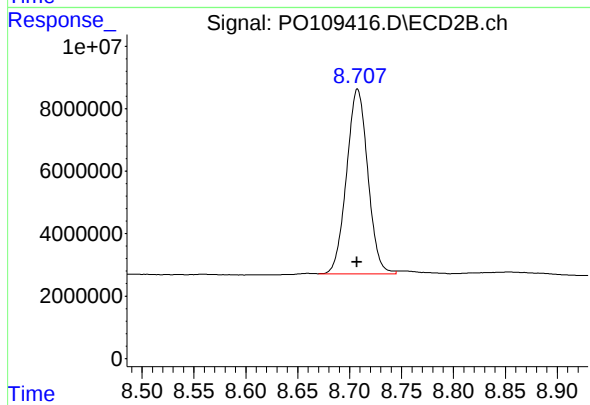

#2 Decachlorobiphenyl

R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 84323270
Conc: 27.06 ng/ml