


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141505.D
Acq On : 07 Feb 2025 14:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

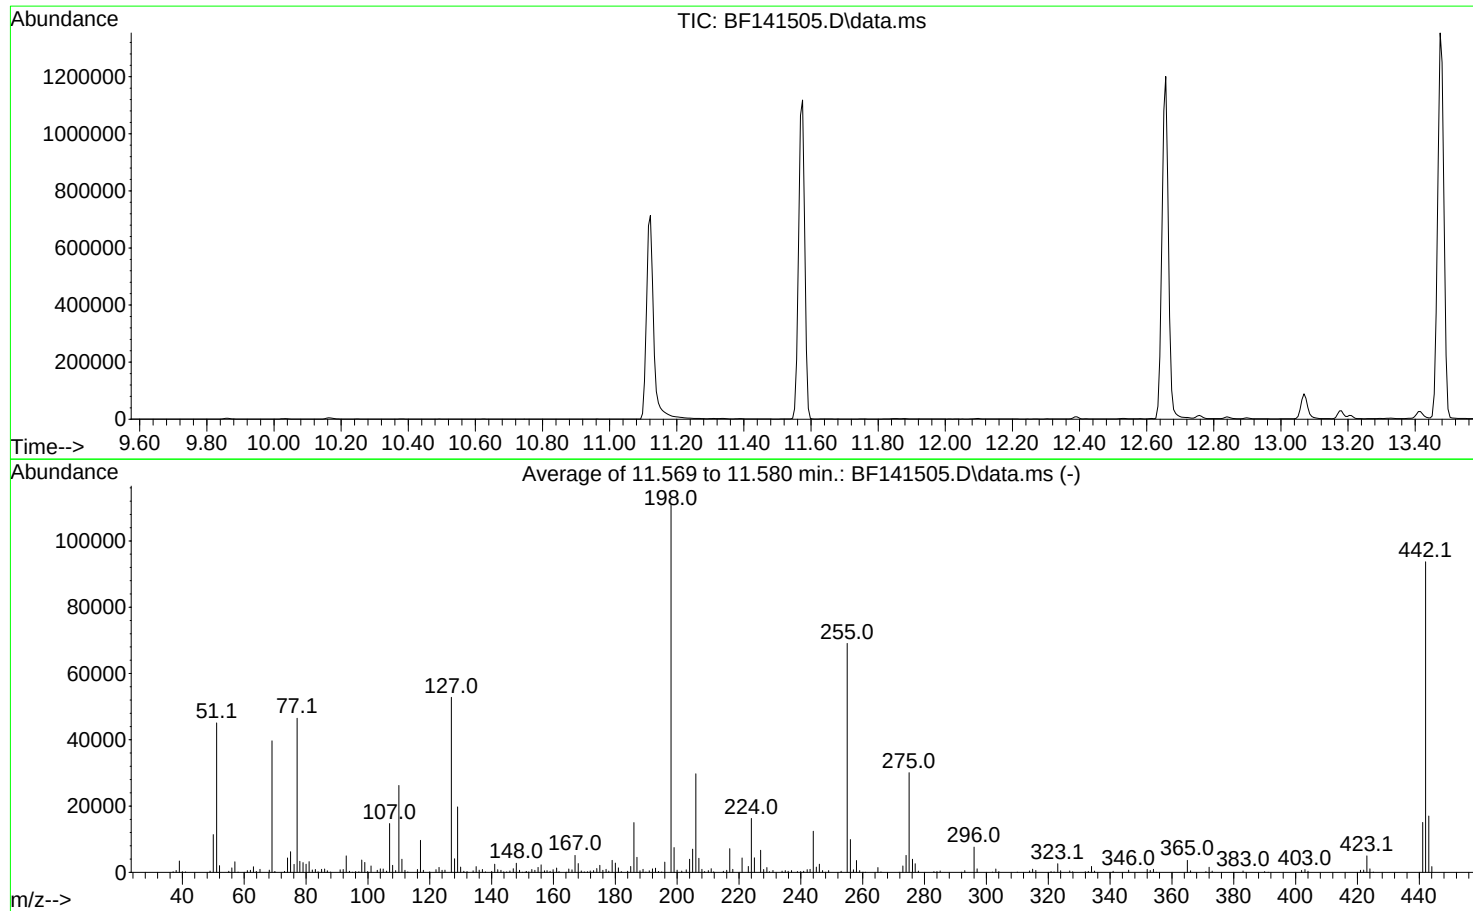

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.6	45085	PASS
68	69	0.00	2	1.7	677	PASS
69	198	0.00	100	35.7	39669	PASS
70	69	0.00	2	0.7	272	PASS
127	198	10	80	47.6	52811	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110989	PASS
199	198	5	9	6.7	7473	PASS
275	198	10	60	27.1	30101	PASS
365	198	1	100	3.3	3633	PASS
441	198	0.01	100	13.6	15067	PASS
442	442	50	100	100.0	93723	PASS
443	442	15	24	18.1	16972	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/7/2025	BNA_F	<u>BF141505.D</u>
Compound Name	Response	Retention Time
DDT	346517	13.474
DDD	12084	13.18
DDE	2082	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14166	360683	3.93

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141505.D
Acq On : 07 Feb 2025 14:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 14:31:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

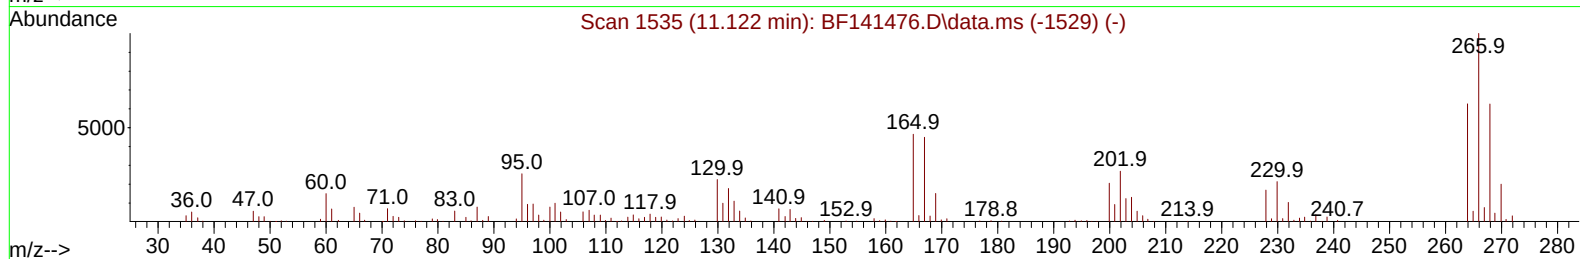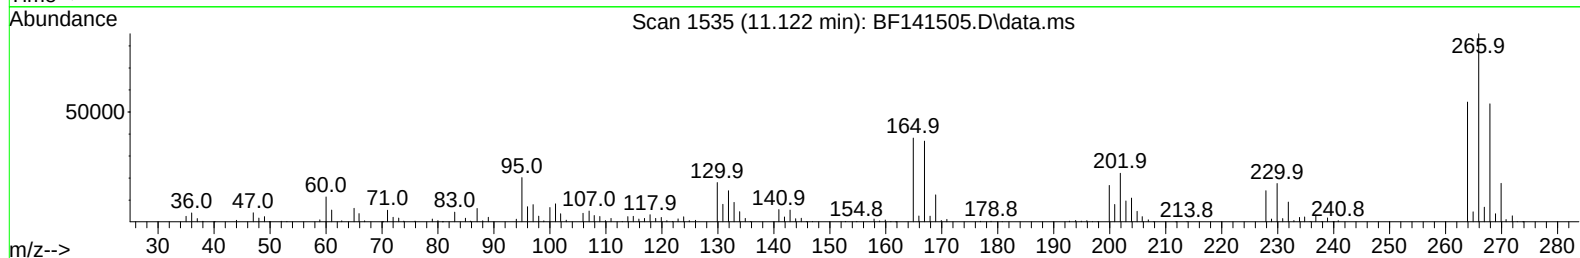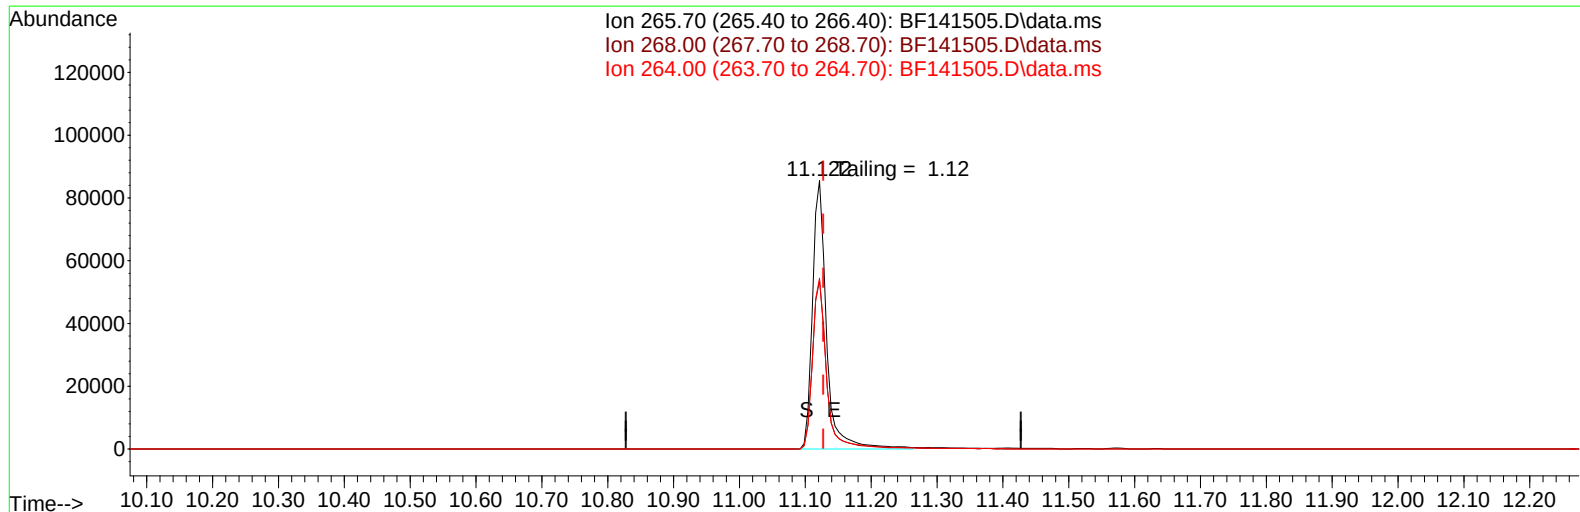

TIC: BF141505.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.006) 20208.15 ng




response 127294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.80
264.00	62.60	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020725\
Data File : BF141505.D
Acq On : 07 Feb 2025 14:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 07 14:31:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

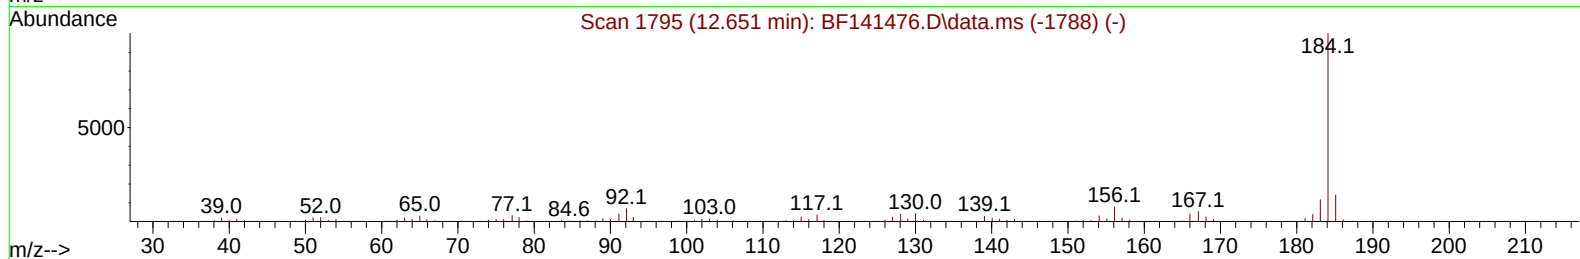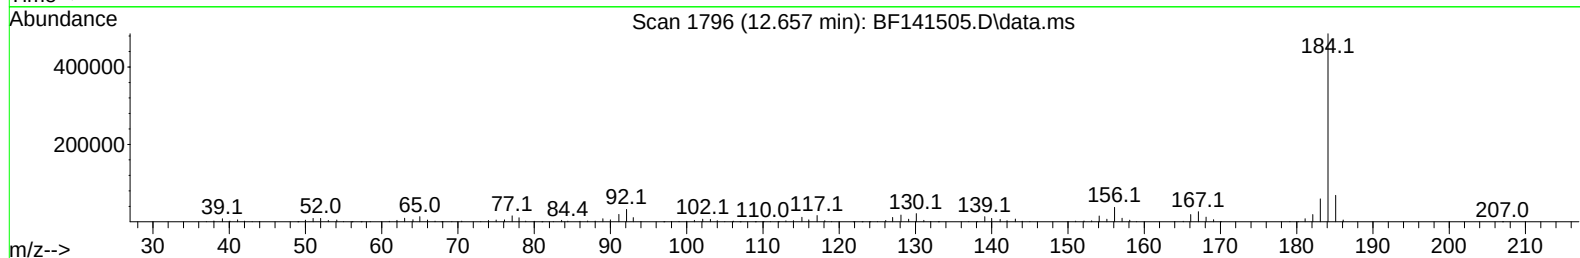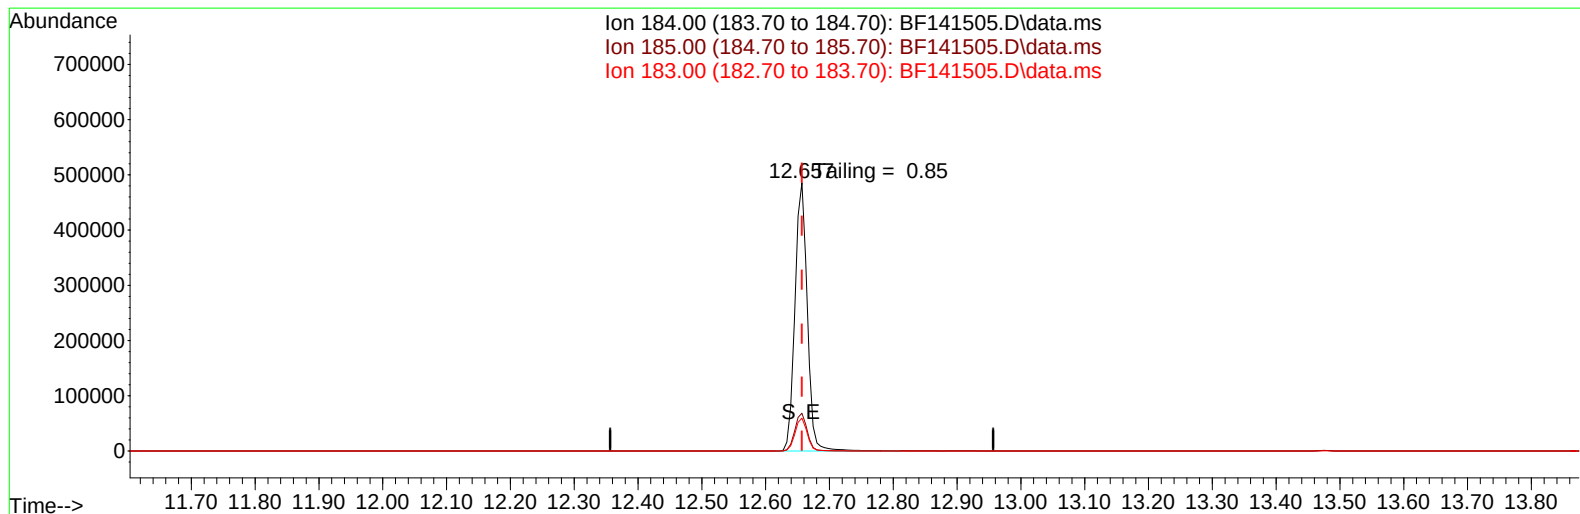

TIC: BF141505.D\data.ms

(77) Benzidine

12.657min (+ 0.000) 44608.91 ng

response 656208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.60	12.23
0.00	0.00	0.00