


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020425\  
Data File : BF141397.D  
Acq On : 04 Feb 2025 10:16  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012925.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Jan 29 17:41:25 2025

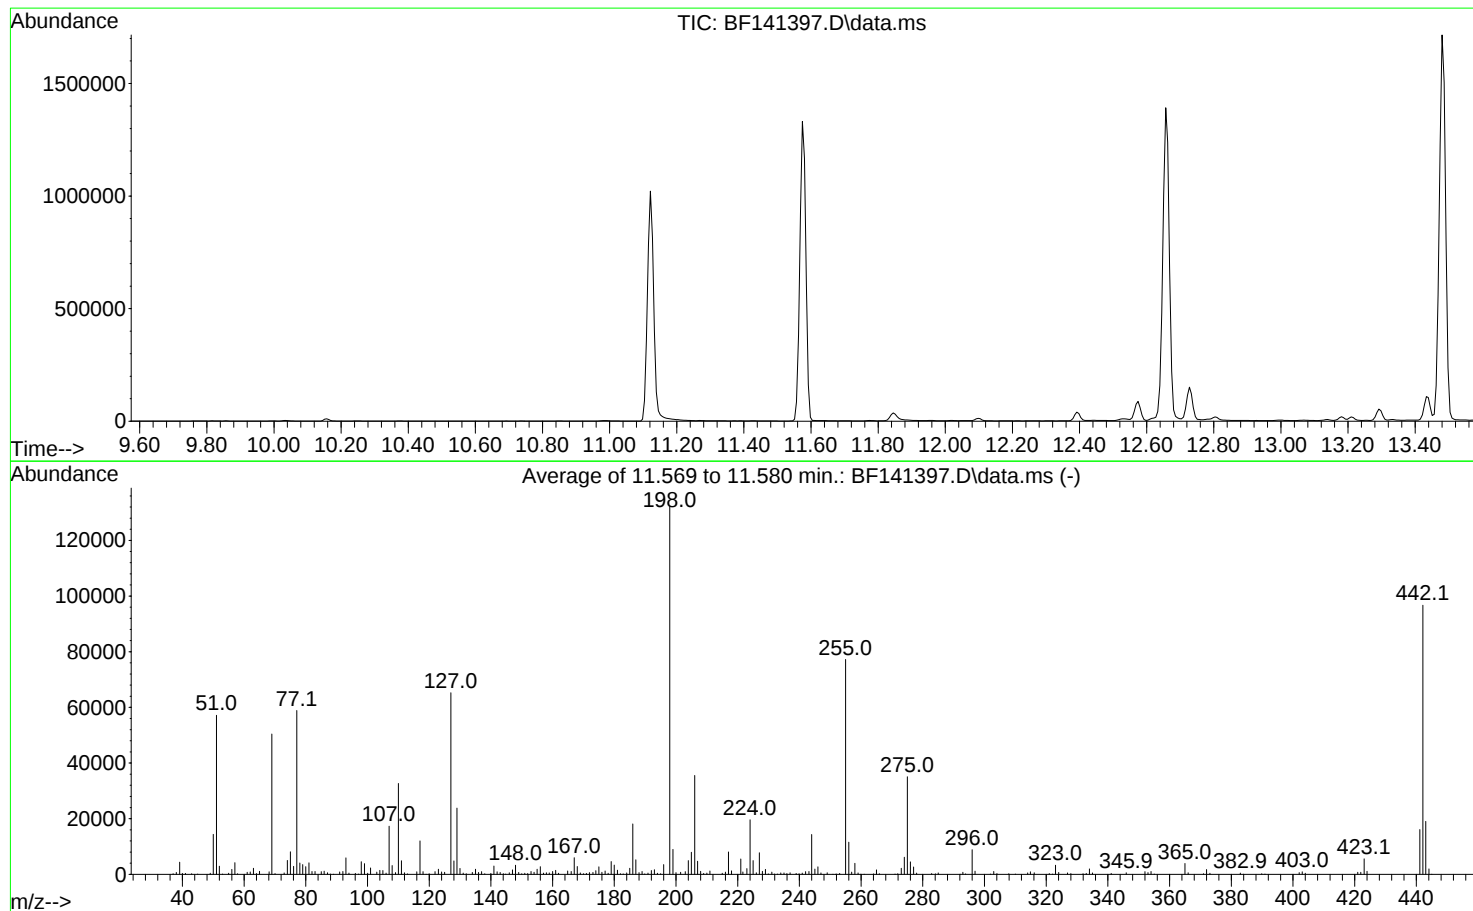

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 43.3         | 57171      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 947        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.1         | 50408      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 288        | PASS                |
| 127            | 198             | 10              | 80              | 49.4         | 65259      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 132187     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 8986       | PASS                |
| 275            | 198             | 10              | 60              | 26.5         | 35069      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 3931       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.2         | 16076      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 96717      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 19012      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/4/2025      | BNA_F            | <u>BF141397.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 430190           | 13.48              |
| DDD           | 8939             | 13.18              |
| DDE           | 241              | 12.845             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9180          | 439370           | 2.09               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020425\  
Data File : BF141397.D  
Acq On : 04 Feb 2025 10:16  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 04 11:33:07 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 29 17:41:25 2025  
Response via : Initial Calibration

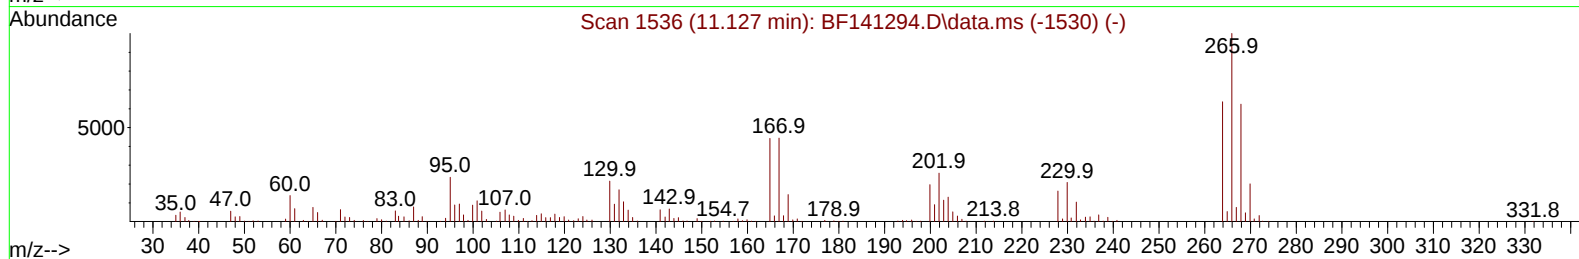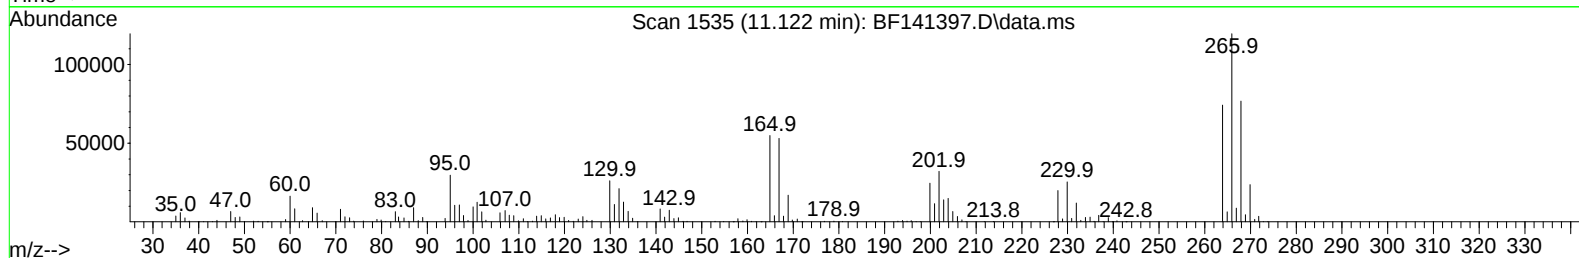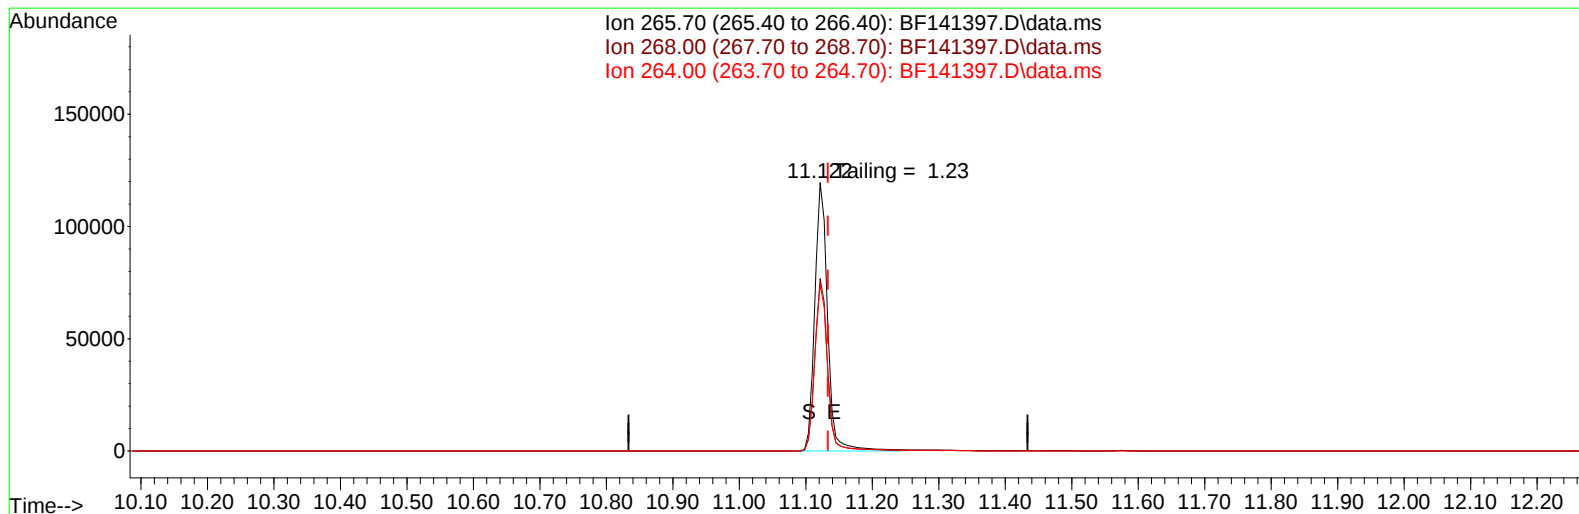

TIC: BF141397.D\data.ms

**(70) Pentachlorophenol (C)**

**11.122min (-0.012) 45312.00 ng**




**response 160702**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 64.23  |
| 264.00 | 63.70  | 62.09  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020425\  
Data File : BF141397.D  
Acq On : 04 Feb 2025 10:16  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 04 11:33:07 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 29 17:41:25 2025  
Response via : Initial Calibration

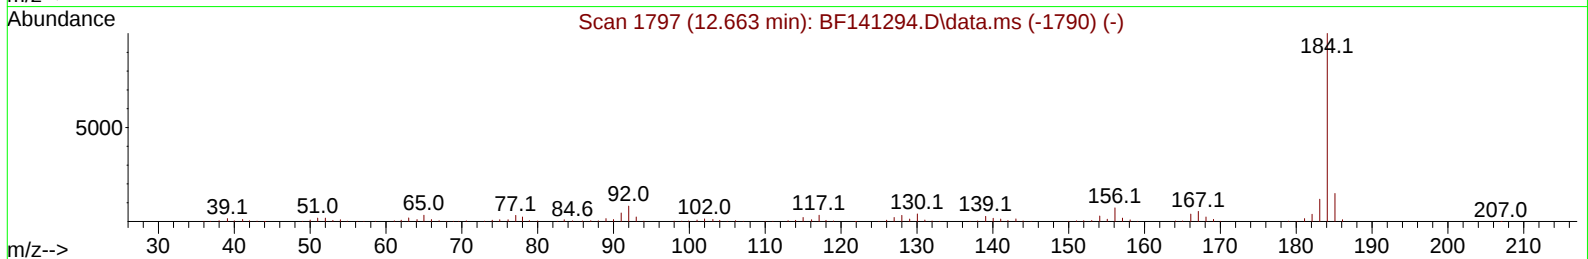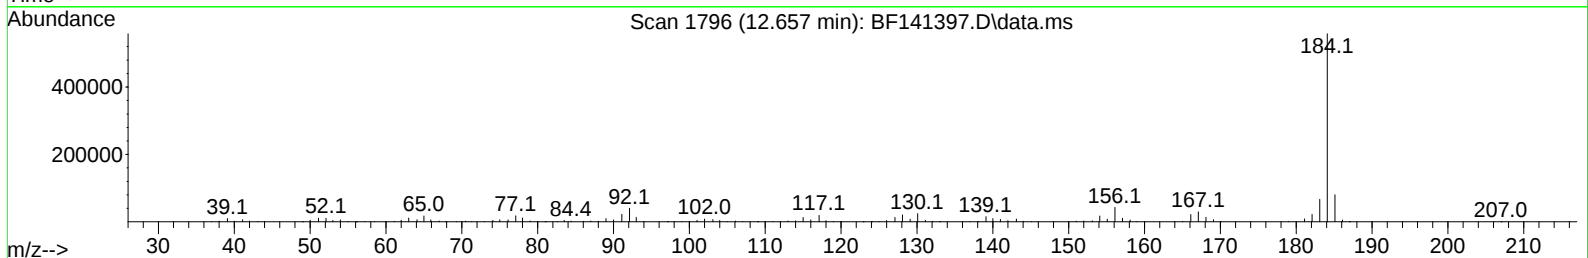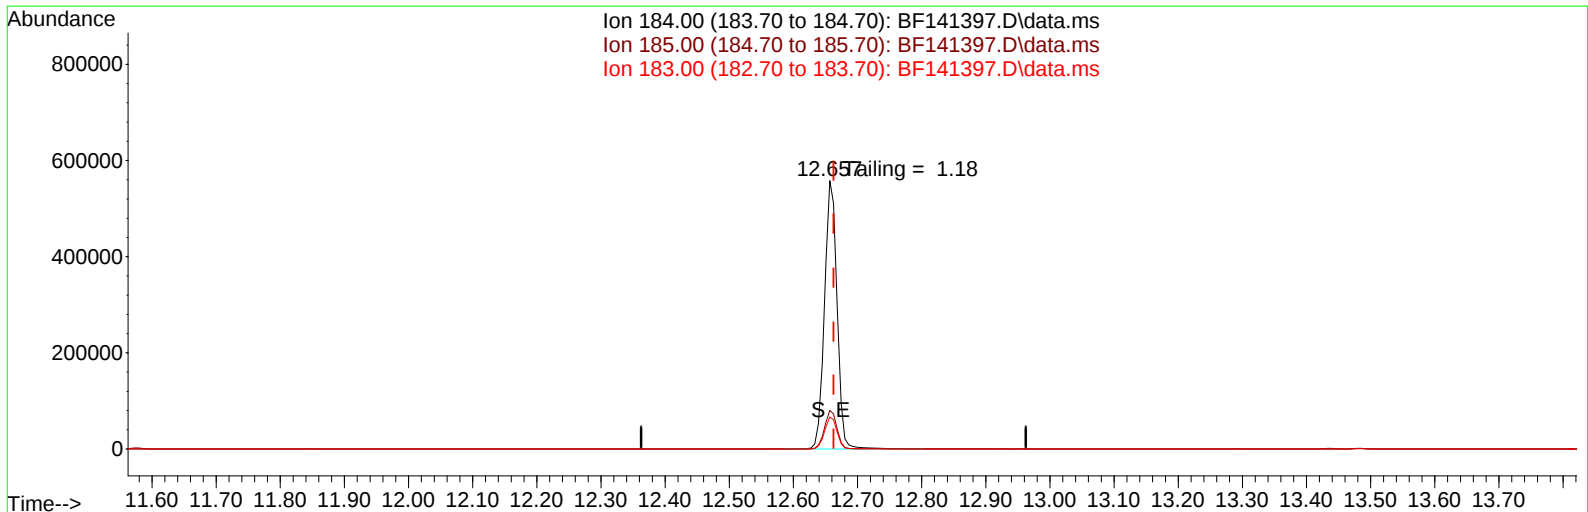

TIC: BF141397.D\data.ms

(77) Benzidine

12.657min (-0.006) 113140.91 ng

response 761695

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.38  |
| 183.00 | 11.90  | 11.93  |
| 0.00   | 0.00   | 0.00   |