


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141409.D
Acq On : 04 Feb 2025 15:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

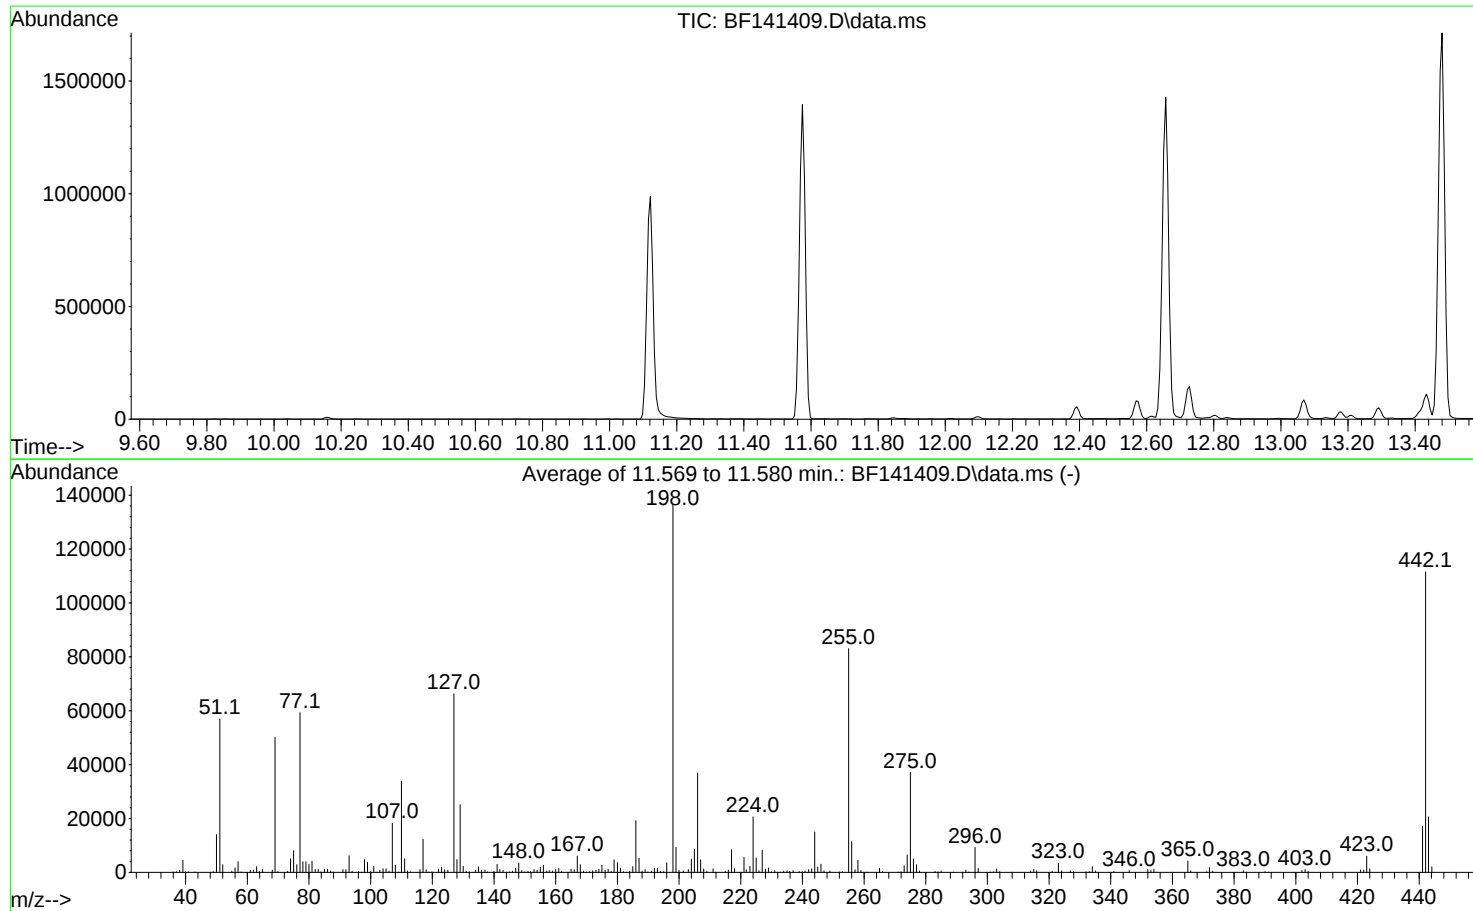

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	56976	PASS
68	69	0.00	2	1.7	844	PASS
69	198	0.00	100	36.7	50160	PASS
70	69	0.00	2	0.6	317	PASS
127	198	10	80	48.6	66312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136541	PASS
199	198	5	9	6.8	9266	PASS
275	198	10	60	27.1	37069	PASS
365	198	1	100	3.1	4251	PASS
441	198	0.01	100	12.5	17108	PASS
442	442	50	100	100.0	111555	PASS
443	442	15	24	18.5	20620	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/4/2025	BNA_F	<u>BF141409.D</u>
Compound Name	Response	Retention Time
DDT	427881	13.48
DDD	13296	13.18
DDE	1486	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14782	442663	3.34

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141409.D
Acq On : 04 Feb 2025 15:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 16:10:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

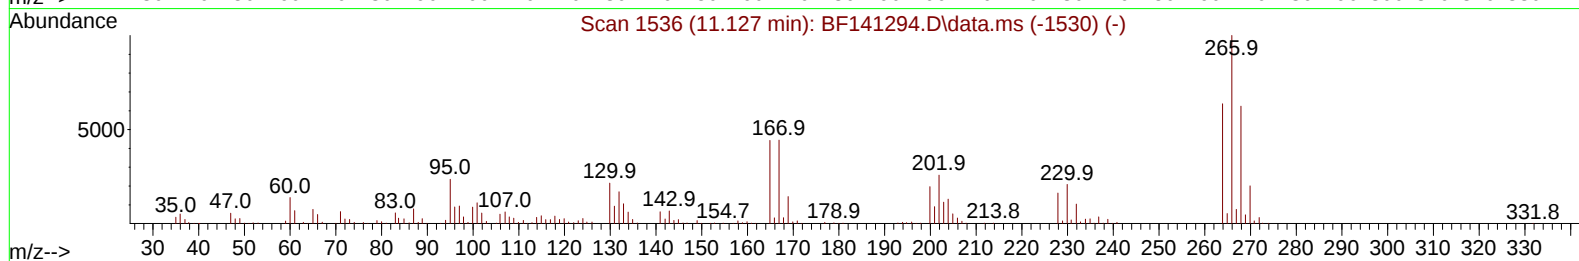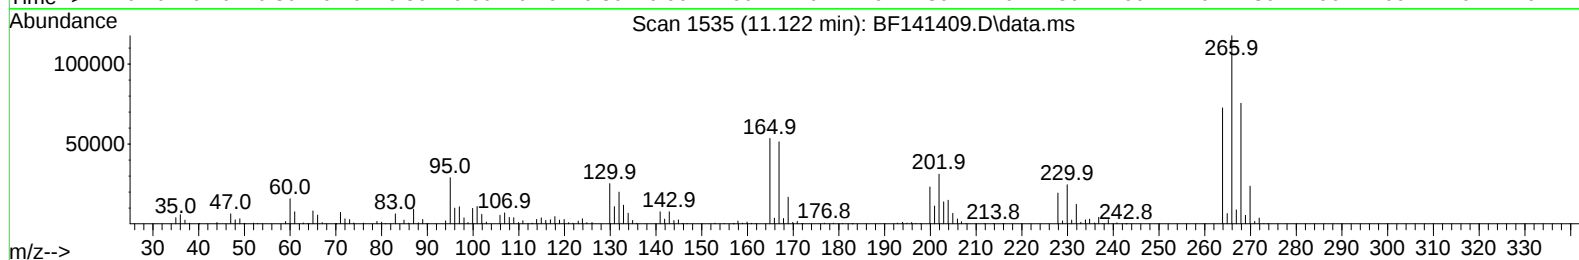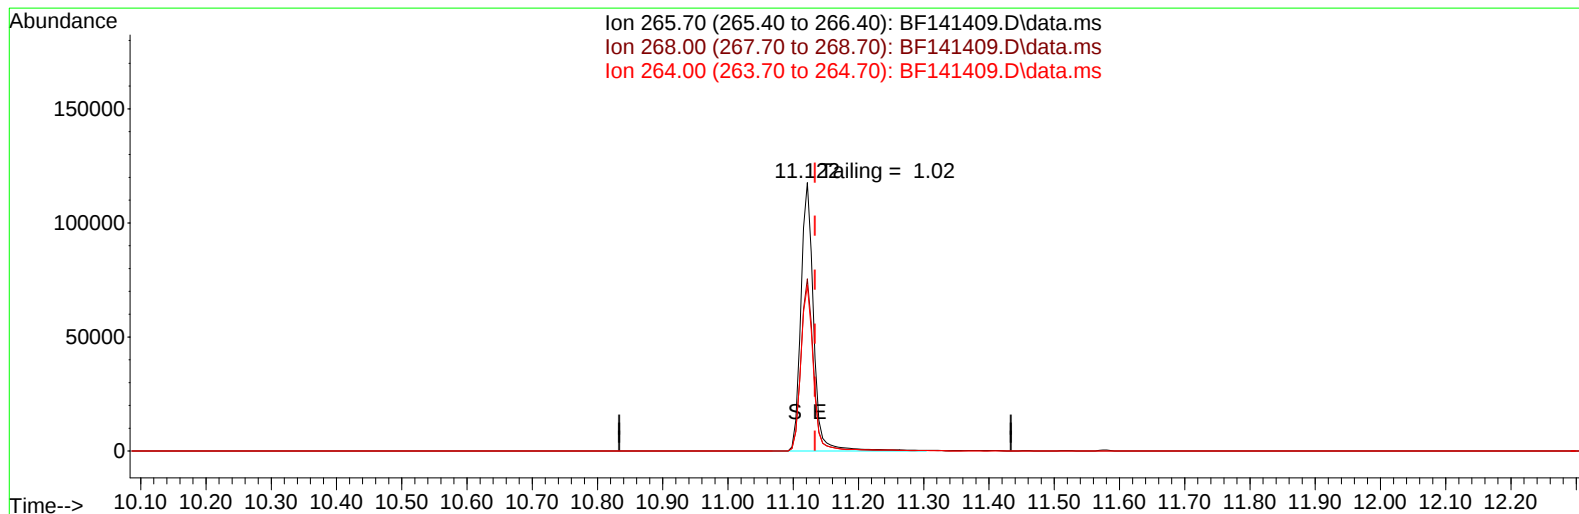

TIC: BF141409.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.012) 188004.57 ng




response 159502

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.16
264.00	63.70	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020425\
Data File : BF141409.D
Acq On : 04 Feb 2025 15:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 04 16:10:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

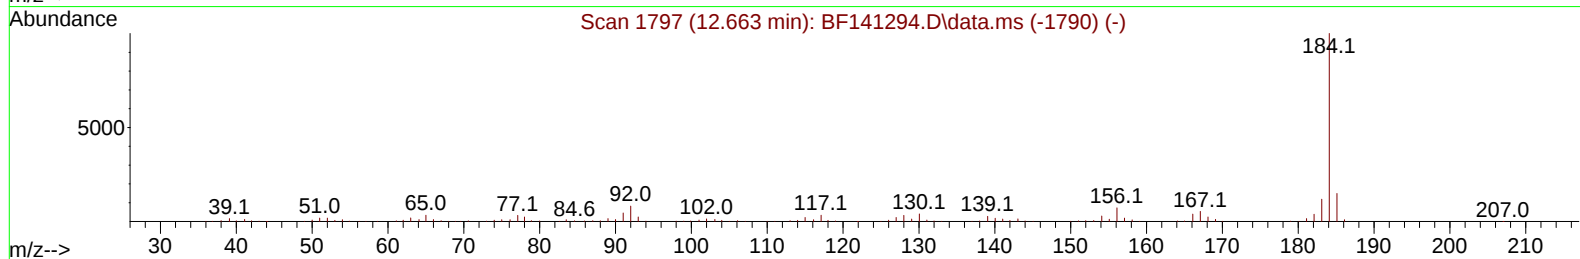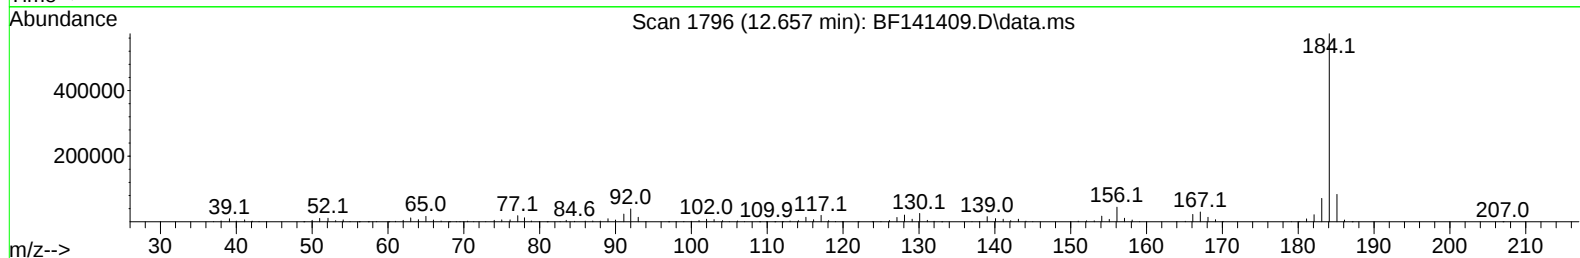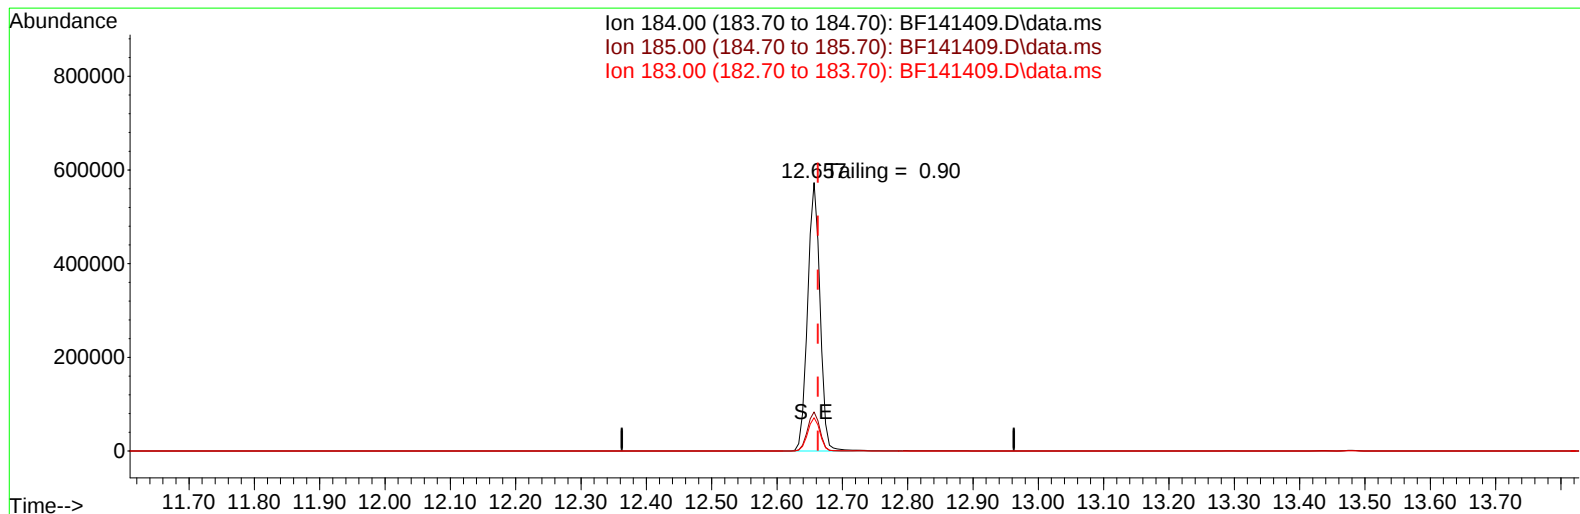

TIC: BF141409.D\data.ms

(77) Benzidine

12.657min (-0.006) 200133.30 ng m

response 757083

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.56
183.00	11.90	12.42
0.00	0.00	0.00