
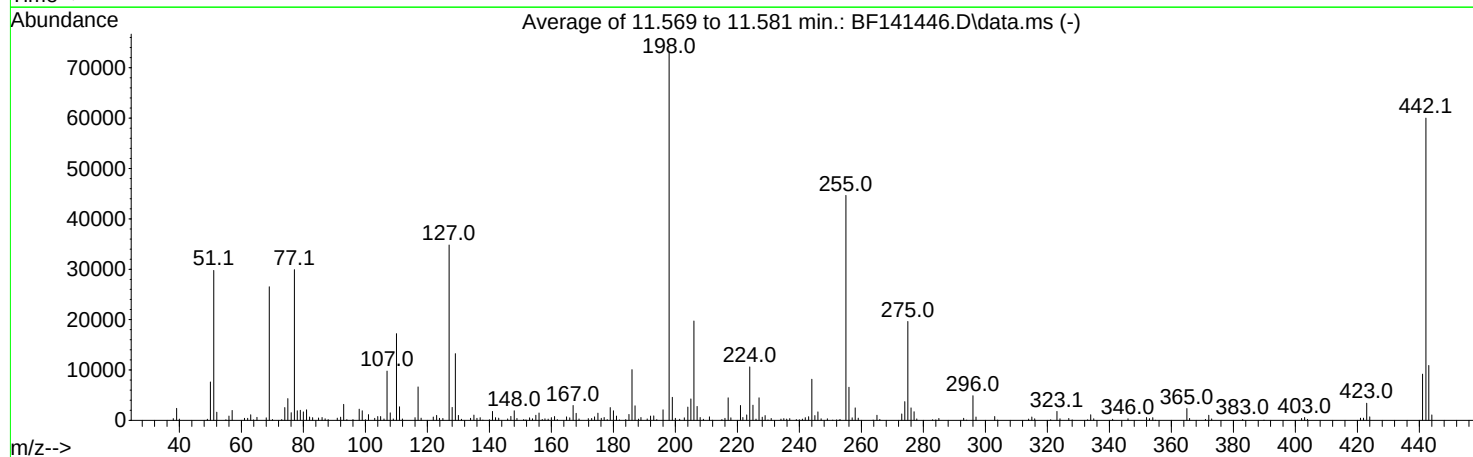


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141446.D
Acq On : 05 Feb 2025 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 29 17:41:25 2025

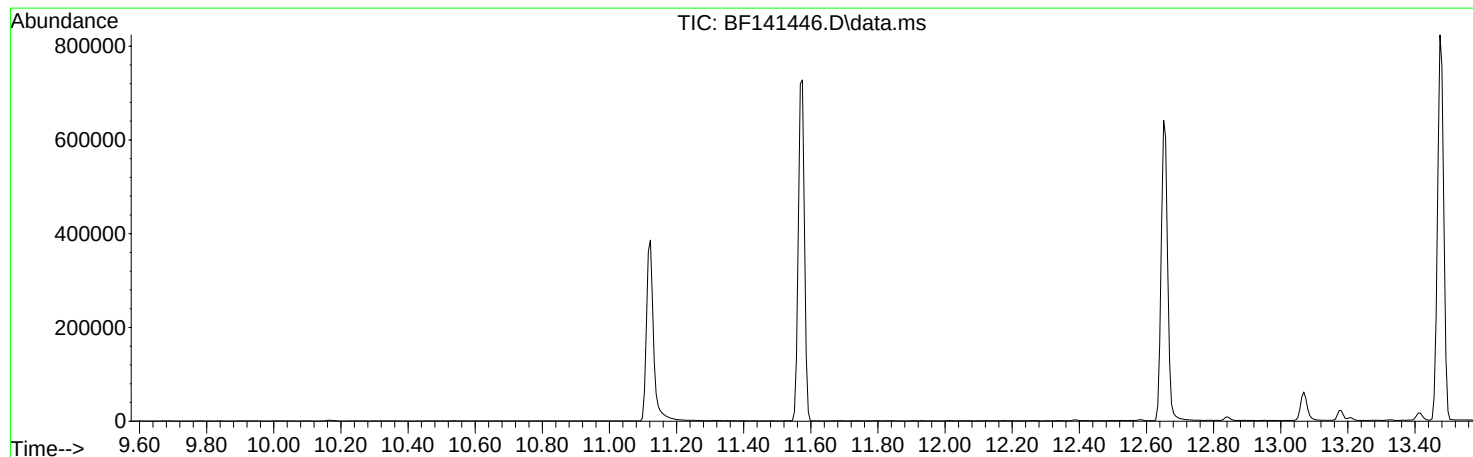

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1604

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.8	29779	PASS
68	69	0.00	2	1.9	505	PASS
69	198	0.00	100	36.3	26508	PASS
70	69	0.00	2	0.6	149	PASS
127	198	10	80	47.7	34819	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73027	PASS
199	198	5	9	6.3	4572	PASS
275	198	10	60	26.9	19638	PASS
365	198	1	100	3.2	2360	PASS
441	198	0.01	100	12.6	9188	PASS
442	442	50	100	100.0	59989	PASS
443	442	15	24	18.2	10895	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/5/2025	BNA_F	<u>BF141446.D</u>
Compound Name	Response	Retention Time
DDT	208681	13.475
DDD	8639	13.18
DDE	1933	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10572	219253	4.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141446.D
Acq On : 05 Feb 2025 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 05 15:11:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

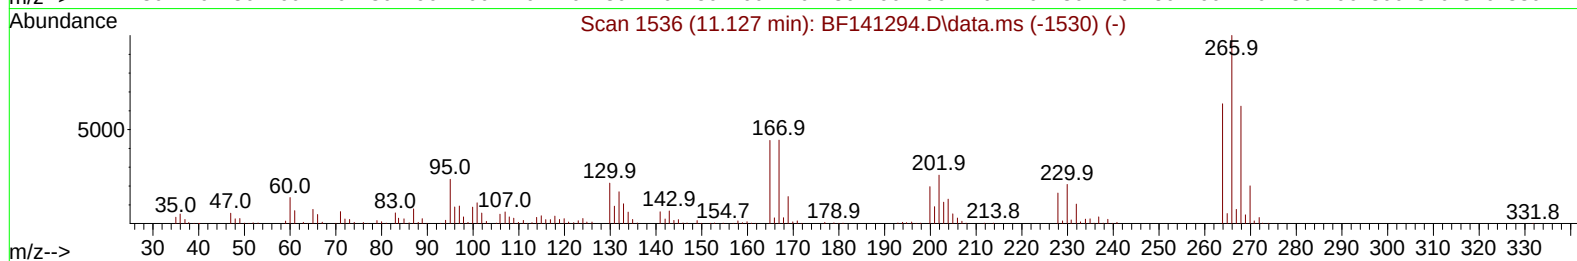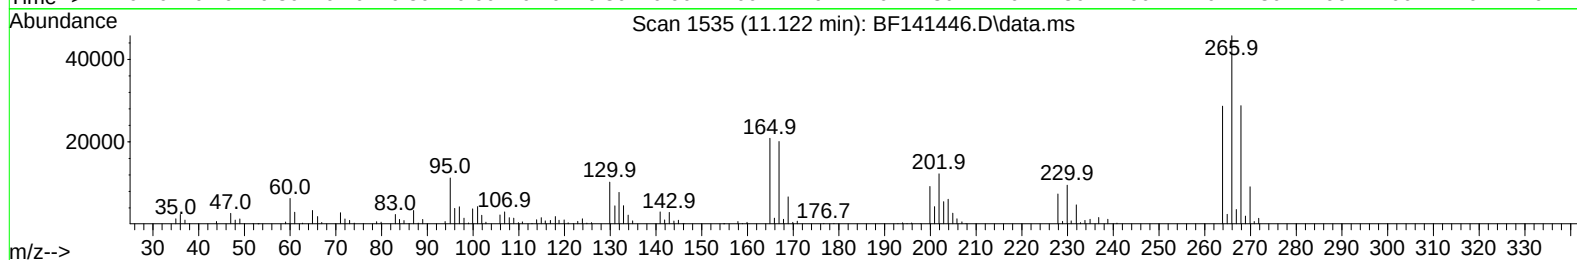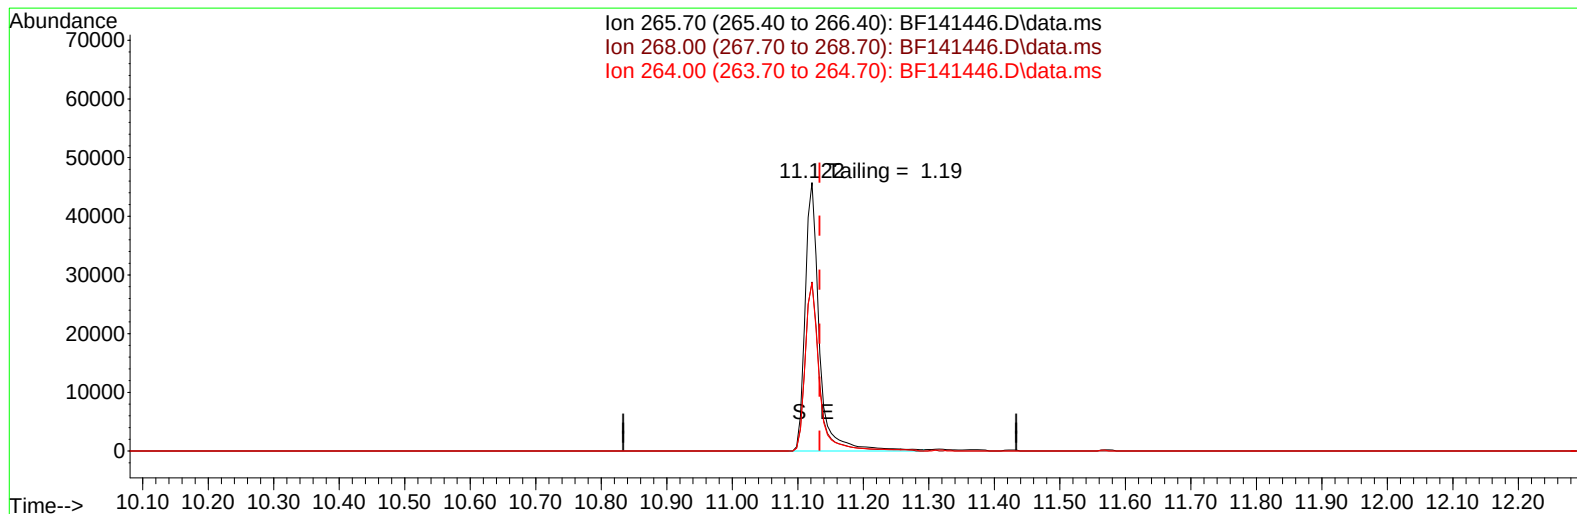

TIC: BF141446.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.012) 28277.45 ng




response 68825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.95
264.00	63.70	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020525\
Data File : BF141446.D
Acq On : 05 Feb 2025 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 05 15:11:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

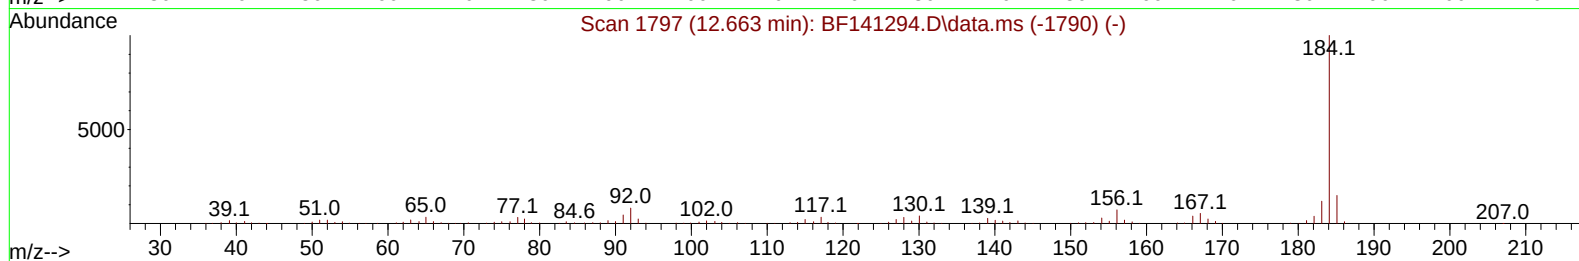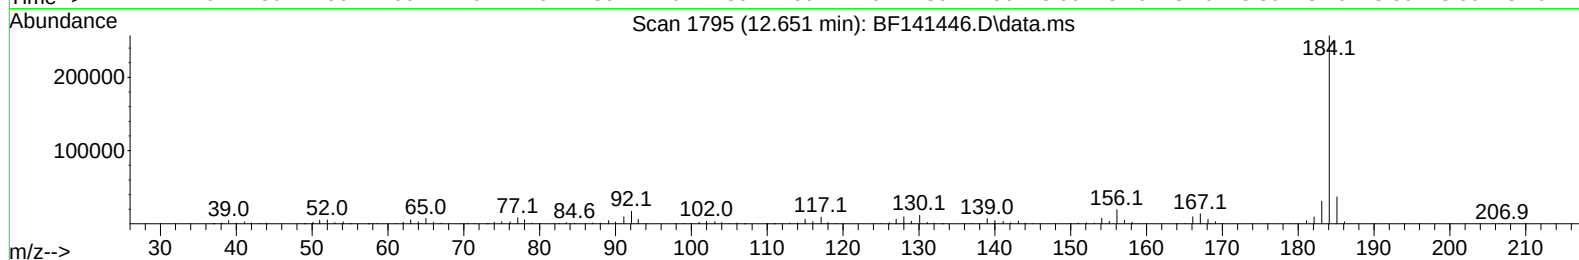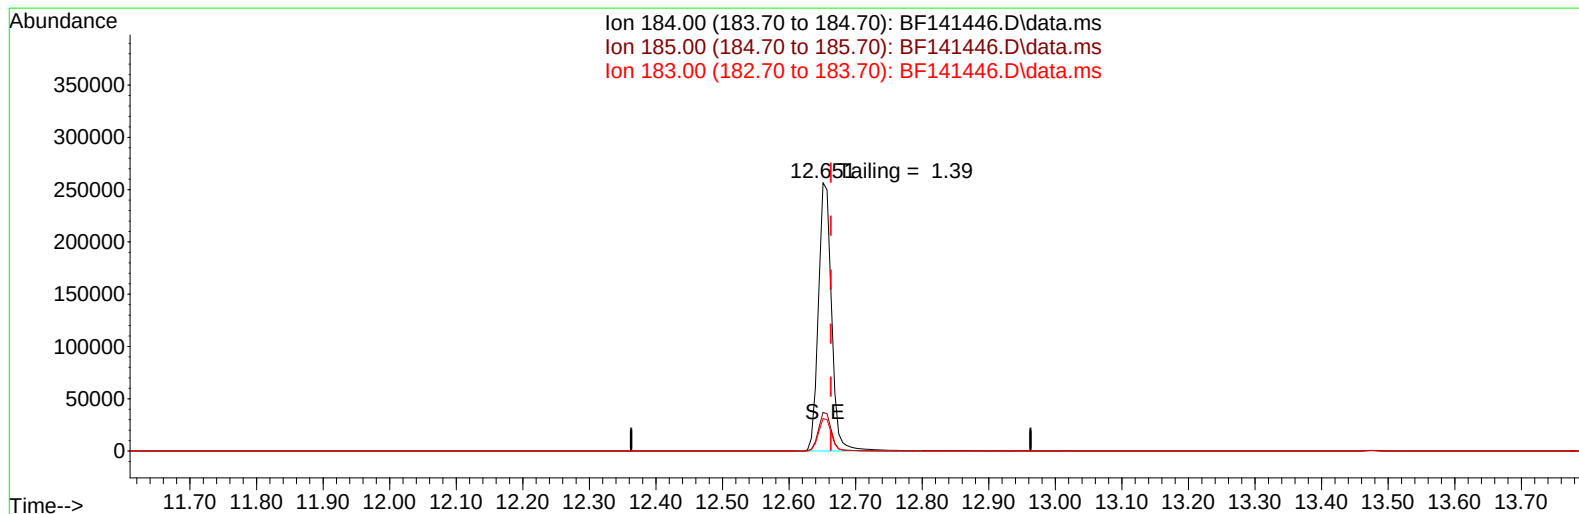

TIC: BF141446.D\data.ms

(77) Benzidine

12.651min (-0.012) 0.00 ng

response 352285

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.37
183.00	11.90	12.10
0.00	0.00	0.00