
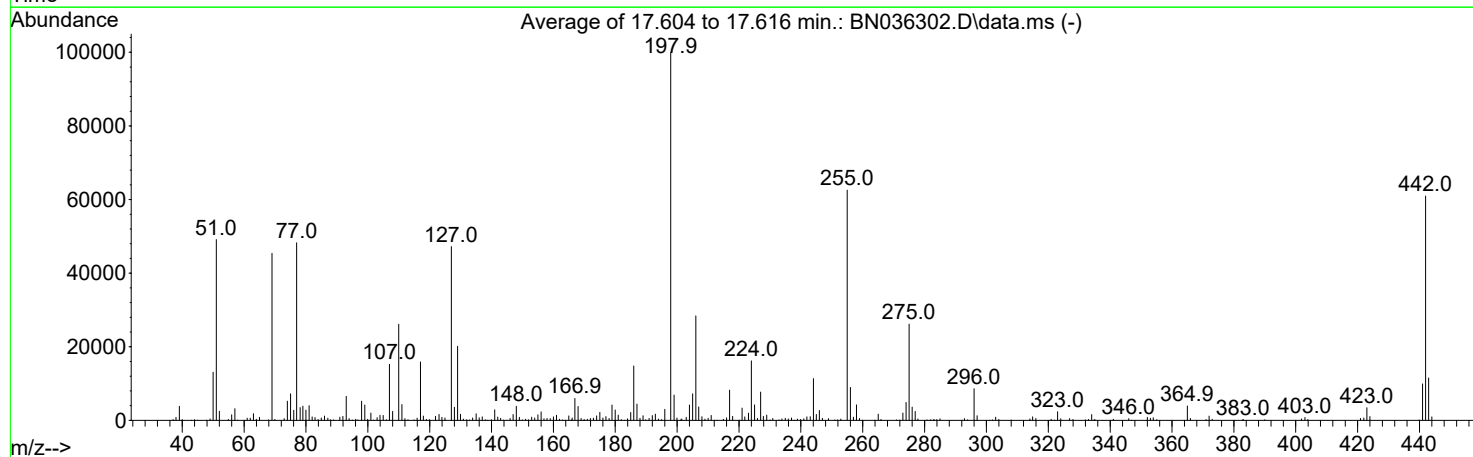


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036302.D
Acq On : 05 Feb 2025 18:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 01:04:09 2025

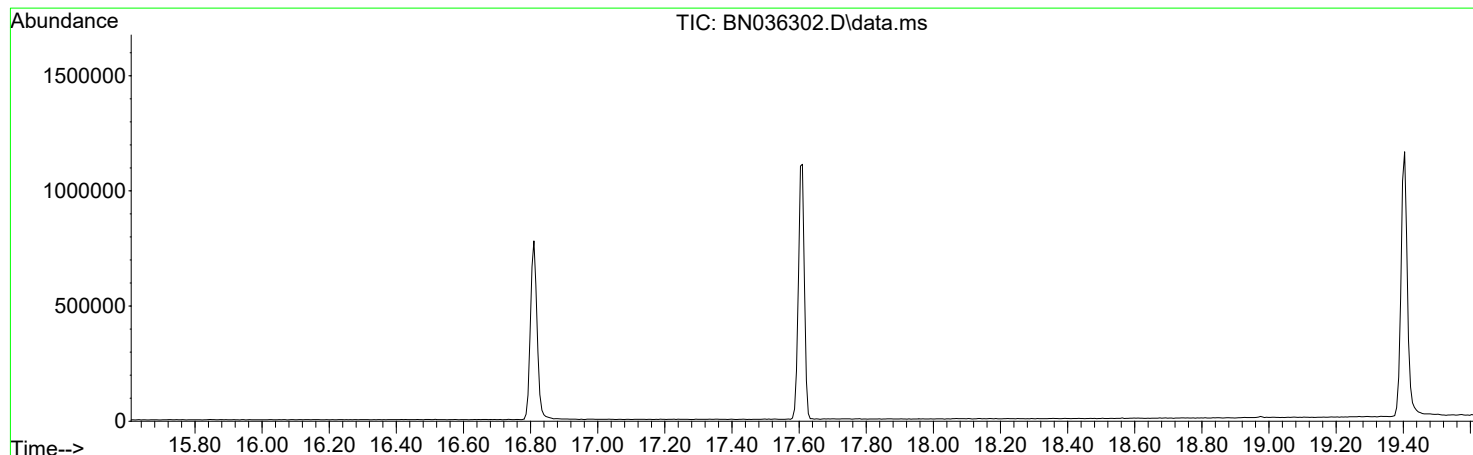

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	49107	PASS
68	69	0.00	2	0.3	138	PASS
69	198	0.00	100	45.4	45403	PASS
70	69	0.00	2	0.6	277	PASS
127	198	10	80	47.2	47213	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99936	PASS
199	198	5	9	6.9	6870	PASS
275	198	10	60	26.2	26165	PASS
365	198	1	100	3.9	3895	PASS
441	198	0.01	100	9.9	9921	PASS
442	442	50	100	100.0	60955	PASS
443	442	15	24	18.9	11502	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/5/2025	BNA_N	<u>BN036302.D</u>
Compound Name	Response	Retention Time
DDT	318276	20.645
DDD	25474	20.204
DDE	705	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26179	344455	7.60

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036302.D
Acq On : 05 Feb 2025 18:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 03:02:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

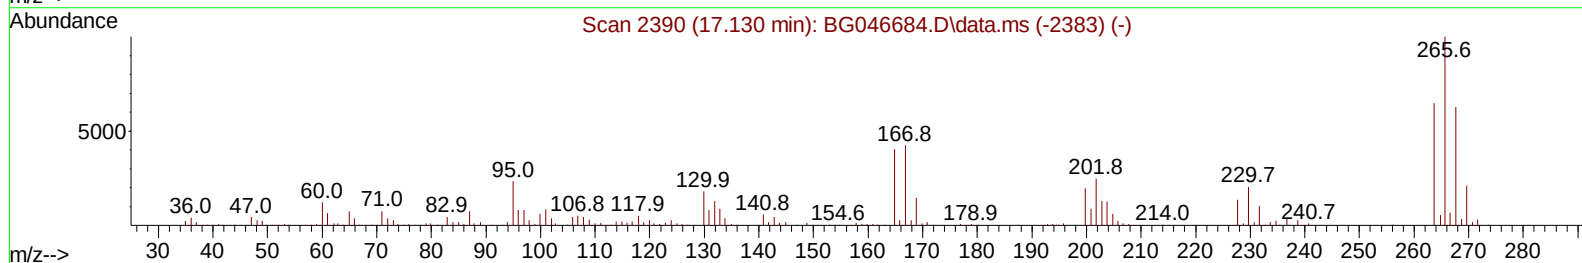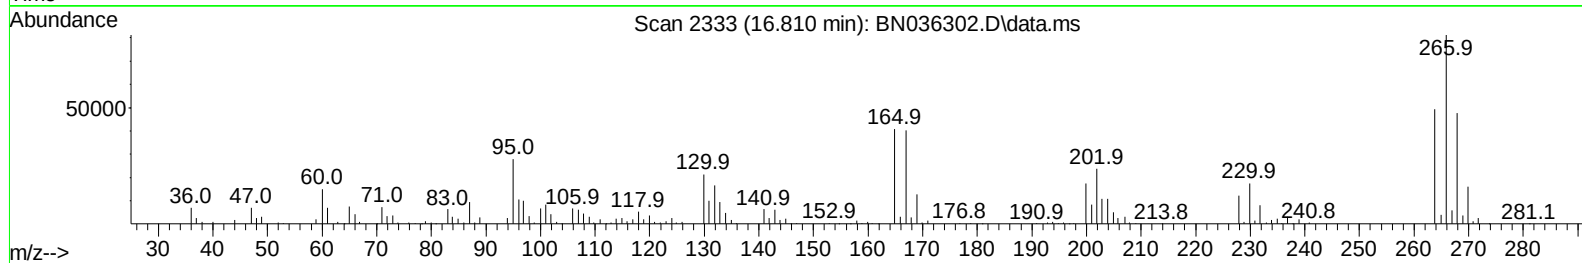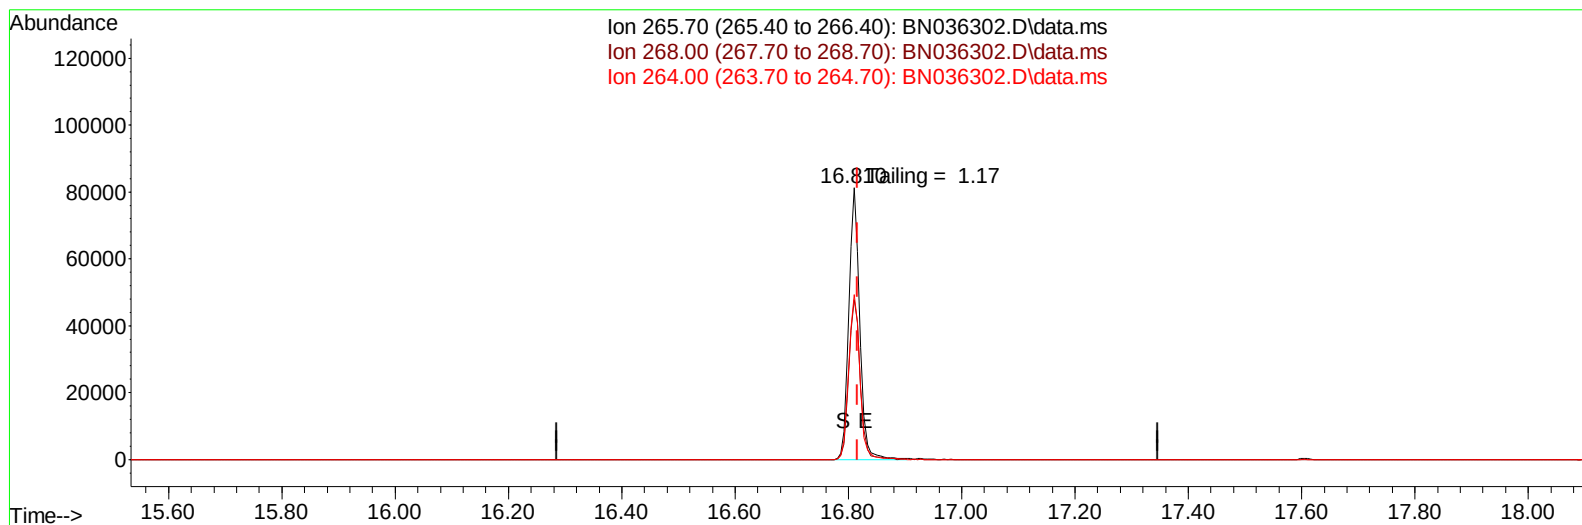

TIC: BN036302.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.006) 17367.43 ng




response 108491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.74
264.00	61.60	60.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036302.D
Acq On : 05 Feb 2025 18:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 03:02:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

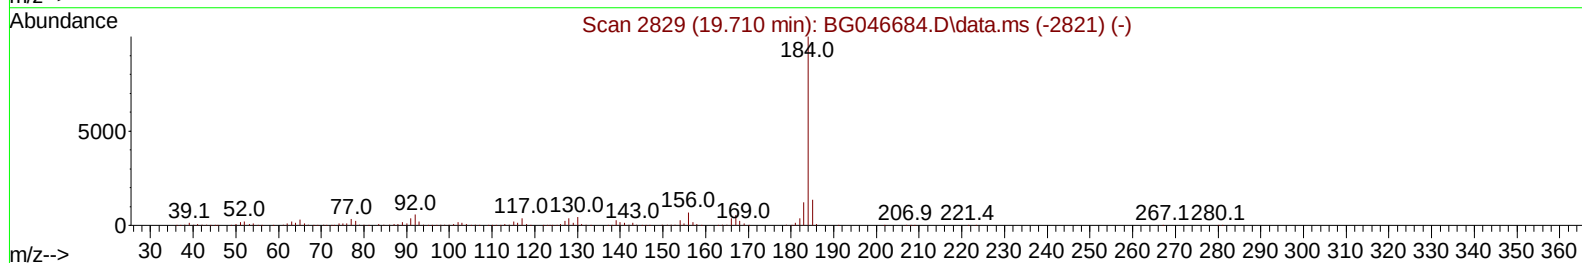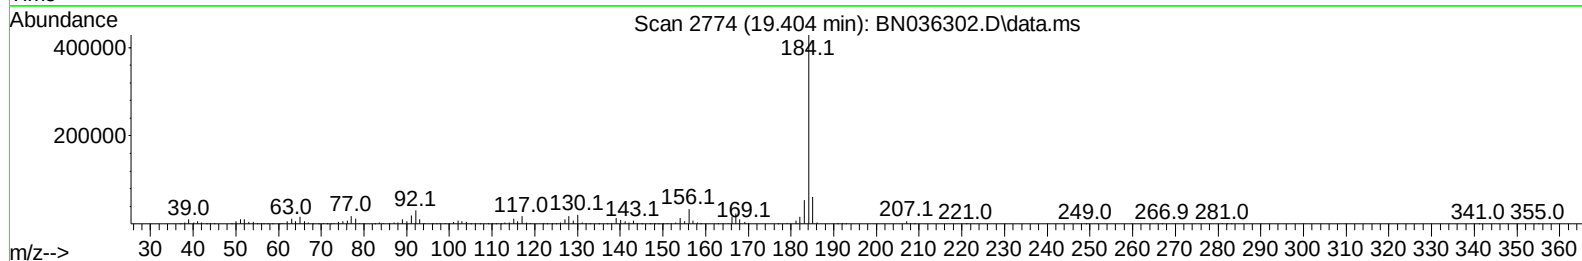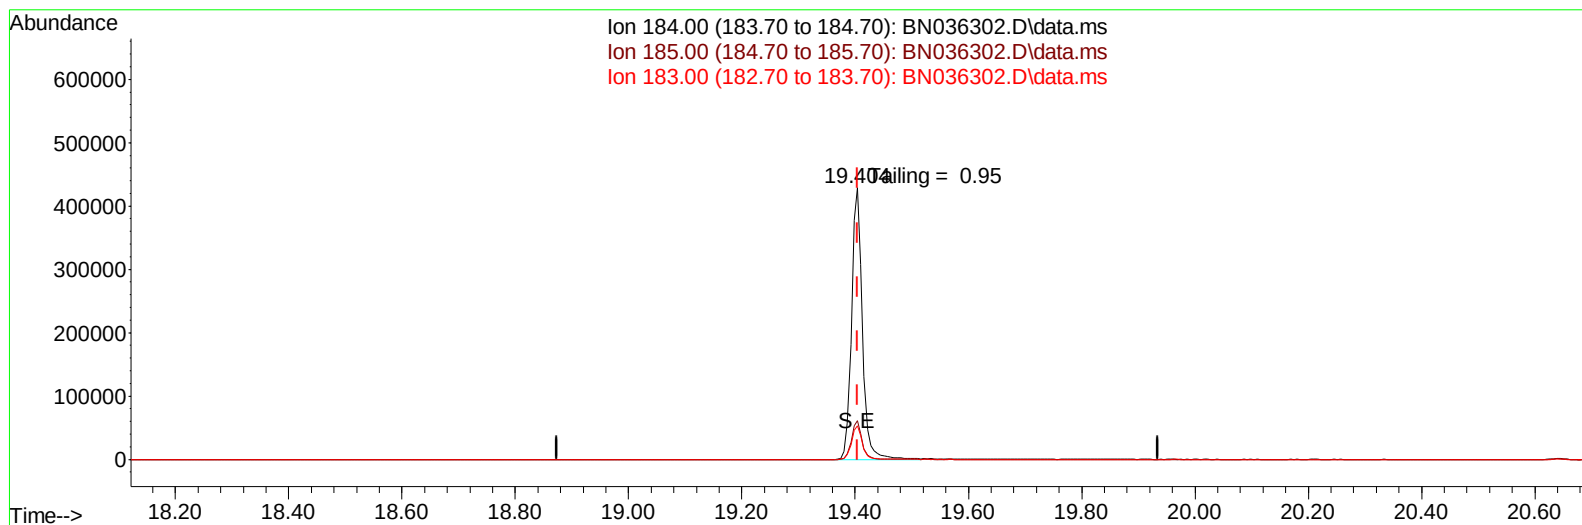

TIC: BN036302.D\data.ms

(77) Benzidine

19.404min (-0.000) 0.00 ng

response 576937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.49
0.00	0.00	0.00