

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011325\
 Data File : FG015060.D
 Signal(s) : FID1A.ch
 Acq On : 13 Jan 2025 11:11
 Operator : YP\AJ
 Sample : 5 TRPH STD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 5 TRPH STD

Integration File: autoint1.e
 Quant Time: Jan 13 11:35:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
 Quant Title :
 QLast Update : Mon Jan 13 11:35:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	648631	5.029 ug/ml
Target Compounds			
1) N-OCTANE	2.012	634654	5.162 ug/ml
2) N-DECANE	4.546	654008	5.028 ug/ml
3) N-DODECANE	6.726	692533	5.049 ug/ml
4) N-TETRADECANE	8.563	693227	5.033 ug/ml
5) N-HEXADECANE	10.177	716946	5.051 ug/ml
6) N-OCTADECANE	11.627	747864	5.071 ug/ml
7) N-EICOSANE	12.942	734881	5.028 ug/ml
8) N-DOCOSANE	14.146	728625	5.053 ug/ml
10) N-TETRACOSANE	15.254	725335	5.053 ug/ml
11) N-HEXACOSANE	16.277	714017	5.045 ug/ml
12) N-OCTACOSANE	17.231	719588	5.113 ug/ml
13) N-TRIACONTANE	18.121	746793	5.225 ug/ml
14) N-DOTRIACONTANE	18.956	739109	5.296 ug/ml
15) N-TETRATRIACONTANE	19.742	661594	5.265 ug/ml
16) N-HEXATRIACONTANE	20.483	565434	5.231 ug/ml
17) N-OCTATRIACONTANE	21.234	509611	5.195 ug/ml
18) N-TETRACONTANE	22.172	475271	5.212 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011325\
Data File : FG015060.D
Signal(s) : FID1A.ch
Acq On : 13 Jan 2025 11:11
Operator : YP\AJ
Sample : 5 TRPH STD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

Integration File: autoint1.e
Quant Time: Jan 13 11:35:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
Quant Title :
QLast Update : Mon Jan 13 11:35:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

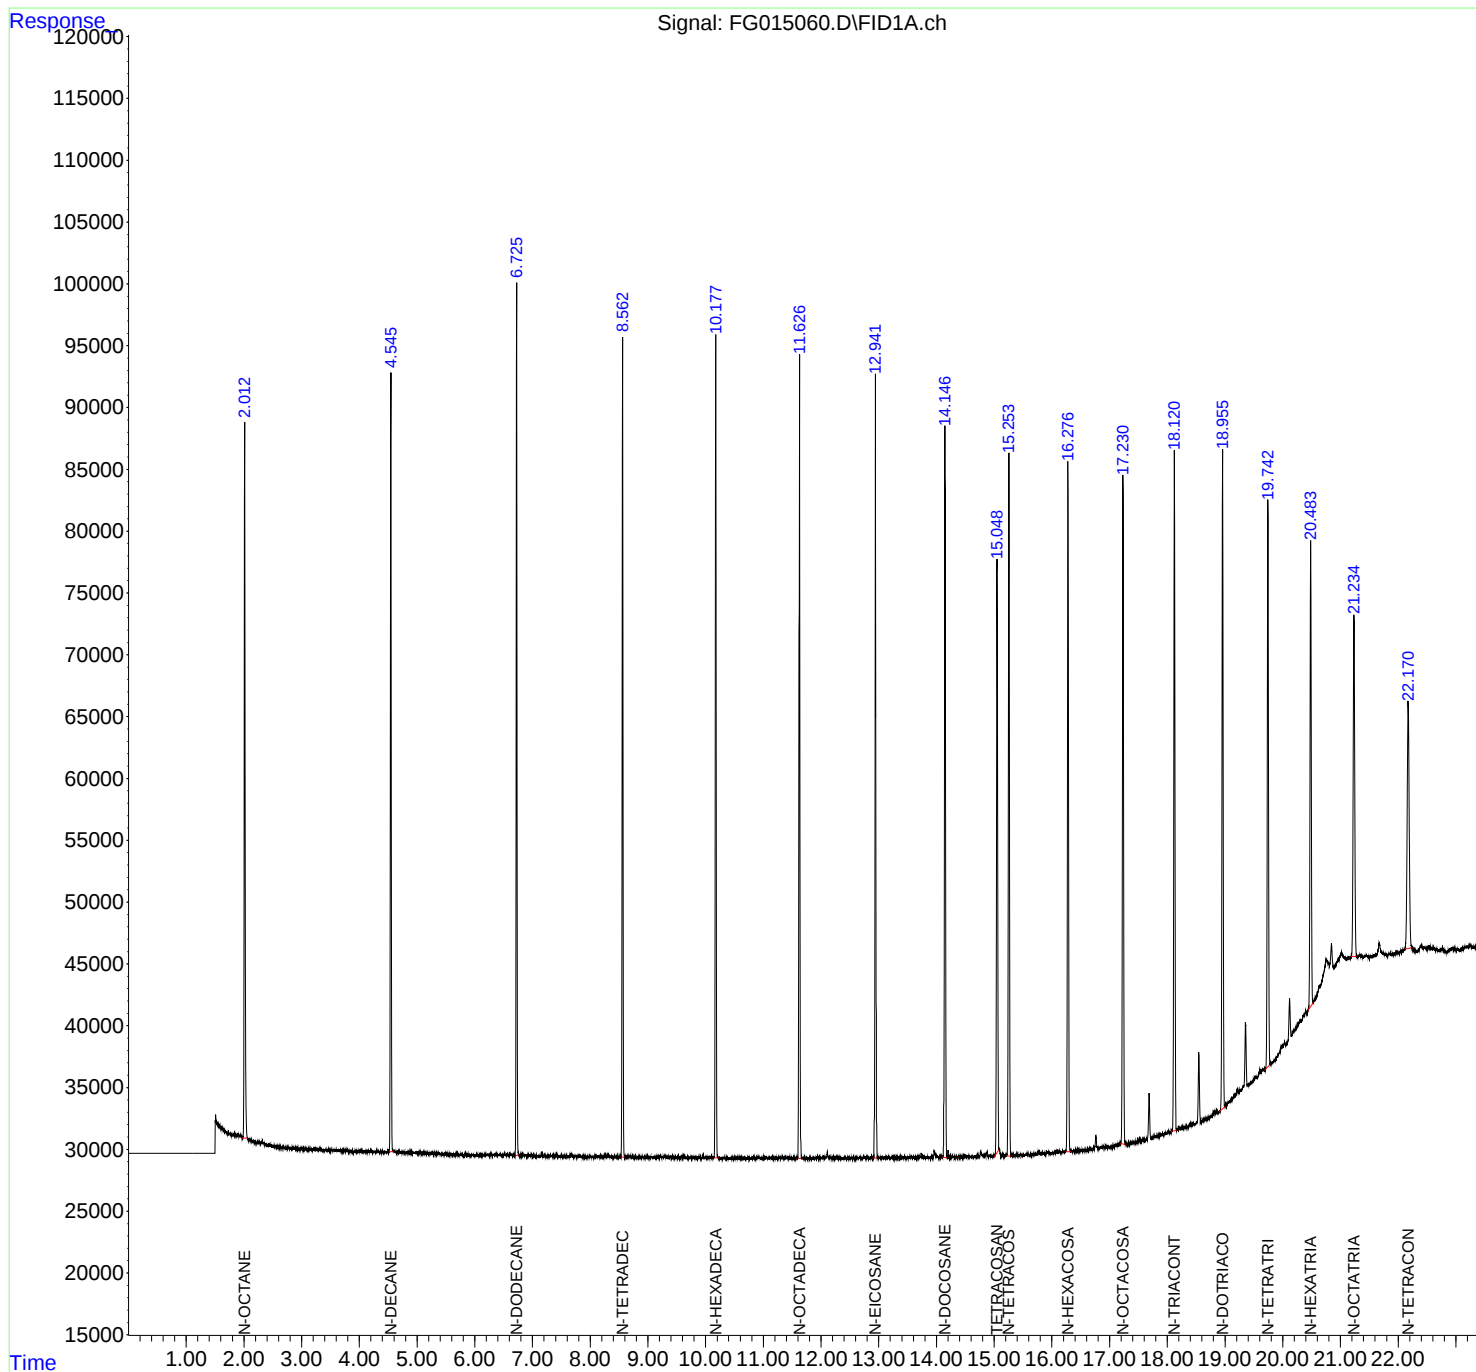


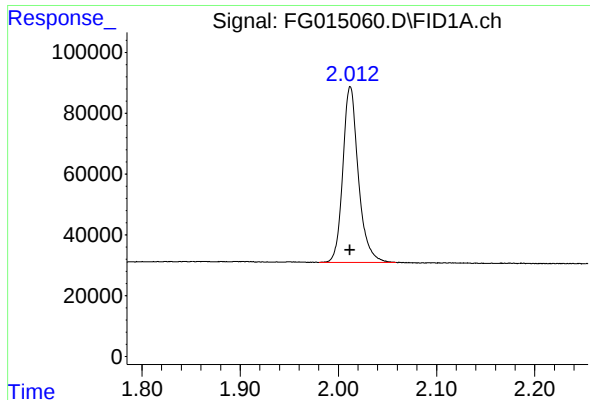

#1 N-OCTANE


R.T.: 2.012 min
Delta R.T.: 0.000 min
Response: 634654
Conc: 5.16 ug/ml

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

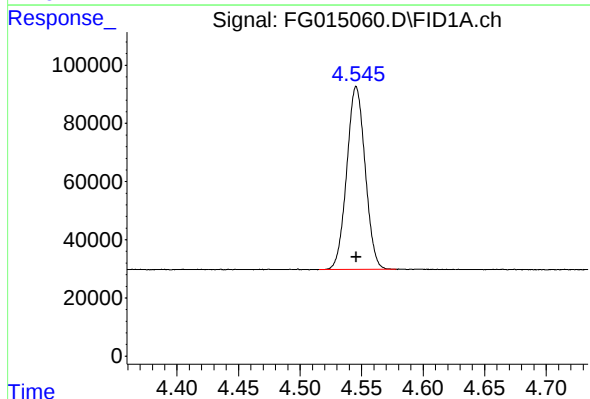


#2 N-DECANE

R.T.: 4.546 min
Delta R.T.: 0.000 min
Response: 654008
Conc: 5.03 ug/ml

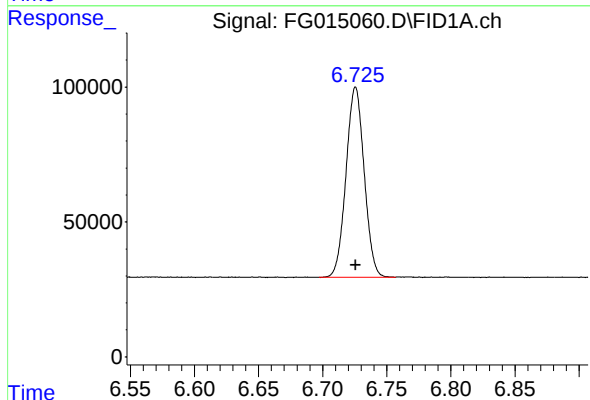


#3 N-DODECANE

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 692533
Conc: 5.05 ug/ml

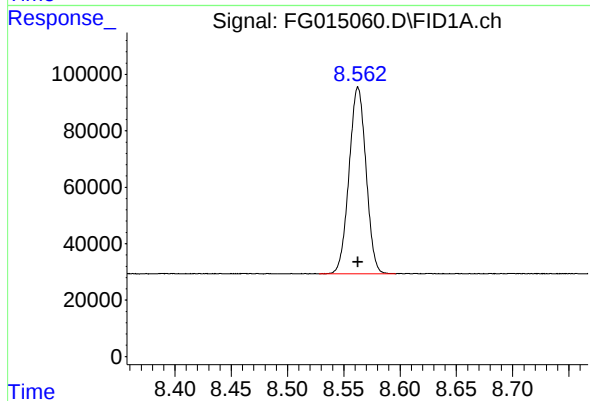

#4 N-TETRADECANE


R.T.: 8.563 min
Delta R.T.: 0.000 min
Response: 693227
Conc: 5.03 ug/ml

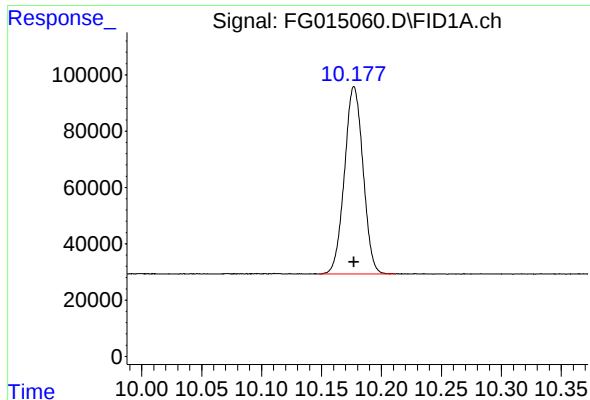

#5 N-HEXADECANE


R.T.: 10.177 min
Delta R.T.: 0.000 min
Response: 716946
Conc: 5.05 ug/ml

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

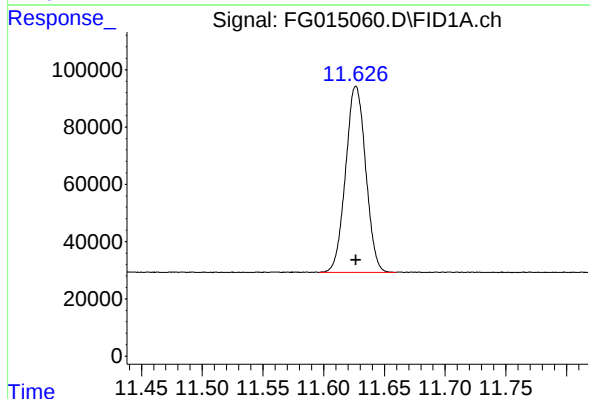


#6 N-OCTADECANE

R.T.: 11.627 min
Delta R.T.: 0.000 min
Response: 747864
Conc: 5.07 ug/ml

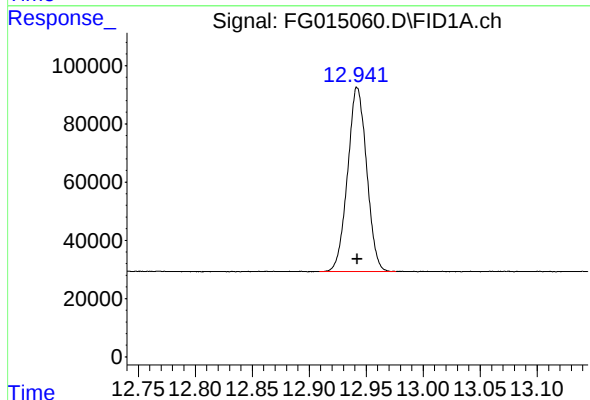


#7 N-EICOSANE

R.T.: 12.942 min
Delta R.T.: 0.000 min
Response: 734881
Conc: 5.03 ug/ml

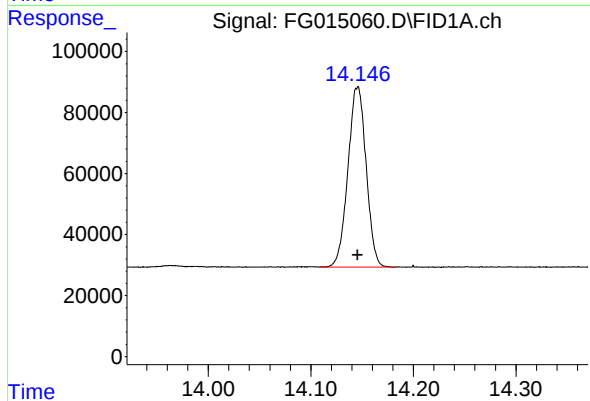

#8 N-DOCOSANE


R.T.: 14.146 min
Delta R.T.: 0.000 min
Response: 728625
Conc: 5.05 ug/ml

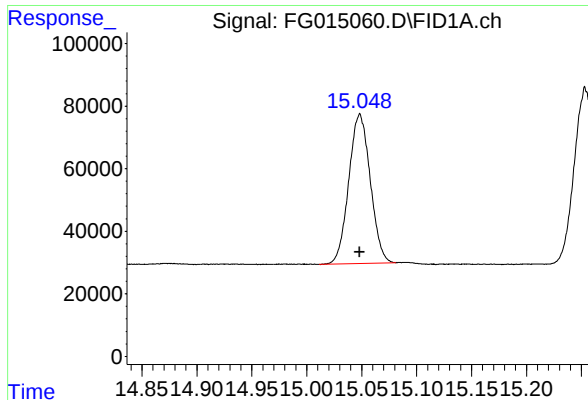

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.048 min
Delta R.T.: 0.000 min
Response: 648631
Conc: 5.03 ug/ml

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

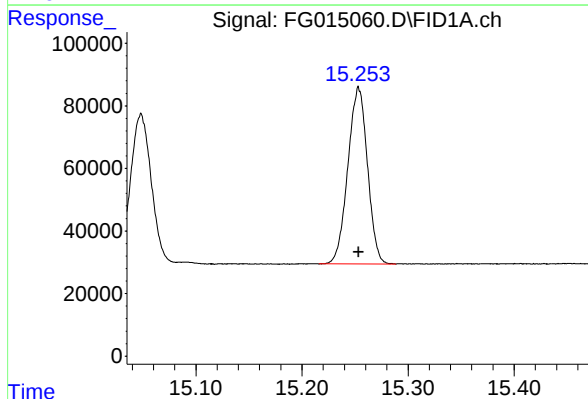


#10 N-TETRACOSANE

R.T.: 15.254 min
Delta R.T.: 0.000 min
Response: 725335
Conc: 5.05 ug/ml

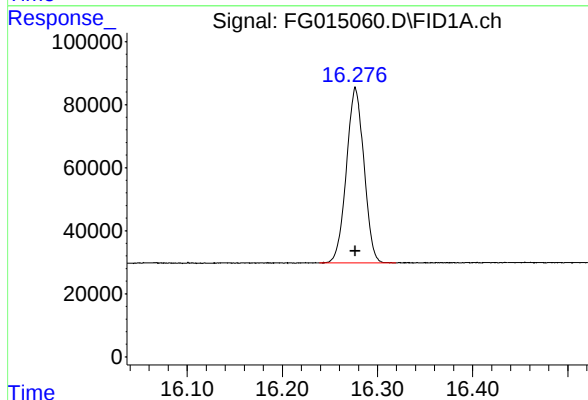


#11 N-HEXACOSANE

R.T.: 16.277 min
Delta R.T.: 0.000 min
Response: 714017
Conc: 5.04 ug/ml

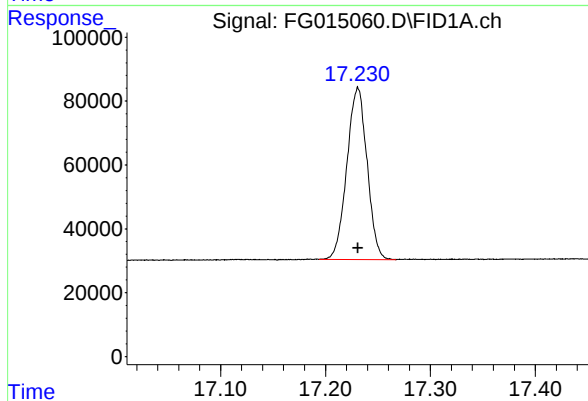

#12 N-OCTACOSANE


R.T.: 17.231 min
Delta R.T.: 0.000 min
Response: 719588
Conc: 5.11 ug/ml

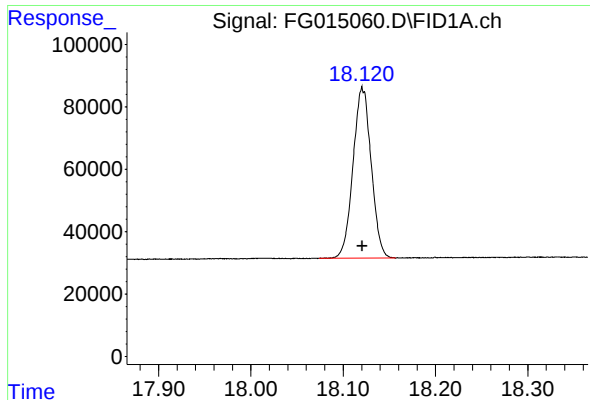

#13 N-TRIACONTANE


R.T.: 18.121 min
Delta R.T.: 0.000 min
Response: 746793
Conc: 5.23 ug/ml

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

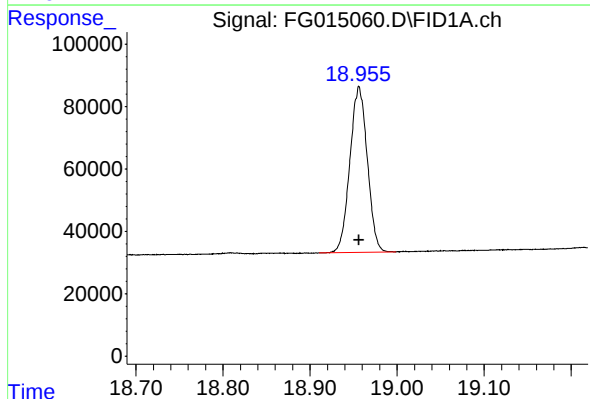


#14 N-DOTRIACONTANE

R.T.: 18.956 min
Delta R.T.: 0.000 min
Response: 739109
Conc: 5.30 ug/ml

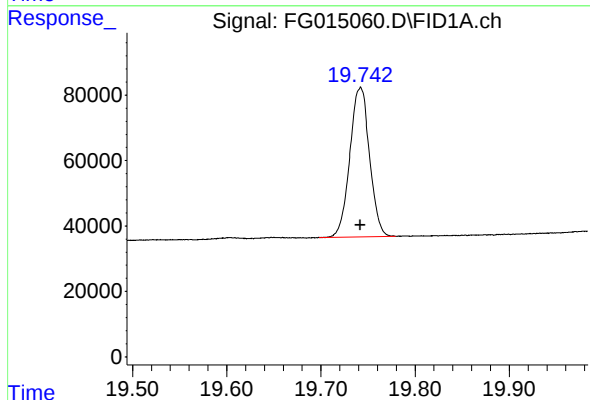


#15 N-TETRATRIACONTANE

R.T.: 19.742 min
Delta R.T.: 0.000 min
Response: 661594
Conc: 5.27 ug/ml

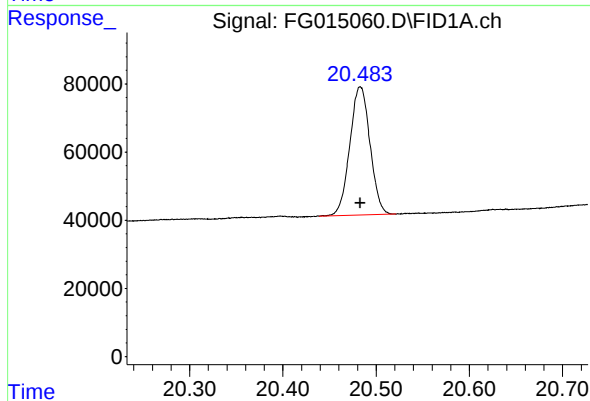

#16 N-HEXATRIACONTANE


R.T.: 20.483 min
Delta R.T.: 0.000 min
Response: 565434
Conc: 5.23 ug/ml

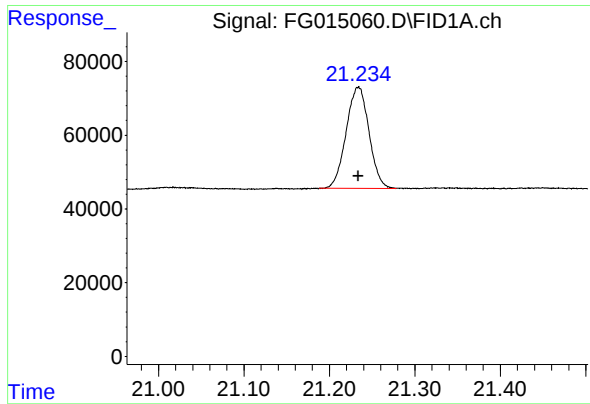

#17 N-OCTATRIACONTANE

R.T.: 21.234 min
Delta R.T.: 0.000 min
Response: 509611
Conc: 5.20 ug/ml

Instrument :
FID_G
ClientSampleId :
5 TRPH STD

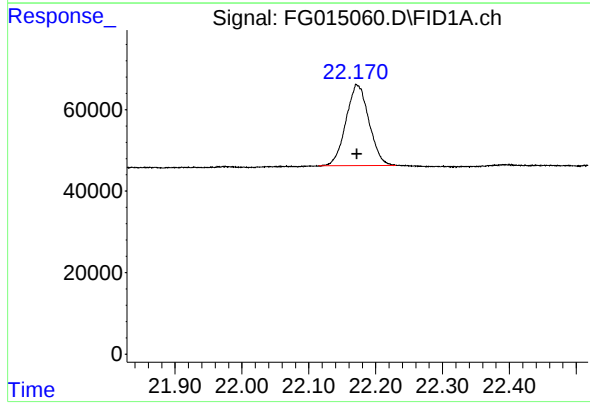

#18 N-TETRACONTANE

R.T.: 22.172 min
Delta R.T.: 0.000 min
Response: 475271
Conc: 5.21 ug/ml