

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB020625\  
Data File : FB031468.D  
Signal(s) : FID2B.CH  
Acq On : 6 Feb 2025 19:06  
Operator : YP/AJ  
Sample : Q1308-04  
Misc : 7.92G/5.00 ML DI WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
EX-11-TPH-5

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/07/2025  
Supervised By :Ankita Jodhani 02/07/2025

Integration File: Calibration.e  
Quant Time: Feb 07 01:45:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011525.M  
Quant Title :  
QLast Update : Wed Jan 15 12:01:08 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units    |
|-----------------------------|-------|----------|---------------|
| -----                       |       |          |               |
| System Monitoring Compounds |       |          |               |
| 5) s AAA-TFT                | 8.833 | 1629086  | 68.298 ng/mlm |
| Target Compounds            |       |          |               |
| -----                       |       |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB020625\  
Data File : FB031468.D  
Signal(s) : FID2B.CH  
Acq On : 6 Feb 2025 19:06  
Operator : YP/AJ  
Sample : Q1308-04  
Misc : 7.92G/5.00 ML DI WATER  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
FID\_B  
ClientSampleId :  
EX-11-TPH-5


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/07/2025  
Supervised By :Ankita Jodhani 02/07/2025

Integration File: Calibration.e  
Quant Time: Feb 07 01:45:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB011525.M  
Quant Title :  
QLast Update : Wed Jan 15 12:01:08 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

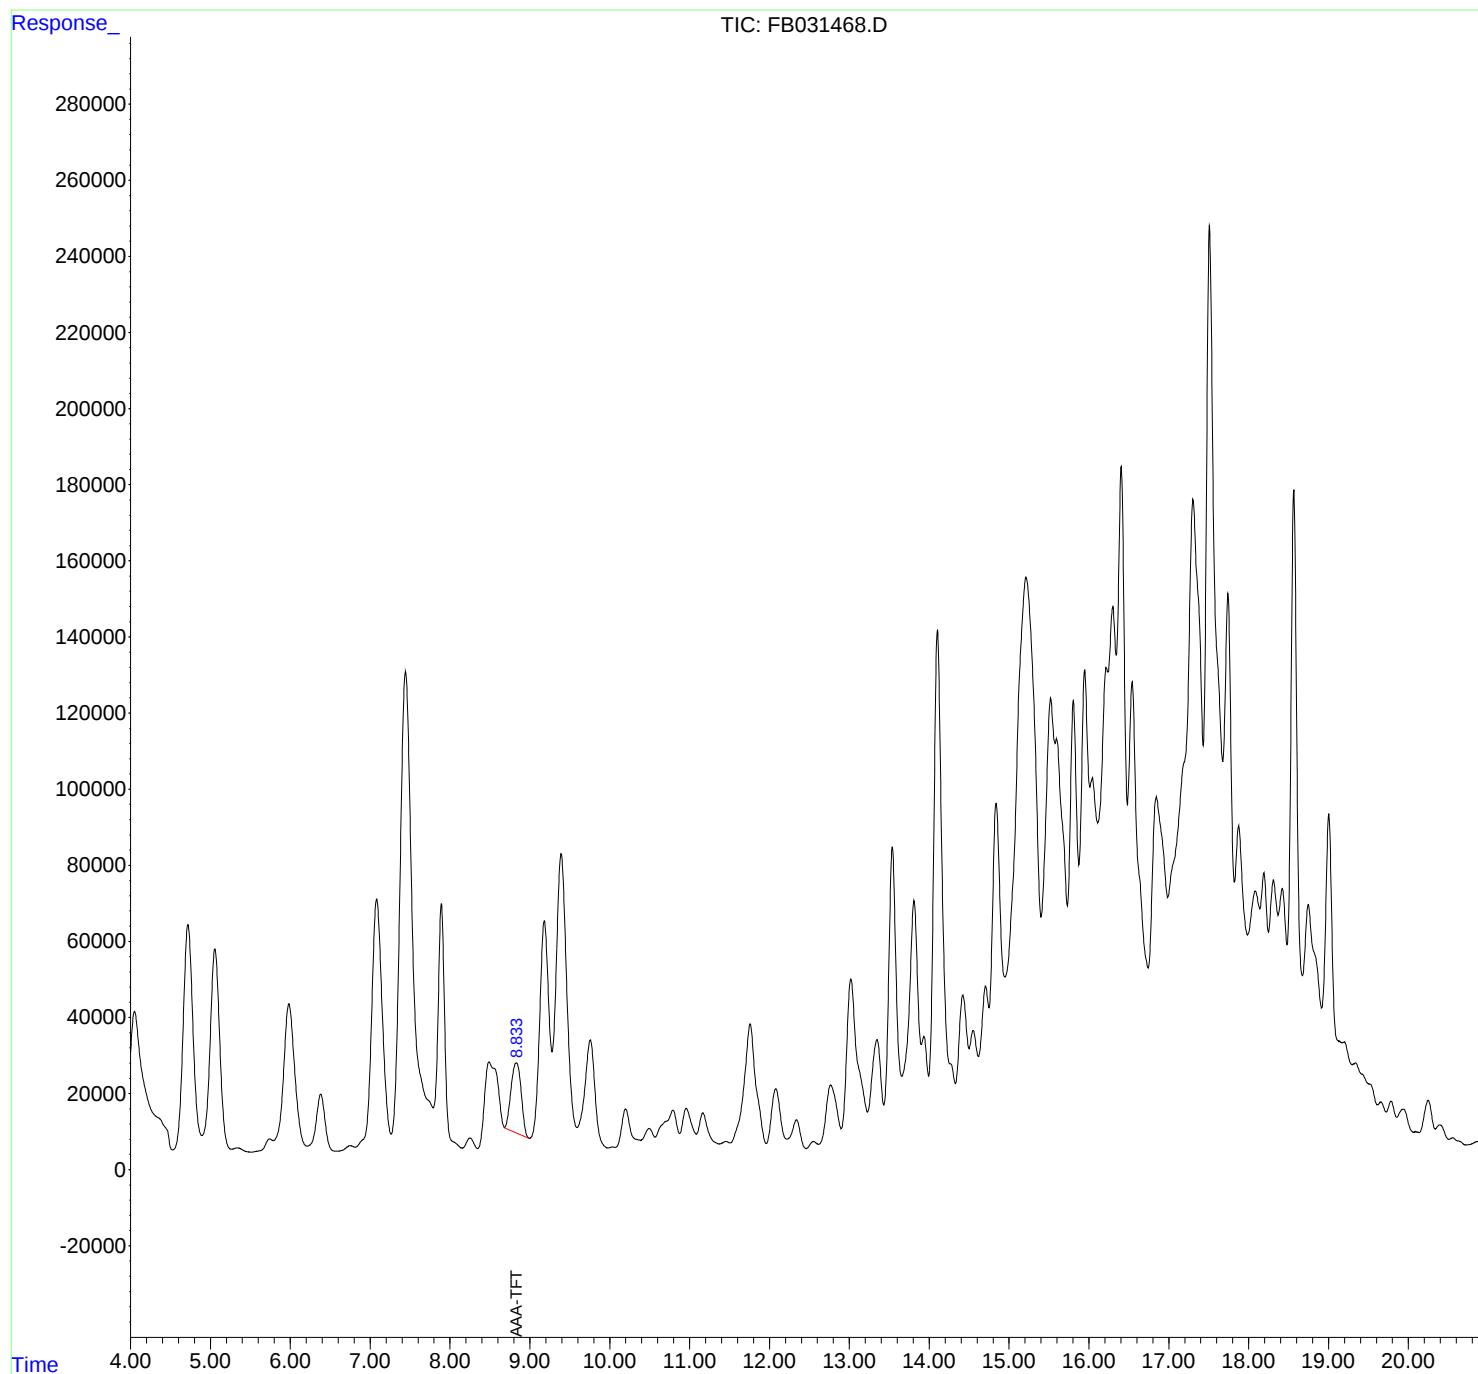

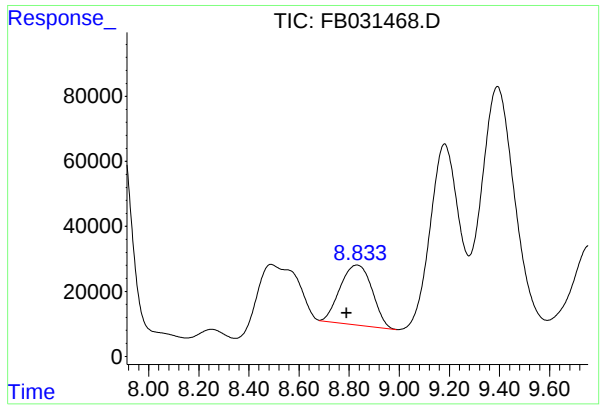

#5 AAA-TFT

R.T.: 8.833 min  
Delta R.T.: 0.044 min  
Response: 1629086  
Conc: 68.30 ng/ml

Instrument :

FID\_B

ClientSampleId :

EX-11-TPH-5

#### Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/07/2025

Supervised By :Ankita Jodhani 02/07/2025