

SDG COVER PAGE

Lab Name: Alliance Technical Group, LLC Contract: 68HERH20D0011
Lab Code: ACE Case No.: 51979 MA No.: _____ SDG No.: MBHHA8
SOW No. : SFAM01.1

EPA Sample No.	Lab Sample Id	ICP-AES	Analysis Method		
			ICP-MS	Mercury	Cyanide
<u>MBHHA8</u>	<u>Q1315-01</u>	<u>X</u>	_____	_____	_____
<u>MBHHA8D</u>	<u>Q1315-02</u>	<u>X</u>	_____	_____	_____
<u>MBHHA8S</u>	<u>Q1315-03</u>	<u>X</u>	_____	_____	_____

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed in the SDG Narrative. All edits and manual integrations have been peer-reviewed. Release of the data contained in this hardcopy Complete SDG File and in the electronic data submitted has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signature.

Signature: _____ Name: _____
Date: _____ Title: _____

No.: 3-020525-095551-0005

Lab Phone: 908-789-8900

[illegible]

Special Instructions: Sample AQ-WC-01F-20250204 is field filtered.

Analysis Key: ICP-AES=CLP ICP-AES 11+ Metals

Shipment for Case Complete? Y

[illegible]

Items/Reason	Relinquished by (Signature and Organization)	Date/Time	Received by (Signature and Organization)	Date/Time	Sample Condition Upon Receipt
	<i>[Signature]</i> (Sovereign)	2/5/25 1200	<i>[Signature]</i>	2-6-25 9:30	IF. 6. #1 2.6
					Custody Seal Intact
					Imp But no

FORM DC-1
SAMPLE LOG-IN SHEET

Lab Name : Alliance Technical Group, LLC		Page <u>1</u> of <u>1</u>
Received By (Print Name) <u>Jose Maria Peria</u>		Log-in Date 2/6/2025
Received By (Signature) <u>[Signature]</u>		
Case Number 51979	SDG No. MBHHA8	MA No. N/A

Remarks:	
1. Custody Seal (s)	Present, Intact
2. Custody Seal Nos.	<u>n/a</u>
3. Traffic Reports/Chain Of Custody Records	Present
4. Airbill	Present
5. Airbill No. and Shipping Container ID No.	<u>771891586681</u> <u>1</u>
6. Shipping Container Temperature Indicator Bottle	Present
7. Shipping Container Temperature	<u>2.6</u> Degree C
8. Sample Condition	Intact
9. Sample Tags Sample Tag Numbers	Absent Listed on Traffic Report
10. Does information on Traffic Reports/Chain of Custody Records and Sample Tags agree ?	Yes
11. Date Received at Lab	<u>02/06/2025</u>
12. Time Received	<u>09:30</u>

	EPA Sample #	Aqueous/ Water Sample pH	Corresponding		Remarks: Condition of Sample Shipment, etc.
			Sample Tag #	Assigned Lab #	
1	MBHHA8	1.3	1072	Q1315-01	Intact
2	MBHHA8D	1.3	1072	Q1315-02	Intact
3	MBHHA8S	1.3	1072	Q1315-03	Intact
4	N/A	N/A	N/A	N/A	N/A
5	N/A	N/A	N/A	N/A	N/A
6	N/A	N/A	N/A	N/A	N/A
7	N/A	N/A	N/A	N/A	N/A
8	N/A	N/A	N/A	N/A	N/A
9	N/A	N/A	N/A	N/A	N/A
10	N/A	N/A	N/A	N/A	N/A
11	N/A	N/A	N/A	N/A	N/A
12	N/A	N/A	N/A	N/A	N/A
13	N/A	N/A	N/A	N/A	N/A
14	N/A	N/A	N/A	N/A	N/A
15	N/A	N/A	N/A	N/A	N/A
16	N/A	N/A	N/A	N/A	N/A
17	N/A	N/A	N/A	N/A	N/A
18	N/A	N/A	N/A	N/A	N/A
19	N/A	N/A	N/A	N/A	N/A
20	N/A	N/A	N/A	N/A	N/A
21	N/A	N/A	N/A	N/A	N/A
22	N/A	N/A	N/A	N/A	N/A
23	N/A	N/A	N/A	N/A	N/A

* Contact SMO and attach record of resolution

Reviewed By <u>[Signature]</u>	Logbook No. N/A
Date <u>2/6/25</u>	Logbook Page No. N/A

FORM DC-2
COMPLETE SDG FILE (CSF) INVENTORY SHEET

LAB NAME	Alliance Technical Group, LLC		
LAB CODE	ACE		
CONTRACT NO.	68HERH20D0011		
CASE NO.	51979	SDG NO.	MBHHA8
MA NO.		SOW NO.	SFAM01.1

All documents delivered in the Complete SDG File must be original documents where possible.
(Reference - Exhibit B Section 2.4)

	PAGE NOS:		CHECK	
	FROM	TO	LAB	REGION
1. SDG Cover Page	1	1	✓	
2. Traffic Report/Chain of Custody Record(s)	2	2	✓	
3. Sample Log-In Sheet (DC-1)	3	3	✓	
4. CSF Inventory Sheet (DC-2)	4	6	✓	
5. SDG Narrative	7	9	✓	
6. Communication Logs	10	11	✓	
7. Percent Solids Log	NA	NA	✓	

Analysis Forms and Data (ICP-AES)

8. Sample Analysis Data Forms (1A-OR, 1B-OR, and 1-IN) for each sample or sample analysis, laboratory QC as applicable	12	12	✓	
9. Instrument raw data by instrument in analysis order	13	109	✓	

Other Data

10. Standard and Reagent Preparation Logs	110	255	✓	
11. Original Preparation and Cleanup forms or copies of Preparation and Cleanup Logbooks	256	257	✓	
12. Original Analysis or Instrument Run forms or copies of Analysis or Instrument Logbooks	258	259	✓	
13. Performance Evaluation (PE)/Proficiency Testing (PT) Sample Instructions	NA	NA	✓	
14. Extraction Logs for TCLP and SPLP	NA	NA	✓	
15. Raw GPC Data	NA	NA	✓	
16. Raw Florisil Data	NA	NA	✓	

Analysis Forms and Data (ICP-MS)

17. Sample Analysis Data Forms (1A-OR, 1B-OR, and 1-IN) for each sample or sample analysis, laboratory QC as applicable	NA	NA	✓	
18. Instrument raw data by instrument in analysis order	NA	NA	✓	

Other Data

19. Standard and Reagent Preparation Logs	NA	NA	✓	
20. Original Preparation and Cleanup forms or copies of Preparation and Cleanup Logbooks	NA	NA	✓	
21. Original Analysis or Instrument Run forms or copies of Analysis or Instrument Logbooks	NA	NA	✓	
22. Performance Evaluation (PE)/Proficiency Testing (PT) Sample Instructions	NA	NA	✓	

- 23 . Extraction Logs for TCLP and SPLP
- 24 . Raw GPC Data
- 25 . Raw Florisil Data

PAGE NOS:		CHECK	
FROM	TO	LAB	REGION
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	

Analysis Forms and Data (Mercury)

- 26 . Sample Analysis Data Forms (1A-OR, 1B-OR, and 1-IN) for each sample or sample analysis, laboratory QC as applicable
- 27 . Instrument raw data by instrument in analysis order

NA	NA	✓	
NA	NA	✓	

Other Data

- 28 . Standard and Reagent Preparation Logs
- 29 . Original Preparation and Cleanup forms or copies of Preparation and Cleanup Logbooks
- 30 . Original Analysis or Instrument Run forms or copies of Analysis or Instrument Logbooks
- 31 . Performance Evaluation (PE)/Proficiency Testing (PT) Sample Instructions
- 32 . Extraction Logs for TCLP and SPLP
- 33 . Raw GPC Data
- 34 . Raw Florisil Data

NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	

Analysis Forms and Data (Cyanide)

- 35 . Sample Analysis Data Forms (1A-OR, 1B-OR, and 1-IN) for each sample or sample analysis, laboratory QC as applicable
- 36 . Instrument raw data by instrument in analysis order

NA	NA	✓	
NA	NA	✓	

Other Data

- 37 . Standard and Reagent Preparation Logs
- 38 . Original Preparation and Cleanup forms or copies of Preparation and Cleanup Logbooks
- 39 . Original Analysis or Instrument Run forms or copies of Analysis or Instrument Logbooks
- 40 . Performance Evaluation (PE)/Proficiency Testing (PT) Sample Instructions
- 41 . Extraction Logs for TCLP and SPLP
- 42 . Raw GPC Data
- 43 . Raw Florisil Data

NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	
NA	NA	✓	

Additional

44. EPA Shipping/Receiving Documents

Airbill (No. of Shipments 1)

Sample Tags

Sample Log-In Sheet (Lab)

45. Misc. Shipping/Receiving Records (list all individual records)

46. Internal Lab Sample Transfer Records and Tracking Sheets
(describe or list)47. Other Records and related Communication Logs
(describe or list)

48. Comments:

Completed by:
(CLP Lab)Audited by:
(EPA)

Nimisha Pandya, Document Control Officer

PAGE NOs:		CHECK	
FROM	TO	LAB	REGION
260	260	✓	
NA	NA	✓	
261	261	✓	
NA	NA	✓	
262	262	✓	
NA	NA	✓	



**284 Sheffield Street
Mountainside, NJ 07092**

SDG NARRATIVE

USEPA

SDG # MBHHA8

CASE # 51979

CONTRACT # 68HERH20D0011

SOW# SFAM01.1

LAB NAME: Alliance Technical Group, LLC

LAB CODE: ACE

LAB ORDER ID # Q1315

A. Number of Samples and Date of Receipt

01 Water samples was delivered to the laboratory intact on 02/06/2025.

B. Parameters

Test requested for Metals CLP FULL = Aluminum, Antimony, Arsenic, Barium, Beryllium, Cadmium, Calcium, Chromium, Cobalt, Copper, Iron, Lead, Magnesium, Manganese, Nickel, Potassium, Selenium, Silver, Sodium, Thallium, Vanadium, Zinc.

C. Cooler Temp

Indicator Bottle: Presence/Absence

Cooler: 2.6°C

D. Detail Documentation (related to Sample Handling Shipping, Analytical Problem, Temp of Cooler etc):

Issue 1 : A "P" or "M" prefix was listed at the beginning of a CLP sample ID.

Issue 2: Laboratory QC is scheduled for soil and water ICP-AES Metals analysis, but no samples were Designated for QC. The laboratory would like to use samples MBHHA7, MBHHA8, and MBHHA9 for laboratory QC. The laboratory confirms that these samples are not blanks, rinsates, or PT samples.

E. Corrective Action taken for above:

Resolution 1 : To maintain COC integrity, ASB requests no changes to the Sample IDs. The laboratory will note the issue in the SDG Narrative and proceed with the analysis of the samples.

Resolution 2: Per SOW SFAM01.1 Exhibit A, Section 5.5.4.1., please note the issue in the SDG Narrative And proceed with the analysis of the samples using the selected samples for QC.



**284 Sheffield Street
Mountainside, NJ 07092**

F. Analytical Techniques:

All analyses were based on CLP Methodology by method SFAM01.1.

Inter Element correction factors (IECs) are determined annually and correction factor are applied during ICP-AES analysis.

G. Calculation:

Calculation for ICP-AES Water Sample:

$$\text{Concentration or Result } (\mu\text{g/L}) = C \times \frac{V_f}{V_i} \times \text{DF} \times 1000$$

Where,

C = Instrument value in ppm (The average of all replicate exposures)

V_f = Final digestion volume (mL)

V_i = Initial aliquot amount (mL) (Sample amount taken in prep)

DF = Dilution Factor

Example Calculation For Sample MBHHA8 For Aluminum:

If C = 0.0273325 ppm

V_f = 50 ml

V_i = 50 ml

DF = 1

$$\text{Concentration or Result } (\mu\text{g/L}) = 0.0273325 \times \frac{50}{50} \times 1 \times 1000$$

$$= 27.3325 \mu\text{g/L}$$

$$= 27 \mu\text{g/L} \text{ (Reported Result with Signification)}$$

H. QA/ QC

Calibrations met requirements. Interference check met requirements. Blank analyses did not indicate any presence of contamination. Laboratory Control sample was within control limits. Spike sample did meet requirements except for Silver. Duplicate sample did meet requirements. Serial Dilution did meet requirements.

I certify that the data package is in compliance with the terms and conditions of the contract both technically and for completeness, for other than the conditions detailed above. Release of the data



**284 Sheffield Street
Mountainside, NJ 07092**

contained in this hard copy data package has been authorized by the Laboratory Director or his designee,
as verified by the following signature.

Signature _____

Name: Nimisha Pandya

Date _____

Title: Document Control Officer

From: DeBerry, Eric <Eric.Deberry@gdit.com>
Sent: Thursday, February 06, 2025 11:02 AM
To: Deepak Parmar; Sohil Jodhani; Mohammad Ahmed
Cc: Bauer, Heather E; Johnson, Matthew; Burman, Jarmael; Roberson, Sharon; 'Moody, Brett'; Gambrah, Derrick; Patel, Bhavita; Vargas.Magda@epa.gov; Britz, Helen
Subject: Region 03 | Case 51979 | Lab ACE | Issue Insufficient/inappropriate designation of laboratory QC | FINAL
Attachments: SKM_95825020609500.pdf

EXTERNAL EMAIL - This email was sent by a person from outside your organization. Exercise caution when clicking links, opening attachments or taking further action, before validating its authenticity.

Secured by Check Point

Good morning Deepak,

Issue: Laboratory QC is scheduled for soil and water ICP-AES Metals analysis, but no samples were designated for QC. The laboratory would like to use samples MBHHA7, MBHHA8, and MBHHA9 for laboratory QC. The laboratory confirms that these samples are not blanks, rinsates, or PT samples.

Resolution: Per SOW SFAM01.1 Exhibit A, Section 5.5.4.1., please note the issue in the SDG Narrative and proceed with the analysis of the samples using the selected samples for QC.

Please note that the laboratory may contact the appropriate CLP PM should any defects need to be waived for this issue.

Thanks,

Eric DeBerry

Associate Environmental Analyst
CLP QSS Coordinator – EPA Regions 1 & 3

Under contract to the EPA

T: (571) 833-5166
Eric.DeBerry@GDIT.com
15036 Conference Center Drive
Chantilly, VA 20151
www.gdit.com

GENERAL DYNAMICS
Information Technology

From: Deepak Parmar <Deepak.Parmar@alliancetg.com>
Sent: Thursday, February 6, 2025 10:14 AM
To: DeBerry, Eric <Eric.Deberry@gdit.com>

Cc: Sohil Jodhani <Sohil.Jodhani@AllianceTG.com>

Subject: Region 3 | Case 51979 | Lab ACE | Issue Discrepancies with tags, jars, and/or COC/QC

This Message Is From an External Sender

Please use caution with links, attachments, and any requests for credentials.

Good morning,


Issue 1: QC Scheduled for soil and water for ICP-AES METALS analysis However, a sample was not designated for Laboratory QC. Lab like to use sample MBHHA7,MBHHA8 and MBHHA9 for Lab QC. these samples is not blanks, rinsates or PT.


Please see attachment for your reference.


Thanks & Regards,





Deepak Parmar
QA/QC
An Alliance Technical Group Company
Main: 908-789-8900
Direct: 908-728-3154
Address: 284 Sheffield St, Ste 1, Mountainside, NJ 07092
www.alliancetg.com    

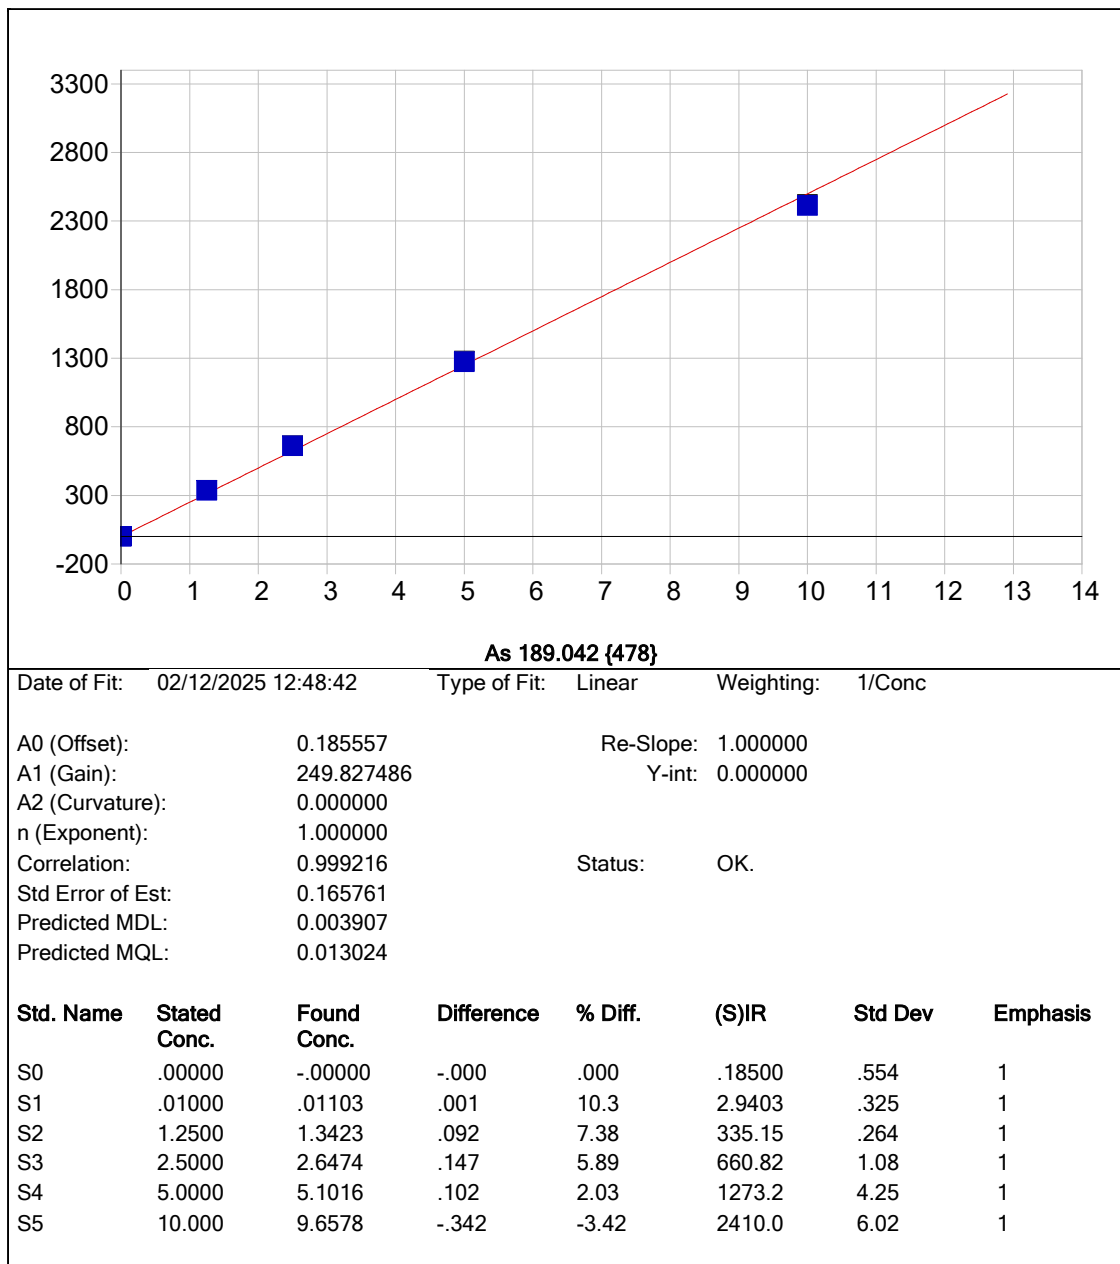


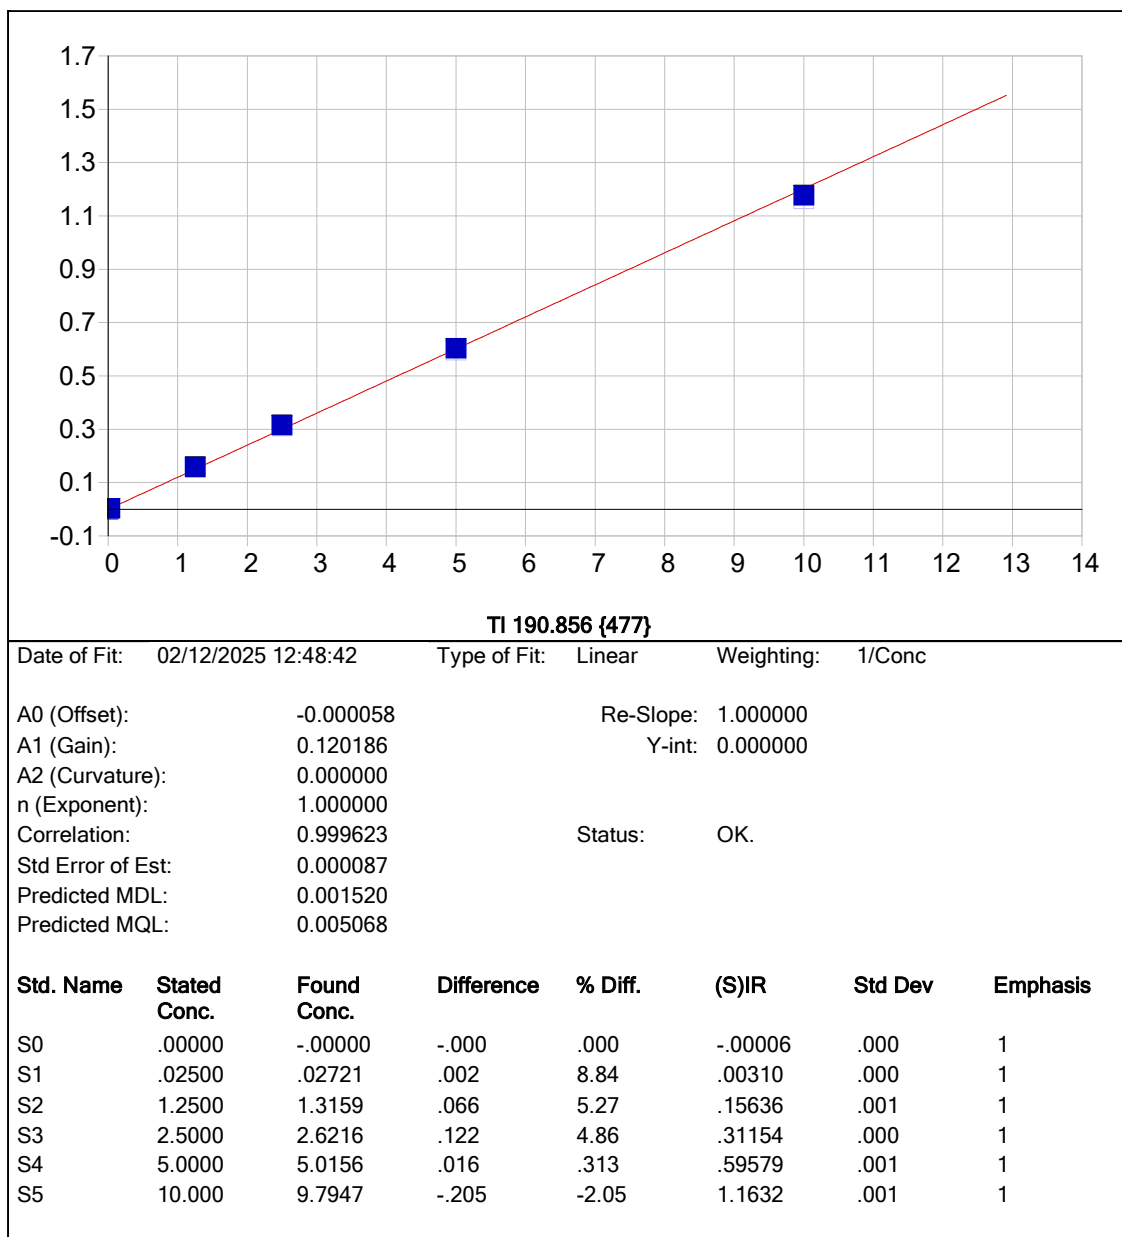


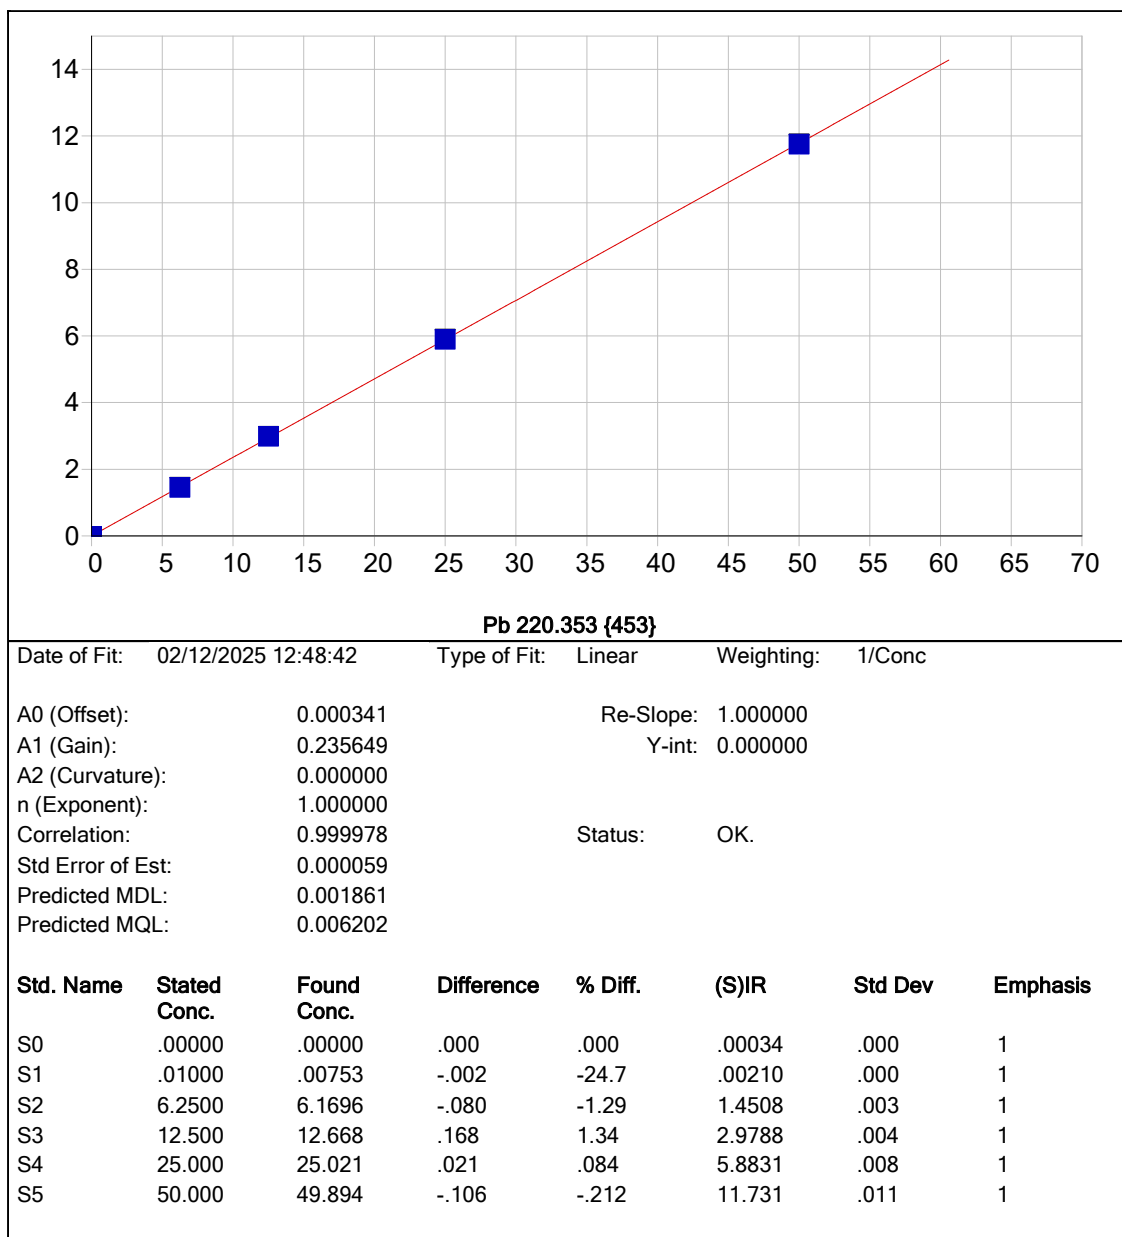


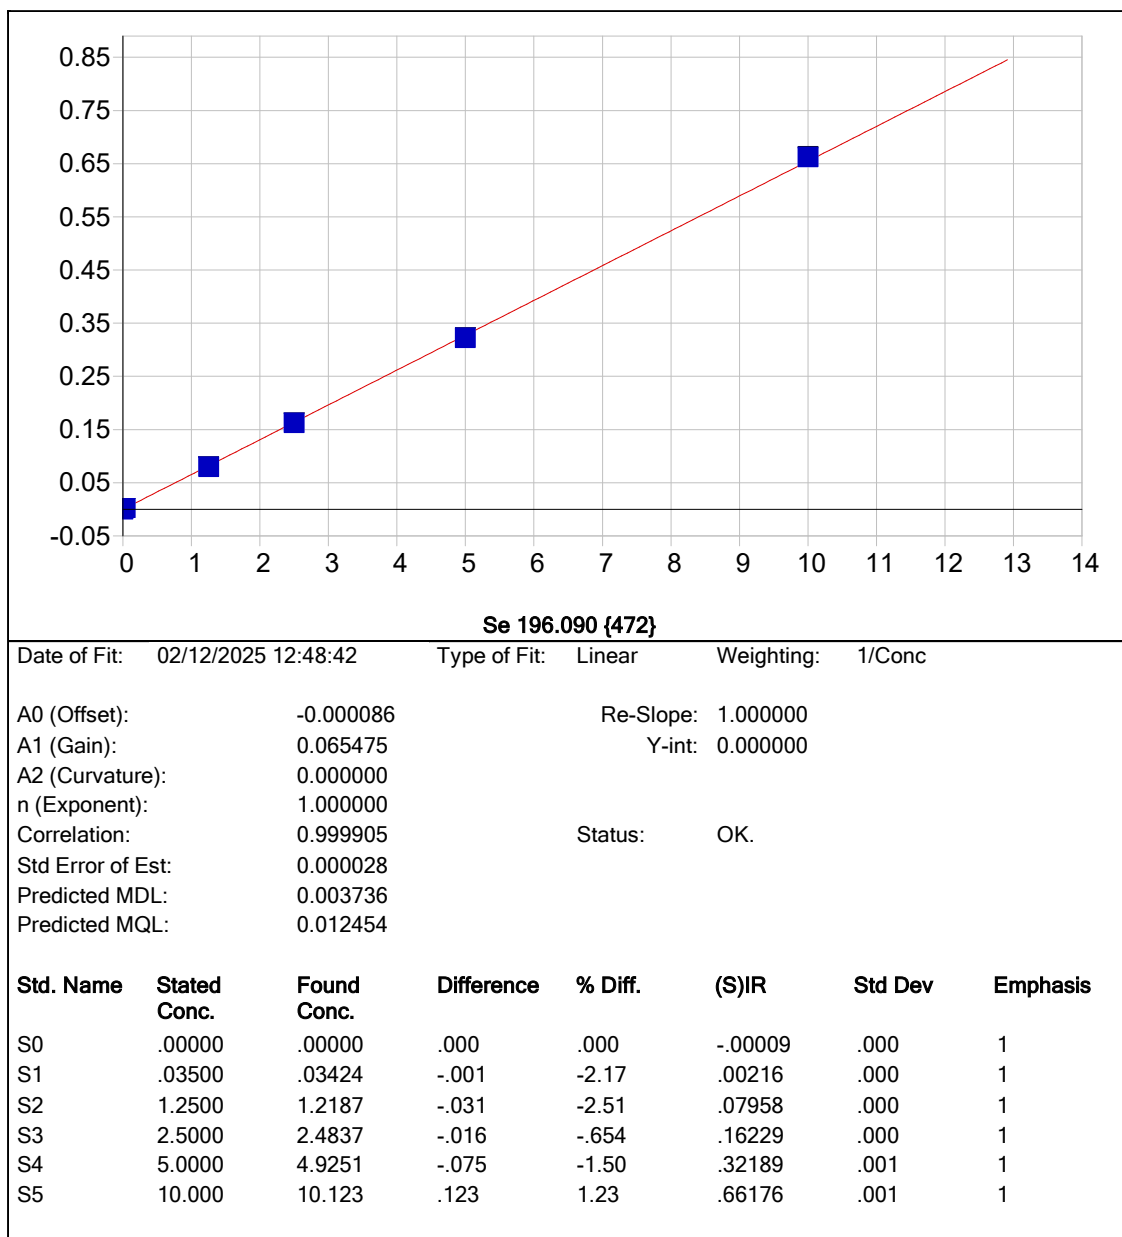


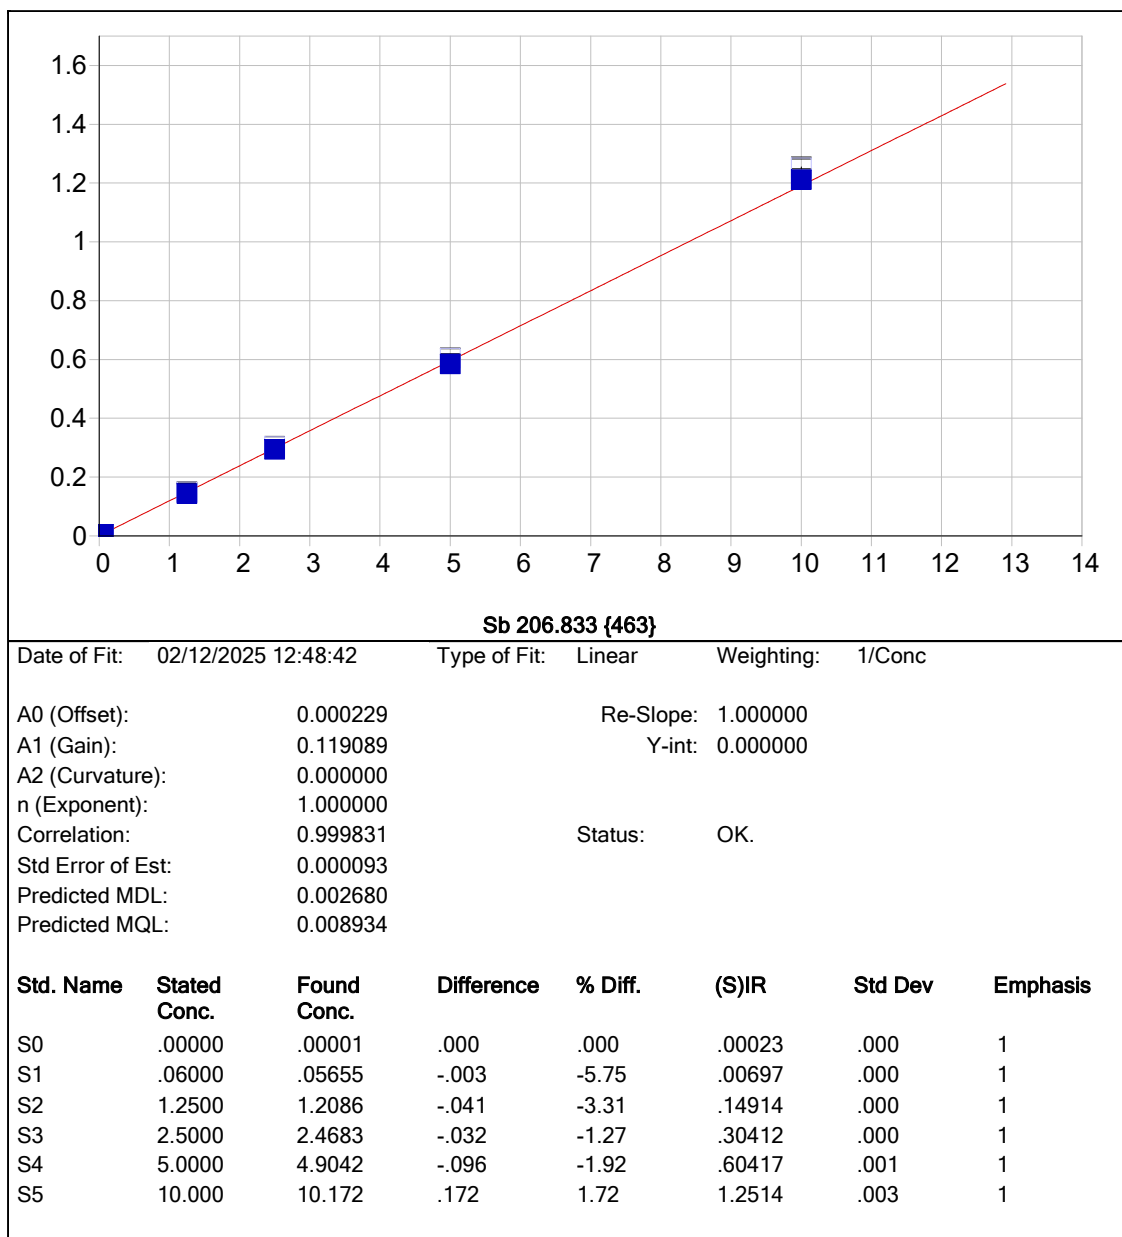


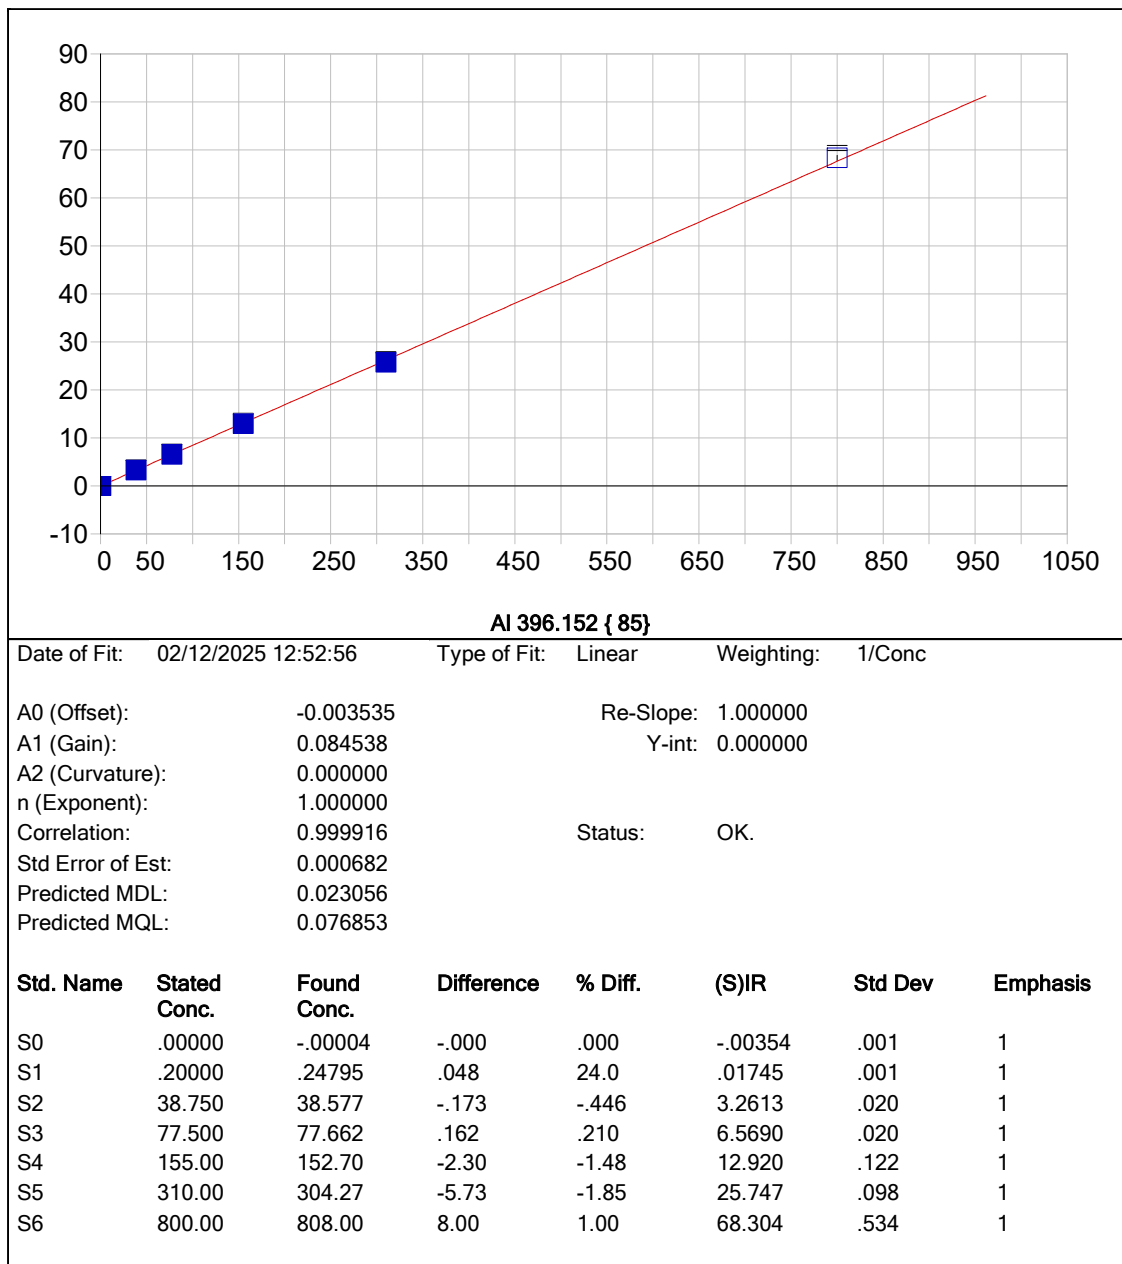


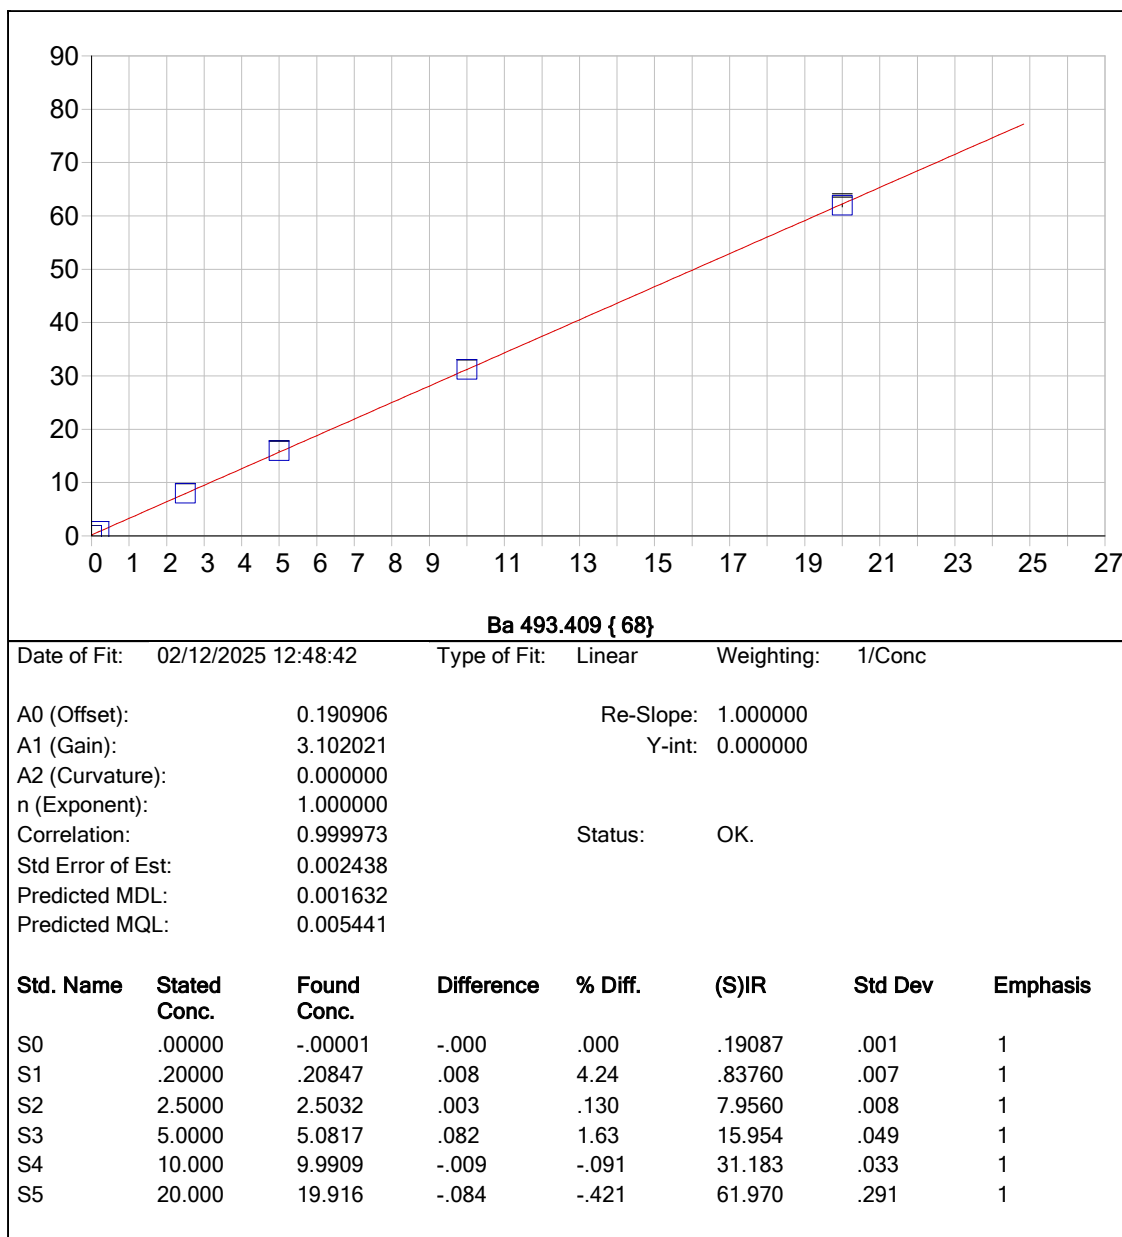


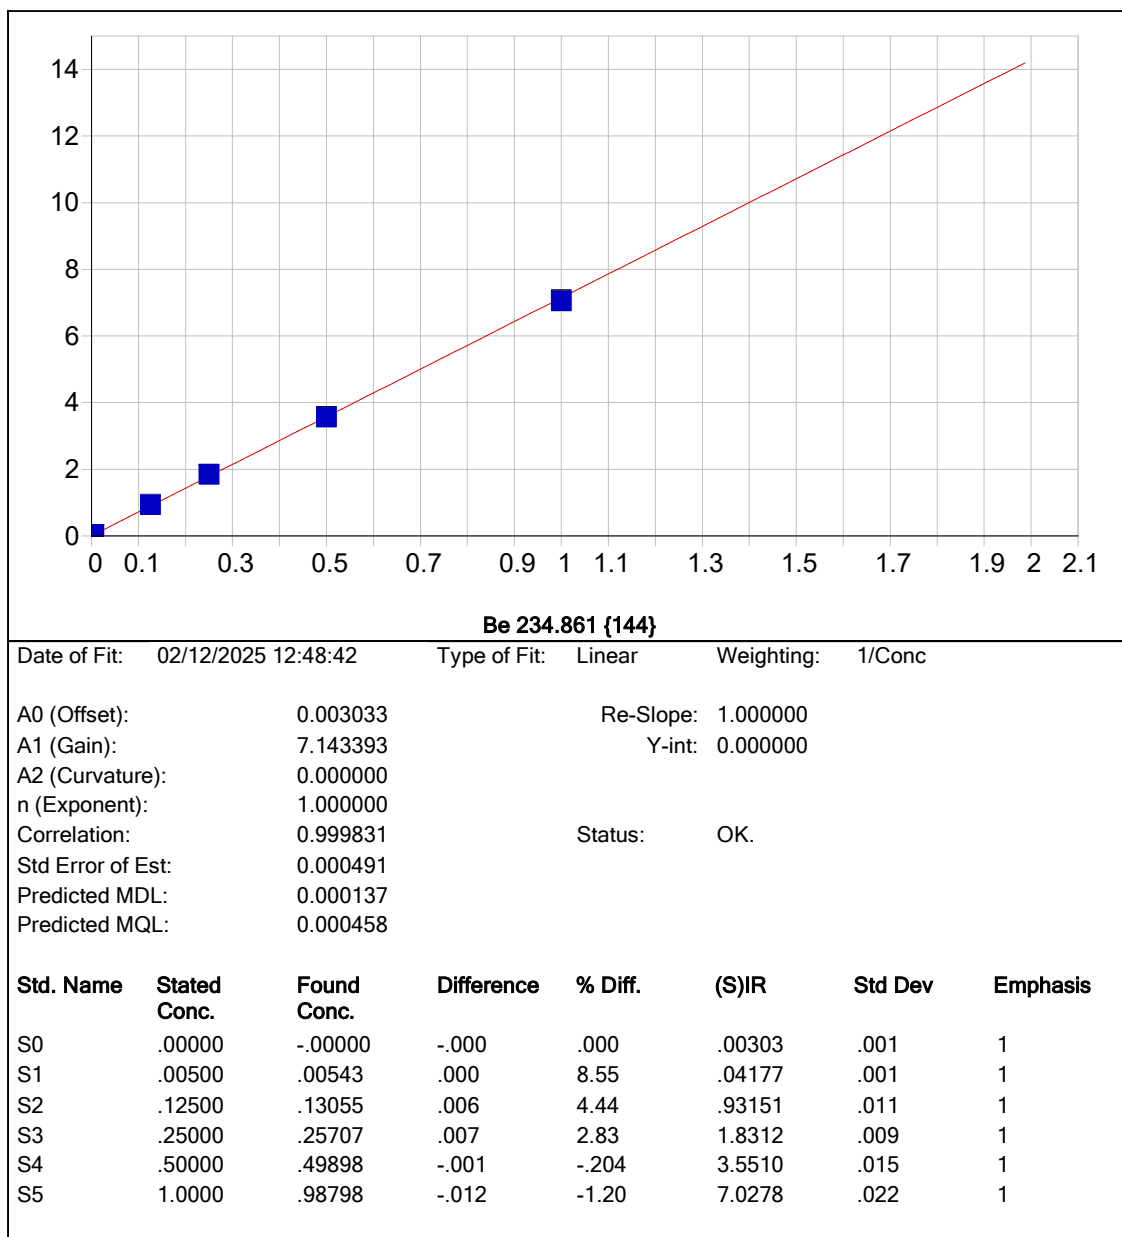


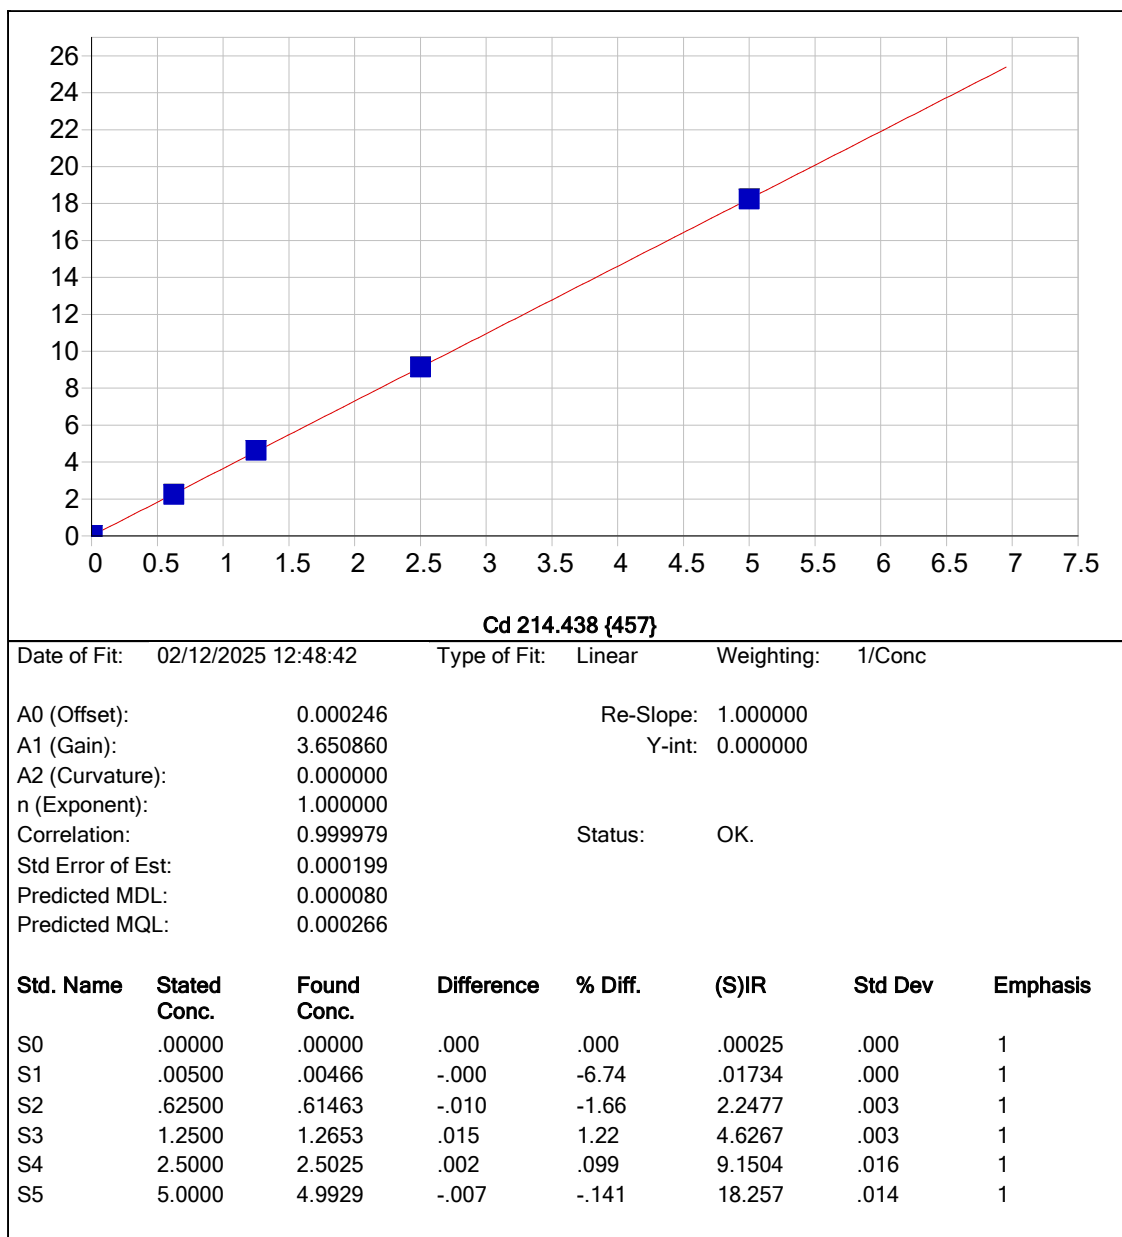


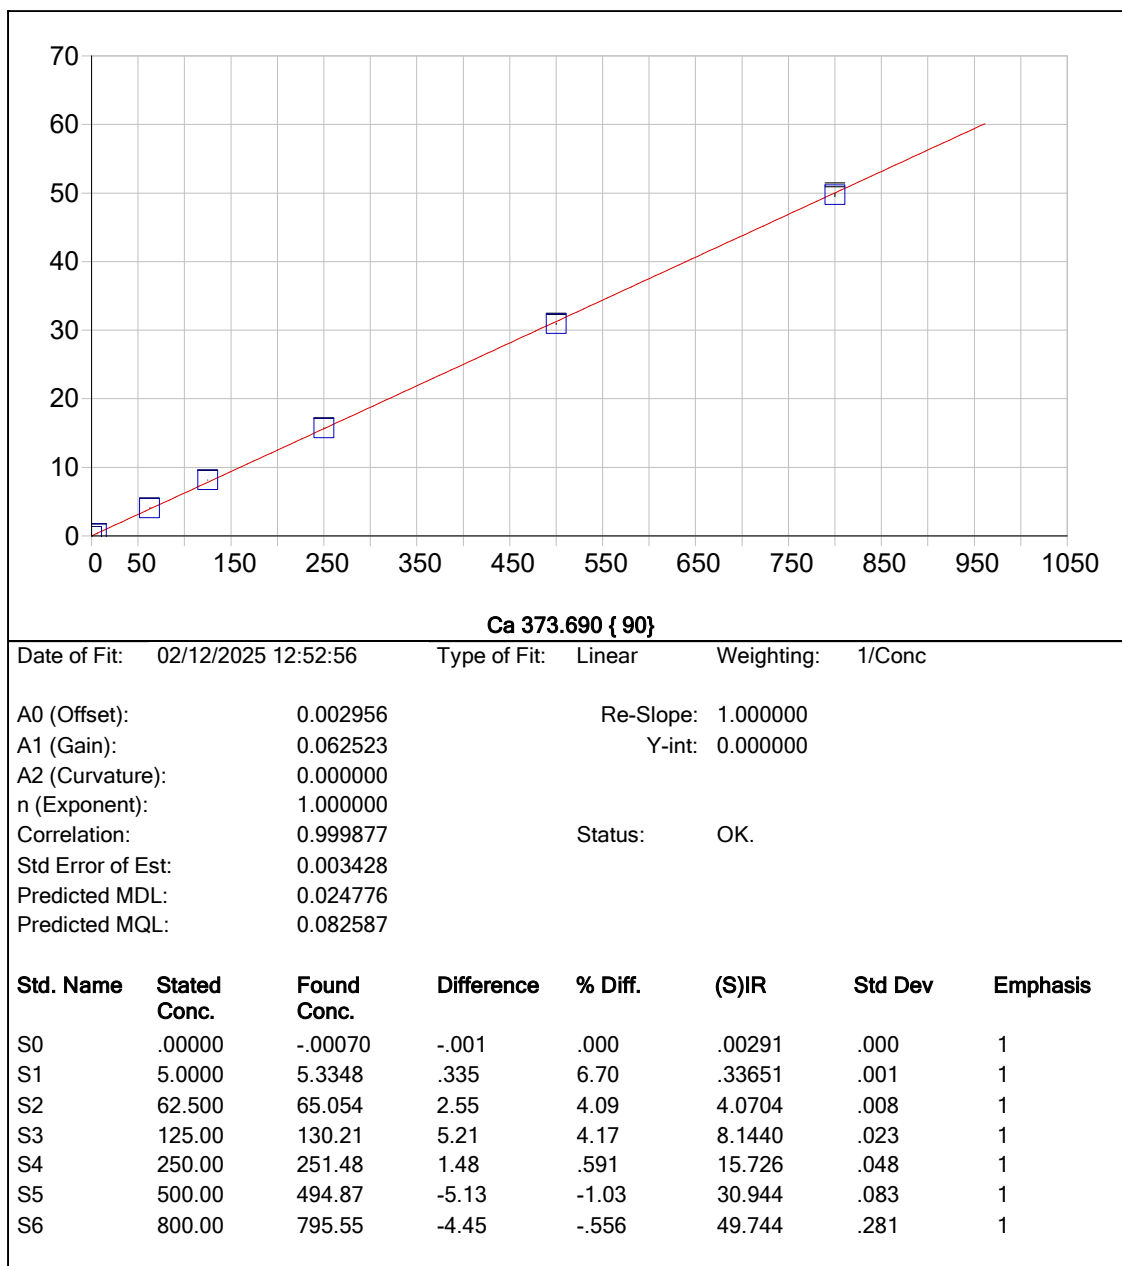


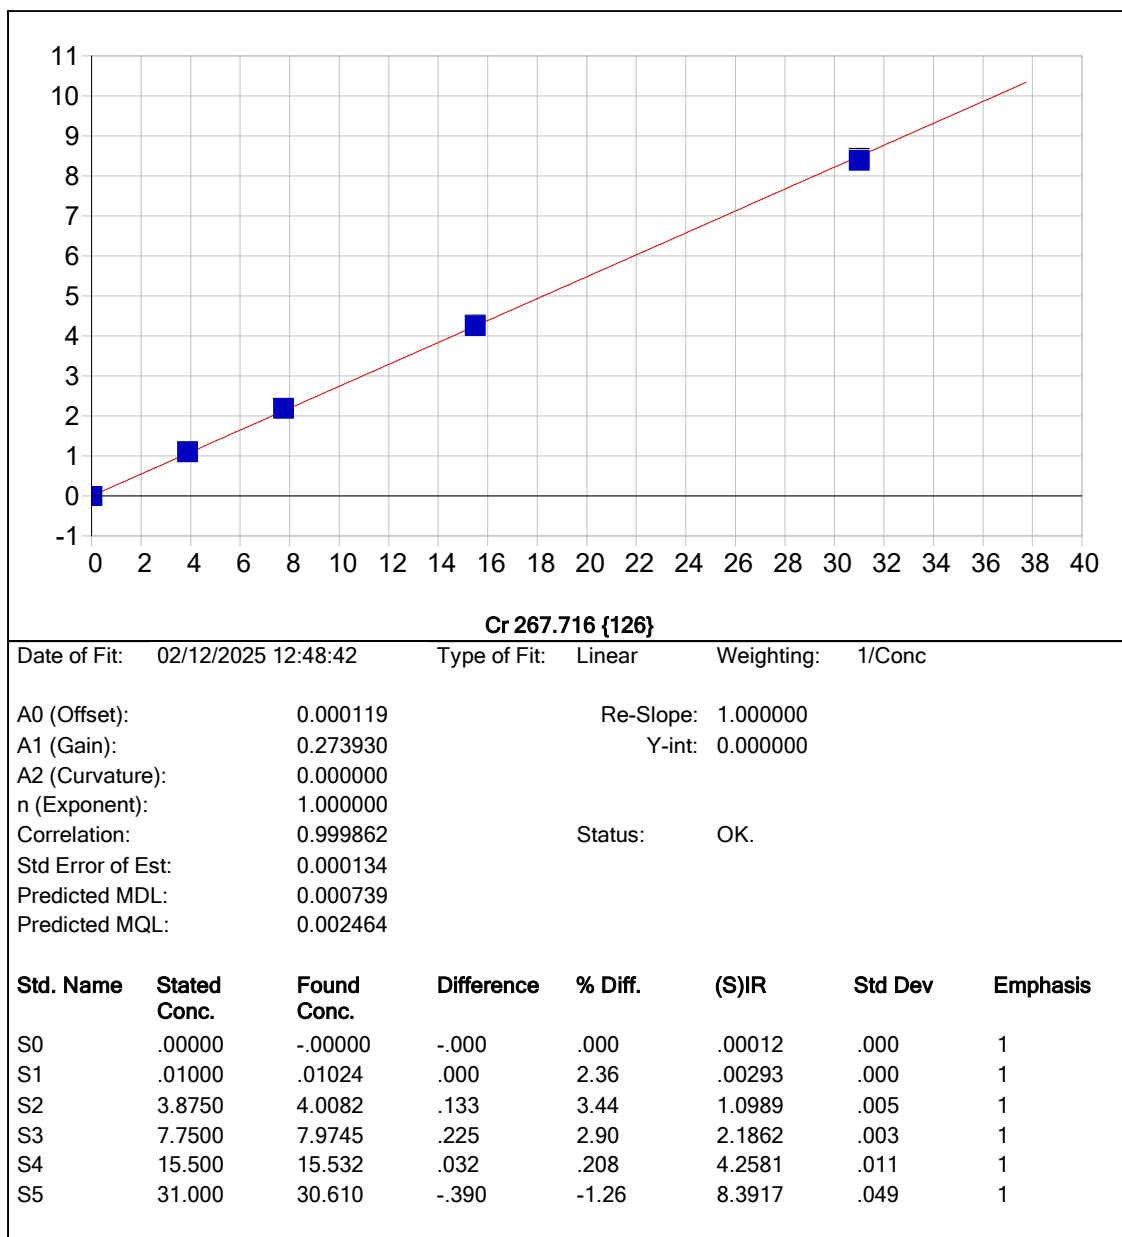


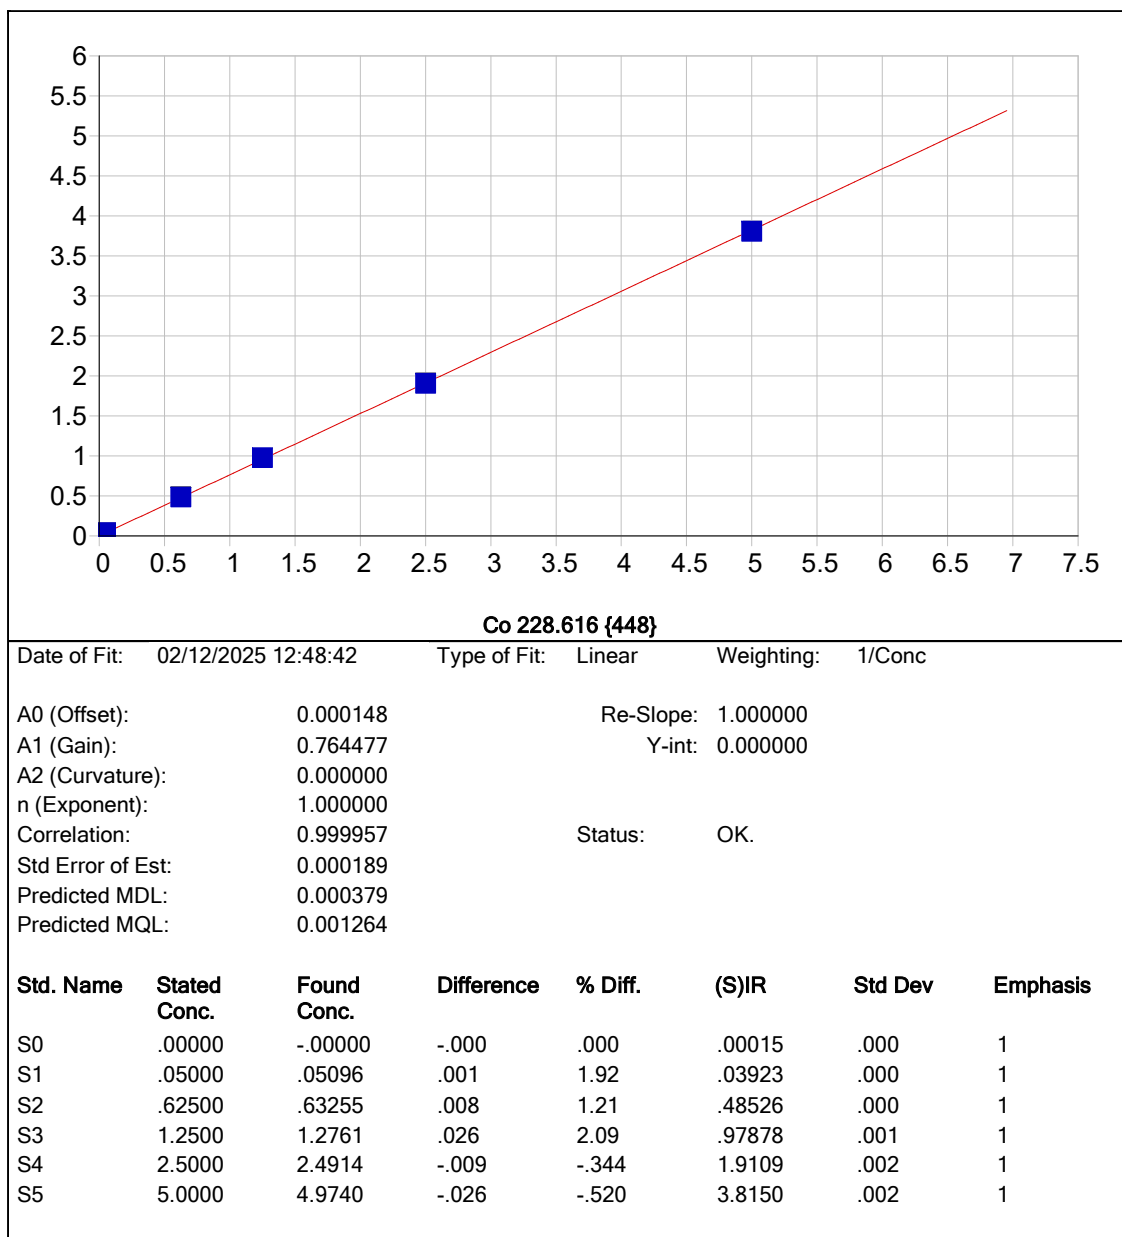


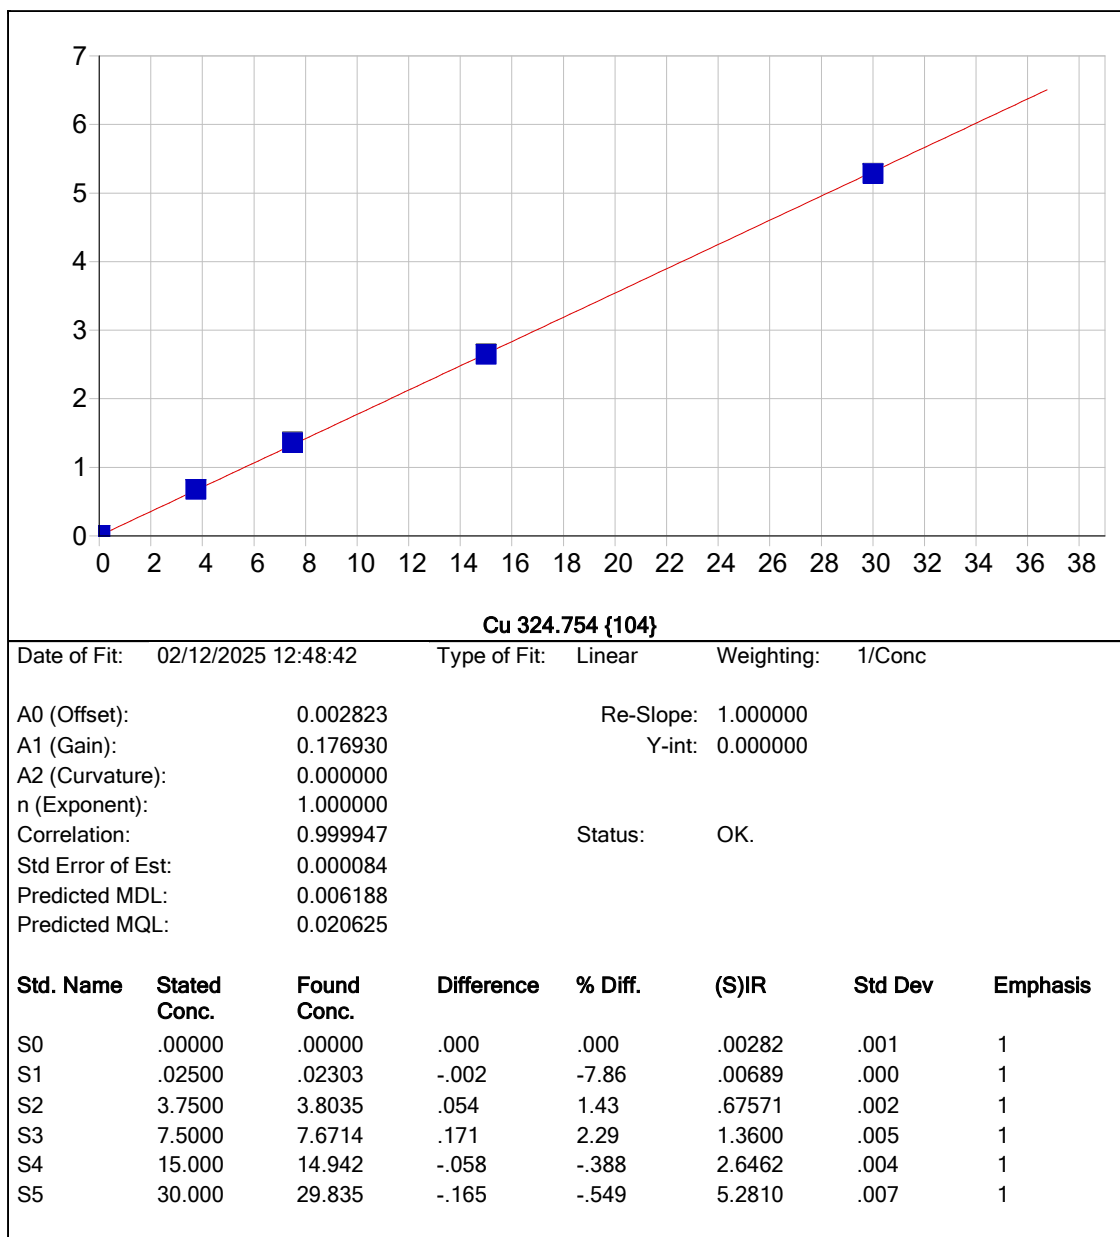


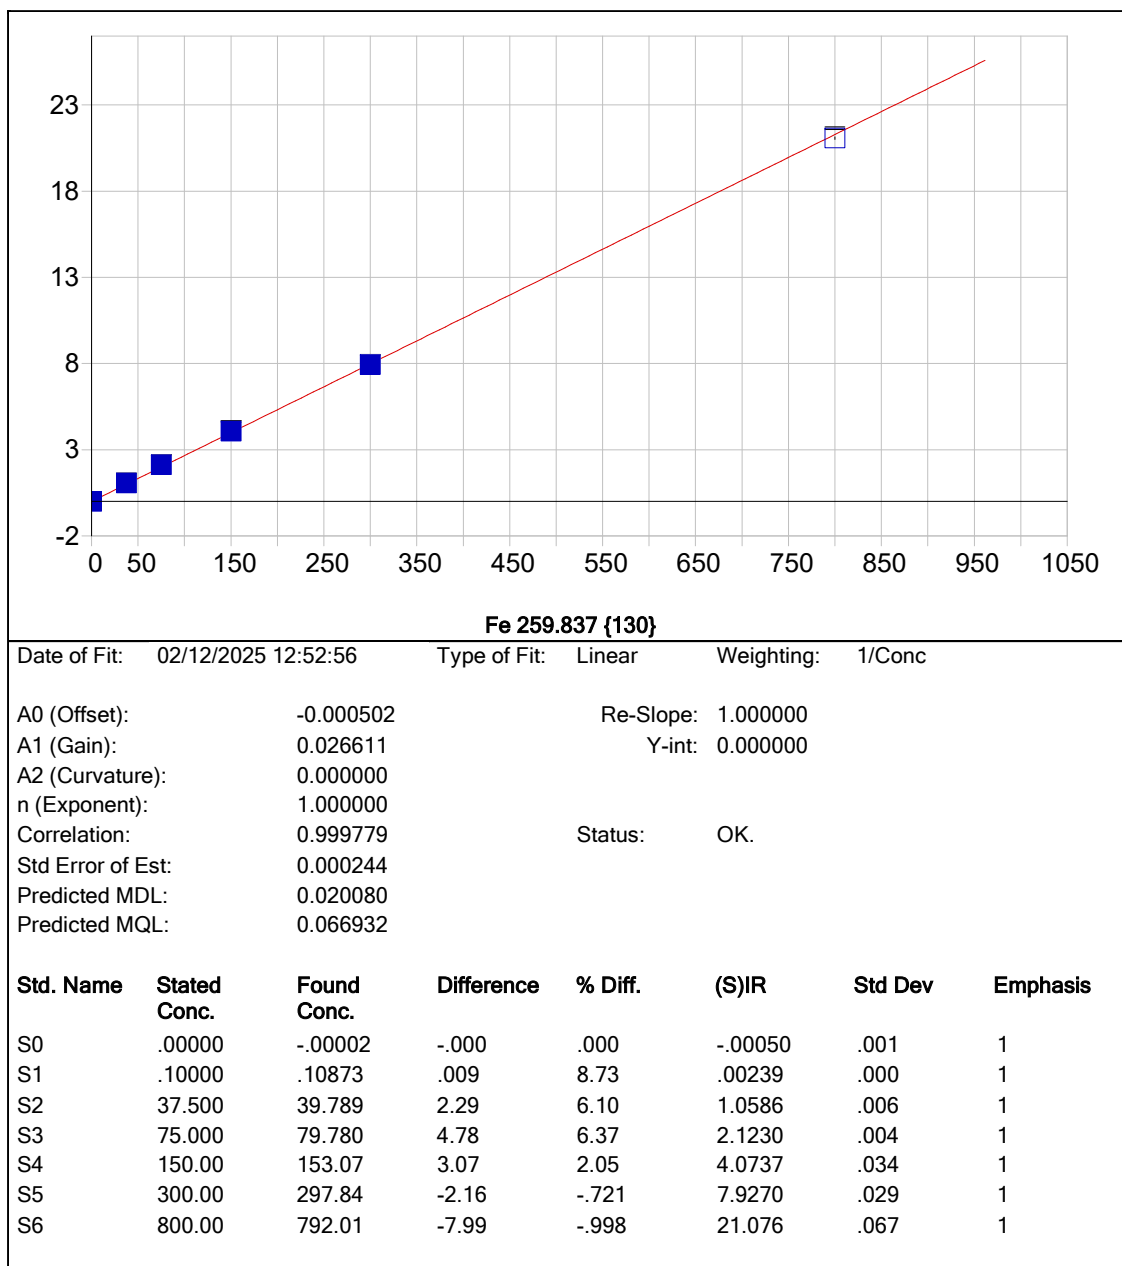


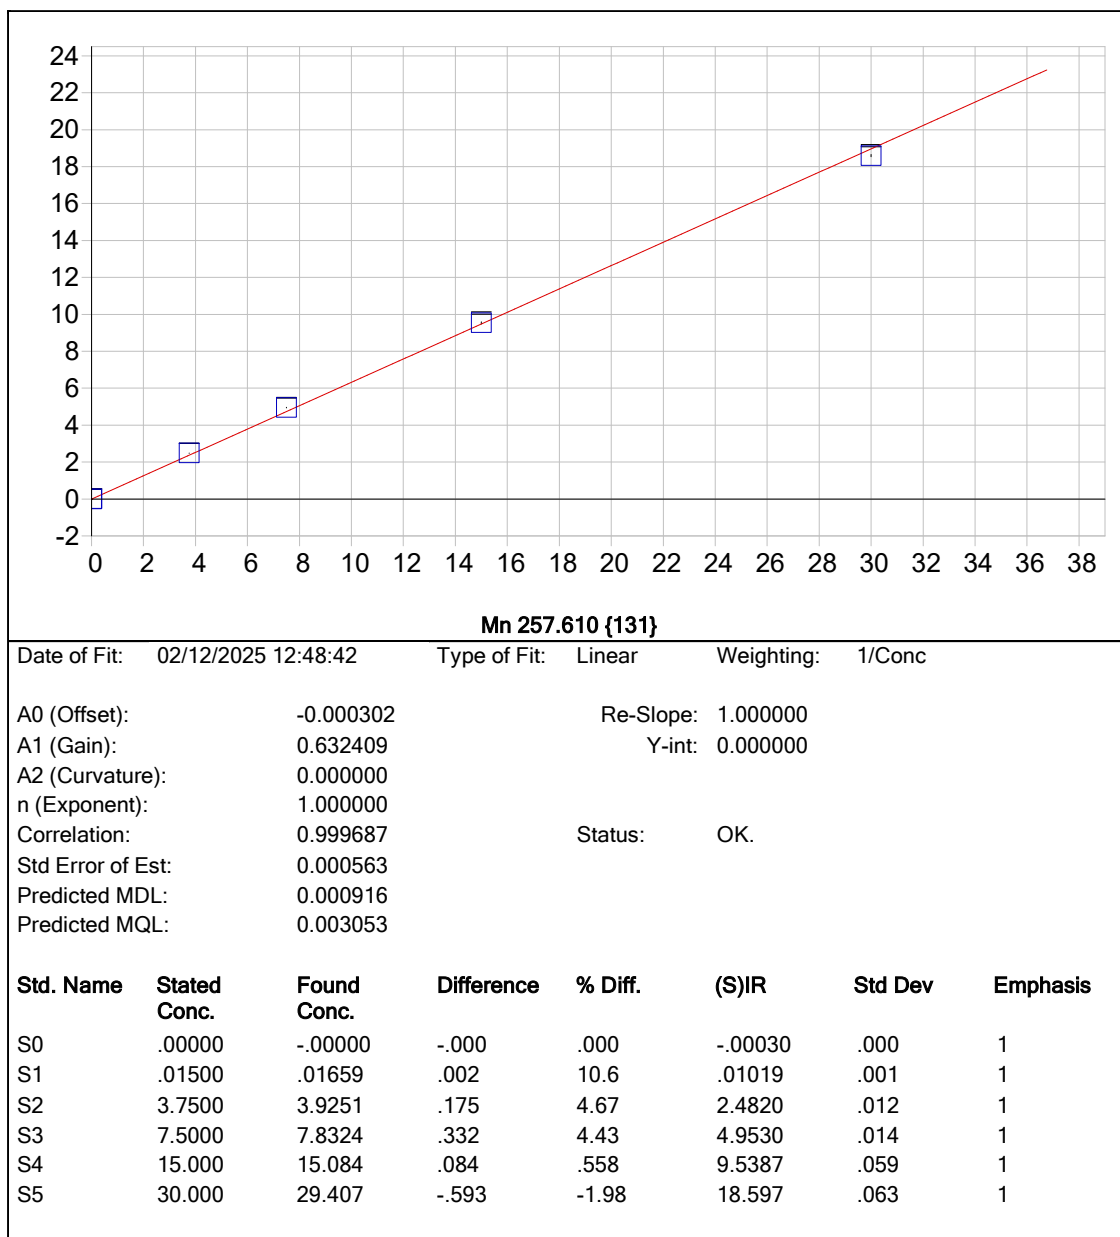


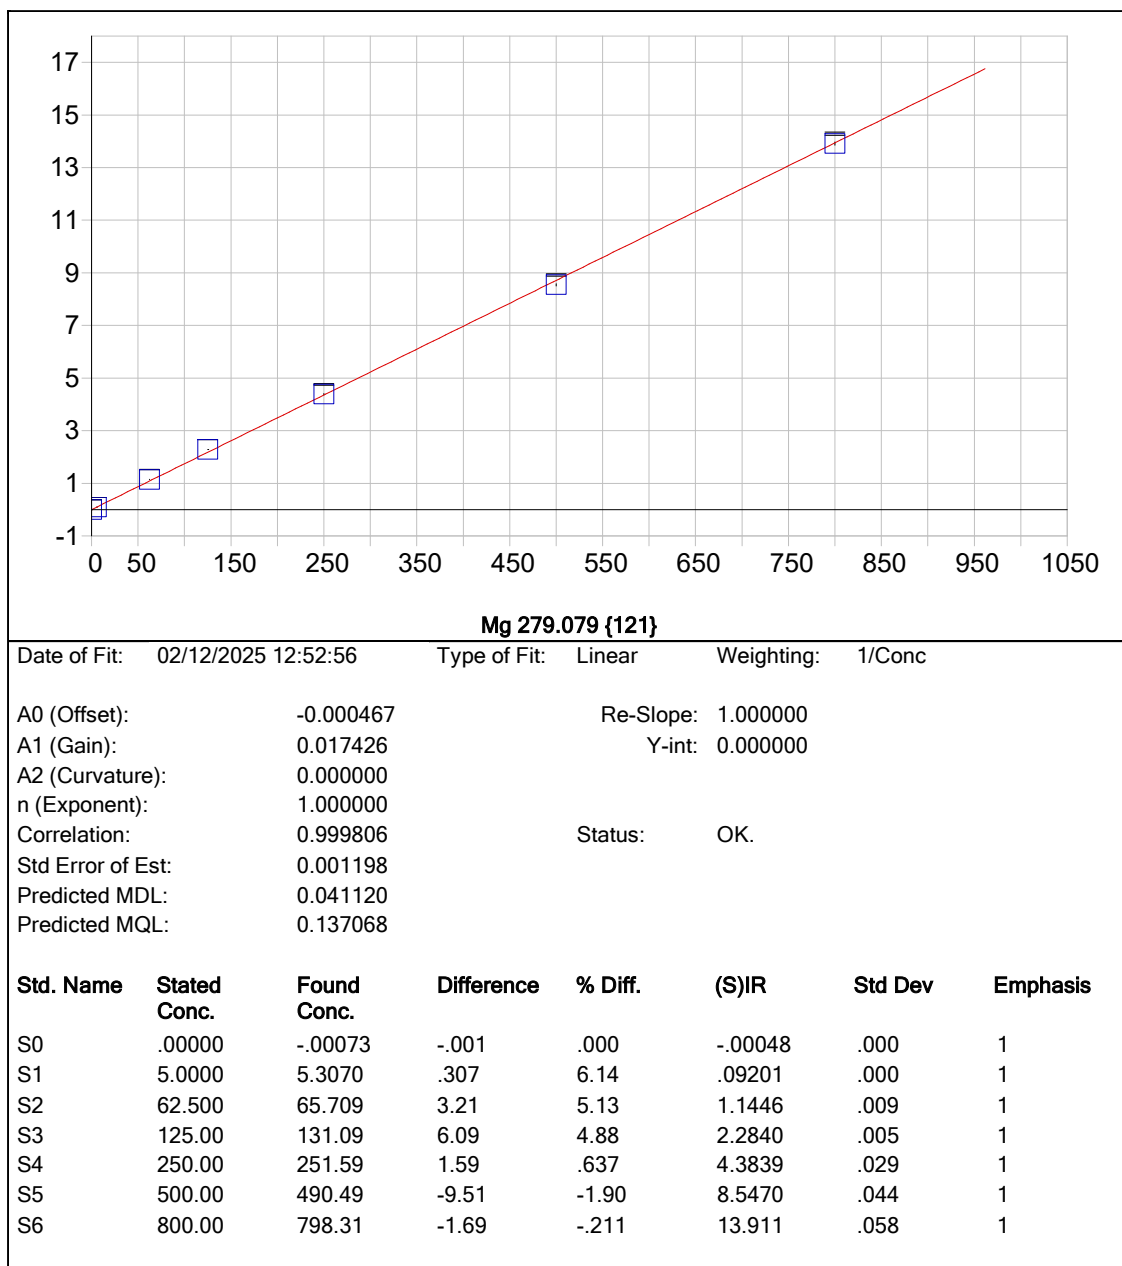


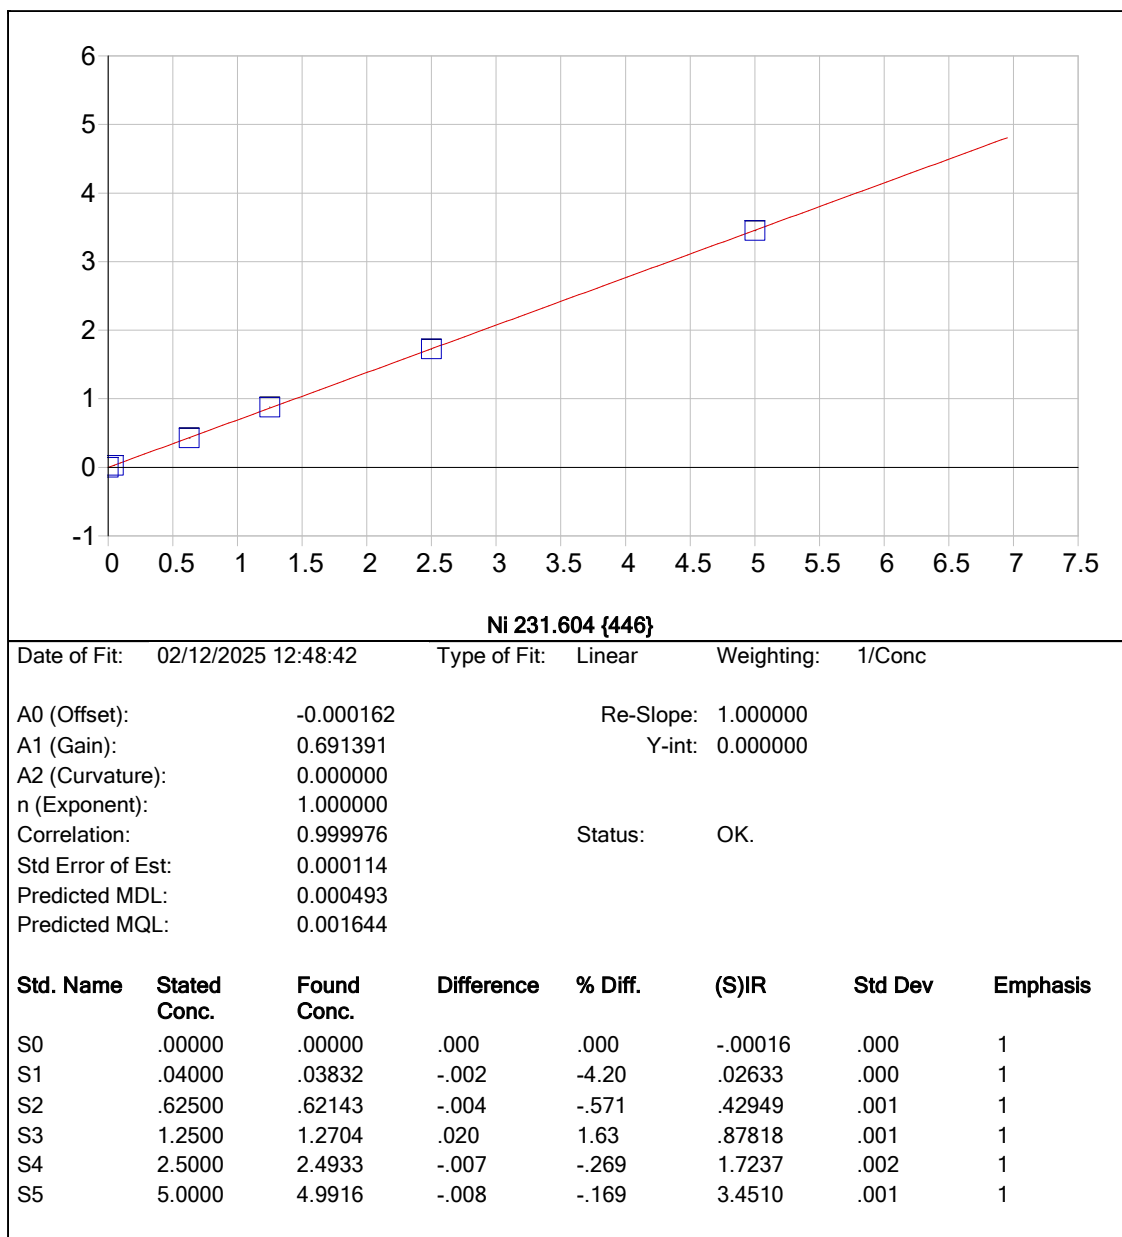


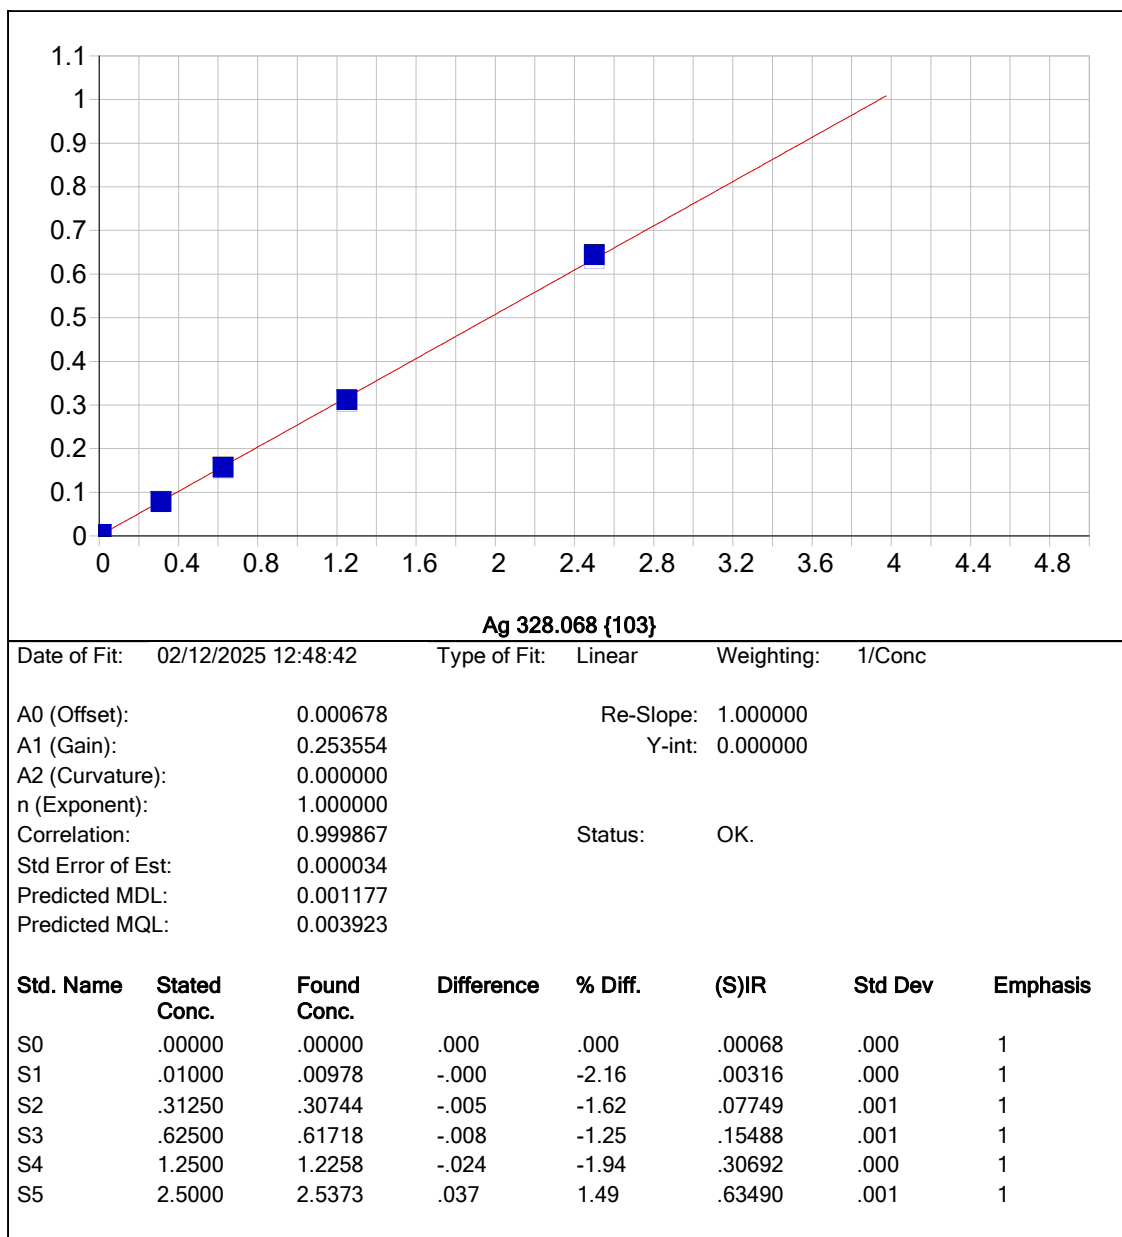


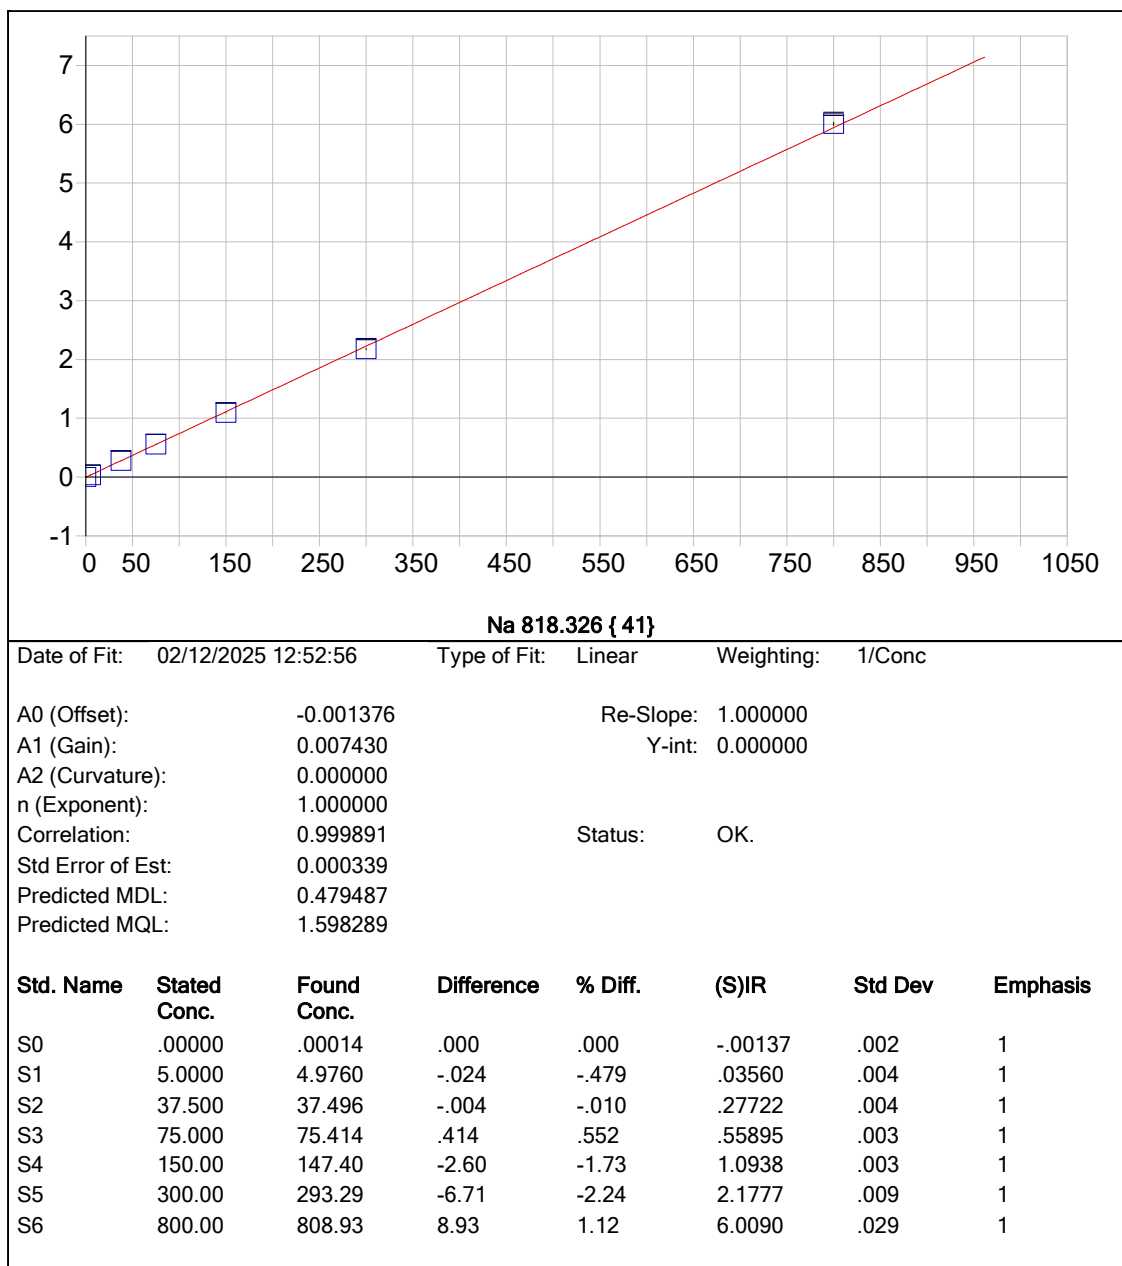


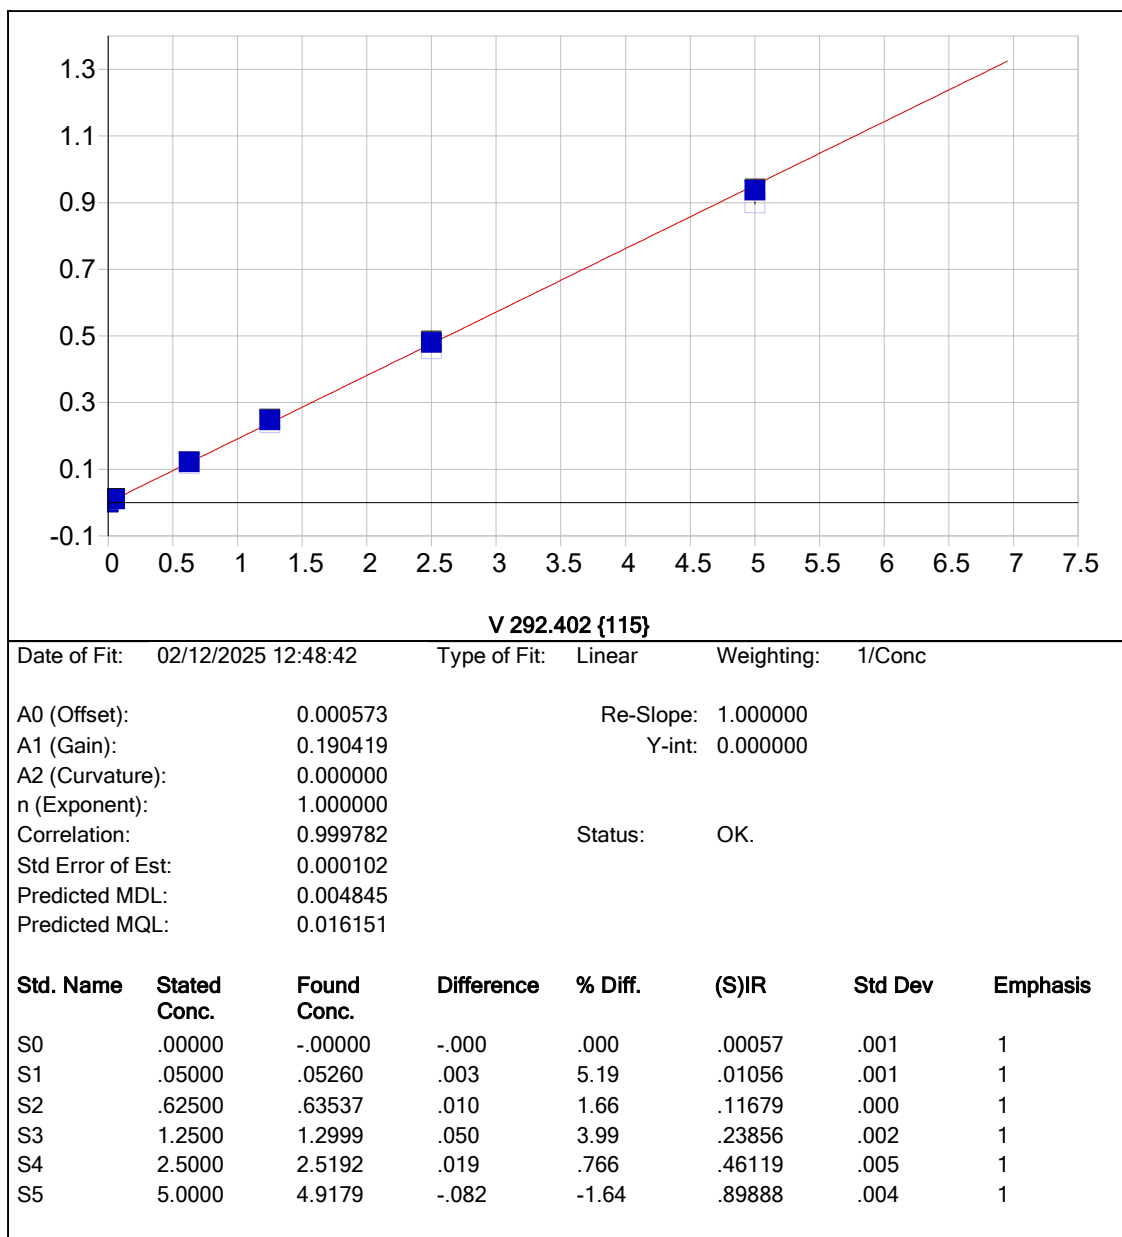


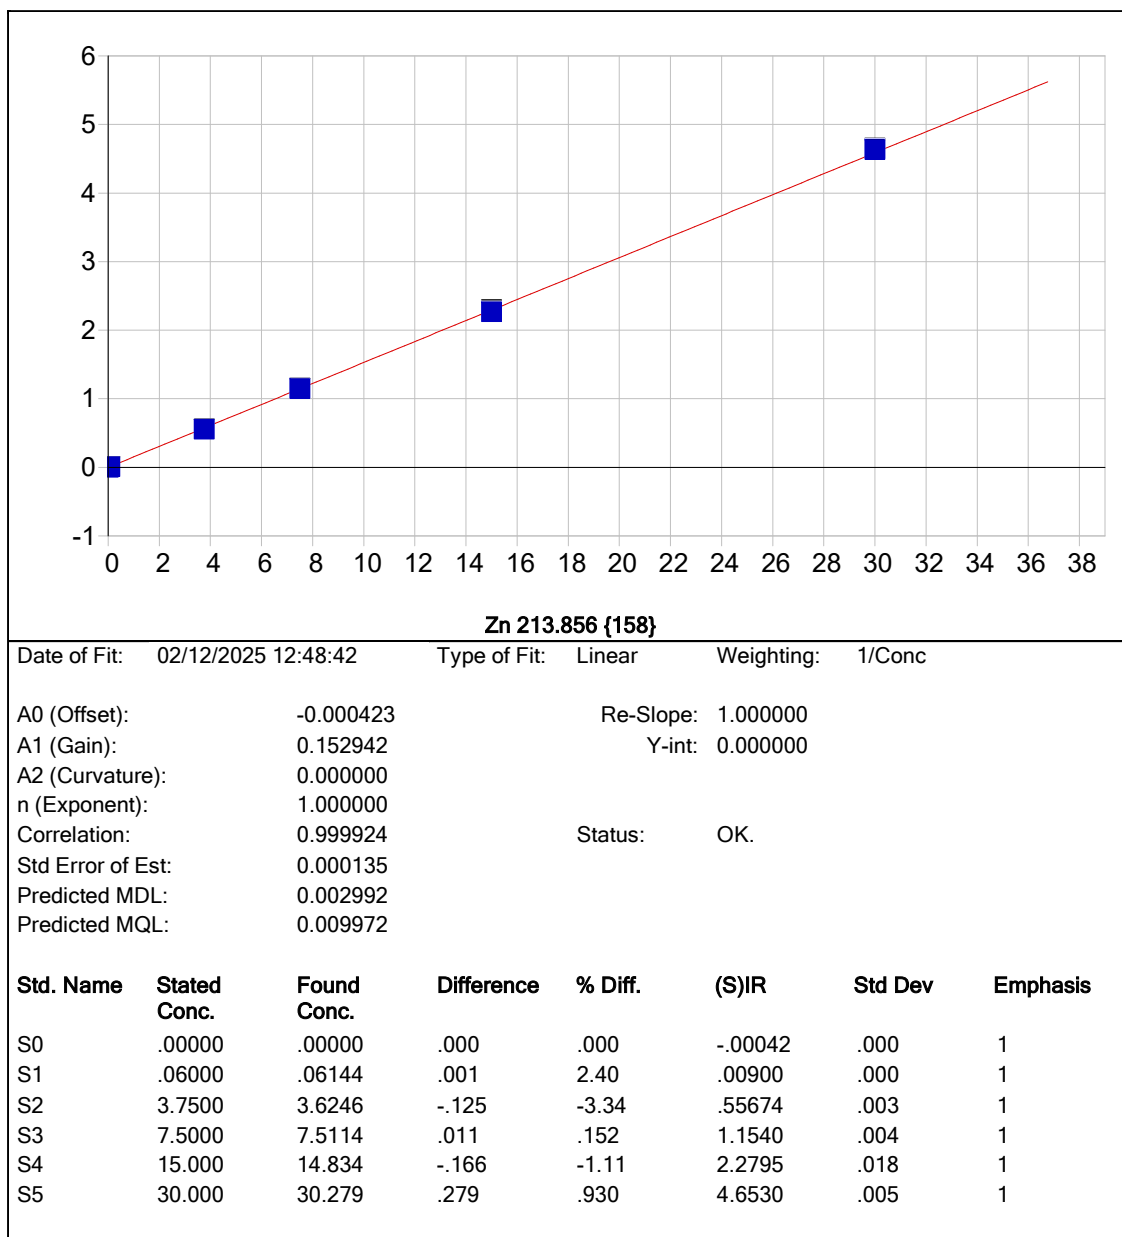


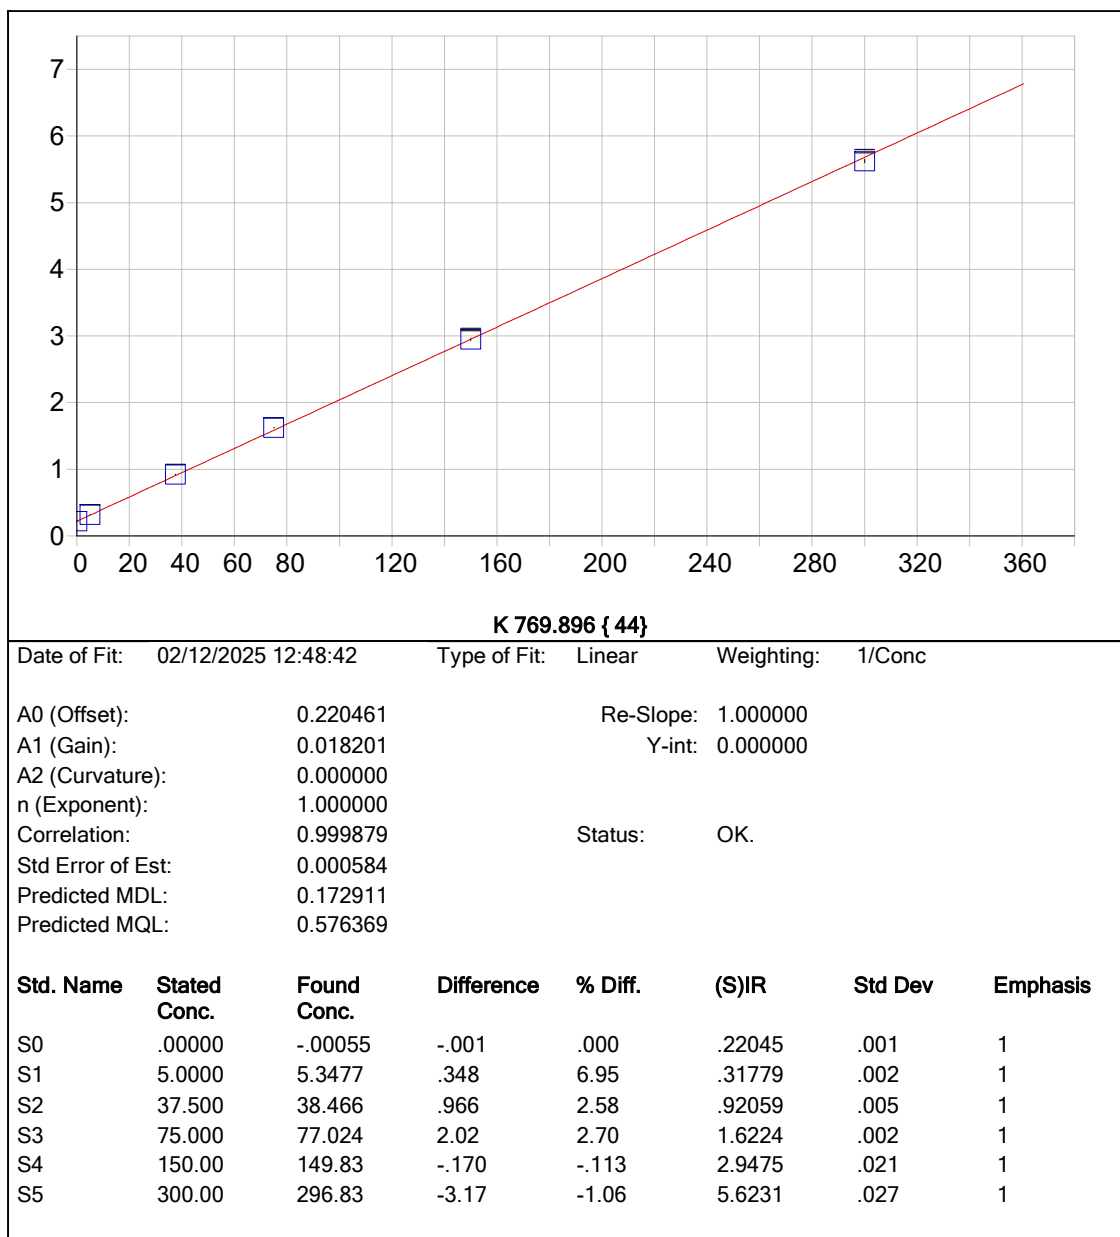


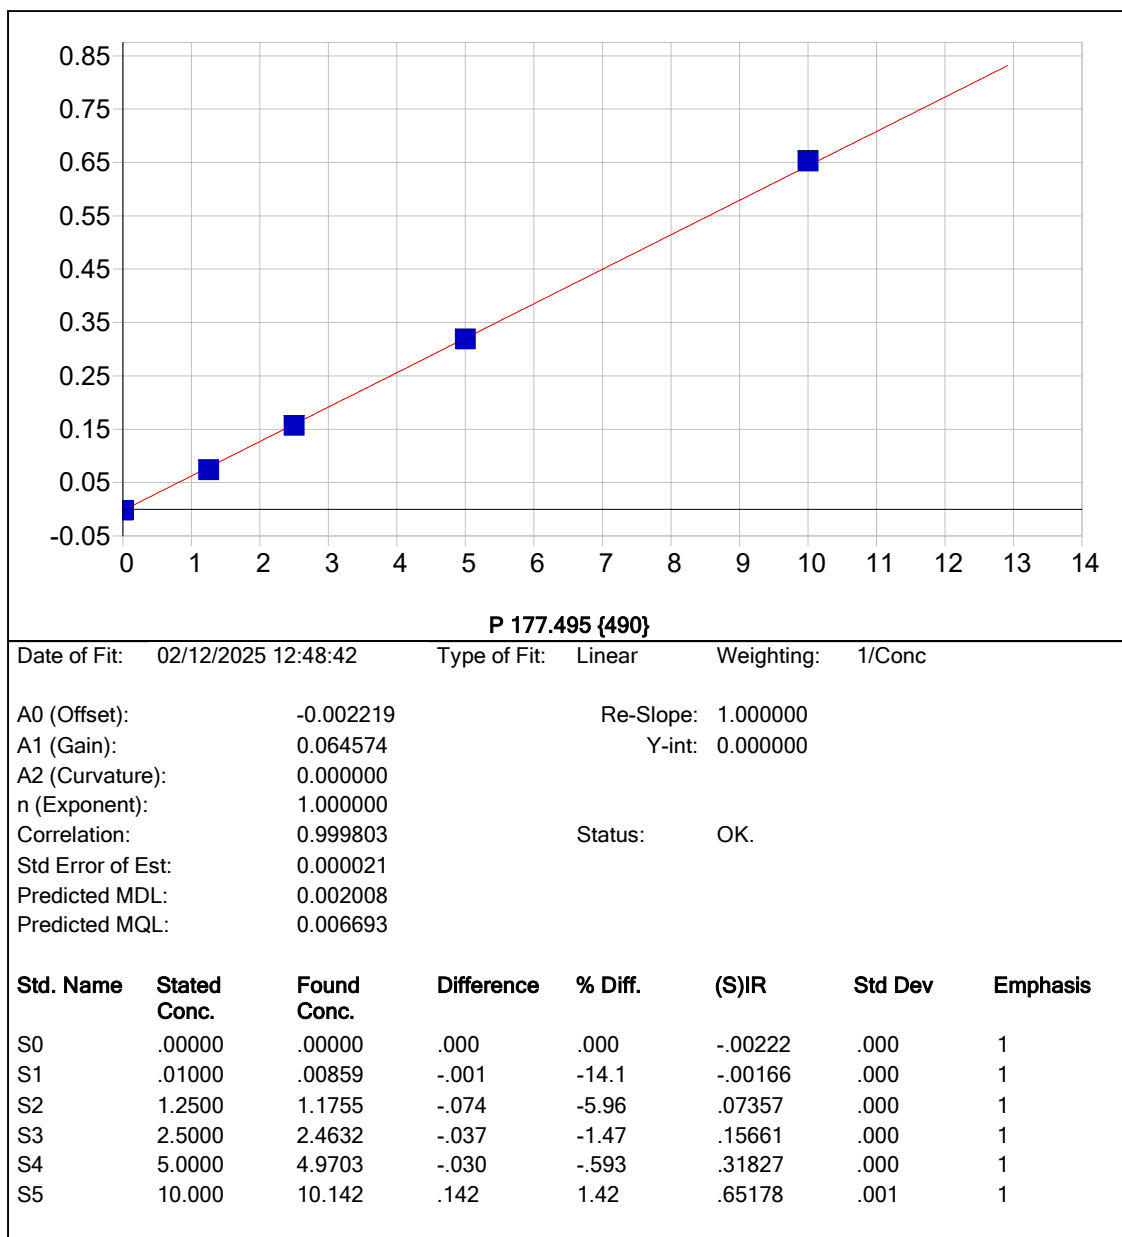


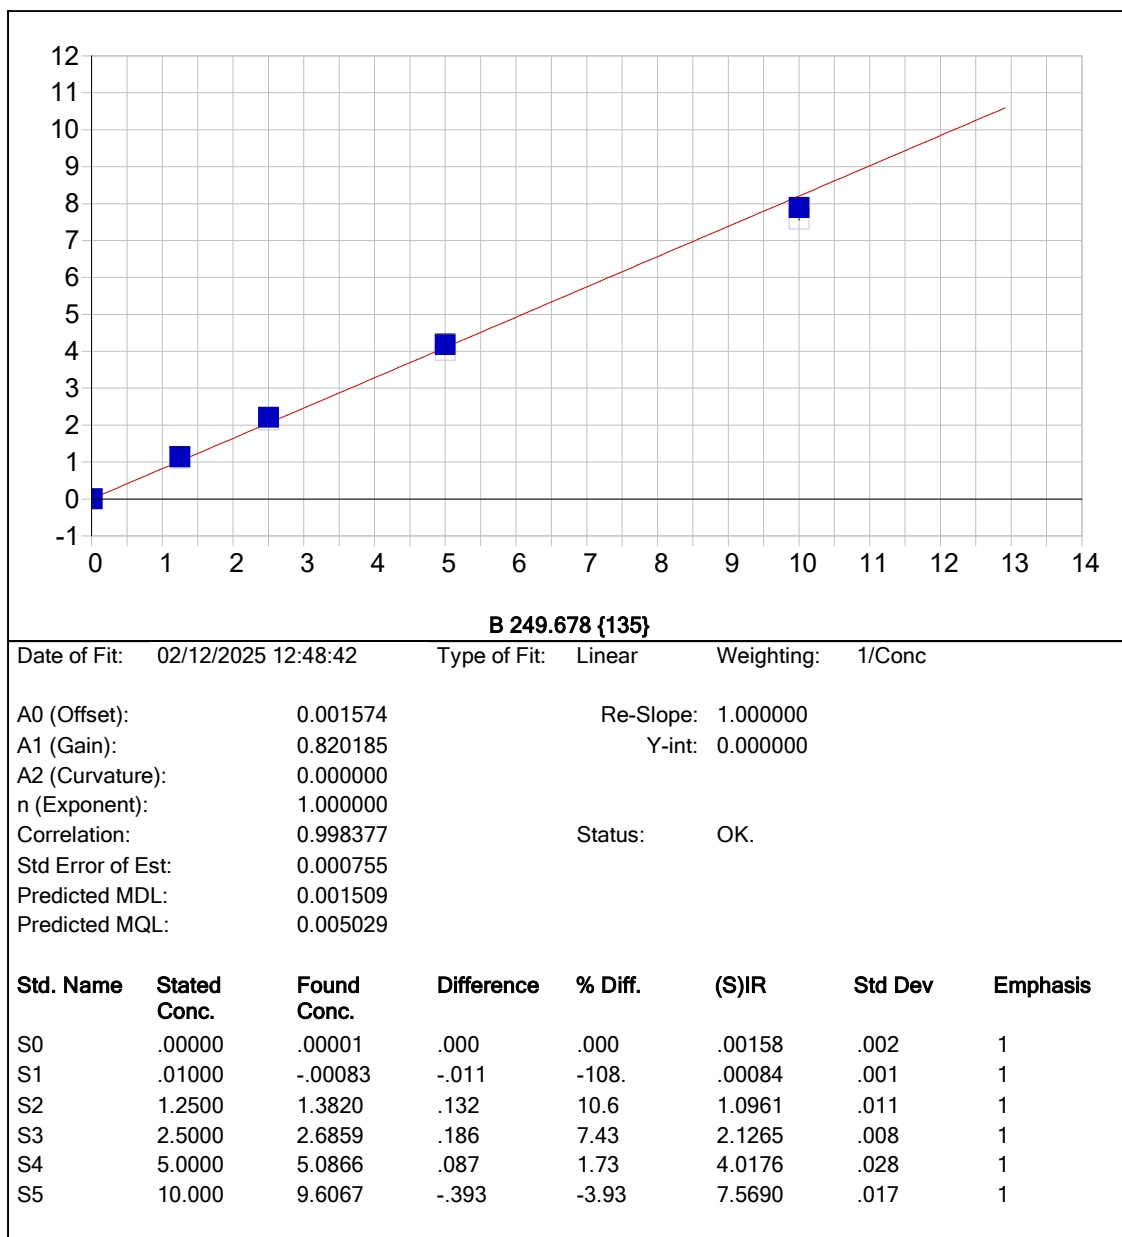


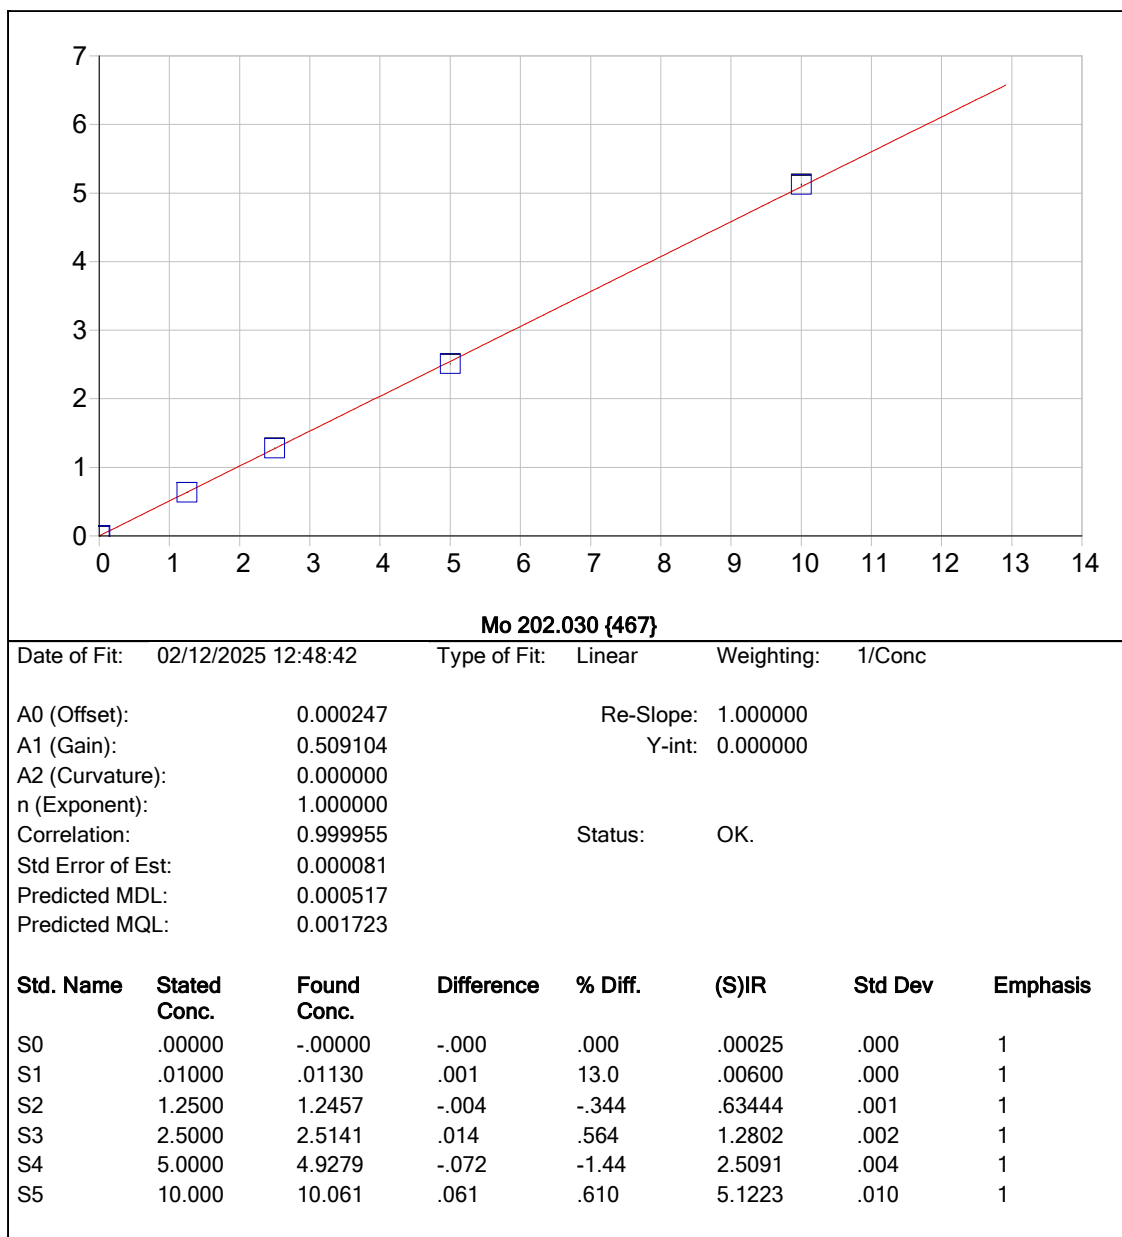


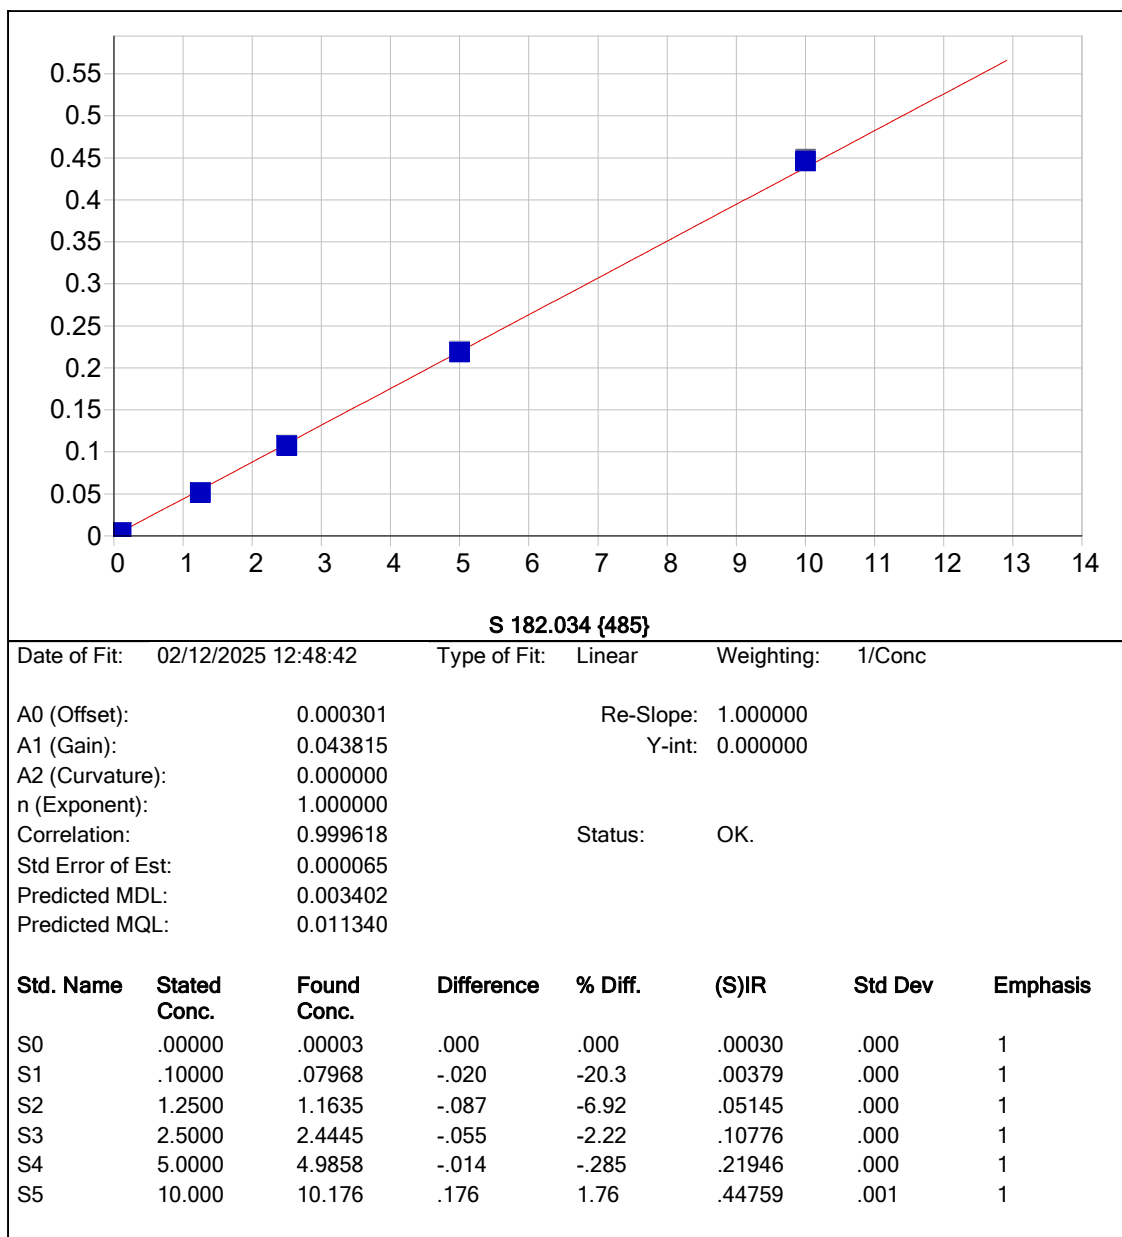


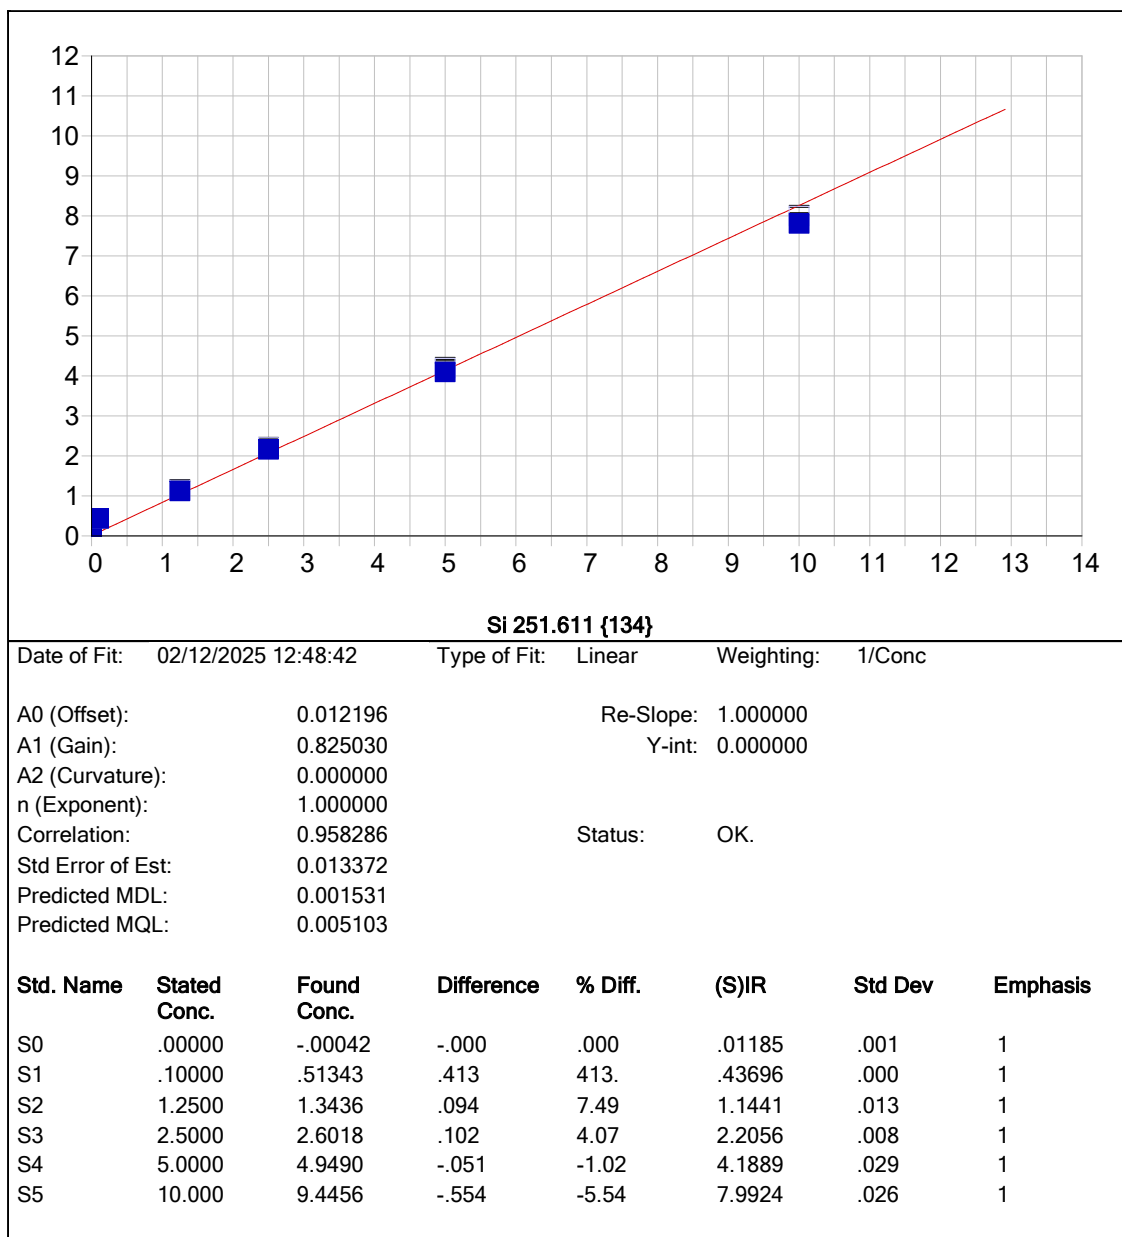


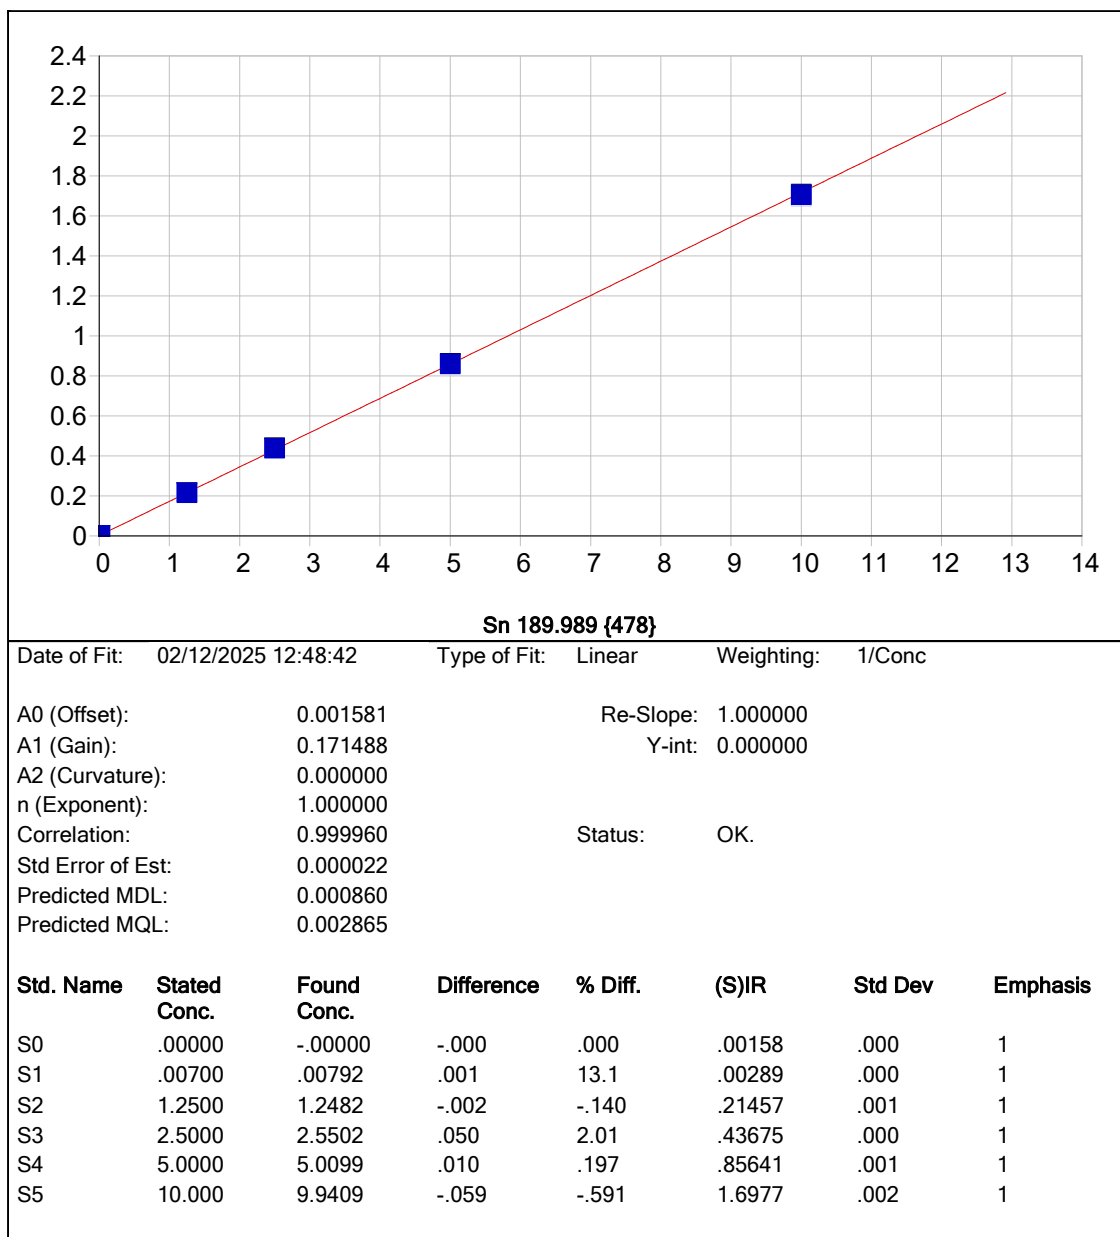


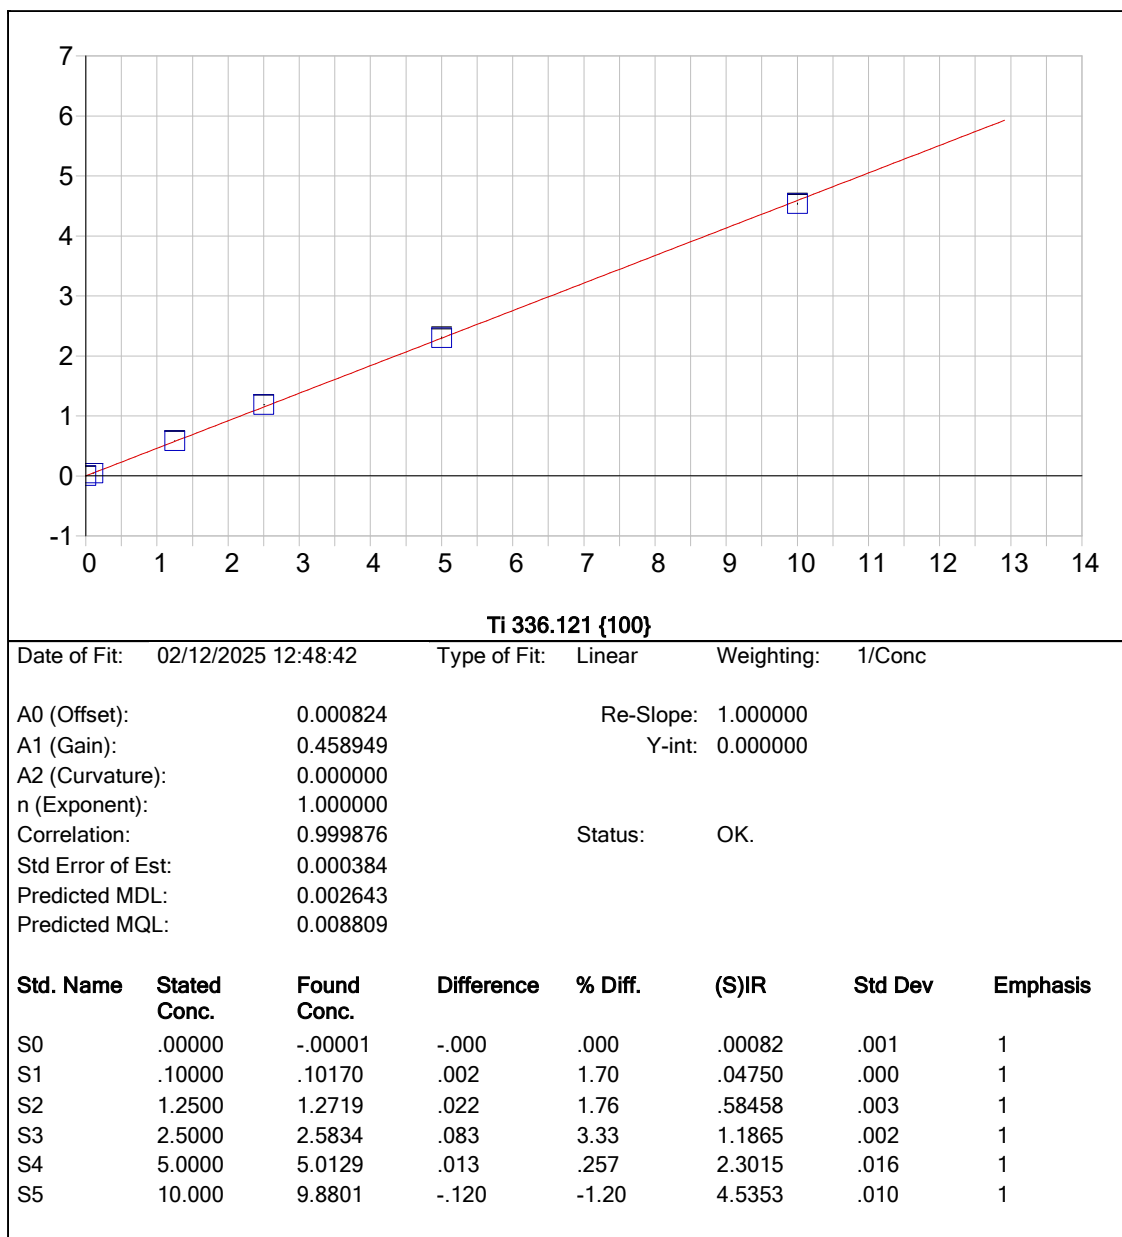


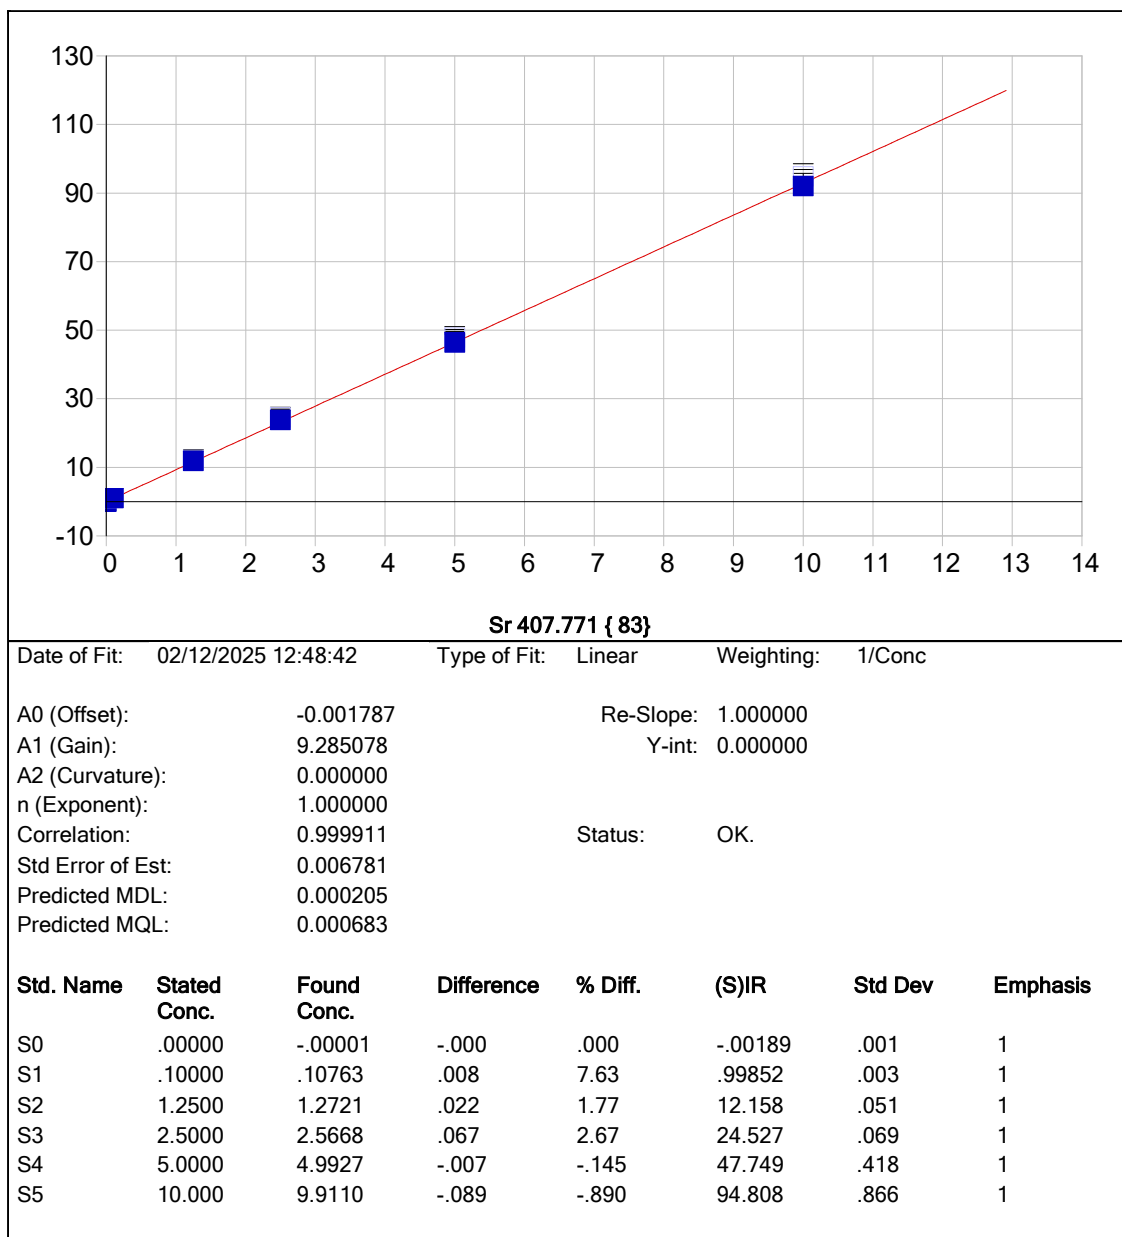

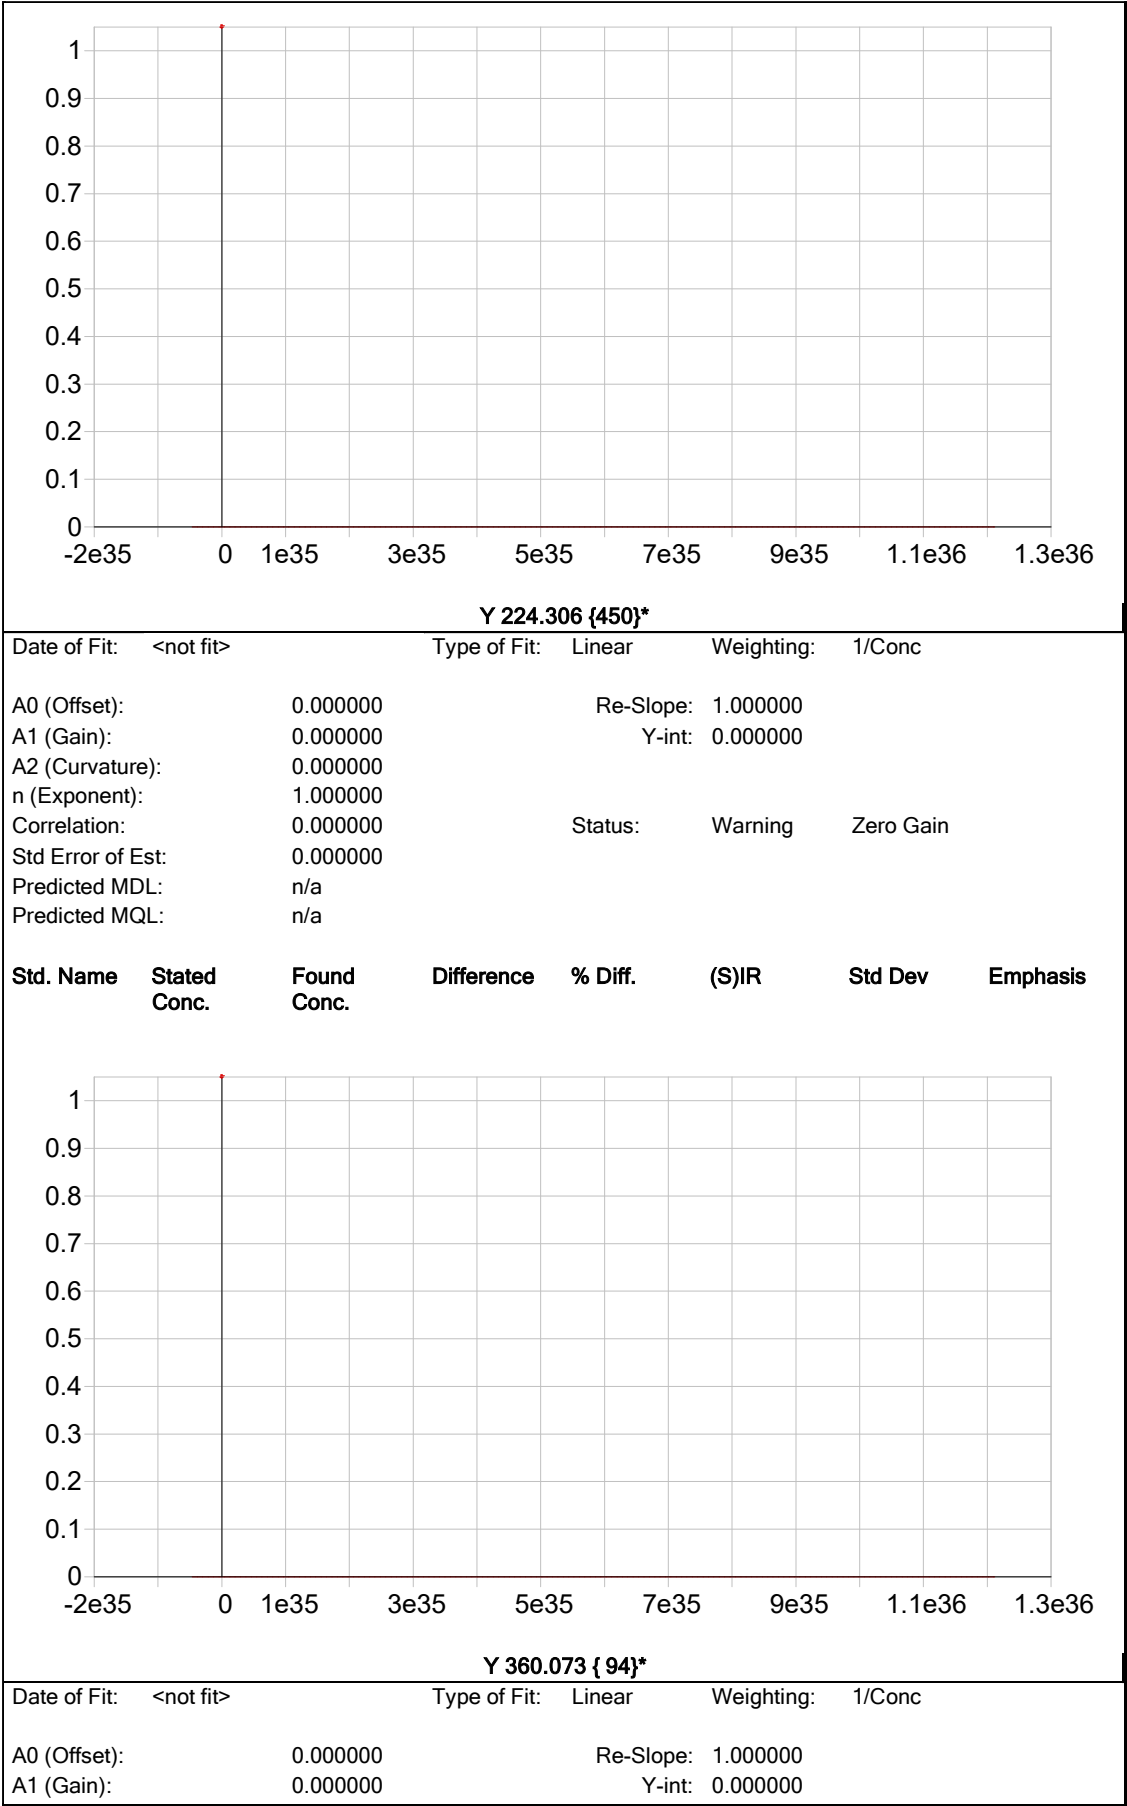

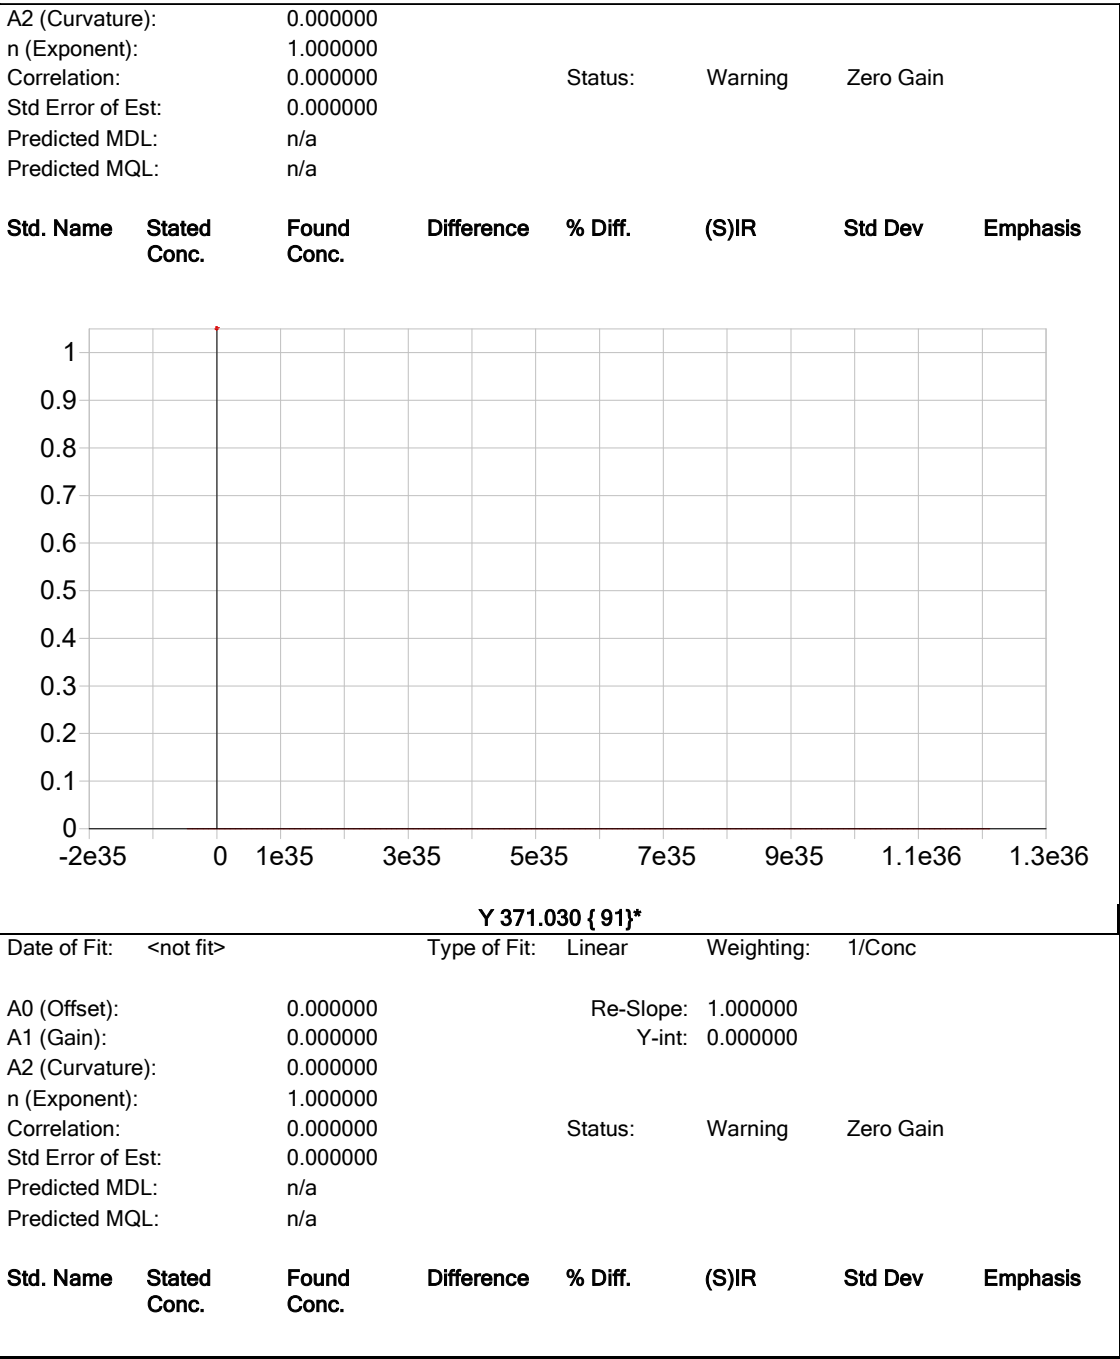

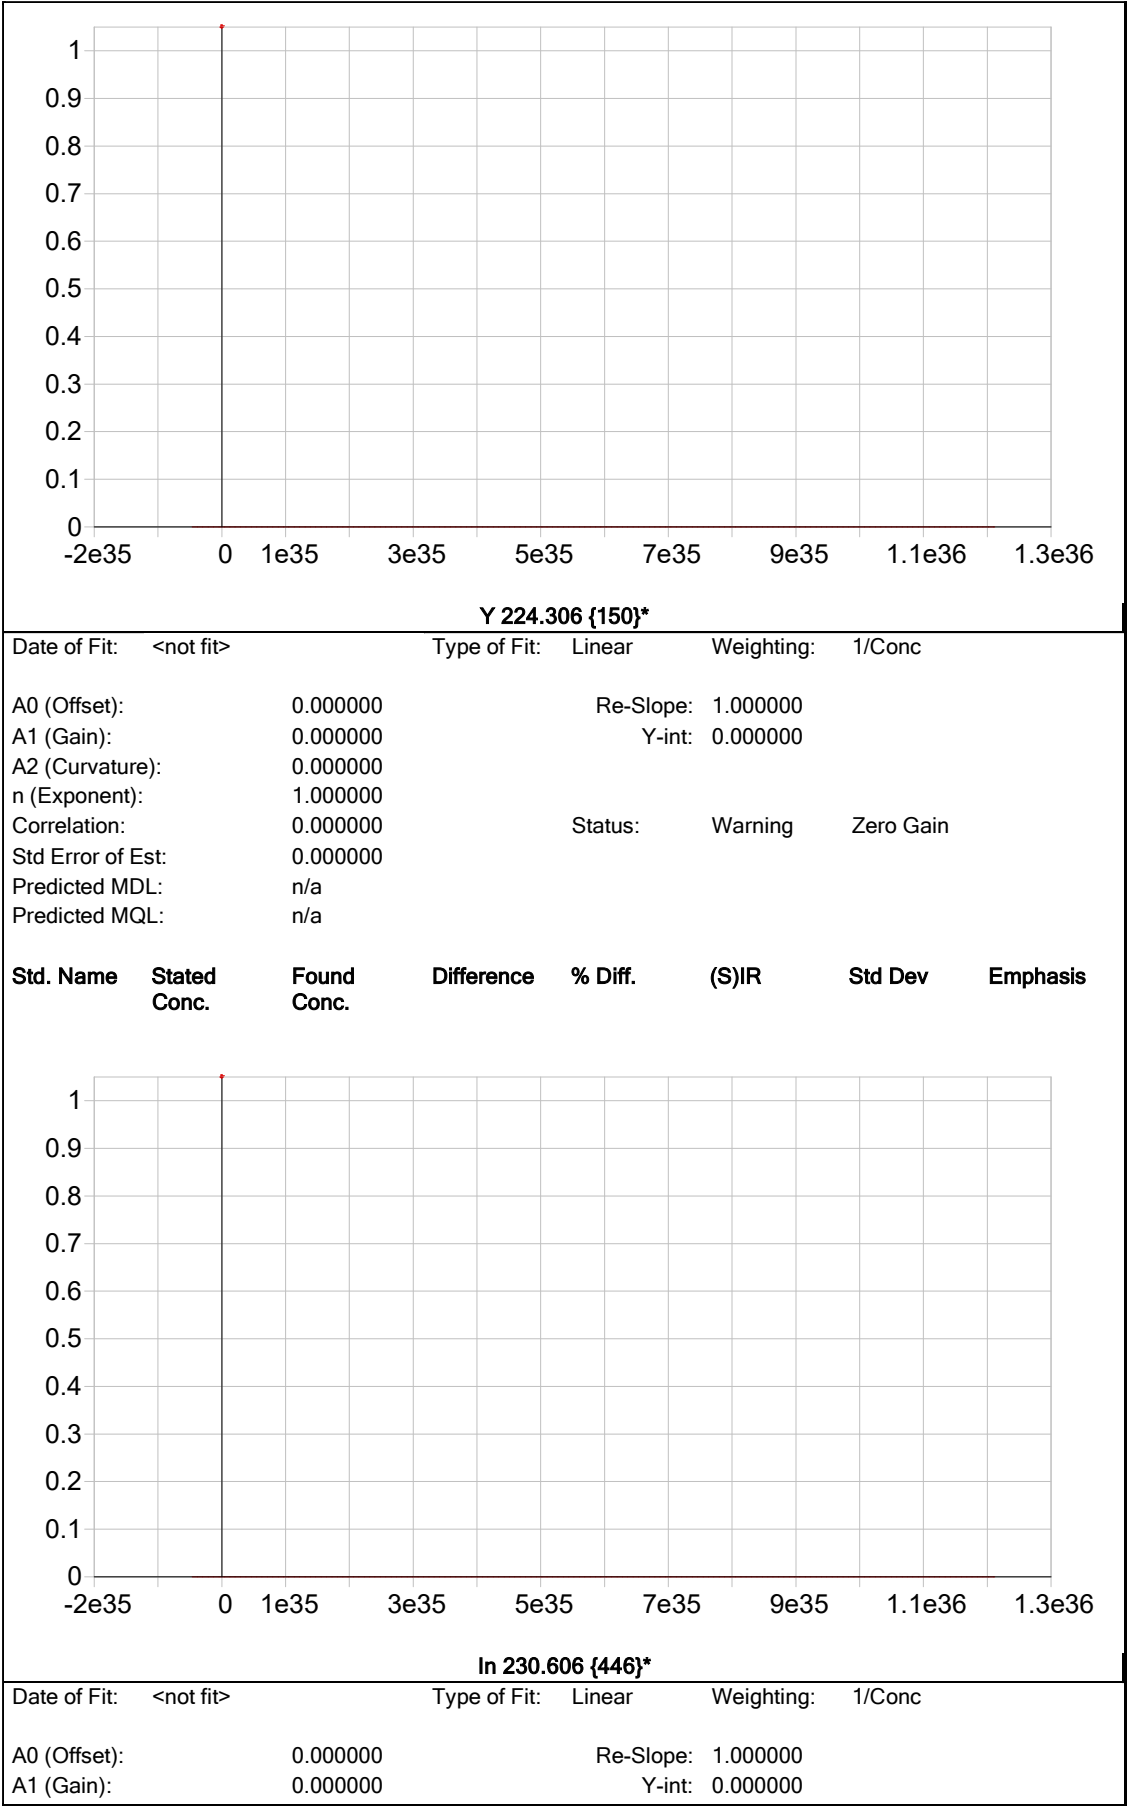

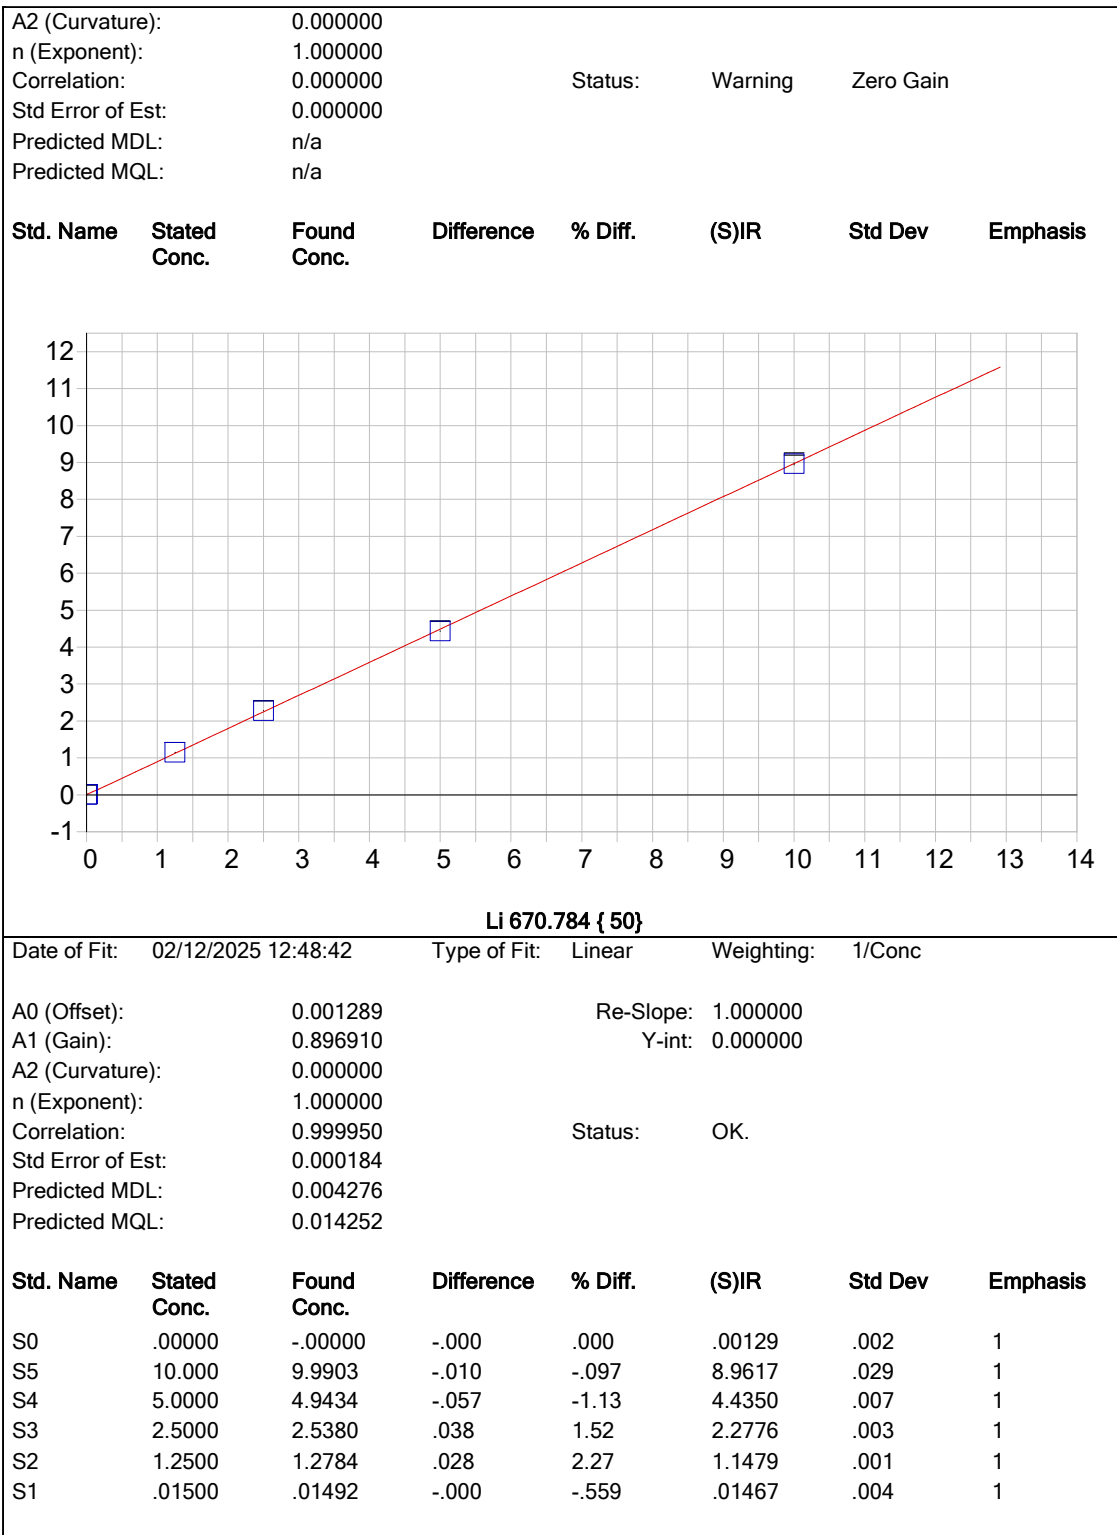

Sample Name: S0 Acquired: 02/12/2025 12:25:13 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S0 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.18500	-.00006	.00034	-.00009	.00023	-.00354	.19087	.00303
Stddev	.55450	.00008	.00011	.00006	.00019	.00109	.00128	.00128
%RSD	299.72	144.59	31.103	64.170	82.572	30.674	.67010	42.118
#1	.77585	.00001	.00040	-.00005	.00038	-.00416	.19235	.00156
#2	.10321	-.00003	.00041	-.00006	.00002	-.00417	.19018	.00380
#3	-.32406	-.00015	.00022	-.00015	.00029	-.00229	.19009	.00373
Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.00025	.00291	.00012	.00015	.00282	-.00050	-.00030	-.00048
Stddev	.00005	.00023	.00018	.00012	.00107	.00067	.00041	.00007
%RSD	22.187	7.7734	154.30	83.705	37.900	132.58	135.19	13.550
#1	.00019	.00305	.00033	.00001	.00374	.00019	.00001	-.00055
#2	.00029	.00304	-.00002	.00023	.00309	-.00114	-.00077	-.00042
#3	.00026	.00265	.00005	.00020	.00165	-.00055	-.00015	-.00048
Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	-.00016	.00068	-.00137	.00057	-.00042	.22045	-.00222	.00158
Stddev	.00047	.00023	.00240	.00131	.00026	.00117	.00018	.00208
%RSD	293.23	33.430	174.83	229.25	62.036	.53013	8.1596	131.28
#1	-.00034	.00046	-.00384	-.00019	-.00015	.22119	-.00202	.00208
#2	.00037	.00091	-.00126	-.00018	-.00067	.21910	-.00225	.00336
#3	-.00052	.00066	.00097	.00208	-.00046	.22106	-.00238	-.00070
Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.00025	.00030	.01185	.00158	.00082	-.00189	.00129	
Stddev	.00008	.00013	.00129	.00010	.00104	.00114	.00182	
%RSD	32.464	44.290	10.879	6.5024	126.39	60.090	141.28	
#1	.00030	.00025	.01122	.00158	.00134	-.00207	.00322	
#2	.00029	.00020	.01333	.00168	-.00037	-.00293	.00106	
#3	.00015	.00045	.01100	.00148	.00150	-.00068	-.00040	

Sample Name: S0 Acquired: 02/12/2025 12:25:13 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S0 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4357.3	37929.	4303.7	3058.9	5230.4
Stddev	2.4	80.	22.6	11.4	11.0
%RSD	.05561	.21017	.52509	.37114	.20980
#1	4356.5	37852.	4320.9	3046.0	5218.3
#2	4355.4	38011.	4312.0	3063.1	5233.3
#3	4360.0	37924.	4278.1	3067.5	5239.7

Sample Name: S1 Acquired: 02/12/2025 12:29:16 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	2.9403	.00310	.00210	.00216	.00697	.01745	.83760	.04177
Stddev	.3249	.00021	.00038	.00018	.00006	.00118	.00682	.00060
%RSD	11.050	6.7990	18.226	8.3720	.81447	6.7863	.81448	1.4346
#1	2.6765	.00325	.00247	.00222	.00698	.01690	.83601	.04212
#2	3.3032	.00286	.00211	.00230	.00690	.01881	.83171	.04211
#3	2.8412	.00320	.00171	.00195	.00701	.01665	.84507	.04108
Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.01734	.33651	.00293	.03923	.00689	.00239	.01019	.09201
Stddev	.00012	.00071	.00009	.00035	.00006	.00025	.00074	.00040
%RSD	.67907	.21135	3.0675	.89904	.84051	10.511	7.2930	.43745
#1	.01723	.33649	.00288	.03946	.00693	.00242	.01098	.09155
#2	.01747	.33580	.00303	.03940	.00683	.00213	.00951	.09221
#3	.01731	.33722	.00286	.03882	.00693	.00263	.01008	.09228
Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.02633	.00316	.03560	.01056	.00900	.31779	-.00166	.00084
Stddev	.00011	.00025	.00386	.00095	.00034	.00245	.00010	.00094
%RSD	.42510	7.8566	10.848	8.9848	3.7792	.77026	6.2360	110.96
#1	.02625	.00343	.03212	.00950	.00886	.31515	-.00175	.00153
#2	.02629	.00308	.03491	.01131	.00939	.31998	-.00155	.00123
#3	.02646	.00295	.03975	.01088	.00875	.31825	-.00169	-.00022
Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.00600	.00379	.43696	.00289	.04750	.99852	.01467	
Stddev	.00009	.00002	.00006	.00010	.00044	.00342	.00413	
%RSD	1.4427	.62017	.01313	3.3591	.91725	.34238	28.178	
#1	.00598	.00378	.43697	.00295	.04705	.99534	.01943	
#2	.00609	.00377	.43689	.00278	.04792	.99808	.01255	
#3	.00592	.00382	.43701	.00293	.04752	1.0021	.01202	

Sample Name: S1 Acquired: 02/12/2025 12:29:16 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S01 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4320.8	37886.	4326.0	3024.6	4975.6
Stddev	5.9	156.	20.6	12.9	12.3
%RSD	.13698	.41295	.47708	.42690	.24639
#1	4315.5	37757.	4317.9	3039.1	4962.4
#2	4319.7	38060.	4349.5	3014.3	4986.6
#3	4327.1	37841.	4310.7	3020.3	4977.7

Sample Name: S2 Acquired: 02/12/2025 12:33:17 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S02 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	335.15	.15636	1.4508	.07958	.14914	3.2613	7.9560	.93151
Stddev	.26	.00071	.0033	.00034	.00030	.0196	.0078	.01143
%RSD	.07883	.45475	.23046	.42162	.20298	.60198	.09858	1.2275

#1	335.41	.15581	1.4472	.07926	.14879	3.2744	7.9623	.93781
#2	335.15	.15610	1.4517	.07956	.14934	3.2387	7.9472	.91831
#3	334.88	.15716	1.4537	.07993	.14929	3.2708	7.9585	.93842

Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	2.2477	4.0704	1.0989	.48526	.67571	1.0586	2.4820	1.1446
Stddev	.0034	.0081	.0050	.00041	.00238	.0062	.0121	.0087
%RSD	.14892	.19971	.45367	.08407	.35239	.58442	.48669	.76116

#1	2.2438	4.0705	1.0959	.48479	.67811	1.0603	2.4880	1.1498
#2	2.2498	4.0622	1.1047	.48546	.67334	1.0517	2.4680	1.1345
#3	2.2494	4.0784	1.0962	.48553	.67567	1.0637	2.4898	1.1495

Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.42949	.07749	.27722	.11679	.55674	.92059	.07357	1.0961
Stddev	.00055	.00067	.00401	.00028	.00308	.00545	.00038	.0112
%RSD	.12723	.85941	1.4458	.24056	.55316	.59230	.51436	1.0214

#1	.42907	.07672	.27337	.11658	.55434	.92303	.07314	1.1047
#2	.43011	.07793	.28137	.11668	.56021	.91435	.07374	1.0834
#3	.42930	.07781	.27693	.11711	.55568	.92441	.07383	1.1002

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.63444	.05145	1.1441	.21457	.58458	12.158	1.1479
Stddev	.00133	.00029	.0126	.00059	.00340	.051	.0012
%RSD	.20912	.55421	1.0999	.27579	.58123	.41877	.10435

#1	.63292	.05122	1.1551	.21409	.58732	12.185	1.1468
#2	.63539	.05138	1.1304	.21438	.58078	12.099	1.1478
#3	.63501	.05177	1.1468	.21523	.58565	12.190	1.1492

Sample Name: S2 Acquired: 02/12/2025 12:33:17 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S02 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4160.6	35865.	4263.5	2890.3	4386.4
Stddev	9.7	322.	25.8	18.8	10.8
%RSD	.23219	.89835	.60492	.65104	.24668
#1	4170.4	35930.	4235.2	2890.8	4398.2
#2	4151.1	35515.	4285.7	2871.2	4377.0
#3	4160.3	36149.	4269.5	2908.9	4384.0

Sample Name: S3 Acquired: 02/12/2025 12:37:03 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S03 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	660.82	.31154	2.9788	.16229	.30412	6.5690	15.954	1.8312
Stddev	1.08	.00010	.0036	.00034	.00016	.0203	.049	.0095
%RSD	.16377	.03247	.12108	.20893	.05217	.30869	.30417	.51735

#1	659.70	.31154	2.9826	.16232	.30397	6.5924	16.003	1.8376
#2	660.91	.31165	2.9754	.16261	.30429	6.5561	15.906	1.8203
#3	661.85	.31144	2.9785	.16193	.30411	6.5586	15.953	1.8355

Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4.6267	8.1440	2.1862	.97878	1.3600	2.1230	4.9530	2.2840
Stddev	.0028	.0233	.0031	.00133	.0053	.0042	.0145	.0048
%RSD	.05958	.28668	.13975	.13626	.39078	.19939	.29236	.20981

#1	4.6299	8.1497	2.1828	.98025	1.3607	2.1272	4.9689	2.2889
#2	4.6249	8.1183	2.1885	.97764	1.3543	2.1188	4.9493	2.2793
#3	4.6254	8.1639	2.1874	.97846	1.3649	2.1230	4.9407	2.2840

Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.87818	.15488	.55895	.23856	1.1540	1.6224	.15661	2.1265
Stddev	.00111	.00075	.00328	.00246	.0035	.0018	.00025	.0076
%RSD	.12690	.48523	.58670	1.0301	.30527	.10863	.15988	.35792

#1	.87946	.15404	.55927	.24128	1.1557	1.6239	.15678	2.1333
#2	.87744	.15511	.55552	.23788	1.1563	1.6228	.15671	2.1183
#3	.87763	.15549	.56206	.23650	1.1499	1.6205	.15632	2.1279

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	1.2802	.10776	2.2056	.43675	1.1865	24.527	2.2776
Stddev	.0017	.00012	.0080	.00042	.0018	.069	.0029
%RSD	.13084	.11214	.36028	.09632	.15236	.28114	.12545

#1	1.2821	.10790	2.2064	.43640	1.1885	24.606	2.2793
#2	1.2791	.10770	2.1973	.43722	1.1859	24.477	2.2743
#3	1.2794	.10768	2.2131	.43665	1.1850	24.499	2.2792

Sample Name: S3 Acquired: 02/12/2025 12:37:03 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S03 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4007.5	34889.	4258.6	2784.6	4122.8
Stddev	8.6	73.	12.5	7.4	8.6
%RSD	.21500	.20911	.29379	.26679	.20964
#1	3997.6	34868.	4244.9	2779.2	4113.0
#2	4013.3	34829.	4269.3	2781.6	4129.2
#3	4011.6	34971.	4261.7	2793.1	4126.4

Sample Name: S4 Acquired: 02/12/2025 12:40:47 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S04 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	1273.2	.59579	5.8831	.32189	.60417	12.920	31.183	3.5510
Stddev	4.3	.00059	.0081	.00093	.00144	.122	.033	.0145
%RSD	.33396	.09949	.13833	.28791	.23897	.94493	.10527	.40956

#1	1268.5	.59540	5.8757	.32215	.60412	12.867	31.180	3.5673
#2	1276.8	.59550	5.8817	.32086	.60275	13.059	31.217	3.5466
#3	1274.2	.59647	5.8918	.32266	.60564	12.833	31.152	3.5392

Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	9.1504	15.726	4.2581	1.9109	2.6462	4.0737	9.5387	4.3839
Stddev	.0158	.048	.0106	.0025	.0038	.0344	.0595	.0290
%RSD	.17229	.30289	.24983	.12946	.14474	.84449	.62321	.66257

#1	9.1334	15.729	4.2473	1.9087	2.6420	4.0632	9.5219	4.3664
#2	9.1534	15.772	4.2585	1.9105	2.6471	4.1121	9.6048	4.4175
#3	9.1645	15.677	4.2686	1.9136	2.6495	4.0458	9.4895	4.3679

Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	1.7237	.30692	1.0938	.46119	2.2795	2.9475	.31827	4.0176
Stddev	.0022	.00035	.0033	.00451	.0181	.0209	.00029	.0281
%RSD	.12490	.11367	.30127	.97720	.79217	.70850	.09139	.70054

#1	1.7216	.30676	1.0913	.45872	2.2599	2.9364	.31807	4.0485
#2	1.7236	.30668	1.0975	.46639	2.2956	2.9716	.31813	4.0109
#3	1.7259	.30732	1.0925	.45846	2.2829	2.9346	.31860	3.9934

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	2.5091	.21946	4.1889	.85641	2.3015	47.749	4.4350
Stddev	.0039	.00047	.0290	.00121	.0160	.418	.0067
%RSD	.15366	.21505	.69244	.14183	.69722	.87465	.15009

#1	2.5101	.21893	4.2197	.85501	2.2999	47.305	4.4274
#2	2.5048	.21983	4.1850	.85714	2.3183	48.133	4.4393
#3	2.5123	.21961	4.1621	.85709	2.2863	47.809	4.4384

Sample Name: S4 Acquired: 02/12/2025 12:40:47 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S04 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3859.7	33702.	4206.7	2676.8	3912.6
Stddev	10.0	141.	15.0	5.6	4.4
%RSD	.25941	.41921	.35764	.20914	.11201
#1	3849.0	33865.	4195.2	2682.3	3907.6
#2	3868.8	33620.	4201.2	2671.1	3915.7
#3	3861.3	33620.	4223.7	2676.8	3914.5

Sample Name: S5 Acquired: 02/12/2025 12:44:37 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S05 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	2410.0	1.1632	11.731	.66176	1.2514	25.747	61.970	7.0278
Stddev	6.0	.0013	.011	.00092	.0030	.098	.291	.0223
%RSD	.24971	.10859	.09019	.13890	.23752	.37965	.46926	.31741

#1	2414.6	1.1632	11.725	.66070	1.2492	25.644	61.897	7.0067
#2	2403.2	1.1620	11.743	.66232	1.2504	25.758	62.290	7.0253
#3	2412.1	1.1645	11.725	.66226	1.2548	25.839	61.722	7.0512

Elem	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	18.257	30.944	8.3917	3.8150	5.2810	7.9270	18.597	8.5470
Stddev	.014	.083	.0486	.0022	.0069	.0291	.063	.0438
%RSD	.07703	.26967	.57908	.05835	.12978	.36753	.33828	.51283

#1	18.267	30.883	8.3367	3.8160	5.2734	7.8964	18.538	8.5097
#2	18.262	30.909	8.4092	3.8124	5.2829	7.9302	18.590	8.5359
#3	18.241	31.039	8.4290	3.8165	5.2866	7.9544	18.663	8.5953

Elem	Ni2316	Ag3280	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3.4510	.63490	2.1777	.89888	4.6530	5.6231	.65178	7.5690
Stddev	.0006	.00086	.0089	.00350	.0045	.0268	.00072	.0170
%RSD	.01863	.13468	.41020	.38978	.09680	.47608	.11072	.22449

#1	3.4516	.63588	2.1676	.89567	4.6487	5.5958	.65261	7.5587
#2	3.4510	.63446	2.1845	.89834	4.6577	5.6243	.65130	7.5596
#3	3.4503	.63434	2.1812	.90262	4.6525	5.6493	.65143	7.5886

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077	Li6707
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5.1223	.44759	7.9924	1.6977	4.5353	94.808	8.9617
Stddev	.0097	.00057	.0255	.0024	.0103	.866	.0291
%RSD	.18891	.12654	.31942	.13988	.22638	.91318	.32496

#1	5.1113	.44801	7.9712	1.6986	4.5276	93.811	8.9339
#2	5.1261	.44695	7.9851	1.6996	4.5313	95.249	8.9592
#3	5.1295	.44783	8.0207	1.6950	4.5470	95.365	8.9920

Sample Name: S5 Acquired: 02/12/2025 12:44:37 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S05 Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3518.4	31584.	4108.9	2462.1	3586.7
Stddev	12.7	66.	21.1	8.7	10.6
%RSD	.35958	.20809	.51448	.35318	.29595
#1	3531.7	31659.	4129.9	2471.5	3595.7
#2	3506.4	31554.	4109.1	2454.4	3575.0
#3	3517.2	31538.	4087.6	2460.3	3589.5

Sample Name: S6 Acquired: 02/12/2025 12:48:46 Type: Cal
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: IR Corr. Factor: 1.000000
User: Kareem Custom ID1: S06 Custom ID2: Custom ID3:
Comment:

Elem	Al3961	Ca3736	Fe2598	Mg2790	Na8183
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	68.304	49.744	21.076	13.911	6.0090
Stddev	.534	.281	.067	.058	.0291
%RSD	.78214	.56444	.31656	.41707	.48403
#1	67.781	49.523	21.024	13.860	5.9898
#2	68.282	49.648	21.052	13.900	5.9946
#3	68.849	50.060	21.151	13.974	6.0424
Int. Std.	Y_3710				
Units	Cts/S				
Avg	3991.9				
Stddev	16.1				
%RSD	.40440				
#1	4003.1				
#2	3999.1				
#3	3973.4				

Sample Name: ICV005 Acquired: 02/12/2025 13:20:54 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICV005 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.068983	1.060684	.9638056	.9927625	.9557956	2.519613
Stddev	.003338	.002353	.0034398	.0030474	.0038800	.014450
%RSD	.3123013	.2218451	.3568989	.3069628	.4059460	.5735049

#1	1.072038	1.058644	.9601099	.9954954	.9533992	2.503644
#2	1.069492	1.060148	.9669139	.9894764	.9537154	2.531787
#3	1.065419	1.063258	.9643932	.9933157	.9602721	2.523408

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.5212881	.5268021	.4713048	10.35835	.5407012	.4897838
Stddev	.0003950	.0042800	.0004474	.02892	.0004235	.0013123
%RSD	.0757835	.8124436	.0949303	.2792354	.0783141	.2679302

#1	.5215276	.5309153	.4712313	10.33752	.5403141	.4903330
#2	.5215045	.5223729	.4708987	10.34616	.5411534	.4882861
#3	.5208321	.5271180	.4717844	10.39138	.5406361	.4907322

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.5187974	10.44575	.5339791	6.084693	.4902381	.2397818
Stddev	.0087686	.03987	.0012813	.033811	.0011249	.0006853
%RSD	1.690168	.3817261	.2399514	.5556764	.2294642	.2858000

#1	.5277851	10.46558	.5325047	6.122603	.4899815	.2398305
#2	.5102658	10.47183	.5348230	6.057657	.4892637	.2390735
#3	.5183412	10.39985	.5346096	6.073820	.4914692	.2404415

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.890092	.5192119	1.042654	10.19748	F .0021881	F .0036425
Stddev	.036054	.0020794	.011456	.08299	.0012899	.0020069
%RSD	.3645464	.4004865	1.098743	.8138035	58.95053	55.09607

#1	9.851588	.5176856	1.029782	10.10171	.0013904	.0034677
#2	9.923054	.5215802	1.051731	10.24829	.0036763	.0017287
#3	9.895635	.5183699	1.046450	10.24242	.0014977	.0057310

Sample Name: ICV005 Acquired: 02/12/2025 13:20:54 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICV005 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	F .0004661	F .0035714	F .0037453	F .0006248	F -.000508	F -.009379
Stddev	.0002214	.0033509	.0013591	.0006293	.003026	.000274
%RSD	47.49074	93.82461	36.28715	100.7214	596.1216	2.925744

#1	.0005895	.0021599	.0041920	.0005420	-.000910	-.009602
#2	.0005983	.0011572	.0022191	.0000410	.002700	-.009072
#3	.0002106	.0073971	.0048248	.0012913	-.003313	-.009462

Elem	Li6707
Units	ppm
Avg	F -.004021
Stddev	.003517
%RSD	87.45700

#1	-.002412
#2	-.008054
#3	-.001596

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4322.395	37726.39	4314.281	3031.942	4868.340
Stddev	7.860	142.90	19.137	17.827	9.667
%RSD	.1818535	.3787918	.4435768	.5879595	.1985739

#1	4327.334	37891.24	4313.002	3052.508	4875.719
#2	4326.521	37650.37	4334.025	3020.907	4871.903
#3	4313.331	37637.58	4295.815	3022.411	4857.396

Sample Name: ICB005 Acquired: 02/12/2025 13:24:45 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICB005 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001827	.0009334	-.000803	.0039378	.0013196	.0182293	.0016771
Stddev	.001375	.0002065	.001823	.0021182	.0008230	.0104851	.0002772
%RSD	75.26668	22.11916	226.9235	53.79129	62.37193	57.51783	16.52789

#1	-.002880	.0008488	-.002418	.0027123	.0022406	.0132178	.0016501
#2	-.000271	.0007826	.001173	.0063837	.0010621	.0111904	.0014144
#3	-.002328	.0011687	-.001165	.0027174	.0006561	.0302798	.0019668

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000049	.0000083	.0044020	-.000468	-.000104	-.002607	.0268073
Stddev	.000108	.0000369	.0233600	.000564	.000112	.004029	.0213177
%RSD	219.8347	443.1617	530.6667	120.5588	108.3597	154.5416	79.52211

#1	-.000032	.0000051	.0299401	-.000349	.000026	-.001781	.0398099
#2	-.000165	-.000027	-.015886	-.001083	-.000159	.000945	.0022050
#3	.000049	.000047	-.000848	.000027	-.000177	-.006986	.0384069

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000059	.0049858	.0002506	.0009355	-.115318	-.006742	.0004265
Stddev	.0005306	.0457077	.0000445	.0004966	.263449	.005149	.0023101
%RSD	9031.069	916.7514	17.75929	53.08595	228.4549	76.36940	541.6067

#1	-.000363	-.047267	.0002372	.0007180	-.302971	-.010999	.0023556
#2	.000614	.024676	.0002142	.0005847	-.228843	-.008207	.0010575
#3	-.000234	.037549	.0003002	.0015037	.185861	-.001019	-.002134

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3384827	.0010635	.0005123	.0005191	-.004799	-.000011	-.000413
Stddev	.2422273	.0018849	.0004158	.0006341	.001813	.001528	.000494
%RSD	71.56268	177.2296	81.17146	122.1511	37.78093	14465.81	119.7699

#1	.0971813	.0032397	.0008695	.0003423	-.004795	-.000469	-.000810
#2	.5816254	.0000080	.0000558	.0012228	-.006614	.001694	-.000568
#3	.3366414	-.000057	.0006114	-.000008	-.002988	-.001258	.000141

Sample Name: ICB005 Acquired: 02/12/2025 13:24:45 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICB005 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0000451	-.000071	.0013711
Stddev	.0016923	.000073	.0037303
%RSD	3753.253	103.1044	272.0670

#1	-.001886	-.000008	.0004273
#2	.000750	-.000152	-.001797
#3	.001271	-.000053	.005483

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4371.891	38343.29	4248.852	3038.168	5229.941
Stddev	4.964	131.75	37.831	9.272	2.727
%RSD	.1135458	.3436194	.8903851	.3051904	.0521502

#1	4369.627	38193.74	4292.438	3028.231	5228.267
#2	4368.462	38393.86	4229.589	3039.685	5228.468
#3	4377.583	38442.26	4224.529	3046.588	5233.088

Sample Name: ICSA005 Acquired: 02/12/2025 13:28:48 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICSA005 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.004561	-.001315	-.002309	-.022891	.0164846	245.6480
Stddev	.002789	.000714	.003986	.001897	.0057092	1.4052
%RSD	61.15130	54.28777	172.6752	8.287731	34.63362	.5720233

#1	-.003799	-.000638	-.002155	-.020848	.0146853	244.5194
#2	-.007653	-.001247	-.006370	-.023228	.0228768	245.2028
#3	-.002233	-.002061	.001599	-.024597	.0118918	247.2218

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0079028	.0030132	.0026586	252.6226	.0534214	.0311239
Stddev	.0002792	.0001590	.0001131	1.1019	.0008533	.0004864
%RSD	3.533597	5.275491	4.252852	.4361686	1.597349	1.562855

#1	.0079121	.0028300	.0026366	251.6619	.0526308	.0310802
#2	.0076190	.0031144	.0025582	252.3806	.0533074	.0306607
#3	.0081772	.0030952	.0027811	253.8254	.0543260	.0316306

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.016468	104.9522	.0085785	254.4094	.0082435	.0004118
Stddev	.002997	.4725	.0004135	1.5475	.0004501	.0007974
%RSD	18.20172	.4501595	4.820510	.6082624	5.459442	193.6315

#1	-.018109	104.6265	.0084861	253.1892	.0077355	.0012900
#2	-.018286	104.7361	.0090304	253.8891	.0084027	.0002120
#3	-.013008	105.4941	.0082190	256.1500	.0085923	-.000267

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0648614	-.000784	-.031385	-1.21287	.0040845	F .0295937
Stddev	.5673432	.003375	.001925	.24205	.0010925	.0010150
%RSD	874.7003	430.3472	6.133171	19.95683	26.74768	3.429646

#1	.5296897	-.002009	-.032106	-1.45830	.0029117	.0284219
#2	-.567339	.003032	-.029203	-1.20598	.0042684	.0301603
#3	.232234	-.003376	-.032844	-.97434	.0050733	.0301988

Sample Name: ICSA005 Acquired: 02/12/2025 13:28:48 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICSA005 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0024310	.0258217	-.006480	F .0095860	-.000041	.0019168
Stddev	.0005683	.0049800	.001446	.0004832	.001210	.0003918
%RSD	23.37738	19.28593	22.31416	5.040696	2987.256	20.44116

#1	.0023668	.0285033	-.006015	.0098702	.001034	.0014793
#2	.0018976	.0200756	-.008102	.0090281	-.001352	.0022354
#3	.0030287	.0288862	-.005324	.0098597	.000196	.0020357

Elem	Li6707
Units	ppm
Avg	.0087508
Stddev	.0046237
%RSD	52.83718

#1	.0128714
#2	.0037504
#3	.0096308

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4002.166	34069.07	4192.752	2811.669	4105.816
Stddev	8.975	45.28	16.840	13.386	8.611
%RSD	.2242530	.1329133	.4016429	.4760931	.2097182

#1	3994.264	34080.77	4182.948	2798.052	4096.587
#2	4000.309	34107.35	4212.197	2812.143	4107.228
#3	4011.923	34019.08	4183.111	2824.811	4113.633

Sample Name: ICSAB005 Acquired: 02/12/2025 13:32:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICSAB005 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1016581	.1020508	.0463316	.0253532	.5994175	245.7738
Stddev	.0019109	.0012945	.0017256	.0030769	.0009839	.2781
%RSD	1.879728	1.268482	3.724394	12.13615	.1641397	.1131687

#1	.1037296	.1032415	.0444645	.0288249	.5983575	245.8099
#2	.1012808	.1006729	.0478678	.0229636	.5995932	246.0322
#3	.0999641	.1022381	.0466623	.0242710	.6003016	245.4794

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.5436094	.5384322	1.022328	254.8505	.6086994	.5384797
Stddev	.0019839	.0019276	.001611	.4420	.0023336	.0007388
%RSD	.3649491	.3579975	.1575897	.1734420	.3833678	.1372073

#1	.5449616	.5406447	1.024127	255.3478	.6075049	.5390882
#2	.5413319	.5375361	1.021839	254.7016	.6072048	.5386934
#3	.5445346	.5371159	1.021018	254.5022	.6113884	.5376576

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.5080746	105.1798	.5409386	255.1530	1.028010	.2129734
Stddev	.0029175	.1375	.0024537	.6157	.002715	.0013633
%RSD	.5742274	.1307440	.4535956	.2413034	.2640727	.6401229

#1	.5113589	105.2485	.5435872	255.7267	1.031067	.2114043
#2	.5070820	105.0214	.5387430	255.2298	1.027086	.2138680
#3	.5057830	105.2694	.5404856	254.5025	1.025879	.2136478

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.160266	.5227678	.9690009	-2.59420	F .0101351	F .0306165
Stddev	.514189	.0051494	.0088612	.11020	.0034757	.0005875
%RSD	320.8343	.9850204	.9144694	4.248025	34.29365	1.918813

#1	-.739919	.5286042	.9640246	-2.54944	.0077272	.0312626
#2	.018240	.5208334	.9637465	-2.51341	.0141197	.0304726
#3	.240881	.5188657	.9792317	-2.71973	.0085585	.0301145

Sample Name: ICSAB005 Acquired: 02/12/2025 13:32:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: ICSAB005 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0028360	.0261924	-.005231	F .0077208	-.000767	.0023838
Stddev	.0004198	.0072064	.000908	.0014350	.001767	.0002816
%RSD	14.80273	27.51327	17.35116	18.58655	230.2735	11.81233
#1	.0026281	.0188570	-.005108	.0093181	-.001531	.0026275
#2	.0033192	.0264576	-.004391	.0065401	-.002024	.0024482
#3	.0025608	.0332624	-.006194	.0073044	.001253	.0020755

Elem	Li6707
Units	ppm
Avg	.0080281
Stddev	.0069298
%RSD	86.31970
#1	.0110674
#2	.0129188
#3	.0000979

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3986.330	33649.51	4167.040	2793.817	4094.206
Stddev	6.711	95.02	25.543	17.613	2.945
%RSD	.1683599	.2823781	.6129804	.6304364	.0719330
#1	3986.892	33748.48	4138.778	2773.518	4094.085
#2	3992.743	33641.02	4173.864	2805.055	4097.209
#3	3979.355	33559.02	4188.479	2802.879	4091.323

Sample Name: CCV011 Acquired: 02/12/2025 13:36:36 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCV011 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.738093	4.768842	24.36925	4.803961	4.921437	391.8105	10.04492
Stddev	.018285	.009413	.01332	.001333	.000990	1.5428	.04155
%RSD	.3859203	.1973950	.0546713	.0277406	.0201182	.3937559	.4135947

#1	4.750745	4.759732	24.37104	4.805018	4.921497	391.6825	10.03357
#2	4.746407	4.778532	24.35513	4.802464	4.920419	390.3358	10.01023
#3	4.717129	4.768262	24.38159	4.804400	4.922396	393.4133	10.09096

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4974895	2.461326	397.3900	15.59536	2.456205	14.76536	394.5813
Stddev	.0036119	.000825	1.5267	.05304	.000736	.06837	1.0319
%RSD	.7260241	.0335136	.3841729	.3401168	.0299630	.4630174	.2615057

#1	.5002235	2.460861	396.9486	15.64153	2.455509	14.77417	394.1443
#2	.4933949	2.462279	396.1326	15.53742	2.456975	14.69302	393.8398
#3	.4988501	2.460840	399.0887	15.60712	2.456130	14.82889	395.7597

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	14.47588	391.4919	2.456245	1.258468	391.9880	2.423090	14.63540
Stddev	.05140	1.4424	.002248	.003016	1.4010	.009661	.06733
%RSD	.3550445	.3684287	.0915125	.2396866	.3574061	.3987264	.4600744

#1	14.46521	390.9203	2.456285	1.260775	391.1744	2.414873	14.56102
#2	14.43066	390.4229	2.453977	1.255055	391.1839	2.420664	14.65297
#3	14.53177	393.1324	2.458472	1.259574	393.6057	2.433733	14.69221

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	148.4186	4.921723	4.868148	4.847289	4.930644	4.674697	4.892557
Stddev	1.0185	.004486	.016717	.008756	.010451	.024871	.004154
%RSD	.6862384	.0911558	.3434000	.1806335	.2119531	.5320430	.0849068

#1	147.8257	4.924401	4.874817	4.840032	4.935065	4.688717	4.894959
#2	147.8353	4.916543	4.849125	4.857014	4.938158	4.645980	4.887761
#3	149.5946	4.924224	4.880501	4.844822	4.918710	4.689392	4.894953

Sample Name: CCV011 Acquired: 02/12/2025 13:36:36 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCV011 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	4.886840	4.658102	5.026152
Stddev	.019278	.027677	.028763
%RSD	.3944856	.5941785	.5722646
#1	4.888295	4.662446	5.012526
#2	4.866877	4.628509	5.006735
#3	4.905350	4.683350	5.059196

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3619.733	31256.98	4062.464	2535.434	3632.972
Stddev	8.631	102.88	22.991	8.445	7.828
%RSD	.2384534	.3291486	.5659414	.3330698	.2154696
#1	3625.706	31196.90	4048.997	2542.275	3637.819
#2	3623.657	31375.78	4089.011	2538.032	3637.157
#3	3609.837	31198.26	4049.385	2525.996	3623.942

Sample Name: CCB011 Acquired: 02/12/2025 13:40:19 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCB011 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0003383	.0004607	-.001375	.0027289	.0002655	.0207165	-.001610
Stddev	.0026144	.0004387	.000657	.0011266	.0018144	.0249436	.001351
%RSD	772.7797	95.21689	47.75947	41.28542	683.2560	120.4041	83.95684

#1	.0033554	.0000656	-.001519	.0040098	.0022471	.0029689	-.000739
#2	-.001261	.0003838	-.001947	.0018918	-.000136	.0492359	-.003167
#3	-.001080	.0009327	-.000658	.0022849	-.001314	.0099448	-.000924

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000295	.0000504	.0237342	.0000515	-.000073	-.005185	.0291035
Stddev	.000071	.0001217	.0216866	.0004210	.000354	.006162	.0089634
%RSD	23.93138	241.5846	91.37289	816.7714	483.2672	118.8388	30.79817

#1	-.000296	-.000088	.0296254	-.000250	-.000282	.001338	.0281821
#2	-.000224	.000096	-.000289	-.000128	-.000273	-.005986	.0384920
#3	-.000365	.000143	.041867	.000532	.000336	-.010908	.0206365

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0002671	.0054489	.0001512	.0003419	-.077288	.0002665	-.000517
Stddev	.0003714	.0295388	.0004247	.0006273	.489283	.0039433	.002396
%RSD	139.0733	542.1026	280.8636	183.4525	633.0654	1479.762	463.2010

#1	.0006709	.0225743	.0001137	-.000366	-.122140	-.002313	.002229
#2	.0001901	.0224320	.0005934	.000827	-.542600	-.001693	-.002178
#3	-.000060	-.028659	-.000253	.000565	.432877	.004806	-.001603

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4157597	.0021882	.0113737	.0005846	-.003443	-.000307	-.000472
Stddev	.1917042	.0001247	.0014242	.0004295	.003481	.000381	.000263
%RSD	46.10938	5.697485	12.52146	73.46467	101.1077	124.2125	55.76893

#1	.2702569	.0022677	.0124996	.0010801	-.001308	-.000106	-.000702
#2	.3440391	.0020445	.0097728	.0003542	-.007459	-.000068	-.000185
#3	.6329833	.0022524	.0118488	.0003195	-.001560	-.000747	-.000530

Sample Name: CCB011 Acquired: 02/12/2025 13:40:19 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCB011 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0012298	.0000252	.0054563
Stddev	.0026062	.0002302	.0047431
%RSD	211.9128	914.0971	86.92879
#1	.0033895	.0002906	.0095629
#2	-.001665	-.000095	.0065414
#3	.001965	-.000121	.0002647

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4303.392	37266.02	4200.150	3028.119	5168.943
Stddev	3.590	188.92	14.480	10.143	7.141
%RSD	.0834291	.5069470	.3447378	.3349530	.1381538
#1	4303.677	37063.78	4216.641	3019.570	5171.304
#2	4299.668	37296.33	4194.294	3039.326	5160.920
#3	4306.831	37437.95	4189.516	3025.461	5174.605

Sample Name: PB166660TB Acquired: 02/12/2025 13:44:23 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LEB660 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0059323	-.001981	-.000798	.0051937	.0014567	.0118865
Stddev	.0008188	.001429	.001399	.0028789	.0021279	.0156789
%RSD	13.80184	72.12931	175.2557	55.43012	146.0726	131.9055

#1	.0066666	-.001172	.000682	.0084697	-.000164	.0135393
#2	.0050494	-.001140	-.002099	.0030676	.000668	-.004553
#3	.0060809	-.003632	-.000978	.0040437	.003866	.026674

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001808	-.000055	.0000187	.0149614	.0011431	.0000905
Stddev	.000740	.000110	.0000144	.0186957	.0005740	.0003335
%RSD	40.95046	201.1582	77.10270	124.9599	50.21810	368.5657

#1	-.001565	-.000104	.0000164	.0027014	.0017782	-.000199
#2	-.001219	.000071	.0000342	.0364796	.0009897	.000455
#3	-.002639	-.000131	.0000056	.0057031	.0006613	.000016

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003706	.0301447	.0020806	-.000757	.0039286	.0012422
Stddev	.003233	.0120443	.0003502	.010167	.0003029	.0010539
%RSD	87.25179	39.95475	16.83224	1342.644	7.709944	84.84409

#1	-.007008	.0184377	.0016812	-.007278	.0035896	.0008969
#2	-.000545	.0294964	.0023350	-.005952	.0041726	.0004042
#3	-.003564	.0425000	.0022256	.010958	.0040235	.0024254

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	F 1393.828	-.004274	.0002517	F -10.3312	-.001229	.0024605
Stddev	5.325	.004986	.0021829	.1788	.002105	.0007609
%RSD	.3820284	116.6738	867.1238	1.730928	171.3225	30.92513

#1	1389.767	.000703	.0010837	-10.5331	.000939	.0024985
#2	1399.856	-.004255	.0018964	-10.2681	-.001361	.0032017
#3	1391.860	-.009269	-.002225	-10.1926	-.003265	.0016813

Sample Name: PB166660TB Acquired: 02/12/2025 13:44:23 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LEB660 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0007162	.0209569	-.000449	-.007627	-.001226	-.000125
Stddev	.0001176	.0025104	.001006	.000416	.002494	.000011
%RSD	16.42632	11.97882	223.8793	5.454474	203.5190	8.445344
#1	.0007360	.0231499	.000712	-.007817	-.002103	-.000136
#2	.0008226	.0215023	-.001061	-.007913	-.003163	-.000115
#3	.0005899	.0182187	-.001000	-.007150	.001589	-.000124

Elem	Li6707
Units	ppm
Avg	-.002712
Stddev	.003084
%RSD	113.7122
#1	.000192
#2	-.002378
#3	-.005949

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4153.246	34296.23	4593.410	2914.173	4151.624
Stddev	9.242	82.37	12.593	4.647	11.338
%RSD	.2225356	.2401717	.2741507	.1594626	.2731045
#1	4162.277	34222.24	4606.263	2916.300	4163.241
#2	4153.655	34281.46	4581.095	2917.375	4151.045
#3	4143.806	34384.98	4592.873	2908.843	4140.587

Sample Name: Q1292-01 Acquired: 02/12/2025 13:48:28 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002865	.0191060	-.005254	-.019067	-.013641	.0722671
Stddev	.001695	.0011916	.001059	.006452	.002040	.0137490
%RSD	59.16458	6.236611	20.16174	33.83603	14.95641	19.02523

#1	-.001152	.0185023	-.005754	-.011637	-.014484	.0876329
#2	-.004542	.0183372	-.005971	-.023246	-.015124	.0680418
#3	-.002900	.0204786	-.004037	-.022318	-.011314	.0611267

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.114435	-.000110	.0035136	F 944.8809	.0024809	.0430995
Stddev	.000701	.000067	.0000746	8.1285	.0007949	.0003148
%RSD	.0331624	60.93096	2.124234	.8602668	32.04174	.7303272

#1	2.114392	-.000112	.0035784	940.4766	.0026217	.0429934
#2	2.115156	-.000176	.0034320	939.9050	.0016250	.0434537
#3	2.113756	-.000042	.0035305	954.2610	.0031960	.0428515

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.007973	.0505834	1.987006	23.15945	.0271061	.0013977
Stddev	.001371	.0197176	.011348	.10000	.0008544	.0004162
%RSD	17.19463	38.98043	.5710863	.4317706	3.151999	29.77655

#1	-.007194	.0302497	1.983002	23.08288	.0279537	.0018590
#2	-.009556	.0696210	1.978204	23.12290	.0271194	.0010505
#3	-.007169	.0518795	1.999813	23.27258	.0262451	.0012836

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	F 1463.482	.0004099	.3885339	F -4.15433	.0218746	.2267060
Stddev	3.928	.0055527	.0015543	.40272	.0022687	.0022243
%RSD	.2684186	1354.665	.4000338	9.694012	10.37133	.9811395

#1	1460.007	-.005841	.3888163	-4.59009	.0200530	.2242383
#2	1462.695	.002302	.3899277	-3.79586	.0211549	.2285565
#3	1467.744	.004769	.3868579	-4.07703	.0244158	.2273232

Sample Name: Q1292-01 Acquired: 02/12/2025 13:48:28 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0020293	4.441607	4.210936	-.002446	-.013903	1.164558
Stddev	.0003047	.010193	.045677	.001353	.002231	.005072
%RSD	15.01406	.2294856	1.084713	55.32277	16.04600	.4355671
#1	.0021266	4.448030	4.161302	-.002491	-.013507	1.161918
#2	.0022735	4.429854	4.220301	-.003777	-.011897	1.161350
#3	.0016879	4.446937	4.251203	-.001071	-.016305	1.170406

Elem	Li6707
Units	ppm
Avg	.0308450
Stddev	.0037237
%RSD	12.07221
#1	.0334504
#2	.0325046
#3	.0265801

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3860.076	32322.97	4355.392	2682.052	3762.024
Stddev	10.210	136.03	28.294	11.248	13.356
%RSD	.2644924	.4208609	.6496279	.4193917	.3550320
#1	3853.588	32168.01	4381.504	2669.410	3747.093
#2	3854.796	32422.71	4359.341	2690.953	3766.145
#3	3871.845	32378.20	4325.331	2685.793	3772.835

Sample Name: Q1292-02 Acquired: 02/12/2025 13:52:33 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9D Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.004709	.0178504	-.006628	-.016896	-.015010	.0410791
Stddev	.001191	.0016449	.000527	.001574	.001764	.0055224
%RSD	25.28588	9.214752	7.947131	9.313513	11.75095	13.44327

#1	-.005960	.0185130	-.006220	-.015200	-.013260	.0464162
#2	-.004578	.0190607	-.006443	-.018308	-.016787	.0353884
#3	-.003589	.0159776	-.007223	-.017179	-.014981	.0414328

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.043405	-.000056	.0035114	F 903.7533	.0024670	.0419587
Stddev	.006676	.000243	.0000819	2.8869	.0001583	.0007504
%RSD	.3267057	437.2290	2.331704	.3194313	6.414579	1.788388

#1	2.035888	-.000272	.0034303	903.4141	.0025900	.0420324
#2	2.048642	.000207	.0035940	901.0511	.0022885	.0426694
#3	2.045686	-.000102	.0035098	906.7949	.0025225	.0411741

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003374	.0567956	1.909714	22.26709	.0262433	.0012713
Stddev	.005843	.0266690	.007303	.06863	.0003529	.0008308
%RSD	173.2006	46.95614	.3824208	.3082226	1.344639	65.34530

#1	-.009470	.0872488	1.902943	22.18899	.0266506	.0021922
#2	.002179	.0376083	1.908748	22.29451	.0260516	.0010437
#3	-.002831	.0455296	1.917453	22.31778	.0260278	.0005782

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	F 1406.246	-.005489	.3740919	F -4.45901	.0213971	.2166149
Stddev	5.643	.004631	.0013592	.28106	.0004178	.0004915
%RSD	.4013064	84.36456	.3633435	6.303110	1.952538	.2269209

#1	1399.840	-.000431	.3726750	-4.77989	.0218756	.2171823
#2	1408.413	-.009520	.3753850	-4.34068	.0211049	.2163450
#3	1410.485	-.006515	.3742157	-4.25647	.0212107	.2163175

Sample Name: Q1292-02 Acquired: 02/12/2025 13:52:33 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9D Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0024230	4.349325	4.058719	-.003946	-.014995	1.122677
Stddev	.0003908	.015408	.011398	.002017	.002084	.004674
%RSD	16.12777	.3542625	.2808209	51.12372	13.89817	.4163104
#1	.0028510	4.359353	4.071244	-.002560	-.017354	1.117794
#2	.0020851	4.331583	4.048957	-.006260	-.013405	1.123128
#3	.0023330	4.357037	4.055954	-.003018	-.014226	1.127109

Elem	Li6707
Units	ppm
Avg	.0317964
Stddev	.0046991
%RSD	14.77883
#1	.0317979
#2	.0364947
#3	.0270965

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3958.761	33168.77	4532.950	2771.045	3857.337
Stddev	9.132	204.30	25.367	18.782	11.656
%RSD	.2306879	.6159407	.5596174	.6777800	.3021734
#1	3950.213	33303.23	4535.259	2780.107	3844.332
#2	3968.383	33269.40	4557.084	2783.577	3866.841
#3	3957.686	32933.67	4506.507	2749.450	3860.838

Sample Name: Q1292-01LX5 Acquired: 02/12/2025 13:56:38 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9L Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000067	.0128111	-.004583	-.012559	-.007403	.0210765	.4197837
Stddev	.000295	.0004101	.000568	.003357	.001270	.0171644	.0018465
%RSD	443.7776	3.201054	12.40211	26.73203	17.15195	81.43857	.4398712

#1	.000169	.0127380	-.003933	-.014893	-.005953	.0036769	.4218825
#2	.000029	.0124425	-.004986	-.008711	-.007942	.0379956	.4184089
#3	-.000398	.0132529	-.004831	-.014072	-.008314	.0215569	.4190596

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000142	.0007561	190.8062	.0007830	.0288329	-.004158	.0229463
Stddev	.0000746	.0000429	.2833	.0007037	.0002967	.005357	.0101841
%RSD	526.8835	5.678762	.1484817	89.87573	1.029112	128.8362	44.38232

#1	-.000056	.0007179	191.1290	.0000147	.0290568	-.009365	.0342398
#2	.000007	.0008026	190.5986	.0009380	.0284963	.001338	.0201382
#3	.000092	.0007479	190.6911	.0013964	.0289455	-.004448	.0144609

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3998183	4.764373	.0051889	.0019882	289.5974	-.006432	.0711921
Stddev	.0011051	.051704	.0004781	.0008014	1.2041	.002154	.0004937
%RSD	.2763954	1.085220	9.214397	40.30822	.4157904	33.49010	.6934931

#1	.3985434	4.798572	.0055985	.0012896	289.9777	-.005772	.0717618
#2	.4005022	4.789655	.0046635	.0018118	288.2491	-.004685	.0708879
#3	.4004093	4.704893	.0053046	.0028630	290.5655	-.008839	.0709267

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.116341	.0073872	.0507509	.0025088	.8031428	.8937235	.0009565
Stddev	.276266	.0022326	.0010889	.0003565	.0029682	.0034363	.0009469
%RSD	24.74746	30.22186	2.145497	14.21098	.3695774	.3844983	98.99536

#1	1.140131	.0050694	.0496222	.0023592	.7999865	.8955797	.0004835
#2	.828949	.0075690	.0508357	.0022514	.8035637	.8897582	.0020467
#3	1.379943	.0095234	.0517950	.0029157	.8058780	.8958326	.0003393

Sample Name: Q1292-01LX5 Acquired: 02/12/2025 13:56:38 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9L Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.002604	.2296351	.0273411
Stddev	.003675	.0003624	.0026599
%RSD	141.1465	.1578271	9.728700

#1	.001499	.2300044	.0243191
#2	-.003717	.2292799	.0283772
#3	-.005594	.2296212	.0293271

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4086.430	34476.79	4303.471	2856.763	4199.102
Stddev	23.012	82.20	8.644	7.711	19.106
%RSD	.5631286	.2384323	.2008507	.2699236	.4549923

#1	4061.268	34531.25	4312.621	2862.202	4178.890
#2	4106.408	34382.23	4302.347	2847.939	4216.865
#3	4091.613	34516.88	4295.444	2860.149	4201.552

Sample Name: Q1292-03 Acquired: 02/12/2025 14:00:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9S Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0404346	.0632650	.0136883	.0917339	.0847349	1.960236
Stddev	.0029215	.0008149	.0016226	.0009952	.0034157	.013343
%RSD	7.225287	1.288012	11.85413	1.084913	4.031017	.6806678

#1	.0410747	.0626734	.0118477	.0928169	.0817441	1.955336
#2	.0372461	.0641945	.0143050	.0908596	.0840035	1.950036
#3	.0429831	.0629272	.0149122	.0915250	.0884570	1.975336

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.151378	.0485325	.0559611	F 1001.271	.2179120	.5499443
Stddev	.016889	.0002364	.0001681	6.318	.0005138	.0015507
%RSD	.4068206	.4870877	.3003778	.6309973	.2357772	.2819650

#1	4.170317	.0484262	.0561297	994.235	.2181973	.5505793
#2	4.145935	.0488033	.0557935	1006.459	.2173189	.5481769
#3	4.137881	.0483679	.0559601	1003.119	.2182198	.5510766

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2508765	1.007452	2.035369	22.02236	.5413476	.0398387
Stddev	.0018632	.014154	.003473	.03160	.0010086	.0002060
%RSD	.7426728	1.404958	.1706563	.1435097	.1863110	.5170839

#1	.2488711	1.008900	2.035558	21.98901	.5418891	.0396903
#2	.2512043	.992630	2.031805	22.05186	.5401839	.0400739
#3	.2525539	1.020827	2.038744	22.02620	.5419697	.0397518

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	F 1525.046	.5028533	.8860490	F -5.19901	.0261410	.2044972
Stddev	2.691	.0039609	.0016737	.14620	.0018976	.0013591
%RSD	.1764377	.7876847	.1888965	2.812150	7.259002	.6645895

#1	1527.678	.5030748	.8879811	-5.30014	.0278536	.2038109
#2	1522.300	.4987862	.8850428	-5.26552	.0264682	.2060626
#3	1525.159	.5066987	.8851231	-5.03138	.0241010	.2036181

Sample Name: Q1292-03 Acquired: 02/12/2025 14:00:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: E1PM9S Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0010816	3.693975	3.653945	-.003491	-.017327	1.204867
Stddev	.0005414	.012182	.019888	.000954	.001232	.002189
%RSD	50.05402	.3297788	.5442885	27.33378	7.109864	.1816791
#1	.0014775	3.705877	3.636078	-.003080	-.018657	1.207392
#2	.0013028	3.681531	3.650384	-.002811	-.017100	1.203505
#3	.0004647	3.694517	3.675373	-.004582	-.016225	1.203704

Elem	Li6707
Units	ppm
Avg	.0305057
Stddev	.0013857
%RSD	4.542375
#1	.0292711
#2	.0320044
#3	.0302416

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3845.633	32226.65	4345.809	2700.459	3741.637
Stddev	16.211	105.69	10.127	3.211	7.079
%RSD	.4215402	.3279489	.2330348	.1188951	.1891980
#1	3861.749	32106.47	4351.319	2698.855	3745.369
#2	3829.329	32268.40	4351.986	2704.155	3733.473
#3	3845.822	32305.09	4334.121	2698.366	3746.070

Sample Name: PB166667BL Acquired: 02/12/2025 14:04:42 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: PBW667 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0002993	.0005271	-.000799	.0006991	-.000448	.0071219
Stddev	.0047117	.0006645	.002138	.0016546	.001421	.0188223
%RSD	1574.175	126.0613	267.5002	236.6665	317.0316	264.2888

#1	.0023200	.0008635	-.000650	.0026043	-.002080	-.003032
#2	-.005086	-.000238	.001260	-.000130	.000218	-.004443
#3	.003664	.000956	-.003008	-.000377	.000518	.028841

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003229	.0001245	.0000002	.0159623	-.000252	-.000056
Stddev	.000728	.0001544	.0000837	.0210812	.000224	.000226
%RSD	22.55284	124.0187	36212.05	132.0683	88.85409	407.1695

#1	-.003822	-.000023	-.000016	-.001965	-.000494	-.000119
#2	-.002416	.000285	-.000074	.010666	-.000208	-.000243
#3	-.003448	.000111	.000091	.039187	-.000053	.000196

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.004478	.0235611	.0067446	.0040361	.0003568	-.000308
Stddev	.000527	.0223304	.0003943	.0244241	.0003256	.000799
%RSD	11.77721	94.77647	5.845526	605.1347	91.26262	259.2656

#1	-.003930	.0415151	.0066834	-.006191	.0000067	-.000919
#2	-.004982	-.001444	.0071658	-.013612	.0004131	-.000601
#3	-.004522	.030612	.0063845	.031911	.0006505	.000596

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.6268458	-.008476	-.002533	F -11.9364	.0033399	-.000280
Stddev	.7836355	.006163	.002228	.0754	.0010700	.001252
%RSD	125.0125	72.70856	87.98715	.6315962	32.03566	446.5363

#1	1.515579	-.014278	-.000549	-11.8497	.0045264	-.000561
#2	.329785	-.009143	-.002105	-11.9868	.0030449	.001088
#3	.035173	-.002007	-.004944	-11.9727	.0024484	-.001368

Sample Name: PB166667BL Acquired: 02/12/2025 14:04:42 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: PBW667 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0002070	.0001788	-.001756	F -.009651	-.001028	-.000174
Stddev	.0001760	.0001016	.001889	.000274	.000852	.000284
%RSD	85.02627	56.83063	107.5810	2.840361	82.91775	163.5656
#1	.0000991	.0002357	-.003926	-.009356	-.001563	-.000221
#2	.0004101	.0002394	-.000862	-.009898	-.001475	-.000431
#3	.0001118	.0000615	-.000480	-.009697	-.000045	.000131

Elem	Li6707
Units	ppm
Avg	-.005756
Stddev	.004531
%RSD	78.70547
#1	-.010888
#2	-.002308
#3	-.004073

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4623.089	39982.99	4453.538	3233.506	5667.566
Stddev	7.592	186.43	9.466	22.678	9.434
%RSD	.1642249	.4662692	.2125590	.7013538	.1664476
#1	4619.706	39793.85	4464.408	3214.996	5661.709
#2	4631.785	40166.58	4447.099	3258.803	5678.448
#3	4617.777	39988.54	4449.110	3226.719	5662.540

Sample Name: PB166667BS Acquired: 02/12/2025 14:08:47 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LCS667 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0238388	.0528574	.0165120	.0718398	.1149970	.4262203
Stddev	.0017106	.0005600	.0015545	.0017434	.0016214	.0219799
%RSD	7.175734	1.059516	9.414059	2.426727	1.409930	5.156929

#1	.0218848	.0523892	.0179110	.0698581	.1164440	.4054924
#2	.0250659	.0534778	.0148386	.0731374	.1132446	.4492681
#3	.0245658	.0527052	.0167864	.0725237	.1153024	.4239004

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4038085	.0107077	.0093122	10.30560	.0207657	.0992929
Stddev	.0040818	.0000502	.0000718	.04138	.0003285	.0005786
%RSD	1.010835	.4689727	.7714645	.4014980	1.581853	.5827273

#1	.4081472	.0106784	.0093504	10.35289	.0206282	.0999218
#2	.4000443	.0106790	.0092293	10.27606	.0205284	.0987831
#3	.4032340	.0107657	.0093568	10.28784	.0211406	.0991738

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0514409	.2225223	.0340318	10.31235	.0740157	.0194639
Stddev	.0079157	.0058948	.0002978	.06103	.0007672	.0006633
%RSD	15.38805	2.649089	.8749665	.5918081	1.036556	3.407623

#1	.0586719	.2183544	.0342984	10.36458	.0748481	.0188883
#2	.0429835	.2199457	.0340864	10.24526	.0738619	.0201892
#3	.0526674	.2292667	.0337105	10.32719	.0733370	.0193142

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.798564	.1008132	.1120166	F -1.75838	.0193435	F -.001169
Stddev	.194510	.0040425	.0021804	.22263	.0018570	.002001
%RSD	1.985088	4.009916	1.946455	12.66110	9.600234	171.1756

#1	9.676028	.1043749	.1100971	-1.54085	.0191912	-.003209
#2	10.02284	.1016453	.1115655	-1.98579	.0212720	.000790
#3	9.69682	.0964193	.1143872	-1.74851	.0175674	-.001088

Sample Name: PB166667BS Acquired: 02/12/2025 14:08:47 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LCS667 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0209980	.1694659	F 1.034842	F .0038484	.1982706	F .0604318
Stddev	.0002431	.0025555	.002309	.0010788	.0022310	.0001930
%RSD	1.157784	1.507973	.2231236	28.03245	1.125243	.3193926
#1	.0212016	.1722955	1.032179	.0038495	.1991058	.0604572
#2	.0210634	.1673262	1.036053	.0049267	.1957425	.0602273
#3	.0207288	.1687760	1.036293	.0027691	.1999635	.0606109

Elem	Li6707
Units	ppm
Avg	.0245736
Stddev	.0023695
%RSD	9.642408
#1	.0222693
#2	.0244482
#3	.0270033

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4510.066	38662.07	4423.333	3132.547	5192.499
Stddev	17.847	441.20	20.727	38.556	19.606
%RSD	.3957168	1.141164	.4685862	1.230830	.3775922
#1	4502.674	38852.86	4399.413	3146.667	5179.360
#2	4530.422	38975.76	4435.998	3162.052	5215.036
#3	4497.103	38157.58	4434.587	3088.921	5183.103

Sample Name: Q1314-08 Acquired: 02/12/2025 14:12:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0016587	.0023678	-.000840	-.000284	-.000116	.0518795	.0104365
Stddev	.0012810	.0012131	.000819	.001914	.001808	.0113036	.0018693
%RSD	77.23264	51.23542	97.51392	674.5029	1558.717	21.78817	17.91089

#1	.0022736	.0036985	-.000212	.000942	.001916	.0388629	.0125242
#2	.0025163	.0020813	-.001767	.000696	-.000715	.0592224	.0098674
#3	.0001861	.0013235	-.000541	-.002490	-.001549	.0575532	.0089179

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000104	-.000029	10.86440	-.000161	.0080066	-.005236	.2929792
Stddev	.0001592	.000048	.04945	.000165	.0003347	.003821	.0138014
%RSD	1527.076	166.7741	.4551182	102.7648	4.180973	72.97797	4.710722

#1	.0001589	-.000046	10.91225	.000030	.0077191	-.001899	.2900399
#2	.0000301	-.000067	10.81350	-.000251	.0083741	-.004405	.3080136
#3	-.000158	.000025	10.86747	-.000260	.0079265	-.009405	.2808843

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1094986	2.455277	.0032493	.0000770	5.639987	-.002401	.0250838
Stddev	.0006853	.036039	.0002328	.0003623	.231373	.004729	.0011911
%RSD	.6258364	1.467833	7.165672	470.4187	4.102369	196.9937	4.748402

#1	.1102884	2.483884	.0033952	.0000818	5.907105	.002635	.0237288
#2	.1091463	2.414800	.0033719	-.000288	5.502025	-.006748	.0255573
#3	.1090612	2.467147	.0029808	.000437	5.510832	-.003089	.0259654

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-3.52809	.0059145	.0175493	.0143363	1.785457	1.149174	-.009063
Stddev	.15540	.0018954	.0010011	.0000921	.002912	.007303	.000240
%RSD	4.404552	32.04717	5.704415	.6424686	.1630994	.6354741	2.647030

#1	-3.69398	.0038574	.0187025	.0143555	1.783925	1.149020	-.009207
#2	-3.50437	.0075903	.0170421	.0142361	1.788815	1.141949	-.008786
#3	-3.38591	.0062957	.0169033	.0144174	1.783630	1.156552	-.009196

Sample Name: Q1314-08 Acquired: 02/12/2025 14:12:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0008582	.0498248	-.000627
Stddev	.0016311	.0001337	.003674
%RSD	190.0635	.2682839	586.2039

#1	.0002130	.0498484	-.000827
#2	-.000352	.0496808	-.004196
#3	.002713	.0499450	.003144

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4558.055	39233.61	4417.049	3175.925	5327.404
Stddev	5.260	172.83	29.957	10.563	14.545
%RSD	.1154020	.4405115	.6782150	.3325851	.2730246

#1	4563.495	39185.27	4384.942	3164.004	5343.030
#2	4552.996	39090.10	4444.251	3179.656	5314.260
#3	4557.673	39425.46	4421.954	3184.116	5324.921

Sample Name: Q1314-09 Acquired: 02/12/2025 14:16:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9D Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000807	.0026566	-.002304	.0004437	-.002159	.0548117	.0135787
Stddev	.003166	.0013176	.000149	.0023708	.001506	.0223234	.0029880
%RSD	392.2751	49.59762	6.467785	534.3766	69.73776	40.72742	22.00478
#1	-.002755	.0024582	-.002269	-.000495	-.003201	.0757359	.0156820
#2	.002846	.0014495	-.002467	.003140	-.000433	.0573866	.0101585
#3	-.002512	.0040622	-.002174	-.001314	-.002843	.0313125	.0148956
Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0001372	.0000295	10.92955	-.000267	.0082930	-.004918	.2962374
Stddev	.0001536	.0000632	.04787	.000847	.0001981	.002032	.0178855
%RSD	111.9262	213.9786	.4379559	316.7325	2.388717	41.30889	6.037570
#1	.0003102	-.000040	10.87731	-.000223	.0083501	-.007254	.3161771
#2	.0000169	.000045	10.97131	.000556	.0084562	-.003938	.2909257
#3	.0000845	.000083	10.94002	-.001136	.0080726	-.003563	.2816094
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1105515	2.467298	.0033710	.0009763	6.017567	.0018292	.0256169
Stddev	.0017843	.036380	.0000435	.0009212	.247976	.0069656	.0028619
%RSD	1.614012	1.474498	1.291597	94.35367	4.120867	380.7942	11.17194
#1	.1113372	2.484610	.0033334	.0013169	6.302631	-.001563	.0242813
#2	.1085092	2.425495	.0033609	-.000067	5.851670	-.002791	.0236669
#3	.1118082	2.491790	.0034187	.001679	5.898400	.009841	.0289024
Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-3.52216	.0044850	.0175310	.0138336	1.786954	1.144567	-.008658
Stddev	.12118	.0010161	.0019769	.0005201	.004844	.005856	.000115
%RSD	3.440413	22.65545	11.27690	3.759887	.2710802	.5116114	1.329336
#1	-3.48760	.0050590	.0195747	.0134824	1.792338	1.151042	-.008777
#2	-3.65686	.0033118	.0173900	.0144311	1.782948	1.139643	-.008650
#3	-3.42202	.0050842	.0156283	.0135872	1.785576	1.143017	-.008547

Sample Name: Q1314-09 Acquired: 02/12/2025 14:16:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9D Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0004029	.0500467	-.001841
Stddev	.0010586	.0002208	.004483
%RSD	262.7423	.4412484	243.5793

#1	-.000818	.0502622	.001398
#2	.001068	.0498209	.000037
#3	.000958	.0500568	-.006958

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4553.475	39299.93	4442.053	3180.353	5328.558
Stddev	8.416	131.65	16.330	8.485	7.958
%RSD	.1848173	.3349902	.3676137	.2667989	.1493507

#1	4563.179	39192.56	4427.409	3170.972	5337.302
#2	4549.073	39446.81	4459.662	3187.492	5326.633
#3	4548.174	39260.41	4439.088	3182.594	5321.739

Sample Name: Q1314-08LX5 Acquired: 02/12/2025 14:20:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9L Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0001347	.0019422	-.001625	-.000339	-.001073	.0149592	.0032197
Stddev	.0005525	.0013856	.000681	.002970	.000630	.0191160	.0002271
%RSD	410.2002	71.34283	41.90813	876.7171	58.71585	127.7873	7.054911

#1	.0007521	.0004155	-.002012	-.001851	-.000346	.0257639	.0030323
#2	-.000313	.0031201	-.002023	-.002249	-.001415	-.007112	.0031546
#3	-.000035	.0022911	-.000838	.003083	-.001458	.026226	.0034723

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000177	-.000001	2.231150	-.000223	.0018134	-.008163	.0688169
Stddev	.0001146	.000040	.035241	.000090	.0001936	.001566	.0114432
%RSD	647.6668	3938.921	1.579479	40.13926	10.67404	19.17965	16.62853

#1	-.000111	.000022	2.206166	-.000131	.0018336	-.009540	.0564597
#2	.000056	.000022	2.215826	-.000229	.0016105	-.008488	.0709431
#3	.000108	-.000047	2.271459	-.000310	.0019960	-.006460	.0790479

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0222104	.4784068	.0004964	.0006625	1.451817	.0007625	.0044420
Stddev	.0011364	.0316953	.0001535	.0007970	.215520	.0031889	.0027400
%RSD	5.116564	6.625183	30.91687	120.2977	14.84485	418.2128	61.68387

#1	.0232548	.4971030	.0006659	.0002310	1.439435	.0023830	.0061556
#2	.0210002	.4418111	.0004569	.0001743	1.673261	.0028157	.0058884
#3	.0223760	.4963063	.0003666	.0015822	1.242755	-.002911	.0012819

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1545976	.0018825	.0026860	.0030769	.3459526	.2268532	-.002019
Stddev	.2725769	.0010258	.0013931	.0001453	.0026523	.0006096	.000822
%RSD	176.3138	54.49393	51.86527	4.721135	.7666581	.2687271	40.68493

#1	-.127914	.0024162	.0041290	.0031247	.3487095	.2262118	-.001081
#2	.175694	.0025314	.0025800	.0029138	.3457291	.2274250	-.002609
#3	.416014	.0006998	.0013489	.0031923	.3434191	.2269227	-.002367

Sample Name: Q1314-08LX5 Acquired: 02/12/2025 14:20:43 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9L Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.000987	.0102149	.0102547
Stddev	.002303	.0002531	.0052587
%RSD	233.4786	2.477483	51.28090
#1	-.003617	.0105043	.0048676
#2	-.000013	.0101051	.0105218
#3	.000670	.0100353	.0153748

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4314.030	37778.57	4202.433	3018.543	5100.963
Stddev	11.317	207.92	7.927	19.061	4.901
%RSD	.2623388	.5503745	.1886213	.6314707	.0960797
#1	4325.716	37768.36	4206.276	2996.995	5105.097
#2	4313.252	37991.41	4207.706	3033.203	5102.245
#3	4303.121	37575.94	4193.318	3025.431	5095.549

Sample Name: Q1314-10 Acquired: 02/12/2025 14:24:45 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9S Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0484862	.0515690	.0170707	.0961748	.0972537	1.980031	2.031277
Stddev	.0017468	.0014465	.0016703	.0032556	.0019264	.028417	.002528
%RSD	3.602734	2.804970	9.784783	3.385045	1.980783	1.435205	.1244575

#1	.0497956	.0518175	.0163368	.0950336	.0950868	1.973598	2.030751
#2	.0491603	.0500144	.0158929	.0936436	.0987724	1.955382	2.034026
#3	.0465028	.0528752	.0189823	.0998474	.0979019	2.011114	2.029053

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0532718	.0449830	10.66515	.2159844	.4684369	.2525956	1.319396
Stddev	.0005988	.0002164	.04173	.0017919	.0013304	.0090187	.008277
%RSD	1.124115	.4811260	.3912735	.8296238	.2839994	3.570415	.6273294

#1	.0539160	.0448741	10.67906	.2155884	.4669544	.2562114	1.324209
#2	.0527320	.0448426	10.69815	.2144236	.4688294	.2423300	1.324140
#3	.0531675	.0452322	10.61824	.2179411	.4695268	.2592452	1.309839

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.6392339	2.356740	.4673785	.0369987	5.578017	.5047914	.4731432
Stddev	.0056846	.005872	.0010242	.0008011	.679719	.0088498	.0042934
%RSD	.8892834	.2491765	.2191352	2.165147	12.18567	1.753168	.9074199

#1	.6371904	2.360480	.4662543	.0362354	6.238456	.5060229	.4709149
#2	.6348535	2.359770	.4676226	.0378329	4.880534	.4953903	.4780926
#3	.6456578	2.349972	.4682586	.0369278	5.615061	.5129609	.4704221

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-3.47518	.0060906	.0162418	.0133707	1.802715	1.127506	-.009301
Stddev	.03173	.0001420	.0012682	.0005433	.002870	.005984	.000335
%RSD	.9130119	2.331004	7.808207	4.063423	.1591830	.5307486	3.606035

#1	-3.44483	.0059598	.0175372	.0132763	1.805112	1.134297	-.008965
#2	-3.50813	.0062416	.0150027	.0139551	1.803498	1.123002	-.009636
#3	-3.47258	.0060703	.0161854	.0128808	1.799535	1.125220	-.009303

Sample Name: Q1314-10 Acquired: 02/12/2025 14:24:45 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA9S Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0005833	.0477604	.0017567
Stddev	.0021016	.0001146	.0034612
%RSD	360.2897	.2399606	197.0329

#1	-.000907	.0478312	.0010137
#2	-.000330	.0478218	-.001273
#3	.002987	.0476282	.005529

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4522.601	39005.58	4401.525	3170.370	5290.403
Stddev	2.885	230.86	6.968	18.481	5.322
%RSD	.0637804	.5918592	.1583100	.5829141	.1005941

#1	4520.078	39272.12	4394.009	3191.513	5285.958
#2	4521.979	38875.80	4402.794	3162.297	5296.300
#3	4525.746	38868.81	4407.771	3157.299	5288.952

Sample Name: Q1315-01 Acquired: 02/12/2025 14:28:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001071	.0048201	-.002566	-.001299	-.003354	.0273325	.0354175
Stddev	.002886	.0023683	.001611	.001918	.000449	.0288339	.0011674
%RSD	269.5573	49.13410	62.79563	147.6665	13.37649	105.4932	3.296173

#1	-.002633	.0075244	-.001179	-.003473	-.002861	.0197946	.0340928
#2	-.002839	.0031155	-.004333	-.000577	-.003463	.0591866	.0362962
#3	.002260	.0038205	-.002186	.000153	-.003738	.0030162	.0358634

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000112	.0000961	26.64938	.0003333	.0165129	.0018744	.4347901
Stddev	.0000862	.0000743	.09665	.0013679	.0002366	.0043692	.0104941
%RSD	769.0716	77.30087	.3626899	410.4523	1.432966	233.1063	2.413609

#1	.0000970	.0001816	26.55615	.0019020	.0166077	.0044420	.4448748
#2	-.000075	.0000592	26.64288	-.000291	.0166874	-.003171	.4355659
#3	.000012	.0000475	26.74913	-.000611	.0162436	.004352	.4239296

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2444120	6.202224	.0078070	.0002758	14.73259	.0003933	.0670105
Stddev	.0022077	.035339	.0005370	.0011275	.08602	.0025919	.0027352
%RSD	.9032552	.5697715	6.878906	408.8132	.5838987	659.0349	4.081818

#1	.2419962	6.175673	.0083763	.0008353	14.82402	-.002578	.0698137
#2	.2449149	6.188664	.0077351	.0010141	14.65326	.002191	.0643487
#3	.2463248	6.242334	.0073095	-.001022	14.72048	.001566	.0668691

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.283986	.0066862	.0474076	.0282407	3.556893	3.111294	-.009598
Stddev	.107730	.0023204	.0010868	.0002233	.008758	.017633	.000218
%RSD	1.160388	34.70381	2.292477	.7906237	.2462126	.5667347	2.276461

#1	9.296194	.0063110	.0461799	.0282124	3.547030	3.092652	-.009559
#2	9.170671	.0045763	.0477962	.0284768	3.563755	3.127705	-.009833
#3	9.385092	.0091713	.0482467	.0280329	3.559895	3.113525	-.009402

Sample Name: Q1315-01 Acquired: 02/12/2025 14:28:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0010035	.1300510	.0050556
Stddev	.0025853	.0008778	.0017101
%RSD	257.6302	.6749841	33.82587
#1	-.001482	.1291939	.0039542
#2	.000815	.1300109	.0070257
#3	.003678	.1309482	.0041869

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4456.976	38187.56	4388.369	3137.058	5056.066
Stddev	9.756	73.44	24.983	9.015	4.083
%RSD	.2188922	.1923122	.5693068	.2873675	.0807458
#1	4461.082	38156.66	4406.984	3135.157	5055.798
#2	4464.009	38271.40	4398.148	3146.872	5060.277
#3	4445.839	38134.62	4359.976	3129.146	5052.125

Sample Name: Q1315-02 Acquired: 02/12/2025 14:32:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8D Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0016443	.0043914	-.001707	-.003668	-.002751	.0101041	.0380775
Stddev	.0015005	.0001721	.000723	.002158	.004071	.0218182	.0005849
%RSD	91.25414	3.919500	42.34751	58.83754	147.9709	215.9342	1.535980

#1	.0031786	.0045889	-.002332	-.001330	.000285	-.014419	.0374370
#2	.0015741	.0043118	-.000916	-.005584	-.007378	.017367	.0382123
#3	.0001801	.0042735	-.001872	-.004091	-.001161	.027364	.0385831

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000646	.0000059	26.77404	.0001619	.0164032	-.001778	.4383086
Stddev	.0000698	.0000750	.02817	.0004568	.0003052	.004519	.0156539
%RSD	107.9767	1261.309	.1052245	282.0759	1.860814	254.1964	3.571440

#1	.0000564	-.000066	26.78464	.0006684	.0166616	-.006568	.4395969
#2	.0001381	-.000000	26.79537	-.000219	.0164817	.002409	.4532786
#3	-.000001	.000084	26.74210	.000036	.0160664	-.001174	.4220503

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2452690	6.263664	.0079625	.0005982	14.94243	.0011420	.0629715
Stddev	.0017589	.057483	.0006017	.0003037	.71192	.0020833	.0012790
%RSD	.7171207	.9177158	7.556544	50.76822	4.764446	182.4132	2.031137

#1	.2434136	6.203829	.0084865	.0007611	14.24955	.0035397	.0642878
#2	.2454814	6.318462	.0080957	.0002478	14.90577	.0001118	.0617333
#3	.2469121	6.268700	.0073054	.0007856	15.67198	-.000225	.0628934

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.423126	.0043870	.0484894	.0287089	3.586885	3.144125	-.008097
Stddev	.146121	.0013162	.0012578	.0005223	.004219	.014813	.000451
%RSD	1.550667	30.00147	2.593881	1.819353	.1176240	.4711232	5.569667

#1	9.485862	.0052990	.0498066	.0286996	3.582653	3.155223	-.007639
#2	9.527403	.0028781	.0483607	.0281913	3.586910	3.127305	-.008113
#3	9.256113	.0049838	.0473010	.0292358	3.591091	3.149846	-.008540

Sample Name: Q1315-02 Acquired: 02/12/2025 14:32:39 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8D Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.000323	.1312578	.0054637
Stddev	.002462	.0003553	.0046352
%RSD	762.8456	.2707199	84.83467

#1	.001633	.1313655	.0093407
#2	-.003087	.1315468	.0003297
#3	.000486	.1308611	.0067208

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4510.613	38935.61	4447.355	3155.436	5101.942
Stddev	1.490	140.99	25.888	13.532	4.497
%RSD	.0330327	.3621065	.5821000	.4288440	.0881412

#1	4510.597	38928.31	4417.607	3142.392	5097.064
#2	4509.131	38798.42	4464.768	3169.408	5102.840
#3	4512.111	39080.11	4459.692	3154.510	5105.923

Sample Name: Q1315-01LX5 Acquired: 02/12/2025 14:36:40 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8L Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001750	.0008985	-.000910	.0001347	-.000346	.0217920	.0106523
Stddev	.002228	.0032294	.000231	.0014554	.002421	.0102912	.0008968
%RSD	127.3109	359.4169	25.37615	1080.340	699.6656	47.22471	8.418664

#1	-.001870	.0000098	-.001177	-.000657	-.002229	.0151235	.0115324
#2	-.003916	-.001793	-.000786	.001814	.002385	.0336443	.0106847
#3	.000536	.004479	-.000768	-.000753	-.001195	.0166082	.0097398

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000156	.0001233	5.562907	-.000630	.0047422	-.006516	.1123237
Stddev	.000172	.0000426	.009554	.000230	.0003697	.005231	.0352004
%RSD	110.1997	34.55004	.1717466	36.43339	7.796526	80.28404	31.33834

#1	-.000349	.0001664	5.554294	-.000380	.0043199	-.004250	.1520228
#2	-.000099	.0001224	5.561244	-.000678	.0050077	-.002800	.1000272
#3	-.000020	.0000812	5.573184	-.000832	.0048990	-.012498	.0849210

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0522480	1.294139	.0018987	.0006497	3.102368	-.000818	.0142118
Stddev	.0002146	.015394	.0002580	.0009907	.434424	.006191	.0039125
%RSD	.4107369	1.189523	13.58839	152.4809	14.00297	757.0049	27.53013

#1	.0522346	1.306764	.0017466	.0004163	2.999785	-.007005	.0119857
#2	.0524689	1.298662	.0017529	.0017362	2.728417	-.000826	.0187294
#3	.0520403	1.276990	.0021966	-.000203	3.578903	.005377	.0119203

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.205566	-.000865	.0104831	.0060398	.6973926	.6299170	-.001349
Stddev	.135938	.000657	.0010492	.0004730	.0024233	.0074484	.000476
%RSD	6.163402	75.99629	10.00858	7.831227	.3474876	1.182434	35.32641

#1	2.342037	-.000133	.0096717	.0057560	.6998420	.6366278	-.000833
#2	2.070167	-.001056	.0101096	.0057775	.6973397	.6312200	-.001439
#3	2.204493	-.001405	.0116679	.0065858	.6949961	.6219031	-.001773

Sample Name: Q1315-01LX5 Acquired: 02/12/2025 14:36:40 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8L Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.002347	.0273873	.0095946
Stddev	.003669	.0001351	.0027186
%RSD	156.3085	.4931083	28.33466
#1	-.003772	.0273799	.0101691
#2	.001820	.0272561	.0119800
#3	-.005089	.0275259	.0066346

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4402.380	38176.21	4333.253	3060.715	5119.822
Stddev	5.252	138.17	18.215	20.626	5.442
%RSD	.1193104	.3619139	.4203437	.6739028	.1062962
#1	4396.461	38209.10	4317.388	3060.397	5115.971
#2	4406.486	38294.96	4329.228	3081.498	5126.048
#3	4404.192	38024.57	4353.144	3040.250	5117.449

Sample Name: Q1315-03 Acquired: 02/12/2025 14:40:42 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8S Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0478048	.0545450	.0155497	.0949813	.0964707	1.991976	2.074616
Stddev	.0021827	.0009142	.0005444	.0018118	.0020127	.024912	.008703
%RSD	4.565776	1.675977	3.500969	1.907495	2.086295	1.250631	.4194849

#1	.0503126	.0545446	.0149266	.0931527	.0961432	1.971883	2.083811
#2	.0467673	.0536310	.0159331	.0967758	.0946419	1.984196	2.073530
#3	.0463343	.0554594	.0157893	.0950152	.0986270	2.019850	2.066507

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0545770	.0469486	26.90465	.2157857	.4923351	.2532694	1.518512
Stddev	.0006060	.0001574	.08848	.0010717	.0005676	.0040686	.015375
%RSD	1.110301	.3353195	.3288667	.4966573	.1152877	1.606417	1.012488

#1	.0543520	.0471302	27.00248	.2148749	.4920034	.2524214	1.504028
#2	.0541156	.0468520	26.88122	.2155154	.4920114	.2576952	1.534645
#3	.0552632	.0468635	26.83024	.2169666	.4929905	.2496917	1.516863

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.7749368	6.336698	.4885911	.0359219	15.55797	.5248031	.5250688
Stddev	.0007133	.020343	.0005582	.0014281	.78830	.0063660	.0034631
%RSD	.0920496	.3210345	.1142493	3.975689	5.066850	1.213022	.6595431

#1	.7757361	6.346500	.4879467	.0362540	16.34097	.5276766	.5290343
#2	.7747093	6.313309	.4888987	.0343570	15.56845	.5292257	.5226399
#3	.7743649	6.350284	.4889279	.0371548	14.76448	.5175069	.5235322

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.819782	.0052499	.0503883	.0279029	3.555076	3.204889	-.009533
Stddev	.180867	.0028705	.0011665	.0001580	.003959	.016904	.000614
%RSD	1.841863	54.67627	2.315019	.5663061	.1113586	.5274456	6.445289

#1	9.611356	.0021260	.0499939	.0280732	3.551145	3.203821	-.009698
#2	9.912523	.0077713	.0494701	.0278742	3.555020	3.188545	-.008853
#3	9.935468	.0058525	.0517009	.0277611	3.559062	3.222302	-.010048

Sample Name: Q1315-03 Acquired: 02/12/2025 14:40:42 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: MBHHA8S Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.000056	.1316911	.0061584
Stddev	.003572	.0002289	.0032677
%RSD	6412.714	.1737951	53.06047
#1	.002630	.1316752	.0025303
#2	.001312	.1314707	.0088698
#3	-.004109	.1319276	.0070752

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4462.906	38628.09	4359.364	3129.340	5034.992
Stddev	18.824	174.05	32.881	13.538	14.132
%RSD	.4217928	.4505715	.7542501	.4326130	.2806792
#1	4483.632	38804.43	4385.913	3144.052	5049.923
#2	4458.212	38623.41	4369.595	3126.561	5033.229
#3	4446.872	38456.43	4322.584	3117.407	5021.824

Sample Name: PB166670BL Acquired: 02/12/2025 14:57:38 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: PBW670 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0003228	.0009221	-.000874	.0002341	-.000738	.0162616	.0006964
Stddev	.0024511	.0001611	.000693	.0019567	.000852	.0065654	.0005991
%RSD	759.3591	17.47552	79.32002	835.6703	115.5365	40.37365	86.03525

#1	.0031369	.0007847	-.001302	.0020804	-.000119	.0216096	.0013637
#2	-.000822	.0008822	-.000074	.0004389	-.000385	.0089343	.0002047
#3	-.001346	.0010994	-.001245	-.001817	-.001710	.0182410	.0005208

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000375	.0000250	.0076838	-.000414	-.000224	-.006451	.0160573
Stddev	.0001258	.0000323	.0214744	.000147	.000362	.005528	.0084003
%RSD	335.9382	129.0963	279.4773	35.46894	161.2931	85.68932	52.31442

#1	-.000103	.0000611	.0314353	-.000362	-.000153	-.001875	.0210193
#2	.000077	-.000001	-.010361	-.000580	-.000616	-.004884	.0063584
#3	.000139	.000015	.001977	-.000300	.000097	-.012592	.0207943

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000297	-.013667	-.000054	.0005035	.1077125	-.001491	-.002226
Stddev	.000642	.020932	.000129	.0011693	.3945350	.002574	.001383
%RSD	216.4828	153.1651	238.3979	232.2390	366.2853	172.6545	62.10065

#1	-.000849	-.017711	-.000199	-.000462	.0411197	-.002760	-.002521
#2	-.000448	.008993	.000047	.001804	-.249288	-.003184	-.000720
#3	.000408	-.032281	-.000010	.000169	.531306	.001471	-.003438

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.5515887	.0004301	.0094844	.0005233	-.000239	.0005259	.0005822
Stddev	.0642256	.0026525	.0014250	.0000146	.000813	.0003538	.0005872
%RSD	11.64375	616.6574	15.02511	2.792717	340.5959	67.27645	100.8689

#1	.4806183	.0006927	.0087354	.0005397	-.000793	.0008881	.0012484
#2	.5684370	.0029416	.0085901	.0005118	-.000618	.0001811	.0003580
#3	.6057107	-.002344	.0111277	.0005183	.000695	.0005084	.0001400

Sample Name: PB166670BL Acquired: 02/12/2025 14:57:38 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: PBW670 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	.0011969	-.000149	.0118796
Stddev	.0010599	.000028	.0043838
%RSD	88.55084	18.67524	36.90228
#1	.0021012	-.000124	.0133463
#2	.0014591	-.000179	.0069505
#3	.0000306	-.000145	.0153420

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4438.584	38699.83	4335.235	3112.723	5309.988
Stddev	7.760	137.97	10.563	7.003	11.333
%RSD	.1748347	.3565022	.2436625	.2249863	.2134269
#1	4435.994	38846.78	4329.650	3114.785	5302.224
#2	4447.308	38679.64	4347.419	3118.464	5322.993
#3	4432.450	38573.07	4328.637	3104.921	5304.748

Sample Name: PB166670BS Acquired: 02/12/2025 15:01:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LCS670 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0248918	.0529841	.0157824	.0682885	.1147844	.4268937
Stddev	.0022173	.0009864	.0018337	.0046170	.0009252	.0139642
%RSD	8.907721	1.861683	11.61875	6.761005	.8060574	3.271124

#1	.0274008	.0531887	.0137678	.0632166	.1154283	.4382449
#2	.0231954	.0538521	.0173541	.0722469	.1152009	.4311360
#3	.0240792	.0519114	.0162252	.0694019	.1137242	.4113003

Elem	Ba4934	Be2348	Cd2144	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4116964	.0106586	.0094341	10.45407	.0213639	.1010616
Stddev	.0053775	.0000757	.0001188	.03647	.0004802	.0006268
%RSD	1.306185	.7102007	1.258949	.3488216	2.247880	.6201773

#1	.4149274	.0105876	.0094079	10.44170	.0218066	.1014690
#2	.4146731	.0107383	.0093306	10.49512	.0208533	.1003399
#3	.4054887	.0106500	.0095638	10.42540	.0214318	.1013759

Elem	Cu3247	Fe2598	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0520106	.2167890	.0323343	10.13559	.0768988	.0209322
Stddev	.0059348	.0035515	.0009623	.02400	.0007824	.0009932
%RSD	11.41074	1.638243	2.976126	.2368250	1.017469	4.744953

#1	.0457007	.2198003	.0332127	10.11582	.0777365	.0219906
#2	.0528503	.2176943	.0324846	10.16230	.0761869	.0207858
#3	.0574809	.2128724	.0313057	10.12866	.0767731	.0200204

Elem	Na8183	V_2924	Zn2138	K_7698	P_1774	B_2496
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	10.68007	.1042889	.1149724	10.70087	.0181113	F .0048652
Stddev	.36779	.0015197	.0025551	.20460	.0005281	.0012211
%RSD	3.443668	1.457165	2.222354	1.911958	2.915665	25.09845

#1	10.76074	.1048860	.1132356	10.82908	.0181453	.0062270
#2	11.00083	.1025614	.1137753	10.80861	.0186216	.0045007
#3	10.27864	.1054194	.1179063	10.46492	.0175671	.0038678

Sample Name: PB166670BS Acquired: 02/12/2025 15:01:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: LCS670 Custom ID2: Custom ID3:
Comment:

Elem	Mo2020	S_1820	Si2516	Sn1899	Ti3361	Sr4077
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0211258	.1666951	F 1.009713	.0150773	.2029348	.2108940
Stddev	.0003474	.0032406	.004832	.0003554	.0003364	.0009468
%RSD	1.644512	1.944031	.4785816	2.357227	.1657423	.4489242
#1	.0207425	.1685133	1.014824	.0146967	.2030318	.2117287
#2	.0214200	.1629537	1.009098	.0154006	.2032121	.2110879
#3	.0212149	.1686184	1.005219	.0151346	.2025606	.2098653

Elem	Li6707
Units	ppm
Avg	F .0407462
Stddev	.0016510
%RSD	4.051851
#1	.0410774
#2	.0389547
#3	.0422065

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4342.008	37604.47	4297.113	3040.249	4909.368
Stddev	7.120	161.99	19.333	11.171	7.368
%RSD	.1639740	.4307768	.4499099	.3674504	.1500719
#1	4346.729	37417.63	4281.951	3027.411	4908.219
#2	4345.477	37705.73	4290.505	3047.756	4917.243
#3	4333.819	37690.03	4318.884	3045.582	4902.642

Sample Name: CCV012 Acquired: 02/12/2025 15:05:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCV012 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.777725	4.732345	24.10192	4.769474	4.867937	387.4174	9.969990
Stddev	.009777	.004550	.01938	.007787	.008012	1.8735	.017813
%RSD	.2046282	.0961488	.0804032	.1632571	.1645782	.4835813	.1786643

#1	4.786438	4.731604	24.11858	4.770782	4.875228	385.9186	9.958530
#2	4.779585	4.737221	24.10653	4.761117	4.859360	389.5177	9.990511
#3	4.767152	4.728211	24.08065	4.776524	4.869223	386.8157	9.960927

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4913589	2.436314	393.5166	15.42262	2.431237	14.59440	387.9924
Stddev	.0059788	.002867	.9669	.02322	.003615	.03990	1.4209
%RSD	1.216783	.1176829	.2457087	.1505710	.1487015	.2733641	.3662095

#1	.4921726	2.439023	392.6711	15.39967	2.433333	14.59500	386.8620
#2	.4968891	2.436608	394.5708	15.42208	2.433316	14.63399	389.5874
#3	.4850149	2.433312	393.3079	15.44611	2.427063	14.55420	387.5279

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	14.22367	383.5744	2.427489	1.253763	388.7086	2.387796	14.34134
Stddev	.03700	1.8393	.000624	.001958	1.1314	.007494	.13156
%RSD	.2601404	.4795100	.0257144	.1561439	.2910743	.3138273	.9173309

#1	14.20312	381.9496	2.428208	1.255696	387.7521	2.391918	14.24604
#2	14.26639	385.5713	2.427173	1.253812	389.9575	2.392324	14.28655
#3	14.20151	383.2023	2.427086	1.251782	388.4161	2.379147	14.49144

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	146.5797	4.883351	4.788982	4.811771	4.892491	4.589425	4.860481
Stddev	.6827	.002983	.056293	.005472	.008017	.055243	.007046
%RSD	.4657706	.0610786	1.175467	.1137192	.1638634	1.203691	.1449684

#1	145.9380	4.881889	4.794673	4.811238	4.892358	4.595543	4.868358
#2	147.2971	4.881382	4.842214	4.806585	4.900574	4.641353	4.854778
#3	146.5040	4.886783	4.730060	4.817490	4.884542	4.531377	4.858307

Sample Name: CCV012 Acquired: 02/12/2025 15:05:44 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCV012 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	4.817721	4.595279	4.994597
Stddev	.019636	.044865	.015491
%RSD	.4075888	.9763218	.3101526
#1	4.796835	4.544482	4.977183
#2	4.835807	4.629487	5.006846
#3	4.820522	4.611867	4.999760

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3677.530	31505.30	4125.277	2561.323	3689.973
Stddev	10.286	139.92	29.384	7.023	2.887
%RSD	.2796907	.4441124	.7122963	.2741952	.0782312
#1	3677.394	31582.22	4115.161	2561.045	3690.781
#2	3687.883	31589.89	4102.287	2568.481	3692.369
#3	3667.313	31343.80	4158.383	2554.443	3686.768

Sample Name: CCB012 Acquired: 02/12/2025 15:09:28 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCB012 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0007618	.0017525	-.001265	.0026277	.0006487	.0308545	-.001865
Stddev	.0009136	.0014561	.001405	.0039856	.0017060	.0031105	.001268
%RSD	119.9183	83.08545	111.0415	151.6763	262.9692	10.08131	67.97942

#1	.0018167	.0004073	.000295	.0060929	.0024835	.0278870	-.000488
#2	.0002251	.0032986	-.002431	.0035179	.0003522	.0340907	-.002123
#3	.0002437	.0015517	-.001659	-.001728	-.000890	.0305858	-.002983

Elem	Be2348	Cd2144	Ca3736	Cr2677	Co2286	Cu3247	Fe2598
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000020	.0000760	.0183258	-.000409	-.000273	-.002027	.0195654
Stddev	.000097	.0000402	.0124548	.000575	.000219	.009612	.0193095
%RSD	495.3703	52.89749	67.96285	140.7498	80.09676	474.3101	98.69187

#1	.000082	.0001217	.0041235	-.000060	-.000372	.005217	.0050864
#2	-.000029	.0000461	.0234672	-.001072	-.000022	-.012931	.0414891
#3	-.000111	.0000602	.0273868	-.000093	-.000425	.001635	.0121208

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na8183	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0017889	.0223298	-.000214	-.000058	.5130144	.0006457	.0010210
Stddev	.0005665	.0093000	.000350	.000444	.2428160	.0033392	.0002700
%RSD	31.66833	41.64853	163.2224	772.2847	47.33124	517.1543	26.44905

#1	.0023442	.0268515	-.000439	.000222	.3175088	-.001014	.0012757
#2	.0018108	.0285044	.000189	.000175	.4367189	.004490	.0007379
#3	.0012117	.0116335	-.000392	-.000570	.7848154	-.001538	.0010494

Elem	K_7698	P_1774	B_2496	Mo2020	S_1820	Si2516	Sn1899
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4384530	.0013862	.0103778	.0011997	.0009120	.0002901	-.000130
Stddev	.2500591	.0016516	.0017602	.0002190	.0025016	.0008835	.000461
%RSD	57.03213	119.1514	16.96138	18.25621	274.2956	304.5073	355.6548

#1	.1930853	.0007077	.0109028	.0009477	-.001477	-.000713	-.000658
#2	.6929532	.0001818	.0118158	.0013442	.003513	.000630	.000191
#3	.4293205	.0032690	.0084148	.0013071	.000700	.000953	.000078

Sample Name: CCB012 Acquired: 02/12/2025 15:09:28 Type: Unk
Method: SFAM01.1 INSTRUMENT P5 WITH 6 POINT ICAL-2(v136) Mode: CONC Corr. Factor: 1.00000
User: Kareem Custom ID1: CCB012 Custom ID2: Custom ID3:
Comment:

Elem	Ti3361	Sr4077	Li6707
Units	ppm	ppm	ppm
Avg	-.000157	-.000074	.0057107
Stddev	.003242	.000125	.0024359
%RSD	2067.381	168.9425	42.65576

#1	.000534	.000054	.0085044
#2	.002684	-.000081	.0040313
#3	-.003689	-.000195	.0045963

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4428.926	38435.07	4334.001	3103.548	5319.696
Stddev	14.289	102.56	31.189	4.761	12.102
%RSD	.3226393	.2668305	.7196461	.1534190	.2274919

#1	4412.949	38334.88	4368.822	3099.389	5307.179
#2	4433.346	38539.84	4308.628	3102.512	5320.573
#3	4440.483	38430.48	4324.552	3108.741	5331.335

Prep Standard - Chemical Standard Summary

Order ID : Q1315

Test : Metals CLP Full

Prepbatch ID : PB166670,

Sequence ID/Qc Batch ID: LB134696,

Standard ID :

MP83500,MP84041,MP84063,MP84070,MP84204,MP84218,MP84219,MP84230,MP84231,MP84297,MP84381,MP84382,MP84383,MP84384,MP84385,MP84386,MP84387,MP84388,MP84392,

Chemical ID :

M4884,M5130,M5223,M5289,M5298,M5393,M5429,M5472,M5476,M5496,M5497,M5498,M5513,M5519,M5565,M5658,M5697,M5798,M5799,M5800,M5801,M5802,M5806,M5811,M5815,M5817,M5819,M5875,M5942,M5959,M5961,M5962,M5970,M5976,M5977,M5978,M5985,M5990,M6021,M6023,M6025,M6028,M6030,M6032,M6077,M6121,M6126,M6127,M6128,M6144,M6145,M6146,mp84446,W3112,

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
902	ICP AES CAL BLK (SO/ICB/CCB)	MP83500	12/06/2024	01/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								12/09/2024

FROM 125.00000ml of M6121 + 2350.00000ml of W3112 + 25.00000ml of M6126 = Final Quantity: 2500.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
169	1:1HNO3	MP84041	01/14/2025	07/14/2025	Eman Mughal	None	None	Sarabjit Jaswal
								01/16/2025

FROM 1250.00000ml of M6126 + 1250.00000ml of W3112 = Final Quantity: 2500.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
994	ICPAES ISM01.2 S1 (CONC.)	MP84063	01/14/2025	02/14/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/16/2025

FROM 0.02000ml of M5815 + 0.03000ml of M5429 + 0.10000ml of M5798 + 0.10000ml of M6028 + 0.14000ml of M5799 + 0.20000ml of M5298 + 0.20000ml of M5476 + 0.20000ml of M5658 + 0.20000ml of M5801 + 0.20000ml of M5817 + 0.20000ml of M5976 + 0.20000ml of M6025 + 0.20000ml of M6030 + 0.30000ml of M6128 + 0.40000ml of M5496 + 0.50000ml of M5697 + 0.50000ml of M6023 + 0.70000ml of M5962 + 0.80000ml of M5961 + 1.00000ml of M5800 + 1.00000ml of M6021 + 1.20000ml of M5802 + 1.20000ml of M5819 + 10.00000ml of M5497 + 10.00000ml of M5519 + 10.00000ml of M5806 + 10.00000ml of M6127 + 2.00000ml of M5942 + 4.00000ml of M6032 + 34.24000ml of MP83500 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
921	ICPAES SPIKE SOL#6	MP84070	01/14/2025	02/14/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/16/2025

FROM 2.50000ml of M5962 + 50.00000ml of M5565 + 50.00000ml of M5990 + 147.50000ml of MP83500 = Final Quantity: 250.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
902	ICP AES CAL BLK (SO/ICB/CCB)	MP84204	01/24/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/27/2025

FROM 125.00000ml of M6121 + 2350.00000ml of W3112 + 25.00000ml of M6126 = Final Quantity: 2500.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
919	ICP AES INTERNAL STD	MP84218	01/24/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/27/2025

FROM 1.00000ml of M5959 + 10.00000ml of M5985 + 1969.00000ml of W3112 + 20.00000ml of M6126 = Final Quantity: 2000.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
903	ICP AES RINSE SOLN	MP84219	01/24/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/27/2025

FROM 200.00000ml of M6126 + 9800.00000ml of W3112 = Final Quantity: 10000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
904	ICP AES ICSA SOLN	MP84230	01/24/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								01/28/2025

FROM 25.00000ml of M5130 + 225.00000ml of MP84204 = Final Quantity: 250.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3494	ICP AES ICSAB SOLN-1	MP84231	01/24/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
FROM 0.01000ml of M5815 + 0.01000ml of M5817 + 0.10000ml of M5472 + 0.10000ml of M5970 + 0.10000ml of M6077 + 10.00000ml of M5130 + 10.00000ml of M5223 + 79.50000ml of MP84204 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
170	1:1HCL	MP84297	01/31/2025	02/28/2025	Eman Mughal	None	None	Sarabjit Jaswal
FROM 1250.00000ml of M6121 + 1250.00000ml of W3112 = Final Quantity: 2500.000 ml								

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2480	ICP AES STD 6 ISM01.3	MP84381	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025
FROM 4.00000ml of M5289 + 4.00000ml of M5497 + 4.00000ml of M5811 + 4.00000ml of M6127 + 4.00000ml of M6144 + 30.00000ml of MP84204 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1004	ICPAES ISM01.2 (S5)	MP84382	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025
FROM 0.25000ml of M5798 + 0.50000ml of M5429 + 0.50000ml of M5476 + 0.50000ml of M5815 + 0.50000ml of M5817 + 12.50000ml of M5519 + 12.50000ml of M6128 + 12.50000ml of M6144 + 13.75000ml of M5697 + 14.50000ml of M5496 + 14.50000ml of M5658 + 14.50000ml of M5811 + 2.00000ml of M5513 + 22.50000ml of M5497 + 22.50000ml of M6127 + 5.00000ml of M4884 + 5.00000ml of M5393 + 5.00000ml of M5875 + 5.00000ml of M6077 + 5.00000ml of M6146 + 303.50000ml of MP84204 = Final Quantity: 500.000 ml								

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1004	ICPAES ISM01.2 (S5)	MP84383	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025

FROM 0.25000ml of M5798 + 0.50000ml of M5429 + 0.50000ml of M5476 + 0.50000ml of M5815 + 0.50000ml of M5817 + 12.50000ml of M5519 + 12.50000ml of M6128 + 12.50000ml of M6144 + 12.50000ml of M6145 + 13.75000ml of M5697 + 14.50000ml of M5496 + 14.50000ml of M5658 + 14.50000ml of M5811 + 2.00000ml of M5513 + 22.50000ml of M5497 + 22.50000ml of M6127 + 5.00000ml of M4884 + 5.00000ml of M5393 + 5.00000ml of M5875 + 5.00000ml of M6077 + 5.00000ml of M6146 + 303.50000ml of MP84204 = Final Quantity: 500.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1005	ICPAES ISM01.2(S4)	MP84384	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025

FROM 250.00000ml of MP84204 + 250.00000ml of MP84382 = Final Quantity: 500.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1007	ICPAES ISM01.2(S3)	MP84385	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025

FROM 25.00000ml of MP84382 + 75.00000ml of MP84204 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1008	ICPAES ISM01.2(S2)	MP84386	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
								02/10/2025

FROM 12.50000ml of MP84382 + 87.50000ml of MP84204 = Final Quantity: 100.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
994	ICPAES ISM01.2 S1 (CONC.)	MP84387	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal 02/10/2025
FROM 0.02000ml of M5815 + 0.03000ml of M5429 + 0.10000ml of M5798 + 0.10000ml of M6028 + 0.14000ml of M5799 + 0.20000ml of M5476 + 0.20000ml of M5658 + 0.20000ml of M5801 + 0.20000ml of M5811 + 0.20000ml of M5817 + 0.20000ml of M5977 + 0.20000ml of M6025 + 0.20000ml of M6030 + 0.30000ml of M6128 + 0.40000ml of M5496 + 0.50000ml of M5697 + 0.50000ml of M6023 + 0.70000ml of M5962 + 0.80000ml of M5961 + 1.00000ml of M5800 + 1.00000ml of M6021 + 1.20000ml of M6145 + 1.20000ml of M6146 + 10.00000ml of M4884 + 10.00000ml of M5498 + 10.00000ml of M5519 + 10.00000ml of M6127 + 10.00000ml of M6144 + 2.00000ml of M5978 + 4.00000ml of M6032 + 34.24000ml of MP84204 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1003	ICPAES ISM01.2 S1	MP84388	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal 02/10/2025
FROM 0.50000ml of MP84387 + 99.50000ml of MP84204 = Final Quantity: 100.000 ml								

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1119	ICPAES ISM01.2(CCV)	MP84392	01/27/2025	02/24/2025	Kareem Khairalla	None	None	Sarabjit Jaswal
FROM 0.75000ml of M5498 + 0.75000ml of M6127 + 1.22500ml of M5496 + 1.25000ml of M5811 + 1.25000ml of M6144 + 19.77500ml of MP84204 + 25.00000ml of MP84382 = Final Quantity: 50.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57014 / Si, 1000 PPM, 125 ml	030921	03/09/2025	08/06/2021 / jaswal	08/05/2021 / jaswal	M4884

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
EPA	PART A / ICSA (ICP) STOCK SOLN	ICSA-1211	01/31/2025	05/20/2024 / jaswal	04/20/2021 / bin	M5130

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
EPA	PART B / ICSAB (ICP) STOCK SOLN	ICSB-0710	01/31/2025	05/20/2024 / jaswal	04/20/2021 / bin	M5223

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58113 / Aluminum (Al) 10,000PPM	070622	07/06/2025	09/02/2022 / jaswal	07/12/2022 / jaswal	M5289

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58126 / Fe, 10000 PPM, 500 ml	020422	02/04/2025	05/02/2023 / jaswal	06/15/2022 / jaswal	M5298

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-CAL-3 / CLP CAL SOLUTION #3, 125mL	T2-MEB714159	01/13/2027	10/12/2022 / bin	09/19/2022 / bin	M5393

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57103 / Li, 10000 PPM, 125 ml	070622	07/06/2025	01/30/2023 / bin	01/26/2023 / bin	M5429

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57038 / Sr, 1000 PPM, 125 ml	082922	08/29/2025	01/14/2025 / Jaswal	03/16/2023 / jaswal	M5472

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57138 / Sr, 10000 PPM, 125 ml	082922	08/29/2025	07/29/2024 / jaswal	03/16/2023 / jaswal	M5476

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58113 / Al, 10000 PPM, 500 ml	011623	01/16/2026	08/15/2023 / jaswal	03/17/2023 / bin	M5496

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58120 / Ca, 10000 PPM, 500 ml	031523	03/15/2026	03/18/2023 / bin	03/17/2023 / bin	M5497

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58120 / Ca, 10000 PPM, 500 ml	031523	03/15/2026	08/15/2023 / jaswal	03/17/2023 / bin	M5498

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57182 / Pb, 10000 PPM, 125 ml	061522	06/15/2025	03/19/2023 / bin	03/17/2023 / bin	M5513

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57119 / Potassium (K) 10,000PPM	120822	12/08/2025	01/08/2024 / bin	03/17/2023 / bin	M5519

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-SPK-1 / SOIL/WATER SPIKE SOLN 1, 125mL	T2-MEB721963	07/27/2027	05/30/2023 / jaswal	05/26/2023 / jaswal	M5565

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58024 / Chromium, Cr, 500 ml, 1000 PPM	060523	06/05/2026	08/28/2023 / jaswal	08/25/2023 / jaswal	M5658

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58029 / Cu, 1000 PPM, 500 ml	102523	10/25/2026	04/03/2024 / jaswal	10/27/2023 / jaswal	M5697

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57004 / Be, 1000 PPM, 125 ml	102523	10/25/2026	02/09/2024 / bin	02/09/2024 / bin	M5798

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57050 / Sn, 1000 PPM, 125 ml	071123	07/11/2026	02/09/2024 / bin	02/09/2024 / bin	M5799

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57027 / CO, 1000 PPM, 125 ml	091923	09/19/2026	05/31/2024 / bin	02/09/2024 / bin	M5800

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57033 / As, 1000 PPM, 125 ml	111323	11/13/2026	02/09/2024 / bin	02/09/2024 / bin	M5801

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57051 / Sb, 1000 PPM, 125 ml	120523	12/05/2026	08/07/2024 / jaswal	01/03/2024 / jaswal	M5802

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58111 / Na, 10000 PPM, 500 ml	122223	12/22/2026	08/01/2024 / Jaswal	01/03/2024 / jaswal	M5806

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58126 / Fe, 10000 PPM, 500 ml	051523	05/15/2026	02/06/2025 / kareem	01/03/2024 / jaswal	M5811

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57115 / P, 10000 PPM, 125 ml	041723	04/17/2026	05/21/2024 / Jaswal	02/09/2024 / jaswal	M5815

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57116 / S, 10000 PPM, 125 ml	071123	07/11/2026	03/01/2024 / jaswal	02/09/2024 / jaswal	M5817

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58030 / Zinc, Zn, 500 ml, 1000 PPM	111623	11/16/2026	03/20/2024 / jaswal	02/09/2024 / jaswal	M5819

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-CAL-1 / CLP CAL SOLUTION #1, 125mL	T2-MEB714417	01/27/2027	04/19/2024 / jaswal	02/22/2024 / jaswal	M5875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGT11-1 / TITANIUM 125mL 1000ug/mL	T2-TI719972	06/17/2027	06/18/2024 / Jaswal	02/22/2024 / Jaswal	M5942

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGY10-1 / YTTRIUM 125mL 10,000ug/mL	V2-Y740548	02/20/2029	07/01/2024 / Jaswal	06/14/2024 / Jaswal	M5959

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57028 / Ni, 1000 PPM, 125 ml	041124	04/11/2027	07/02/2024 / Jaswal	06/11/2024 / Jaswal	M5961

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57034 / Se, 1000 PPM, 125 ml	060624	06/06/2027	07/02/2024 / Jaswal	06/14/2024 / Jaswal	M5962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57003 / Li, 1000 PPM, 125 ml	061224	06/21/2027	07/01/2024 / Jaswal	07/01/2024 / Jaswal	M5970

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGMO1-1 / MOLYBDENUM 125mL 1000ug/mL	T2-MO720876	07/17/2027	08/07/2024 / jaswal	02/22/2024 / Jaswal	M5976

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGMO1-1 / MOLYBDENUM 125mL 1000ug/mL	T2-MO720876	07/17/2027	01/16/2025 / JANVI	02/22/2024 / Jaswal	M5977

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGTI1-1 / TITANIUM 125mL 1000ug/mL	T2-TI719972	06/17/2027	08/07/2024 / jaswal	02/22/2024 / Jaswal	M5978

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGIN10-5 / INDIUM 1 x 500 ml	U2-IN729349	02/21/2028	10/08/2024 / Jaswal	06/14/2024 / Jaswal	M5985

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-SPK-5 / CLP Spike Standard 5	V2-MEB742037	03/12/2029	10/04/2024 / Jaswal	02/22/2024 / Jaswal	M5990

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57023 / V, 1000 PPM, 125 ml	062424	06/24/2027	09/28/2024 / jaswal	08/05/2024 / Jaswal	M6021

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57081 / TI, 1000 PPM, 125 ml	0624724	06/27/2027	08/05/2024 / kareem	08/05/2024 / Jaswal	M6023

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57082 / Pb, 1000 PPM, 125 ml	061224	11/09/2026	08/05/2024 / Jaswal	08/05/2024 / Jaswal	M6025

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57048 / Cd, 1000 PPM, 125 ml	070124	07/01/2027	08/05/2024 / kareem	08/05/2024 / Jaswal	M6028

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57047 / Ag, 1000 PPM, 125 ml	122823	12/28/2026	08/05/2024 / kareem	08/05/2024 / Jaswal	M6030

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57056 / Ba, 1000 PPM, 125 ml	010924	01/09/2027	01/14/2025 / Jaswal	08/05/2024 / Jaswal	M6032

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	Z9651Q / CHEM-CLP-4/.25L	V2-MEB746762	09/06/2029	01/23/2025 / kareem	09/19/2024 / kareem	M6077

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	0000275677	05/13/2025	11/13/2024 / Eman	10/13/2024 / Eman	M6121

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L)	24D1062002	06/03/2025	12/03/2024 / Janvi	11/12/2024 / Janvi	M6126

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58112 / Mg, 10000 PPM, 500 ml	112124	11/21/2027	01/13/2025 / kareem	01/13/2025 / kareem	M6127

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58025 / Mn, 1000 PPM, 500 ml	101124	10/11/2027	01/13/2025 / kareem	01/13/2025 / kareem	M6128

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58111 / Na, 10000 PPM, 500 ml	072424	07/24/2027	01/23/2025 / kareem	01/13/2025 / Jaswal	M6144

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58030 / Zinc, Zn, 500 ml, 1000 PPM	121724	12/17/2027	02/04/2025 / jaswal	01/13/2025 / Jaswal	M6145

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57051 / Sb, 1000 PPM, 125 ml	071724	07/17/2027	01/31/2025 / kareem	10/18/2024 / kareem	M6146

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Certificate of Analysis

R: 02/22/24 M5986, M5987, M5988, M5989, M5990

300 Technology Drive
 Christiansburg, VA 24073 USA
 inorganicventures.com

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
 Catalog Number: CLPP-SPK-5
 Lot Number: V2-MEB742037
 Matrix: 5% (v/v) HNO₃
 Value / Analyte(s):
 100 µg/mL ea:
 Antimony,
 50 µg/mL ea:
 Selenium, Thallium,
 Cadmium,
 40 µg/mL ea:
 Arsenic,
 20 µg/mL ea:
 Lead

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Antimony, Sb	100.0 ± 0.7 µg/mL	Arsenic, As	40.00 ± 0.26 µg/mL
Cadmium, Cd	49.99 ± 0.22 µg/mL	Lead, Pb	19.99 ± 0.09 µg/mL
Selenium, Se	50.00 ± 0.23 µg/mL	Thallium, Tl	50.00 ± 0.22 µg/mL

Density: 1.025 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
As	ICP Assay	3103a	100818
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Cd	Calculated		See Sec. 4.2
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Pb	Calculated		See Sec. 4.2
Sb	ICP Assay	3102a	140911
Se	ICP Assay	3149	100901
Se	Calculated		See Sec. 4.2
Tl	ICP Assay	3158	151215
Tl	Calculated		See Sec. 4.2

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i})^2 / (\sum (1/(u_{\text{char } i})^2))$$

$$\text{CRM/RM Expanded Uncertainty (k)} = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = (\sum ((w_i)^2 (u_{\text{char } i})^2))^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty (k)} = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ In the Inorganic Ventures Terms and Conditions of Sale, <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

March 12, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **March 12, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Joseph Burns
Custom VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57056
010924
Barium (Ba)

Solvent: Nitric Acid
Lot #

Expiration Date:

010927

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Weight shown below was diluted to (mL): 2000.02 0.058 Flask Uncertainty

2% 40.0 (mL) Nitric Acid


Giovanni Caporaso	
Formulated By:	Giovanni Esposito
	010924
Reviewed By:	Pedro L. Renteria
	010924

Compound

RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
-----	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Barium nitrate (Ba) IN023 BA0022019A1 1000 99.999 0.10 52.3 3.82417 3.82441 1000.1 2.0 10022-31-8 0.5 mg/m3 or-hat 355 mg/kg 3104a

[1] Spectrum No.1 [12.514 sec]:58156.D# [Count] [Linear]

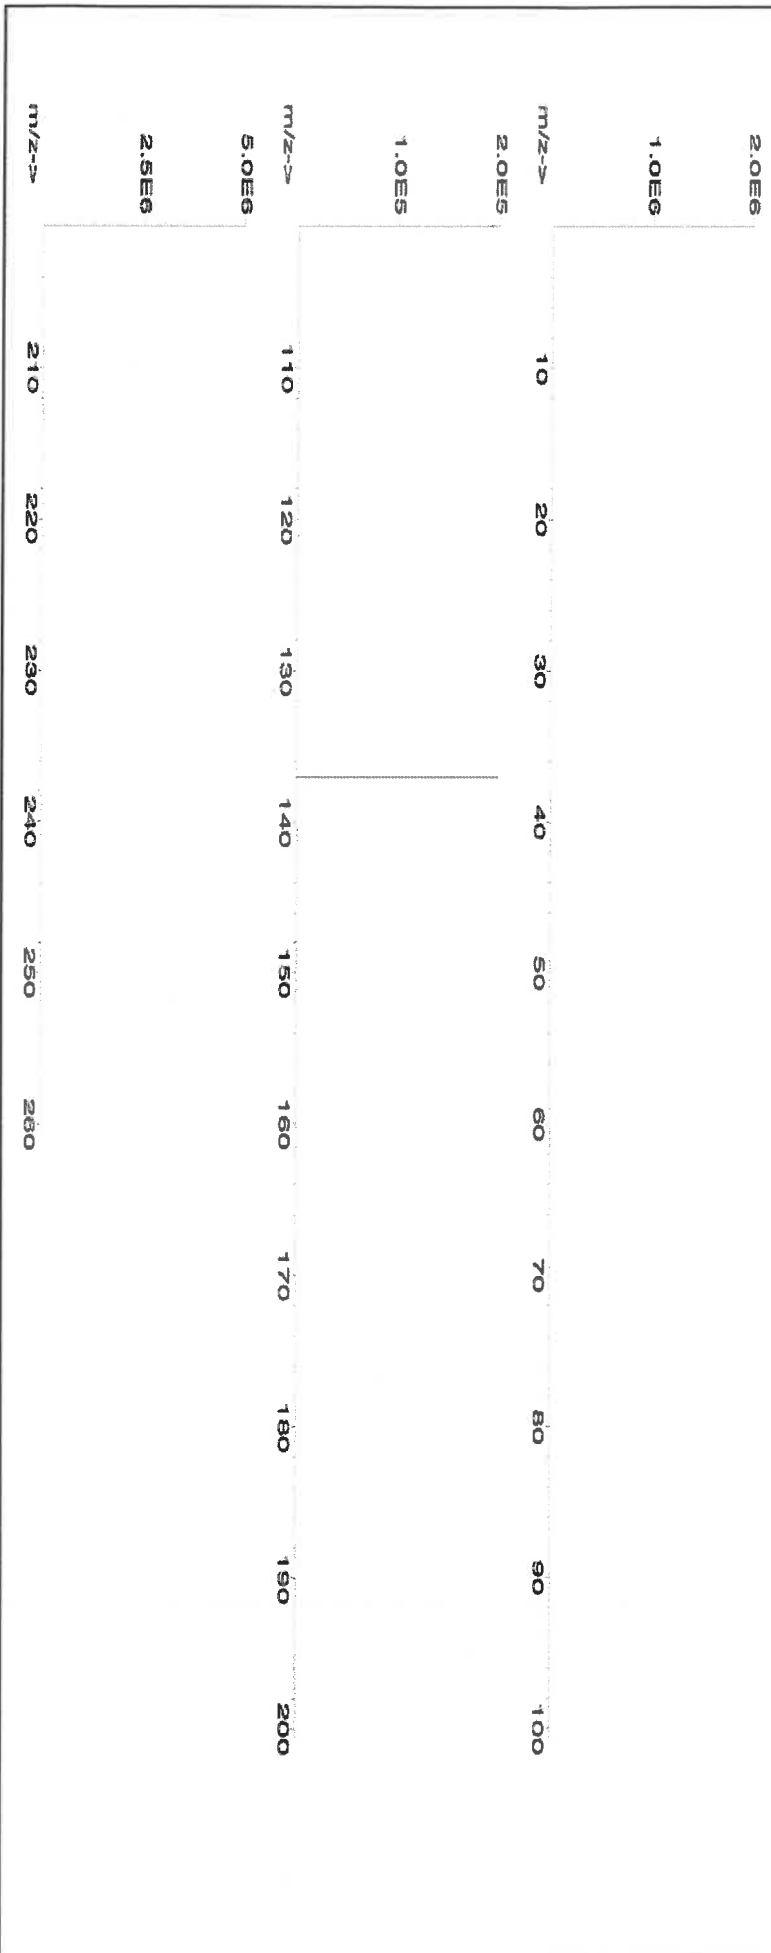



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

135

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	T	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57048
Lot Number: 070124
Description: Cadmium (Cd)

Lot #
Solvent: 24002546 Nitric Acid

2% 40.0 Nitric Acid (mL)

Expiration Date: 070127

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

SE-05 Balance Uncertainty

Weight shown below was diluted to (mL): 2000.07 0.100 Flask Uncertainty


<i>Aleah O'Brady</i>	
Formulated By:	Aleah O'Brady
	070124
<i>Pedro L. Rentas</i>	
Reviewed By:	Pedro L. Rentas
	070124

Compound

Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Cadmium nitrate tetrahydrate (Cd) IN024 CDM09221A1 1000 99.999 0.10 36.5 5.4797 5.4804 1000.1 2.0 10022-68-1 0.01 mg/m3 or-rat 60.2mg/kg 3108

[1] Spectrum No.1 [12.514 sec]:\$8148.D# [Count] [Linear]

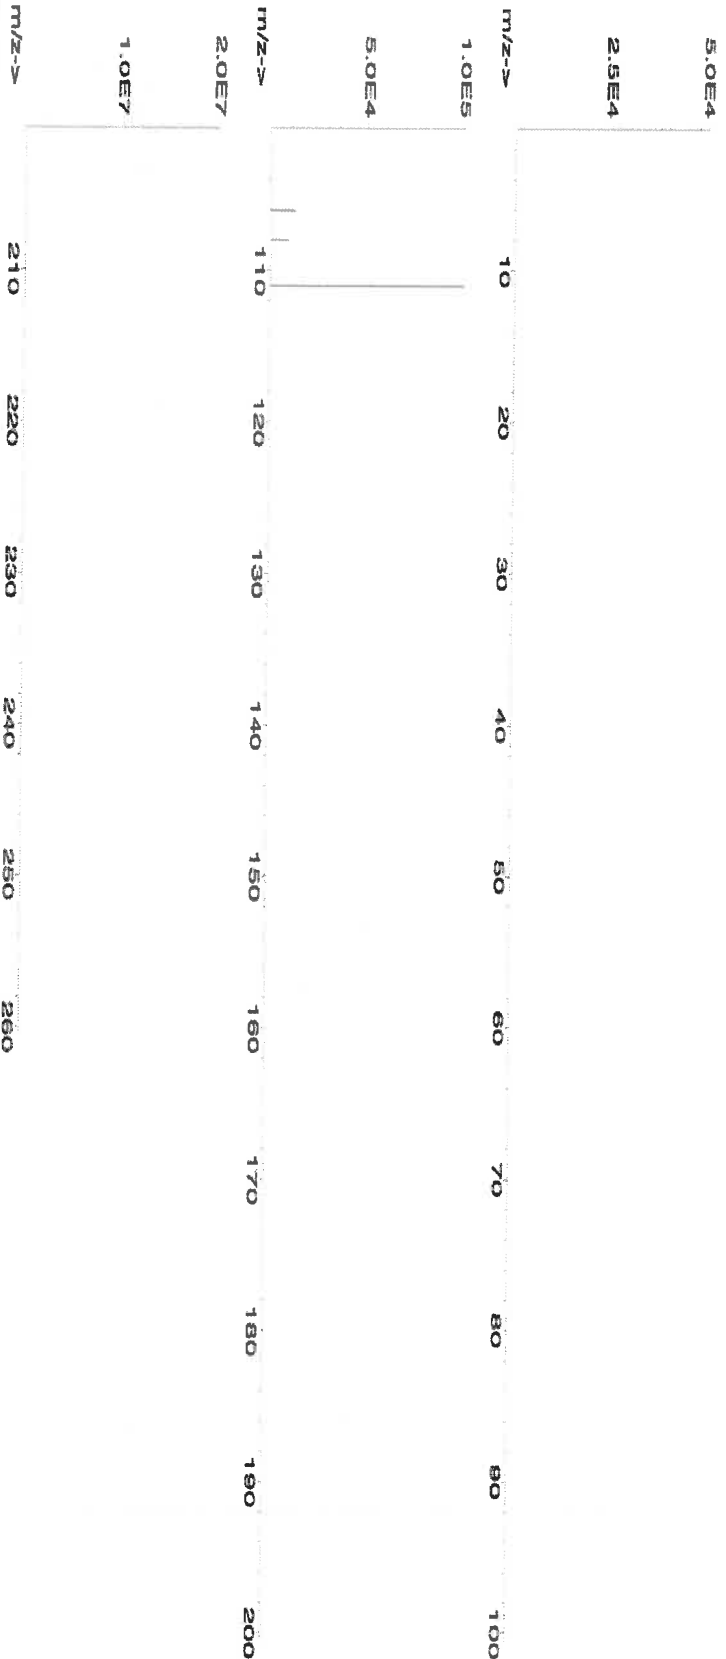



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

137

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.2	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Ba	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Cd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pr	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Certificate of Analysis

300 Technology Drive
 Christiansburg, VA 24073 USA
 inorganicventures.com

P: 800-669-6799/540-585-3030
 F: 540-585-3012
 info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code:	Multi Analyte Custom Grade Solution	
Catalog Number:	CLPP-CAL-1	
Lot Number:	T2-MEB714417	
Matrix:	5% (v/v) HNO ₃	
Value / Analyte(s):	5 000 µg/mL ea:	Potassium, Sodium,
	Calcium, Magnesium,	
	2 000 µg/mL ea:	Barium,
	Aluminum,	
	1 000 µg/mL ea:	
	Iron,	
	500 µg/mL ea:	Vanadium, Cobalt,
	Nickel, Zinc, Manganese,	
	250 µg/mL ea:	Copper,
	Silver,	
	200 µg/mL ea:	
	Chromium,	
	50 µg/mL ea:	
	Beryllium	

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Aluminum, Al	2 000 ± 7 µg/mL	Barium, Ba	2 000 ± 9 µg/mL
Beryllium, Be	50.00 ± 0.26 µg/mL	Calcium, Ca	5 000 ± 22 µg/mL
Chromium, Cr	200.0 ± 1.0 µg/mL	Cobalt, Co	500.0 ± 2.4 µg/mL
Copper, Cu	250.0 ± 1.0 µg/mL	Iron, Fe	1 000 ± 4 µg/mL
Magnesium, Mg	5 000 ± 20 µg/mL	Manganese, Mn	500.0 ± 2.0 µg/mL
Nickel, Ni	500.0 ± 2.2 µg/mL	Potassium, K	5 000 ± 19 µg/mL
Silver, Ag	250.0 ± 1.1 µg/mL	Sodium, Na	5 000 ± 18 µg/mL
Vanadium, V	499.7 ± 2.2 µg/mL	Zinc, Zn	500.0 ± 2.2 µg/mL

Density: 1.118 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Be	Calculated		See Sec. 4.2
Ca	ICP Assay	3109a	130213
Ca	EDTA	928	928
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cr	Calculated		See Sec. 4.2
Cu	ICP Assay	3114	121207
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
K	ICP Assay	3141a	140813
K	Gravimetric		See Sec. 4.2
Mg	ICP Assay	3131a	140110
Mg	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Na	ICP Assay	3152a	120715
Na	Gravimetric		See Sec. 4.2
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
V	IC Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Note: This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information.

<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

January 27, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- January 27, 2027

- The date after which this CRM/RM should not be used.
- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





Refine your results. Redefine your industry.

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CLPP-CAL-3
Lot Number: T2-MEB714159
Matrix: 7% (v/v) HNO₃
Value / Analyte(s):
1 000 µg/mL ea:
Arsenic, Lead,
Selenium, Thallium,
500 µg/mL ea:
Cadmium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Arsenic, As	1 000 ± 8 µg/mL	Cadmium, Cd	500.0 ± 2.1 µg/mL
Lead, Pb	1 000 ± 5 µg/mL	Selenium, Se	1 000 ± 8 µg/mL
Thallium, Tl	1 000 ± 7 µg/mL		

Density: 1.043 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
As	ICP Assay	3103a	100818
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Se	ICP Assay	3149	100901
Tl	ICP Assay	3158	151215

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

January 13, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **January 13, 2027**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





CERTIFIED WEIGHT REPORT:

Part Number: 58126
Lot Number: 051523
Description: Iron (Fe)

Solvent: 21110221 Nitric Acid

Lot #

Expiration Date: 051526

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 5000.1

5E-05 Balance Uncertainty

0.12 Flask Uncertainty

5.0% 250.0 (mL) Nitric Acid


<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
	051523
<i>Pedro L. Renias</i>	
Reviewed By:	Pedro L. Renias
	051523

Compound

RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
-----	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Iron (Fe)	IN346	2302010-500	10000	99.995	0.10	100.0	50.0034	50.0111	10001.5	20.0	7439-89-6	5 mg/m3	or-tral 7500mg/kg 3126a
--------------	-------	-------------	-------	--------	------	-------	---------	---------	---------	------	-----------	---------	-------------------------

[1] Spectrum No. 1 [30.763 sec]:58126.D# [Count] [Linear]

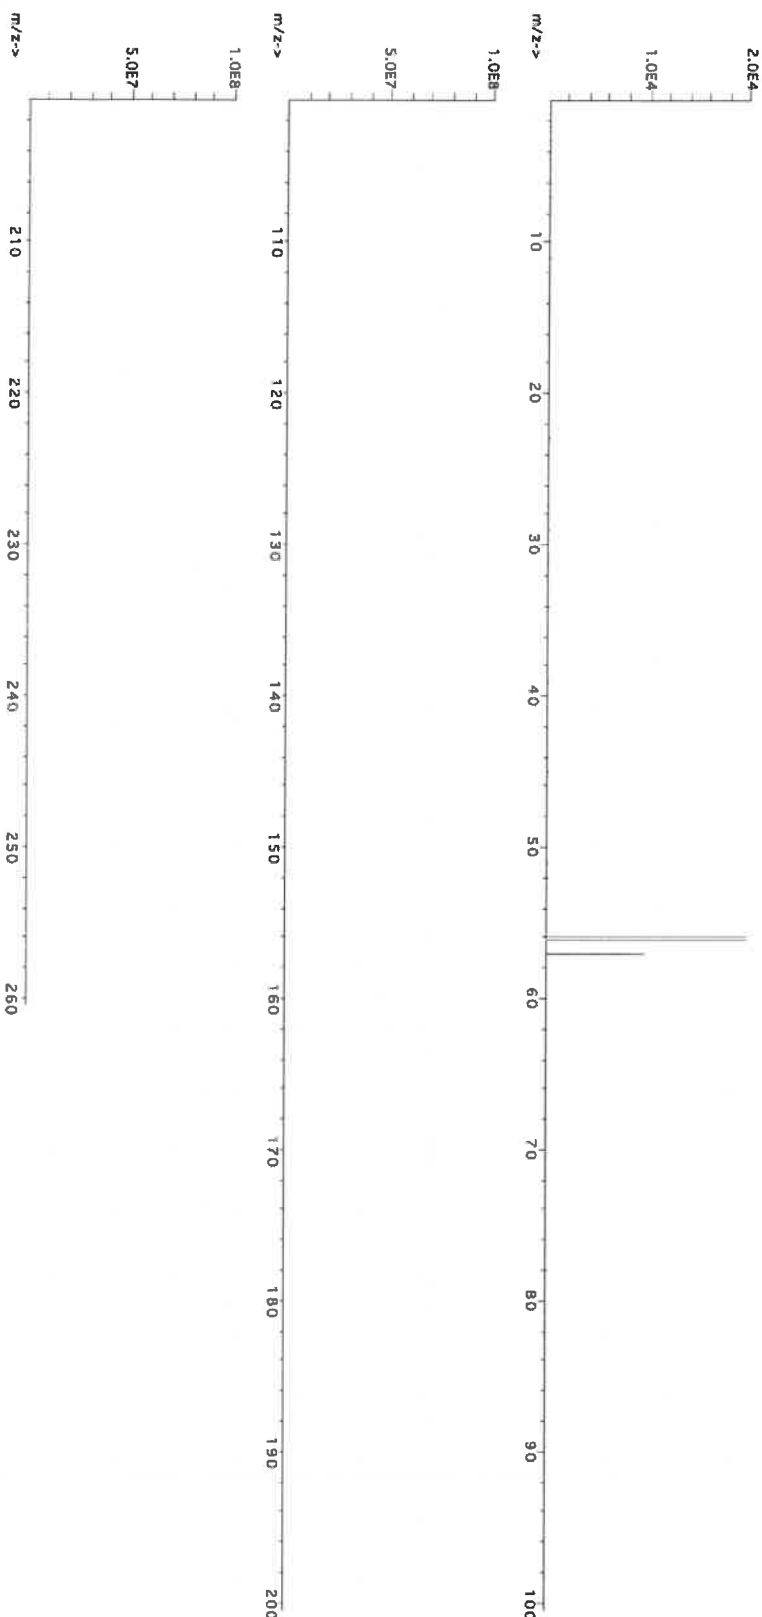



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.10	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ce	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rb	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.10	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.05	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.10	Ge	<0.10	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.10
B	<0.02	Cu	<0.10	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: 57182
Lot Number: 110923
Description: Lead (Pb)
Solvent: 24002546 Nitric Acid
Lot #


Expiration Date: 110926
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 2000.02
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Lawrence Barry
Reviewed By:	Pedro L. Rentas
110923	

Compound	SDS Information									
	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)

1. Lead(II) nitrate (Pb) IN029 PED122016A1 10000 99.999 0.10 62.5 32.0006 32.0040 10001.1 20.0 10099-74-8 0.05 mg/m3 Inverse rat 83 mg/kg 3128

[1] Spectrum No.1 [17.284 sec]:58182.D# [Count] [Linear]

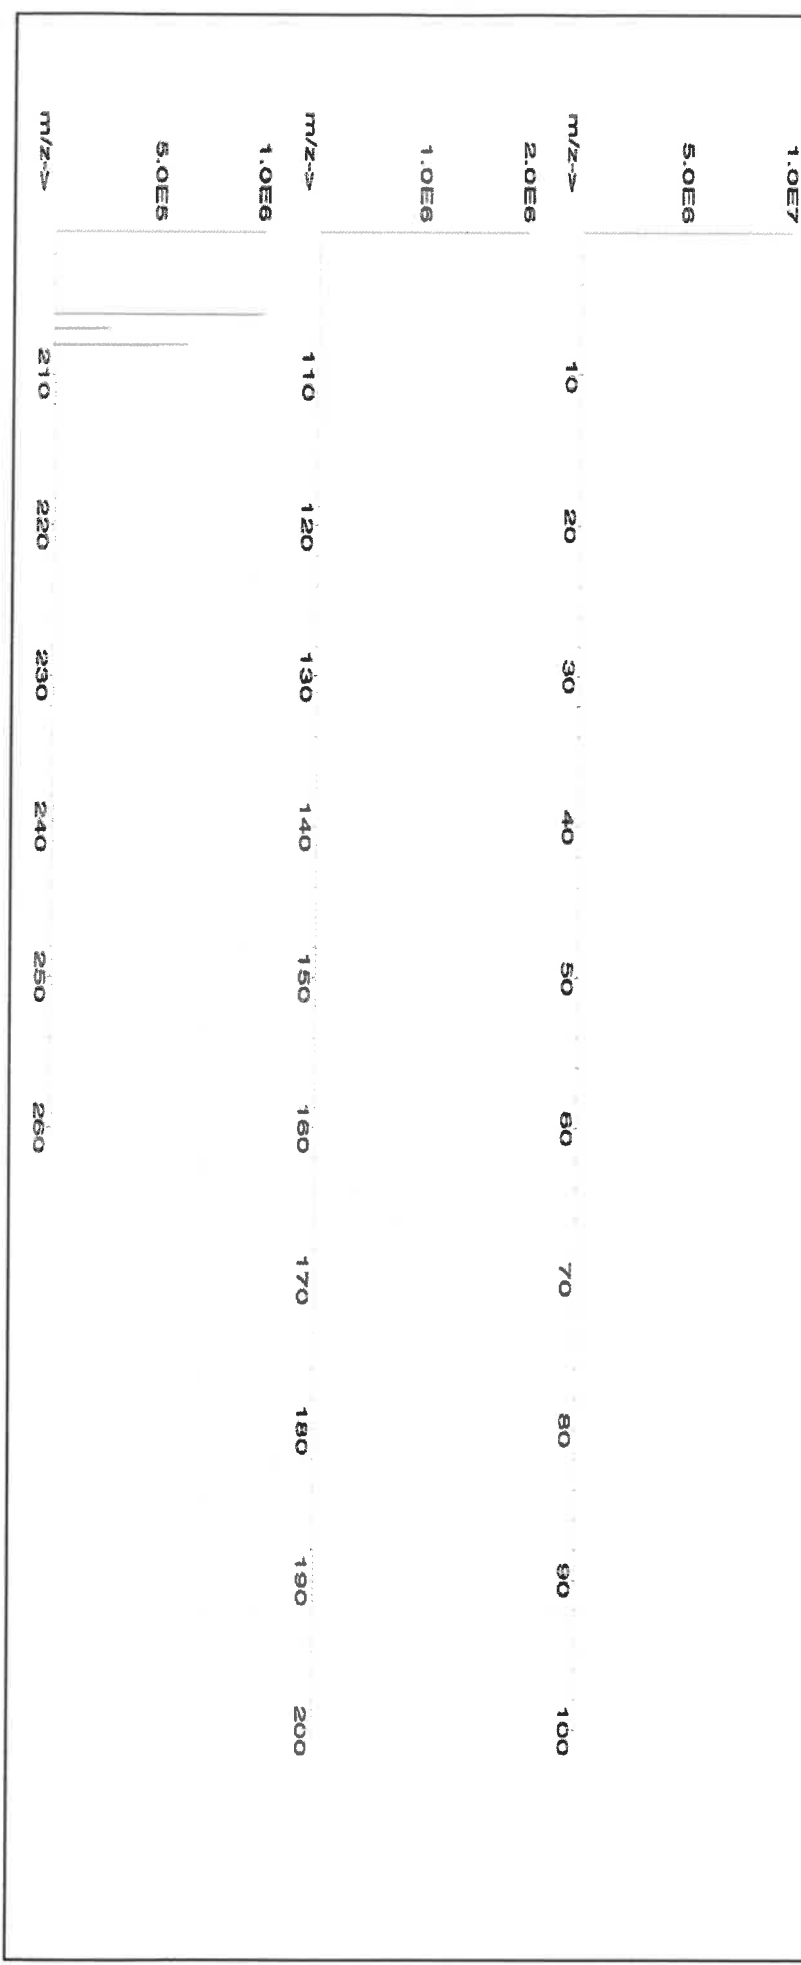



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

148

Trace Metals Verification by ICP-MS ($\mu\text{g/mL}$)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	T	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

Physical Characterization:

(T)= Target analyte

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57014
Lot Number: 030921
Description: Silicon (Si)

Lot # 19410105
Solvent: Nitric Acid

Expiration Date: 030924

2.0% 60.0 (mL) Nitric Acid

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

5E-05 Balance Uncertainty


Volume shown below was diluted to (mL): 3000.41 0.058 Flask Uncertainty

Formulated By:	Lawrence Barry
	030921
Reviewed By:	Pedro L. Rentas
	030921

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Ammonium hexafluorosilicate (Si) 58114 070120 0.1000 300.0 0.084 1000 10000.0 1000.0 2.1 16919-19-0 2.50 mg/m3 orl-rat 70 mg/kg NA

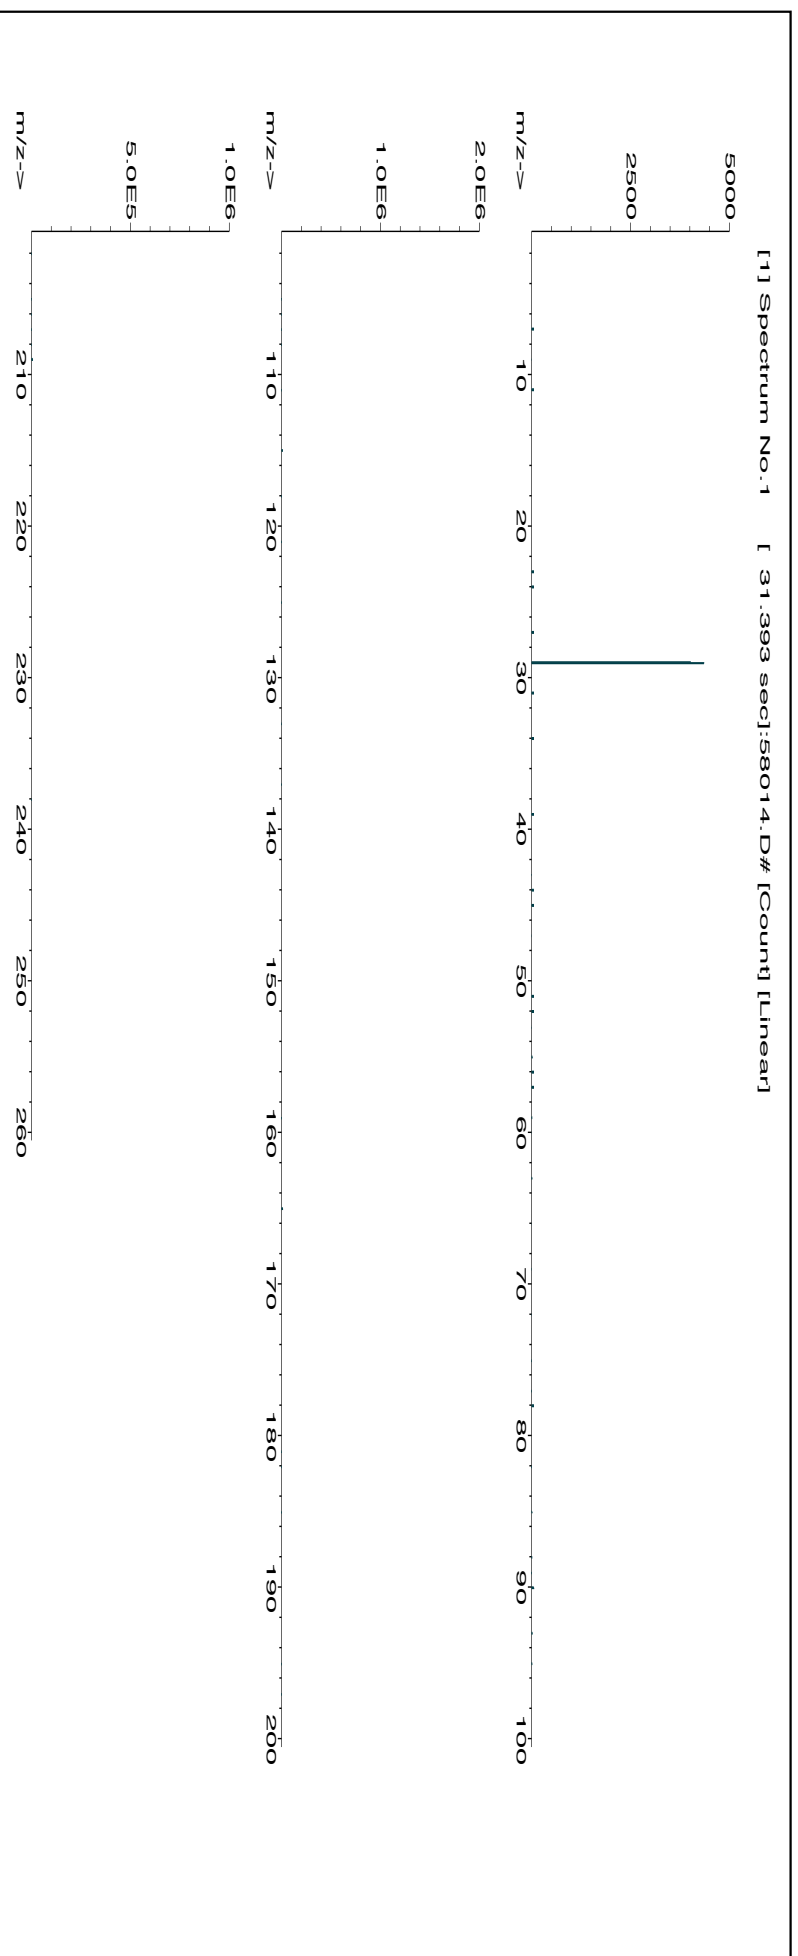



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

150

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	T	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T)= Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY
"An ISO 9001:2015 Certified Program"

Instructions for QATS Reference Material: ICP-AES ICS

**QATS LABORATORY INORGANIC REFERENCE MATERIAL
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)**

NOTE: These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

APPLICATION: For use with the CLP SFAM01.0 SOW and revisions.

CAUTION: Read instructions carefully before opening bottle(s) and proceeding with the analyses.

Contains Heavy Metals
HAZARDOUS MATERIAL

Safety Data Sheets
Available Upon Request

(A) SAMPLE DESCRIPTION

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

CAUTION: The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

(B) BREAKAGE OR MISSING ITEMS

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY
APTIM Federal Services, LLC
2700 Chandler Avenue - Building C
Las Vegas, NV 89120

(C) ANALYSIS OF SAMPLES

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,



Instructions for QATS Reference Material: ICP-AES ICS

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSA solution by ICP-AES.

ICSB-0710, Analytes, mixed with ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSAB solution by ICP-AES.

(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.

Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710

Element	CRQL	Part A (µg/L)	Low Limit (µg/L)	High Limit (µg/L)	Part A +Part B (µg/L)	Low Limit (µg/L)	High Limit (µg/L)
Al	200	255000	216000	294000	247000	209000	285000
Sb	60	(0.0)	-60.0	60.0	618	525	711
As	10	(0.0)	-10.0	10.0	104	88.4	120
Ba	200	(6.0)	-194	206	(537)	337	737
Be	5.0	(0.0)	-5.0	5.0	495	420	570
Cd	5.0	(1.0)	-4.0	6.0	972	826	1120
Ca	5000	245000	208000	282000	235000	199000	271000
Cr	10	(52.0)	42.0	62.0	542	460	624
Co	50	(0.0)	-50.0	50.0	476	404	548
Cu	25	(2.0)	-23.0	27.0	511	434	588
Fe	100	101000	85600	116500	99300	84400	114500
Pb	10	(0.0)	-10.0	10.0	(49.0)	39.0	59.0
Mg	5000	255000	216000	294000	248000	210000	286000
Mn	15	(7.0)	-8.0	22.0	507	430	584
Ni	40	(2.0)	-38.0	42.0	954	810	1100
Se	35	(0.0)	-35.0	35.0	(46.0)	11.0	81.0
Ag	10	(0.0)	-10.0	10.0	201	170	232
Tl	25	(0.0)	-25.0	25.0	(108)	83.0	133
V	50	(0.0)	-50.0	50.0	491	417	565
Zn	60	(0.0)	-60.0	60.0	952	809	1095

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value ± 1 times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value ± 15 percent of the listed certified value.

ICSA
M5126
M5127
M5128
M5129
M5130

ICSB
M5219
M5220
M5221
M5222
M5223

**QATS LABORATORY INORGANIC REFERENCE MATERIAL
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)**

NOTE: These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

APPLICATION: For use with the CLP SFAM01.0 SOW and revisions.

CAUTION: Read instructions carefully before opening bottle(s) and proceeding with the analyses.

Contains Heavy Metals
HAZARDOUS MATERIAL

Safety Data Sheets
Available Upon Request

(A) SAMPLE DESCRIPTION

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

CAUTION: The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

(B) BREAKAGE OR MISSING ITEMS

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

**QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY
APTIM Federal Services, LLC
2700 Chandler Avenue - Building C
Las Vegas, NV 89120**

(C) ANALYSIS OF SAMPLES

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,

Instructions for QATS Reference Material: ICP-AES ICS

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSA solution by ICP-AES.

ICSB-0710, Analytes, mixed with ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSAB solution by ICP-AES.

(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.

Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710

Element	CRQL	Part A (µg/L)	Low Limit (µg/L)	High Limit (µg/L)	Part A +Part B (µg/L)	Low Limit (µg/L)	High Limit (µg/L)
Al	200	255000	216000	294000	247000	209000	285000
Sb	60	(0.0)	-60.0	60.0	618	525	711
As	10	(0.0)	-10.0	10.0	104	88.4	120
Ba	200	(6.0)	-194	206	(537)	337	737
Be	5.0	(0.0)	-5.0	5.0	495	420	570
Cd	5.0	(1.0)	-4.0	6.0	972	826	1120
Ca	5000	245000	208000	282000	235000	199000	271000
Cr	10	(52.0)	42.0	62.0	542	460	624
Co	50	(0.0)	-50.0	50.0	476	404	548
Cu	25	(2.0)	-23.0	27.0	511	434	588
Fe	100	101000	85600	116500	99300	84400	114500
Pb	10	(0.0)	-10.0	10.0	(49.0)	39.0	59.0
Mg	5000	255000	216000	294000	248000	210000	286000
Mn	15	(7.0)	-8.0	22.0	507	430	584
Ni	40	(2.0)	-38.0	42.0	954	810	1100
Se	35	(0.0)	-35.0	35.0	(46.0)	11.0	81.0
Ag	10	(0.0)	-10.0	10.0	201	170	232
Tl	25	(0.0)	-25.0	25.0	(108)	83.0	133
V	50	(0.0)	-50.0	50.0	491	417	565
Zn	60	(0.0)	-60.0	60.0	952	809	1095

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value ± 1 times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value ± 15 percent of the listed certified value.

ICSA
M5126
M5127
M5128
M5129
M5130

ICSB
M5219
M5220
M5221
M5222
M5223



M5289 R: 07/12/22
Certified Reference Material CRM

(34)



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
https://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT:

Part Number: 58113
Lot Number: 070622
Description: Aluminum (Al)

Lot #
Solvent: 20370011 Nitric Acid

Expiration Date: 070625
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB


2% 40.0 Nitric Acid
(mL)

Weight shown below was diluted to (mL): 2000.02 5E-05 Balance Uncertainty 0.058 Flask Uncertainty

Formulated By:	Lawrence Barry
	070622
Reviewed By:	Pedro L. Renteria
	070622

SDS Information														
Expanded (Solvent Safety Info. On Attached pg.)														
Compound		Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Uncertainty	CAS#	NIST		
RM#	Number	Conc. (µg/mL)	(%)	Purity (%)	(%)	Weight (g)	Weight (g)	Conc. (µg/mL)	± (µg/mL)		NSDA DEL (TWA)	LD50	SRM	

1. Aluminum nitrate nonahydrate (Al) IN022 ALD012021A1 10000 99.999 0.10 7.10 281.6956 281.6977 10000.1 20.0 7784-27-2 2 mg/m3 or-tal 3671 mg/kg 3101a

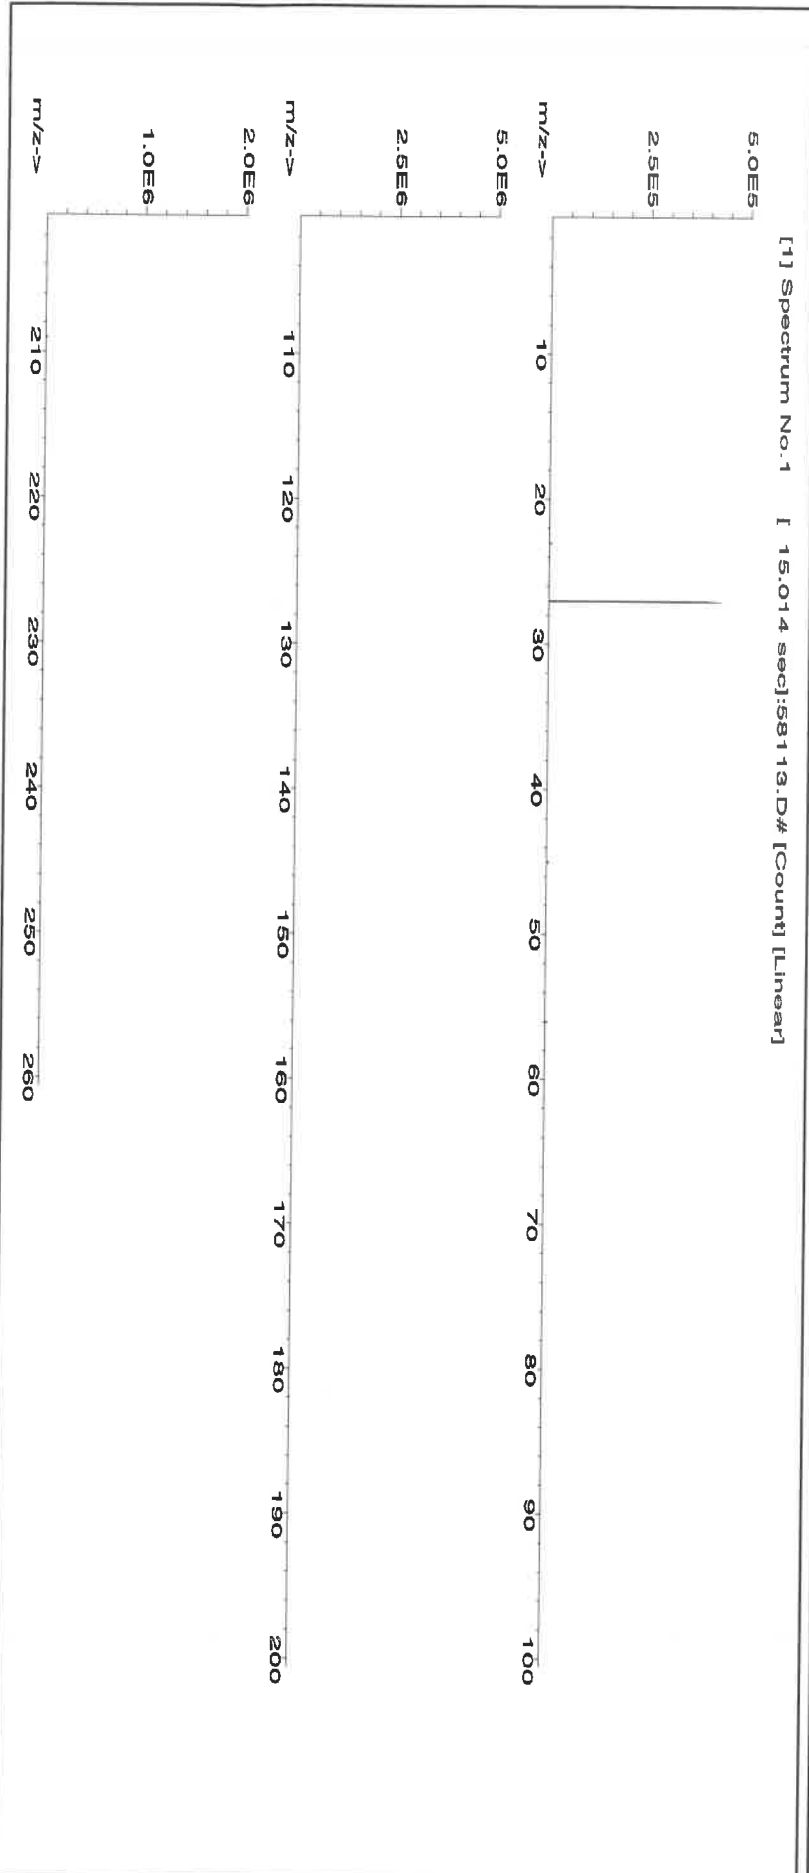



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	T	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ti	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

58126
020422
Iron (Fe)

Lot #

Solvent: 20370011 Nitric Acid

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test Number:

020425
Ambient (20 °C)
10000
6UTB
5E-05 Balance Uncertainty
0.058 Flask Uncertainty
3000.41
Weight shown below was diluted to (mL):

5.0%
150.0
(mL)
Nitric Acid

Giovanni Esposito
Formulated By: Giovanni Esposito 020422

Pedro L. Rentas
Reviewed By: Pedro L. Rentas 020422

SDS Information

Expanded
Uncertainty
+/- (µg/mL)
CAS#
OSHA PEL (TWA)
LD50

(Solvent Safety Info. On Attached pg.)
NIST
SRM

Actual

Actual

Target

Assay

Purity (%)

Purity (%)

Nominal

Lot

RM#

Conc. (µg/mL)


Conc. (µg/mL)

Conc. (µg/mL)

Conc. (µg/mL)

1. Iron(III) nitrate nonahydrate (Fe) IN346 221035107 10000 99.999 0.10 100.0 30.0044 30.0090 10001.5 20.0 7782-61-8 5 mg/m3 or-hat 7500mg/kg 3126a

[1] Spectrum No.1 [30.763 sec]:58126.D# [Count] [Linear]

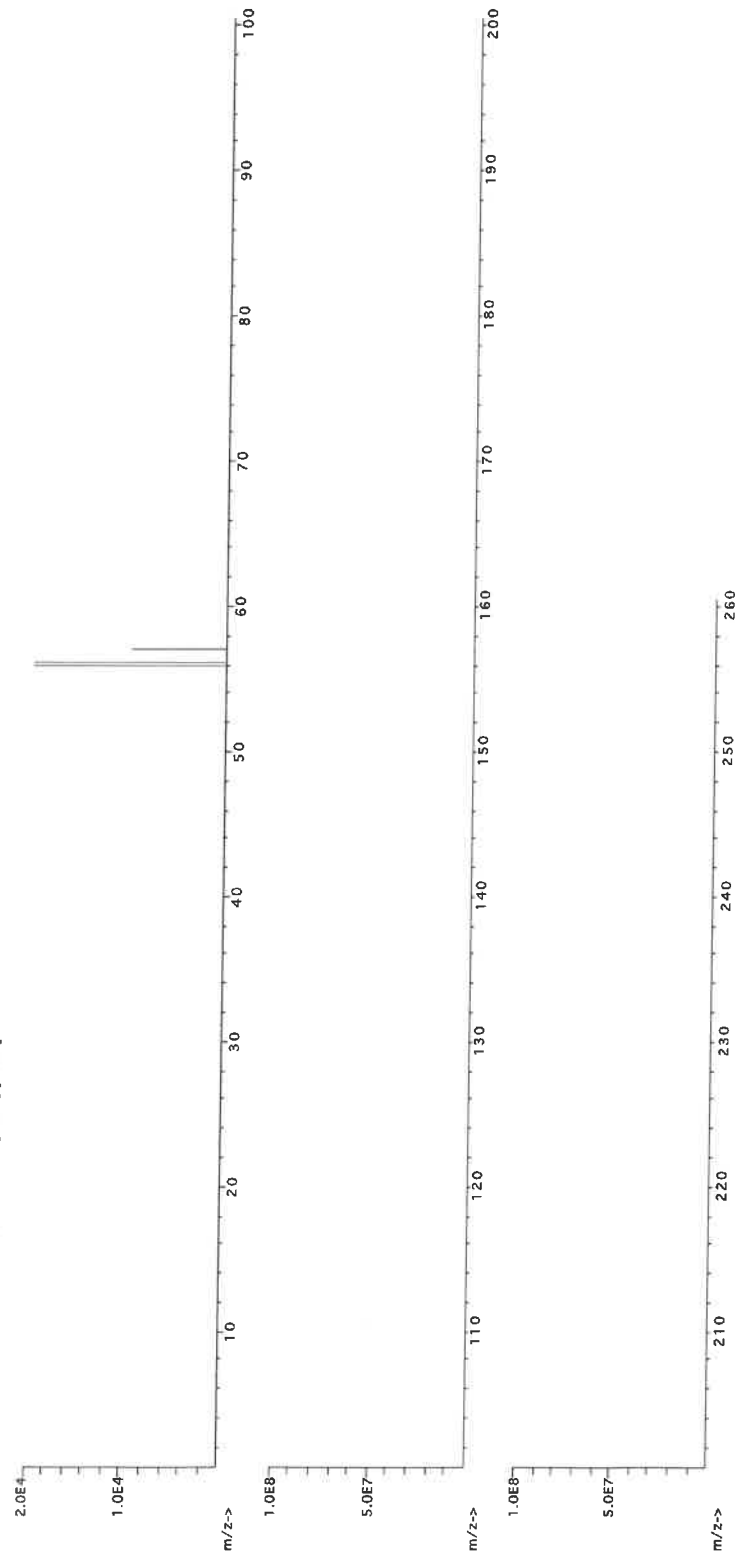

157



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS ($\mu\text{g/mL}$)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.10	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.10	Mn	<0.10	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.5	Ga	<0.2	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.10	Ge	<0.02	La	<0.10	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.10	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T)= Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

M5429 R1 0126/23 (B)

CERTIFIED WEIGHT REPORT:

Part Number: 57103
Lot Number: 070622
Description: Lithium (Li)

Expiration Date: 070625
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 1000.12

Solvent: 20510011 Nitric Acid

2% 20.0 (mL)


5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Lawrence Barry	070622
Reviewed By:	Pedro L. Rentas	070622

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	LD50	NIST SRM
----------	-----	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	--	------	----------

1. Lithium nitrate (Li)	IN019	L2042018A1	10000	99.999	0.10	10.0	100.0134	100.0173	10000.4	20.0	7790-69-4	5 mg/m3	of-rat 1426 mg/kg	NA
-------------------------	-------	------------	-------	--------	------	------	----------	----------	---------	------	-----------	---------	-------------------	----

[1] Spectrum No.1 [9.619 sec]:58103.D# [Count] [Linear]

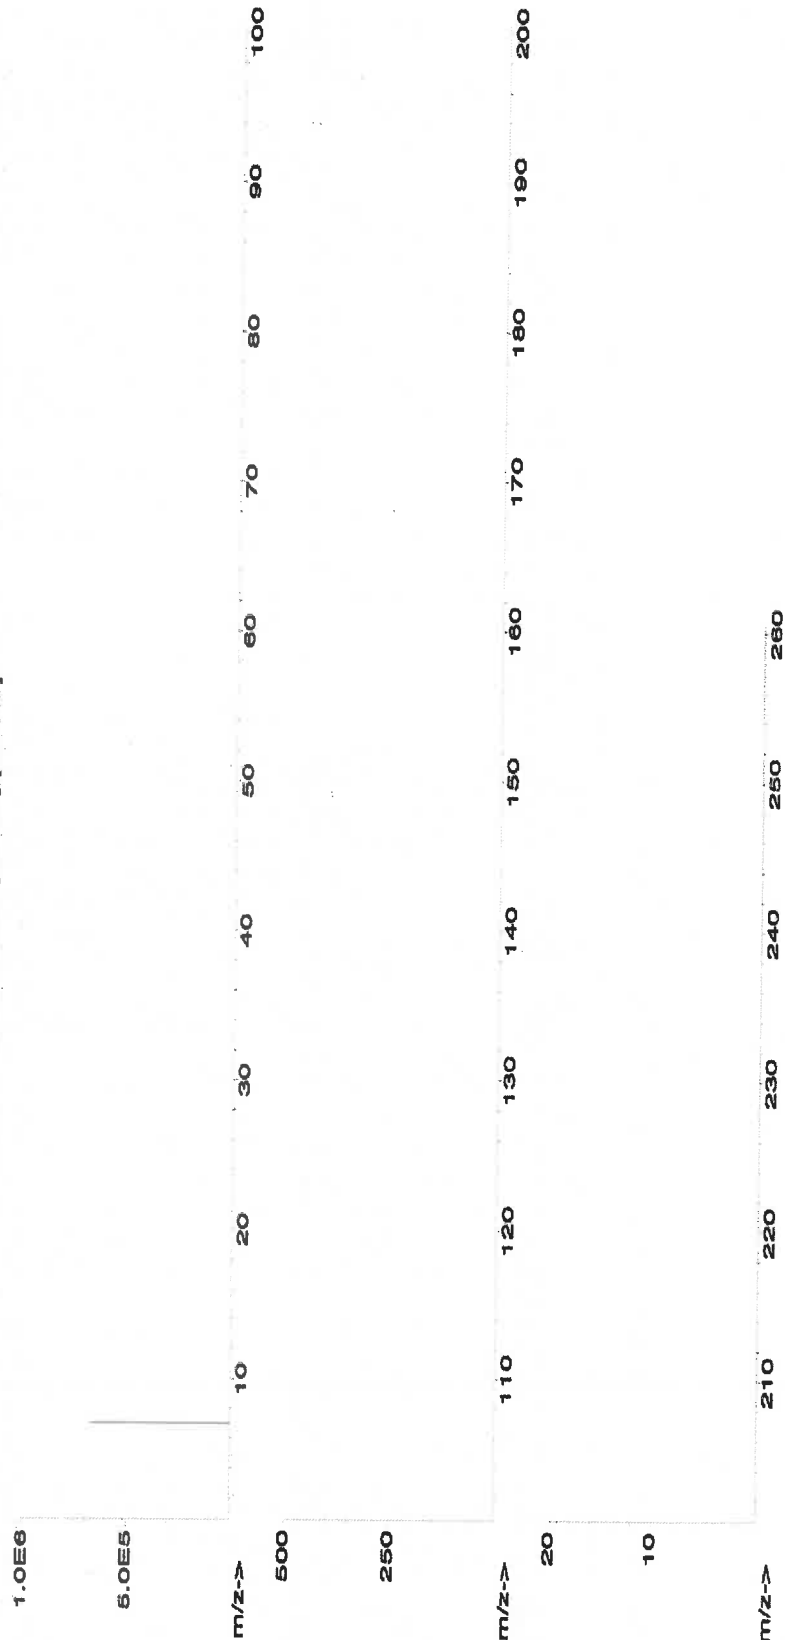

159



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.02	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.2	Ho	<0.02	La	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.02	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: **58113**

Lot Number: **011623**

Description: **Aluminum (Al)**

Solvent: **20510011 Nitric Acid**

Lot #

M5496

R 17/20/23

Expiration Date:

011626

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL):

10000

NIST Test Number:

6UTB

Weight shown below was diluted to (mL):

2000.02

5E-05 Balance Uncertainty
0.058 Flask Uncertainty


2% 40.0 (mL) Nitric Acid

<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
	011623
<i>Pedro L. Rentas</i>	
Reviewed By:	Pedro L. Rentas
	011623

SDS Information

Compound	Lot	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
1. Aluminum nitrate nonahydrate (Al)	IN022 ALM112021A1	10000	99.999	0.10	7.30	273.9779	274.0078	10001.1	20.0	7784-27-2	2 mg/m3	or-hat 3671 mg/kg	3101a

[1] Spectrum No. 1 [15.014 sec]:58113.D# [Count] [Linear]

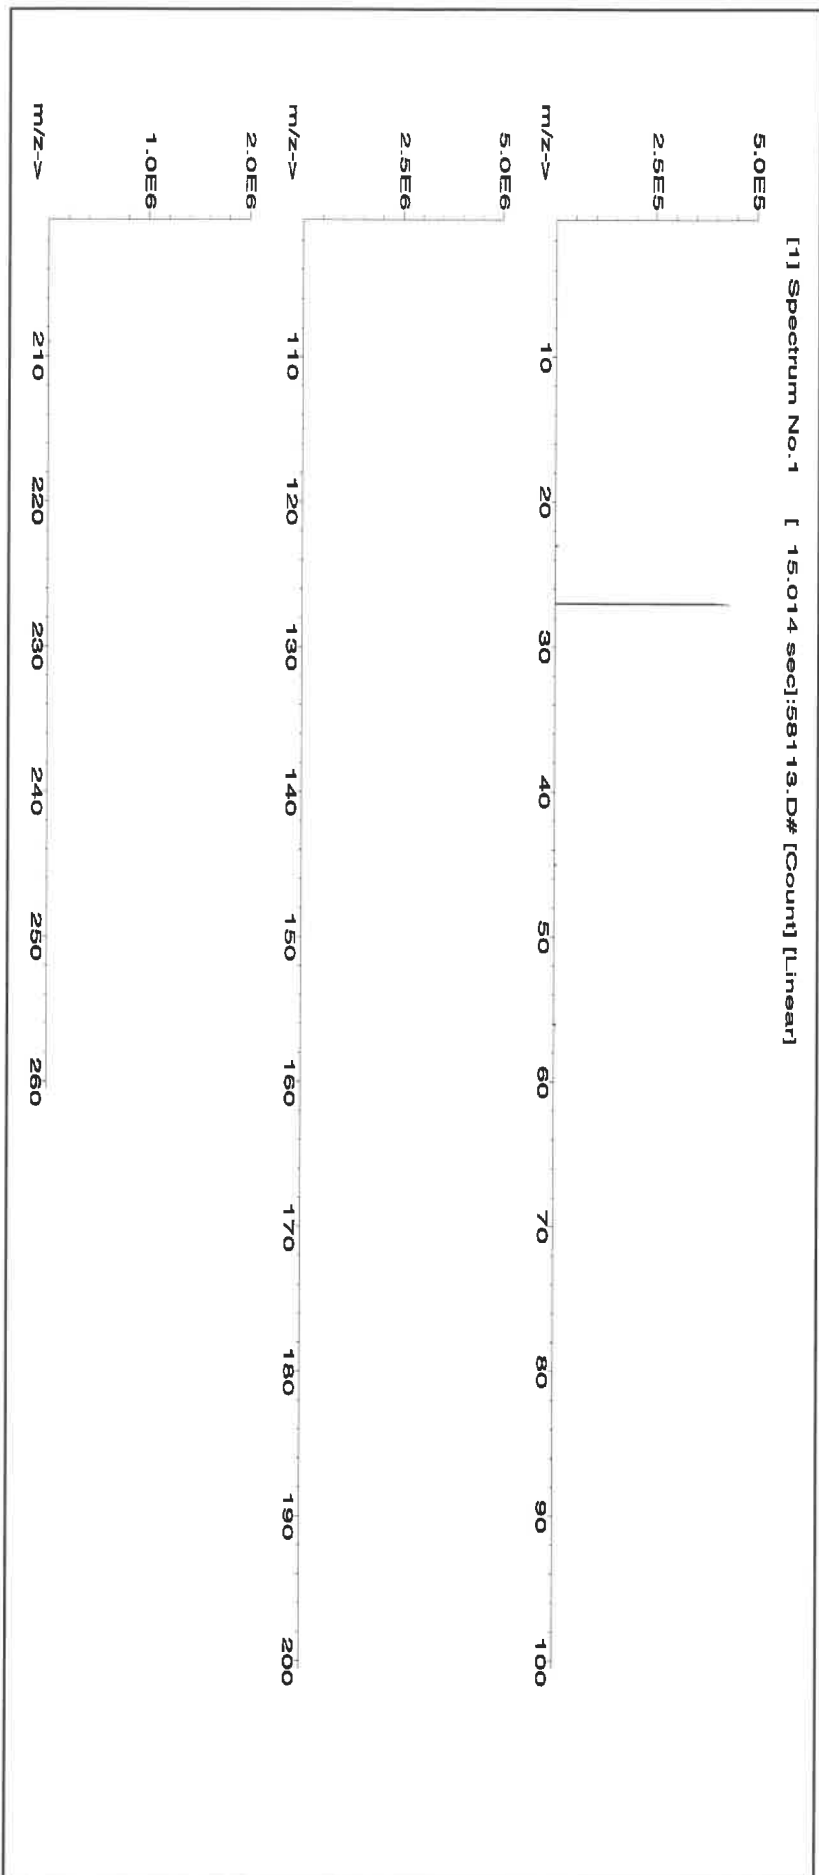



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.02	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.2	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



15497-15498 R: 03/17/23 (2)

CERTIFIED WEIGHT REPORT:

Part Number:

Lot Number: 031523

Description:

Expiration Date:

Recommended Storage:

Nominal Concentration ($\mu\text{g/mL}$):

NIST Test Number:

Weight shown below was diluted to (mL):

THE CONCEPT OF THE "CITY OF THE FUTURE"

Solvent: 21110221 Nitric Acid

Concentration	Chemical
2%	Nitric Acid
60.0	

(mL)

5E-05 Balance Uncertainty

0.058 Flask Uncertainty

Expanded

Uncertainty

Actual

 $\mu\text{g}/\text{mL}$

Actual

Weight (g)

Target

Weight (g)

Assay

(%)

Uncer

Purity

inal

 $\mu\text{g/mL}$

er Co

3

#RM#

[illegible]

[1] Spectrum No.1 [12.514 sec]:58120.D# [Count] [Linear]



164



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	T	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.2	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

05



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.02	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.2	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pr	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T)= Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT:

Part Number: **58119**
Lot Number: **120822**
Description: **Potassium (K)**

Solvent: 20510011 Nitric Acid

Lot #

Giovanni Esposito

Formulated By: Giovanni Esposito 120822

Expiration Date: 120825
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB

2% 60.0 (mL) Nitric Acid

Pedro L. Rantas

Reviewed By: Pedro L. Rantas 120822


Weight shown below was diluted to (mL): 3000.4 0.06 Flask Uncertainty

Compound

Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Expanded	SDS Information	NIST
RM#	Number	Conc. (µg/mL)	(%)	Purity (%)	Weight (g)	Weight (g)	Conc. (µg/mL)	Uncertainty +/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	SRM

1. Potassium nitrate (K) IN034 KD022021A1 10000 99.989 0.10 37.6 79.7990 79.8075 10001.1 20.0 7757-79-1 5 mg/m3 crtat 3015 mg/kg 3141a

[1] Spectrum No.1 [35.763 sec]:58119.D# [Count] [Linear]

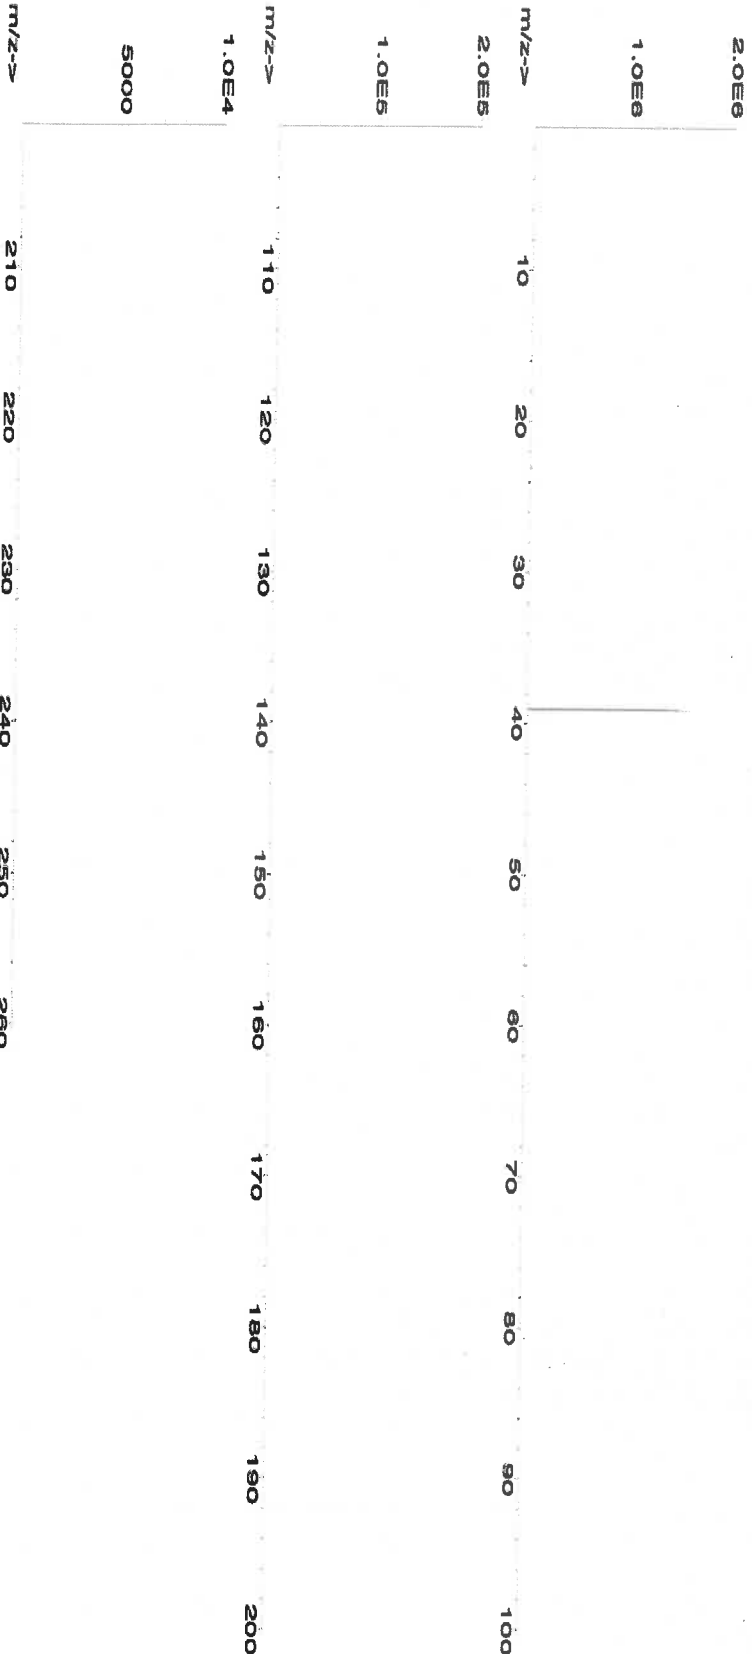



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

169

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.02	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Certificate of Analysis

300 Technology Drive
 Christiansburg, VA 24073 USA
 inorganicventures.com

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
 Catalog Number: CLPP-SPK-1
 Lot Number: T2-MEB721963
 Matrix: 7% (v/v) HNO₃
 Value / Analyte(s):
 2 000 µg/mL ea:
 Aluminum, Barium,
 1 000 µg/mL ea:
 Iron,
 500 µg/mL ea:
 Manganese, Nickel,
 Vanadium, Zinc,
 Cobalt,
 250 µg/mL ea:
 Copper,
 200 µg/mL ea:
 Chromium,
 50 µg/mL ea:
 Beryllium, Silver

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Aluminum, Al	2 000 ± 7 µg/mL	Barium, Ba	2 000 ± 9 µg/mL
Beryllium, Be	50.00 ± 0.26 µg/mL	Chromium, Cr	200.0 ± 1.1 µg/mL
Cobalt, Co	500.0 ± 2.4 µg/mL	Copper, Cu	250.0 ± 1.0 µg/mL
Iron, Fe	1 000 ± 4 µg/mL	Manganese, Mn	500.0 ± 2.0 µg/mL
Nickel, Ni	500.0 ± 2.2 µg/mL	Silver, Ag	50.00 ± 0.22 µg/mL
Vanadium, V	500.0 ± 2.2 µg/mL	Zinc, Zn	500.0 ± 2.2 µg/mL

Density: 1.070 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Ag	Calculated		See Sec. 4.2
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Be	Calculated		See Sec. 4.2
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cu	ICP Assay	3114	121207
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
V	IC Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char\ i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char\ i}^2) / \sum (1/u_{char\ i}^2)$$

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char\ i})^2]^{1/2}$ where $u_{char\ i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (\bar{X}_a) (u_{char\ a})$$

$\bar{X}_a$ = mean of Assay Method A with

$u_{char\ a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k (u_{char\ a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char\ a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Note: This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information.

<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va, 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

July 27, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- July 27, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





CERTIFIED WEIGHT REPORT:

Part Number: 58024
Lot Number: 060523
Description: Chromium (Cr)

Lot #
21110221
Solvent: Nitric Acid

2.0%

40.0 (mL)
Nitric Acid

Formulated By: *Lawrence Barry*
Reviewed By: *Pedro L. Renteria*

Expiration Date: 060526
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000


Formulated By: *Lawrence Barry*
Reviewed By: *Pedro L. Renteria*

NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 2000.02
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Chromium(III) nitrate nonahydrate (Cr) 58124 071122 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 7789-02-8 0.5 mg(Cr)/m3 or rat 3250 mg/kg 3112a

[1] Spectrum No.1 [31.393 sec]:57024.D# [Count] [Linear]

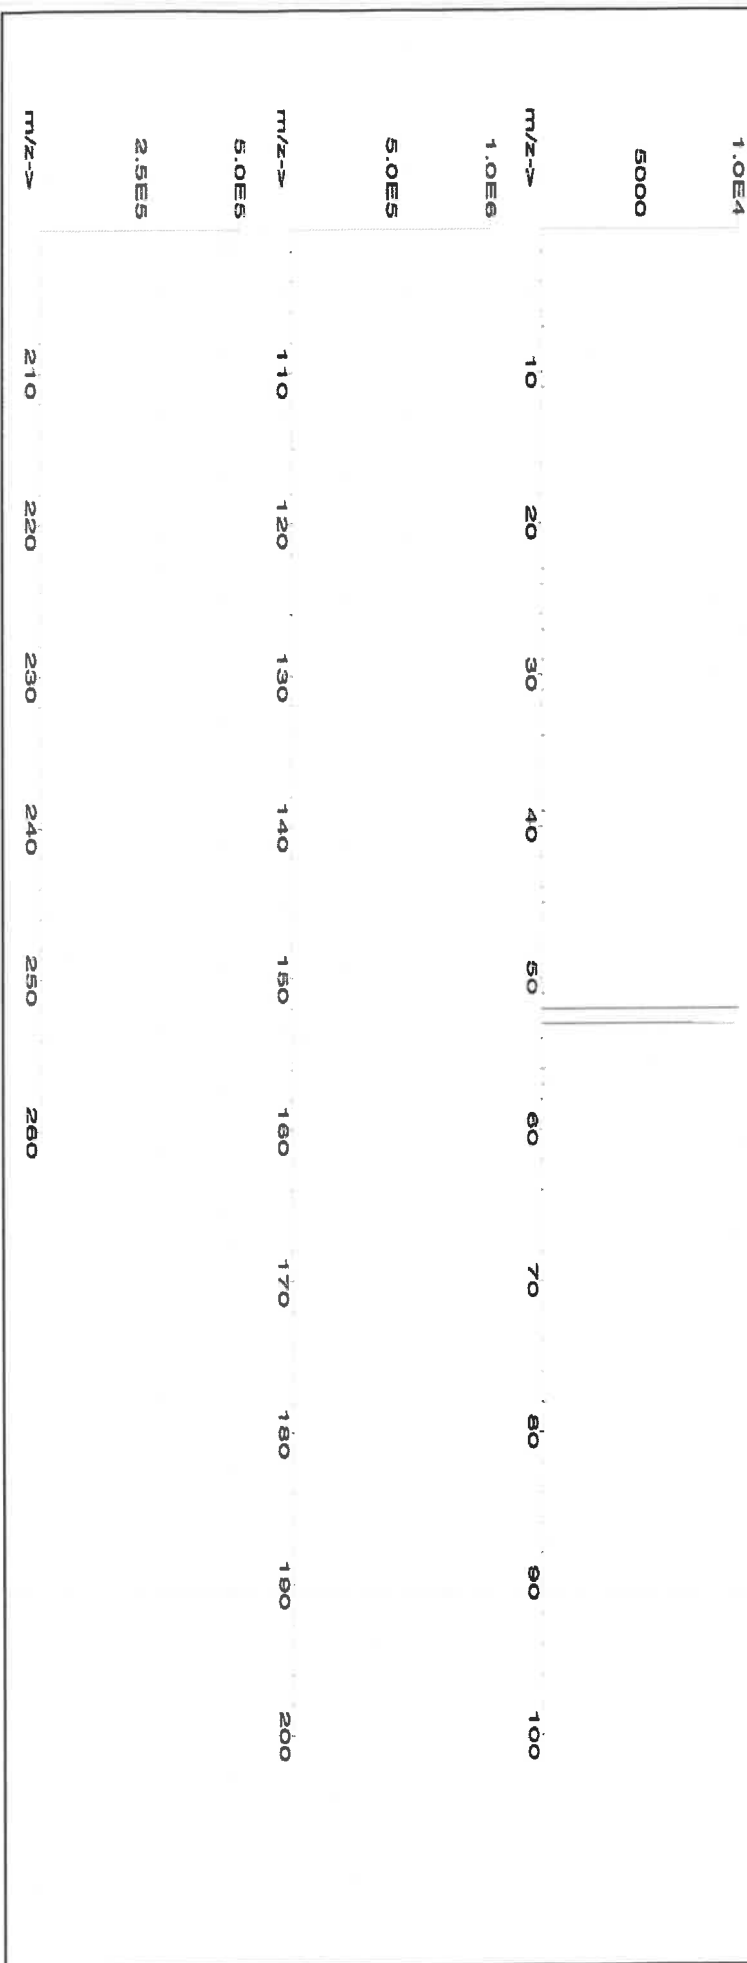



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

175

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	T	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58029
Lot Number: 102523
Description: Copper (Cu)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date: 102526

2.0%

40.0 (mL)

Nitric Acid

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

5E-05 Balance Uncertainty

Volume shown below was diluted to (mL): 2000.02

0.058 Flask Uncertainty

Formulated By:

Benson Chan

102523

Reviewed By:

Pedro L. Rentas


102523

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Copper(II) nitrate trihydrate (Cu) 58129 100223 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 10031-43-3 1 mg/m3 or-rat 794 mg/kg 3114

[1] Spectrum No. 1 [33.422 sec]:58029.D# [Count] [Linear]

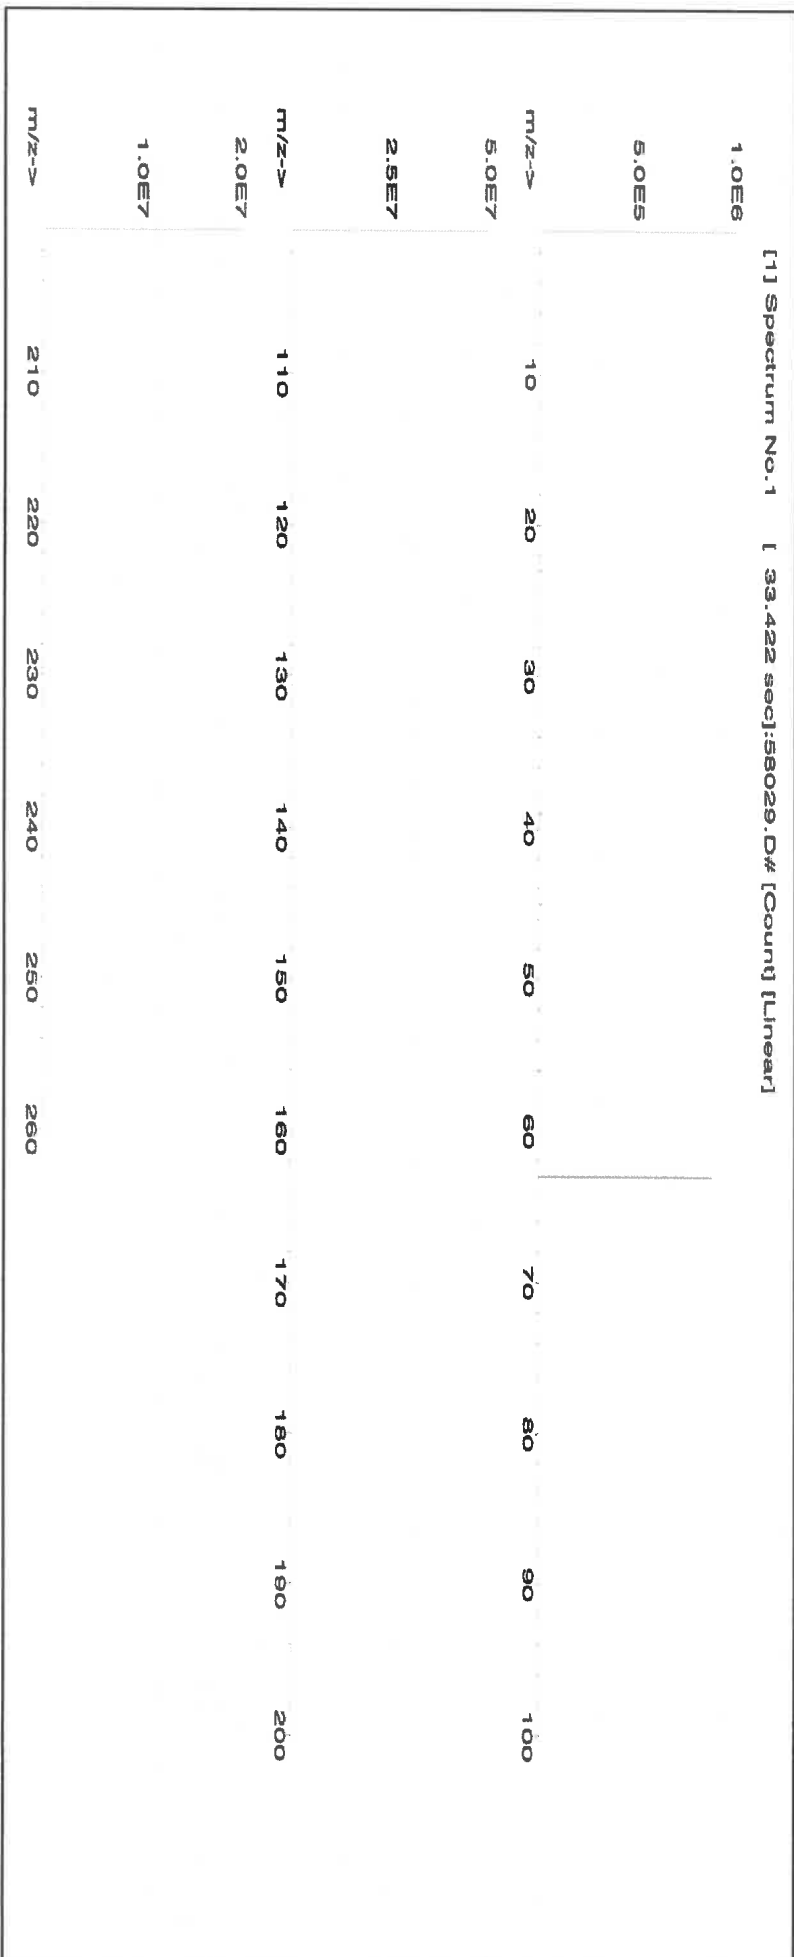



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	T	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57004
Lot Number: 102523
Description: Beryllium (Be)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date:

102526

2.0%

40.0 (mL)

Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Volume shown below was diluted to (mL):

5E-05

Balance Uncertainty

0.058


Flask Uncertainty

Formulated By:	Benson Chan	102523
Reviewed By:	Pedro L. Rentas	102523

SDS Information

Compound	Part Number	Lot	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	-----	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Beryllium nitrate (Be)	58104	091423	0.1000	200.0	0.084	1000	10001.5	1000.0	2.2	13597-99-4	0.2µg/m3	intrinsc-rat 3.16mg/kg	NA
---------------------------	-------	--------	--------	-------	-------	------	---------	--------	-----	------------	----------	------------------------	----

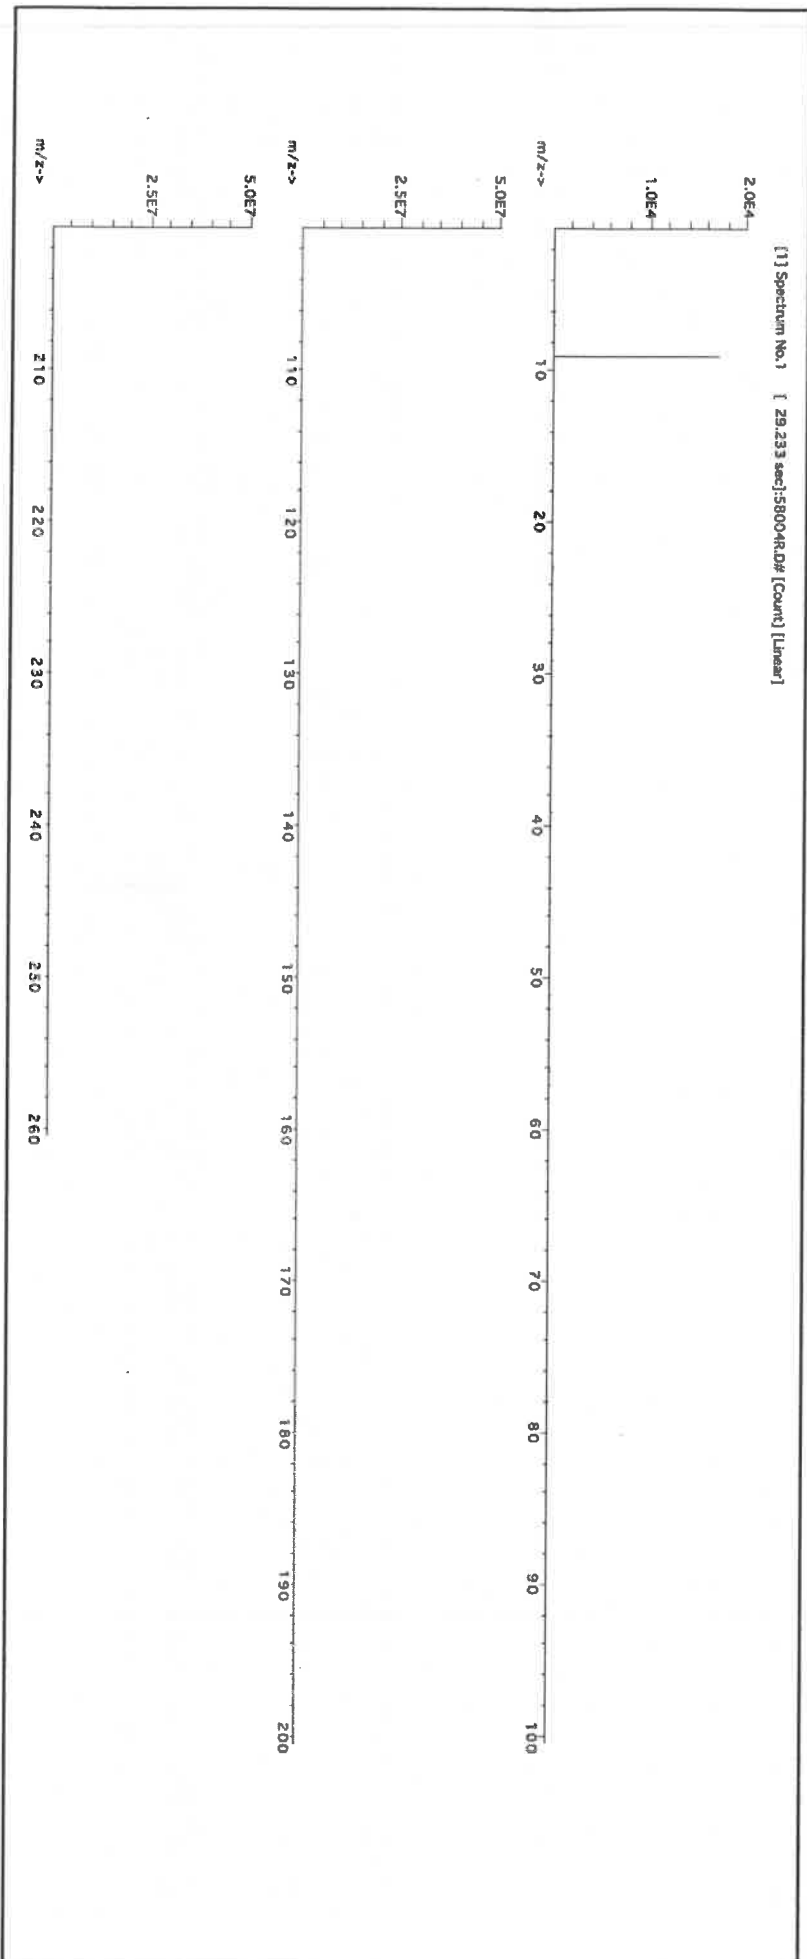



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.02	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	T	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Ta	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E. "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT:


Part Number: 57050
Lot Number: 071123
Description: Tin (Sn)

Solvents: 21110221 Nitric Acid
22D0562008 Hydrochloric acid

Lot #

R-02509124

M599



Expiration Date: 071126
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB


Weight shown below was diluted to (mL): 499.93
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Benson Chan
	071123
Reviewed By:	Pedro L. Rentas
	071123

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty		CAS#	OSHA PEL (TWA)	LD50	SRM
										+/- (µg/mL)	(µg/mL)				

1. Ammonium hexafluoroantimonate(V) (Sn) IN010 SMD042023A1 1000 99.999 0.10 44.2 1.13107 1.13286 1001.6 2.0 16919-24-7 7 mg/m3 NA 3161a

[1] Spectrum No. 1 [15.034 sec]:56150.D# [Count] [Linear]

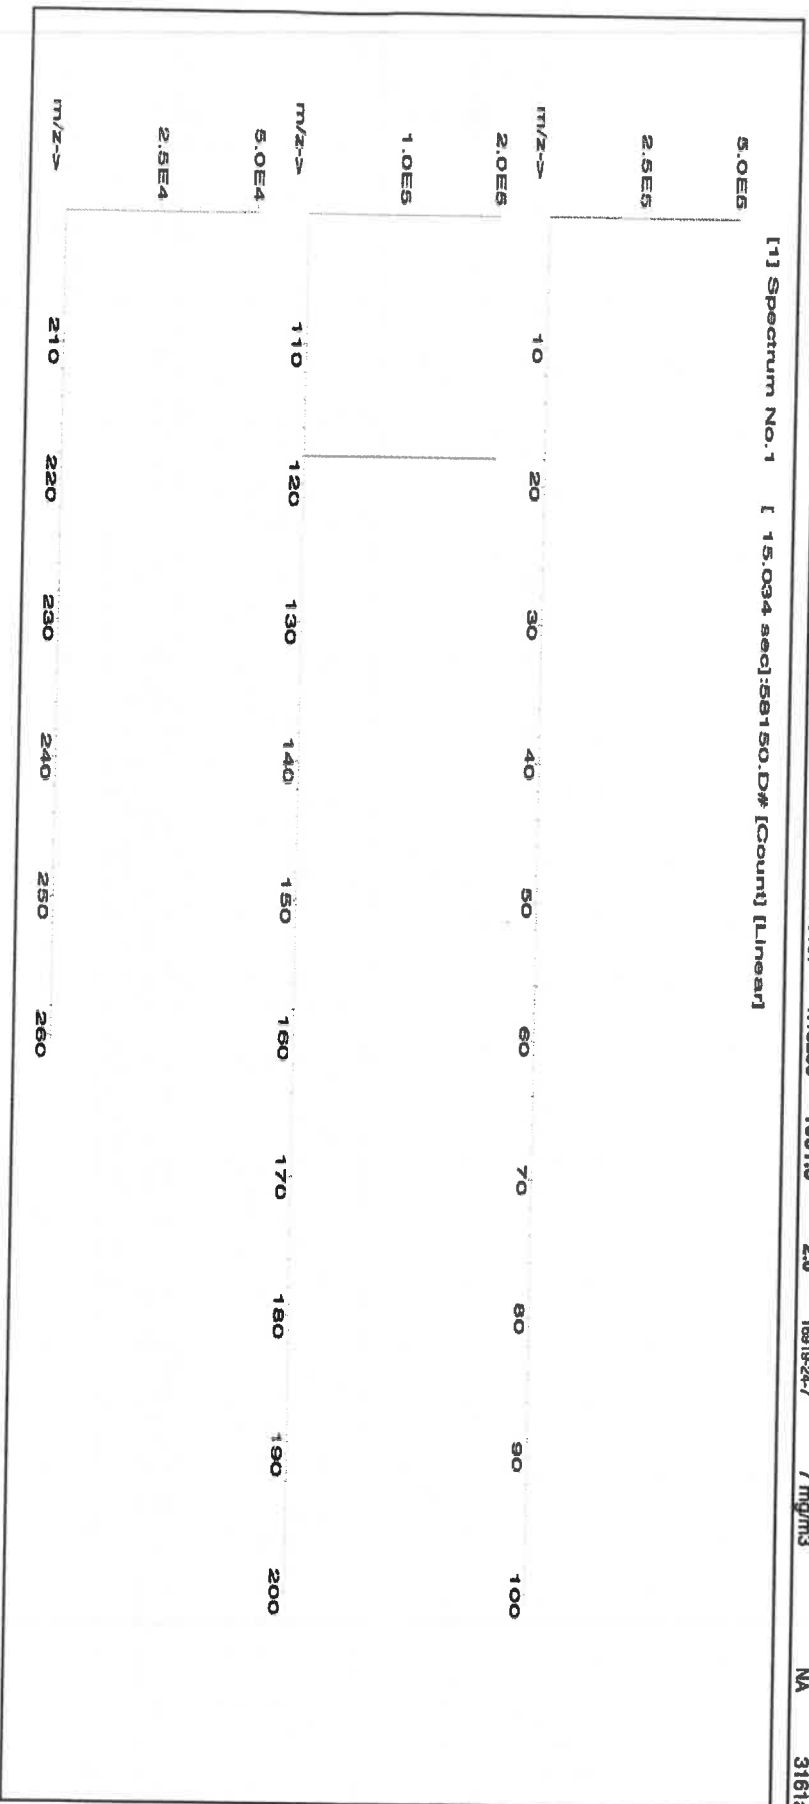



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

181

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<500	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 02/09/24 115800 (54)

CERTIFIED WEIGHT REPORT:

Part Number: 57027
Lot Number: 091923
Description: Cobalt (Co)

Expiration Date: 091926
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB

Volume shown below was diluted to (mL): 2000.02

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Lot # 24002546
Solvent: Nitric Acid

2.0% Nitric Acid
40.0 (mL)

Formulated By:	Lawrence Barry
Reviewed By:	Pedro L. Rentas


SDS Information

Expanded Uncertainty +/- (µg/mL)
(Solvent Safety Info. On Attached pg.)
NIST SRM
CAS# OSHA PEL (TWA) LD50

Compound

1. Cobalt(II) nitrate hexahydrate (Co)	58127	050923	0.1000	200.0	0.084	1000	10000.0	1000.0	2.2	10026-22-9	0.02 mg/m3	or-rat 691 mg/kg	3113
--	-------	--------	--------	-------	-------	------	---------	--------	-----	------------	------------	------------------	------

[1] Spectrum No.1 [34.243 sec]:58027.D# [Count] [Linear]

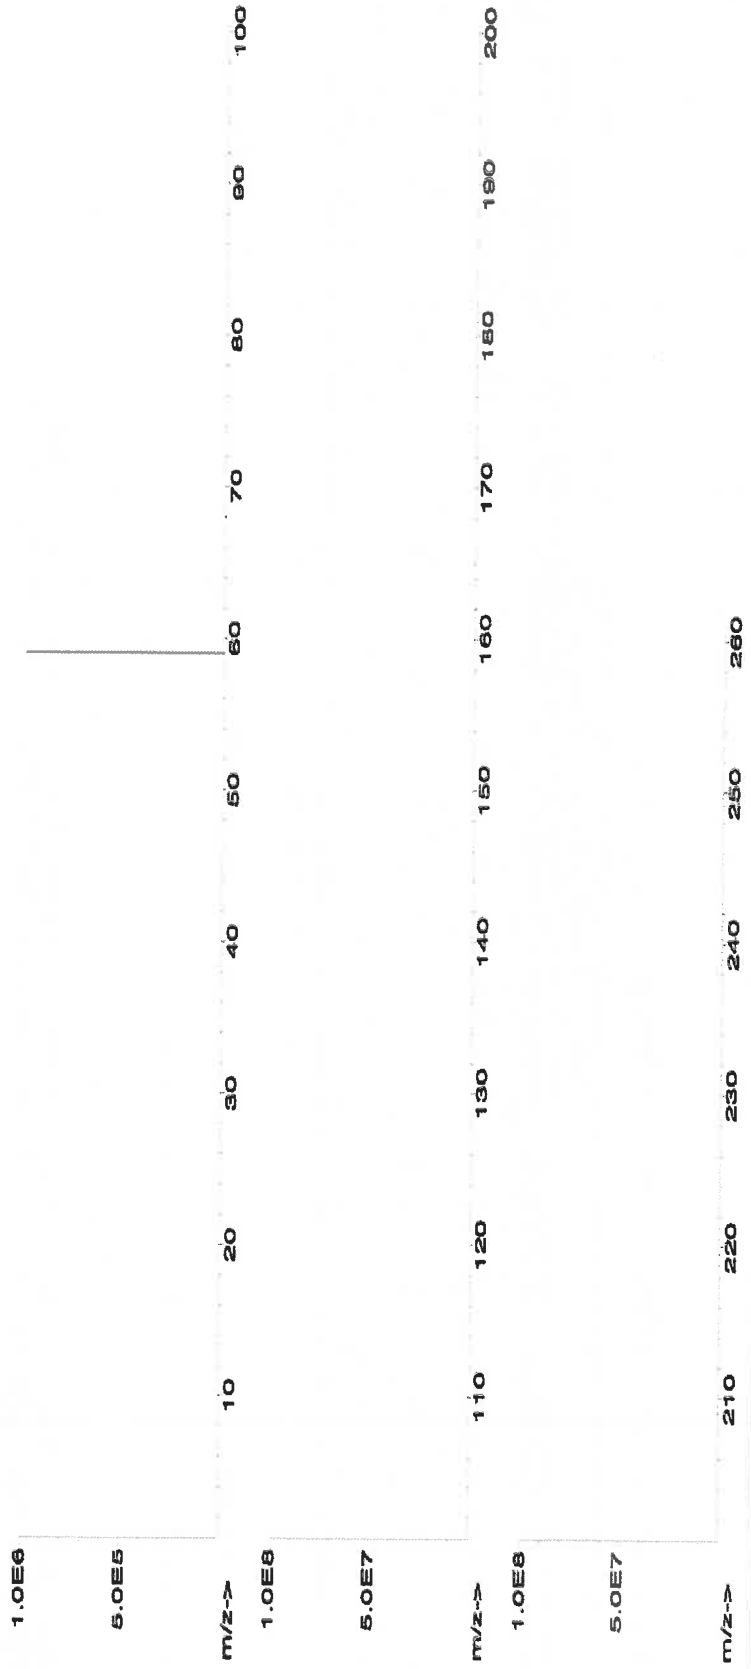

182



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.02	Os	<0.01	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.2	Na	<0.02	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	T	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T)= Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



AR: 02/09/24

M5801

BA



CERTIFIED WEIGHT REPORT:

Part Number: 57033
Lot Number: 111323
Description: Arsenic (As)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date: 111326

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

Volume shown below was diluted to (mL): 4000.0

Balance Uncertainty: 5E-05
Flask Uncertainty: 0.06

2.0%

80.0 (mL)

Nitric Acid


Formulated By:	Lawrence Barry	111323
Reviewed By:	Pedro L. Rendas	111323

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	--	------	----------------	------	----------

1. Arsenic (As)	58133	020522	0.1000	400.0	0.084	1000	10001.0	1000.0	2.0	7440-38-2	0.5 mg/m3	or-hat 500 mg/kg	3103a	
-----------------	-------	--------	--------	-------	-------	------	---------	--------	-----	-----------	-----------	------------------	-------	--

[1] Spectrum No. 1 [34.433 sec]:57033.D# [Count] [Linear]

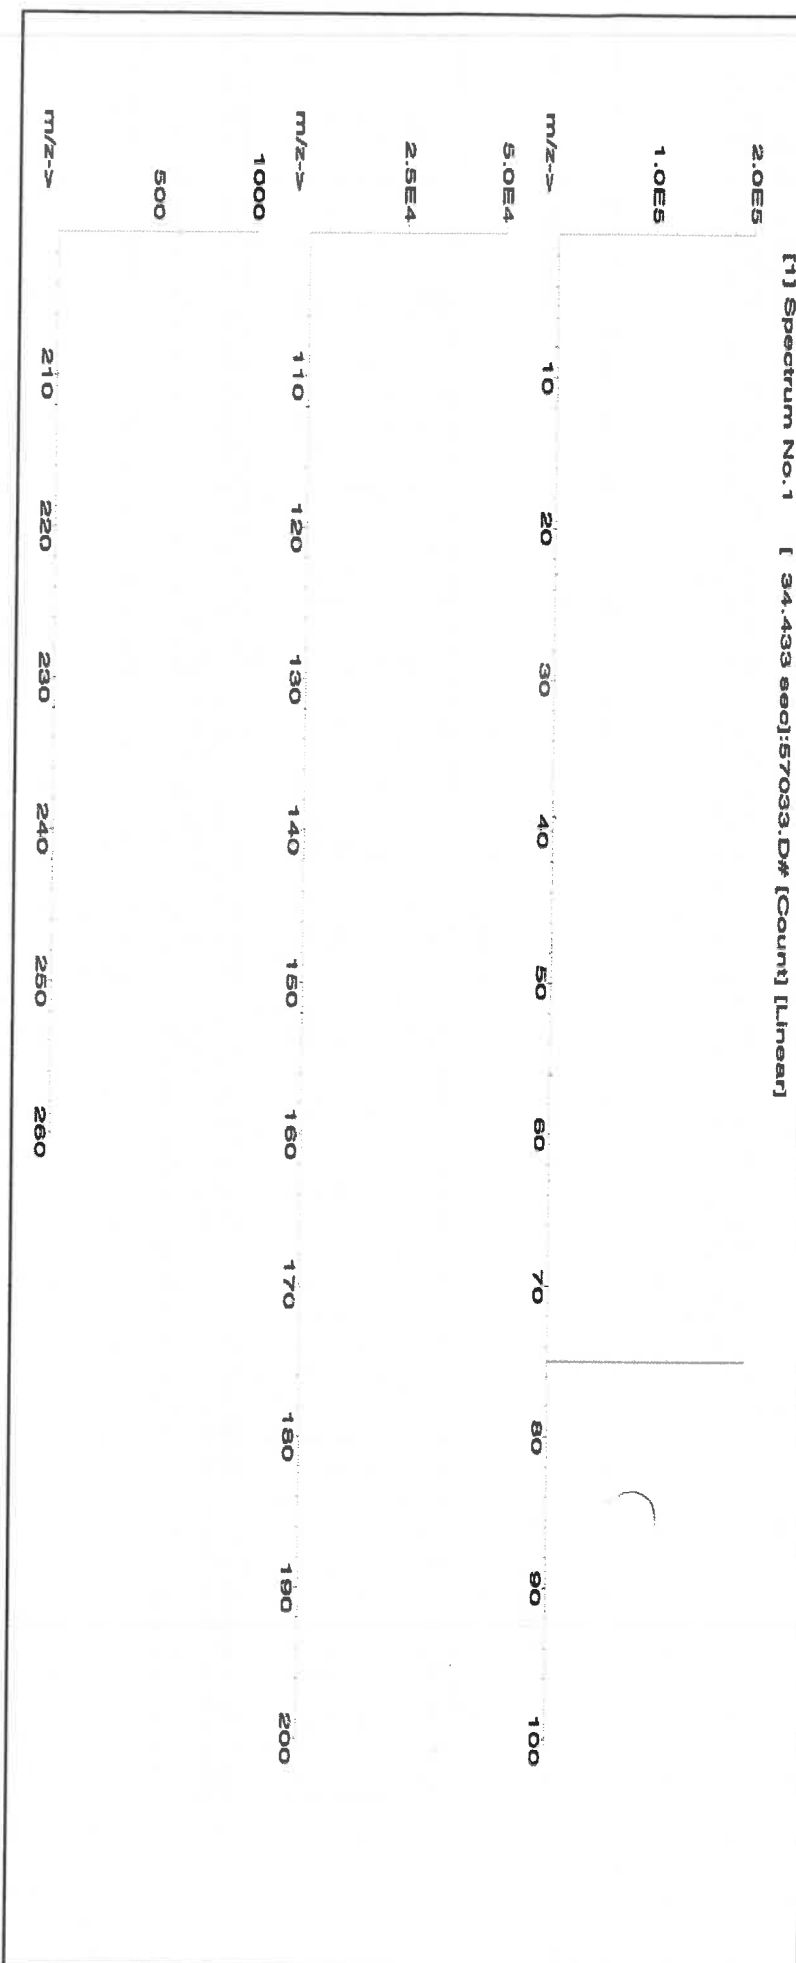



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	T	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Tl	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge*	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Su	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57115
Lot Number: 041723
Description: Phosphorous (P)

Solvent: 21110221 Nitric Acid

Lot #

Expiration Date: 041726

2% 40.0 (mL) Nitric Acid

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB

5E-05 Balance Uncertainty

Weight shown below was diluted to (mL): 2000.02 0.058 Flask Uncertainty


Formulated By:	Lawrence Barry
	041723
Reviewed By:	Pedro L. Rentas
	041723

SDS Information

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Ammonium dihydrogen phosphate (P) IN008 PVR2019A1 10000 99.999 0.10 27.5 72.7287 72.7289 10000.0 20.0 7722-76-1 5 mg/m3 or-hal->2000mg/kg 3186

[1] Spectrum No.1 [12.074 sec]:58115.D# [Count] [Linear]

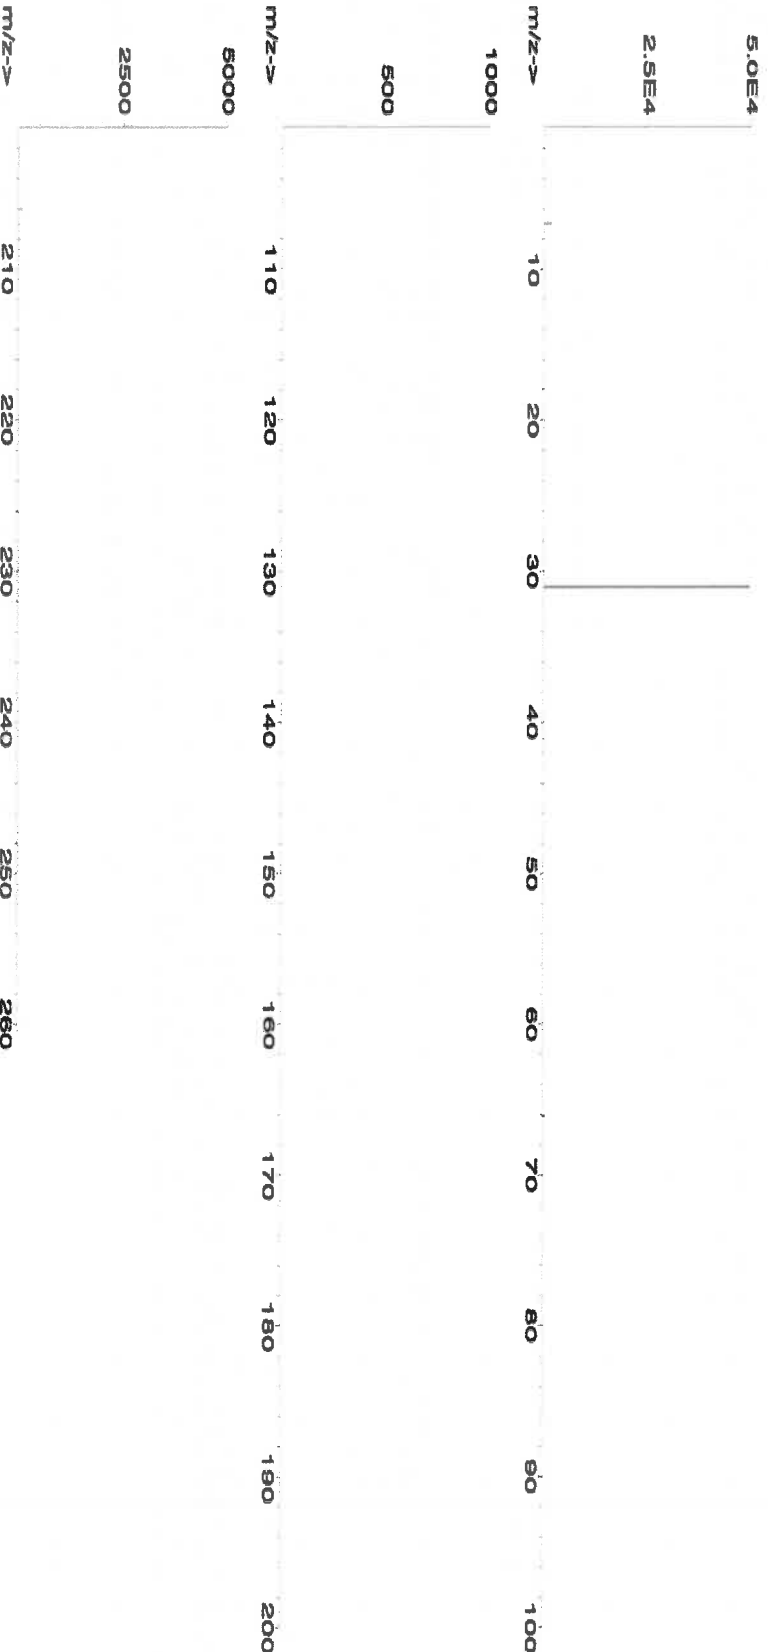



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	T	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57116
071123
Sulfur (S)

Lot #
Solvent: 071123
ASTM Type 1 Water

Formulated By:	Lawrence Barry
Reviewed By:	
Pedro L. Rentas	
071123	

188

Expiration Date: 071126
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 1999.48
5E-05 Balance Uncertainty
0.058 Flask Uncertainty


Compound

Lot	Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
-----	--------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

SDS Information

1. Ammonium sulfate (S)	IN117	SLBR725V	10000	99.9	0.10	24.3	82.4675	82.4692	10000.1	20.0	7783-20-2	NA	oral 4250mg/kg	3181
-------------------------	-------	----------	-------	------	------	------	---------	---------	---------	------	-----------	----	----------------	------

[1] Spectrum No. 1 [24.004 sec]:58116.D# [Count] [Linear]

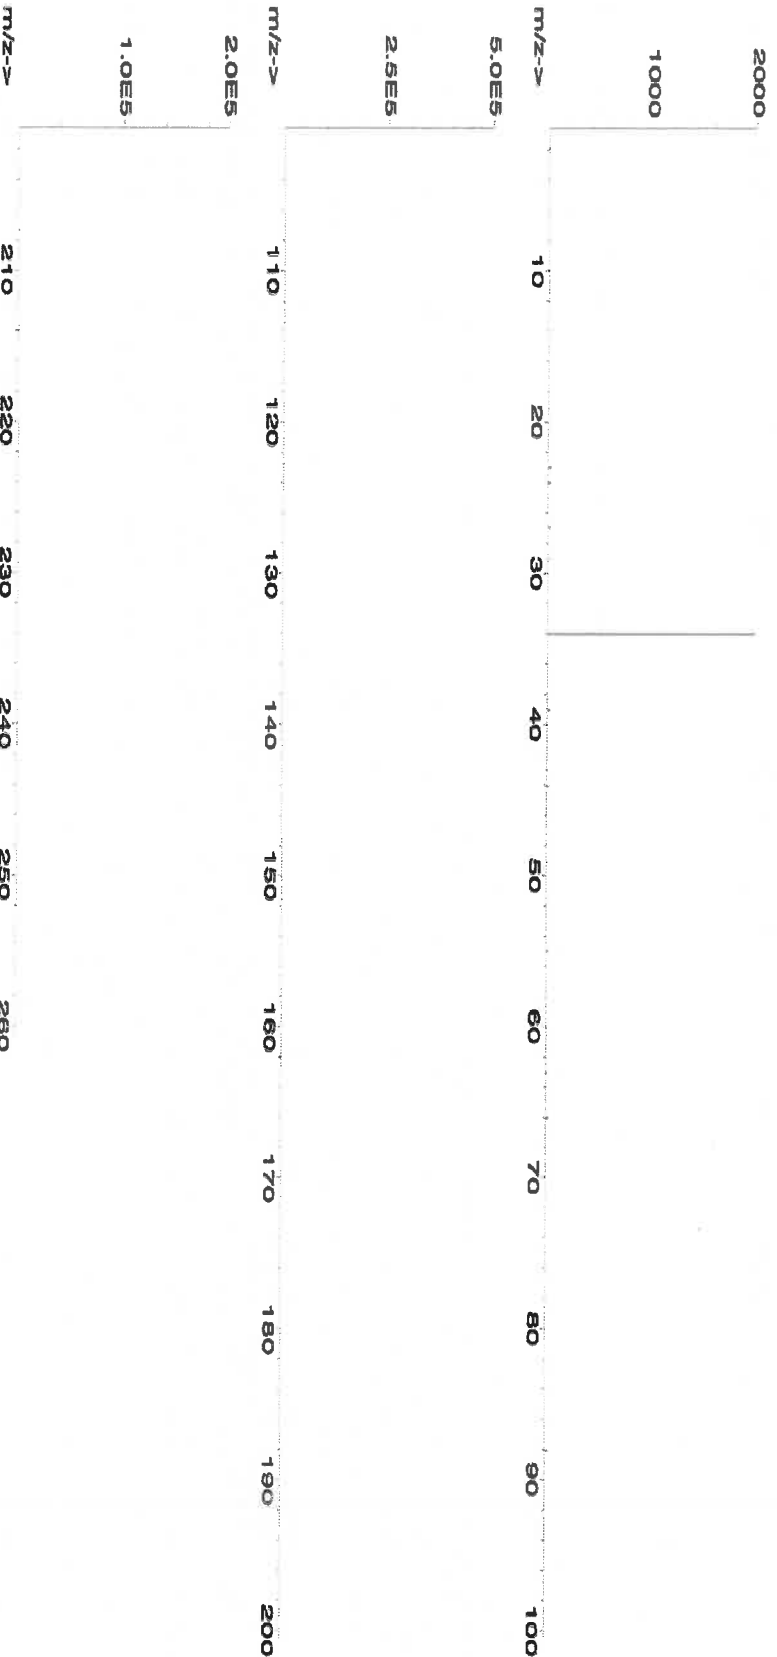



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Tm	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Sn	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	T	Ti	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02			Zr	<0.02

Physical Characterization:

(T)= Target analyte

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58030
Lot Number: 111623
Description: Zinc (Zn)

Solvent: 24002546 Nitric Acid

Lot # R: 02109124 MS819

2% 60.0 (mL) Nitric Acid

Expiration Date: 111626

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 3000.4

5E-05 Balance Uncertainty

0.06 Flask Uncertainty


Formulated By:	Benson Chan	111623
Reviewed By:	Pedro L. Rientas	111623

Compound

Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LDSO	NIST SRM
------------	-----------------------	------------	------------------------	------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Zinc nitrate hexahydrate (Zn) IN016 ZNE03021A1 1000 99.999 0.10 24.3 12.3475 12.3502 1000.2 2.0 10196-16-6 1 mg/mL 3168

[1] Spectrum No.1 [31.103 sec]58130.D# [Count] [Linear]

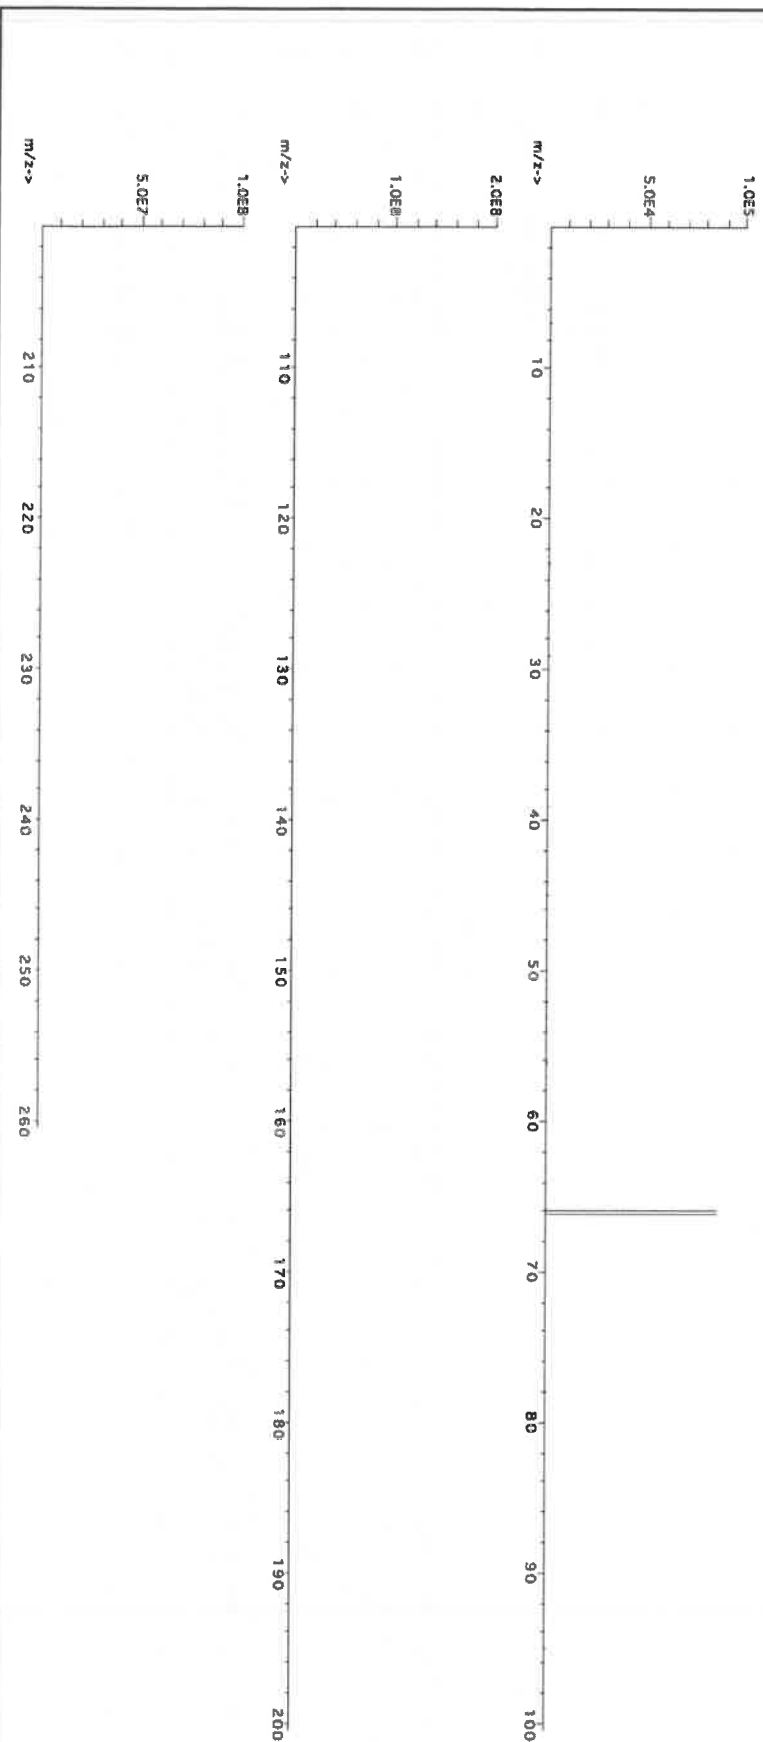



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

R: 02/22/24 M.5942

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGT11
Lot Number: T2-TI719972
Matrix: 2% (v/v) HNO₃
tr. HF
Value / Analyte(s): 1 000 µg/mL ea:
Titanium
Starting Material: Ti Metal
Starting Material Lot#: 2094
Starting Material Purity: 99.9975%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 1002 ± 5 µg/mL
Density: 1.012 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1 1002 ± 4 µg/mL
ICP Assay NIST SRM 3162a Lot Number: 130925

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum (1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k (u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000536	M	Eu	<	0.000268	O	Na	<	0.032670	M	Se		0.001204	O	Zn	<	0.003267
O	Al		0.000872	O	Fe		0.003225	O	Nb	<	0.043560	O	Si		0.004735	O	Zr	<	0.043560
M	As	<	0.008586	M	Ga	<	0.000268	M	Nd	<	0.000268	M	Sm	<	0.000268				
M	Au	<	0.004577	M	Gd	<	0.000268	O	Ni	<	0.010890	M	Sn		0.000096				
O	B	<	0.008929	M	Ge	<	0.002146	M	Os	<	0.000269	O	Sr		0.000096				
M	Ba	<	0.002683	M	Hf		0.002161	O	P	<	0.054450	M	Ta		0.010560				
M	Be	<	0.005366	M	Hg	<	0.003231	M	Pb	<	0.001073	M	Tb	<	0.000268				
M	Bi	<	0.001609	M	Ho	<	0.000268	M	Pd	<	0.000268	M	Te	<	0.001341				
O	Ca		0.000676	M	In	<	0.002683	M	Pr	<	0.000268	M	Th	<	0.053663				
M	Cd	<	0.000268	M	Ir	<	0.000269	M	Pt	<	0.000536	s	Ti	<					
M	Ce	<	0.000268	M	K		0.001172	M	Rb	<	0.000268	M	Tl	<	0.000268				
M	Co	<	0.004293	M	La	<	0.000268	M	Re	<	0.000268	M	Tm	<	0.000268				
M	Cr		0.000752	O	Li	<	0.027225	M	Rh	<	0.000268	M	U	<	0.000268				
M	Cs	<	0.000268	M	Lu	<	0.000268	M	Ru	<	0.000269	M	V	<	0.019855				
O	Cu	<	0.010890	O	Mg	<	0.005445	i	S	<		M	W		0.000473				
M	Dy	<	0.000268	O	Mn	<	0.003267	M	Sb	<	0.006976	M	Y	<	0.002146				
M	Er	<	0.000268	M	Mo		0.000774	O	Sc	<	0.004900	M	Yb	<	0.000536				

M - Checked by ICP-MS O - Checked by ICP-OES i - Spectral Interference
n - Not Checked For s - Solution Standard Element

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form in Solution - 47.87 +4 6 Ti(F)6-2

Chemical Compatibility - Soluble in concentrated HCl, HF, H3PO4 H2SO4 and HNO3. Avoid neutral to basic media. Unstable at ppm levels with metals that would pull F- away (i.e. Do not mix with Alkaline or Rare Earths or high levels of transition elements unless they are fluorinated). Stable with most inorganic anions with a tendency to hydrolyze forming the hydrated oxide in all dilute acids except HF.

Stability - 2-100 ppb levels stable (Alone or mixed with all other metals) as the Ti(F)6-2 for months in 1% HNO3 / LDPE container. 1-10,000 ppm single element solutions as the Ti(F)6-2 chemically stable for years in 2-5% HNO3 / trace HF in an LDPE container.

Ti Containing Samples (Preparation and Solution) - Metal (Soluble in H2O / HF caution -powder reacts violently); Oxide - low temperature history anatase or rutile (Dissolved by heating in 1:1:1 H2O / HF / H2SO4); Oxide - high temperature history (~800EC) brookite (fuse in Pt0 with K2S2O7); Ores (fuse in Pt0 with KF + K2S2O7 - no KF if silica not present); Organic Matrices (Dry ash at 450EC in Pt0 and dissolve by heating with 1:1:1 H2O / HF / H2SO4 or fuse ash with pyrosulfate if oxide is as plastic pigment and likely in brookite crystalline form).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 48 amu	14 ppt	N/A	32S16O, 32S14N, 14N16O18O, 14N17N2, 36Ar12C, 48Ca, [96X=2 (where X = Zr, Mo, Ru)]
ICP-OES 323.452 nm	0.0054 / 0.00092 µg/mL	1	Ce, Ar, Ni
ICP-OES 334.941 nm	0.0038 / 0.000028 µg/mL	1	Nb, Ta, Cr, U
ICP-OES 336.121 nm	0.0053 / 0.000034 µg/mL	1	W, Mo, Co

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

June 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- June 17, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



M5959 R: 6/14/24

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGY10
Lot Number: V2-Y740548
Matrix: 2% (v/v) HNO₃
Value / Analyte(s): 10 000 µg/mL ea:
Yttrium
Starting Material: Yttrium Oxide
Starting Material Lot#: 2661 and 06230520YL
Starting Material Purity: 99.9984%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 10000 ± 30 µg/mL
Density: 1.032 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	10011 ± 25 µg/mL EDTA NIST SRM 928 Lot Number: 928
Assay Method #2	9997 ± 50 µg/mL ICP Assay NIST SRM 3167a Lot Number: 190730
Assay Method #3	9984 ± 31 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum(1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k(u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum(w_i)^2(u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a)(u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (z) = U_{CRM/RM} = k(u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M Ag <	0.004600	M Eu	0.009037	M Na	0.086360	M Se <	0.005200	M Zn	0.030125
M Al	0.014862	O Fe	0.002410	M Nb <	0.000570	O Si	0.024100	O Zr <	0.002600
M As <	0.003500	M Ga <	0.000570	M Nd	0.000923	M Sm	0.000461		
M Au <	0.001700	M Gd <	0.003500	M Ni <	0.005700	M Sn <	0.002300		
O B	0.002209	M Ge <	0.005200	M Os <	0.001200	M Sr <	0.004600		
O Ba <	0.002500	M Hf <	0.000570	n P <		M Ta <	0.000570		
O Be <	0.001400	M Hg <	0.000570	M Pb	0.005020	M Tb	0.001044		
M Bi <	0.003500	M Ho	0.009037	M Pd <	0.005100	M Te <	0.002300		
O Ca	0.009841	M In <	0.002300	M Pr <	0.002300	M Th <	0.000570		
M Cd <	0.000570	M Ir <	0.000570	M Pt <	0.000570	M Ti <	0.003500		
M Ce <	0.002300	O K	0.018677	M Rb <	0.000570	M Tl <	0.000570		
M Co <	0.000570	M La	0.000461	M Re <	0.000570	M Tm <	0.003500		
M Cr <	0.004000	O Li <	0.009300	M Rh <	0.008000	M U <	0.000570		
M Cs <	0.000570	M Lu	0.000582	M Ru <	0.000570	M V	0.001265		
M Cu	0.002610	O Mg	0.001486	n S <		M W <	0.002300		
M Dy	0.003815	M Mn	0.000582	M Sb	0.005422	s Y <			
M Er	0.003615	M Mo <	0.005700	M Sc <	0.001200	M Yb	0.001827		

M - Checked by ICP-MS O - Checked by ICP-OES i - Spectral Interference
n - Not Checked For s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale, <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form in Solution - 88.91 +3 6 Y(OH)(H₂O)_{x+2}

Chemical Compatibility -Soluble in HCl, H₂SO₄ and HNO₃. Avoid HF, H₃PO₄ and neutral to basic media.

Stable with most metals and inorganic anions forming an insoluble carbonate, oxide, oxalate, and fluoride.

Avoid mixing with elements / solutions containing moderate amounts of fluoride.

Stability - 2-100 ppb levels stable for months in 1% HNO₃ / LDPE container. 1-10,000 ppm solutions chemically stable for years in 2-5% HNO₃ / LDPE container.

Y Containing Samples (Preparation and Solution) - Metal (Soluble in acids); Oxide (Dissolve by heating in H₂O / HNO₃); Ores (Carbonate fusion in PtO followed by HCl dissolution); Organic Matrices (Dry ash and dissolve in 1:1 H₂O / HCl or HNO₃).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 89 amu	0.8 ppt	N/A	73Ge16O, 178Hf+2
ICP-OES 360.073 nm	0.005 / 0.000036 µg/mL	1	Ce, Th
ICP-OES 371.030 nm	0.004 / 0.00007 µg/mL	1	Ce
ICP-OES 377.433 nm	0.005 / 0.0009 µg/mL	1	Ta, Th

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

February 20, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- February 20, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Custom Processing Supervisor



Certificate Approved By:

Muzzammil Khan
Stock Laboratory Supervisor



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





CERTIFIED WEIGHT REPORT:

Lot #

MS961 R-611124

Part Number: **57028**

Lot Number: **041124**

Description: **Nickel (NI)**

Solvent: 24002546 Nitric Acid

2% 5.0 (mL) Nitric Acid

Expiration Date: 041127

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): **1000**

NIST Test Number: 6UTB


Weight shown below was diluted to (mL): 249.85 5E-05 Balance Uncertainty 0.002 Flask Uncertainty

Formulated By:	Brian Geddes	041124
Reviewed By:	Pedro L. Rentas	041124

SDS Information

Compound	Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Uncertainty	(Solvent Safety Info. On Attached pg.)			NIST
	Number	Conc. (µg/mL)	(%)	Purity (%)	(%)	Weight (g)	Weight (g)	Conc. (µg/mL)	+/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	SRM

1. Nickel(II) nitrate hexahydrate (NI) IN033 NIM052023A1 1000 99.999 0.10 20.2 1.2369 1.2369 1000.0 2.0 13478-00-7 1 mg/m3 01-rat 1620 mg/kg 3136

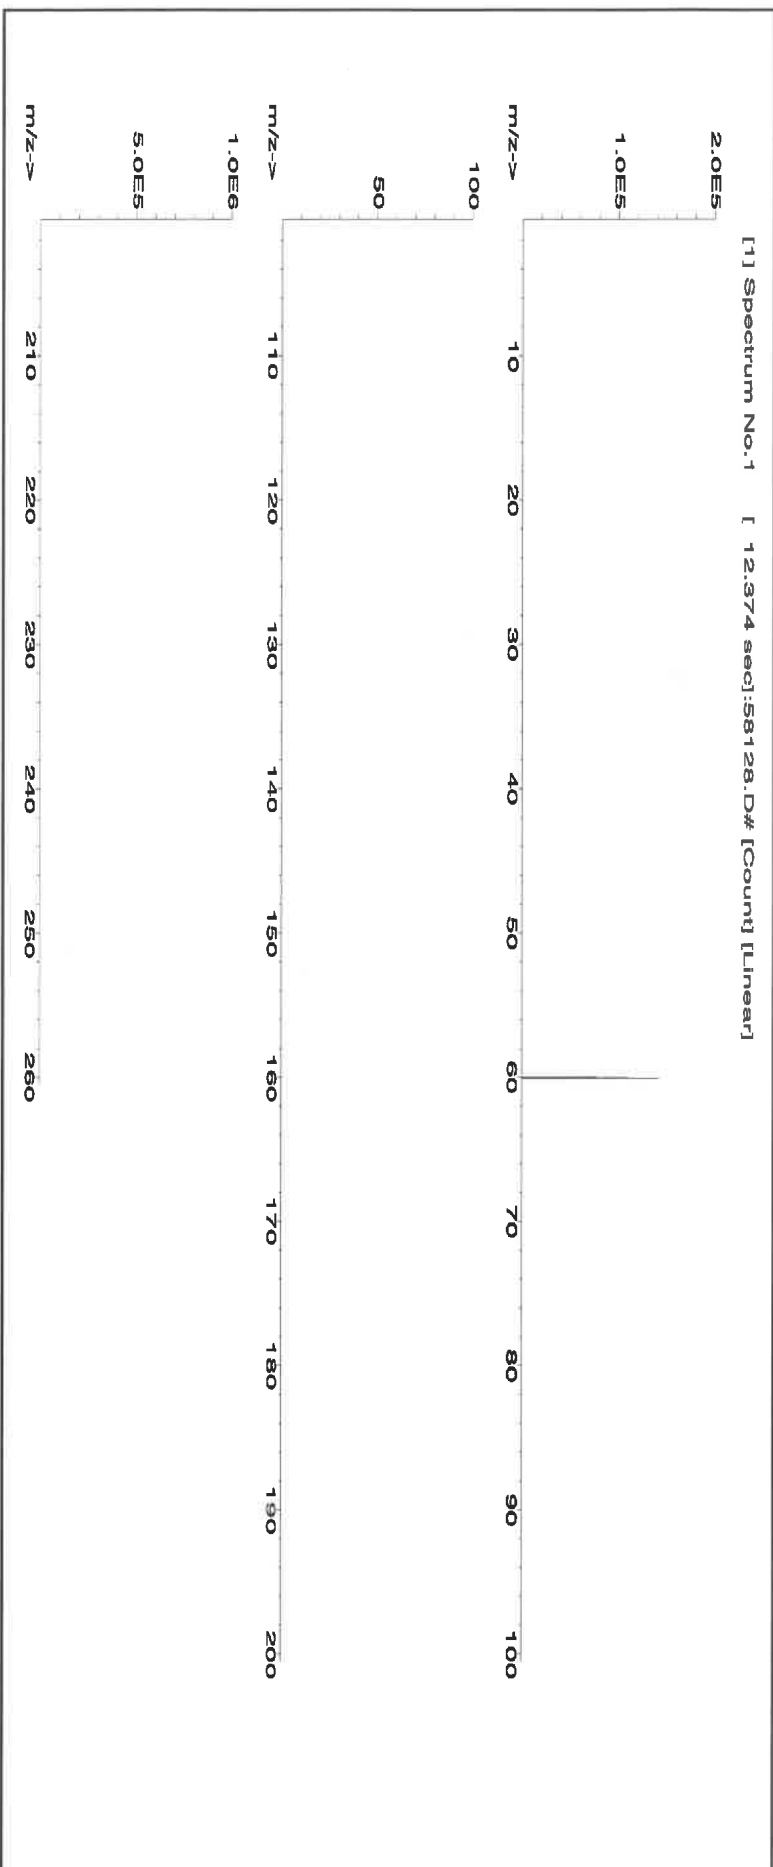



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	T	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Ba	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Bc	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

MS962 **R: 06/14/24**

Lot # **24002546** Solvent: **Nitric Acid**

Part Number: **57034**
Lot Number: **060624**
Description: **Selenium (Se)**

2.0%

40.0 (mL)

Nitric Acid

Expiration Date: **060627**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**

NIST Test Number: **6LUTB**

Volume shown below was diluted to (mL): **2000.07**

SE-05 Balance Uncertainty
0.100 Flask Uncertainty


Expanded

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	NIST SRM
1. Selenium (Se)	58134	071223	0.1000	200.0	0.084	1000	10002.5	1000.0	2.2	7782-49-2 0.2 mg/m3 or-tral 6700 mg/kg	3149

CAS# OSHA PEL (TWA) LDSO

Formulated By:	Benson Chan	060624
Reviewed By:	Pedro L. Rantas	060624

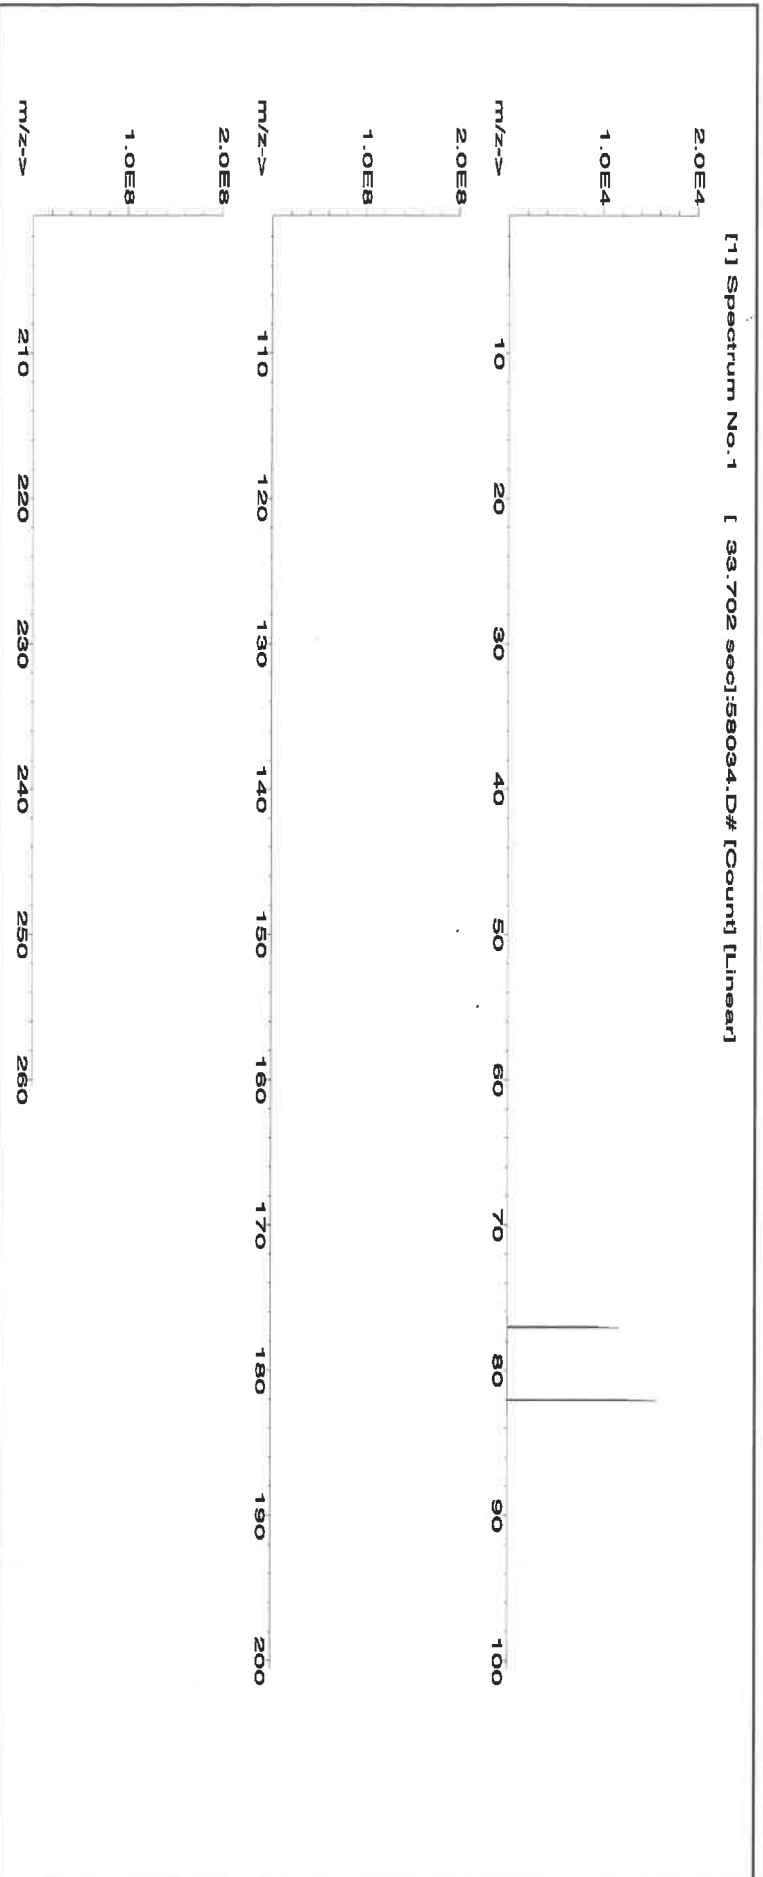



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

203

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	T	Tb	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Sn	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com



Certified Reference Material CRM
M5970 M5971 R1 710124


ANAB ISO 17034 Accredited
AR-1539 Certificate Number
https://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT:

Part Number: 57003
Lot Number: 062124
Description: Lithium (Li)
Expiration Date: 06/127
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 250.11
SE-05 Balance Uncertainty: 0.016
Fisk Uncertainty:

Microvite Capable	
Formulated By:	Giovanni Esposito
Reviewed By:	Petro L. Parias
Part Number:	062124

Compound		Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	SDS Information	NIST
1. Lithium nitrate (Li)		58103	070622	0.1000	25.0	0.004	1000	1000.0	10000.4	1000.0	2.0	7790-68-4 5 mg/mL 5 mL/1428 mg/kg	NA

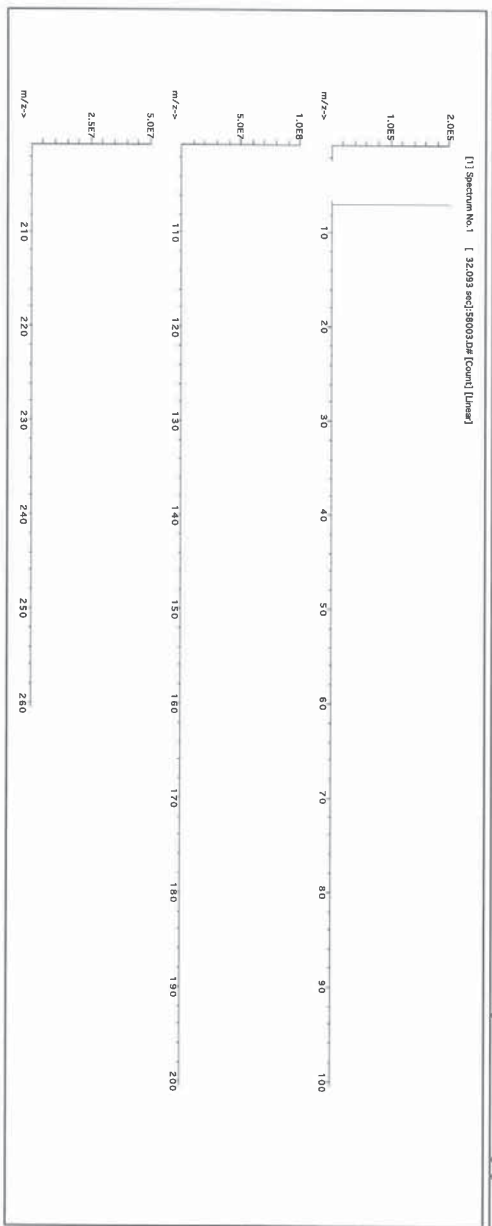

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com



Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
<https://AbsoluteStandards.com>

Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)															
Al	<0.02	Ca	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pb	<0.02	Se	<0.02
Sb	<0.02	Ce	<0.2	Er	<0.02	In	<0.02	Mg	<0.02	Nb	<0.02	Rb	<0.02	Si	<0.02
As	<0.2	Co	<0.02	Eu	<0.02	Ir	<0.02	Mn	<0.02	Os	<0.02	Sb	<0.02	Ag	<0.02
Ba	<0.02	Cr	<0.02	Gd	<0.02	La	<0.2	Hg	<0.2	Pd	<0.02	Sn	<0.02	Nd	<0.2
Be	<0.01	Cu	<0.02	Ga	<0.02	Mo	<0.02	K	<0.02	Pt	<0.02	Sm	<0.02	Sr	<0.02
Bi	<0.02	Fe	<0.02	Ge	<0.02	Nd	<0.02	Sc	<0.02	Te	<0.02	Ti	<0.02	Th	<0.02
B	<0.02	Ca	<0.02	Au	<0.02	Ta	<0.02	Na	<0.02	Tb	<0.02	Tm	<0.02	U	<0.02
														V	<0.02
														Yb	<0.02
														Y	<0.02
														Zn	<0.02
														Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

[Signature]

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST* (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Certificate of Analysis

M5976, M5977

R: 02/22/24

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGMO1
Lot Number: T2-MO720876
Matrix: H2O
tr. NH4OH
Value / Analyte(s): 1 000 µg/mL ea:
Molybdenum
Starting Material: Ammonium Molybdate
Starting Material Lot#: 2361
Starting Material Purity: 99.9893%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 998 ± 7 µg/mL
Density: 1.000 g/mL (measured at 20 ± 4 °C)
Assay Information:

Assay Method #1 998 ± 4 µg/mL
ICP Assay NIST SRM 3134 Lot Number: 130418

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance.

$$w_i = (1/u_{char i}^2) / (\sum (1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000590	M	Eu	<	0.000300	M	Na		0.000879	M	Se	<	0.008000	M	Zn		0.000598
M	Al		0.000563	M	Fe	<	0.006500	M	Nb	<	0.029000	i	Si	<		M	Zr	<	0.001800
M	As	<	0.002100	M	Ga	<	0.000300	i	Nd	<		M	Sm	<	0.000300				
M	Au	<	0.000300	M	Gd	<	0.000300	M	Ni	<	0.008000	M	Sn	<	0.008900				
M	B	<	0.003300	M	Ge	<	0.000300	M	Os	<	0.000590	M	Sr		0.000175				
M	Ba		0.001689	M	Hf	<	0.001800	i	P	<		M	Ta	<	0.004200				
M	Be	<	0.000890	M	Hg	<	0.003300	M	Pb	<	0.000300	M	Tb	<	0.000300				
M	Bi	<	0.000890	M	Ho	<	0.000300	M	Pd	<	0.001800	M	Te	<	0.021000				
O	Ca		0.006334	M	In	<	0.032000	M	Pr	<	0.013000	M	Th	<	0.000300				
O	Cd	<	0.026000	M	Ir	<	0.000300	M	Pt	<	0.000300	O	Tl	<	0.032000				
M	Ce	<	0.008300	M	K		0.130213	M	Rb		0.004575	M	Tl		0.001266				
M	Co		0.000598	M	La	<	0.000300	M	Re	<	0.000300	M	Tm	<	0.000300				
M	Cr		0.000527	O	Li		0.000059	M	Rh	<	0.000300	M	U	<	0.005300				
M	Cs		0.000527	M	Lu	<	0.000300	M	Ru	<	0.079000	M	V	<	0.000890				
M	Cu		0.002252	M	Mg		0.000563	i	S	<		M	W		0.087982				
M	Dy	<	0.000300	M	Mn	<	0.005900	M	Sb		0.001513	M	Y	<	0.000300				
M	Er	<	0.000300	s	Mo	<		M	Sc	<	0.001200	M	Yb	<	0.000300				

M - Checked by ICP-MS O - Checked by ICP-OES i - Spectral Interference
n - Not Checked For s - Solution Standard Element

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form in Solution - 95.94 +6 6,7,8,9

[MoO4]-2(chemical form as received)

Chemical Compatibility -Mo is received in a NH4OH matrix giving the operator the option of using HCl or HF to stabilize acidic solutions. The [MoO4]-2 is soluble in concentrated HCl [MoOCl5]-2, dilute HF / HNO3 [MoOF5]-2 and basic media [MoO4]-2. Stable at ppm levels with some metals provided it is fluorinated. Do not mix with Alkaline or Rare Earths when HF is present. Stable with most inorganic anions provided it is in the [MoO4]-2 chemical form.

Stability - 2-100 ppb levels stable (alone or mixed with all other metals that are at comparable levels) as the [MoOF5]-2 for months in 1% HNO3 / LDPE container. 1-10,000 ppm single element solutions as the [MoO4]-2 chemically stable for years in 1% NH4OH in a LDPE container.

Mo Containing Samples (Preparation and Solution) -Metal (Soluble in HF / HNO3 or hot dilute HCl); Oxide (soluble in HF or NH4OH) ; Organic Matrices (Dry ash at 450EC in Pt0 and dissolve oxide with HF or HCl).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 95 amu	3 ppt	n/a	40Ar39K16O,79Br16O,190Os2+,190Pt2+
ICP-OES 202.030 nm	0.008 / 0.0002 µg/mL	1	Os, Hf
ICP-OES 203.844 nm	0.012 / 0.002 µg/mL	1	
ICP-OES 204.598 nm	0.012 / 0.001 µg/mL	1	Ir, Ta

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6798; 540.585.3030, Fax: 540.585.3012; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

July 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- July 17, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Supervisor, Product Documentation



Certificate Approved By:

Michael Booth
Director, Technical



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate of Analysis

M5976, M5977

R: 02/22/24

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGMO1
Lot Number: T2-MO720876
Matrix: H2O
tr. NH4OH
Value / Analyte(s): 1 000 µg/mL ea:
Molybdenum
Starting Material: Ammonium Molybdate
Starting Material Lot#: 2361
Starting Material Purity: 99.9893%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 998 ± 7 µg/mL
Density: 1.000 g/mL (measured at 20 ± 4 °C)
Assay Information:

Assay Method #1 998 ± 4 µg/mL
ICP Assay NIST SRM 3134 Lot Number: 130418

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance.

$$w_i = (1/u_{char i}^2) / (\sum (1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i^2 (u_{char i}^2))]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000590	M	Eu	<	0.000300	M	Na		0.000879	M	Se	<	0.008000	M	Zn		0.000598
M	Al		0.000563	M	Fe	<	0.006500	M	Nb	<	0.029000	i	Si	<		M	Zr	<	0.001800
M	As	<	0.002100	M	Ga	<	0.000300	i	Nd	<		M	Sm	<	0.000300				
M	Au	<	0.000300	M	Gd	<	0.000300	M	Ni	<	0.008000	M	Sn	<	0.008900				
M	B	<	0.003300	M	Ge	<	0.000300	M	Os	<	0.000590	M	Sr		0.000175				
M	Ba		0.001689	M	Hf	<	0.001800	i	P	<		M	Ta	<	0.004200				
M	Be	<	0.000890	M	Hg	<	0.003300	M	Pb	<	0.000300	M	Tb	<	0.000300				
M	Bi	<	0.000890	M	Ho	<	0.000300	M	Pd	<	0.001800	M	Te	<	0.021000				
O	Ca		0.006334	M	In	<	0.032000	M	Pr	<	0.013000	M	Th	<	0.000300				
O	Cd	<	0.026000	M	Ir	<	0.000300	M	Pt	<	0.000300	O	Tl	<	0.032000				
M	Ce	<	0.008300	M	K		0.130213	M	Rb		0.004575	M	Tl		0.001266				
M	Co		0.000598	M	La	<	0.000300	M	Re	<	0.000300	M	Tm	<	0.000300				
M	Cr		0.000527	O	Li		0.000059	M	Rh	<	0.000300	M	U	<	0.005300				
M	Cs		0.000527	M	Lu	<	0.000300	M	Ru	<	0.079000	M	V	<	0.000890				
M	Cu		0.002252	M	Mg		0.000563	i	S	<		M	W		0.087982				
M	Dy	<	0.000300	M	Mn	<	0.005900	M	Sb		0.001513	M	Y	<	0.000300				
M	Er	<	0.000300	s	Mo	<		M	Sc	<	0.001200	M	Yb	<	0.000300				

M - Checked by ICP-MS O - Checked by ICP-OES i - Spectral Interference
n - Not Checked For s - Solution Standard Element

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form in Solution - 95.94 +6 6,7,8,9

[MoO4]-2(chemical form as received)

Chemical Compatibility -Mo is received in a NH4OH matrix giving the operator the option of using HCl or HF to stabilize acidic solutions. The [MoO4]-2 is soluble in concentrated HCl [MoOCl5]-2, dilute HF / HNO3 [MoOF5]-2 and basic media [MoO4]-2. Stable at ppm levels with some metals provided it is fluorinated. Do not mix with Alkaline or Rare Earths when HF is present. Stable with most inorganic anions provided it is in the [MoO4]-2 chemical form.

Stability - 2-100 ppb levels stable (alone or mixed with all other metals that are at comparable levels) as the [MoOF5]-2 for months in 1% HNO3 / LDPE container. 1-10,000 ppm single element solutions as the [MoO4]-2 chemically stable for years in 1% NH4OH in a LDPE container.

Mo Containing Samples (Preparation and Solution) -Metal (Soluble in HF / HNO3 or hot dilute HCl); Oxide (soluble in HF or NH4OH) ; Organic Matrices (Dry ash at 450EC in Pt0 and dissolve oxide with HF or HCl).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 95 amu	3 ppt	n/a	40Ar39K16O,79Br16O,190Os2+,190Pt2+
ICP-OES 202.030 nm	0.008 / 0.0002 µg/mL	1	Os, Hf
ICP-OES 203.844 nm	0.012 / 0.002 µg/mL	1	
ICP-OES 204.598 nm	0.012 / 0.001 µg/mL	1	Ir, Ta

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

July 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- July 17, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Supervisor, Product Documentation



Certificate Approved By:

Michael Booth
Director, Technical



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate of Analysis



Refine your results. Redefine your industry.

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

R: 2/22/24

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution

Catalog Number: CGT1

Lot Number: T2-T1719972

Matrix: 2% (v/v) HNO₃

Value / Analyte(s): tr. HF

Starting Material: 1 000 µg/mL ea.

Starting Material: Titanium

Starting Material: Ti Metal

Starting Material Lot#: 2094

Starting Material Purity: 99.9975%

CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 1002 ± 5 µg/mL

Density: 1.012 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1 1002 ± 4 µg/mL

ICP Assay NIST SRM 3162a Lot Number: 130925

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods
Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = 2(w) / (w_1 + w_2)$$

w_1 = the weighting factors for each method calculated using the inverse square of the variance

$$w_1 = (1/u_{CRM}^2) / (1/u_{CRM}^2 + 1/u_{CRM}^2)$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

$$u_{CRM} = \sqrt{u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2 + u_{CRM}^2}$$

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0

TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an UHPA-filtered Clean Room. An UHPA-filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M Ag	<	0.000536	M Eu	<	0.000268	O Na	<	0.032670	M Se	0.001204	O Zn	<	0.003267
M Al	<	0.000872	O Fe	<	0.003225	O Nb	<	0.043560	O Si	0.004735	O Zr	<	0.043560
M As	<	0.008586	M Ga	<	0.000268	M Nd	<	0.000268	M Sm	<	0.000268		
M Au	<	0.004577	M Gd	<	0.000268	O Ni	<	0.010890	M Sn	<	0.00096		
O B	<	0.008929	M Ge	<	0.002146	M Os	<	0.000269	O Sr	<	0.00096		
M Ba	<	0.002683	M Hf	<	0.002161	O P	<	0.054450	M Ta	<	0.010560		
M Be	<	0.005366	M Hg	<	0.003231	M Pb	<	0.001073	M Tb	<	0.000268		
M Bi	<	0.001609	M Ho	<	0.000268	M Pd	<	0.000268	M Th	<	0.001341		
O Ca	<	0.000676	M In	<	0.002683	M Pr	<	0.000268	M Tl	<	0.053663		
M Cd	<	0.000268	M Ir	<	0.000269	M Pt	<	0.000536	S Tl	<			
M Co	<	0.000268	M K	<	0.001172	M Rb	<	0.000268	M Ti	<	0.000268		
M Cr	<	0.000752	O Li	<	0.000268	M Re	<	0.000268	M Tm	<	0.000268		
M Cs	<	0.000268	M Lu	<	0.000268	M Rh	<	0.000268	M U	<	0.000268		
O Cu	<	0.010890	O Mg	<	0.005445	I S	<	0.006976	M Y	<	0.002146		
M Dy	<	0.000268	O Mn	<	0.003267	M Sb	<	0.004900	M Yb	<	0.000536		
M Er	<	0.000268	M Mo	<	0.000774	O Sc	<						

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence: Soluble in concentrated HCl, HF, H₃PO₄, H₂SO₄ and HNO₃. Avoid neutral to basic media. Unstable at ppm levels with metals that would pull F⁻ away (i.e. Do not mix with Alkaline or Rare Earths or high levels of transition elements unless they are fluorinated). Stable with most inorganic anions with a tendency to hydrolyze forming the hydrated oxide in all dilute acids except HF.

Stability: - 2-100 ppb levels stable (Alone or mixed with all other metals) as the Ti(F)₆-2 for months in 1% HNO₃ / LDPE container. - 1-10,000 ppm single element solutions as the Ti(F)₆-2 chemically stable for years in 2-5% HNO₃ / trace HF in an LDPE container.

Ti Containing Samples (Preparation and Solution) - Metal (Soluble in H₂O / HF caution - powder reacts violently): Oxide - low temperature history anatase or rutile (Dissolved by heating in 1:1:1 H₂O / HF / H₂SO₄); K₂SiO₃ - no KF if silica not present); Organic Matrices (Dry ash at 450°C in P10 and dissolve by heating with 1:1:1 H₂O / HF / H₂SO₄ or fuse ash with pyrosulfate if oxide is as plastic pigment and likely in brookite crystalline form).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 48 amu	14 ppt	N/A	32S16O, 32S14N, 14N16O18O, 14N17N2, 36Ar12C, 48Ca, [96X=2 (where X = Zr, Mo, W, Mo, Co, Nb, Ta, Cr, U, Ce, Ar, Ni, Ru)]
ICP-OES 323.452 nm	0.0054 / 0.00092 µg/mL	1	
ICP-OES 334.941 nm	0.0038 / 0.00028 µg/mL	1	
ICP-OES 336.121 nm	0.0053 / 0.00034 µg/mL	1	

HAZARDOUS INFORMATION

HF Note: This standard should not be prepared or stored in glass.

8.0

HOMOGENEITY

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.
- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous.
- Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0

QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY
Inorganic Ventures, 300 Technology Drive, Chesapeake, VA 24073, USA. Telephone: 800.868.6786; 540.565.3030; Fax: 540.565.3012; info@inorganicventures.com

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

11.1 Certification Issue Date

June 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- June 17, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date:

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Thomas Kozlikowski
Manager, Quality Control

Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director

Paul Gaines

80978

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

M5985
R: 6/14/24

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGIN10
Lot Number: U2-IN729349
Matrix: 5% (v/v) HNO₃
Value / Analyte(s): 10 000 µg/mL ea:
Indium
Starting Material: Indium Metal
Starting Material Lot#: 2511
Starting Material Purity: 99.9995%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 10022 ± 30 µg/mL
Density: 1.044 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	10021 ± 56 µg/mL ICP Assay NIST SRM 3124a Lot Number: 110516
Assay Method #2	10035 ± 25 µg/mL EDTA NIST SRM 928 Lot Number: 928
Assay Method #3	10001 ± 33 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum (1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k (u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000760	M	Eu	<	0.000760	O	Na	0.012771	M	Se	<	0.023000	M	Zn	<	0.006100
M	Al	0.003385	O	Fe	0.004462	M	Nb	<	0.000760	O	Si	0.024619	M	Zr	<	0.000760		
M	As	<	0.004600	M	Ga	<	0.000760	M	Nd	<	0.000760	M	Sm	<	0.000760			
M	Au	<	0.002300	M	Gd	<	0.000760	O	Ni	<	0.005100	M	Sn	<	0.000760			
O	B	0.003692	M	Ge	<	0.001600	M	Os	<	0.000760	O	Sr	<	0.000610				
M	Ba	<	0.001600	M	Hf	<	0.000760	n	P	<		M	Ta	<	0.000760			
O	Be	<	0.000130	M	Hg	<	0.003100	M	Pb	0.001400	M	Tb	<	0.000760				
M	Bi	<	0.000760	M	Ho	<	0.000760	M	Pd	<	0.001600	M	Te	<	0.000760			
O	Ca	0.004616	s	In	<			M	Pr	<	0.000760	M	Th	<	0.000760			
M	Cd	<	0.000760	M	Ir	<	0.000760	M	Pt	<	0.000760	O	Ti	<	0.001100			
M	Ce	<	0.000760	O	K	0.007078	M	Rb	<	0.000760	M	Tl	<	0.000760				
M	Co	<	0.000760	M	La	<	0.000760	M	Re	<	0.000760	M	Tm	<	0.000760			
O	Cr	<	0.001300	O	Li	<	0.000130	M	Rh	<	0.000760	M	U	<	0.000760			
M	Cs	<	0.000760	M	Lu	<	0.000760	M	Ru	<	0.000760	M	V	<	0.001600			
M	Cu	<	0.003800	O	Mg	0.000707	n	S	<		M	W	<	0.001600				
M	Dy	<	0.000760	O	Mn	0.000149	M	Sb	<	0.000760	M	Y	<	0.000760				
M	Er	<	0.000760	M	Mo	<	0.002300	M	Sc	<	0.000760	M	Yb	<	0.000760			

M - Checked by ICP-MS

O - Checked by ICP-OES

i - Spectral Interference

n - Not Checked For

s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale, <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form In Solution - 114.82 +3 6 In(H₂O)₆+3

Chemical Compatibility -Soluble in HCl, HNO₃, and H₂SO₄. Avoid neutral and basic media. Stable with most metals and inorganic anions. The oxalate, sulfide, carbonate, hydroxide and phosphate are insoluble in water.

Stability - 2-100 ppb levels stable for months in 1% HNO₃ / LDPE container. 1-10,000 ppm solutions chemically stable for years in 2-5% HNO₃ / LDPE container.

In Containing Samples (Preparation and Solution) -Metal (Best dissolved in HCl / HNO₃); Oxide (Soluble in mineral acids); Ores (Carbonate fusion in PtO followed by HCl dissolution); Organic Matrices (Sulfuric/peroxide digestion or dry ash and dissolution in dilute HCl).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 115 amu	1 ppt	n/a	115Sn, 99Ru16O
ICP-OES 158.583 nm	0.05 / 0.002 µg/mL	1	
ICP-OES 230.606 nm	0.1 / 0.03 µg/mL	1	Ni, Os
ICP-OES 325.609 nm	0.2 / 0.05 µg/mL	1	Mn, Mo, Th

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; Info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

February 21, 2023

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- February 21, 2028

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

Certificate of Analysis

M6074

M6075

M6076

M6077

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

EXP: 9/6/2029

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CHEM-CLP-4
Lot Number: V2-MEB746762
Matrix: 3% (v/v) HNO₃
3% (v/v) HF
Value / Analyte(s): 1 000 µg/mL ea:
Boron, Molybdenum,
Silicon, Tin,
Titanium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Boron, B	1 000 ± 5 µg/mL	Molybdenum, Mo	1 000 ± 5 µg/mL
Silicon, Si	1 000 ± 7 µg/mL	Tin, Sn	1 000 ± 5 µg/mL
Titanium, Ti	1 000 ± 6 µg/mL		

Density: 1.033 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
B	ICP Assay	3107	190605
B	Calculated		See Sec. 4.2
Mo	ICP Assay	traceable to 3134	U2-MO739068
Si	ICP Assay	Traceable to 3150	S2-SI702546
Sn	ICP Assay	3161a	140917
Ti	ICP Assay	traceable to 3162a	T2-TI725816

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

September 06, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **September 06, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Joseph Burns
Custom VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Hydrochloric Acid, 36.5-38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



R → 16/13/24
Met dig

M 6121

Material No.: 9530-33
Batch No.: 0000275677
Manufactured Date: 2020/12/16
Retest Date: 2025/12/15
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 - 38.0 %	37.6
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Specific Gravity at 60°/60°F	1.185 - 1.192	1.190
ACS - Bromide (Br)	<= 0.005 %	< 0.005
ACS - Extractable Organic Substances	<= 5 ppm	1
ACS - Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities - Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities - Aluminum (Al)	<= 10.0 ppb	< 0.2
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities - Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities - Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	29.7
Trace Impurities - Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC


100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

226

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	< 0.2
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	< 1
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.1
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.3
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use
Product Information (not specifications):
Appearance (clear, fuming liquid)
Meets ACS Specifications

Country of Origin: US
Packaging Site: Phillipsburg Mfg Ctr & DC

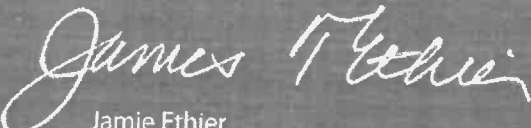
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

227

Nitric Acid 69%
CMOS

avantor™



R → 11/12/24

M6126

Material No.: 9606-03
Batch No.: 24D1062002
Manufactured Date: 2024-03-26
Retest Date: 2029-03-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (HNO ₃)	69.0 – 70.0 %	69.7 %
Appearance	Passes Test	Passes Test
Color (APHA)	≤ 10	5
Residue after Ignition	≤ 2 ppm	1 ppm
Chloride (Cl)	≤ 0.08 ppm	< 0.03 ppm
Phosphate (PO ₄)	≤ 0.10 ppm	< 0.03 ppm
Sulfate (SO ₄)	≤ 0.2 ppm	< 0.2 ppm
Trace Impurities – Aluminum (Al)	≤ 40.0 ppb	< 1.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities – Barium (Ba)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 50 ppb	< 1 ppb
Trace Impurities – Calcium (Ca)	≤ 50.0 ppb	2.3 ppb
Trace Impurities – Chromium (Cr)	≤ 30.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 20 ppb	< 10 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Heavy Metals (as Pb)	≤ 100 ppb	100 ppb
Trace Impurities – Iron (Fe)	≤ 40.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Nickel (Ni)	≤ 20.0 ppb	< 5.0 ppb

>>> Continued on page 2 >>>

Nitric Acid 69%
CMOS

 **avantor**TM



Material No.: 9606-03
Batch No.: 24D1062002

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak
Director Quality Operations, Bioscience Production

229



Lot

Hieranni Capote

230

40.0 Nitric Acid
(mL)

296

40.0 Nitric Acid

5E-05 Balance Uncertainty

0.100 Flask Uncertainty

Formulated By:	Giovanni Esposito	112124
Reviewed By:	Pedro L. Rents	112124

Pedro L. Rentas


112124

SDS Information

[illegible]

Magnesium nitrate hexahydrate (Mg)	INCO	MOORECZAK
10000	98.999	0.10
8.51	234.9183	234.9459
10001.2	20.0	13446-18-9
NA		on-fat 5440 mg/kg 3131a

[1] Spectrum No.1	[19.823 sec]:58112.D#	[Count]	[Linear]
-------------------	-----------------------	---------	----------

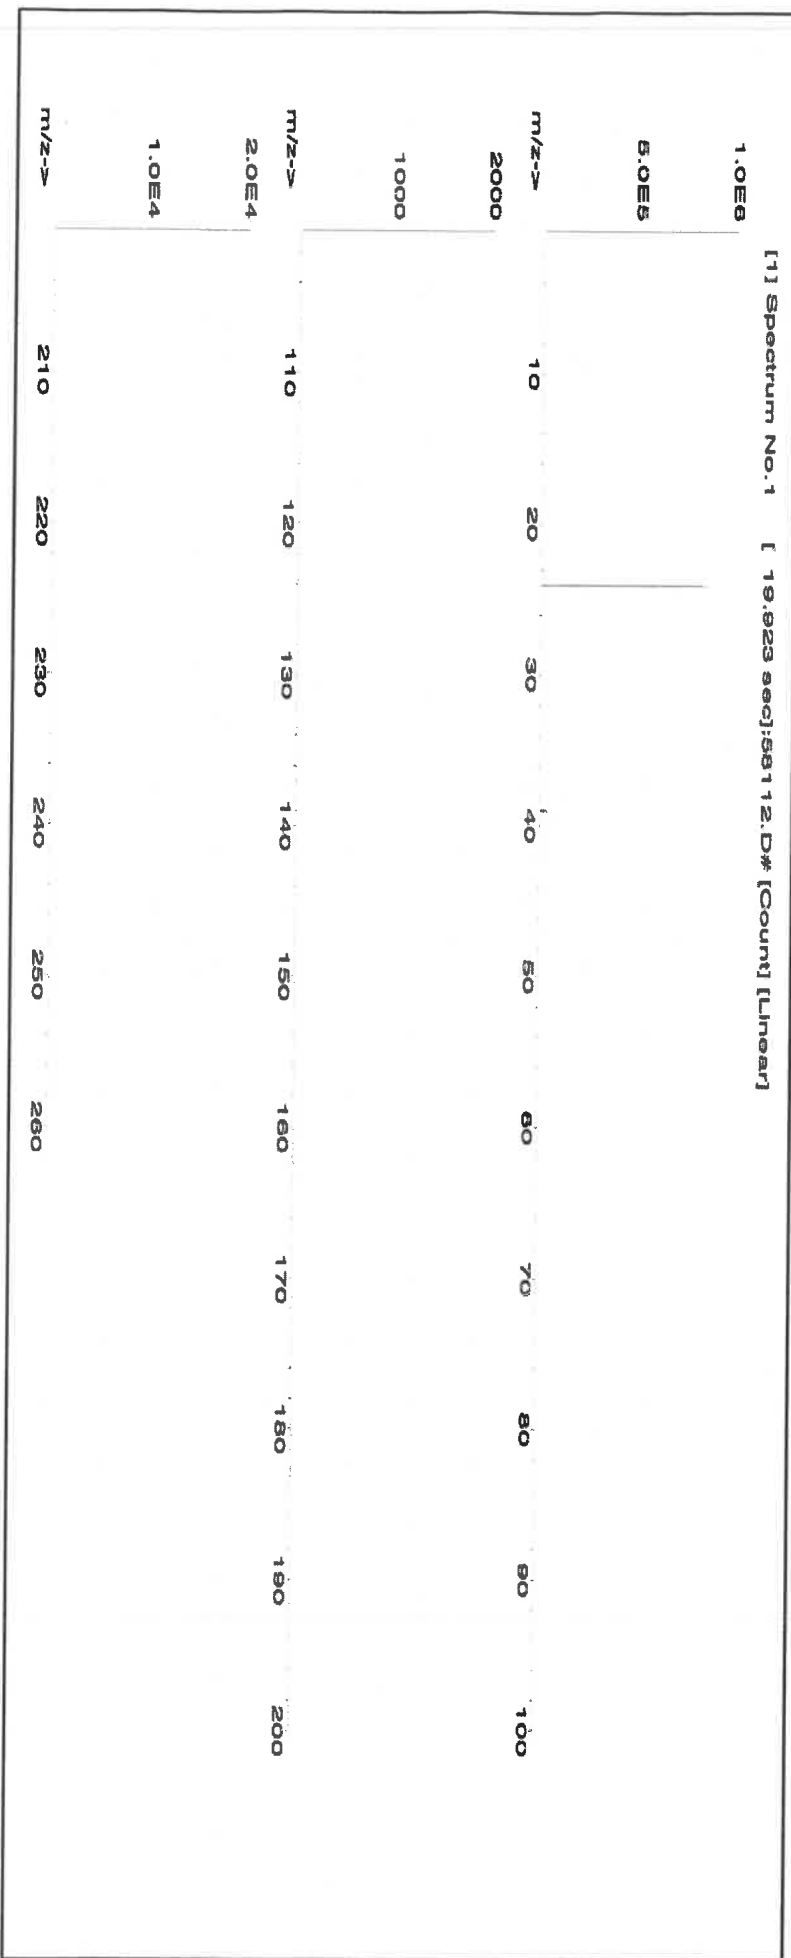



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Rc	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	T	Os	<0.02	Rb	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Tm	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sm	<0.02	Sr	<0.02	Sn	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sc	<0.02	S	<0.02	Ti	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2			Ta	<0.02			Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

233

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	T	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58111
Lot Number: 072424
Description: Sodium (Na)

Lot #

R-→ 1113/25 Solvent: 24002546 Nitric Acid

Expiration Date: 072427
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB

146144 2% 80.0 (mL) Nitric Acid

Weight shown below was diluted to (mL): 4000.2 0.10 Flask Uncertainty


Formulated By:	Benson Chan	072424
Reviewed By:	Pedro L. Renteria	072424

SDS Information

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Sodium nitrate (Na) IN036 NAV01201511 10000 99.999 0.10 26.9 148.7096 ##### 10000.0 20.0 7631-99-4 5 mg/m3 orl-rat 3430 mg/kg 3152a

[1] Spectrum No. 1 [8.935 sec]: 58111.D# [Count] [Linear]

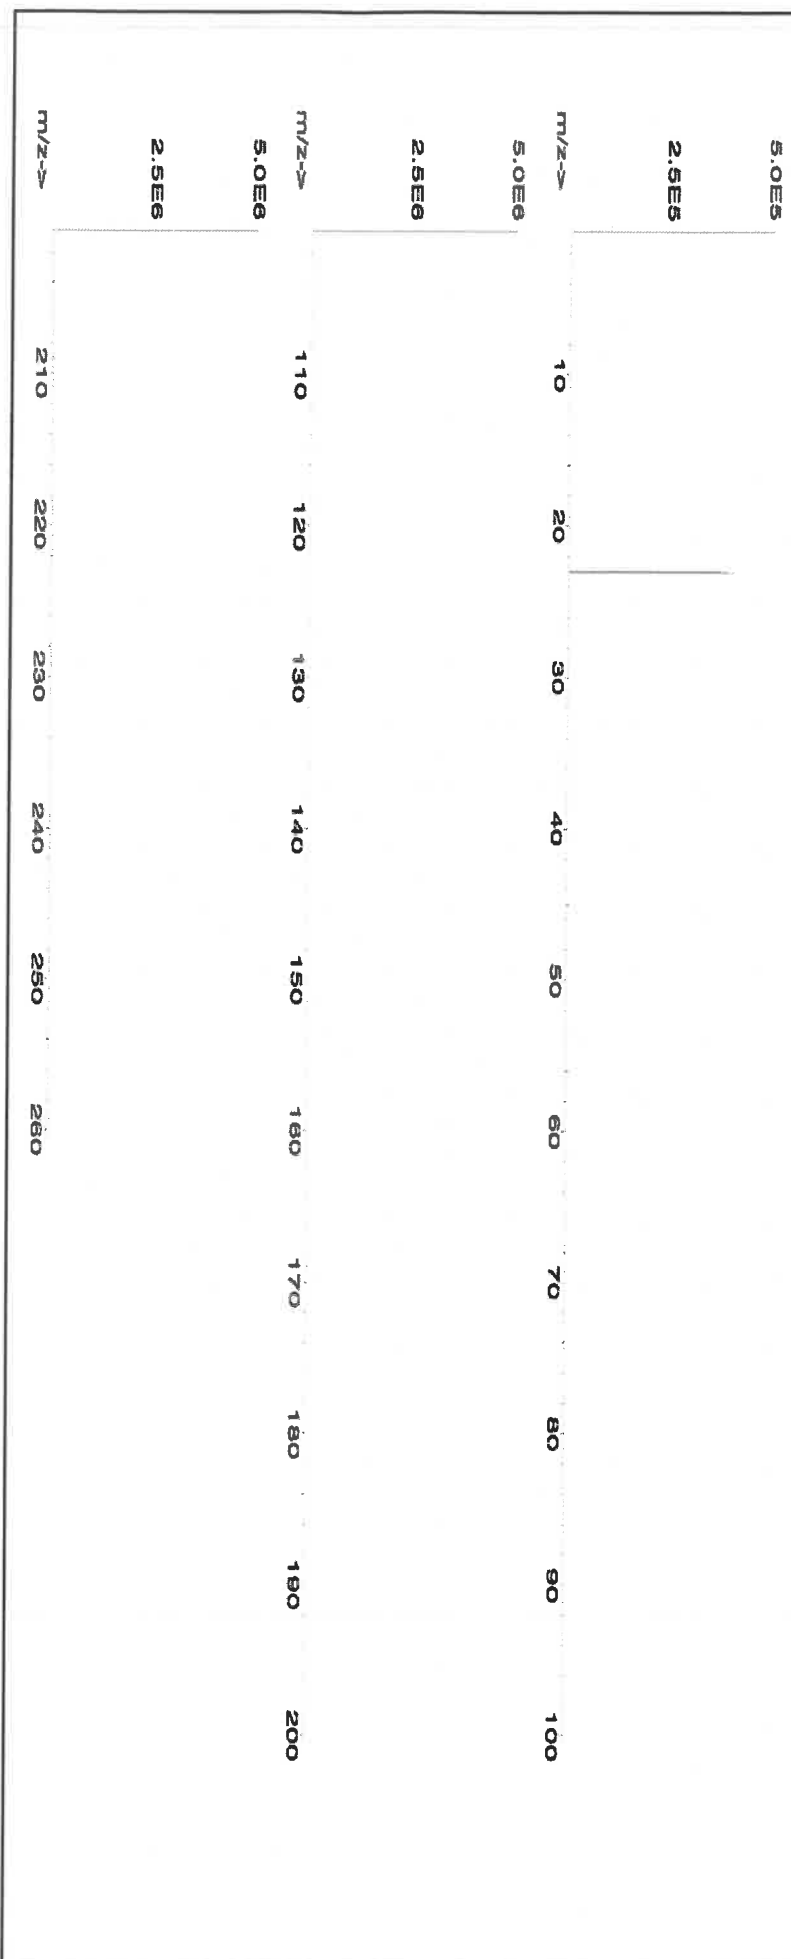



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

235

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rb	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	T	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: **58030** Lot # **24012496**
Lot Number: **121724** Nitric Acid
Description: **Zinc (Zn)**

Expiration Date: **121727** 2%
Recommended Storage: **Ambient (20 °C)** 40.0 (mL)
Nominal Concentration (µg/mL): **1000** Nitric Acid

NIST Test Number: **6UTB**

Weight shown below was diluted to (mL): **2000.1** 0.10 Balance Uncertainty
Flask Uncertainty


<i>Aleah O'Brady</i>	
Formulated By:	Aleah O'Brady
Reviewed By:	<i>Pedro L. Rentias</i>
	Pedro L. Rentias
	121724

Compound

RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
-----	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Zinc nitrate hexahydrate (Zn) IN016 ZNE032021A1 1000 99.999 0.10 24.3 8.2308 8.2311 1000.0 2.0 10196-18-6 1 mg/m3 or-rat 1190mg/kg 3168

[1] Spectrum No.1 [31.103 sec; 58130.D# [Count] [Linear]

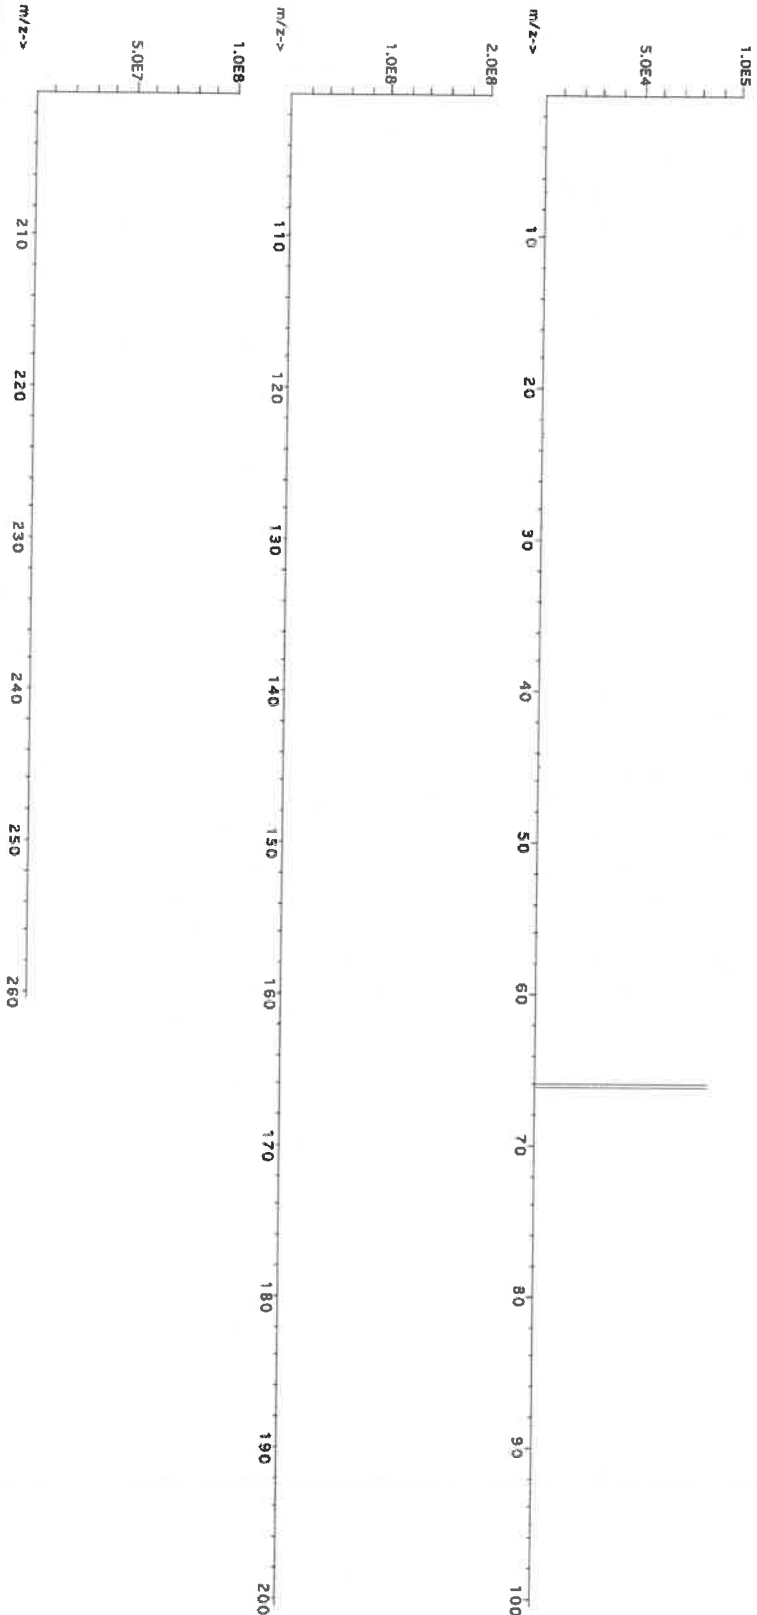



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Md	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58111
Lot Number: 122223
Description: Sodium (Na)

Solvent: 24002546 Nitric Acid

Lot #

Expiration Date: 122226

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 3000.4 0.06 Flask Uncertainty

2% 60.0 (mL) Nitric Acid

<i>Aleah O Brady</i>	
Formulated By:	Aleah O Brady
Reviewed By:	Pedro L. Rentas
	122223


Expanded

SDS Information

Compound	Lot	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-----	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	-------------------------	------	----------------	------	----------

1. Sodium nitrate (Na) IN036 NAV01201511 10000 99.999 0.10 26.9 111.5406 111.5479 10000.7 20.0 7631-99-4 5 mg/m3 or-trat 3430 mg/kg 3152a

[1] Spectrum No.1 [8.935 sec]:58111.D# [Count] [Linear]

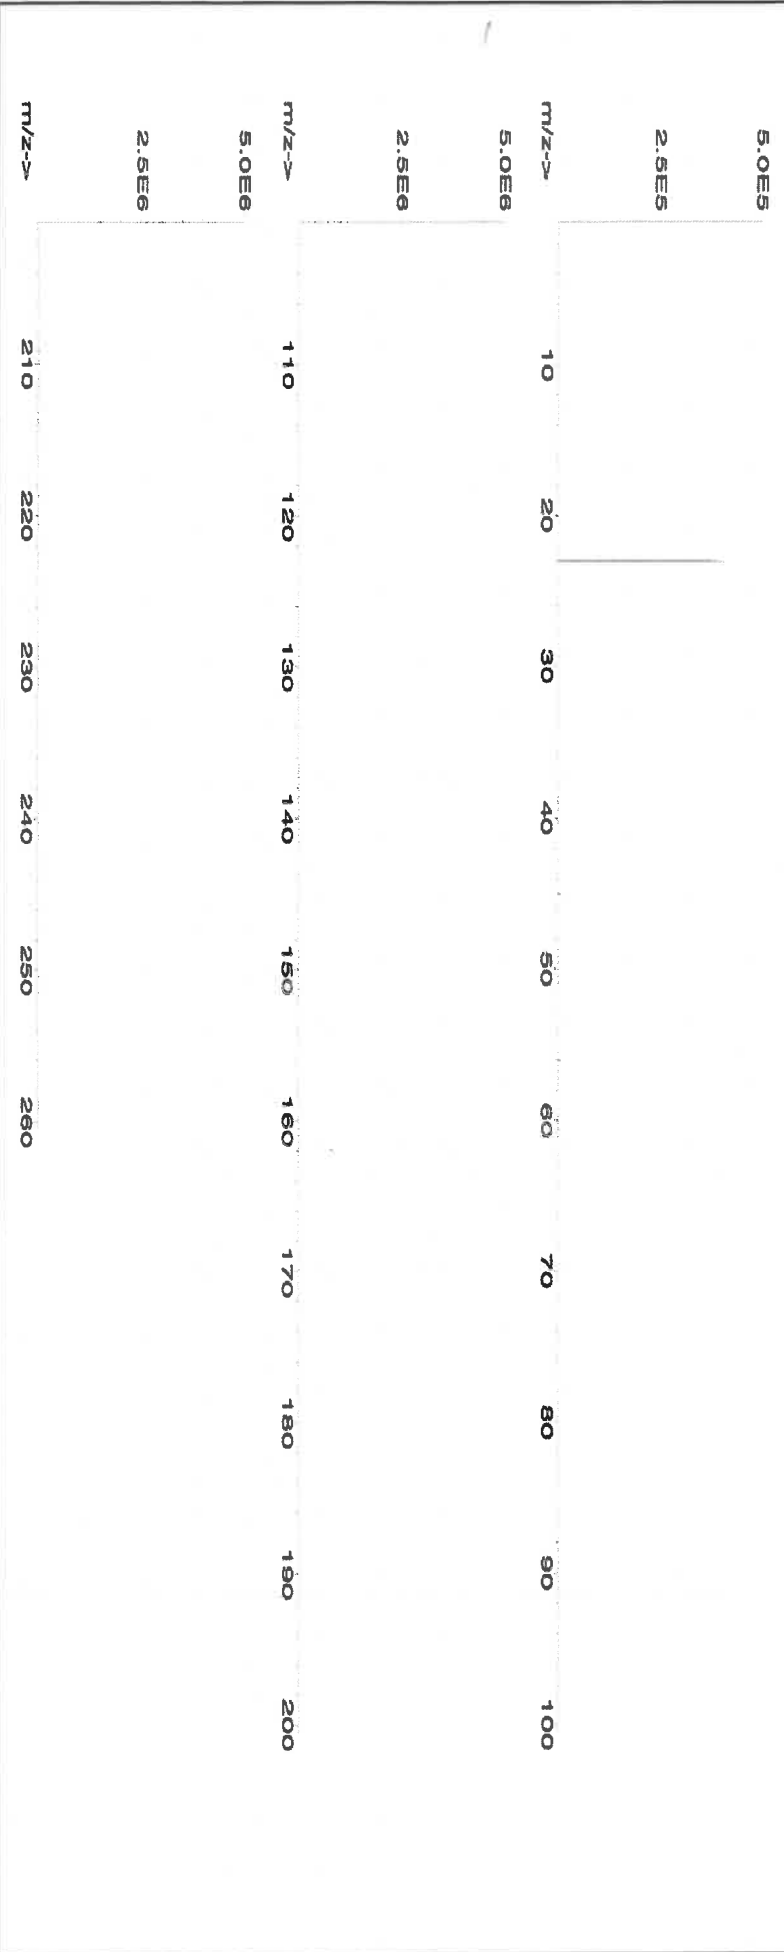



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.02	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57051
120523
Antimony (Sb)

Lot #
Solvent:

24002546 Nitric Acid

2.0% 60.0 Nitric Acid (mL)

Expiration Date:

120526

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6U7B

Volume shown below was diluted to (mL):

3000.41

5E-05 Balance Uncertainty
0.058 Flask Uncertainty


Formulated By:	Lawrence Barry	120523
Reviewed By:	Pedro L. Renteria	120523

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Antimony (Sb) 58151 100923 0.1000 300.0 0.084 1000 10001.4 1000.0 2.1 7440-36-0 0.5 mg/m3 or-rel 7000 mg/kg 3102a

[1] Spectrum No.1 [17.964 sec]:58051.D# [Count] [Linear]

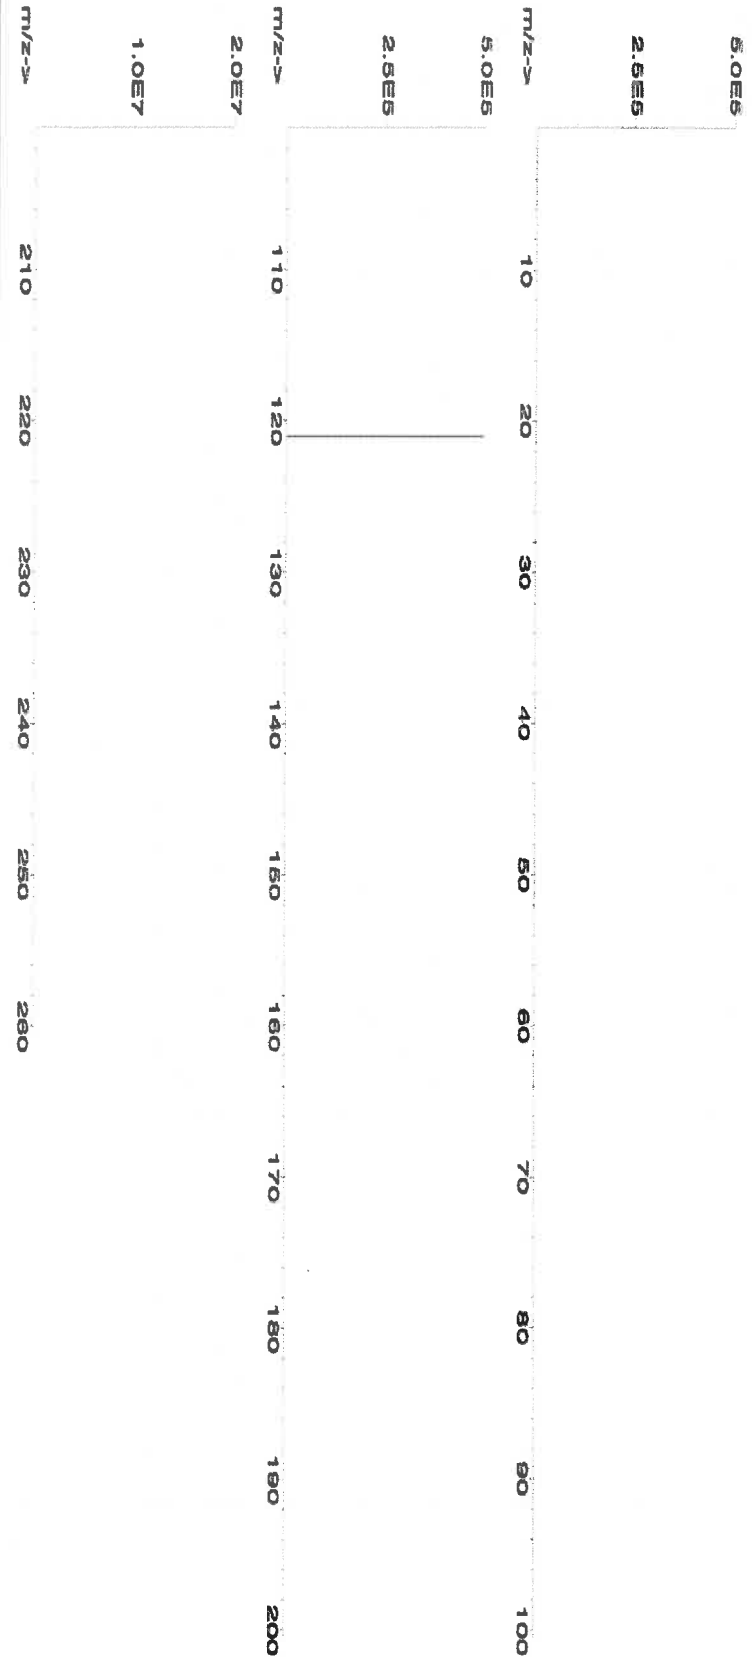



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	T	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



M6030



CERTIFIED WEIGHT REPORT:

Part Number: **57047**
Lot Number: **122823**
Description: **Silver (Ag)**

Lot #
Solvent: 24002546 Nitric Acid

Formulated By:	Benson Chan
Reviewed By:	Pedro L. Rentas
	122823


2% 80.0 (mL) Nitric Acid

Expiration Date: 122826
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 4000.30
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty		CAS#	SDS Information		NIST SRM
										+/- (µg/mL)	(µg/mL)		(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	

1. Silver nitrate (Ag) IN035 J0612AGA1 1000.0 99.999 0.10 63.7 6.27992 6.27998 1000.0 2.0 7761-88-8 10 µg/m³ NA 3151

[1] Spectrum No. 1 [14.044 sec]:58147.D# [Count] [Linear]

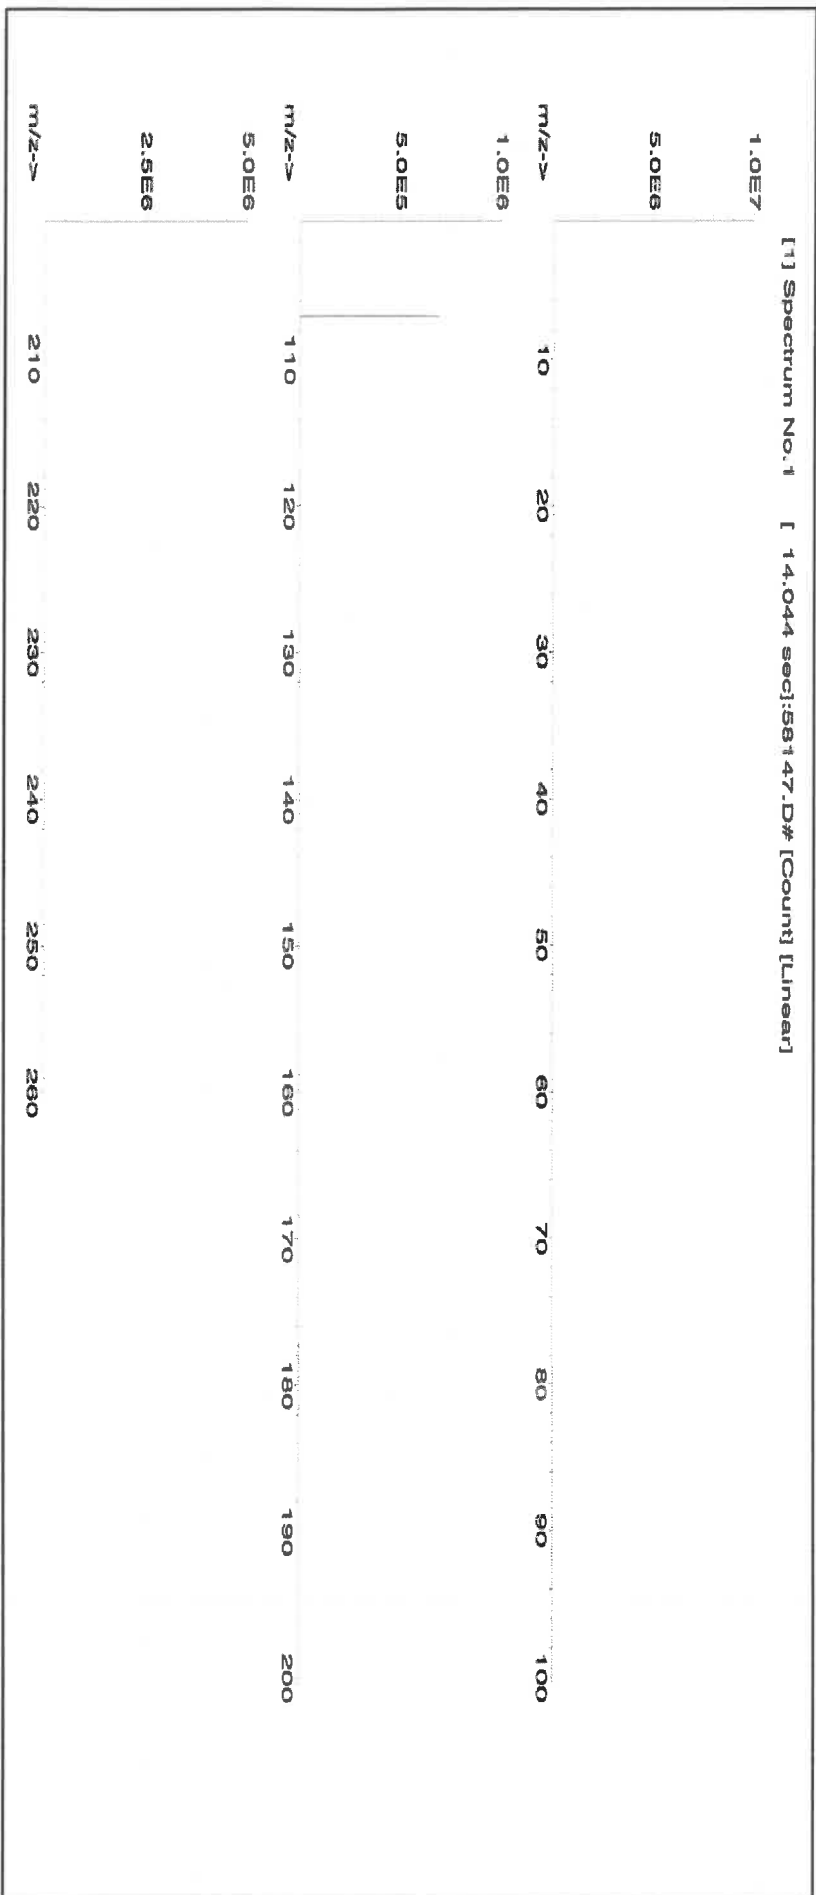



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

243

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	T	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

Physical Characterization:

(T)= Target analyte

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 meqohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 10/18/24
Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number:

Lot Number:

Description:

57051

071724

Antimony (Sb)

Lot #
24002546

Solvent:
Nitric Acid

Expiration Date:

Recommended Storage:

Nominal Concentration (µg/mL):

NIST Test Number:

Volume shown below was diluted to (mL):

2.0%

40.0 (mL)

Nitric Acid

071727

Ambient (20 °C)

1000

6UJB

2000.26

5E-05 Balance Uncertainty


0.058 Flask Uncertainty

<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
	071724
<i>Pedro L. Rentas</i>	
Reviewed By:	Pedro L. Rentas
	071724

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Antimony (Sb)	58151	060324	0.1000	200.0	0.084	1000	10001.4	1000.0	2.2	7440-36-0	0.5 mg/m3	or-rat 7000 mg/kg	3102a
------------------	-------	--------	--------	-------	-------	------	---------	--------	-----	-----------	-----------	-------------------	-------

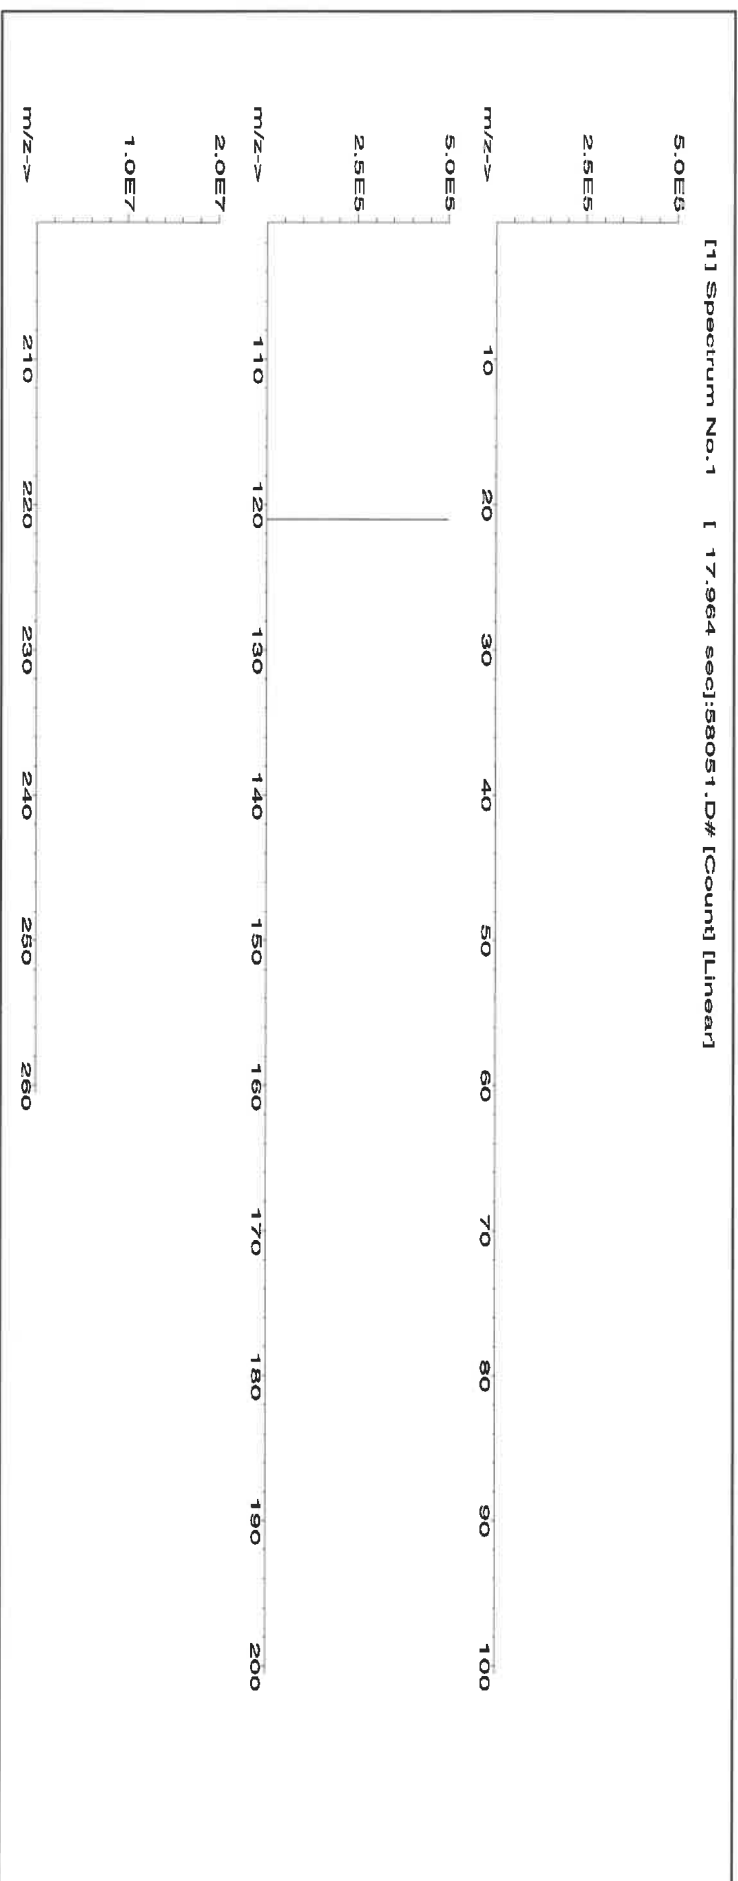



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	T	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

R: 8/5/24

M6019

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).

**2.0 PRODUCT DESCRIPTION**

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGSR1
Lot Number: U2-SR730227
Matrix: 0.1% (v/v) HNO₃
Value / Analyte(s): 1 000 µg/mL ea:
Strontium
Starting Material: SrCO₃
Starting Material Lot#: M2-2192
Starting Material Purity: 99.9993%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 1001 ± 3 µg/mL
Density: 1.000 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	998 ± 4 µg/mL ICP Assay NIST SRM Traceable to 3153a Lot Number: K2-SR650985
Assay Method #2	1001 ± 3 µg/mL EDTA NIST SRM 928 Lot Number: 928
Assay Method #3	1001 ± 2 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char\ i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char\ i})^2 / (\sum(1/u_{char\ i})^2)$$

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k(u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum(w_i)^2(u_{char\ i})^2]^{1/2}$ where $u_{char\ i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a)(u_{char\ a})$$

X_a = mean of Assay Method A with

$u_{char\ a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k(u_{char\ a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char\ a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.001980	M	Eu	<	0.000495	O	Na	0.000200	M	Se	<	0.013862	O	Zn	0.000143	
O	Al	0.000370	O	Fe	0.000410	M	Nb	<	0.000495	i	Si	<			M	Zr	<	0.000495
M	As	<	0.000495	M	Ga	<	0.000495	M	Nd	<	0.000495	M	Sm	<	0.000495			
M	Au	<	0.000989	M	Gd	<	0.000495	O	Ni	<	0.007631	M	Sn	<	0.000990			
M	B	<	0.039606	M	Ge	<	0.000495	M	Os	<	0.000494	s	Sr	<				
M	Ba	0.006486	M	Hf	<	0.000495	i	P	<			M	Ta	<	0.000495			
M	Be	<	0.000990	M	Hg	<	0.000989	M	Pb	<	0.002970	M	Tb	<	0.000495			
M	Bi	<	0.000495	M	Ho	<	0.000495	M	Pd	<	0.003957	M	Te	<	0.027724			
O	Ca	0.004255	M	In	<	0.000495	M	Pr	<	0.000495	M	Th	<	0.000990				
M	Cd	0.001339	M	Ir	<	0.000494	M	Pt	<	0.002970	M	Ti	<	0.005940				
M	Ce	<	0.004950	O	K	<	0.008184	M	Rb	<	0.002970	M	Tl	<	0.000495			
M	Co	<	0.000495	M	La	<	0.000495	M	Re	<	0.000495	M	Tm	<	0.000495			
O	Cr	<	0.003207	O	Li	<	0.000884	O	Rh	<	0.012829	M	U	<	0.001485			
M	Cs	<	0.000990	M	Lu	<	0.002970	M	Ru	<	0.000989	M	V	<	0.001980			
M	Cu	0.000099	O	Mg	0.000064	i	S	<				M	W	<	0.003960			
M	Dy	<	0.000495	O	Mn	0.000066	M	Sb	<	0.014852	O	Y	<	0.000995				
M	Er	<	0.000495	M	Mo	<	0.001980	M	Sc	<	0.001980	M	Yb	<	0.000495			

M - Checked by ICP-MS

O - Checked by ICP-OES

i - Spectral Interference

n - Not Checked For

s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale, <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form in Solution - 87.62 +2 6 Sr(H₂O)₆+2

Chemical Compatibility - Soluble in HCl, and HNO₃. Avoid H₂SO₄, HF and neutral to basic media. Stable with most metals and inorganic anions forming insoluble silicate, carbonate, hydroxide, oxide, fluoride, sulfate, oxalate, chromate, arsenate and tungstate in neutral aqueous media.

Stability - 2-100 ppb levels stable for months in 1% HNO₃ / LDPE container. 1-10,000 ppm solutions chemically stable for years in 1 - 3.5% HNO₃ / LDPE container.

Sr Containing Samples (Preparation and Solution) -Metal (Best dissolved in diluted HNO₃); Ores (Carbonate fusion in PtO followed by HCl dissolution); Organic Matrices (Dry ash and dissolution in dilute HCl).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 88 amu	1200 ppt	N/A	72Ge16O, 176Yb+2, 176Lu+2, 176Hf+2
ICP-OES 407.771 nm	0.0004 / 0.00006 µg/mL	1	U, Ce
ICP-OES 421.552 nm	0.0008 / 0.00004 µg/mL	1	Rb
ICP-OES 460.733 nm	0.07 / 0.003 µg/mL	1	Ce

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

March 03, 2023

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- March 03, 2028

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



**CERTIFIED WEIGHT REPORT:**

Part Number:

Lot Number:

Description:

Solvent: 2051001

Nitric Acid

2% 20.0 Nitric Acid

(mL)

Nominal Concentration (µg/mL):

NIST Test Number:


Weight shown below was diluted to (mL):

Flask	Uncertainty
1000.12	0.058

Expanded **SDS Information**

Compound

1. Strontium nitrate (Sr)	INO17	SR202016A1	10000	99.997	0.10	41.2	24,2756	24,2758	10000.1	20.0	10042-76-9	NA	or-rat >2000mg/kg	3153a
---------------------------	-------	------------	-------	--------	------	------	---------	---------	----------------	-------------	------------	----	-------------------	-------

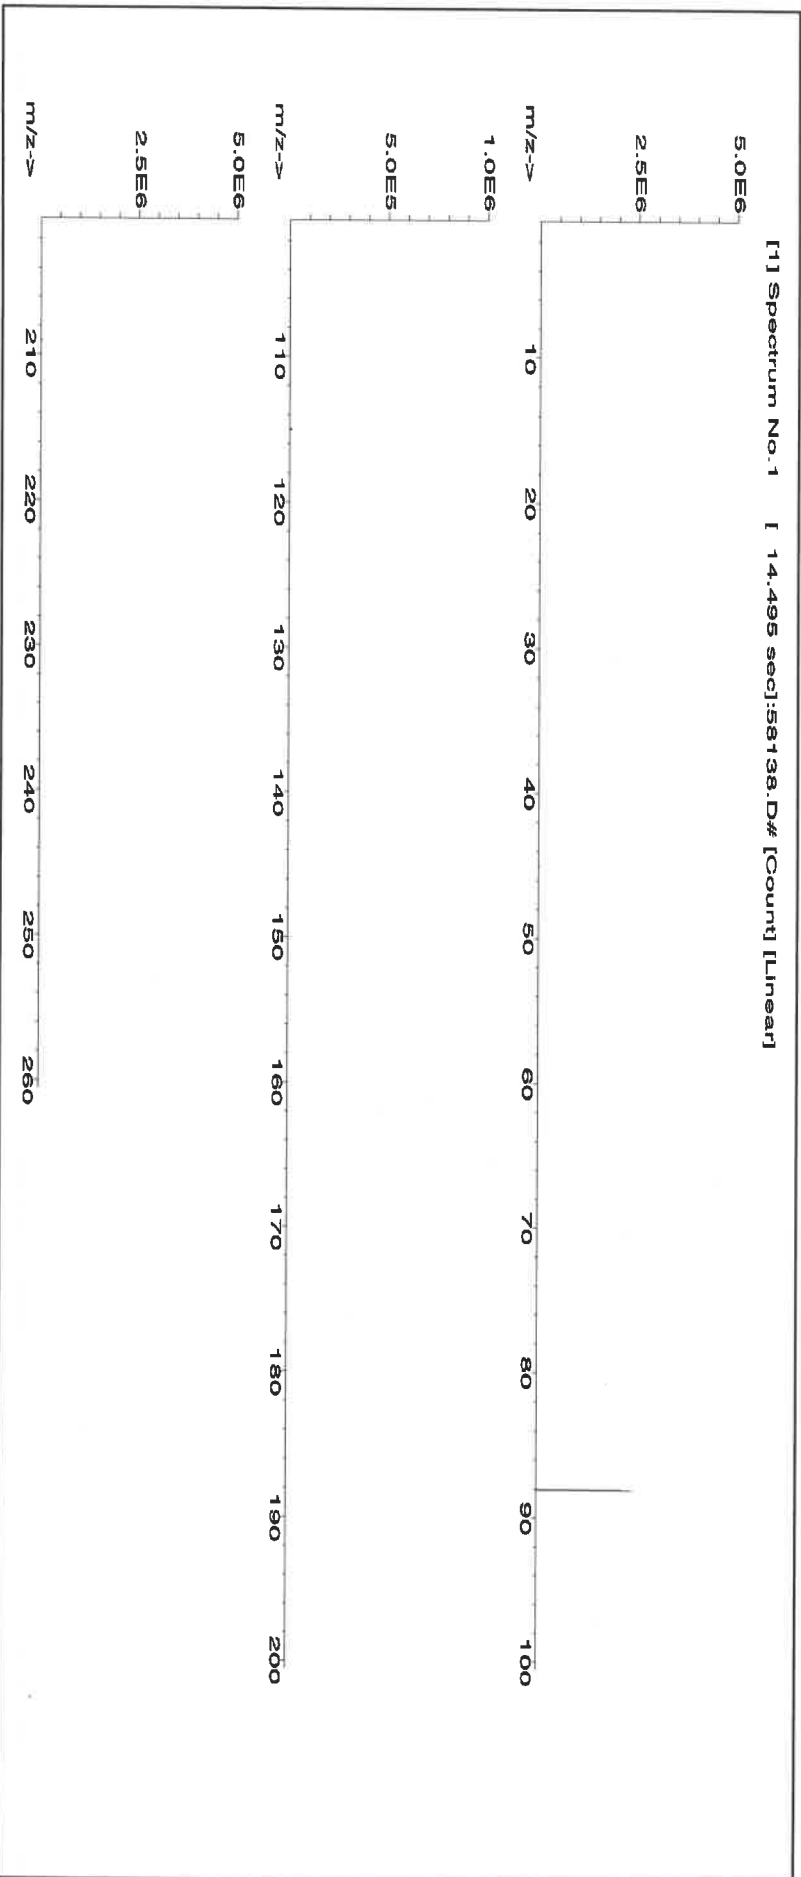



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	T	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57081
Lot Number: 062724
Description: Thallium (TI)

Solvent: 24002546 Nitric Acid
Lot #

Expiration Date:

062727

2% 40.0 Nitric Acid (mL)

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6UTB

5E-05 Balance Uncertainty

Weight shown below was diluted to (mL): 2000.1 0.10 Flask Uncertainty


<i>Aleah O'Brady</i>	
Formulated By:	Aleah O'Brady
	062724
Reviewed By:	<i>Pedro L. Renteria</i>
	Pedro L. Renteria
	062724

SDS Information

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Thallium nitrate (TI) IN037 BCCF4399 1000 99.999 0.10 77.0 2.5975 2.5977 1000.1 2.0 10102-45-1 0.1 mg/m3 orl-mus 15mg/kg 3158

[1] Spectrum No.1 [14.044 sec]:57081.D# [Count] [Linear]

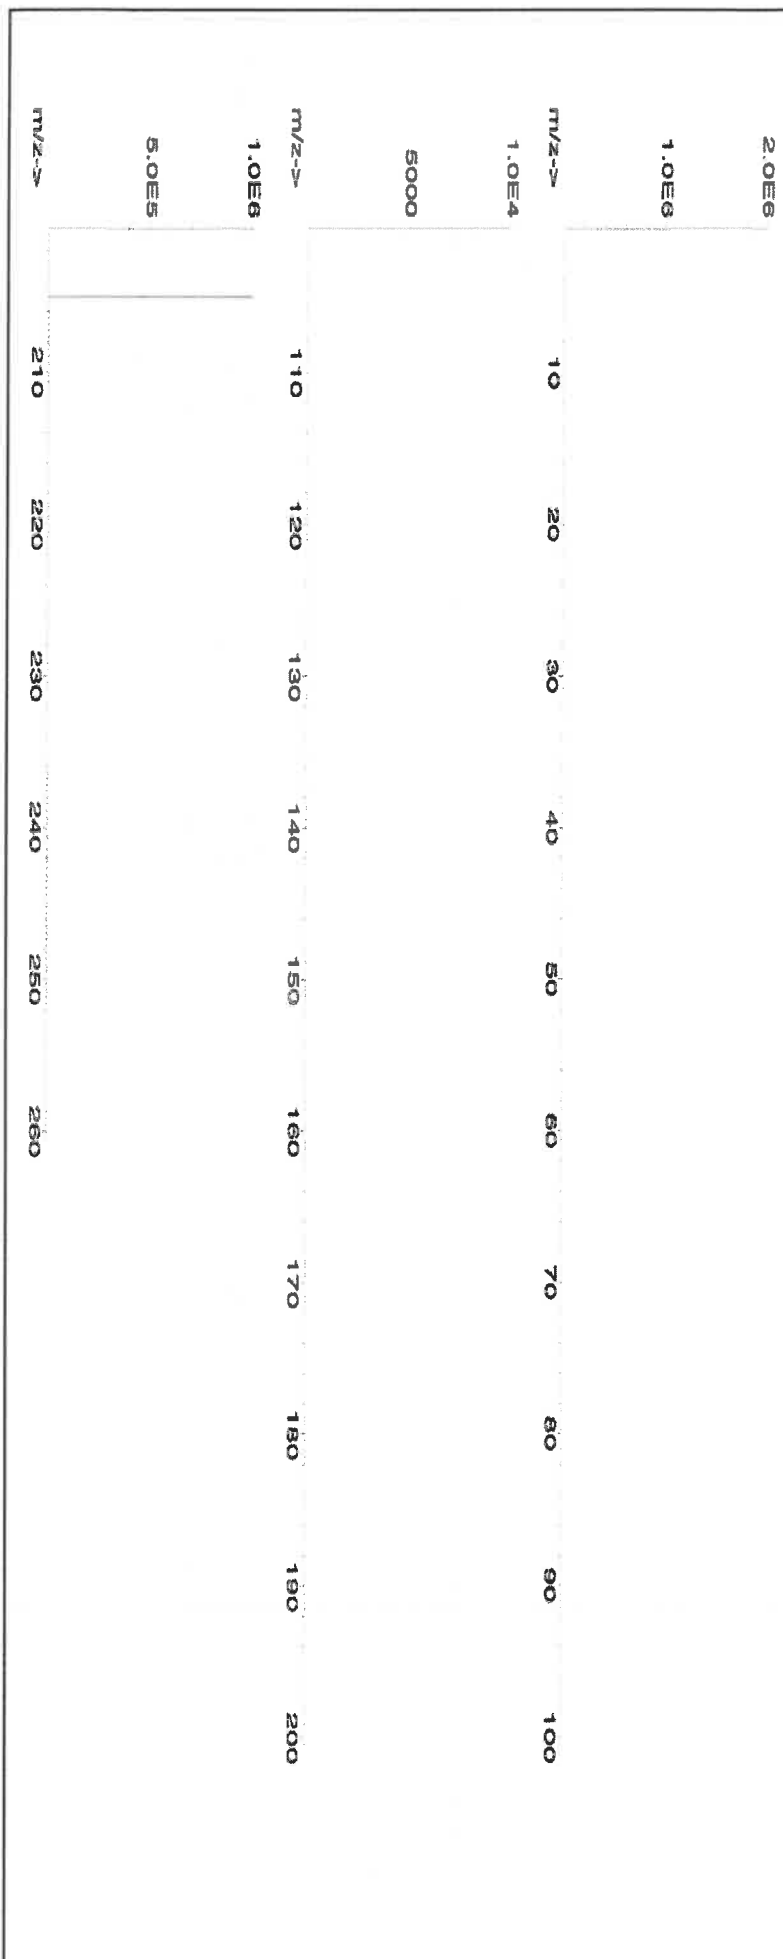



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

253

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Sc	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	T	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Tm	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Sn	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Ti	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02			Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

M6021



CERTIFIED WEIGHT REPORT:

Part Number: **57023**
Lot Number: **062424**
Description: **Vanadium (V)**

Lot # **24002546**
Solvent: **Nitric Acid**

<i>Aleah O'Brady</i>	
Formulated By:	Aleah O'Brady
Reviewed By:	Pedro L. Rantas


2.0%	40.0 (mL)	Nitric Acid
Formulated By: Aleah O'Brady		
Reviewed By: Pedro L. Rantas		

2.0%	40.0 (mL)	Nitric Acid
Formulated By: Aleah O'Brady		
Reviewed By: Pedro L. Rantas		

Expiration Date: **062427**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test Number: **6UTB**
Volume shown below was diluted to (mL): **2000.3**
5E-05 Balance Uncertainty
0.06 Flask Uncertainty

SDS Information									
(Solvent Safety Info. On Attached pg.)									
Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)
1. Ammonium metavanadate (V)	58123	021224	0.1000	200.0	0.084	1000	10000.3	1000.0	2.2
						7803-55-6		0.05 mg/m3	or -rat 58.1mg/kg
									3165

[1] Spectrum No.1 [34.243 sec]:58023.D# [Count] [Linear]

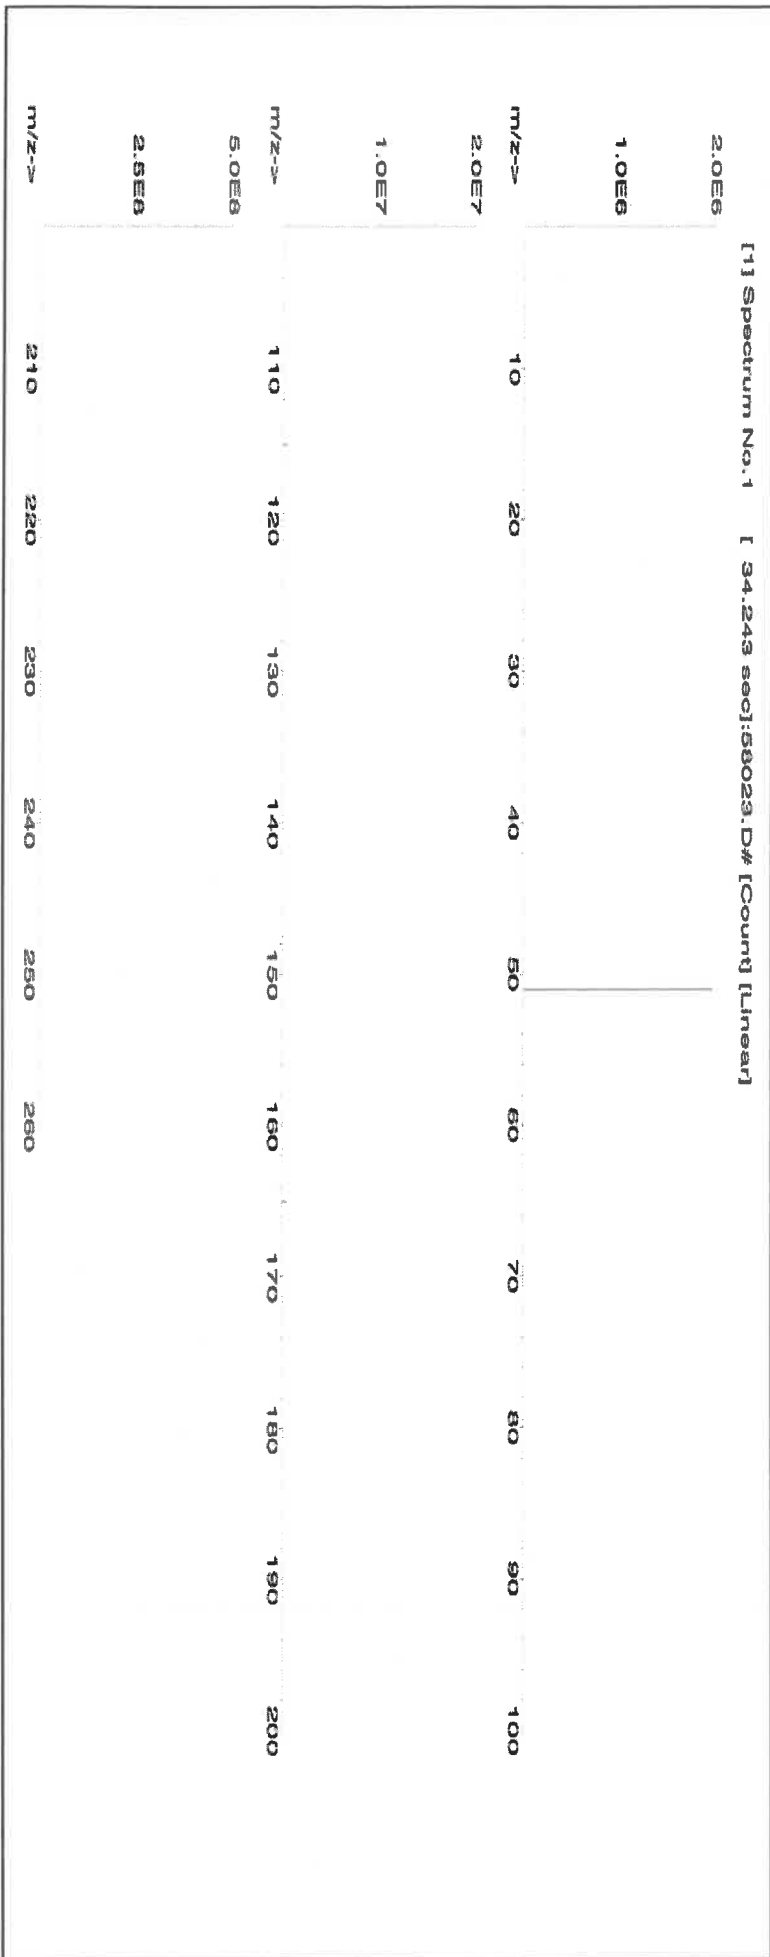



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

255

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	T
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pr	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

SOP ID : M200.7-Trace Elements-22, MSFAM01.1-Trace Metals-2

SDG No : MBHHA3,MBHHA8

Start Digest Date: 02/11/2025 Time : 11:05 Temp : 96 °C

Matrix : WATER

End Digest Date: 02/11/2025 Time : 13:10 Temp : 96 °C

Pipette ID: ICP A

Digestion tube ID: M5595

Balance ID : N/A

Block thermometer ID: MET-DIG. #1

Filter paper ID : N/A

Dig Technician Signature: *S. J. S.*

pH Strip ID : M6069

Supervisor Signature: *[Signature]*

Hood ID : #3

Temp : 1. 96°C 2. N/A

Block ID: 1. HOT BLOCK #1 2. N/A

Standardized Name	MLS USED	STD REF. # FROM LOG
LCSW	0.50	MP84063
Spike Sol 6	0.25	MP84070
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
1:1 HNO3	1.00	MP84041
1:1 HCL	0.50	MP84297
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

HOT BLOCK #1 CELL #55 :96

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
02/11/25 14:10	<i>S. J. S. metal dig</i>	<i>MS metal lab</i>
	Preparation Group	Analysis Group

Lab Sample ID	Client Sample ID	pH	Initial Vol (ml)	Final Vol (ml)	Color Before	Color After	Clarity Before	Clarity After	Comment	Prep Pos
PB166670BL	PBW670	<2	50	50	Colorless	Colorless	Clear	Clear	N/A	1
PB166670BS	LCS670	<2	50	50	Colorless	Colorless	Clear	Clear	MP84063	2
Q1314-08	MBHHA9	<2	50	50	Colorless	Colorless	Clear	Clear	N/A	3
Q1314-09	MBHHA9D	<2	50	50	Colorless	Colorless	Clear	Clear	N/A	4
Q1314-10	MBHHA9S	<2	50	50	Colorless	Colorless	Clear	Clear	MP84070	5
Q1315-01	MBHHA8	<2	50	50	Colorless	Colorless	Clear	Clear	N/A	6
Q1315-02	MBHHA8D	<2	50	50	Colorless	Colorless	Clear	Clear	N/A	7
Q1315-03	MBHHA8S	<2	50	50	Colorless	Colorless	Clear	Clear	MP84070	8

Instrument ID: P5

Daily Analysis Runlog For Sequence/QC Batch ID # LB134696

Review By	Mohan Bera	Review On	2/13/2025 11:53:27 AM
Supervise By	Kareem Khairalla	Supervise On	2/13/2025 1:12:52 PM
STD. NAME	STD REF.#		
ICAL Standard	MP84204,MP84388,MP84386,MP84385,MP84384,MP84383,MP84381		
ICV Standard	MP84446		
CCV Standard	MP84392		
ICSA Standard	MP84230,MP84231		
CRI Standard			
LCS Standard	MP84063		
Chk Standard	MP84218,MP84219		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	S0	S0	CAL1	02/12/25 12:25		Kareem	OK
2	S1	S01	CAL2	02/12/25 12:29		Kareem	OK
3	S2	S02	CAL3	02/12/25 12:33		Kareem	OK
4	S3	S03	CAL4	02/12/25 12:37		Kareem	OK
5	S4	S04	CAL5	02/12/25 12:40		Kareem	OK
6	S5	S05	CAL6	02/12/25 12:44		Kareem	OK
7	S6	S06	CAL7	02/12/25 12:48		Kareem	OK
8	ICV005	ICV005	ICV	02/12/25 13:20	Inst. paused for calibration review	Kareem	OK
9	ICB005	ICB005	ICB	02/12/25 13:24		Kareem	OK
10	ICSA005	ICSA005	ICSA	02/12/25 13:28		Kareem	OK
11	ICSAB005	ICSAB005	ICSAB	02/12/25 13:32		Kareem	OK
12	CCV011	CCV011	CCV	02/12/25 13:36		Kareem	OK
13	CCB011	CCB011	CCB	02/12/25 13:40		Kareem	OK
14	PB166660TB	LEB660	MB	02/12/25 13:44		Kareem	OK
15	Q1292-01	E1PM9	SAM	02/12/25 13:48		Kareem	OK
16	Q1292-02	E1PM9D	DUP	02/12/25 13:52		Kareem	OK
17	Q1292-01L	E1PM9L	SD	02/12/25 13:56		Kareem	OK
18	Q1292-03	E1PM9S	MS	02/12/25 14:00	MS Fail For Pb(below RI)	Kareem	OK

Instrument ID: P5

Daily Analysis Runlog For Sequence/QC Batch ID # LB134696

Review By	Mohan Bera	Review On	2/13/2025 11:53:27 AM
Supervise By	Kareem Khairalla	Supervise On	2/13/2025 1:12:52 PM

STD. NAME	STD REF.#
ICAL Standard	MP84204,MP84388,MP84386,MP84385,MP84384,MP84383,MP84381
ICV Standard	MP84446
CCV Standard	MP84392
ICSA Standard	MP84230,MP84231
CRI Standard	
LCS Standard	MP84063
Chk Standard	MP84218,MP84219

19	PB166667BL	PBW667	MB	02/12/25 14:04		Kareem	OK
20	PB166667BS	LCS667	LCS	02/12/25 14:08		Kareem	OK
21	Q1314-08	MBHHA9	SAM	02/12/25 14:12		Kareem	OK
22	Q1314-09	MBHHA9D	DUP	02/12/25 14:16		Kareem	OK
23	Q1314-08L	MBHHA9L	SD	02/12/25 14:20		Kareem	OK
24	Q1314-10	MBHHA9S	MS	02/12/25 14:24		Kareem	OK
25	Q1315-01	MBHHA8	SAM	02/12/25 14:28		Kareem	OK
26	Q1315-02	MBHHA8D	DUP	02/12/25 14:32		Kareem	OK
27	Q1315-01L	MBHHA8L	SD	02/12/25 14:36		Kareem	OK
28	Q1315-03	MBHHA8S	MS	02/12/25 14:40		Kareem	OK
29	PB166670BL	PBW670	MB	02/12/25 14:57		Kareem	OK
30	PB166670BS	LCS670	LCS	02/12/25 15:01		Kareem	OK
31	CCV012	CCV012	CCV	02/12/25 15:05		Kareem	OK
32	CCB012	CCB012	CCB	02/12/25 15:09		Kareem	OK

ORIGIN ID:TTNA (609) 250-8200
SANDRA HERNANDEZ

111A N. GOLD DR.

ROBINSVILLE, NJ 08891
UNITED STATES, US

SHIP DATE: 05FEB25
ACTWGT: 20.00 LB
CAD: 101231258/NET4535

BILL SENDER

TO **MOHAMMAD AHMED**

ALLIANCE TECHNICAL GROUP LLC
284 SHEFFIELD STREET

MOUNTAINSIDE NJ 07092

(908) 789-8900

REF: CN003.100.09

INV: PO: CN003.100.09

DEPT:



J051624121791uv


TRK# 7718 9158 6681

THU - 06 FEB 10:30A
PRIORITY OVERNIGHT

E2KBCA

07092

NJ-US EWR

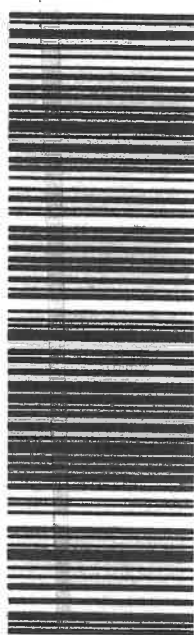

After printing this label:

CONSIGNEE COPY - PLEASE PLACE IN FRONT OF POUCH

1. Fold the printed page along the horizontal line.
2. Place label in shipping pouch and affix it to your shipment.

Use of this system constitutes your agreement to the service conditions in the current FedEx Service Guide, available on fedex.com. FedEx will not be responsible for any claim in excess of \$100 per package, whether the result of loss, damage, delay, non-delivery, misdelivery, or misinformation, unless you declare a higher value, pay an additional charge, document your actual loss and file a timely claim. Limitations found in the current FedEx Service Guide apply. Your right to recover from FedEx for any loss, including intrinsic value of the package, loss of sales, income interest, profit, attorney's fees, costs, and other forms of damage whether direct, incidental, consequential, or special is limited to the greater of \$100 or the authorized declared value. Recovery cannot exceed actual documented loss. Maximum for items of extraordinary value is \$1,000, e.g. jewelry, precious metals, negotiable instruments and other items listed in our Service Guide. Written claims must be filed within strict time limits, see current FedEx Service Guide.

Handwritten:
2/6/25
9:30

Login Summary Report

Order ID :	Q1315	Order Date :	2/6/2025 9:30:00 AM	Project Mgr :	Deepak
Client :	USEPA CLP SMO	Project :	51979	Report Type :	USEPA CLP
Contact :	Anita Kapadia	Receive Date :	2/6/2025 9:30:00 AM	EDD Type :	EPA CLP
Date Sign Off :	2/6/2025 11:17:45 AM				

Sample ID	Client ID	Matrix	Sampling Date	Test	Test Group	Method	TAT Days	Fax Due Date	HC Due Date
Q1315-01	MBHHA8	Water	02/04/2025		DM				
				Metals CLP Full		SFAM_AES	10	02/20/2025	02/20/2025
Q1315-02	MBHHA8D	Water	02/04/2025		DM				
				Metals CLP Full		SFAM_AES	10	02/20/2025	02/20/2025
Q1315-03	MBHHA8S	Water	02/04/2025		DM				
				Metals CLP Full		SFAM_AES	10	02/20/2025	02/20/2025

WORKLIST(Hardcopy Internal Chain)

Worklist Name : PB166670

Worklist ID : 187631

Department : Digestion

Date : 02-11-2025 10:25:55

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1314-08	MBHHA9	Water	Metals CLP Full	1:1 HNO3 to pH < 2	USEP01	C11	02/04/2025	SFAM_AES
Q1314-09	MBHHA9D	Water	Metals CLP Full	1:1 HNO3 to pH < 2	USEP01	C11	02/04/2025	SFAM_AES
Q1314-10	MBHHA9S	Water	Metals CLP Full	Cool 4 deg C	USEP01	C11	02/04/2025	SFAM_AES
Q1315-01	MBHHA8	Water	Metals CLP Full	1:1 HNO3 to pH < 2	USEP01	C12	02/04/2025	SFAM_AES
Q1315-02	MBHHA8D	Water	Metals CLP Full	1:1 HNO3 to pH < 2	USEP01	C12	02/04/2025	SFAM_AES
Q1315-03	MBHHA8S	Water	Metals CLP Full	1:1 HNO3 to pH < 2	USEP01	C12	02/04/2025	SFAM_AES

Date/Time 02/11/25 10:50

Raw Sample Received by: S128. Jndh.109

Raw Sample Relinquished by: gh1/201

Date/Time 02/11/25 11:50

Raw Sample Received by: S128. Jndh.109

Raw Sample Relinquished by: gh1/201