
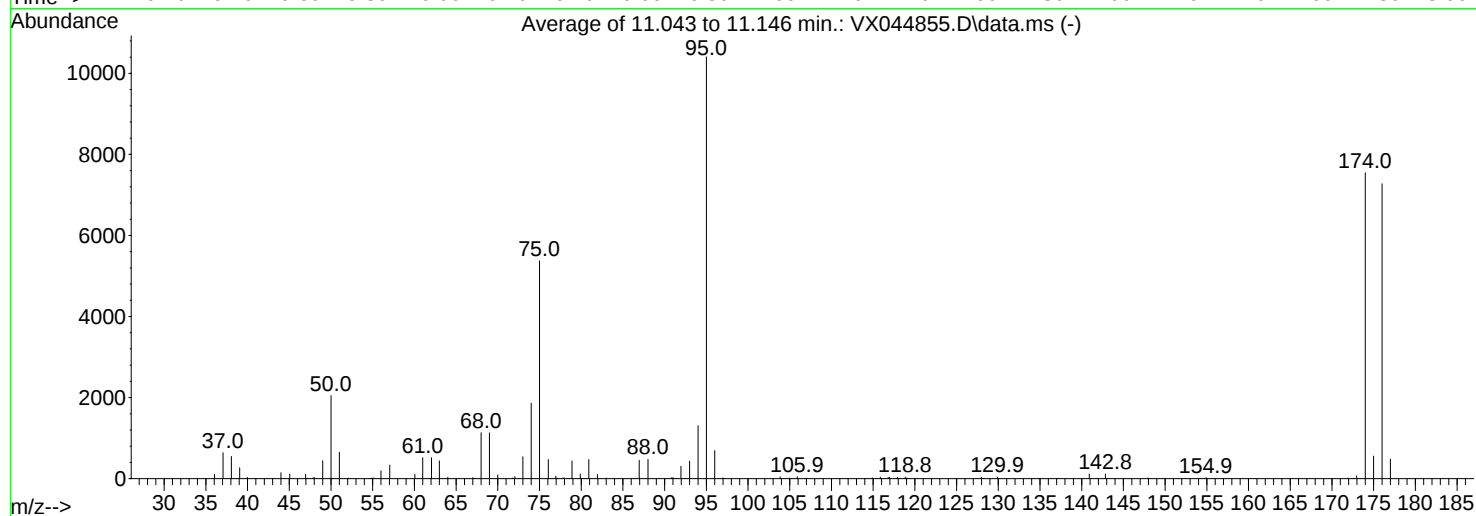


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020725\
Data File : VX044855.D
Acq On : 07 Feb 2025 09:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011625W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jan 17 01:21:41 2025

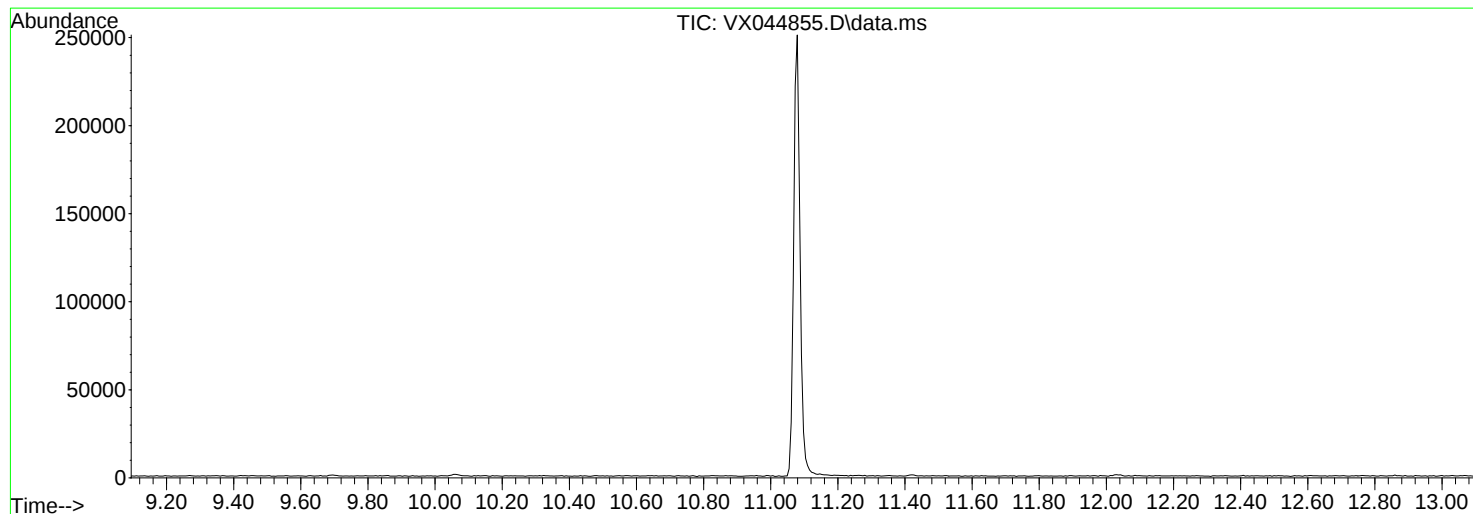

AutoFind: Averaged scan 1633 to 1650; Bkg corrected with scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	2049	PASS
75	95	30	60	51.6	5371	PASS
95	95	100	100	100.0	10407	PASS
96	95	5	9	6.6	691	PASS
173	174	0.00	2	0.9	70	PASS
174	95	50	100	72.5	7547	PASS
175	174	5	9	7.4	557	PASS
176	174	95	101	96.4	7277	PASS
177	176	5	9	6.6	483	PASS